

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020724\
 Data File : PS025839.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2024 21:58
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 00:45:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.347	6.754	751.2E6	382.6E6	532.323	543.956
Target Compounds							
1) T	Dalapon	0.000	2.556	0	2410182	N.D.	2.173
2) T	3,5-DICHL...	5.690	0.000	7062670	0	3.277	N.D. #
5) T	DICAMBA	0.000	6.951	0	8090253	N.D.	2.666
6) T	MCP	6.706f	6.951f	26370206	8090253	7.249	3.955 #
7) T	MCPA	6.706f	0.000	26370206	0	4.898	N.D. #
8) T	DICHLORPROP	0.000	7.549	0	10902130	N.D.	13.652
9) T	2,4-D	7.242	7.765f	19725429	98201	11.099	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020724\
Data File : PS025839.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2024 21:58
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 00:45:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

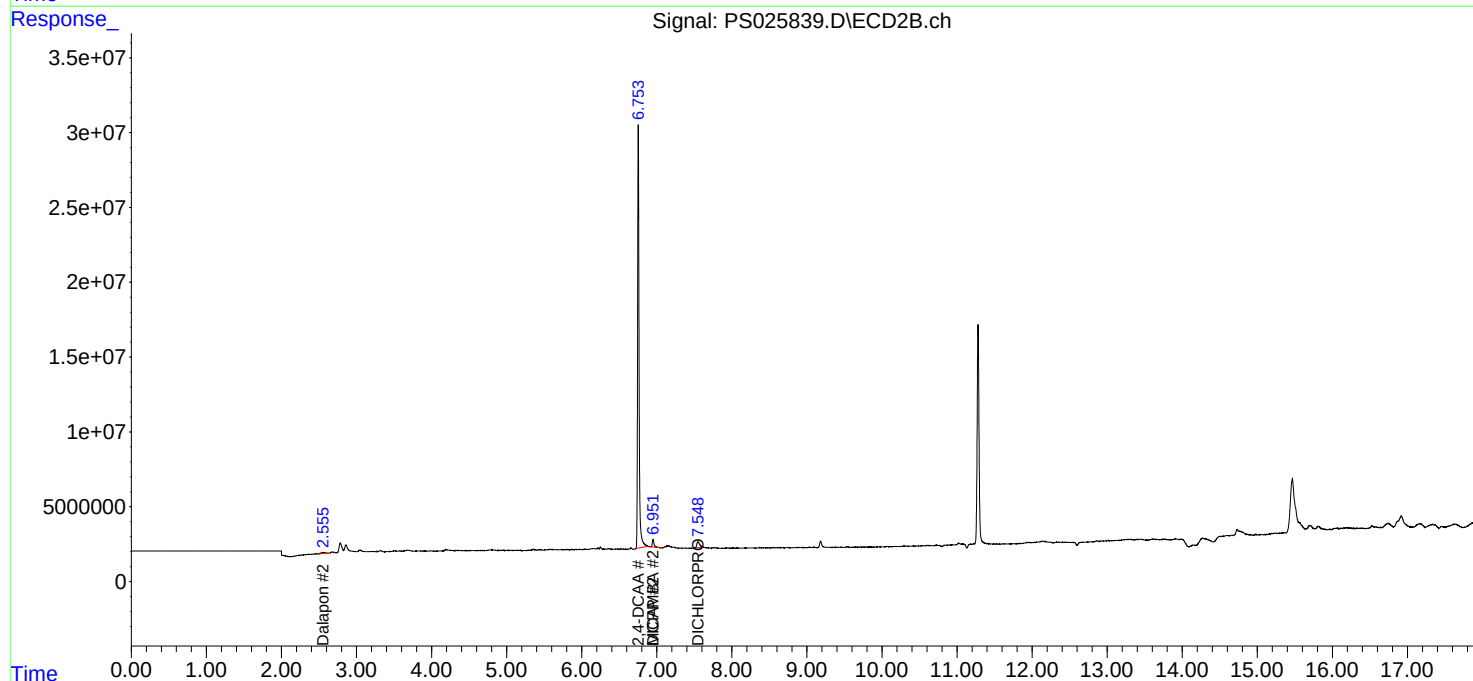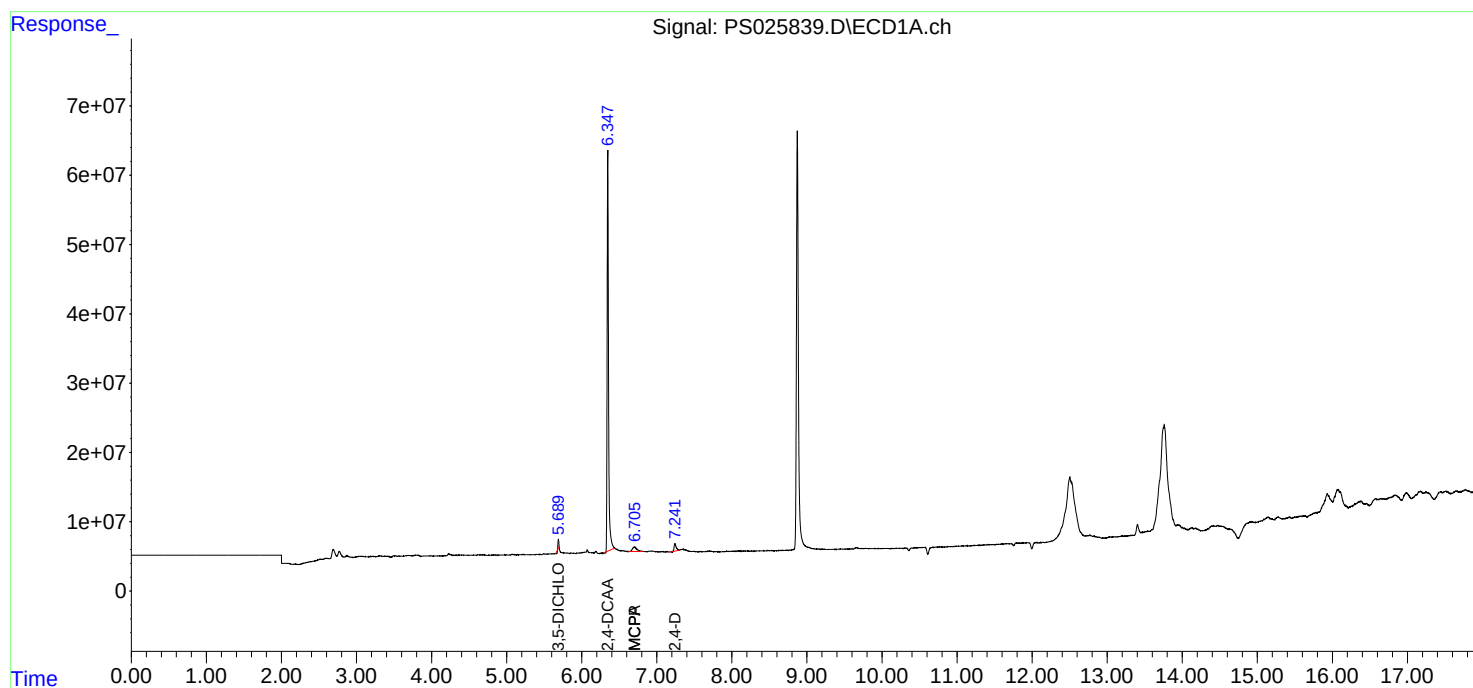


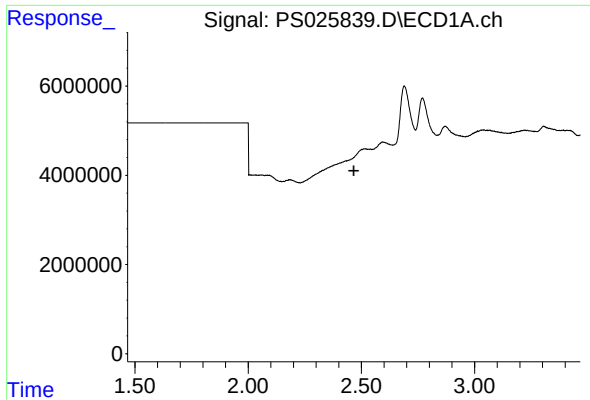

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

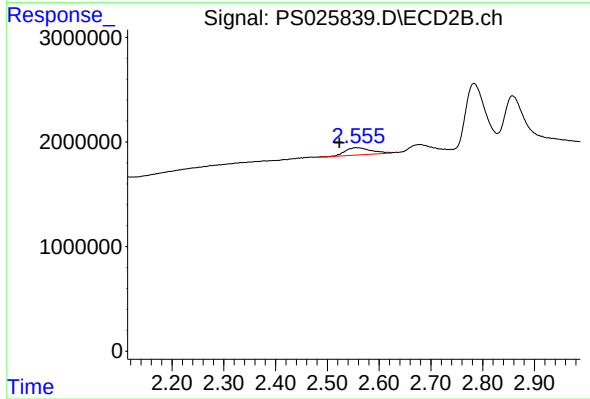


#1 Dalapon

R.T.: 2.556 min
Delta R.T.: 0.032 min
Response: 2410182
Conc: 2.17 ng/ml

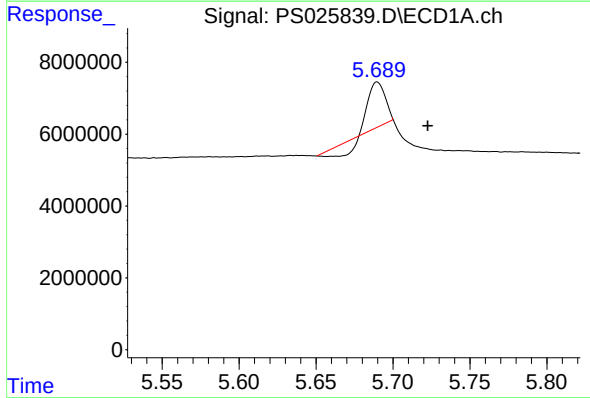


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.690 min
Delta R.T.: -0.033 min
Response: 7062670
Conc: 3.28 ng/ml

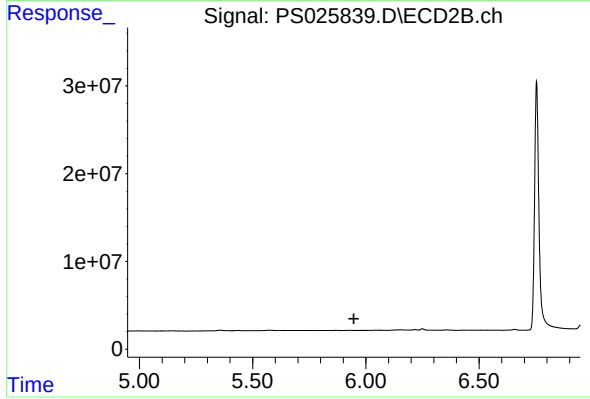

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.947 min
Response: 0
Conc: N.D.

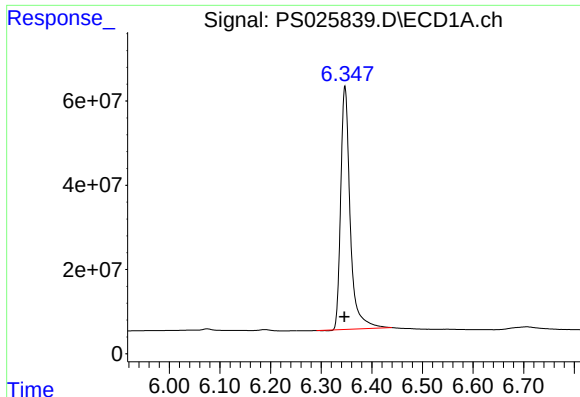

#4 2,4-DCAA


R.T.: 6.347 min
Delta R.T.: 0.001 min
Response: 751241545
Conc: 532.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

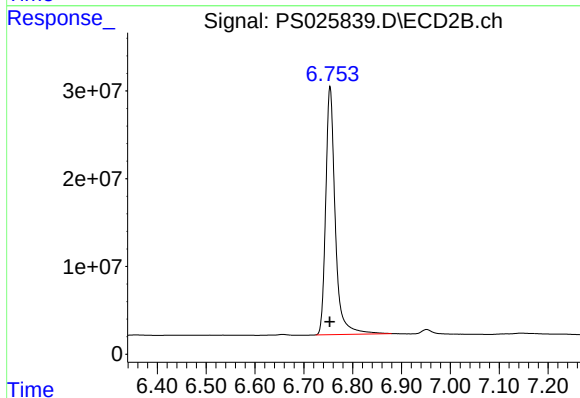


#4 2,4-DCAA

R.T.: 6.754 min
Delta R.T.: 0.000 min
Response: 382642074
Conc: 543.96 ng/ml

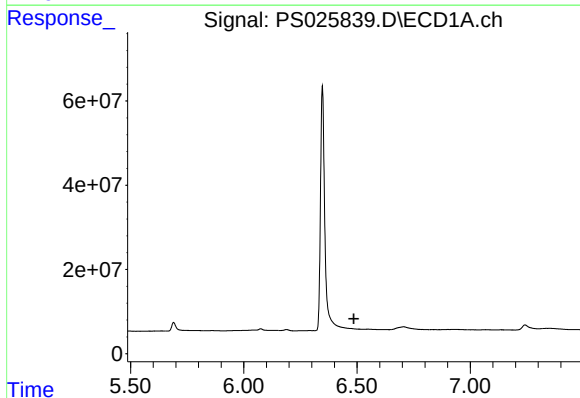


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.486 min
Response: 0
Conc: N.D.

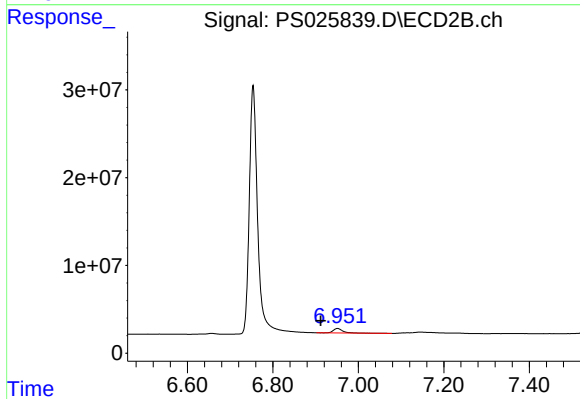

#5 DICAMBA


R.T.: 6.951 min
Delta R.T.: 0.039 min
Response: 8090253
Conc: 2.67 ng/ml

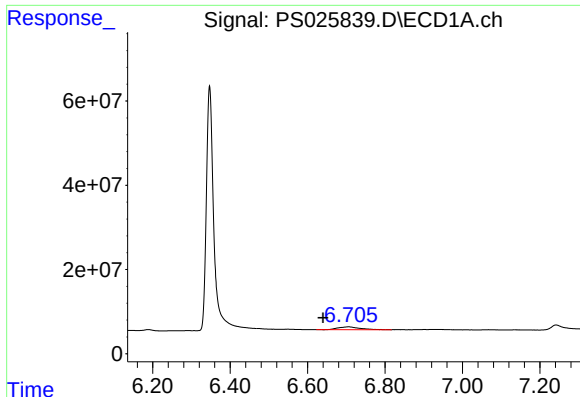

#6 MCPP


R.T.: 6.706 min
Delta R.T.: 0.066 min
Response: 26370206
Conc: 7.25 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

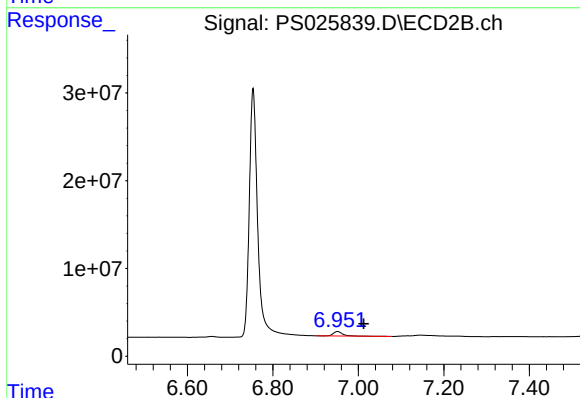


#6 MCPP

R.T.: 6.951 min
Delta R.T.: -0.061 min
Response: 8090253
Conc: 3.95 ug/ml

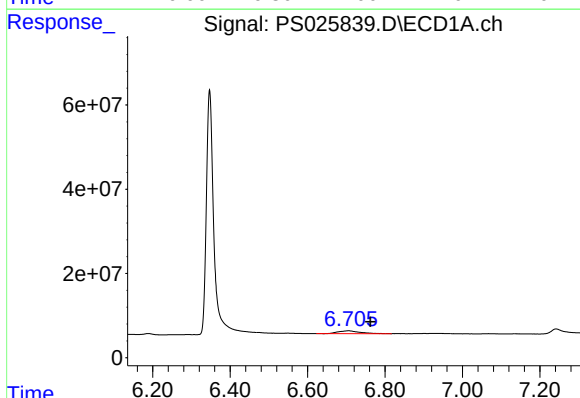


#7 MCPA

R.T.: 6.706 min
Delta R.T.: -0.057 min
Response: 26370206
Conc: 4.90 ug/ml

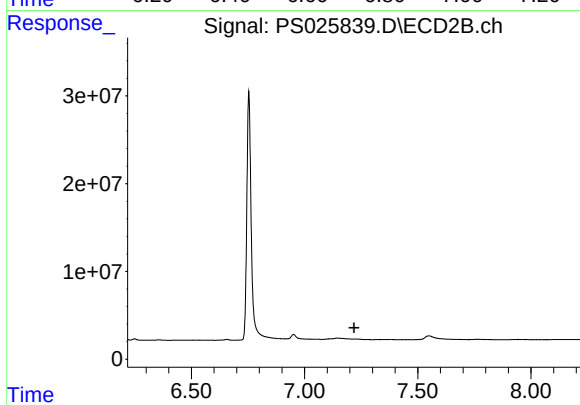

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.218 min
Response: 0
Conc: N.D.

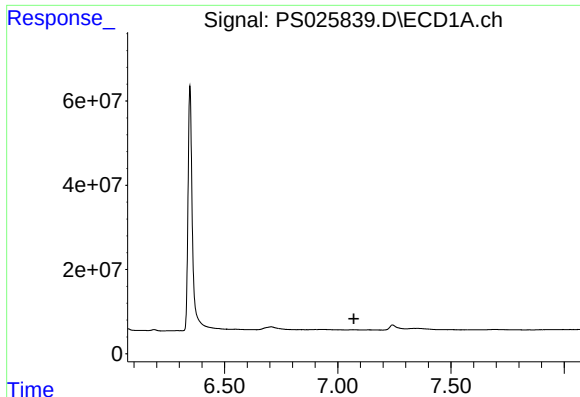

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

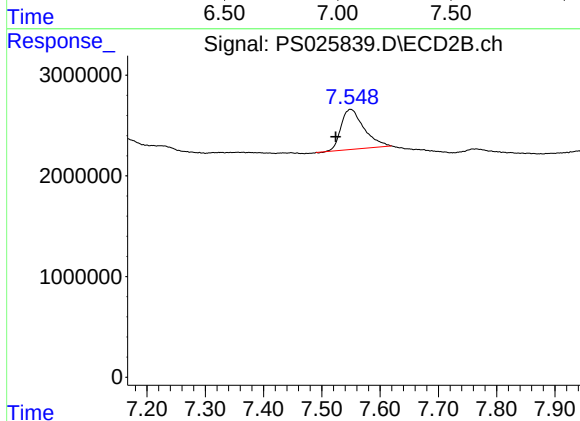


#8 DICHLORPROP

R.T.: 7.549 min
Delta R.T.: 0.025 min
Response: 10902130
Conc: 13.65 ng/ml

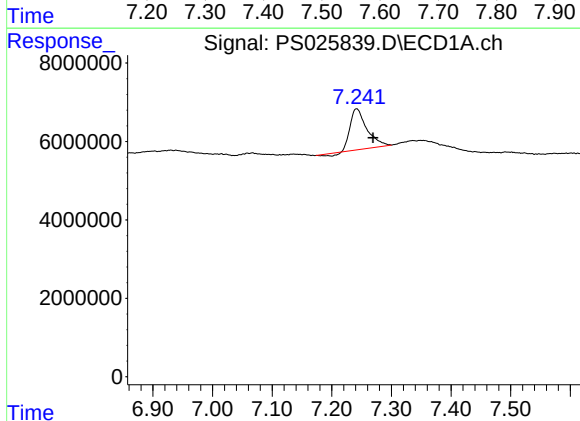

#9 2,4-D

R.T.: 7.242 min
Delta R.T.: -0.028 min
Response: 19725429
Conc: 11.10 ng/ml

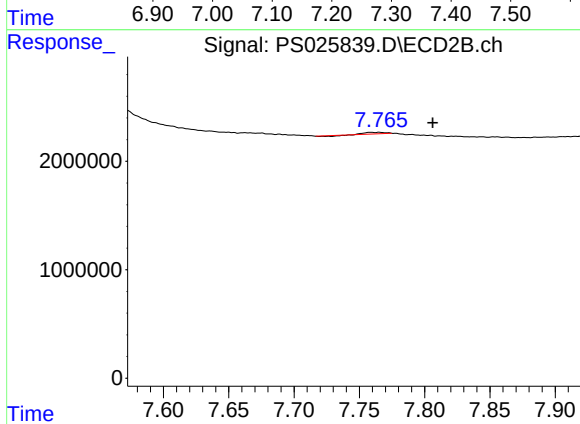

#9 2,4-D

R.T.: 7.765 min
Delta R.T.: -0.041 min
Response: 98201
Conc: N.D.