

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020724\
 Data File : PS025848.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2024 01:34
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 04:29:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.347	6.754	757.7E6	389.9E6	536.893	554.251
Target Compounds							
1) T	Dalapon	0.000	2.556	0	3044160	N.D.	2.744
2) T	3,5-DICHL...	5.691	0.000	6704168	0	3.111	N.D. #
5) T	DICAMBA	0.000	6.951	0	10232438	N.D.	3.372
6) T	MCP	6.710f	6.951f	25776958	10232438	7.086	5.002 #
7) T	MCPA	6.710f	0.000	25776958	0	4.788	N.D. #
8) T	DICHLORPROP	0.000	7.553	0	11039831	N.D.	13.825
9) T	2,4-D	7.243	0.000	26253424	0	14.772	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020724\
Data File : PS025848.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2024 01:34
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 04:29:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

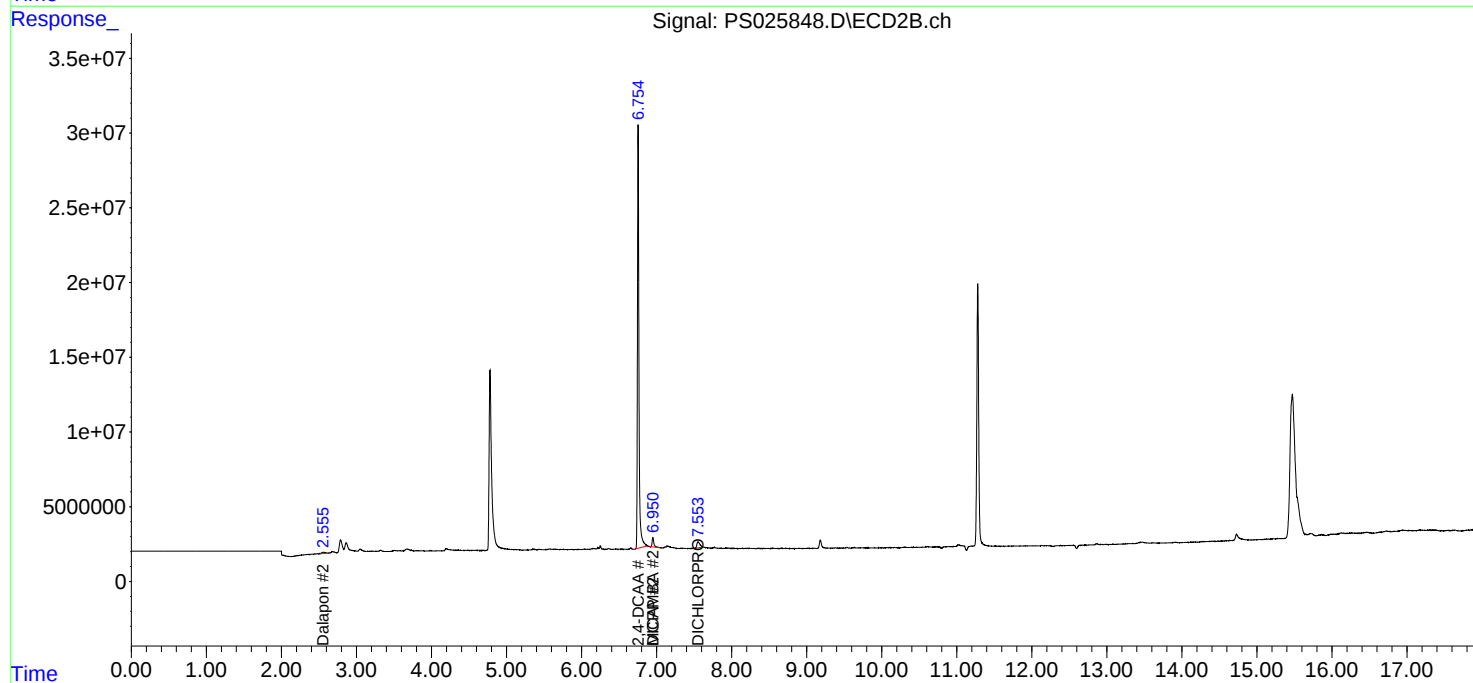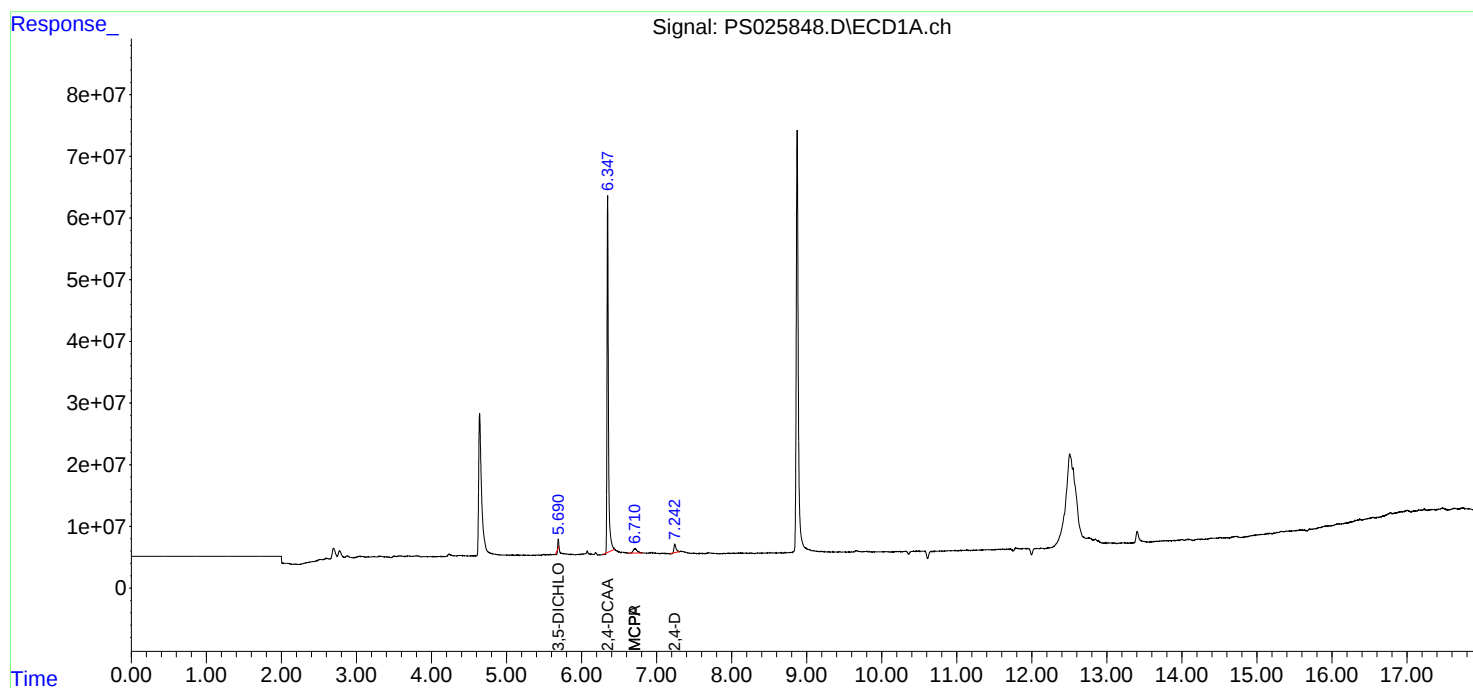


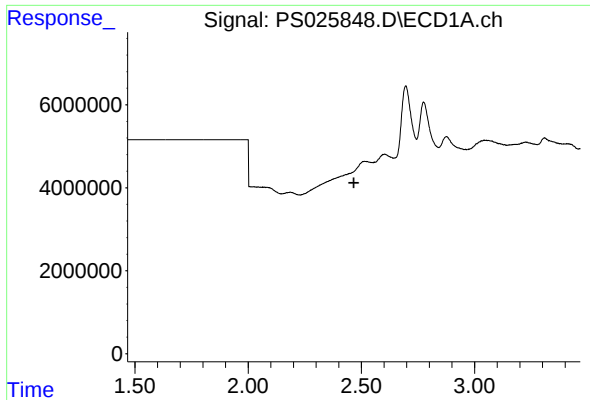

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

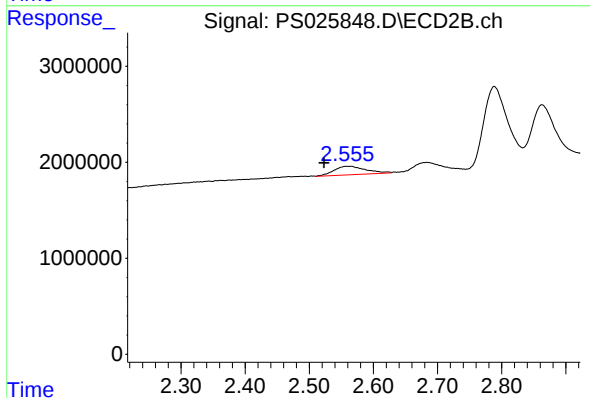


#1 Dalapon

R.T.: 2.556 min
Delta R.T.: 0.032 min
Response: 3044160
Conc: 2.74 ng/ml

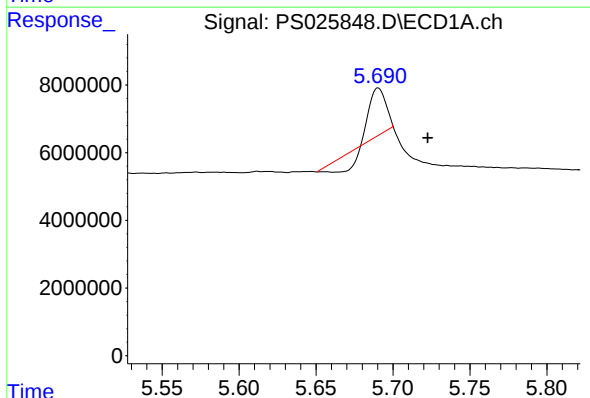


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.691 min
Delta R.T.: -0.032 min
Response: 6704168
Conc: 3.11 ng/ml

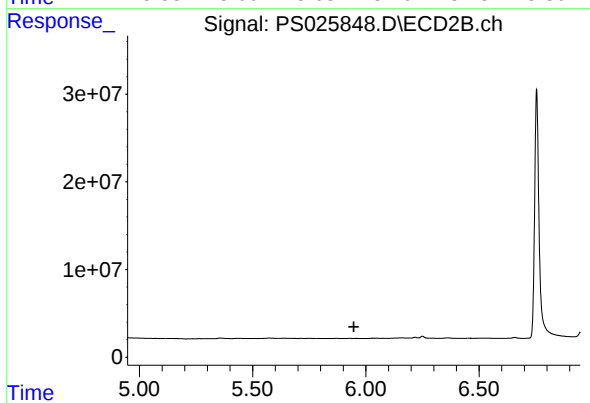

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.947 min
Response: 0
Conc: N.D.

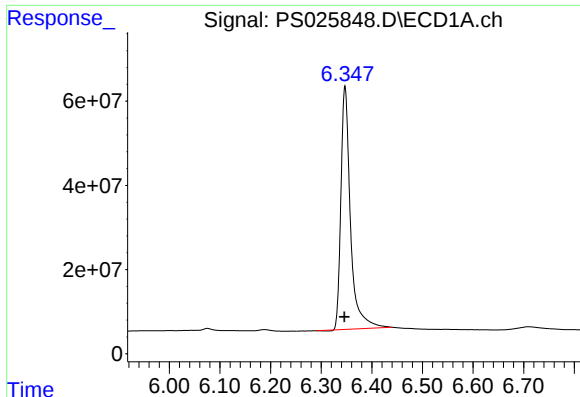

#4 2,4-DCAA


R.T.: 6.347 min
Delta R.T.: 0.001 min
Response: 757690584
Conc: 536.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

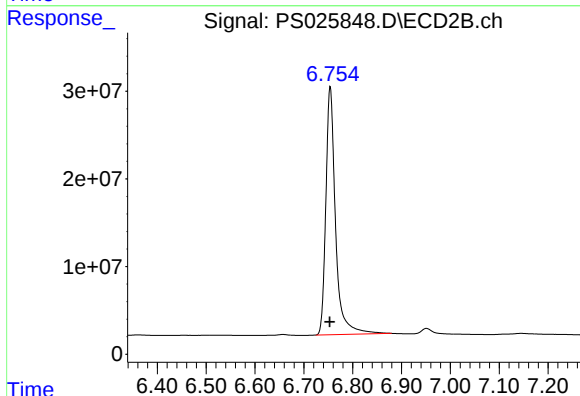


#4 2,4-DCAA

R.T.: 6.754 min
Delta R.T.: 0.000 min
Response: 389883951
Conc: 554.25 ng/ml

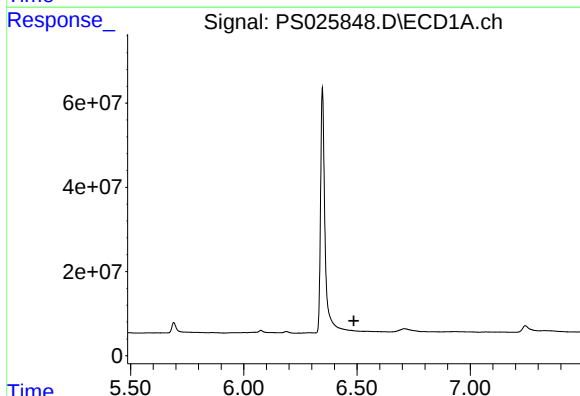


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.486 min
Response: 0
Conc: N.D.

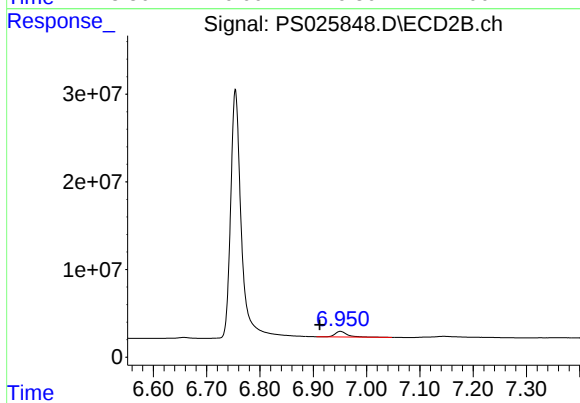

#5 DICAMBA


R.T.: 6.951 min
Delta R.T.: 0.039 min
Response: 10232438
Conc: 3.37 ng/ml

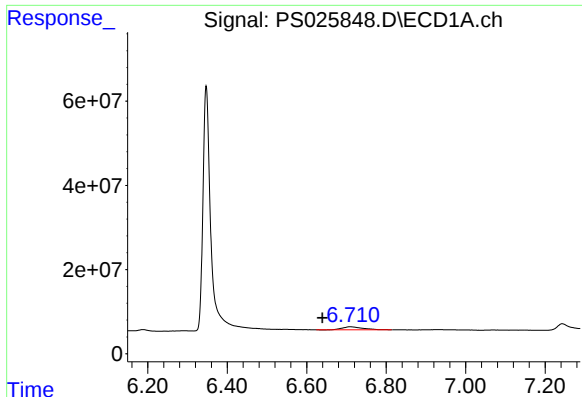

#6 MCPP


R.T.: 6.710 min
Delta R.T.: 0.070 min
Response: 25776958
Conc: 7.09 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

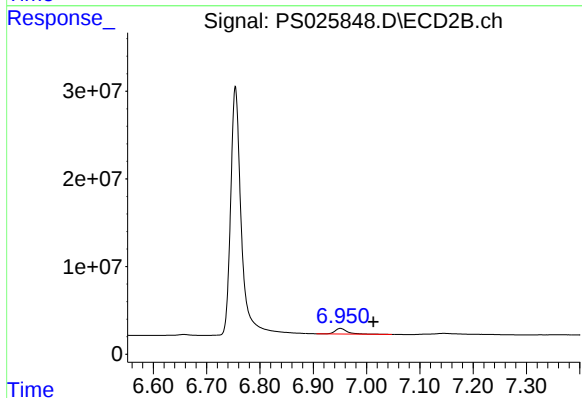


#6 MCPP

R.T.: 6.951 min
Delta R.T.: -0.062 min
Response: 10232438
Conc: 5.00 ug/ml

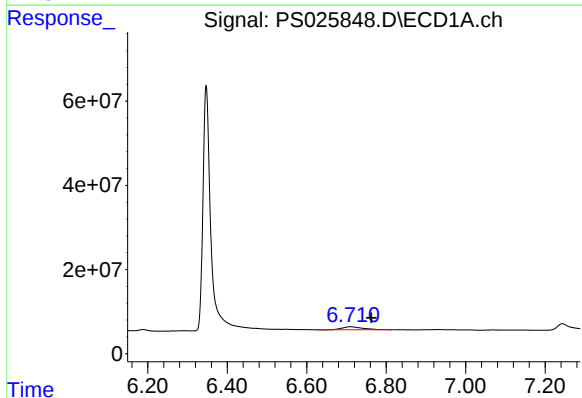


#7 MCPA

R.T.: 6.710 min
Delta R.T.: -0.053 min
Response: 25776958
Conc: 4.79 ug/ml

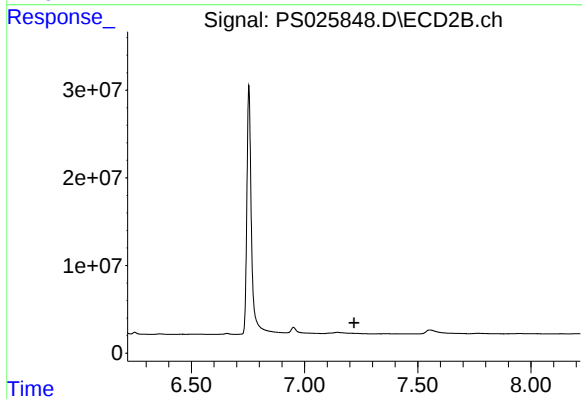

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.218 min
Response: 0
Conc: N.D.

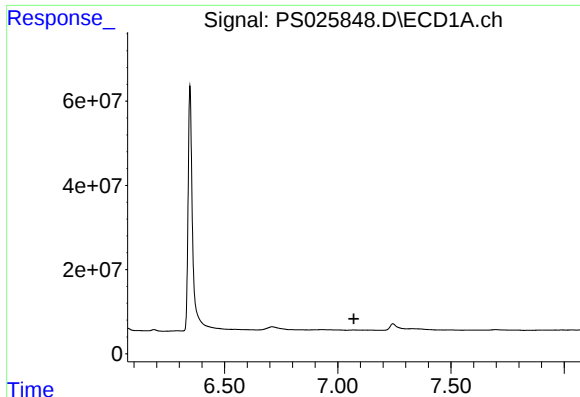

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

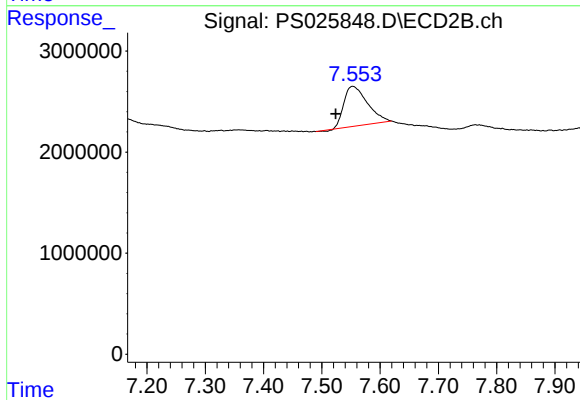


#8 DICHLORPROP

R.T.: 7.553 min
Delta R.T.: 0.029 min
Response: 11039831
Conc: 13.82 ng/ml

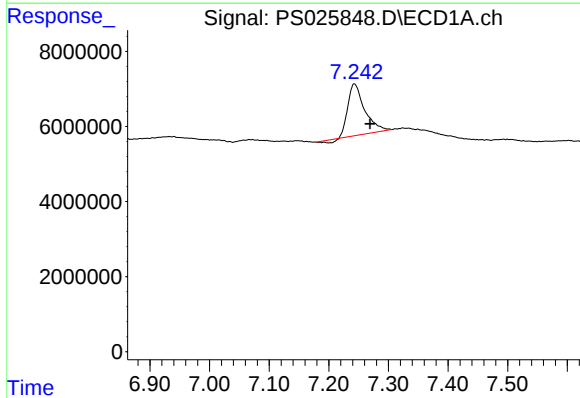

#9 2,4-D

R.T.: 7.243 min
Delta R.T.: -0.026 min
Response: 26253424
Conc: 14.77 ng/ml

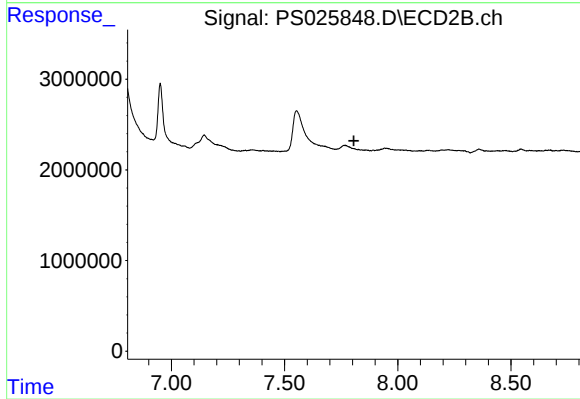

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.806 min
Response: 0
Conc: N.D.