

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020724\
 Data File : PS025855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2024 04:22
 Operator : AR\AJ
 Sample : P1337-17
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 06:06:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.347	6.754	429.3E6	184.5E6	304.216	262.341
Target Compounds							
2) T	3,5-DICHL...	5.690	5.953	14370827	-332908	6.668	N.D. #
5) T	DICAMBA	6.508	6.909	-279482	2019703	N.D.	<MDL
6) T	MCP	6.668	7.025	138.8E6	536165	38.159	<MDL #
7) T	MCPA	6.791	7.210	7952349	6627204	1.477	2.127 #
8) T	DICHLORPROP	7.108	7.533	13003787	69081130	8.273	86.507 #
9) T	2,4-D	7.234	7.828	99271011	2404769	55.858	2.819 #
10) T	Pentachlo...	7.500	8.224	8238957	3331710	<MDL	<MDL #
12) T	2,4,5-T	8.291	8.956	79611807	2624212	8.410	<MDL #
14) T	DINOSEB	9.773f	9.771	325.7E6	70087411	48.460	24.377 #
15) T	Picloram	9.701f	10.708	106.2E6	-2123721	9.028	N.D. #
16) T	DCPA	10.087	10.708	11643321	-2123721	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020724\
Data File : PS025855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2024 04:22
Operator : AR\AJ
Sample : P1337-17
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 06:06:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

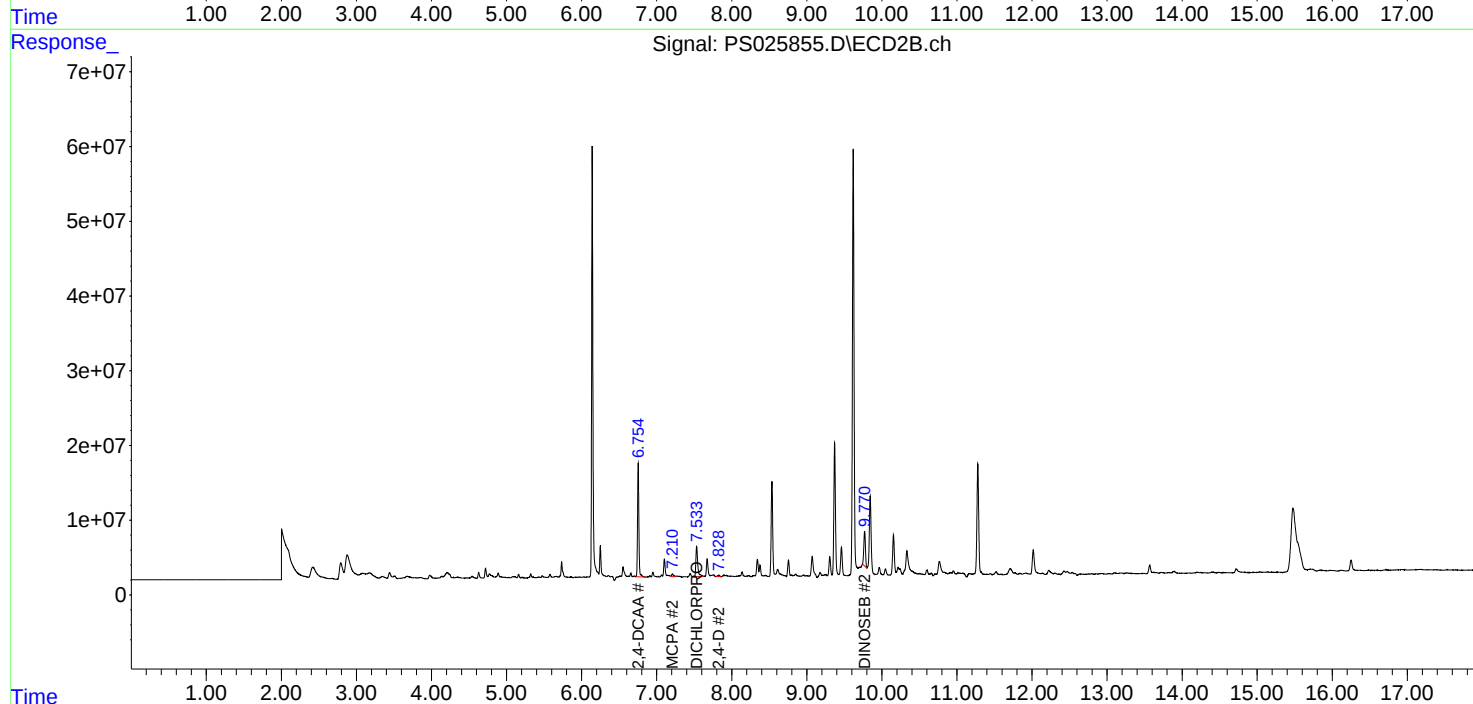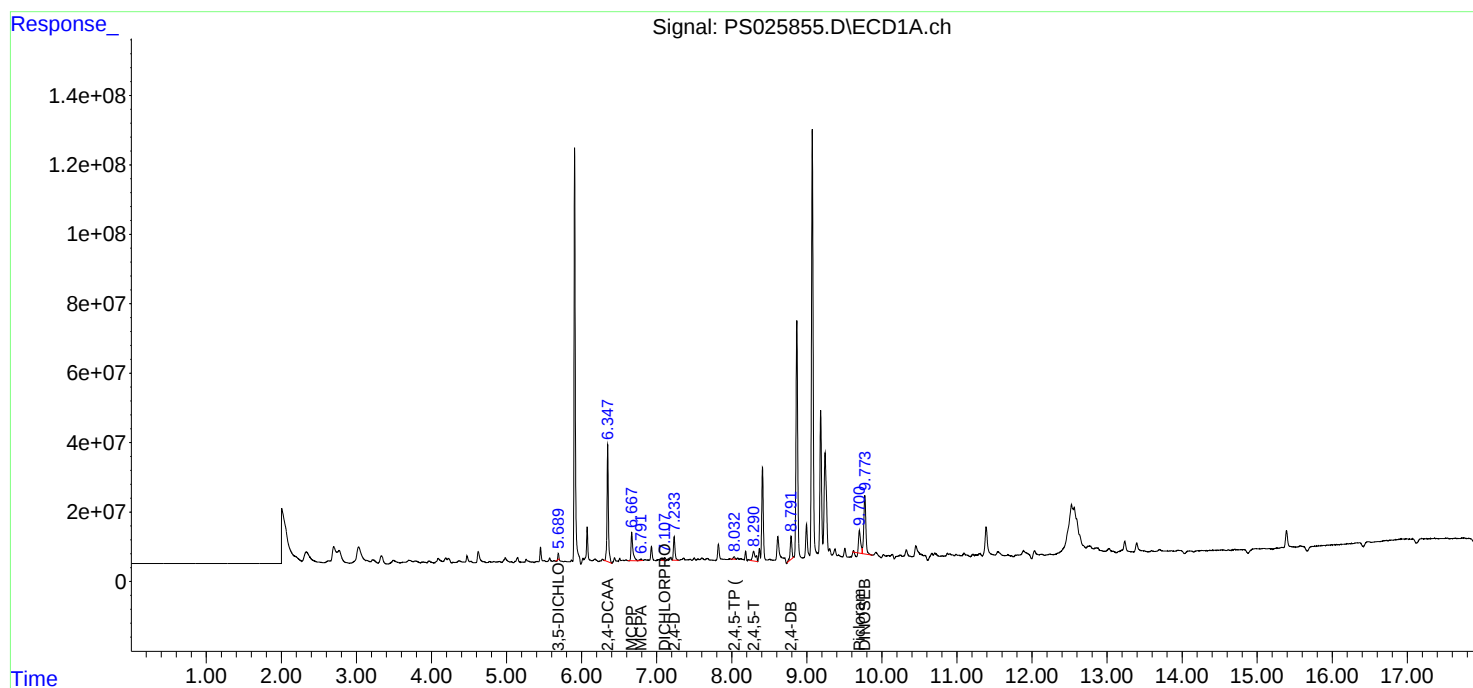


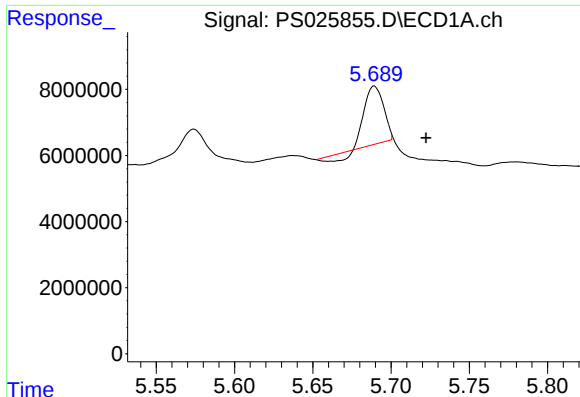

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.690 min
Delta R.T.: -0.033 min
Response: 14370827
Conc: 6.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6

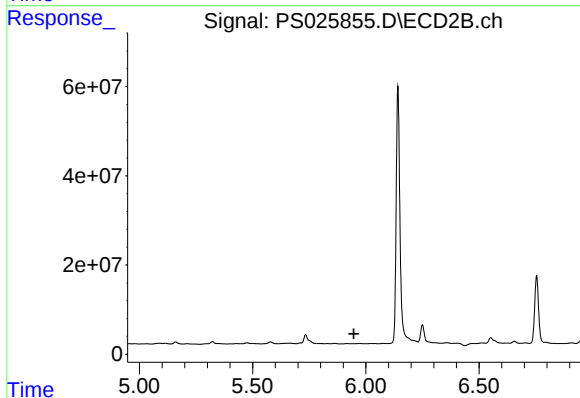


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.953 min
Delta R.T.: 0.005 min
Response: -332908
Conc: N.D.

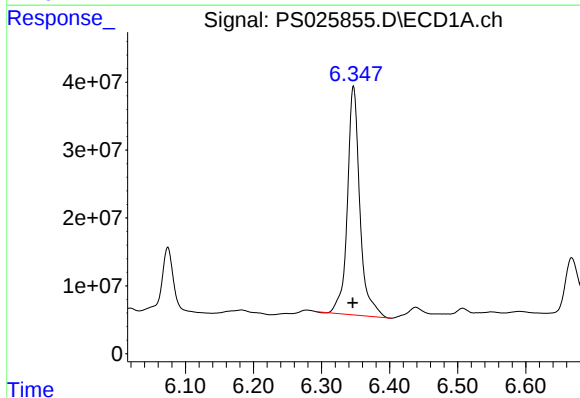


#4 2,4-DCAA

R.T.: 6.347 min
Delta R.T.: 0.001 min
Response: 429324708
Conc: 304.22 ng/ml

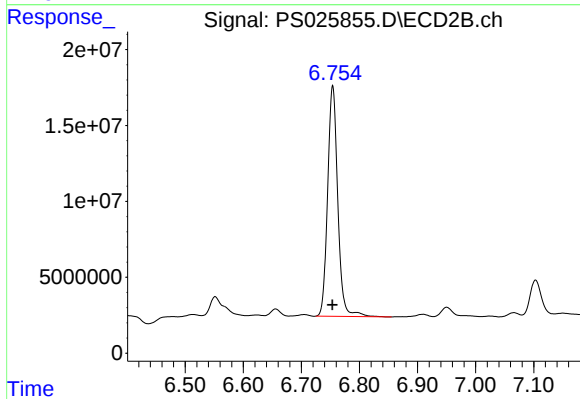

#4 2,4-DCAA


R.T.: 6.754 min
Delta R.T.: 0.000 min
Response: 184542340
Conc: 262.34 ng/ml

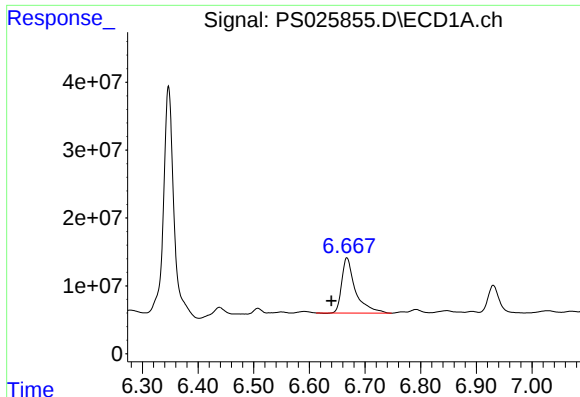

#6 MCPP


R.T.: 6.668 min
Delta R.T.: 0.029 min
Response: 138822188
Conc: 38.16 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-6

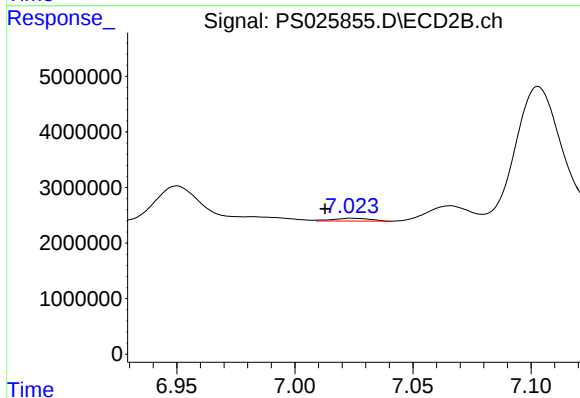


#6 MCPP

R.T.: 7.025 min
Delta R.T.: 0.012 min
Response: 536165
Conc: N.D.

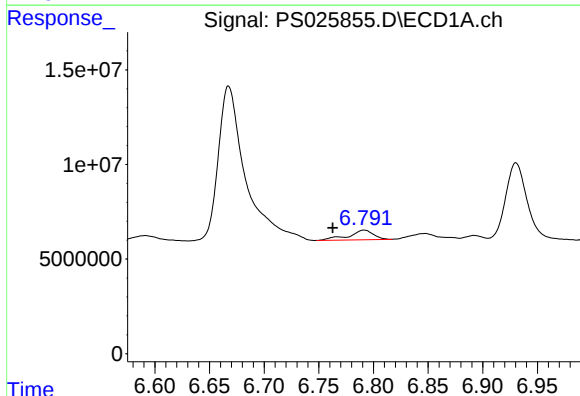


#7 MCPA

R.T.: 6.791 min
Delta R.T.: 0.029 min
Response: 7952349
Conc: 1.48 ug/ml

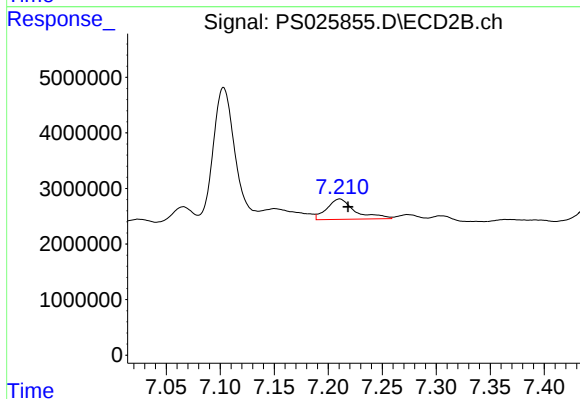

#7 MCPA


R.T.: 7.210 min
Delta R.T.: -0.008 min
Response: 6627204
Conc: 2.13 ug/ml

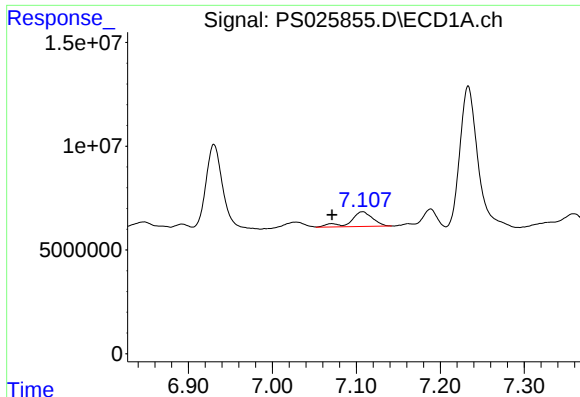

#8 DICHLORPROP


R.T.: 7.108 min
Delta R.T.: 0.037 min
Response: 13003787
Conc: 8.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6

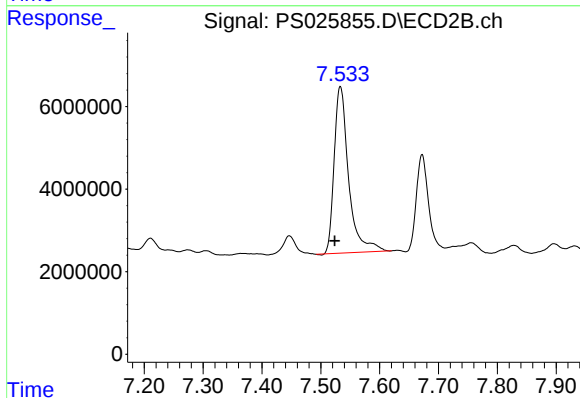


#8 DICHLORPROP

R.T.: 7.533 min
Delta R.T.: 0.010 min
Response: 69081130
Conc: 86.51 ng/ml

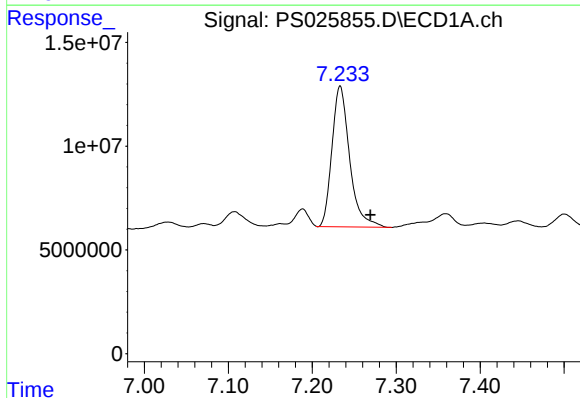


#9 2,4-D

R.T.: 7.234 min
Delta R.T.: -0.036 min
Response: 99271011
Conc: 55.86 ng/ml

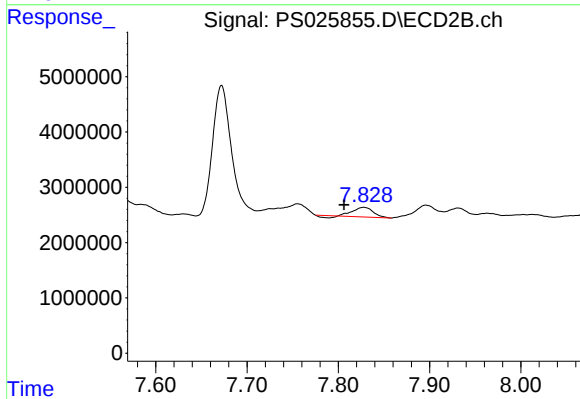

#9 2,4-D


R.T.: 7.828 min
Delta R.T.: 0.022 min
Response: 2404769
Conc: 2.82 ng/ml

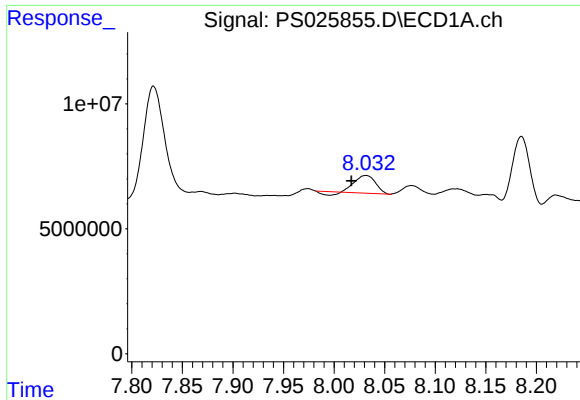

#11 2,4,5-TP (SILVEX)


R.T.: 8.031 min
Delta R.T.: 0.014 min
Response: 9060865
Conc: 1.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6

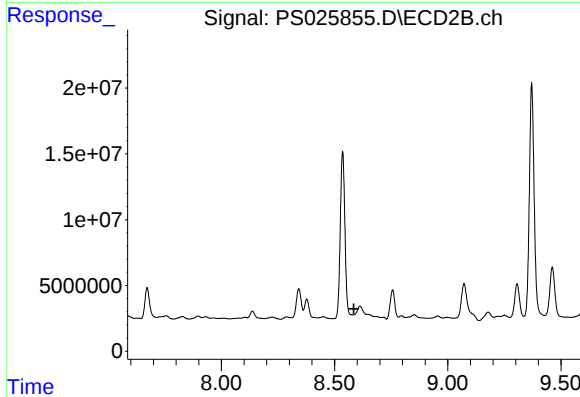


#11 2,4,5-TP (SILVEX)

R.T.: 8.612 min
Delta R.T.: 0.027 min
Response: -250468426
Conc: N.D.

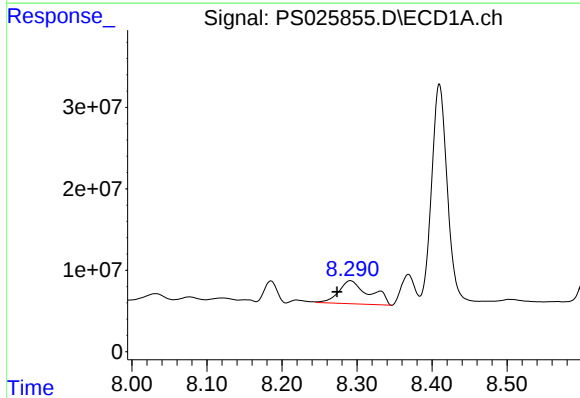


#12 2,4,5-T

R.T.: 8.291 min
Delta R.T.: 0.018 min
Response: 79611807
Conc: 8.41 ng/ml

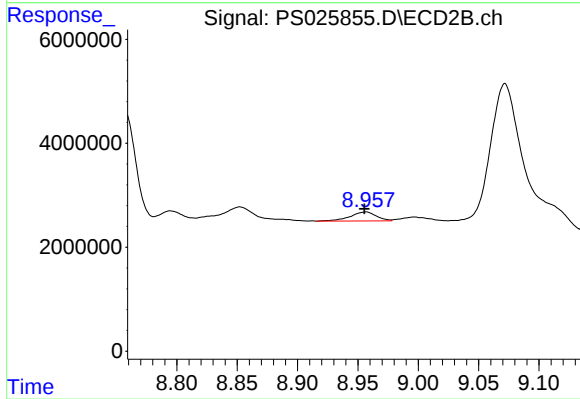

#12 2,4,5-T


R.T.: 8.956 min
Delta R.T.: 0.000 min
Response: 2624212
Conc: N.D.

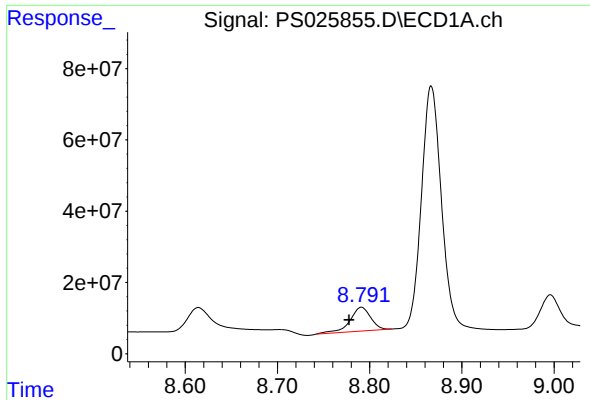

#13 2,4-DB


R.T.: 8.791 min
Delta R.T.: 0.013 min
Response: 104224599
Conc: 90.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6

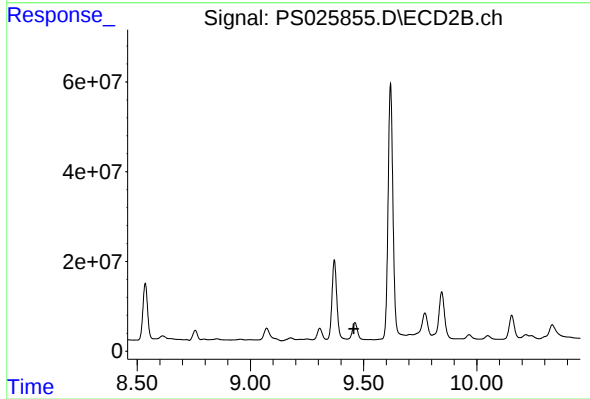


#13 2,4-DB

R.T.: 9.462 min
Delta R.T.: 0.004 min
Response: -450923446
Conc: N.D.

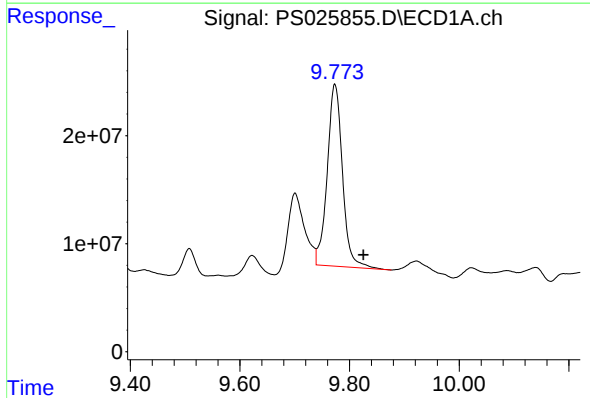


#14 DINOSEB

R.T.: 9.773 min
Delta R.T.: -0.052 min
Response: 325675700
Conc: 48.46 ng/ml

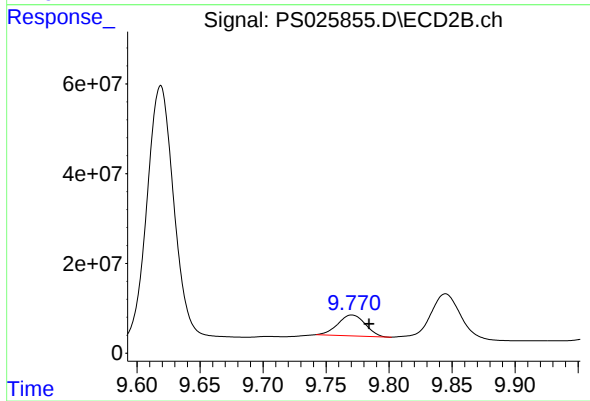

#14 DINOSEB


R.T.: 9.771 min
Delta R.T.: -0.014 min
Response: 70087411
Conc: 24.38 ng/ml

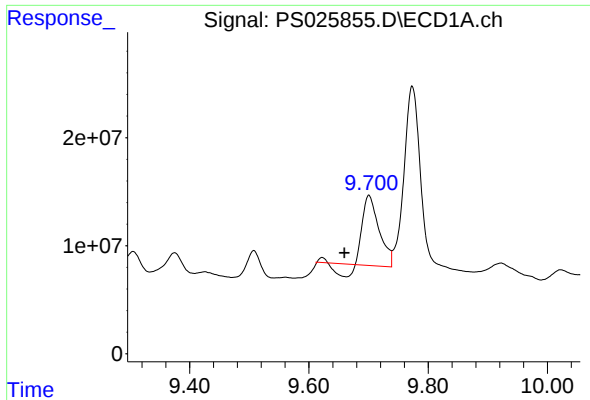

#15 Picloram

R.T.: 9.701 min
Delta R.T.: 0.042 min
Response: 106172378
Conc: 9.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6

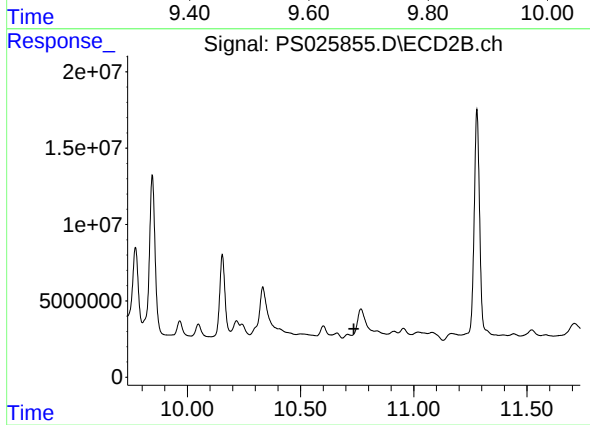

#15 Picloram

R.T.: 10.708 min
Delta R.T.: -0.028 min
Response: -2123721
Conc: N.D.