

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020819\
 Data File : PS003075.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2019 10:41
 Operator : EI\SJ
 Sample : PB116923BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB116923BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 22:10:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.315	10.809	279.3E6	281.0E6	735.623	657.135
Target Compounds							
1) T	Dalapon	2.833	2.314	16778018	92919382	30.414	173.382 #
3) T	4-Nitroph...	0.000	10.028	0	4665318	N.D.	22.320 #
8) T	DICHLORPROP	0.000	12.223	0	3603000	N.D.	9.424 #
9) T	2,4-D	13.176	12.677	8499829	2303739	18.435	4.595 #
12) T	2,4,5-T	14.845	14.415	5427749	4464858	2.225	2.333
13) T	2,4-DB	15.586	15.072	53372708	52676576	204.158	207.389
14) T	DINOSEB	0.000	15.482	0	6392964	N.D.	3.647 #
15) T	Picloram	16.834	16.739	7986744	31759863	2.525	10.564 #
16) T	DCPA	0.000	16.739	0	31759863	N.D.	10.253 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020819\
Data File : PS003075.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2019 10:41
Operator : EI\SJ
Sample : PB116923BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB116923BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 22:10:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

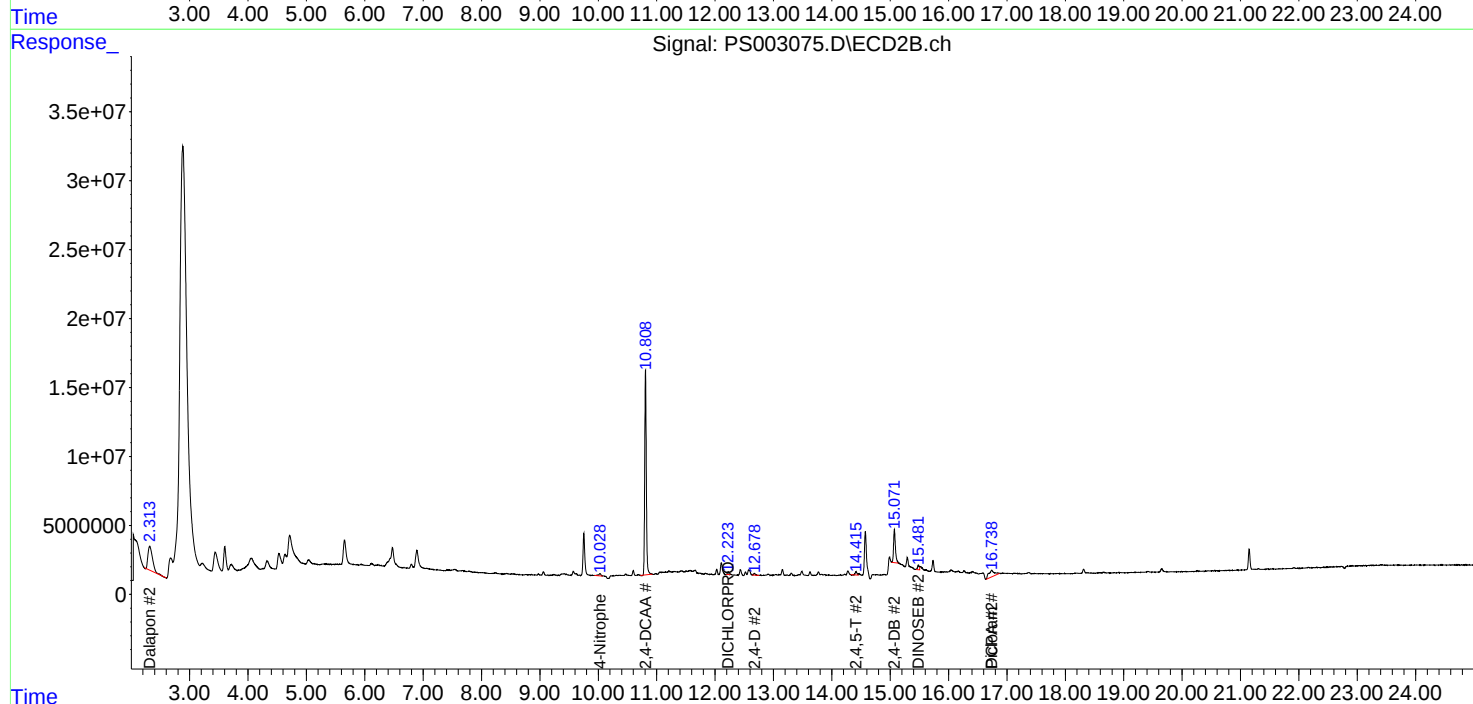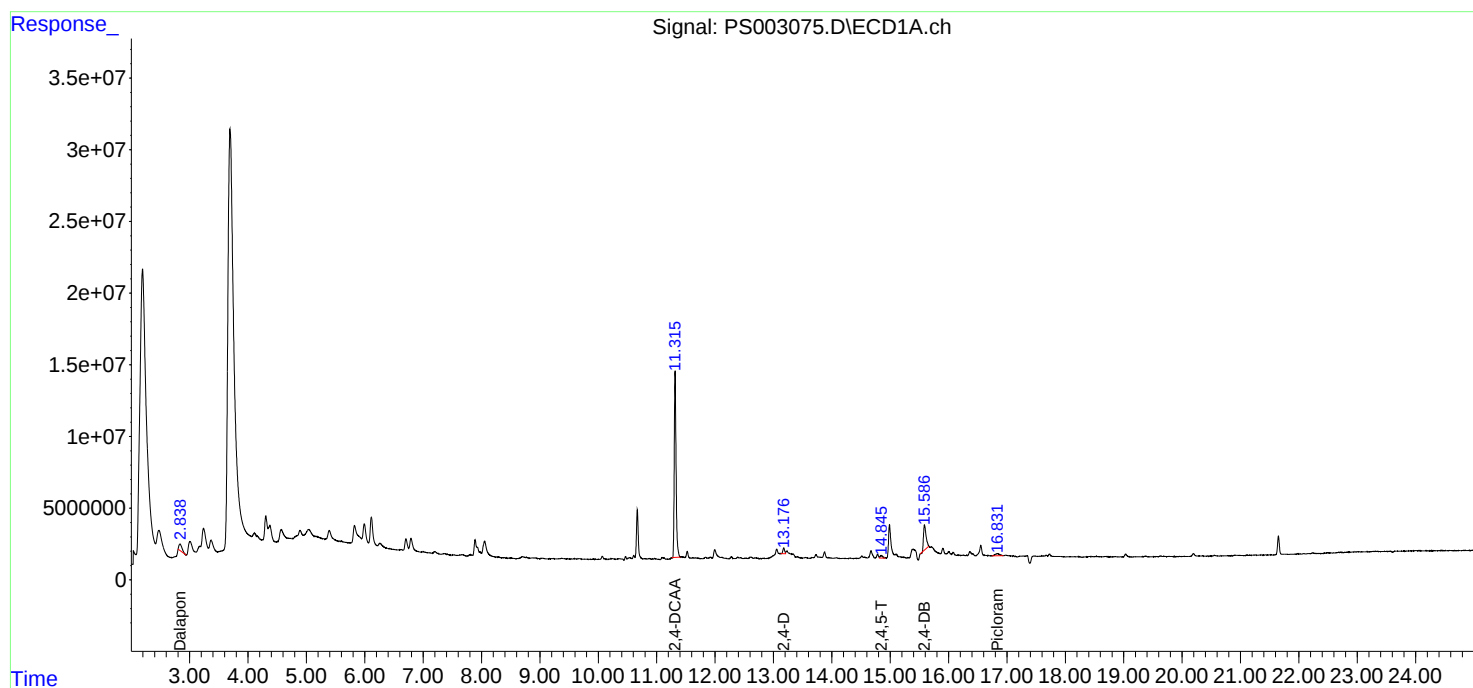


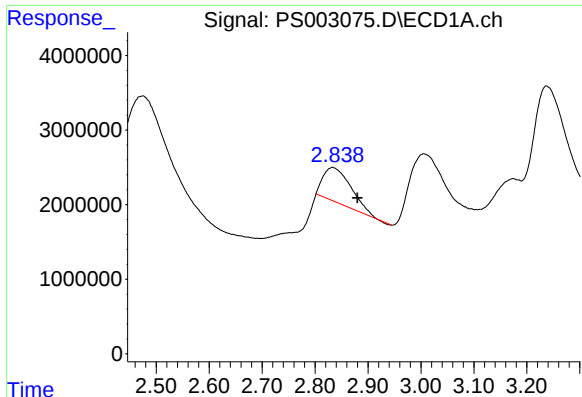

#1 Dalapon


R.T.: 2.833 min
Delta R.T.: -0.047 min
Response: 16778018
Conc: 30.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116923BL

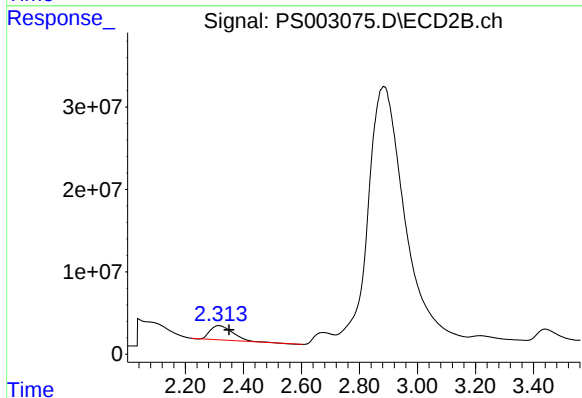


#1 Dalapon

R.T.: 2.314 min
Delta R.T.: -0.037 min
Response: 92919382
Conc: 173.38 ng/ml

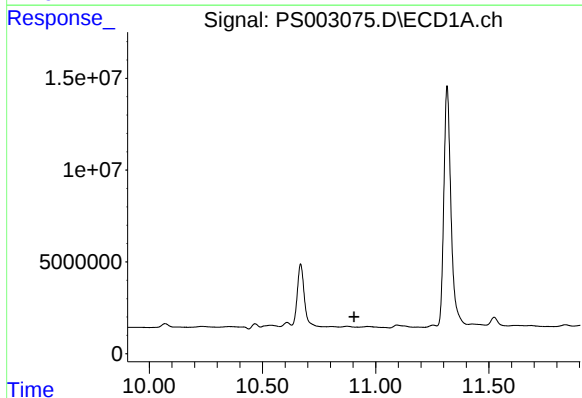


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.904 min
Response: 0
Conc: N.D.

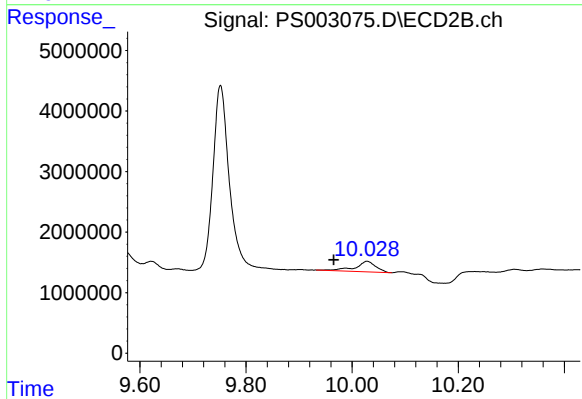

#3 4-Nitrophenol


R.T.: 10.028 min
Delta R.T.: 0.063 min
Response: 4665318
Conc: 22.32 ng/ml

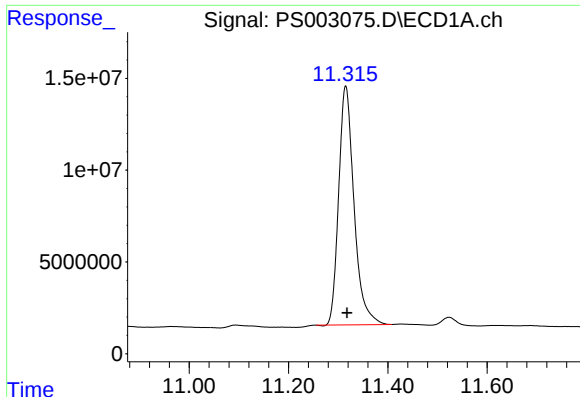

#4 2,4-DCAA


R.T.: 11.315 min
Delta R.T.: -0.003 min
Response: 279272465
Conc: 735.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116923BL

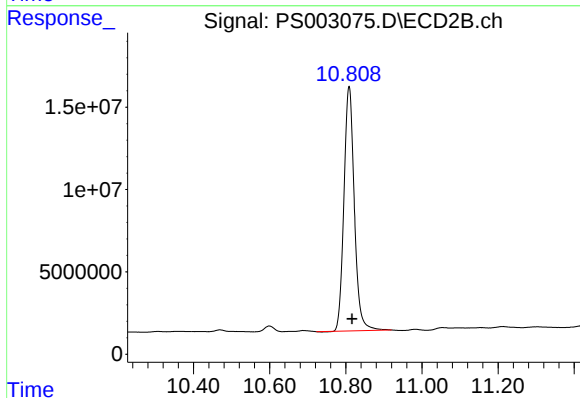


#4 2,4-DCAA

R.T.: 10.809 min
Delta R.T.: -0.008 min
Response: 280955068
Conc: 657.13 ng/ml

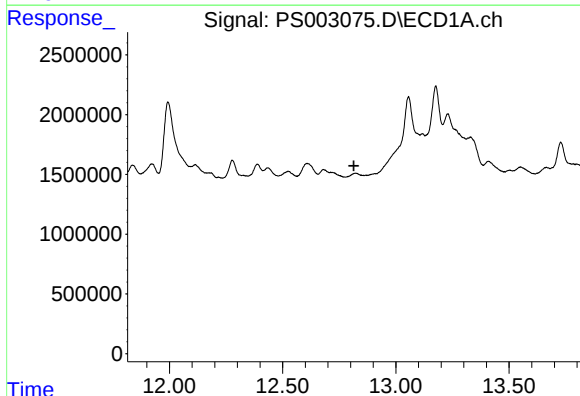


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.815 min
Response: 0
Conc: N.D.

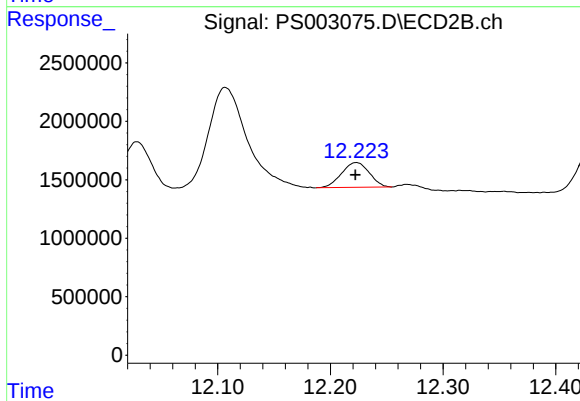

#8 DICHLORPROP


R.T.: 12.223 min
Delta R.T.: 0.000 min
Response: 3603000
Conc: 9.42 ng/ml

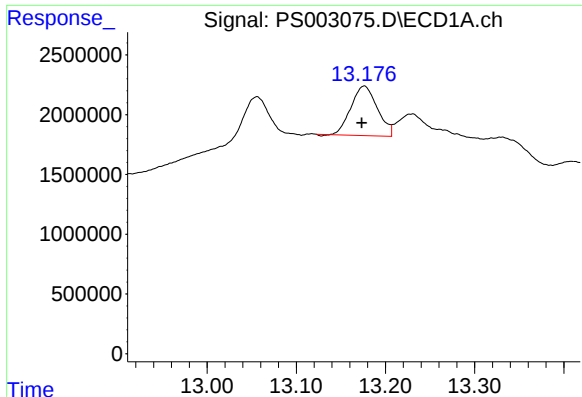

#9 2,4-D


R.T.: 13.176 min
Delta R.T.: 0.003 min
Response: 8499829
Conc: 18.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116923BL

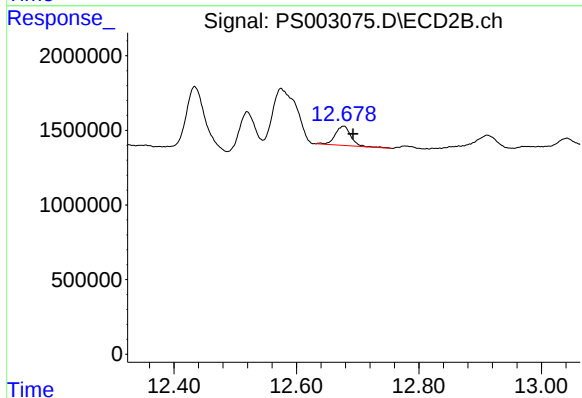


#9 2,4-D

R.T.: 12.677 min
Delta R.T.: -0.016 min
Response: 2303739
Conc: 4.59 ng/ml

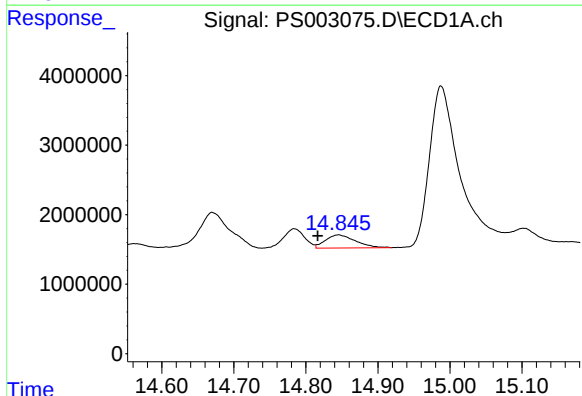


#12 2,4,5-T

R.T.: 14.845 min
Delta R.T.: 0.029 min
Response: 5427749
Conc: 2.23 ng/ml

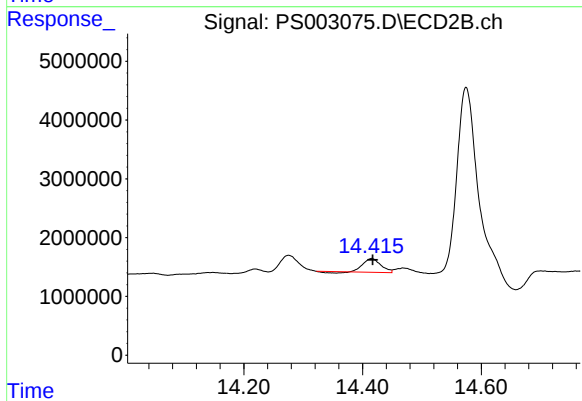

#12 2,4,5-T


R.T.: 14.415 min
Delta R.T.: -0.002 min
Response: 4464858
Conc: 2.33 ng/ml

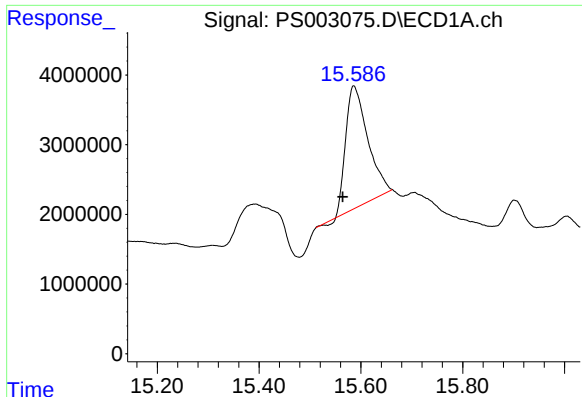

#13 2,4-DB


R.T.: 15.586 min
Delta R.T.: 0.022 min
Response: 53372708
Conc: 204.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116923BL

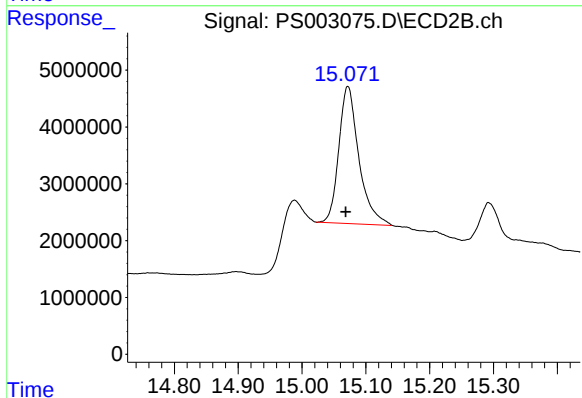


#13 2,4-DB

R.T.: 15.072 min
Delta R.T.: 0.003 min
Response: 52676576
Conc: 207.39 ng/ml

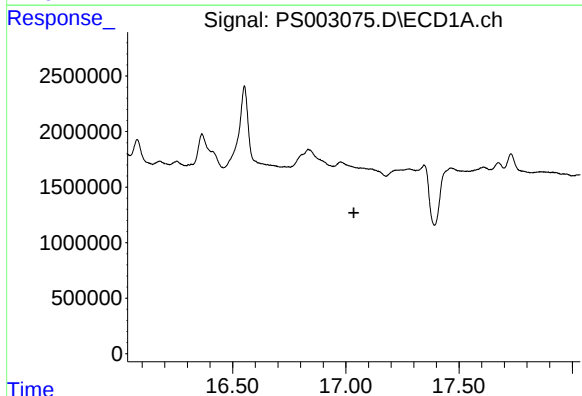


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

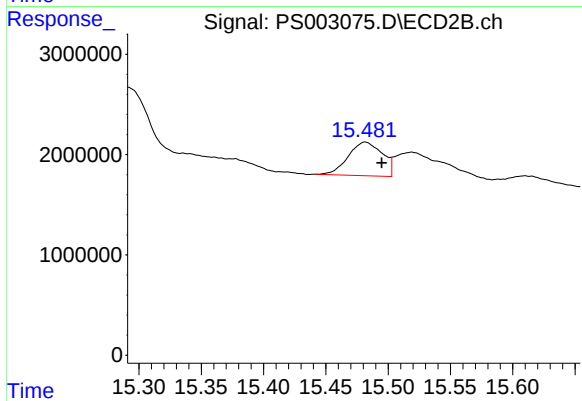

#14 DINOSEB


R.T.: 15.482 min
Delta R.T.: -0.013 min
Response: 6392964
Conc: 3.65 ng/ml

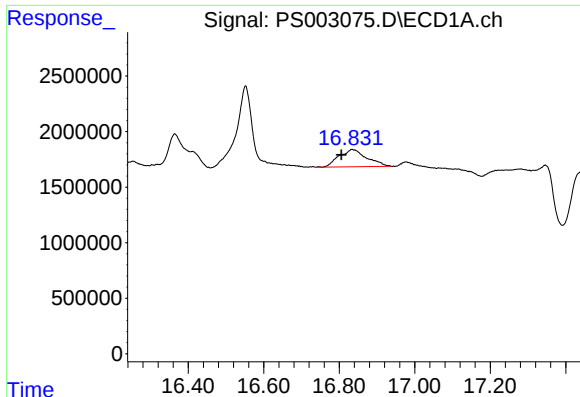

#15 Picloram


R.T.: 16.834 min
Delta R.T.: 0.028 min
Response: 7986744
Conc: 2.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116923BL

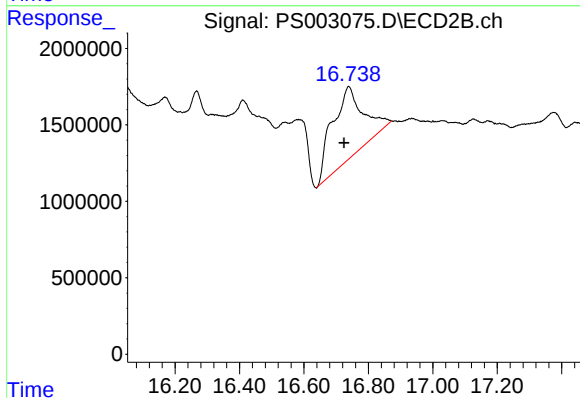


#15 Picloram

R.T.: 16.739 min
Delta R.T.: 0.015 min
Response: 31759863
Conc: 10.56 ng/ml

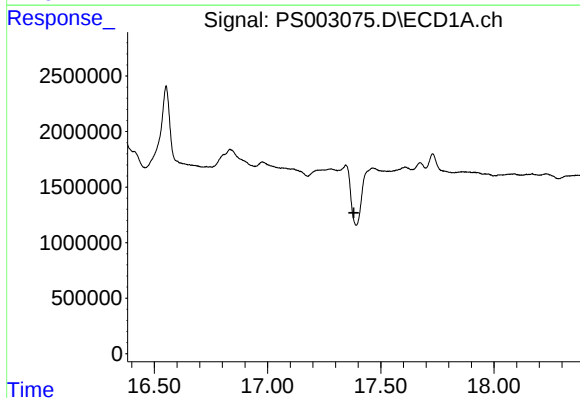

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

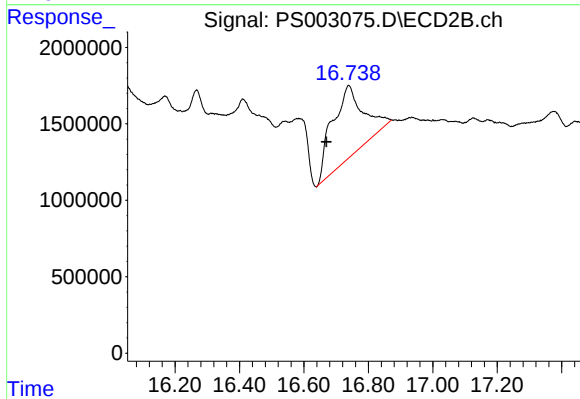

#16 DCPA

R.T.: 16.739 min
Delta R.T.: 0.069 min
Response: 31759863
Conc: 10.25 ng/ml