

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020819\
 Data File : PS003083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2019 14:50
 Operator : EI\SJ
 Sample : K1389-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 M-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 22:12:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.316	10.816	189.3E6	187.6E6	498.519	438.713
Target Compounds							
1) T	Dalapon	2.835	2.320	18341979	65930512	33.249	123.023 #
2) T	3,5-DICHL...	0.000	8.984	0	8332869	N.D.	14.786 #
6) T	MCPD	11.989	0.000	4247747	0	3.545	N.D. #
7) T	MCPA	0.000	11.771	0	166.7E6	N.D.	105.946 #
9) T	2,4-D	13.176	0.000	5855987	0	12.701	N.D. #
12) T	2,4,5-T	0.000	14.418	0	3567917	N.D.	1.865 #
14) T	DINOSEB	0.000	15.522	0	6895715	N.D.	3.934 #
15) T	Picloram	16.807	16.742	5804739	13536331	1.835	4.502 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020819\
Data File : PS003083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2019 14:50
Operator : EI\SJ
Sample : K1389-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
M-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 22:12:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

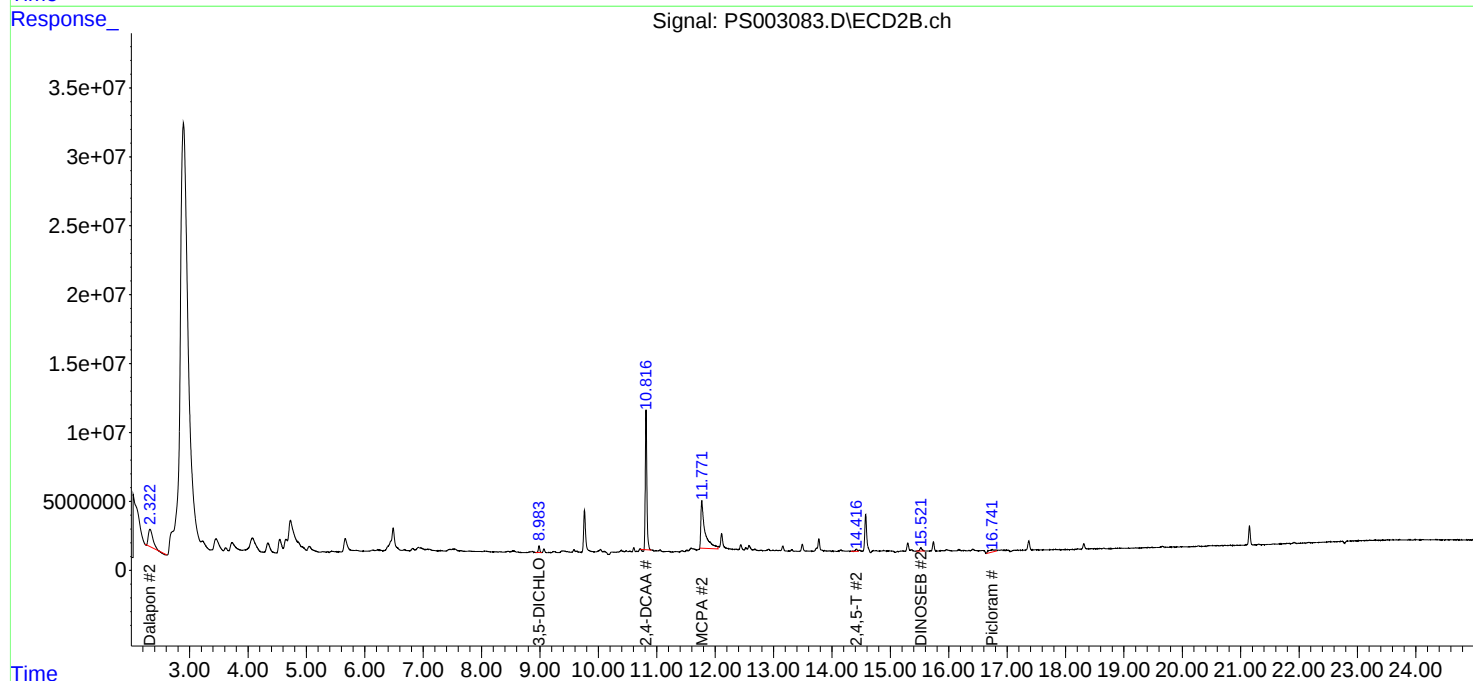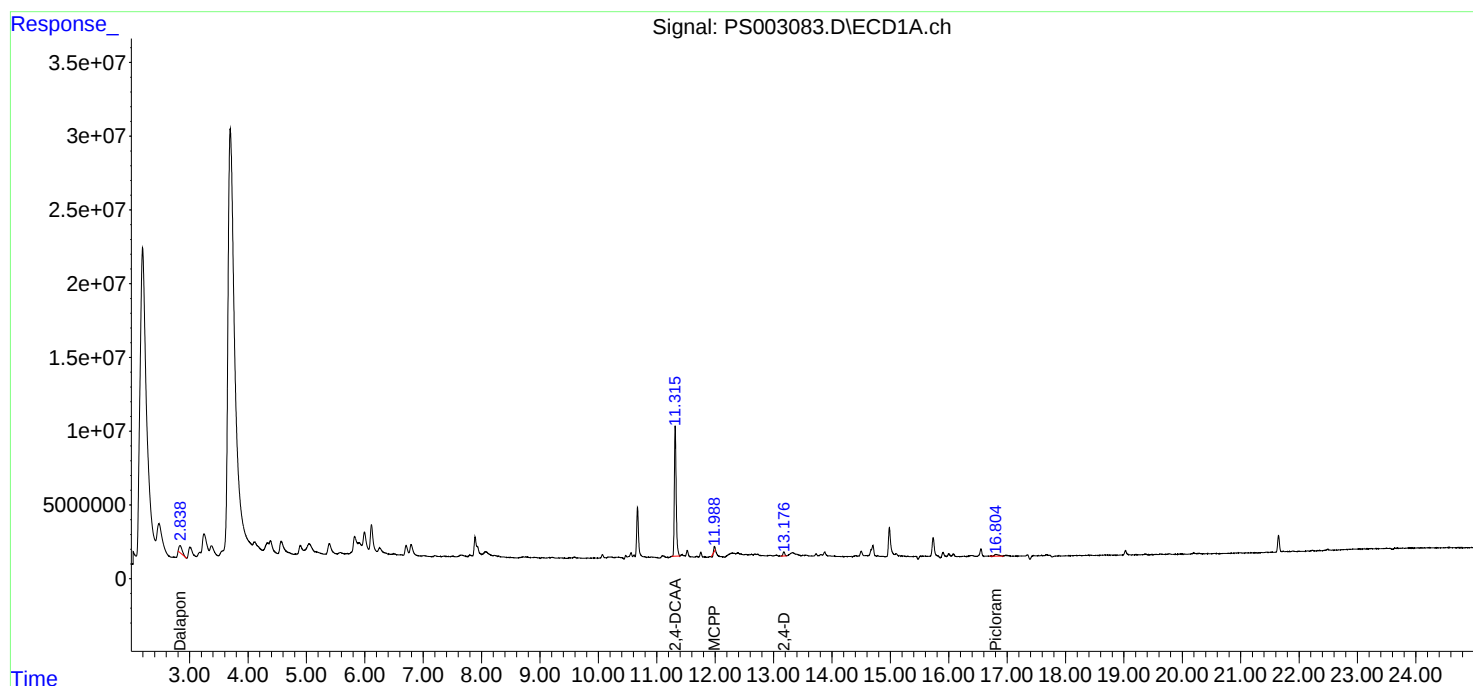


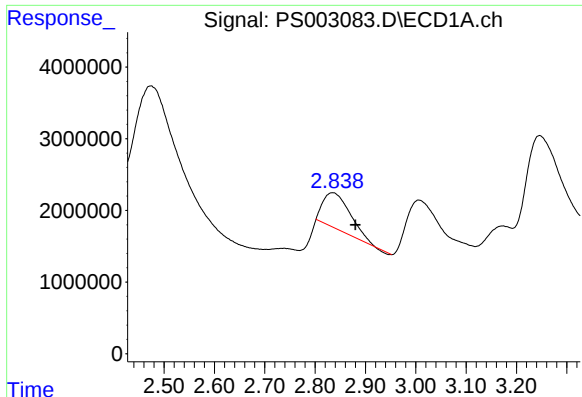

#1 Dalapon


R.T.: 2.835 min
Delta R.T.: -0.045 min
Response: 18341979
Conc: 33.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
M-6

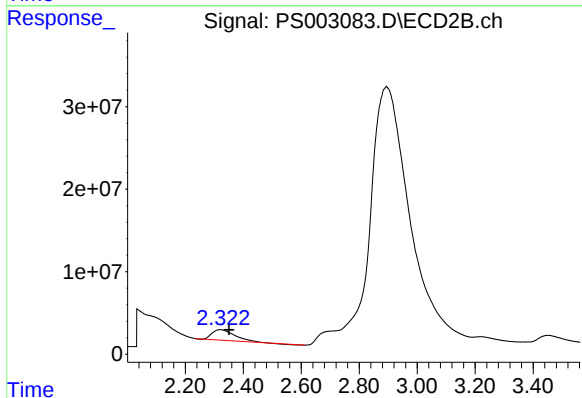


#1 Dalapon

R.T.: 2.320 min
Delta R.T.: -0.031 min
Response: 65930512
Conc: 123.02 ng/ml

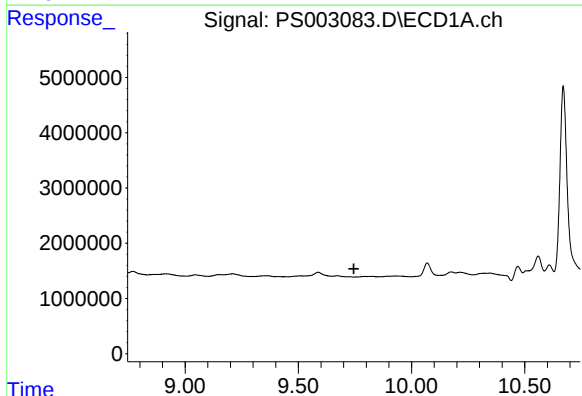


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

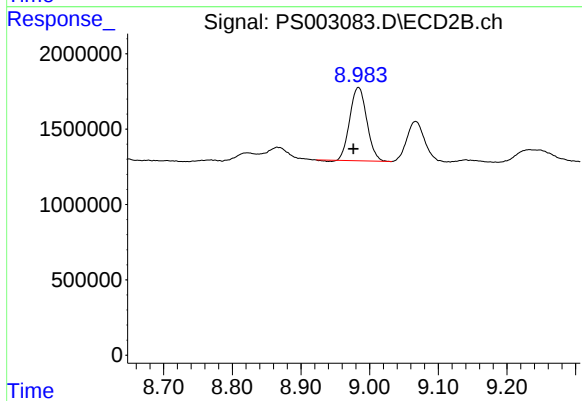

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.984 min
Delta R.T.: 0.007 min
Response: 8332869
Conc: 14.79 ng/ml

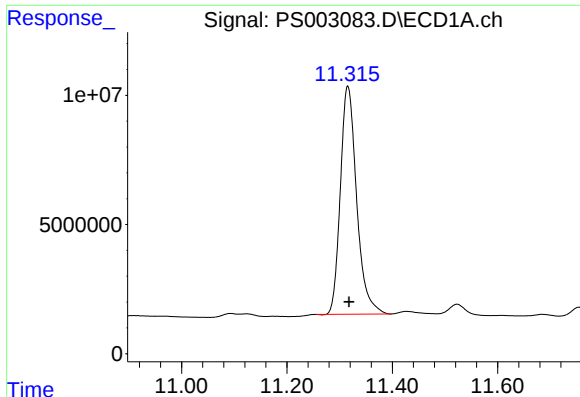

#4 2,4-DCAA


R.T.: 11.316 min
Delta R.T.: -0.002 min
Response: 189258180
Conc: 498.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
M-6

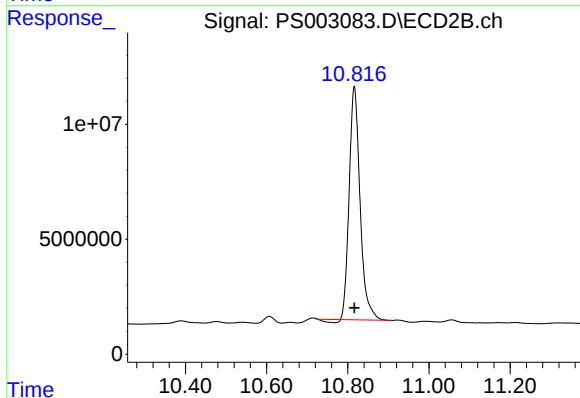


#4 2,4-DCAA

R.T.: 10.816 min
Delta R.T.: 0.000 min
Response: 187569943
Conc: 438.71 ng/ml

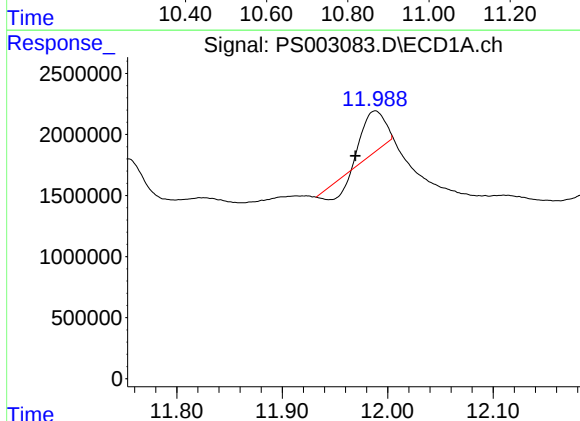


#6 MCP

R.T.: 11.989 min
Delta R.T.: 0.019 min
Response: 4247747
Conc: 3.55 ug/ml

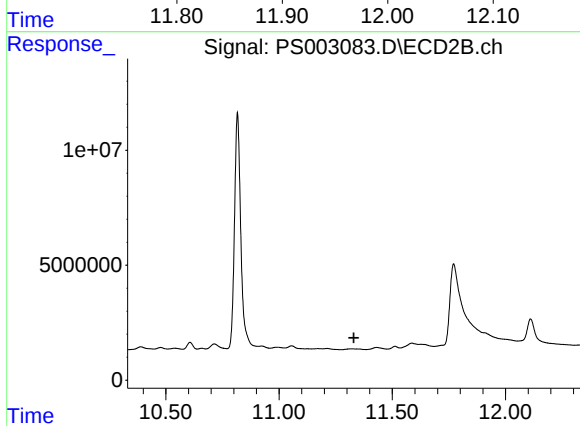

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

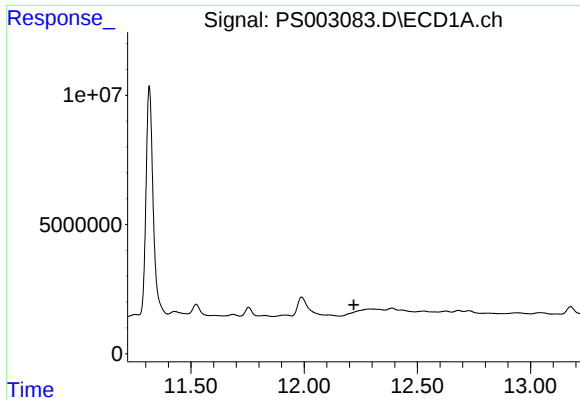

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-6

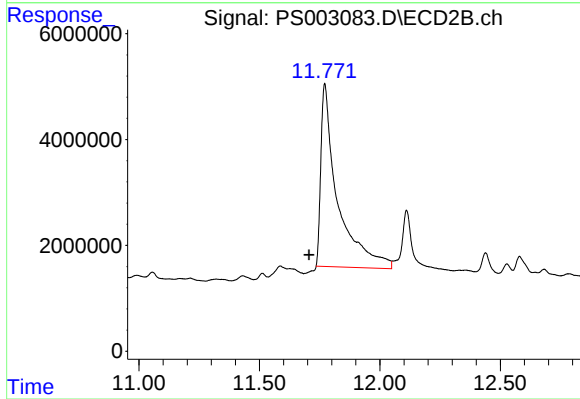


#7 MCPA

R.T.: 11.771 min
Delta R.T.: 0.065 min
Response: 166659500
Conc: 105.95 ug/ml

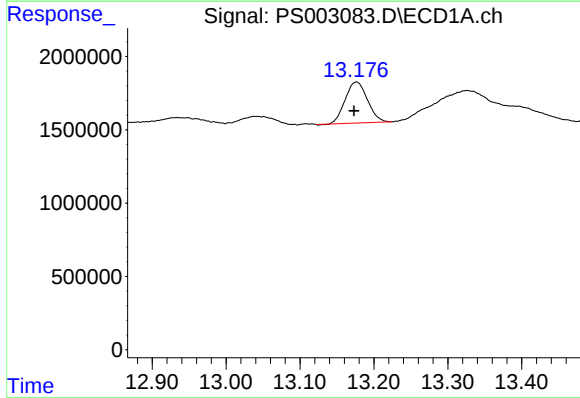


#9 2,4-D

R.T.: 13.176 min
Delta R.T.: 0.003 min
Response: 5855987
Conc: 12.70 ng/ml

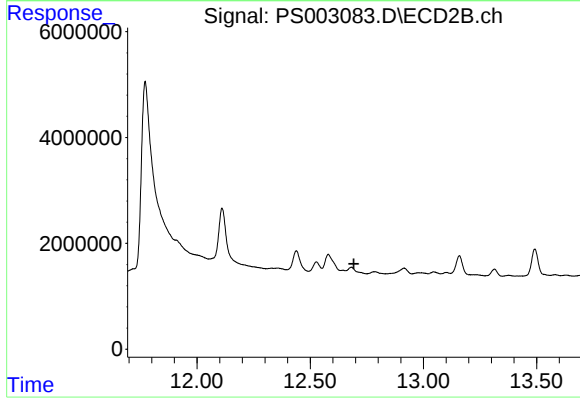

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 12.693 min
Response: 0
Conc: N.D.

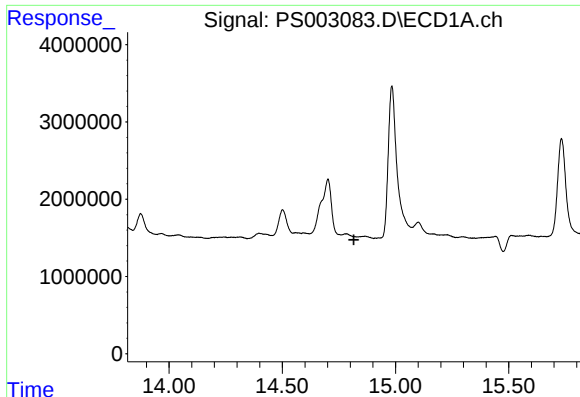

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-6

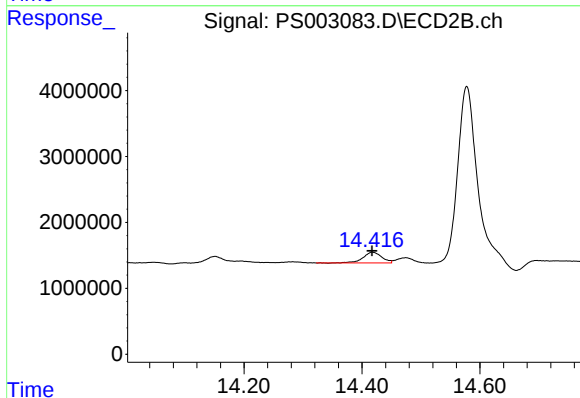


#12 2,4,5-T

R.T.: 14.418 min
Delta R.T.: 0.000 min
Response: 3567917
Conc: 1.86 ng/ml

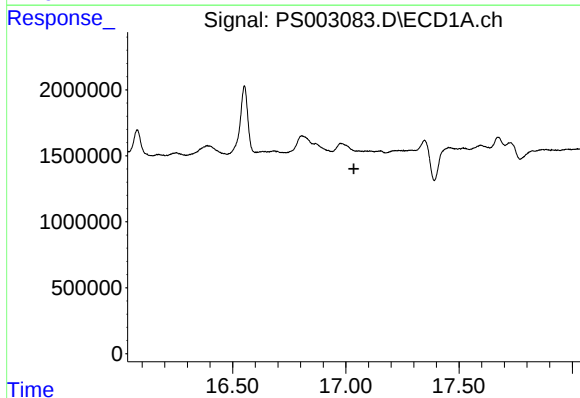


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

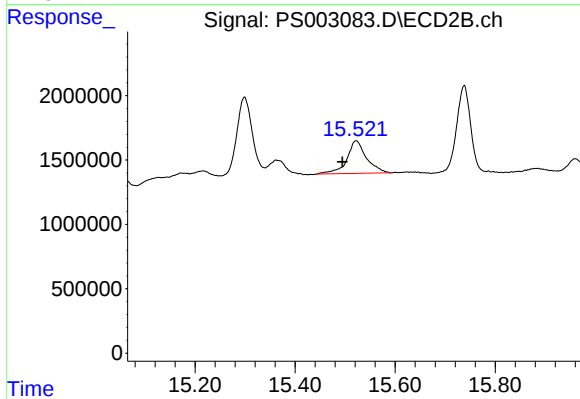

#14 DINOSEB


R.T.: 15.522 min
Delta R.T.: 0.027 min
Response: 6895715
Conc: 3.93 ng/ml

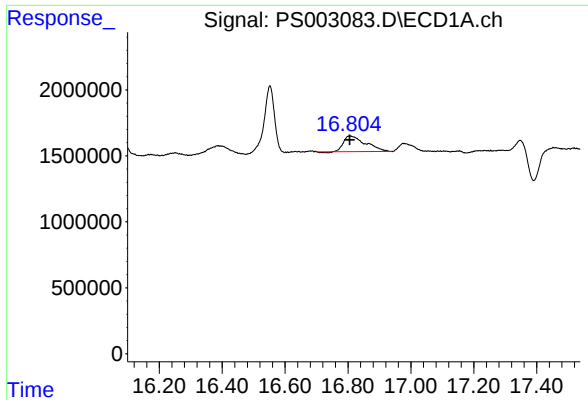

#15 Picloram

R.T.: 16.807 min
Delta R.T.: 0.001 min
Response: 5804739
Conc: 1.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
M-6

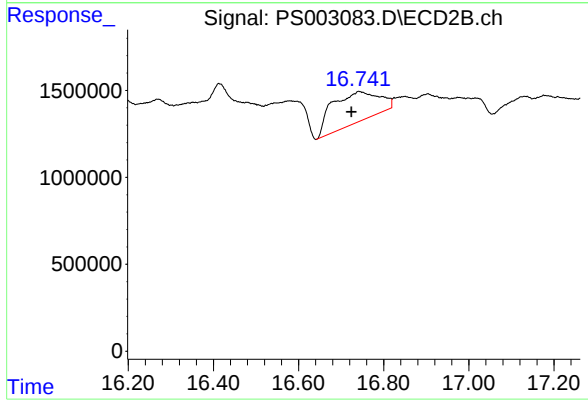

#15 Picloram

R.T.: 16.742 min
Delta R.T.: 0.018 min
Response: 13536331
Conc: 4.50 ng/ml