

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020819\
 Data File : PS003084.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2019 15:21
 Operator : EI\SJ
 Sample : K1389-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 M-5S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 22:12:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.281	10.781	163.9E6	214.8E6	431.784	502.339
Target Compounds							
1) T	Dalapon	0.000	2.285	0	74246015	N.D.	138.539 #
2) T	3,5-DICHL...	0.000	8.948	0	8348790	N.D.	14.814 #
3) T	4-Nitroph...	0.000	10.003	0	6267947	N.D.	29.987 #
6) T	MCP	11.954	0.000	10265074	0	8.568	N.D. #
9) T	2,4-D	13.141	0.000	4219729	0	9.152	N.D. #
10) T	Pentachlo...	0.000	13.277	0	1833630	N.D.	0.297 #
11) T	2,4,5-TP ...	14.469	0.000	8199551	0	3.256	N.D. #
12) T	2,4,5-T	0.000	14.438	0	3089214	N.D.	1.614 #
14) T	DINOSEB	0.000	15.487	0	6705319	N.D.	3.825 #
15) T	Picloram	16.770	16.712	2125230	15758740	0.672	5.242 #
16) T	DCPA	17.422	16.712	-6304651	15758740	N.D.	5.087



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020819\
Data File : PS003084.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2019 15:21
Operator : EI\SJ
Sample : K1389-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
M-5S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 22:12:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

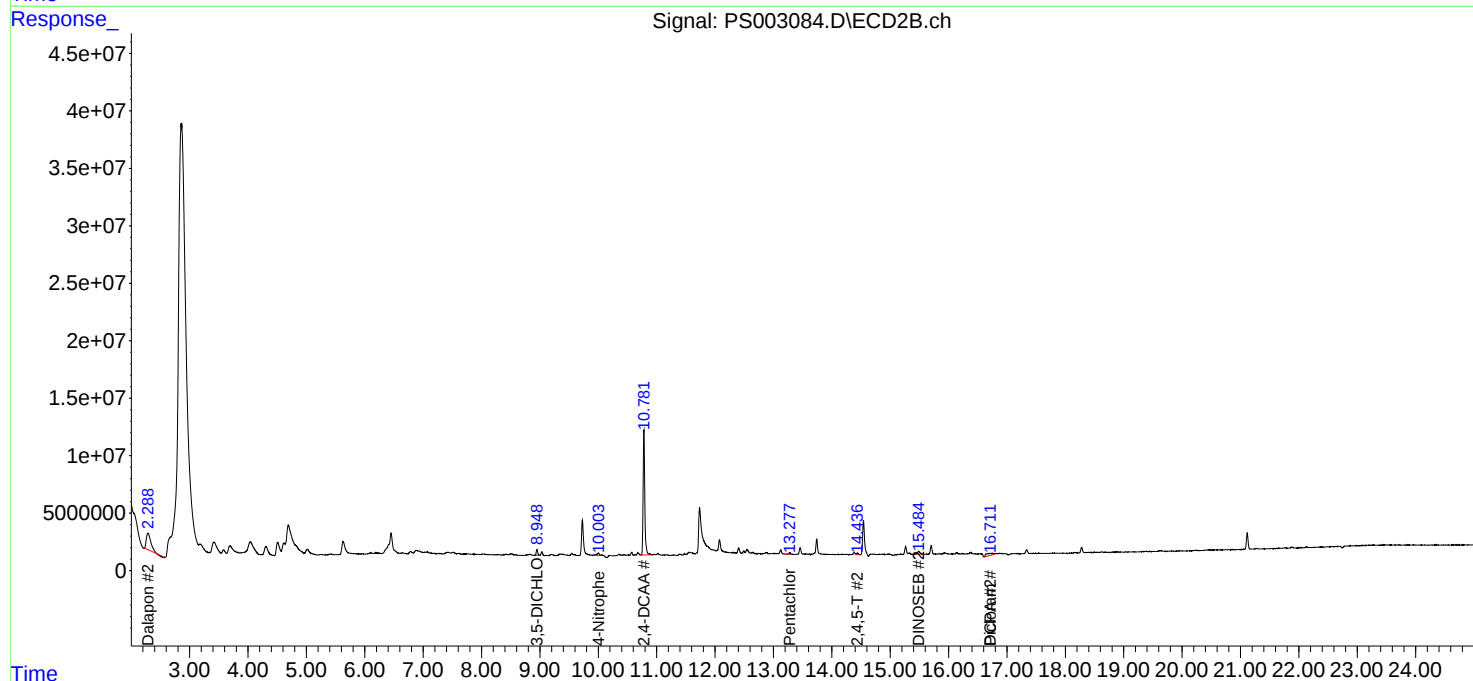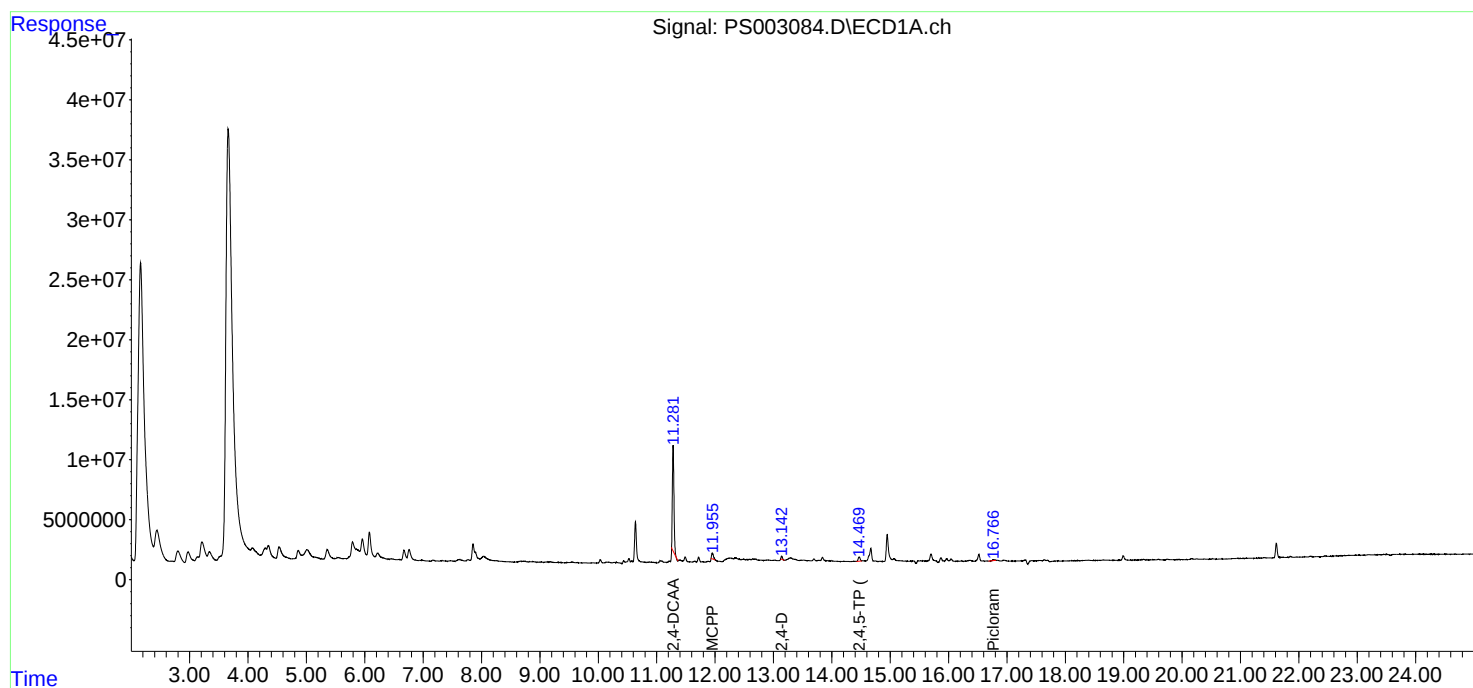


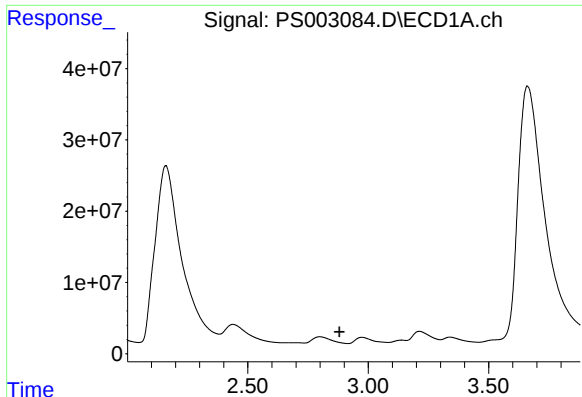

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-5S

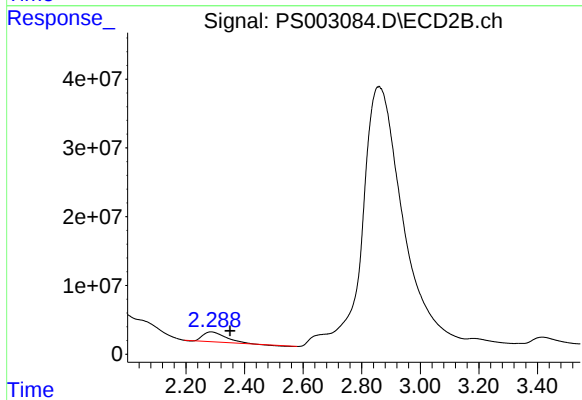


#1 Dalapon

R.T.: 2.285 min
Delta R.T.: -0.066 min
Response: 74246015
Conc: 138.54 ng/ml

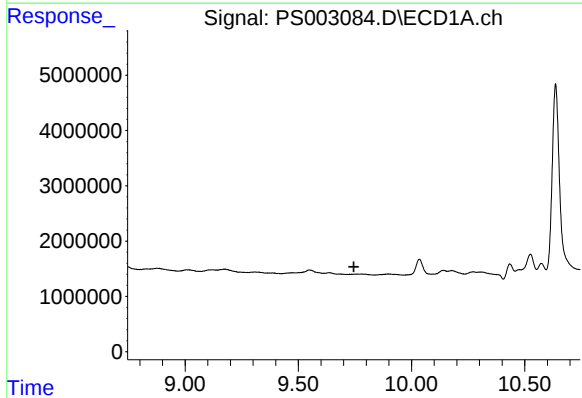


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

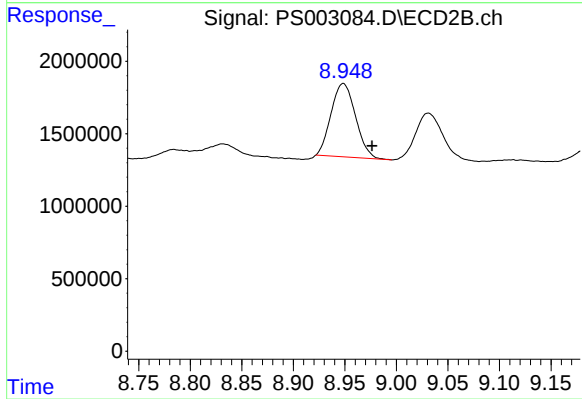

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.948 min
Delta R.T.: -0.028 min
Response: 8348790
Conc: 14.81 ng/ml

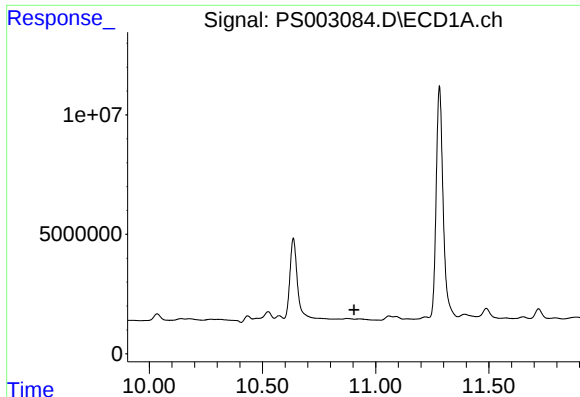

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-5S

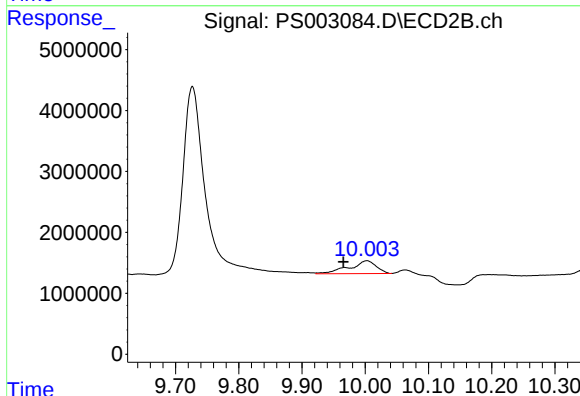


#3 4-Nitrophenol

R.T.: 10.003 min
Delta R.T.: 0.037 min
Response: 6267947
Conc: 29.99 ng/ml

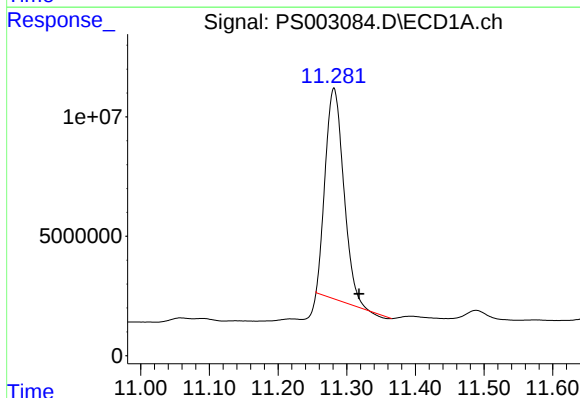


#4 2,4-DCAA

R.T.: 11.281 min
Delta R.T.: -0.036 min
Response: 163922643
Conc: 431.78 ng/ml

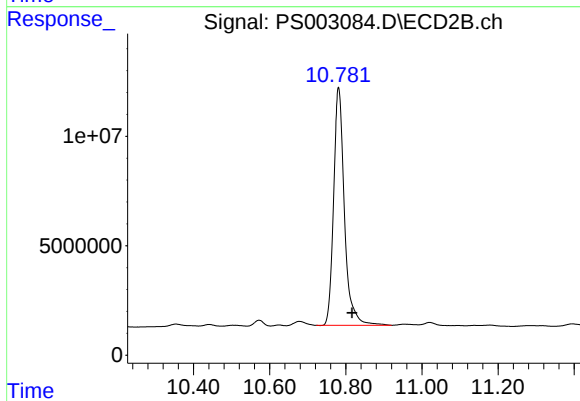

#4 2,4-DCAA


R.T.: 10.781 min
Delta R.T.: -0.035 min
Response: 214772783
Conc: 502.34 ng/ml

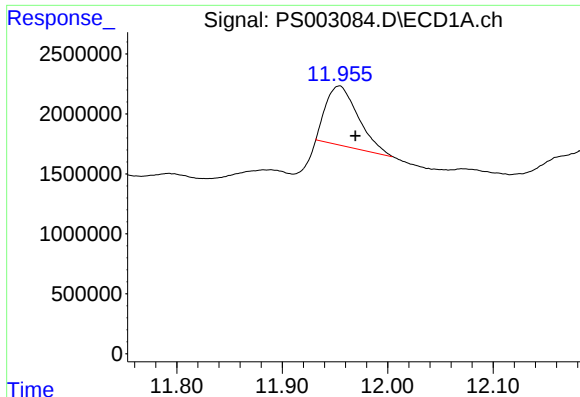

#6 MCP


R.T.: 11.954 min
Delta R.T.: -0.015 min
Response: 10265074
Conc: 8.57 ug/ml

Instrument :
ECD_S
ClientSampleId :
M-5S

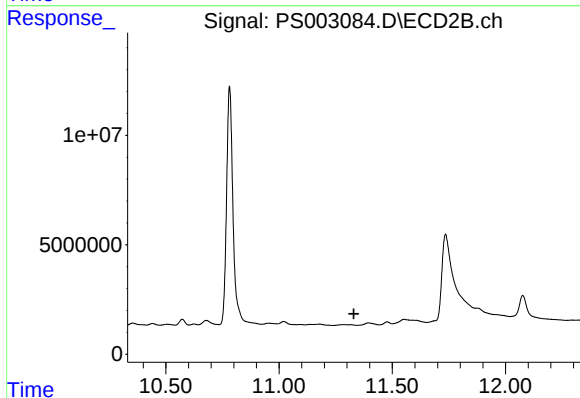


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

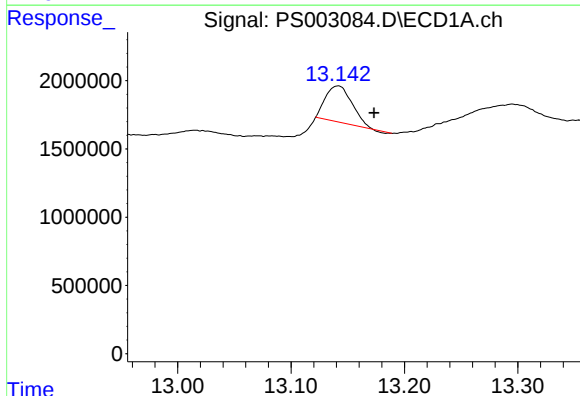


#9 2,4-D

R.T.: 13.141 min
Delta R.T.: -0.032 min
Response: 4219729
Conc: 9.15 ng/ml

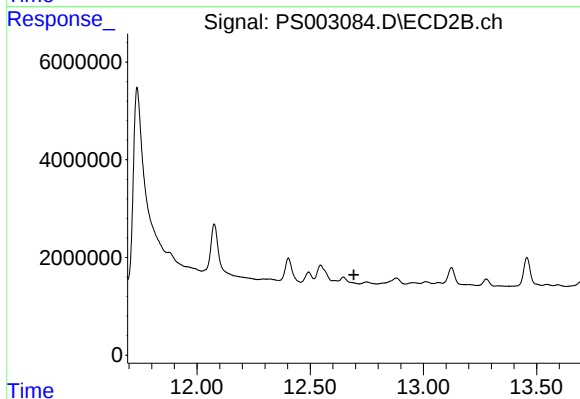

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 12.693 min
Response: 0
Conc: N.D.

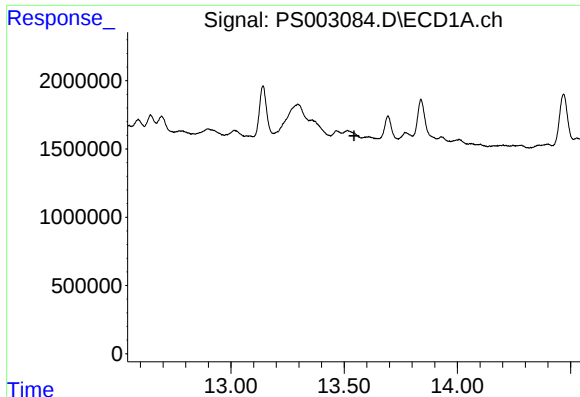

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.543 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-5S

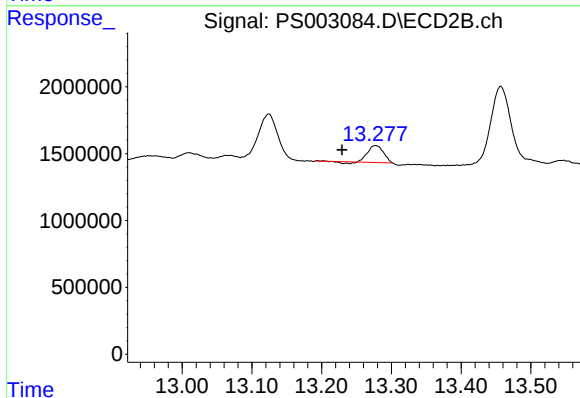


#10 Pentachlorophenol

R.T.: 13.277 min
Delta R.T.: 0.048 min
Response: 1833630
Conc: 0.30 ng/ml

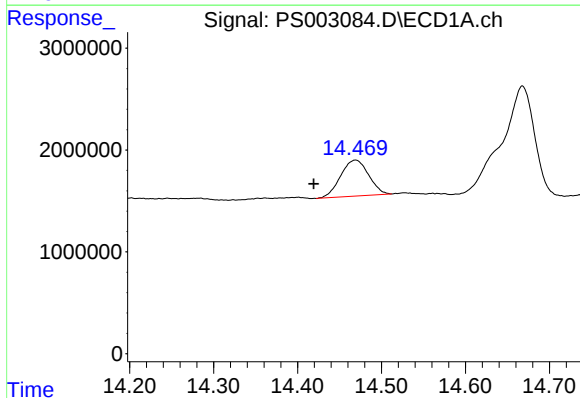


#11 2,4,5-TP (SILVEX)

R.T.: 14.469 min
Delta R.T.: 0.049 min
Response: 8199551
Conc: 3.26 ng/ml

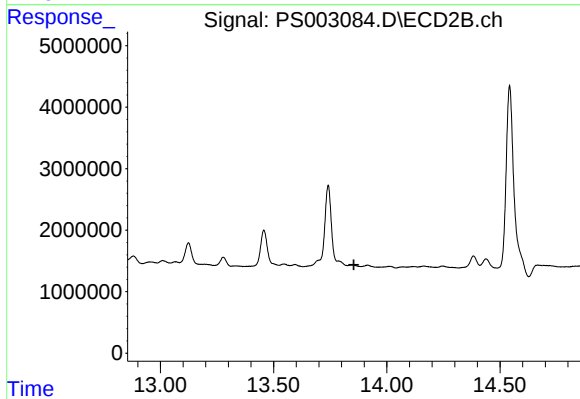

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 13.854 min
Response: 0
Conc: N.D.

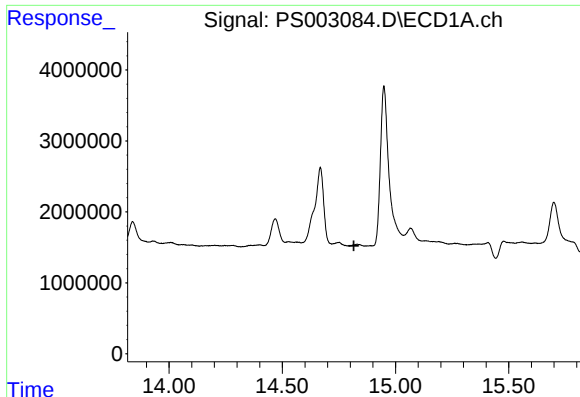

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-5S

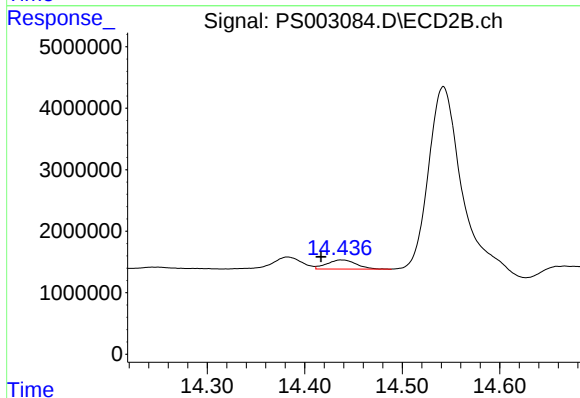


#12 2,4,5-T

R.T.: 14.438 min
Delta R.T.: 0.021 min
Response: 3089214
Conc: 1.61 ng/ml

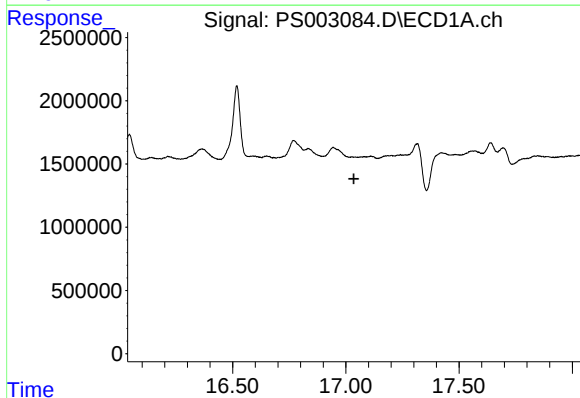


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

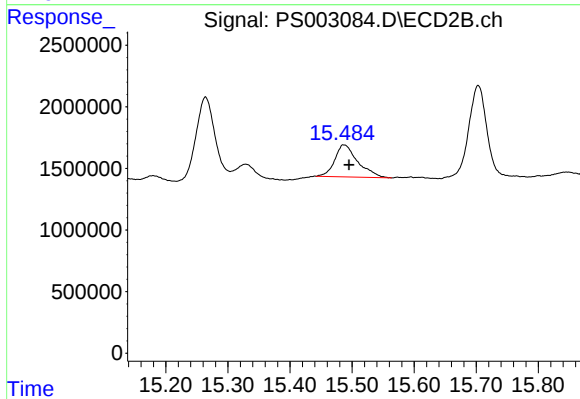

#14 DINOSEB


R.T.: 15.487 min
Delta R.T.: -0.008 min
Response: 6705319
Conc: 3.83 ng/ml

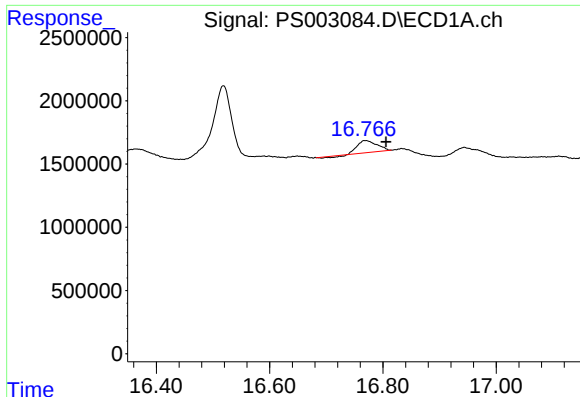

#15 Picloram


R.T.: 16.770 min
Delta R.T.: -0.036 min
Response: 2125230
Conc: 0.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
M-5S

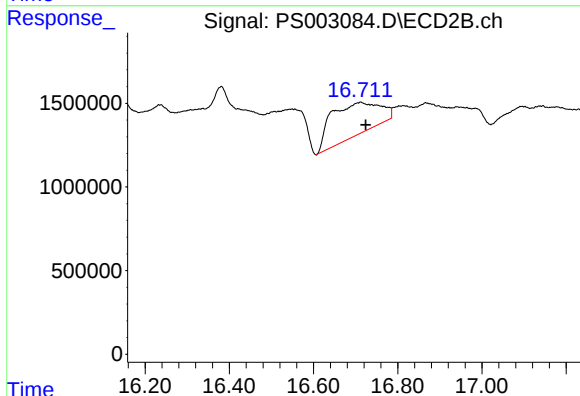


#15 Picloram

R.T.: 16.712 min
Delta R.T.: -0.012 min
Response: 15758740
Conc: 5.24 ng/ml

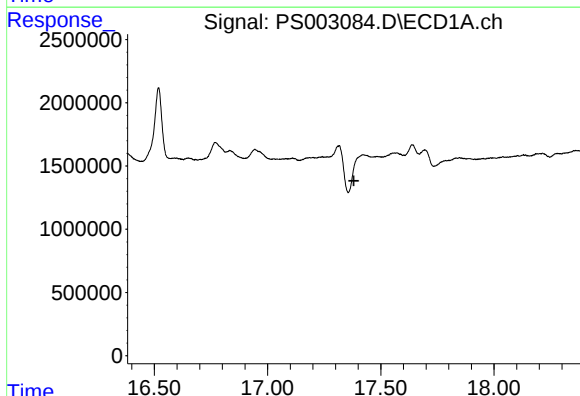

#16 DCPA

R.T.: 17.422 min
Delta R.T.: 0.041 min
Response: -6304651
Conc: N.D.

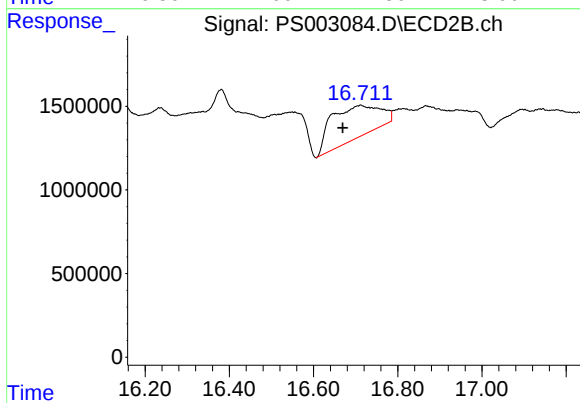

#16 DCPA

R.T.: 16.712 min
Delta R.T.: 0.042 min
Response: 15758740
Conc: 5.09 ng/ml