

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020819\
 Data File : PS003086.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2019 16:23
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 22:13:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.283	10.783	214.3E6	325.1E6	564.378	760.312 #
Target Compounds							
1) T	Dalapon	2.843	2.315	157.2E6	368.8E6	284.959	688.239 #
2) T	3,5-DICHL...	0.000	8.943	0	238.0E6	N.D.	422.354 #
3) T	4-Nitroph...	0.000	9.932	0	152.3E6	N.D.	728.469 #
5) T	DICAMBA	0.000	11.063	0	721.8E6	N.D.	454.916 #
8) T	DICHLORPROP	0.000	12.189	0	277.6E6	N.D.	726.066 #
9) T	2,4-D	0.000	12.660	0	316.3E6	N.D.	630.921 #
10) T	Pentachlo...	13.507	13.195	2102.4E6	1468.7E6	327.827	237.638 #
11) T	2,4,5-TP ...	14.384	13.821	1864.6E6	1802.8E6	740.381	726.836
12) T	2,4,5-T	14.782	14.383	1804.5E6	1141.6E6	739.732	596.631
14) T	DINOSEB	16.998	15.460	1361.8E6	35739229	723.848	20.388 #
15) T	Picloram	16.770	16.690	2270.1E6	2139.8E6	717.575	711.754
16) T	DCPA	17.344	16.690	1073.1E6	2139.8E6	356.846	690.802 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020819\
Data File : PS003086.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2019 16:23
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 22:13:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

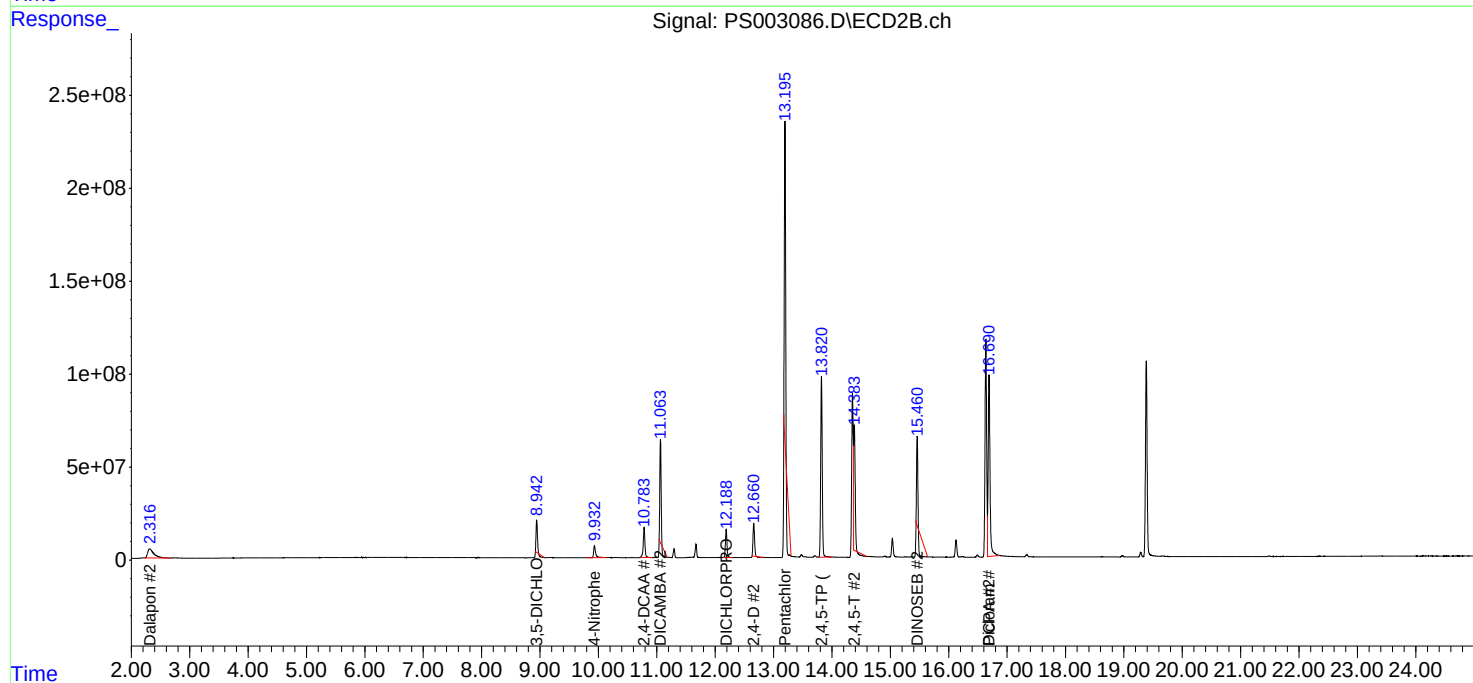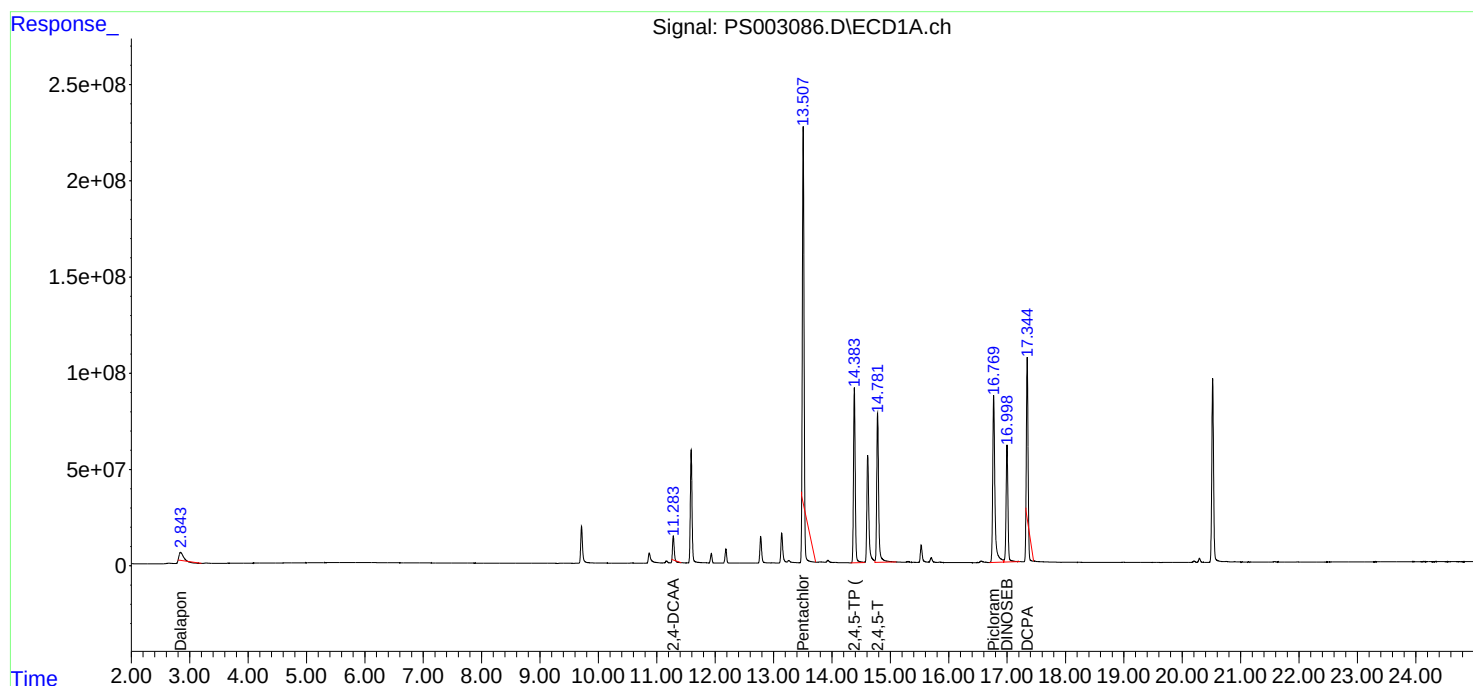


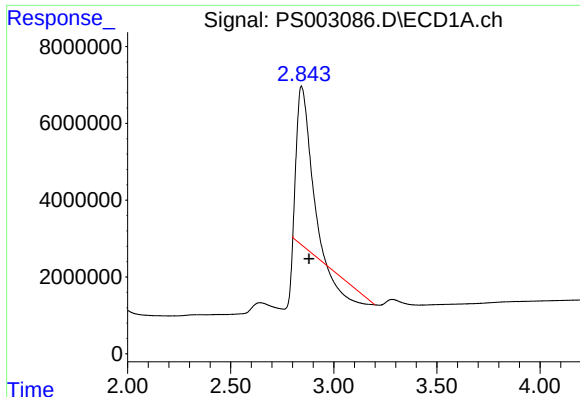

#1 Dalapon


R.T.: 2.843 min
Delta R.T.: -0.037 min
Response: 157196927
Conc: 284.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

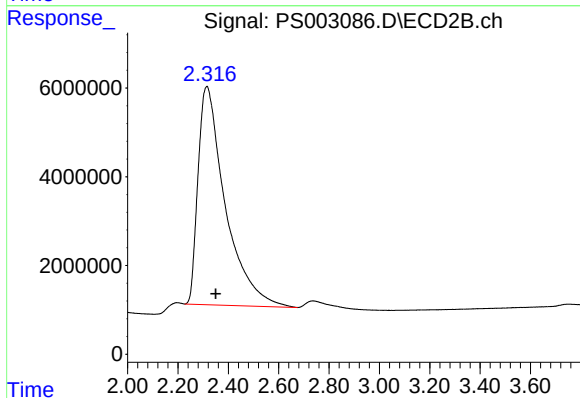


#1 Dalapon

R.T.: 2.315 min
Delta R.T.: -0.036 min
Response: 368842009
Conc: 688.24 ng/ml

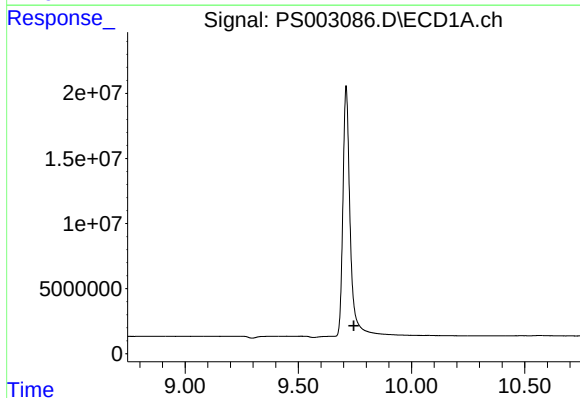


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

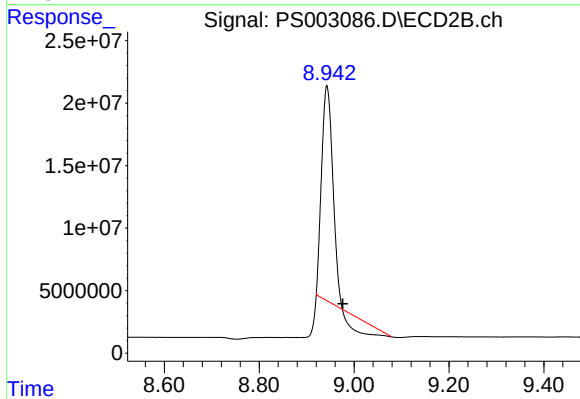

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.943 min
Delta R.T.: -0.033 min
Response: 238025070
Conc: 422.35 ng/ml

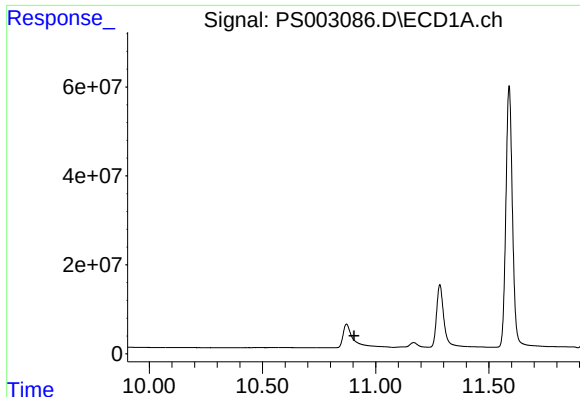

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

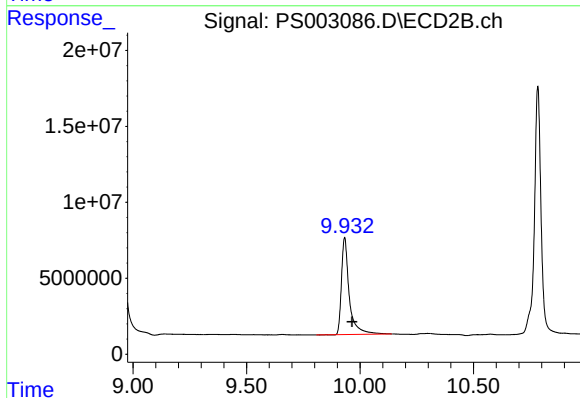


#3 4-Nitrophenol

R.T.: 9.932 min
Delta R.T.: -0.033 min
Response: 152266349
Conc: 728.47 ng/ml

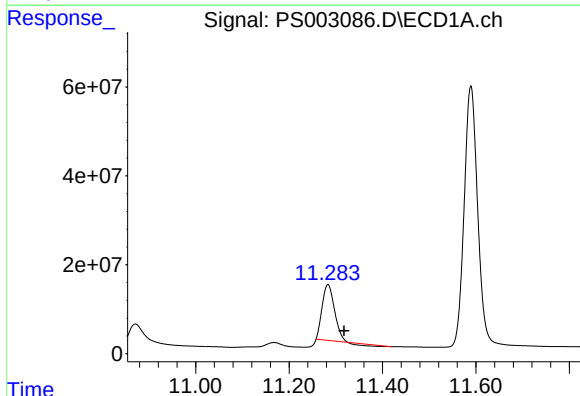


#4 2,4-DCAA

R.T.: 11.283 min
Delta R.T.: -0.034 min
Response: 214261037
Conc: 564.38 ng/ml

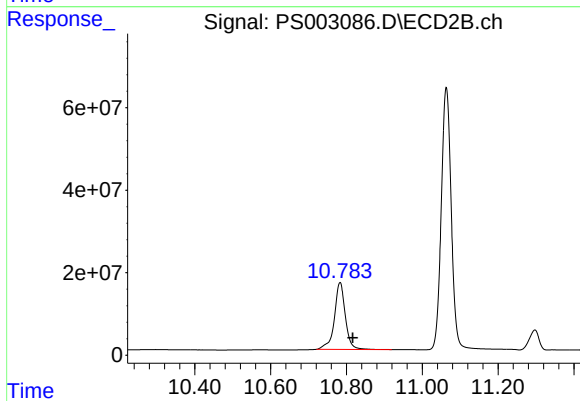

#4 2,4-DCAA


R.T.: 10.783 min
Delta R.T.: -0.034 min
Response: 325068064
Conc: 760.31 ng/ml

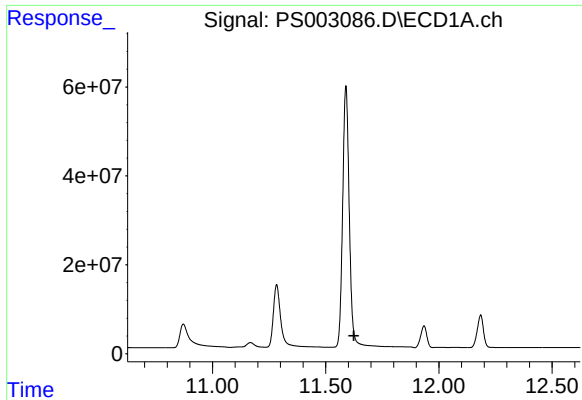

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.624 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

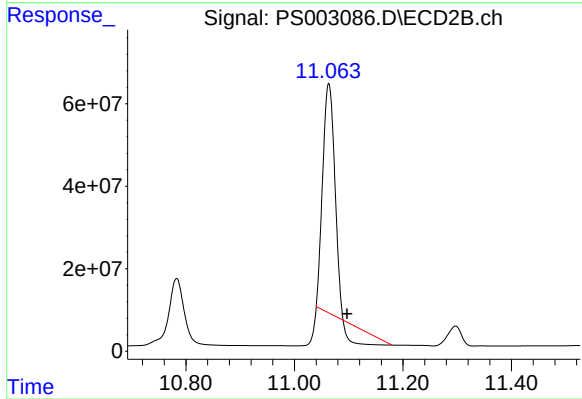


#5 DICAMBA

R.T.: 11.063 min
Delta R.T.: -0.034 min
Response: 721799665
Conc: 454.92 ng/ml

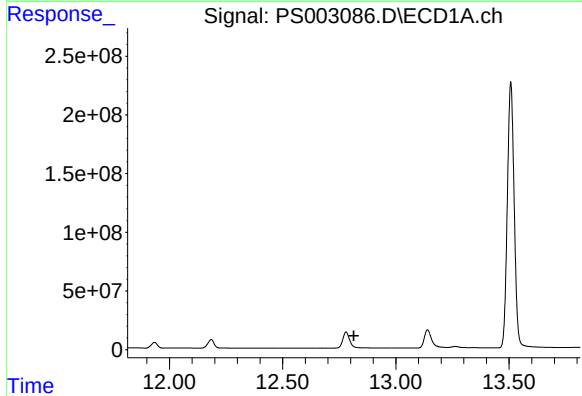


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

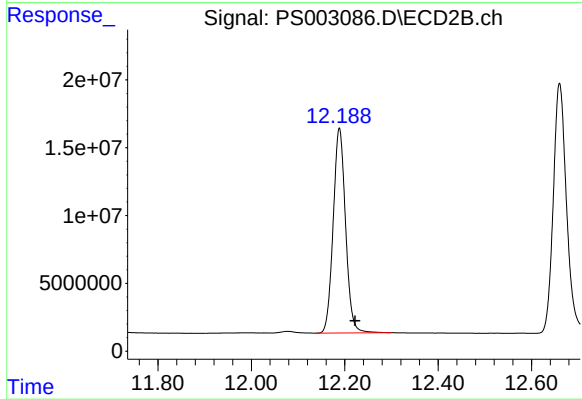

#8 DICHLORPROP


R.T.: 12.189 min
Delta R.T.: -0.034 min
Response: 277605083
Conc: 726.07 ng/ml

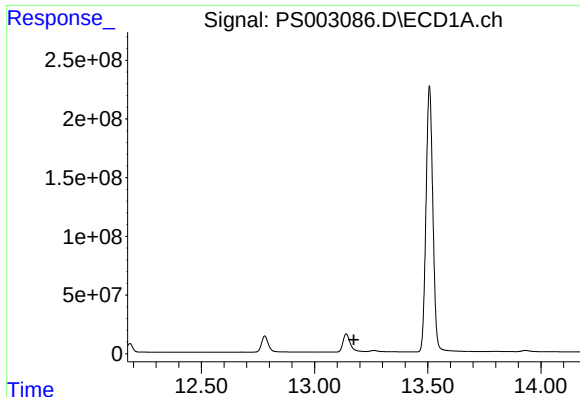

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.173 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

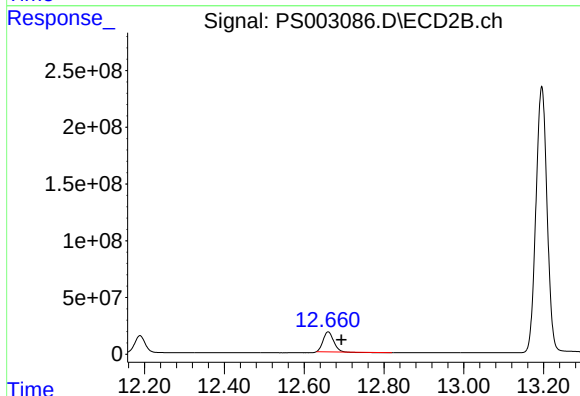


#9 2,4-D

R.T.: 12.660 min
Delta R.T.: -0.033 min
Response: 316334917
Conc: 630.92 ng/ml

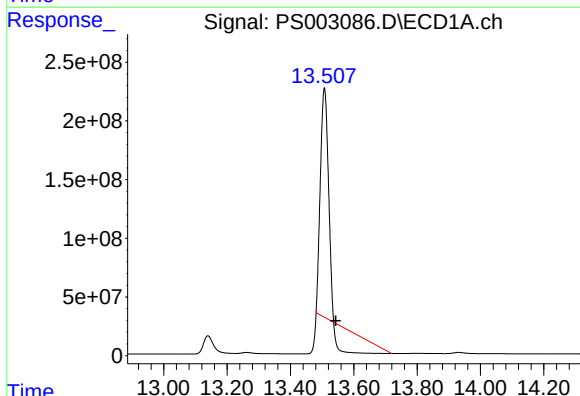


#10 Pentachlorophenol

R.T.: 13.507 min
Delta R.T.: -0.036 min
Response: 2102351793
Conc: 327.83 ng/ml

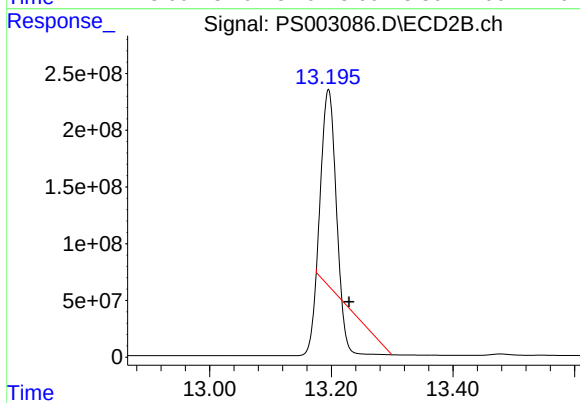

#10 Pentachlorophenol


R.T.: 13.195 min
Delta R.T.: -0.034 min
Response: 1468746396
Conc: 237.64 ng/ml

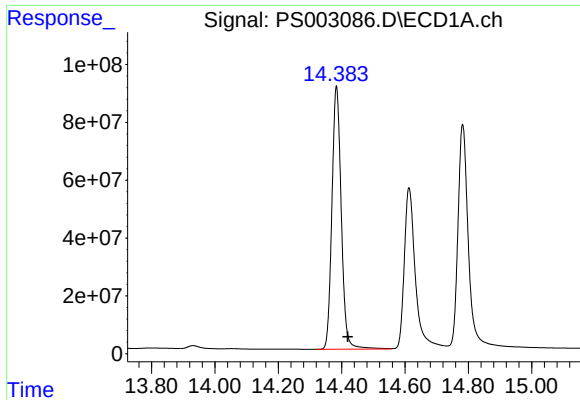

#11 2,4,5-TP (SILVEX)


R.T.: 14.384 min
Delta R.T.: -0.036 min
Response: 1864556594
Conc: 740.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

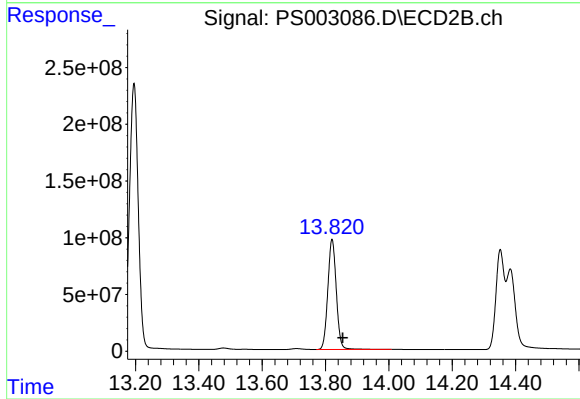


#11 2,4,5-TP (SILVEX)

R.T.: 13.821 min
Delta R.T.: -0.034 min
Response: 1802811284
Conc: 726.84 ng/ml

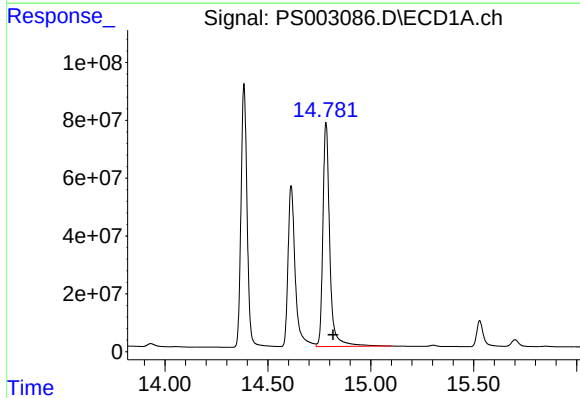


#12 2,4,5-T

R.T.: 14.782 min
Delta R.T.: -0.034 min
Response: 1804505671
Conc: 739.73 ng/ml

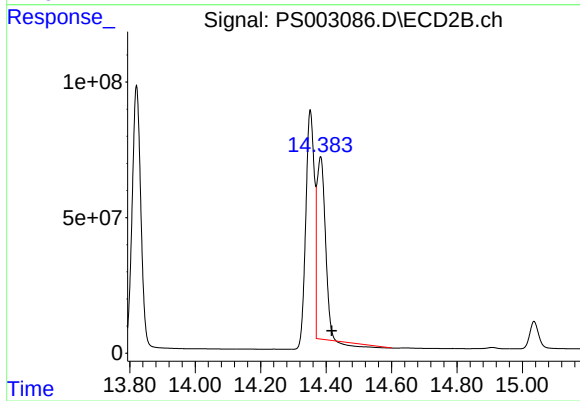

#12 2,4,5-T


R.T.: 14.383 min
Delta R.T.: -0.034 min
Response: 1141646129
Conc: 596.63 ng/ml

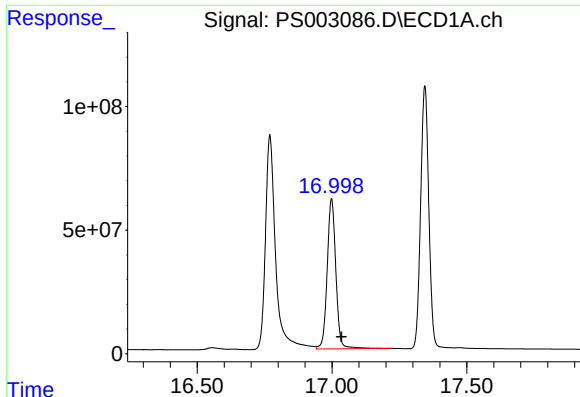

#14 DINOSEB


R.T.: 16.998 min
Delta R.T.: -0.037 min
Response: 1361795192
Conc: 723.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

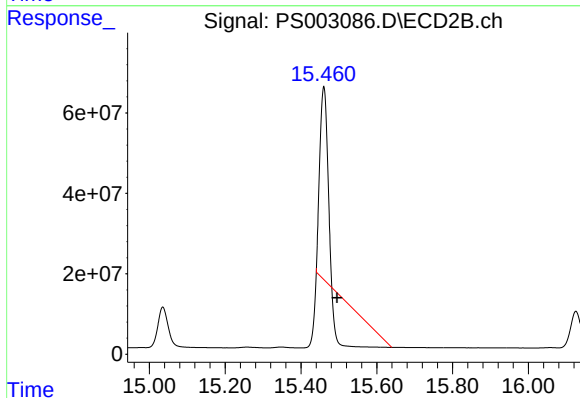


#14 DINOSEB

R.T.: 15.460 min
Delta R.T.: -0.035 min
Response: 35739229
Conc: 20.39 ng/ml

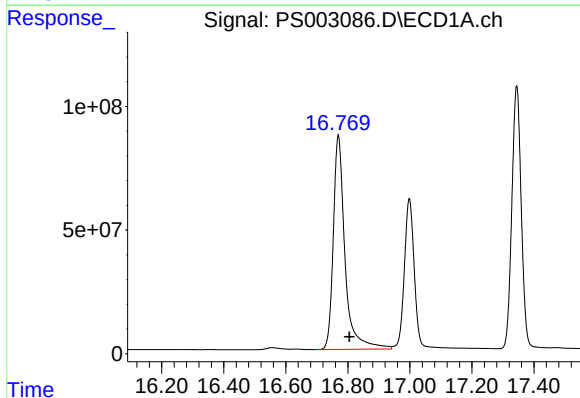


#15 Picloram

R.T.: 16.770 min
Delta R.T.: -0.036 min
Response: 2270143835
Conc: 717.58 ng/ml

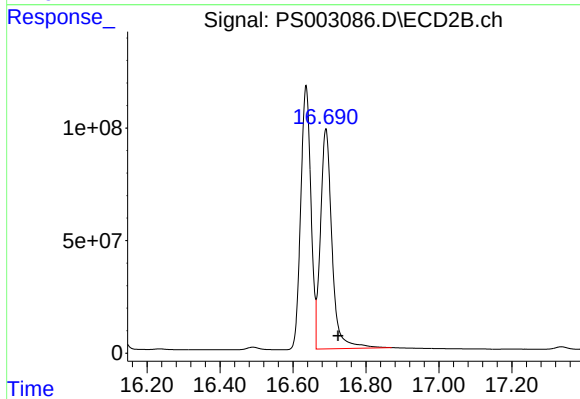

#15 Picloram


R.T.: 16.690 min
Delta R.T.: -0.034 min
Response: 2139820392
Conc: 711.75 ng/ml

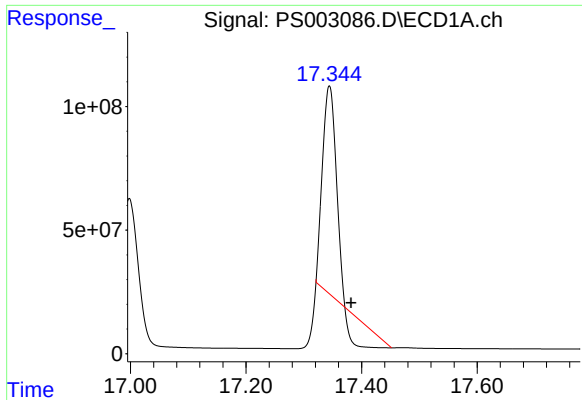

#16 DCPA

R.T.: 17.344 min
Delta R.T.: -0.037 min
Response: 1073141999
Conc: 356.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

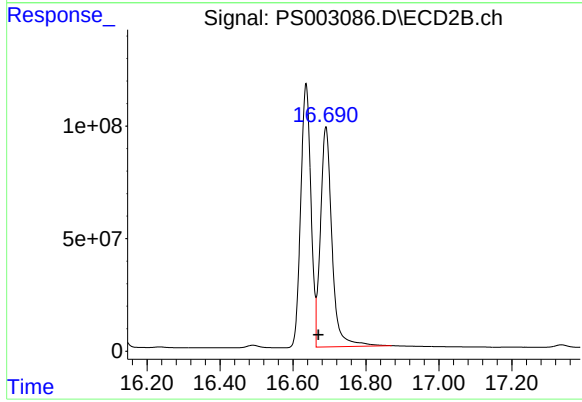

#16 DCPA

R.T.: 16.690 min
Delta R.T.: 0.021 min
Response: 2139820392
Conc: 690.80 ng/ml