

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020819\
 Data File : PS003087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2019 16:54
 Operator : EI\SJ
 Sample : K1389-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 M-5-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 22:13:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.769	0	247.9E6	N.D.	579.755 #
Target Compounds							
3) T	4-Nitroph...	0.000	9.990	0	16733742	N.D.	80.057 #
7) T	MCPA	0.000	11.725	0	3519909	N.D.	2.238 #
10) T	Pentachlo...	0.000	13.265	0	2046436	N.D.	0.331 #
11) T	2,4,5-TP ...	14.456	0.000	9766474	0	3.878	N.D. #
12) T	2,4,5-T	0.000	14.425	0	5086037	N.D.	2.658 #
13) T	2,4-DB	0.000	15.119	0	1322043	N.D.	5.205 #
14) T	DINOSEB	0.000	15.475	0	6605977	N.D.	3.768 #
15) T	Picloram	16.781	16.691	10470443	24128773	3.310	8.026 #
16) T	DCPA	0.000	16.691	0	24128773	N.D.	7.790 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020819\
Data File : PS003087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2019 16:54
Operator : EI\SJ
Sample : K1389-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
M-5-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 22:13:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

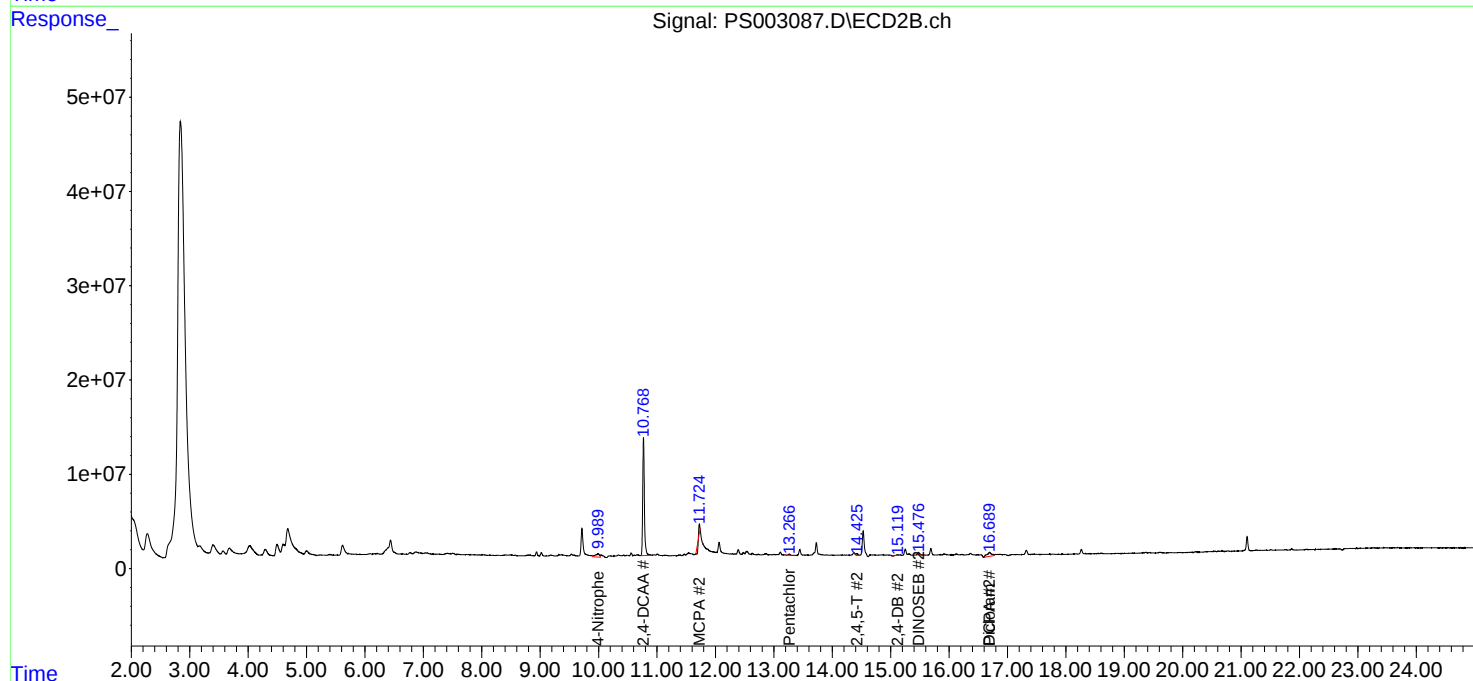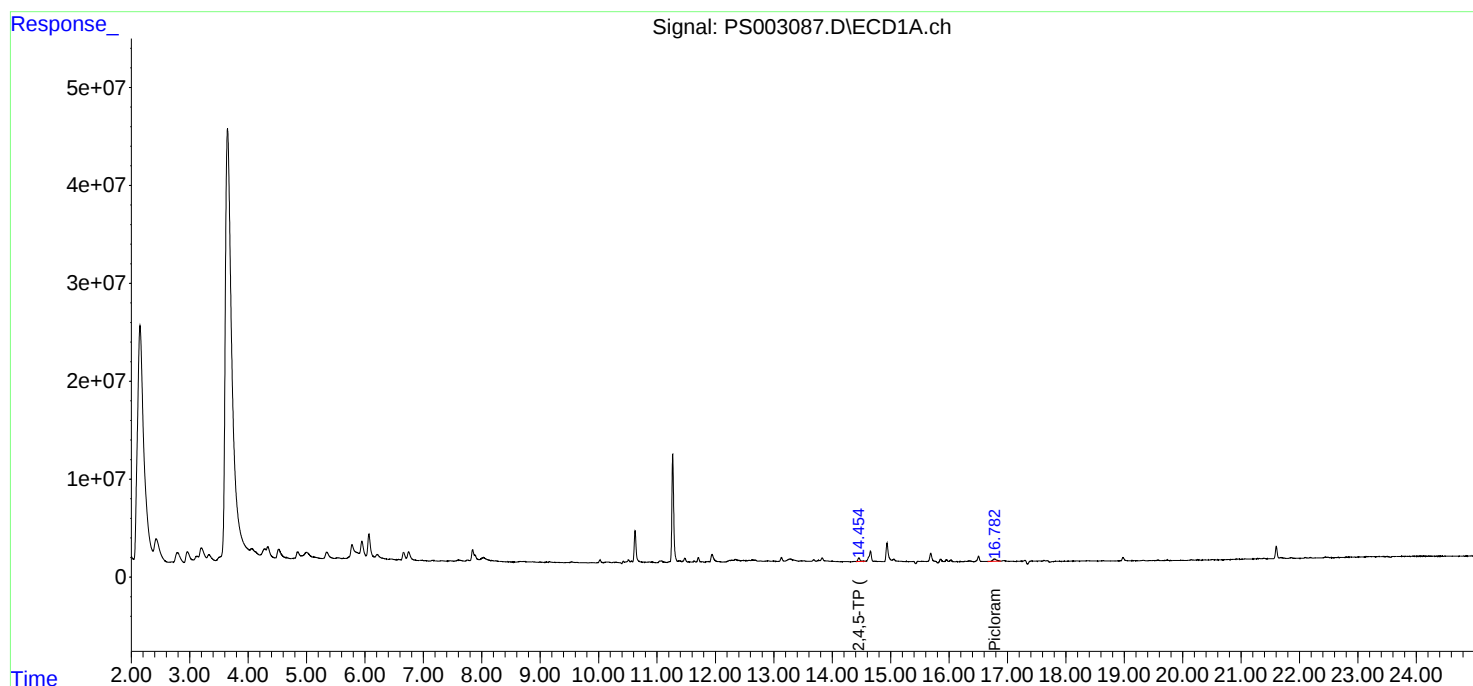


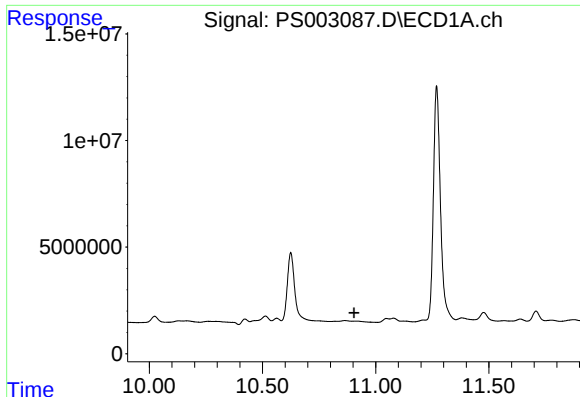

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-5-D

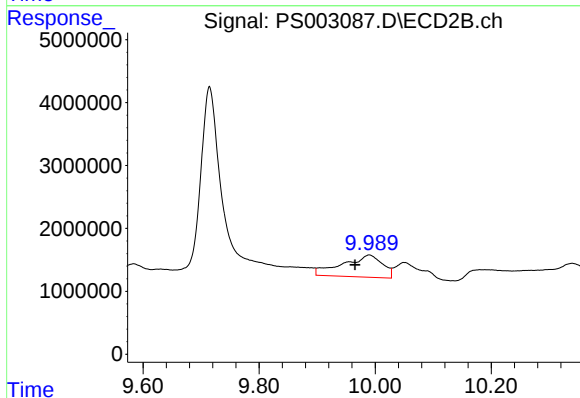


#3 4-Nitrophenol

R.T.: 9.990 min
Delta R.T.: 0.025 min
Response: 16733742
Conc: 80.06 ng/ml

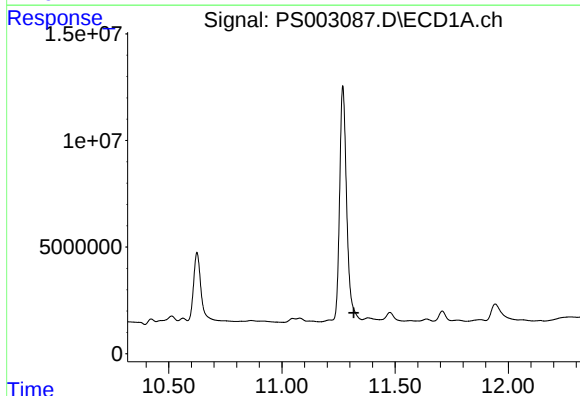


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.318 min
Response: 0
Conc: N.D.

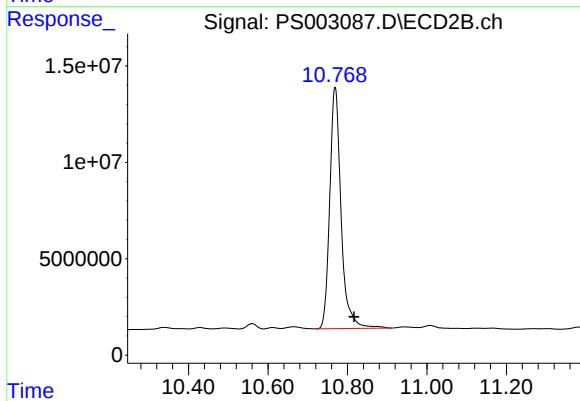

#4 2,4-DCAA


R.T.: 10.769 min
Delta R.T.: -0.048 min
Response: 247871759
Conc: 579.75 ng/ml

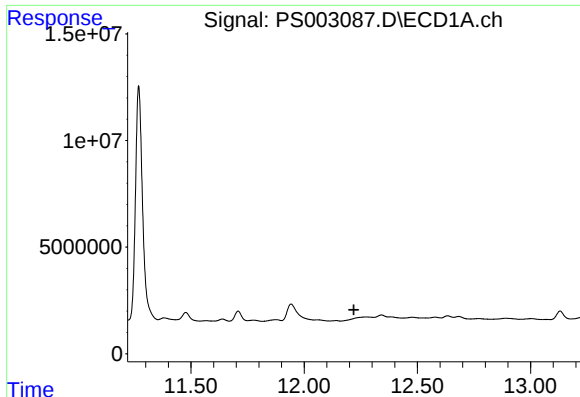

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-5-D

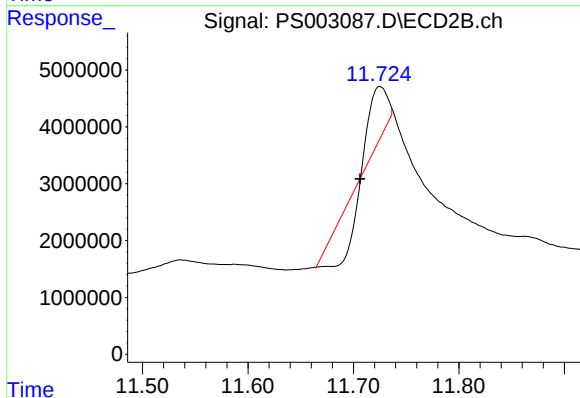


#7 MCPA

R.T.: 11.725 min
Delta R.T.: 0.019 min
Response: 3519909
Conc: 2.24 ug/ml

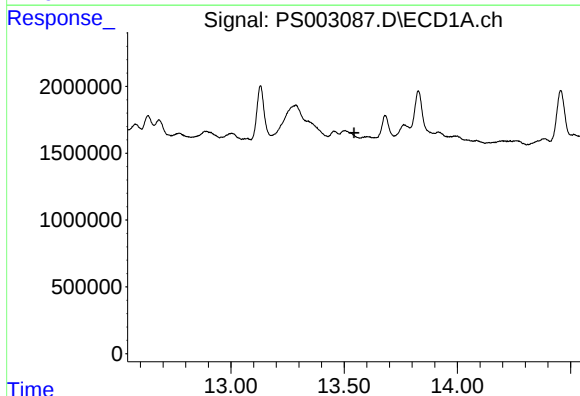


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.543 min
Response: 0
Conc: N.D.

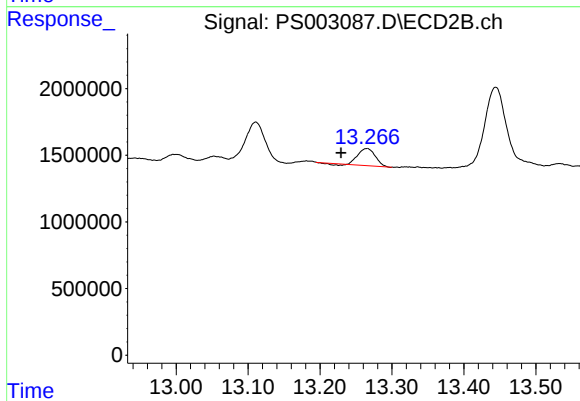

#10 Pentachlorophenol


R.T.: 13.265 min
Delta R.T.: 0.036 min
Response: 2046436
Conc: 0.33 ng/ml

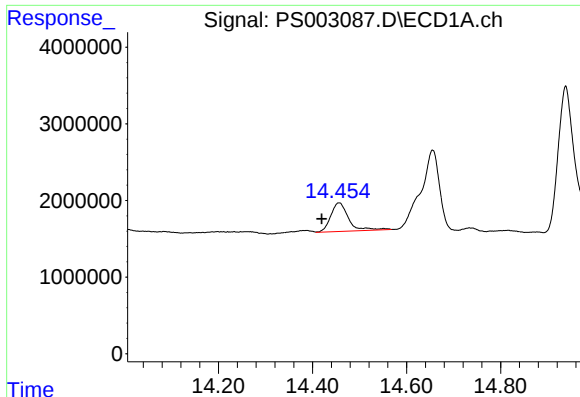

#11 2,4,5-TP (SILVEX)


R.T.: 14.456 min
Delta R.T.: 0.037 min
Response: 9766474
Conc: 3.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
M-5-D

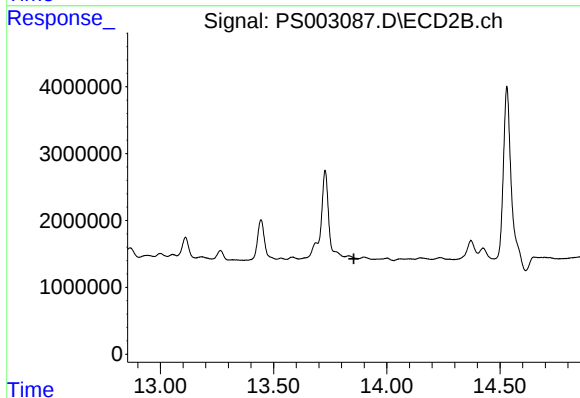


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

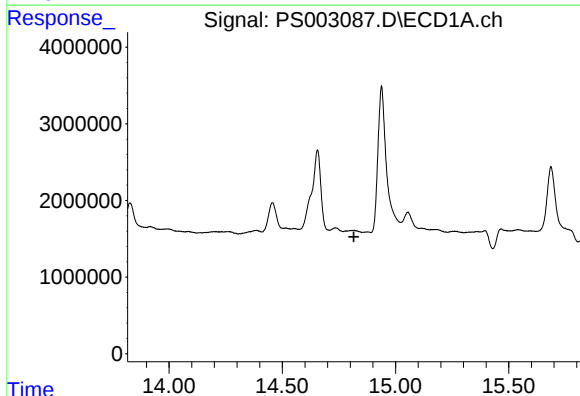


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

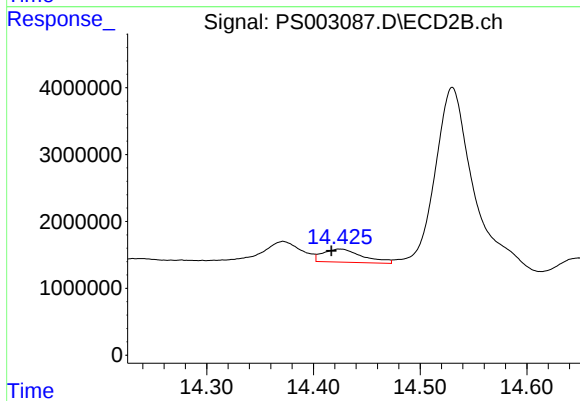

#12 2,4,5-T


R.T.: 14.425 min
Delta R.T.: 0.008 min
Response: 5086037
Conc: 2.66 ng/ml

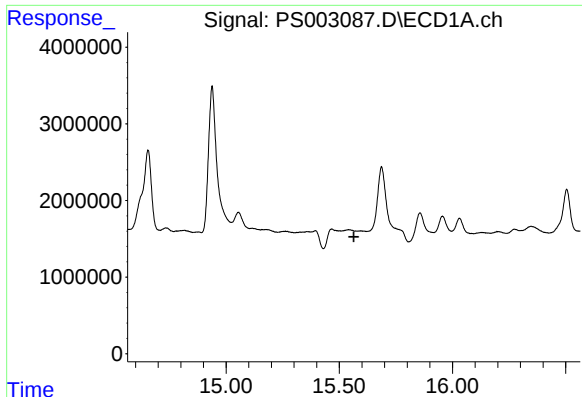

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-5-D

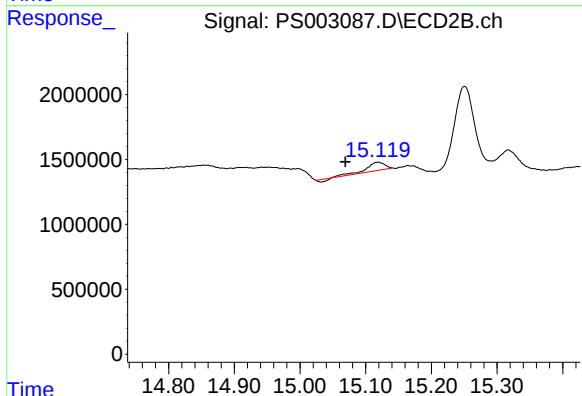


#13 2,4-DB

R.T.: 15.119 min
Delta R.T.: 0.050 min
Response: 1322043
Conc: 5.20 ng/ml

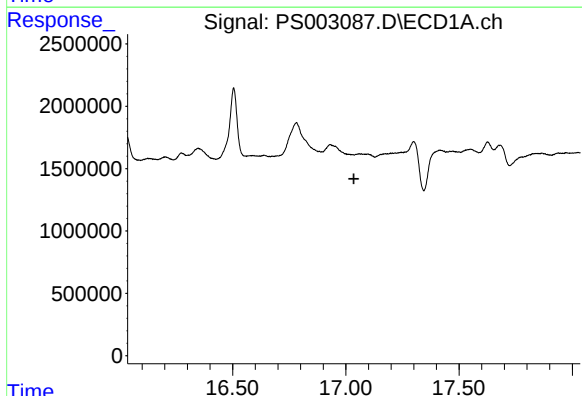


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

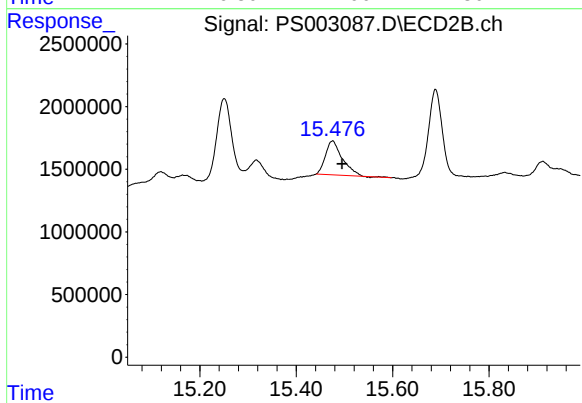

#14 DINOSEB


R.T.: 15.475 min
Delta R.T.: -0.020 min
Response: 6605977
Conc: 3.77 ng/ml

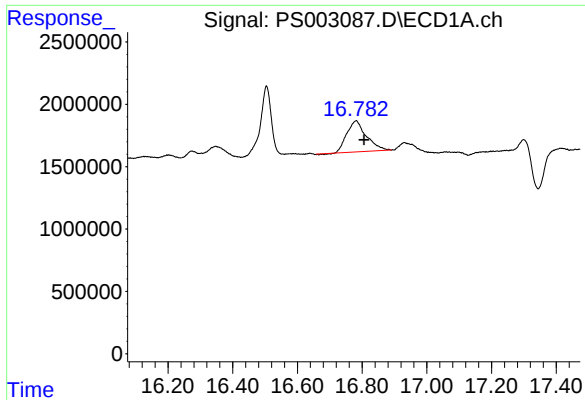

#15 Picloram


R.T.: 16.781 min
Delta R.T.: -0.025 min
Response: 10470443
Conc: 3.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
M-5-D

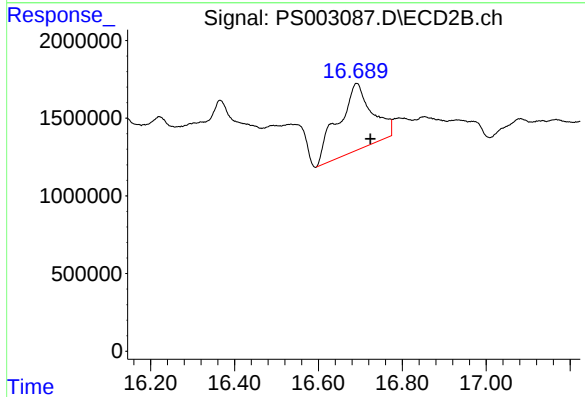


#15 Picloram

R.T.: 16.691 min
Delta R.T.: -0.033 min
Response: 24128773
Conc: 8.03 ng/ml

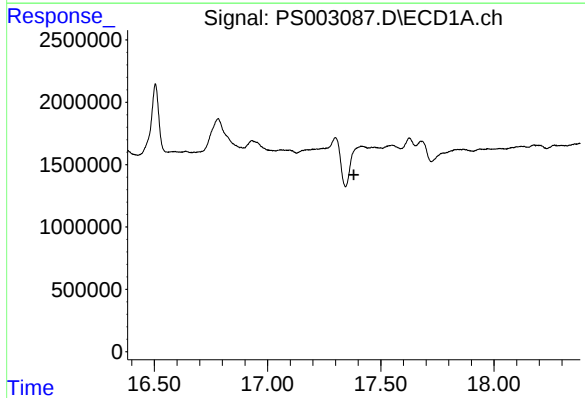

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

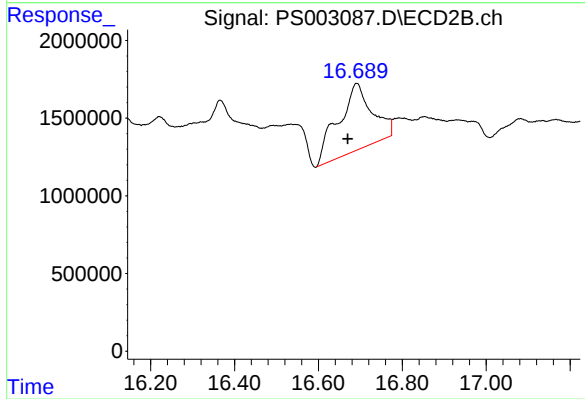

#16 DCPA

R.T.: 16.691 min
Delta R.T.: 0.022 min
Response: 24128773
Conc: 7.79 ng/ml