

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020819\
 Data File : PS003088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2019 17:25
 Operator : EI\SJ
 Sample : K1389-20
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 M-7-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 22:14:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.296	10.796	227.9E6	238.4E6	600.240	557.566
Target Compounds							
1) T	Dalapon	0.000	2.303	0	93863155	N.D.	175.144 #
2) T	3,5-DICHL...	0.000	8.963	0	7269788	N.D.	12.900 #
3) T	4-Nitroph...	0.000	10.017	0	6606479	N.D.	31.607 #
6) T	MCP	11.967	0.000	14390638	0	12.011	N.D. #
9) T	2,4-D	13.156	0.000	7377919	0	16.002	N.D. #
10) T	Pentachlo...	0.000	13.293	0	1446575	N.D.	0.234 #
11) T	2,4,5-TP ...	14.482	0.000	7750077	0	3.077	N.D. #
12) T	2,4,5-T	0.000	14.398	0	4717517	N.D.	2.465 #
14) T	DINOSEB	0.000	15.502	0	7842345	N.D.	4.474 #
15) T	Picloram	16.783	16.723	6828040	13390258	2.158	4.454 #
16) T	DCPA	0.000	16.723	0	13390258	N.D.	4.323 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020819\
Data File : PS003088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2019 17:25
Operator : EI\SJ
Sample : K1389-20
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
M-7-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 22:14:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

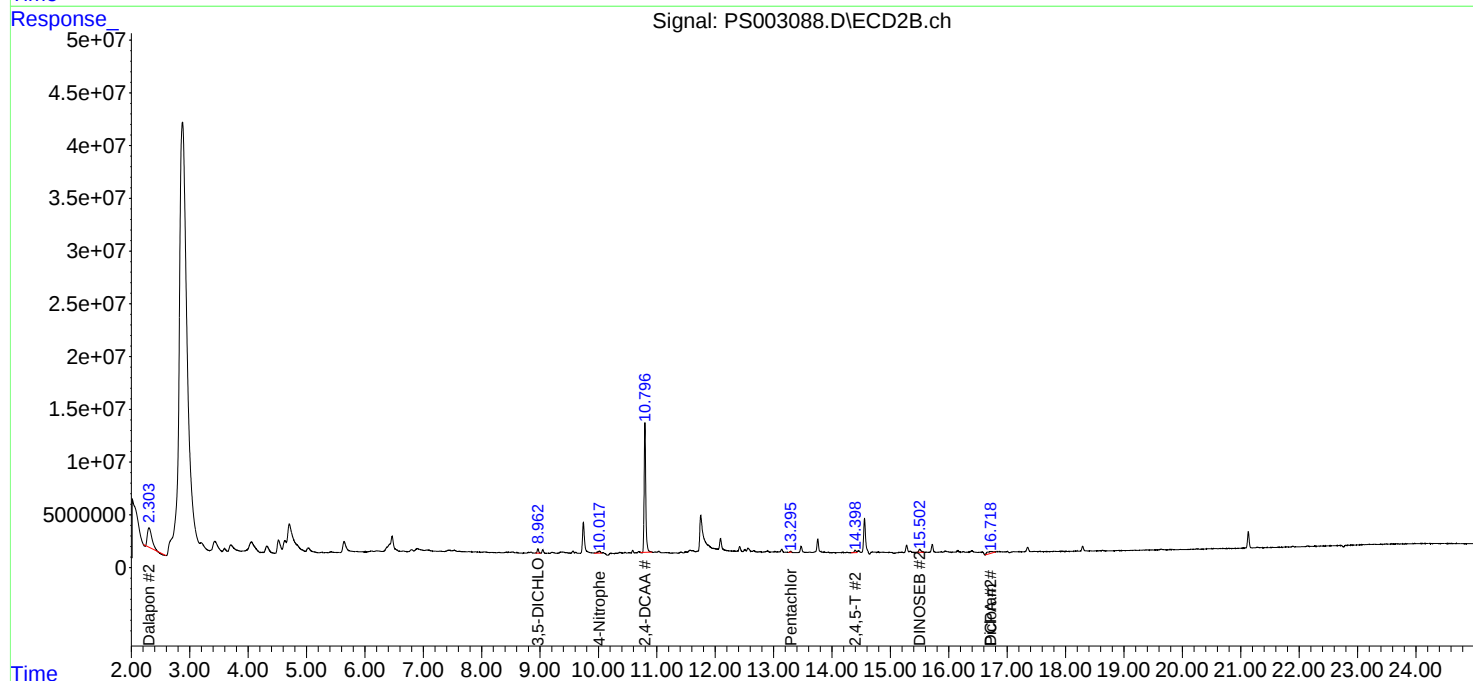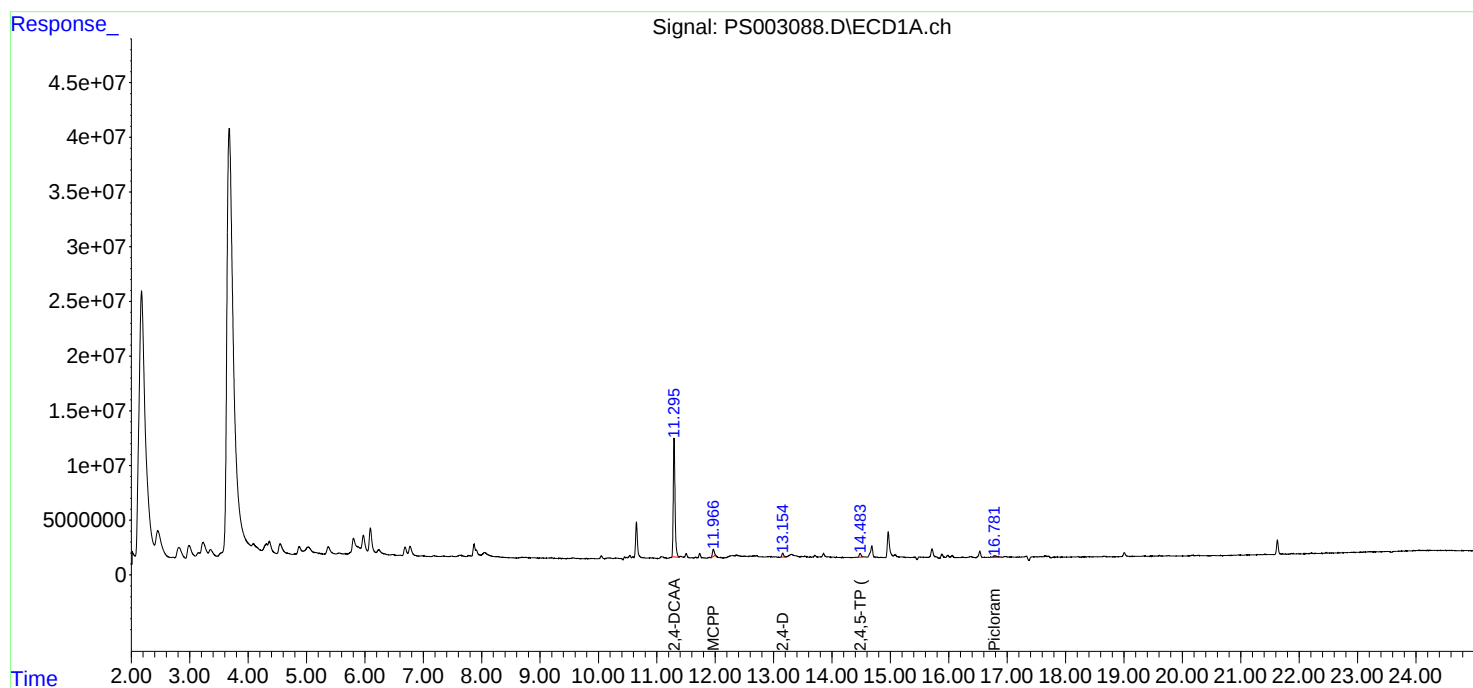


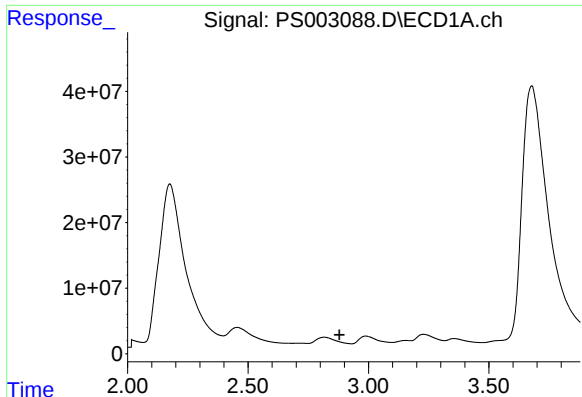

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-7-S

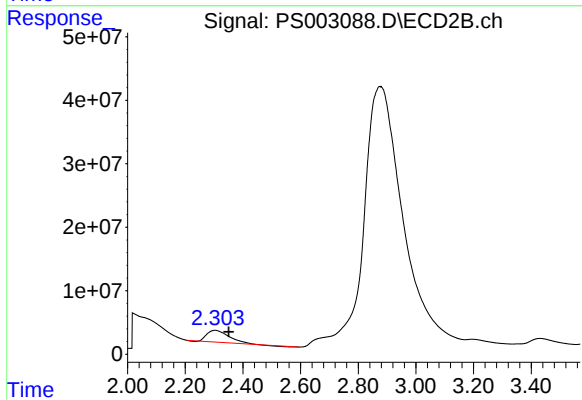


#1 Dalapon

R.T.: 2.303 min
Delta R.T.: -0.048 min
Response: 93863155
Conc: 175.14 ng/ml

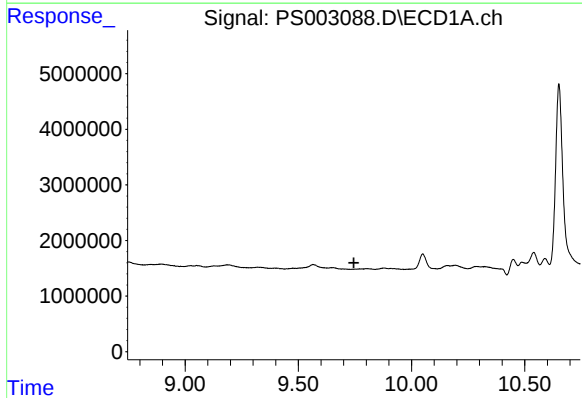


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

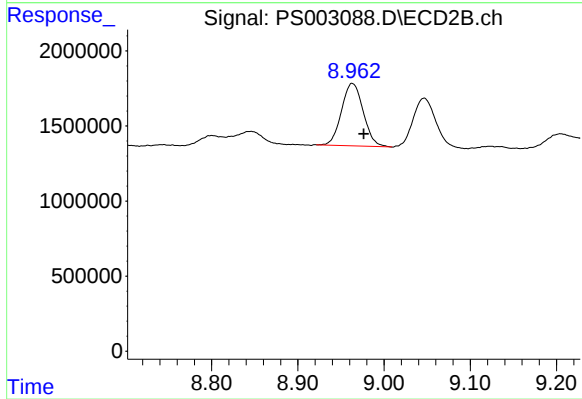

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.963 min
Delta R.T.: -0.013 min
Response: 7269788
Conc: 12.90 ng/ml

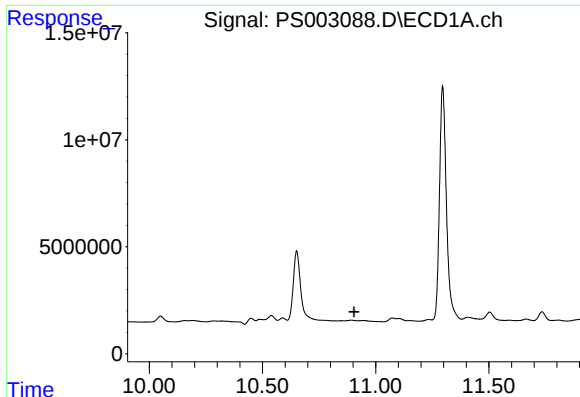

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-7-S

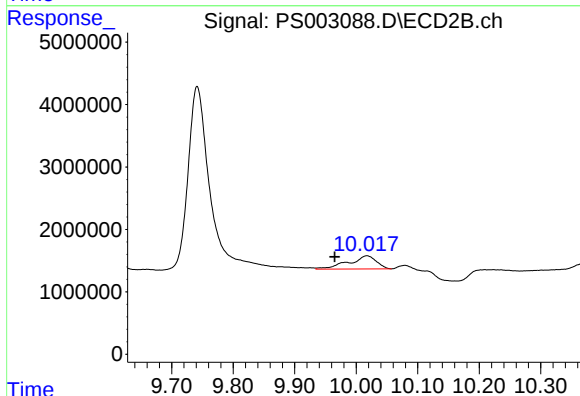


#3 4-Nitrophenol

R.T.: 10.017 min
Delta R.T.: 0.052 min
Response: 6606479
Conc: 31.61 ng/ml

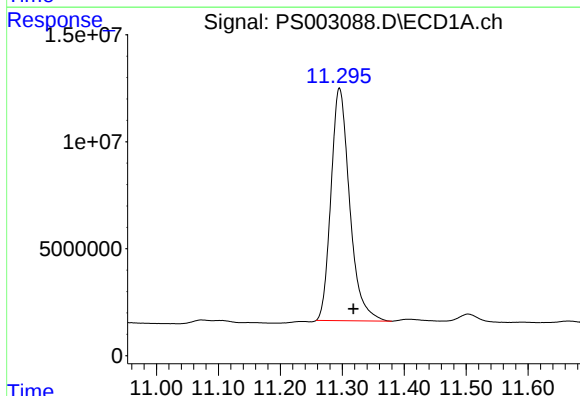


#4 2,4-DCAA

R.T.: 11.296 min
Delta R.T.: -0.022 min
Response: 227875631
Conc: 600.24 ng/ml

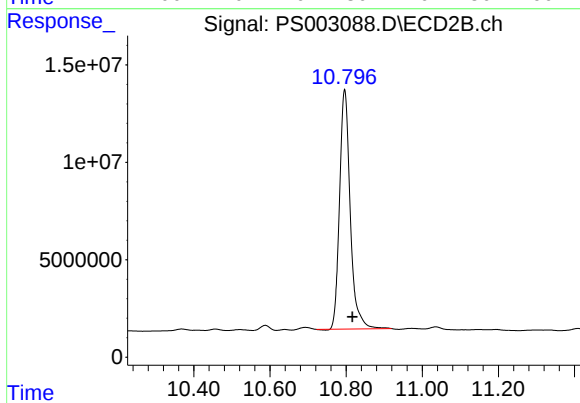

#4 2,4-DCAA


R.T.: 10.796 min
Delta R.T.: -0.021 min
Response: 238385122
Conc: 557.57 ng/ml

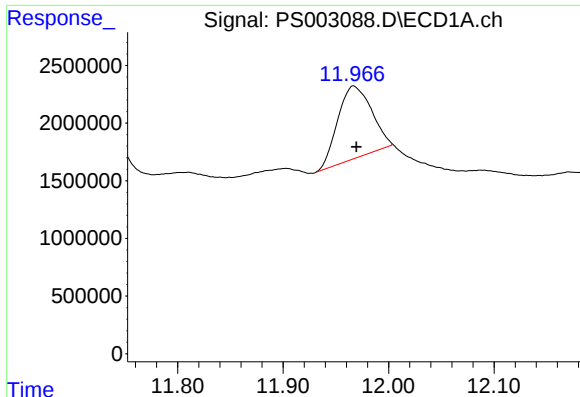

#6 MCP


R.T.: 11.967 min
Delta R.T.: -0.002 min
Response: 14390638
Conc: 12.01 ug/ml

Instrument :
ECD_S
ClientSampleId :
M-7-S

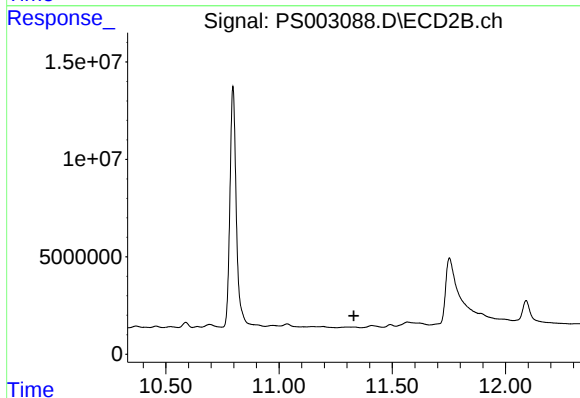


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

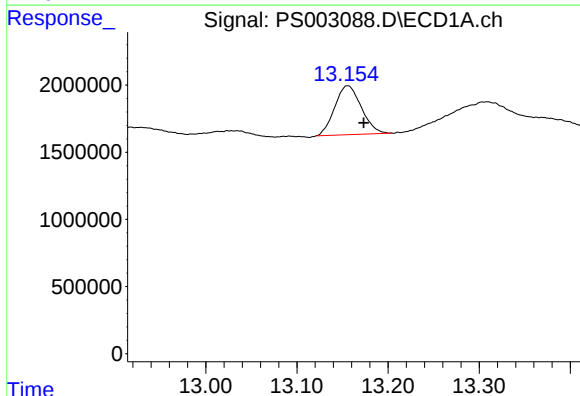


#9 2,4-D

R.T.: 13.156 min
Delta R.T.: -0.018 min
Response: 7377919
Conc: 16.00 ng/ml

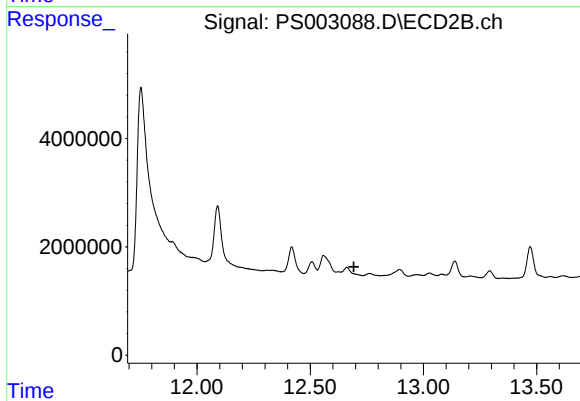

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 12.693 min
Response: 0
Conc: N.D.

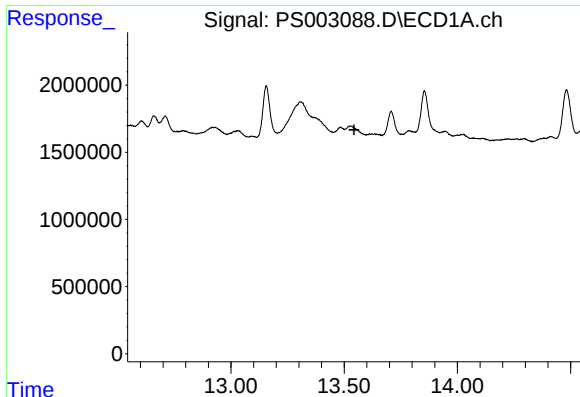

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.543 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-7-S

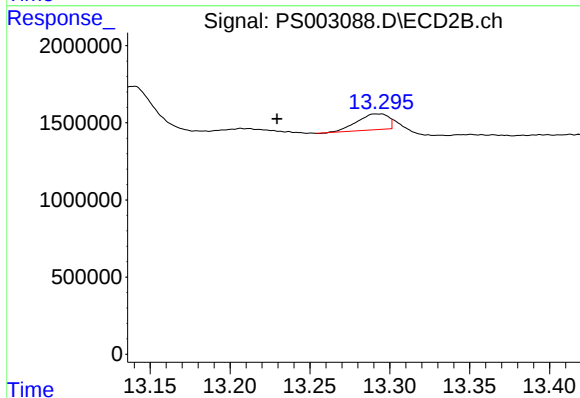


#10 Pentachlorophenol

R.T.: 13.293 min
Delta R.T.: 0.063 min
Response: 1446575
Conc: 0.23 ng/ml

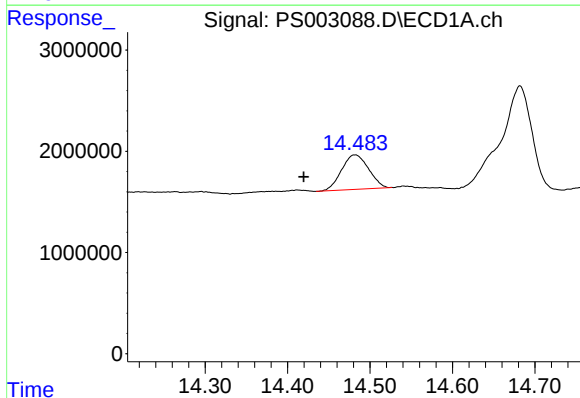


#11 2,4,5-TP (SILVEX)

R.T.: 14.482 min
Delta R.T.: 0.062 min
Response: 7750077
Conc: 3.08 ng/ml

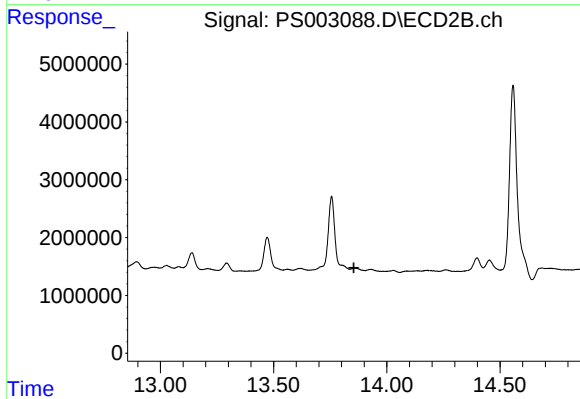

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 13.854 min
Response: 0
Conc: N.D.

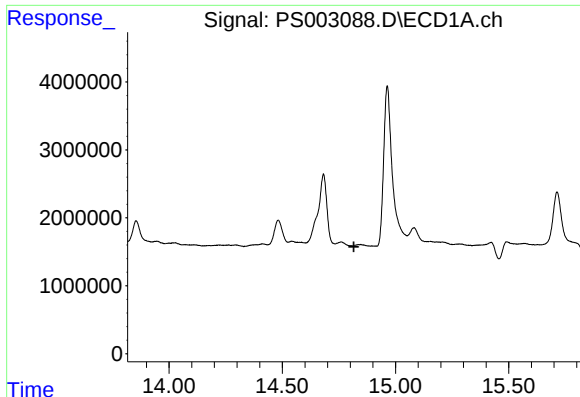

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-7-S

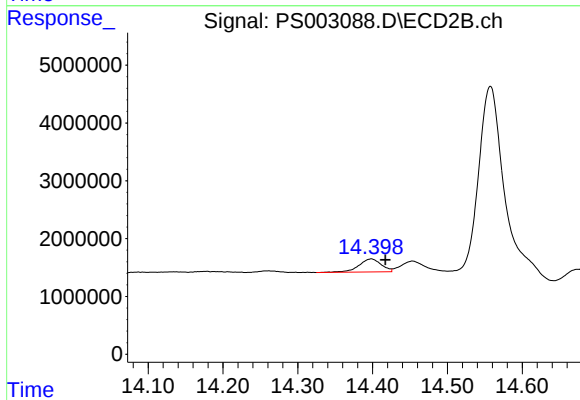


#12 2,4,5-T

R.T.: 14.398 min
Delta R.T.: -0.019 min
Response: 4717517
Conc: 2.47 ng/ml

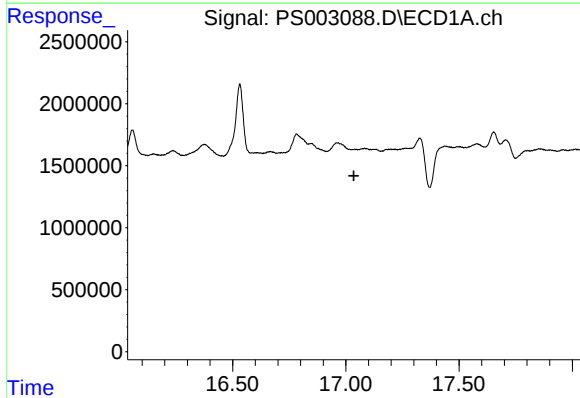


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

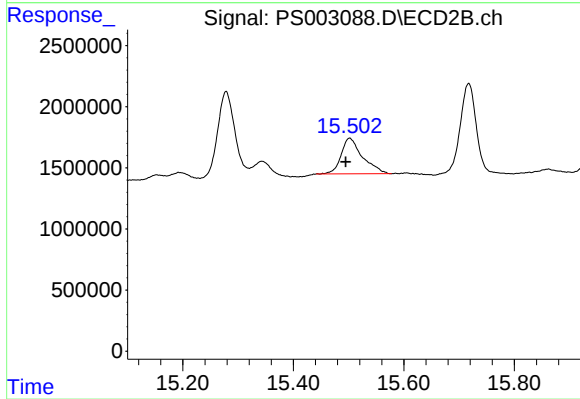

#14 DINOSEB


R.T.: 15.502 min
Delta R.T.: 0.007 min
Response: 7842345
Conc: 4.47 ng/ml

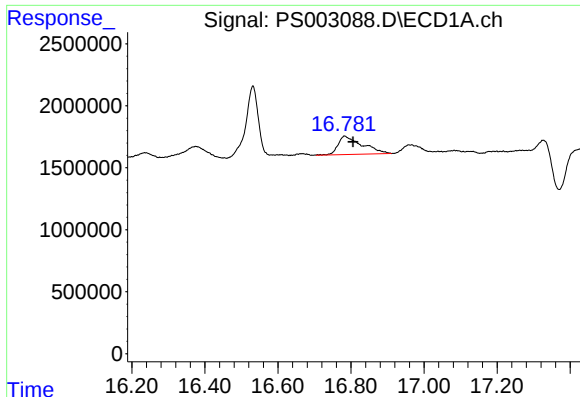

#15 Picloram


R.T.: 16.783 min
Delta R.T.: -0.023 min
Response: 6828040
Conc: 2.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
M-7-S

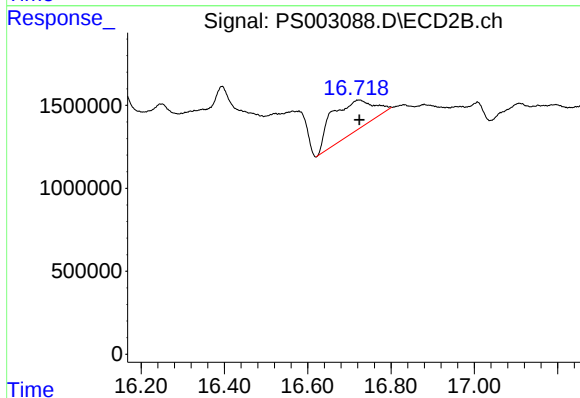


#15 Picloram

R.T.: 16.723 min
Delta R.T.: -0.001 min
Response: 13390258
Conc: 4.45 ng/ml

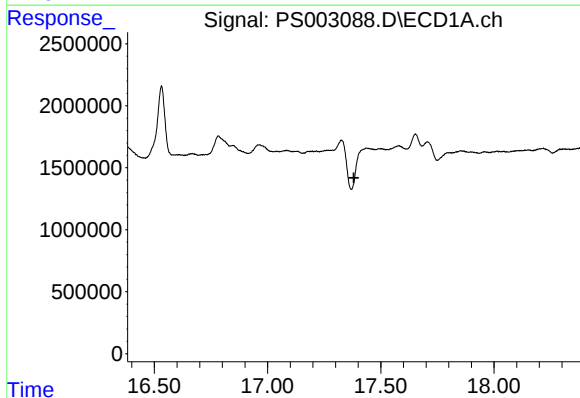

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

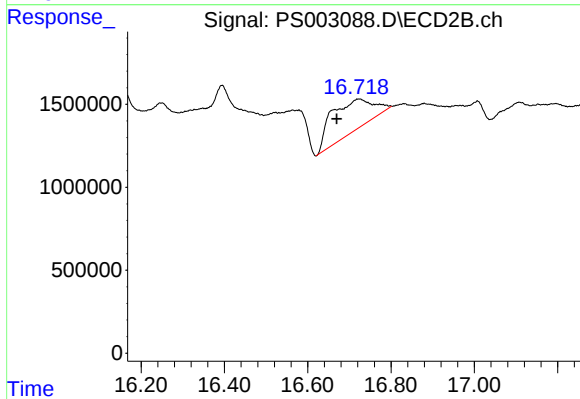

#16 DCPA

R.T.: 16.723 min
Delta R.T.: 0.053 min
Response: 13390258
Conc: 4.32 ng/ml