

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020819\
 Data File : PS003094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2019 20:31
 Operator : EI\SJ
 Sample : K1401-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RT-3451

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 22:15:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.278	10.778	153.8E6	227.9E6	405.187	532.943 #
Target Compounds							
1) T	Dalapon	0.000	2.283	0	67956019	N.D.	126.802 #
2) T	3,5-DICHL...	0.000	8.946	0	7424259	N.D.	13.174 #
3) T	4-Nitroph...	0.000	9.966	0	1901942	N.D.	9.099 #
6) T	MCP	0.000	11.393	0	6107031	N.D.	5.537 #
7) T	MCPA	12.245	0.000	1753484	0	0.991	N.D. #
10) T	Pentachlo...	13.504	0.000	21025694	0	3.279	N.D. #
11) T	2,4,5-TP ...	14.465	0.000	6456320	0	2.564	N.D. #
12) T	2,4,5-T	0.000	14.434	0	3451504	N.D.	1.804 #
14) T	DINOSEB	0.000	15.486	0	9489251	N.D.	5.413 #
15) T	Picloram	16.827	16.702	4328148	16407136	1.368	5.457 #
16) T	DCPA	17.417	16.702	-7589239	16407136	N.D.	5.297



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020819\
Data File : PS003094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2019 20:31
Operator : EI\SJ
Sample : K1401-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
RT-3451

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 22:15:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

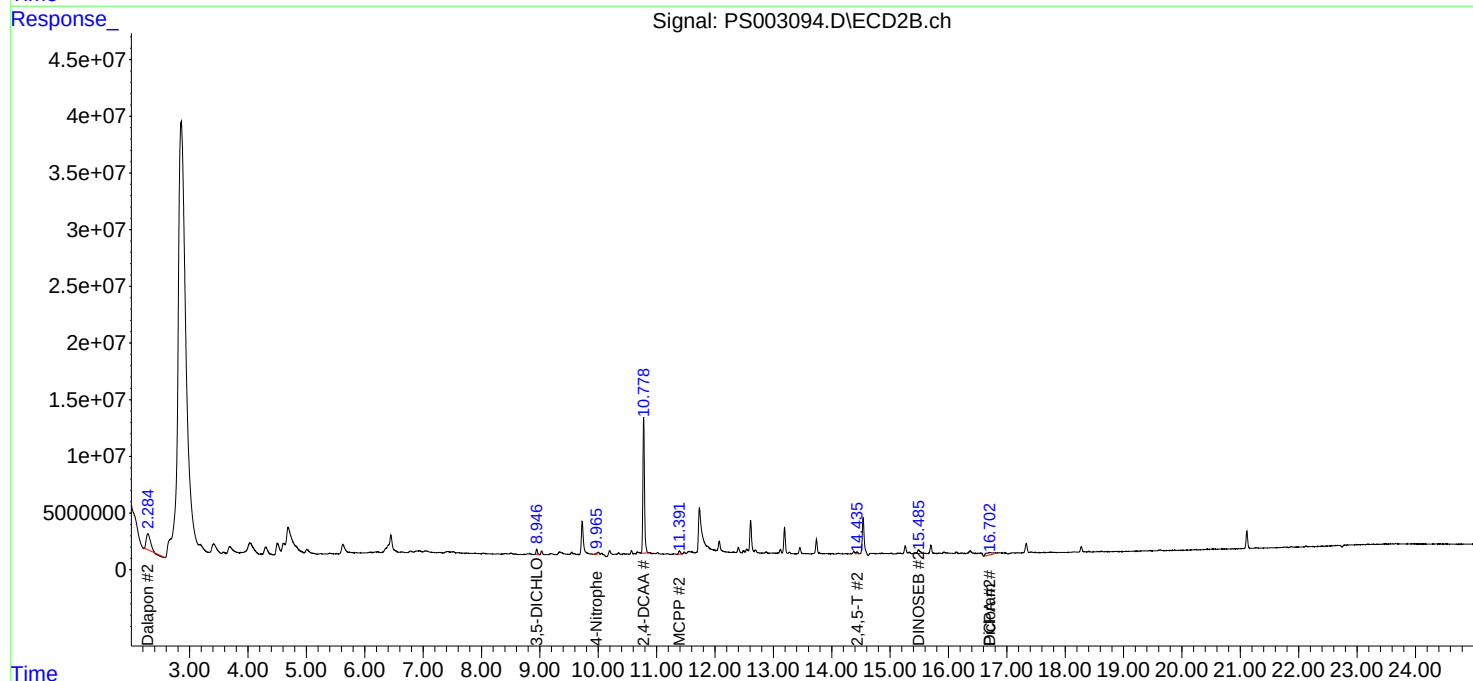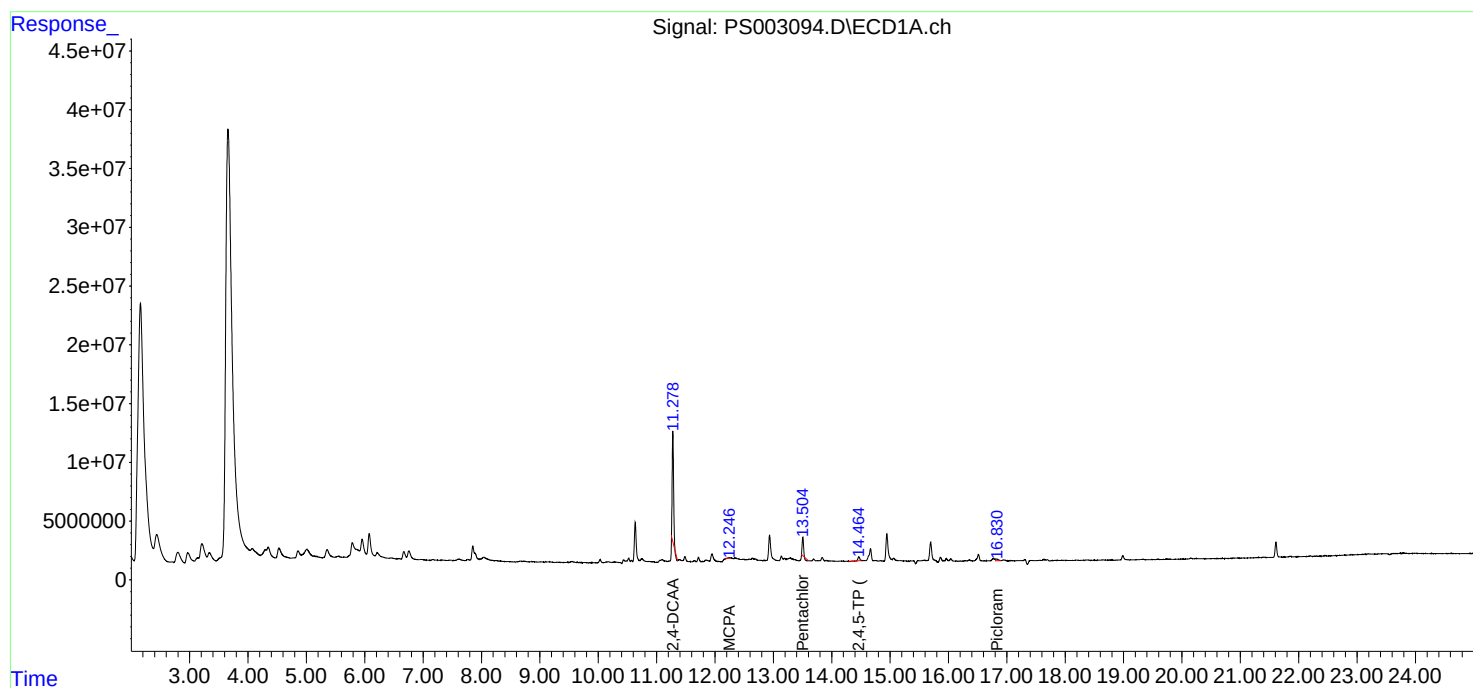


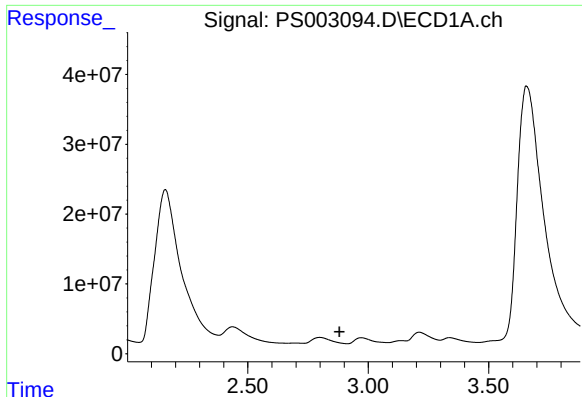

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RT-3451

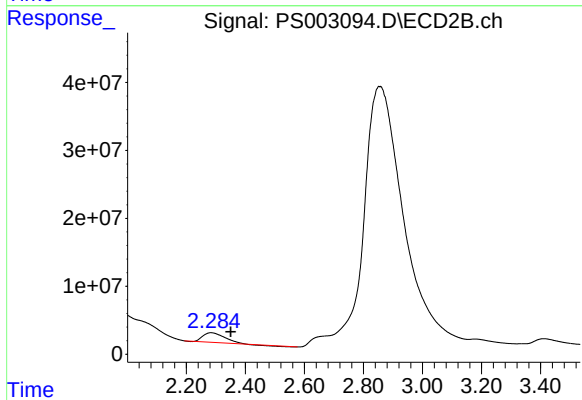


#1 Dalapon

R.T.: 2.283 min
Delta R.T.: -0.067 min
Response: 67956019
Conc: 126.80 ng/ml

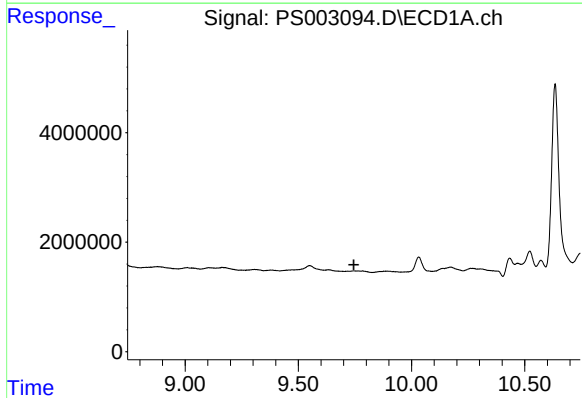


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

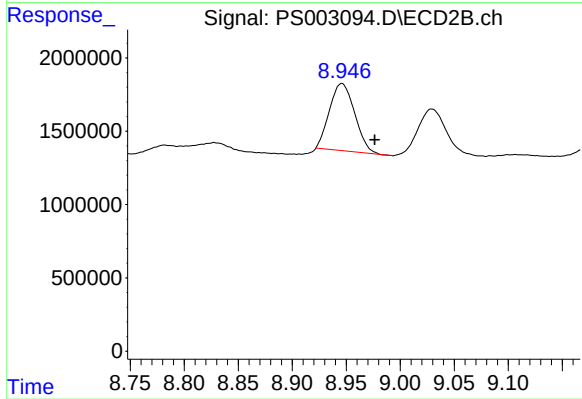

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.946 min
Delta R.T.: -0.030 min
Response: 7424259
Conc: 13.17 ng/ml

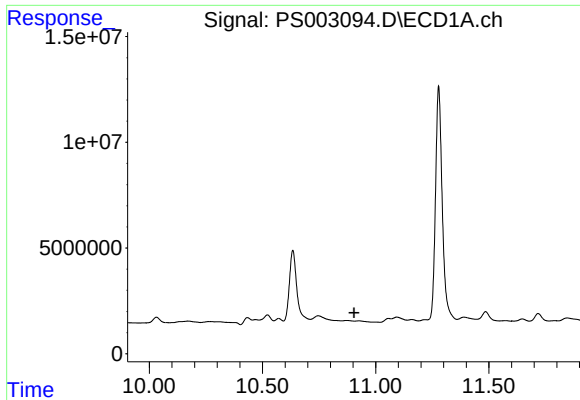

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RT-3451

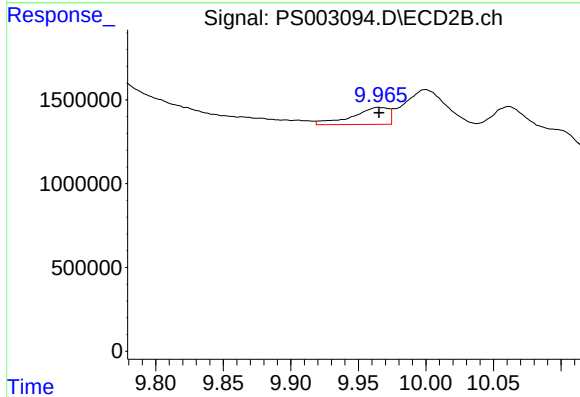


#3 4-Nitrophenol

R.T.: 9.966 min
Delta R.T.: 0.000 min
Response: 1901942
Conc: 9.10 ng/ml

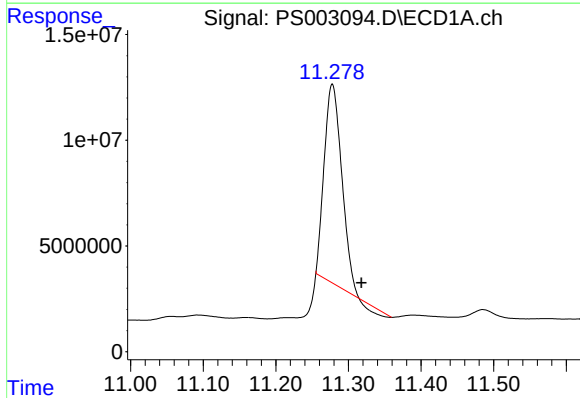


#4 2,4-DCAA

R.T.: 11.278 min
Delta R.T.: -0.040 min
Response: 153825570
Conc: 405.19 ng/ml

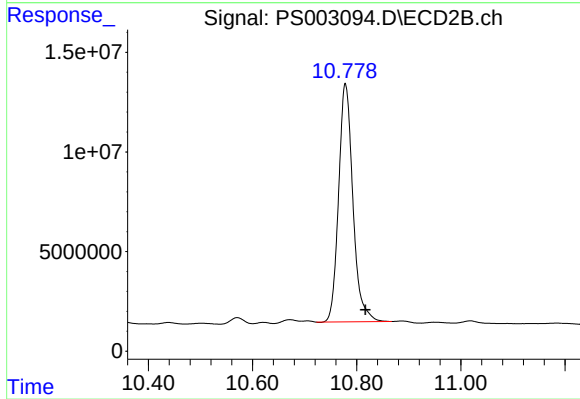

#4 2,4-DCAA


R.T.: 10.778 min
Delta R.T.: -0.038 min
Response: 227857377
Conc: 532.94 ng/ml

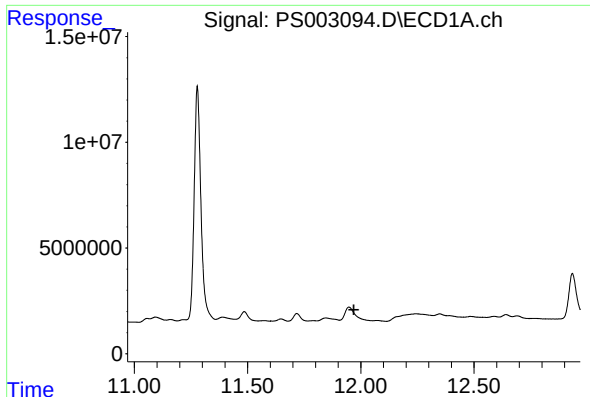

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RT-3451

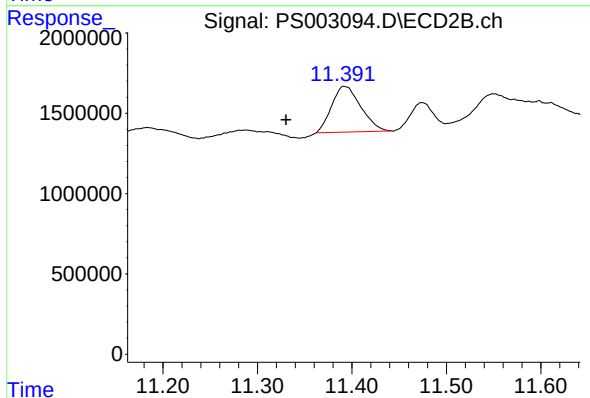


#6 MCPP

R.T.: 11.393 min
Delta R.T.: 0.062 min
Response: 6107031
Conc: 5.54 ug/ml

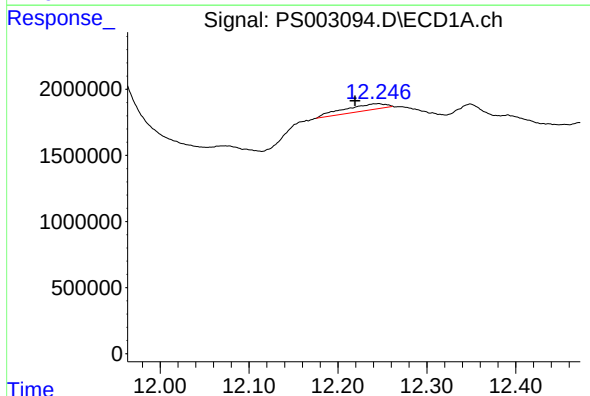


#7 MCPA

R.T.: 12.245 min
Delta R.T.: 0.026 min
Response: 1753484
Conc: 0.99 ug/ml

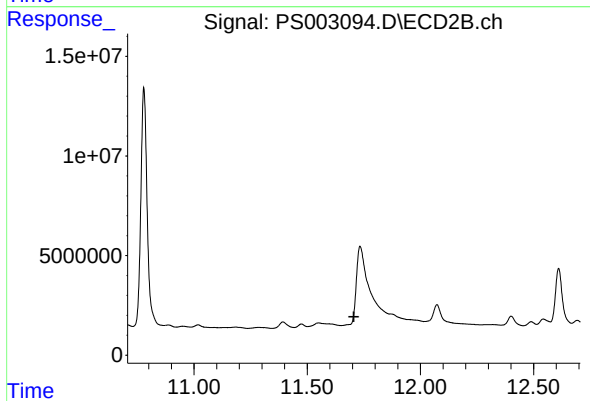

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.706 min
Response: 0
Conc: N.D.

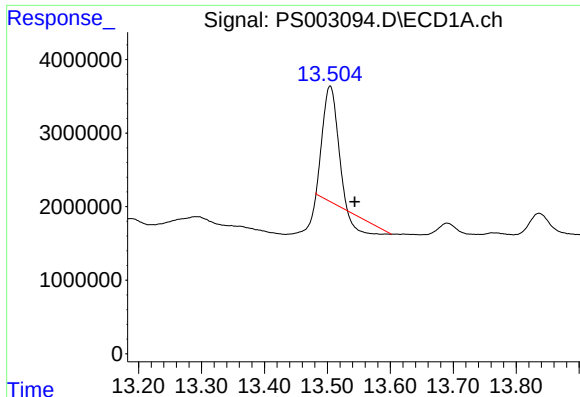

#10 Pentachlorophenol


R.T.: 13.504 min
Delta R.T.: -0.039 min
Response: 21025694
Conc: 3.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
RT-3451

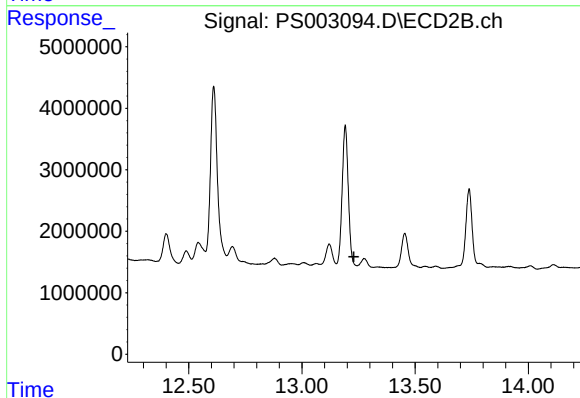


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.229 min
Response: 0
Conc: N.D.

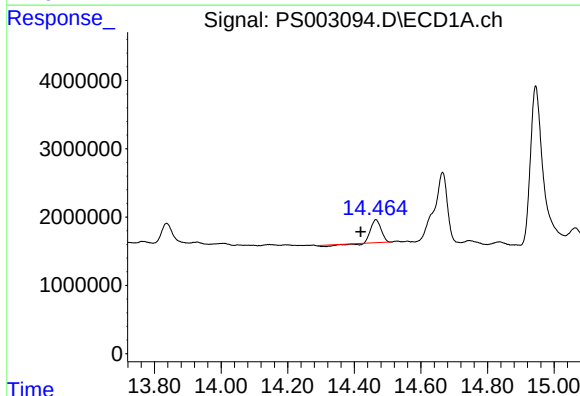


#11 2,4,5-TP (SILVEX)

R.T.: 14.465 min
Delta R.T.: 0.045 min
Response: 6456320
Conc: 2.56 ng/ml

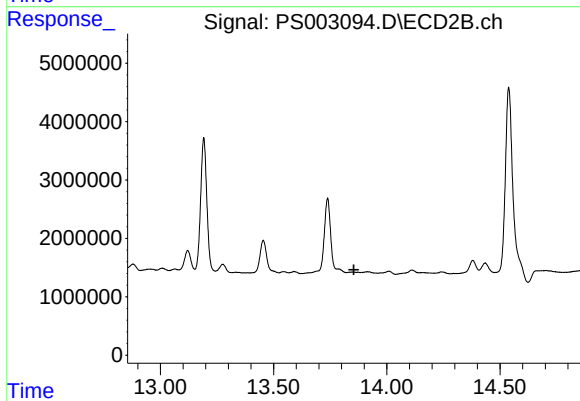

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

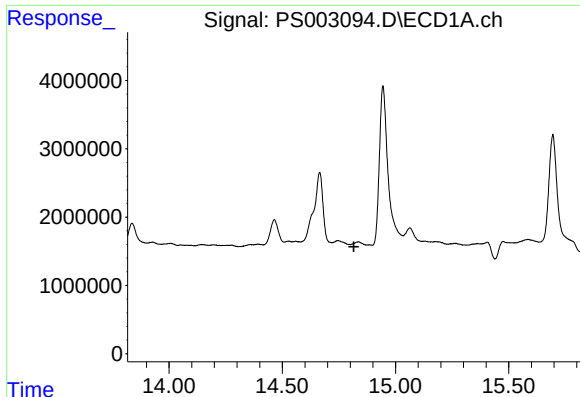

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RT-3451

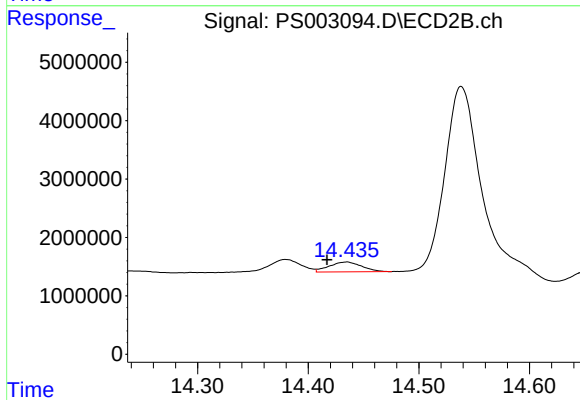


#12 2,4,5-T

R.T.: 14.434 min
Delta R.T.: 0.017 min
Response: 3451504
Conc: 1.80 ng/ml

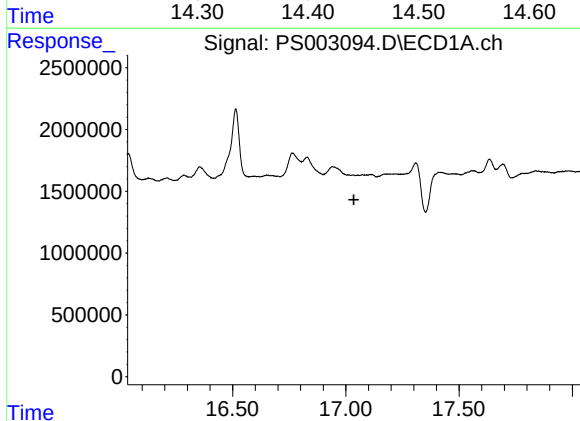


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

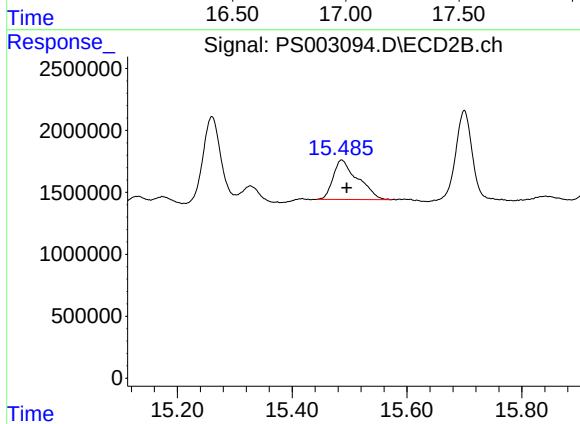

#14 DINOSEB


R.T.: 15.486 min
Delta R.T.: -0.009 min
Response: 9489251
Conc: 5.41 ng/ml

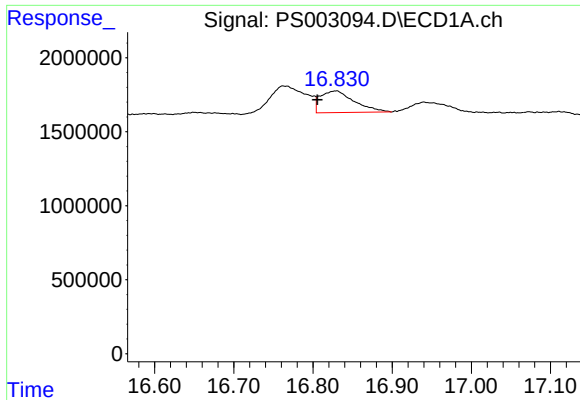

#15 Picloram


R.T.: 16.827 min
Delta R.T.: 0.022 min
Response: 4328148
Conc: 1.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
RT-3451

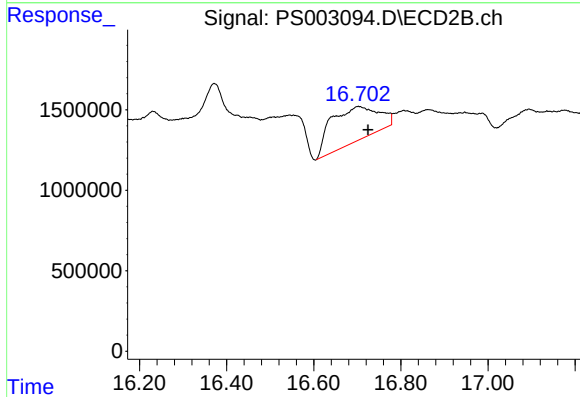


#15 Picloram

R.T.: 16.702 min
Delta R.T.: -0.022 min
Response: 16407136
Conc: 5.46 ng/ml

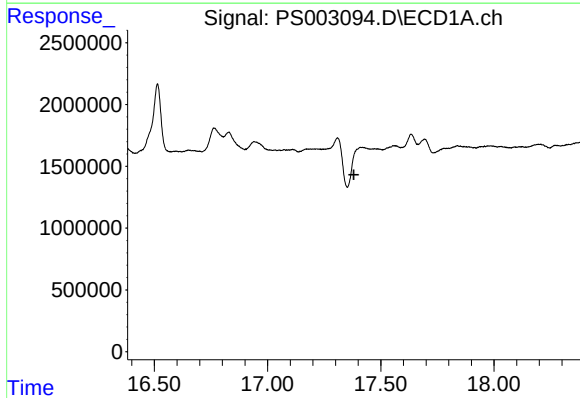

#16 DCPA

R.T.: 17.417 min
Delta R.T.: 0.035 min
Response: -7589239
Conc: N.D.

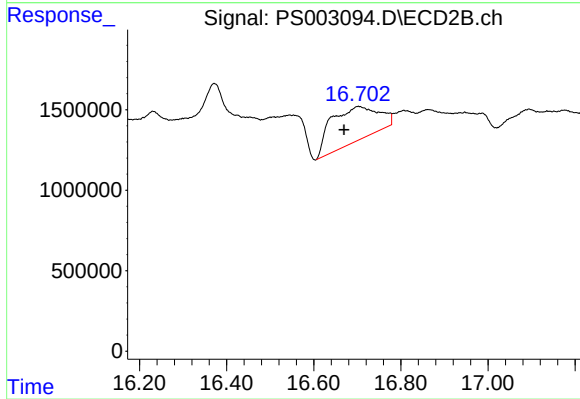

#16 DCPA

R.T.: 16.702 min
Delta R.T.: 0.033 min
Response: 16407136
Conc: 5.30 ng/ml