

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020821\
 Data File : PD061134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2021 11:42
 Operator : DD\AJ
 Sample : PIBLK03
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 06:12:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 26 00:33:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.495	4.019	24668756	164.3E6	24.304	22.959
2) SA Decachlor...	8.274	9.101	44335253	259.5E6	35.186	38.217
Target Compounds						
3) MA gamma-BHC...	0.000	4.693	0	280148	N.D.	<MDL
4) MA Heptachlor	4.482f	0.000	235007	0	0.156	N.D. #
6) B beta-BHC	4.482	0.000	235007	0	0.377	N.D. #
7) B delta-BHC	0.000	5.056f	0	2798405	N.D.	0.275
8) B Heptachlo...	0.000	5.854f	0	7491910	N.D.	0.865
10) B trans-Chl...	0.000	6.098f	0	1210467	N.D.	0.129


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020821\
Data File : PD061134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2021 11:42
Operator : DD\AJ
Sample : PIBLK03
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 06:12:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jan 26 00:33:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

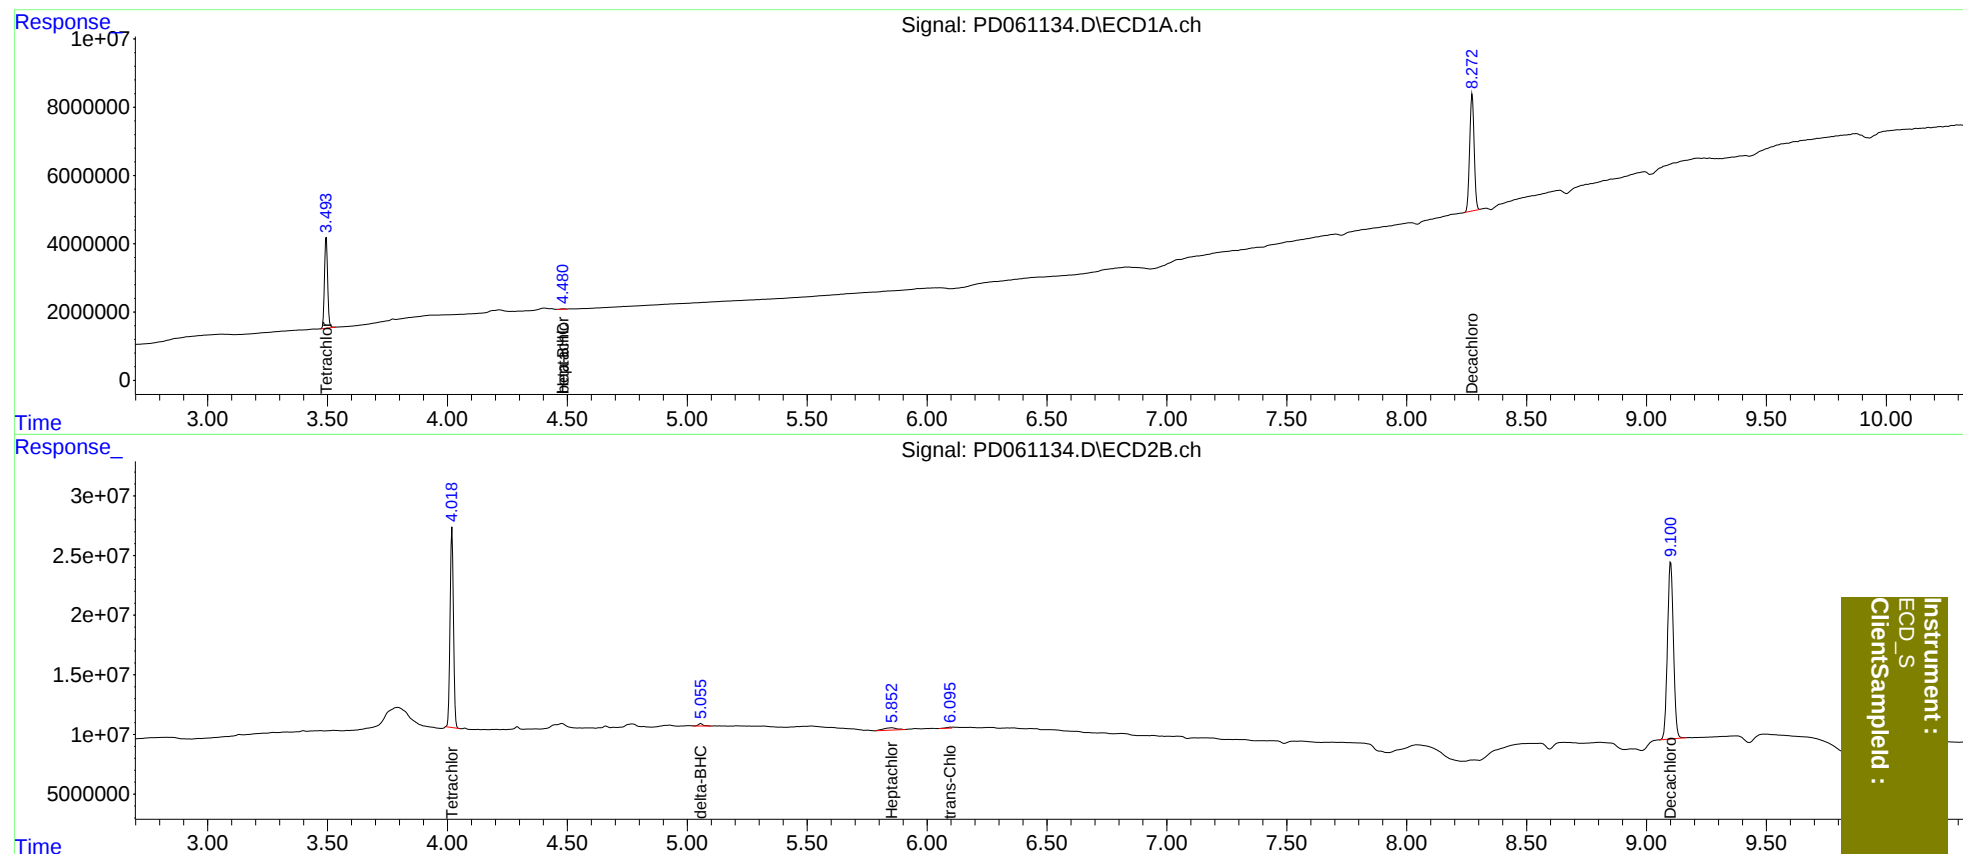


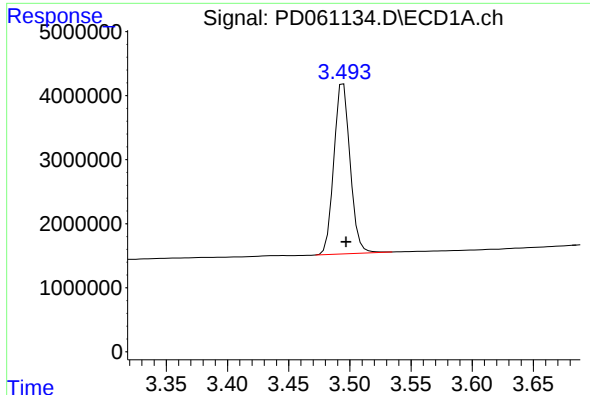

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: -0.002 min
Response: 24668756
Conc: 24.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

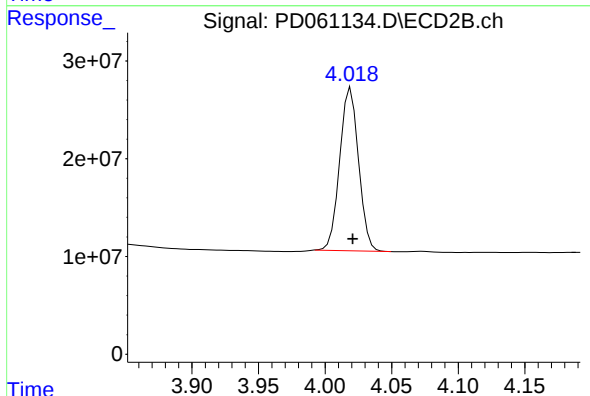


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: -0.001 min
Response: 164293388
Conc: 22.96 ng/ml

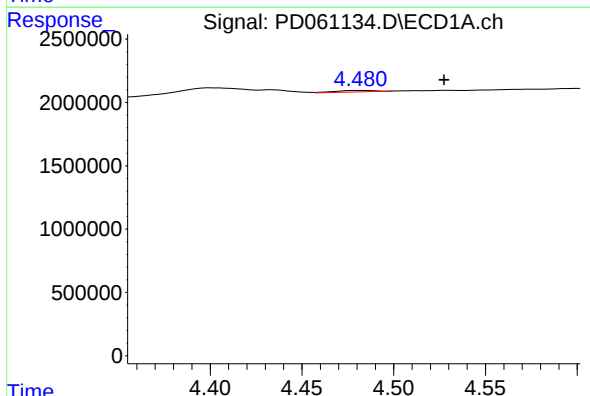


#4 Heptachlor

R.T.: 4.482 min
Delta R.T.: -0.046 min
Response: 235007
Conc: 0.16 ng/ml

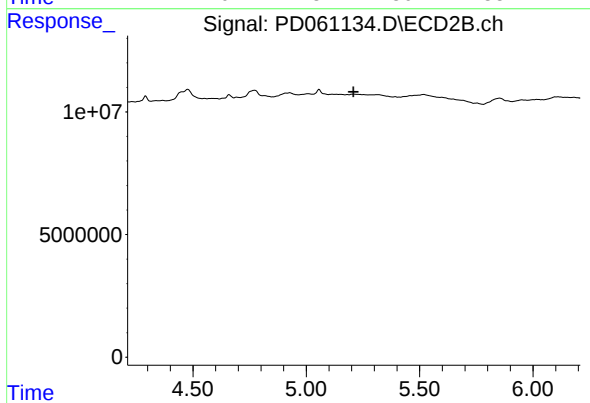

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.209 min
Response: 0
Conc: N.D.

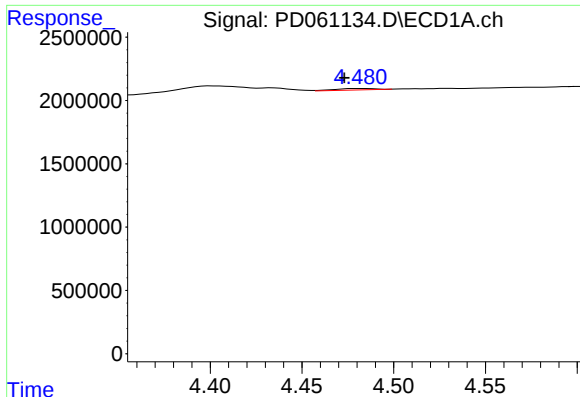

#6 beta-BHC


R.T.: 4.482 min
Delta R.T.: 0.008 min
Response: 235007
Conc: 0.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

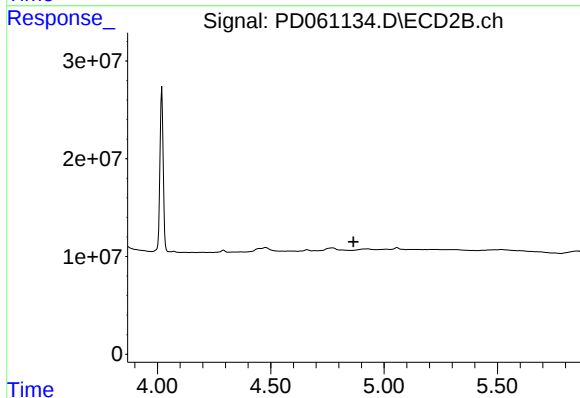


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.866 min
Response: 0
Conc: N.D.

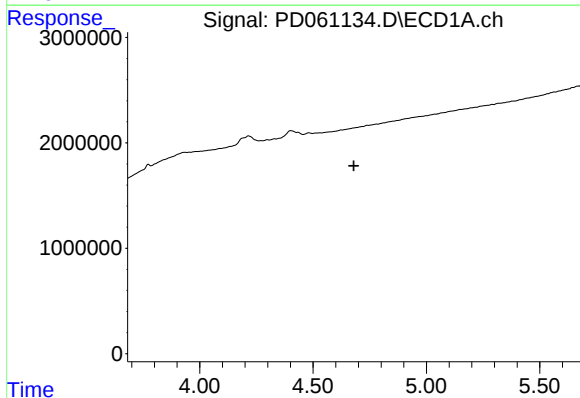


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.680 min
Response: 0
Conc: N.D.

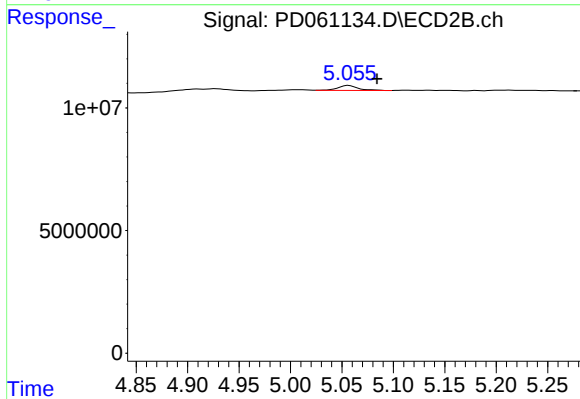

#7 delta-BHC


R.T.: 5.056 min
Delta R.T.: -0.028 min
Response: 2798405
Conc: 0.27 ng/ml

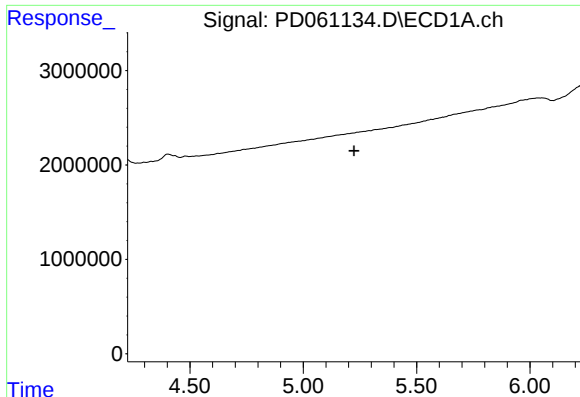

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.224 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

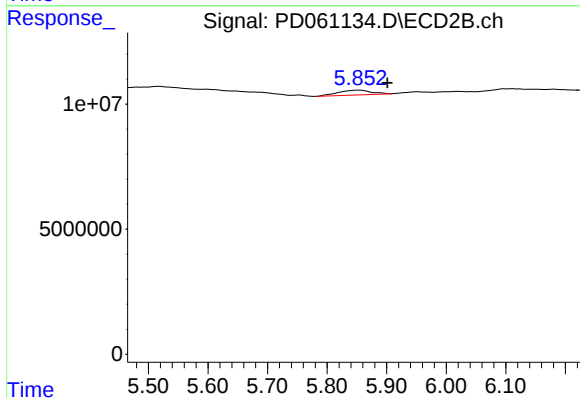


#8 Heptachlor epoxide

R.T.: 5.854 min
Delta R.T.: -0.048 min
Response: 7491910
Conc: 0.86 ng/ml

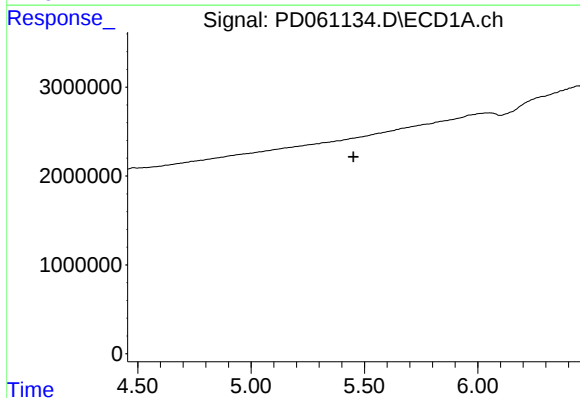


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.452 min
Response: 0
Conc: N.D.

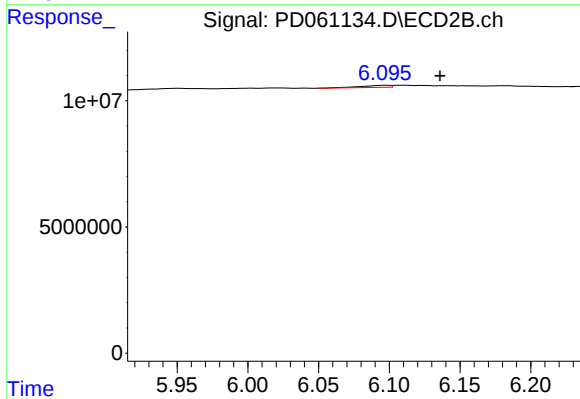

#10 trans-Chlordane


R.T.: 6.098 min
Delta R.T.: -0.038 min
Response: 1210467
Conc: 0.13 ng/ml

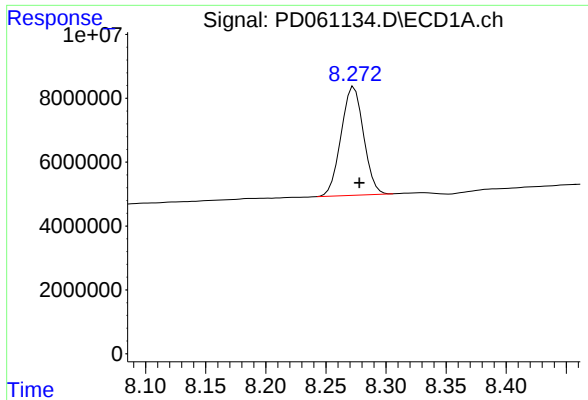

#27 Decachlorobiphenyl

R.T.: 8.274 min
Delta R.T.: -0.004 min
Response: 44335253
Conc: 35.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

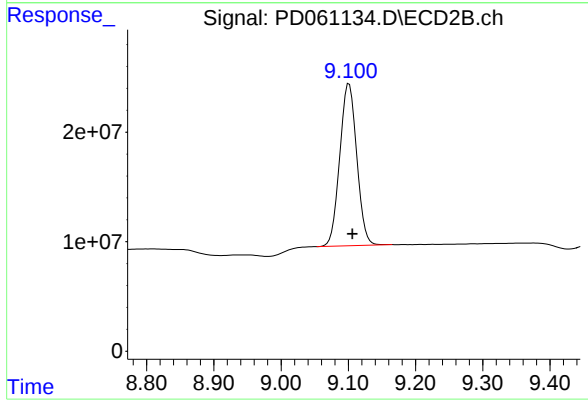

#27 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: -0.005 min
Response: 259525588
Conc: 38.22 ng/ml