

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020822\
 Data File : PS018263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2022 15:51
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 04:01:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 09 03:44:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.030	6.640	659.2E6	313.2E6	419.081	499.276
Target Compounds							
5) T	DICAMBA	7.216	0.000	8931107	0	1.414	N.D. #
9) T	2,4-D	8.179f	0.000	15870500	0	8.619	N.D. #
10) T	Pentachlo...	8.426	8.110	27170565	11362990	1.286	1.316
11) T	2,4,5-TP ...	8.982	0.000	11724801	0	1.372	N.D. #
12) T	2,4,5-T	9.281	0.000	37526117	0	4.240	N.D. #
13) T	2,4-DB	9.845	0.000	15713735	0	8.928	N.D. #
14) T	DINOSEB	10.944	0.000	26466482	0	3.964	N.D. #
15) T	Picloram	10.765	10.684	2361029	78052758	<MDL	15.573 #
16) T	DCPA	11.214	10.590	19407177	7782675	1.761	1.710



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020822\
Data File : PS018263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2022 15:51
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 04:01:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
Quant Title : 8080.M
QLast Update : Wed Feb 09 03:44:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

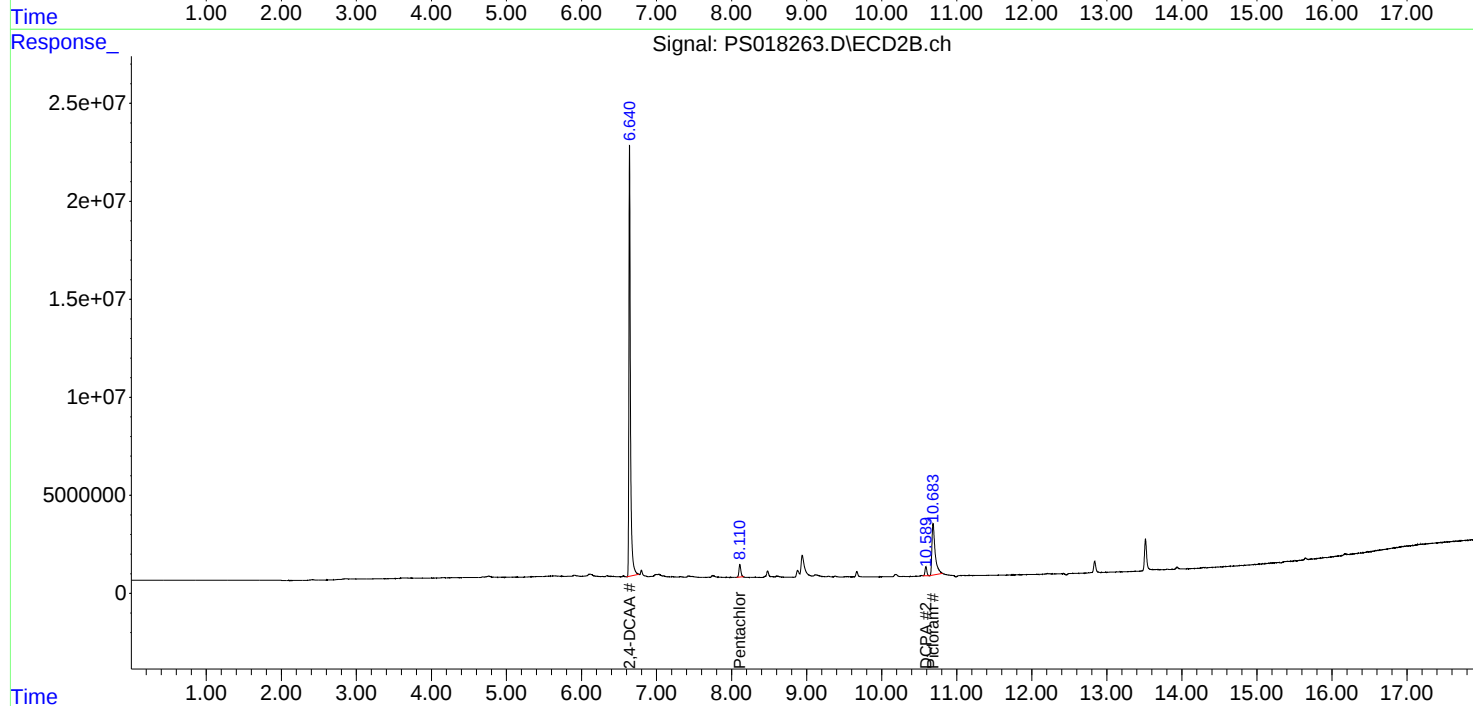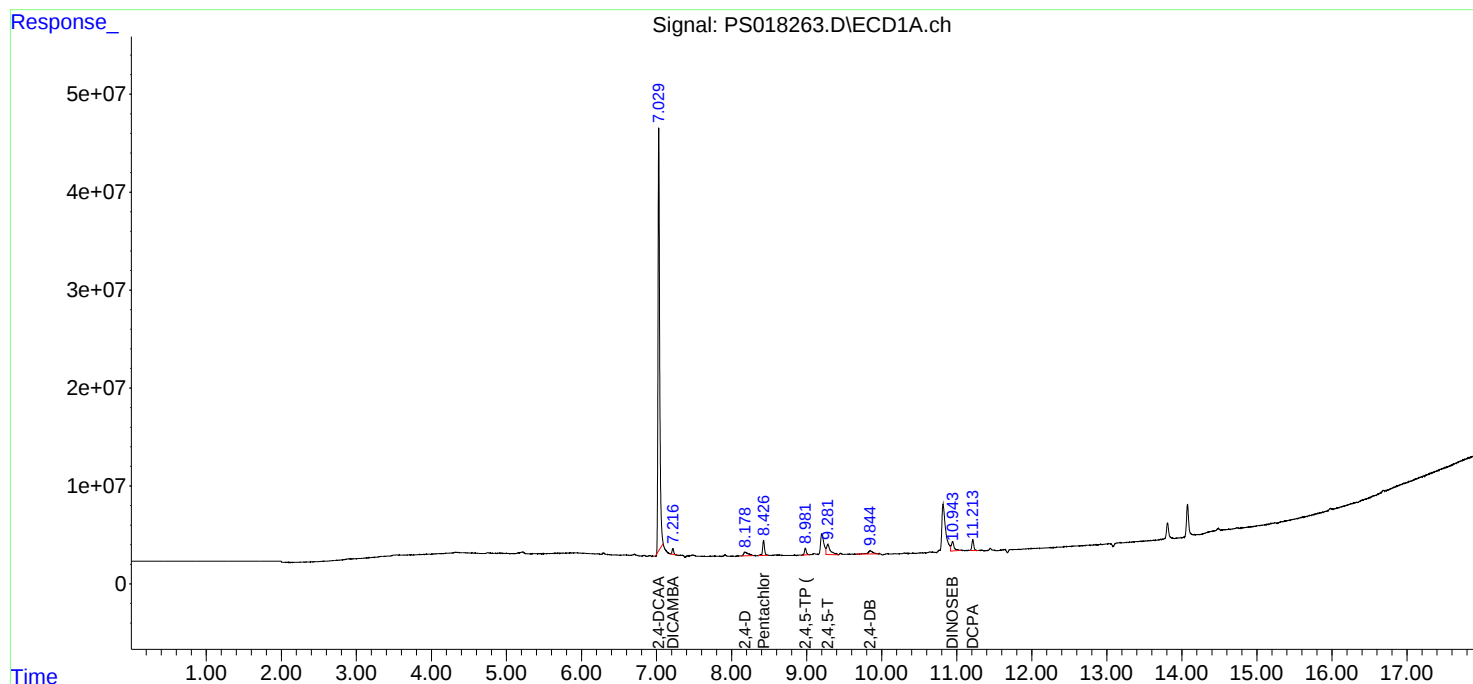


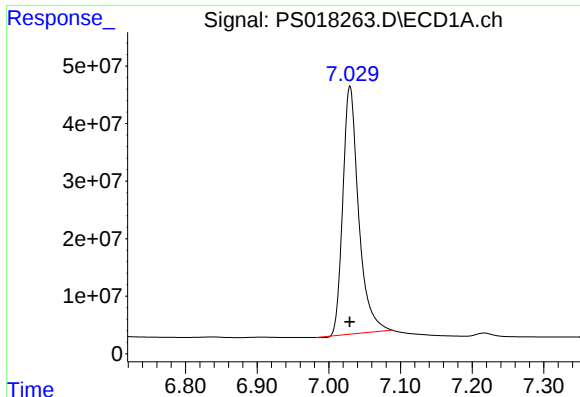

#4 2,4-DCAA


R.T.: 7.030 min
Delta R.T.: 0.000 min
Response: 659246250
Conc: 419.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

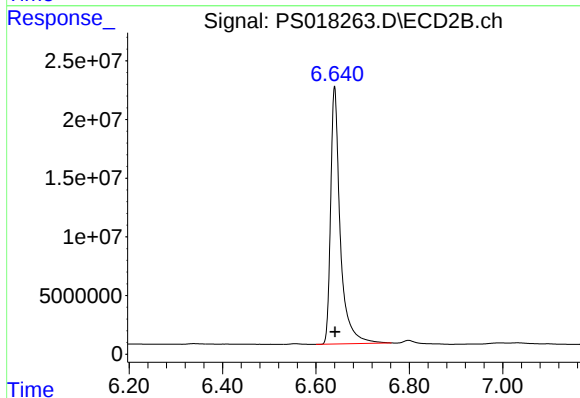


#4 2,4-DCAA

R.T.: 6.640 min
Delta R.T.: -0.001 min
Response: 313161083
Conc: 499.28 ng/ml

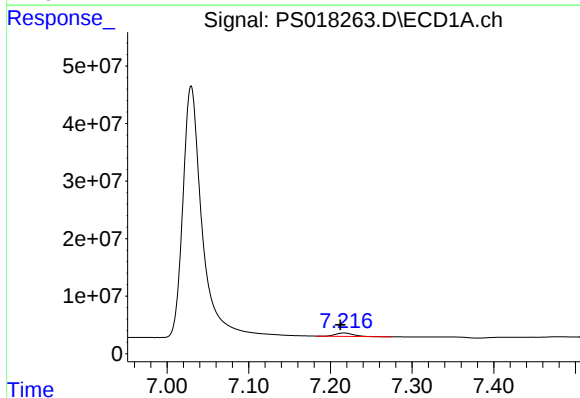


#5 DICAMBA

R.T.: 7.216 min
Delta R.T.: 0.004 min
Response: 8931107
Conc: 1.41 ng/ml

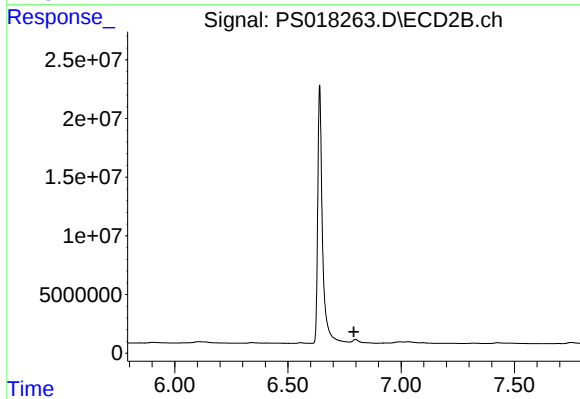

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.791 min
Response: 0
Conc: N.D.

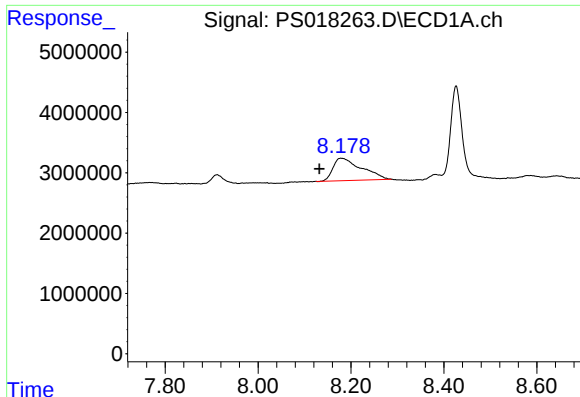

#9 2,4-D


R.T.: 8.179 min
Delta R.T.: 0.047 min
Response: 15870500
Conc: 8.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

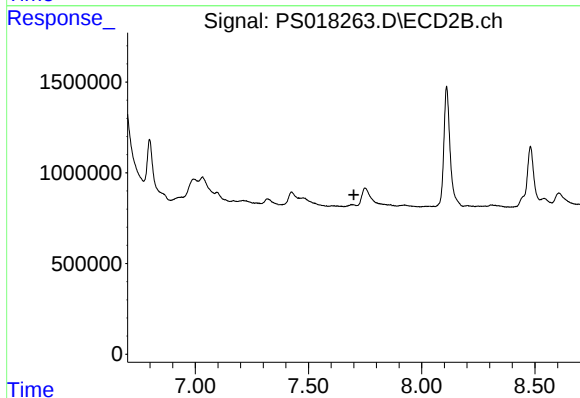


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.

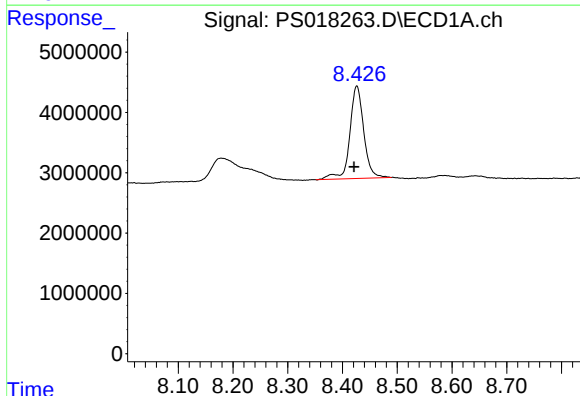


#10 Pentachlorophenol

R.T.: 8.426 min
Delta R.T.: 0.005 min
Response: 27170565
Conc: 1.29 ng/ml

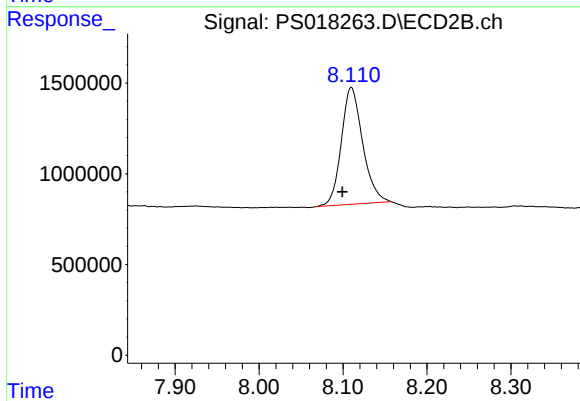

#10 Pentachlorophenol


R.T.: 8.110 min
Delta R.T.: 0.011 min
Response: 11362990
Conc: 1.32 ng/ml

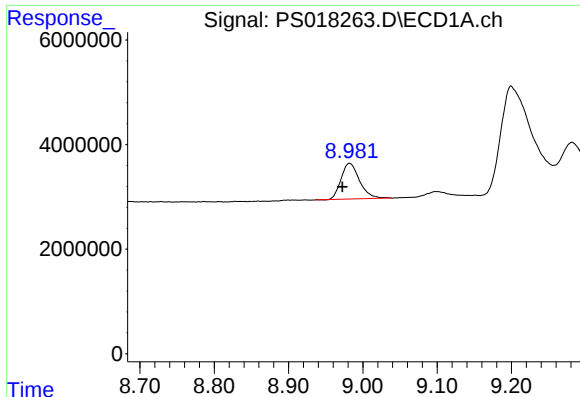

#11 2,4,5-TP (SILVEX)


R.T.: 8.982 min
Delta R.T.: 0.009 min
Response: 11724801
Conc: 1.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

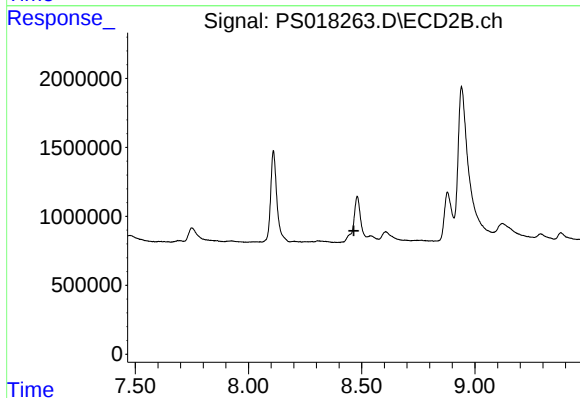


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.465 min
Response: 0
Conc: N.D.

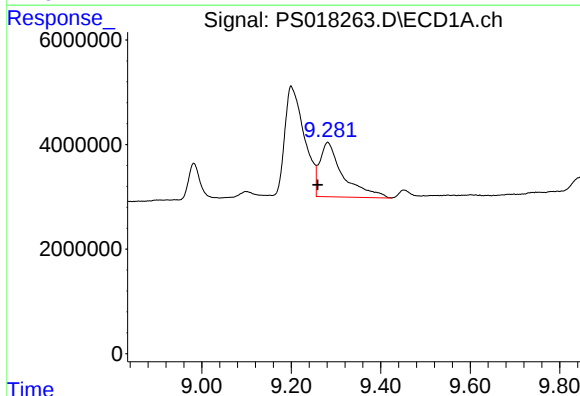


#12 2,4,5-T

R.T.: 9.281 min
Delta R.T.: 0.022 min
Response: 37526117
Conc: 4.24 ng/ml

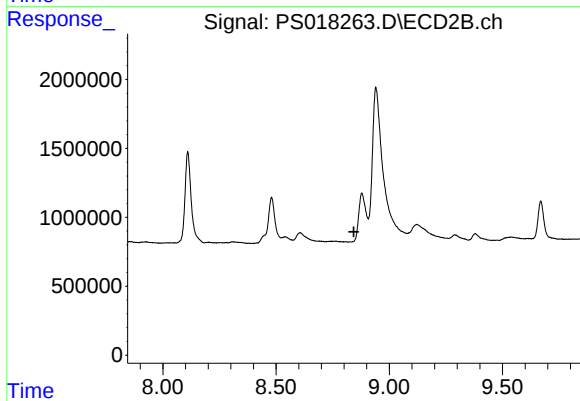

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.844 min
Response: 0
Conc: N.D.

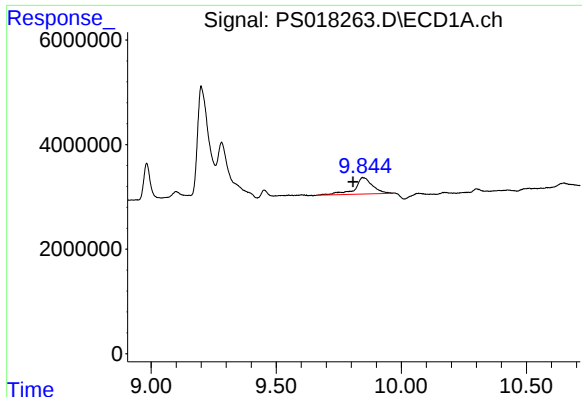

#13 2,4-DB


R.T.: 9.845 min
Delta R.T.: 0.037 min
Response: 15713735
Conc: 8.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

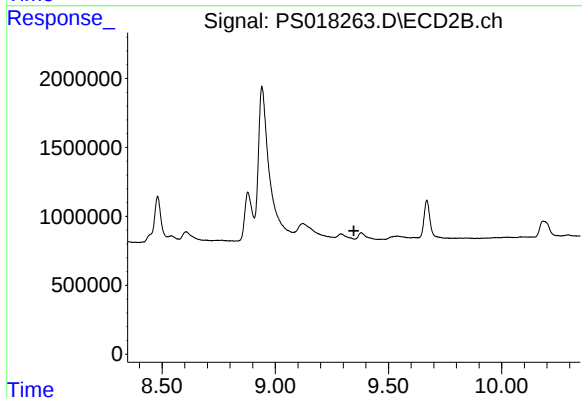


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.347 min
Response: 0
Conc: N.D.

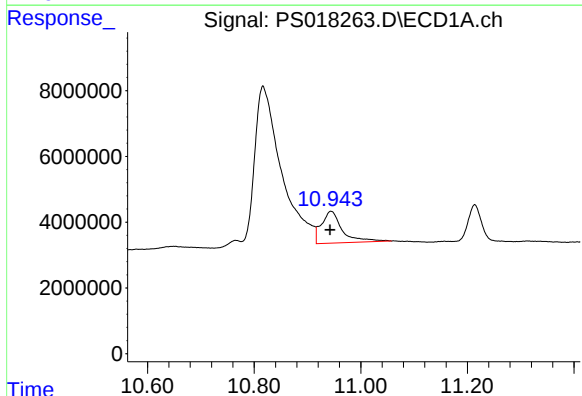


#14 DINOSEB

R.T.: 10.944 min
Delta R.T.: 0.002 min
Response: 26466482
Conc: 3.96 ng/ml

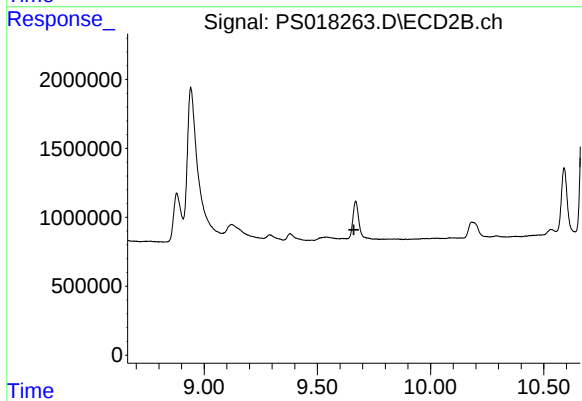

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.661 min
Response: 0
Conc: N.D.

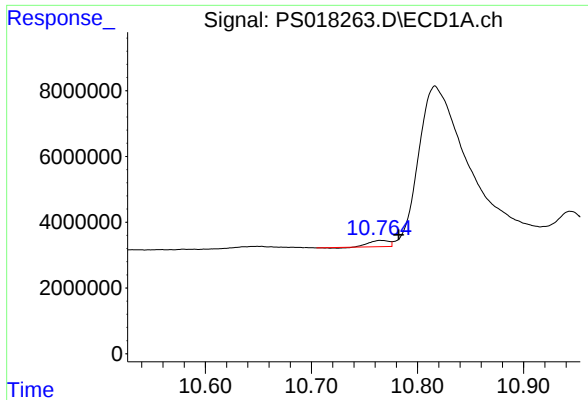

#15 Picloram


R.T.: 10.765 min
Delta R.T.: -0.017 min
Response: 2361029
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

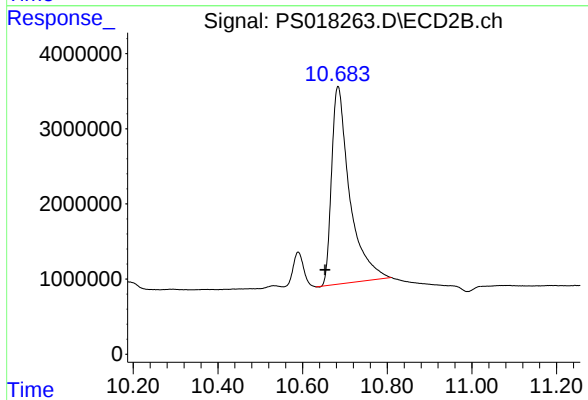


#15 Picloram

R.T.: 10.684 min
Delta R.T.: 0.031 min
Response: 78052758
Conc: 15.57 ng/ml

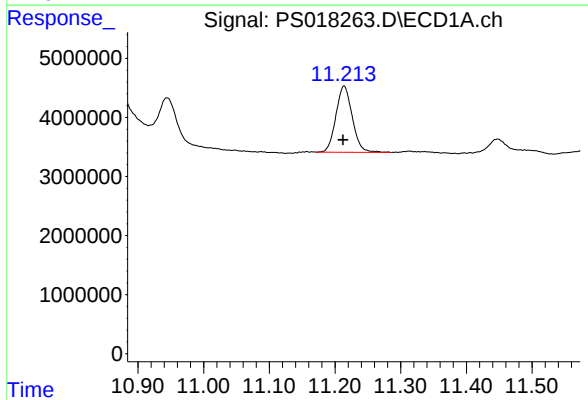

#16 DCPA

R.T.: 11.214 min
Delta R.T.: 0.001 min
Response: 19407177
Conc: 1.76 ng/ml

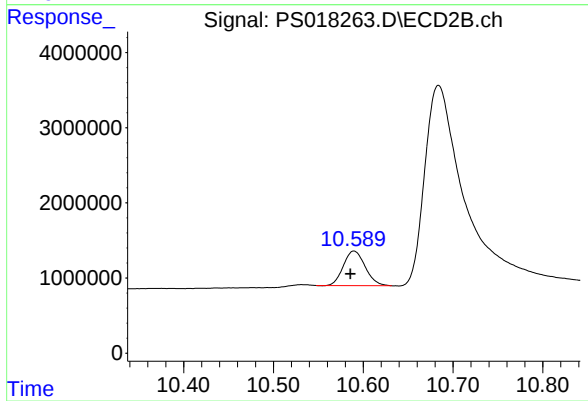

#16 DCPA

R.T.: 10.590 min
Delta R.T.: 0.004 min
Response: 7782675
Conc: 1.71 ng/ml