

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020822\
 Data File : PS018261.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2022 15:02
 Operator : AJ\MA
 Sample : HSTDICC1500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC1500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 03:38:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 09 03:30:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.027	6.636	2311.8E6	945.2E6	1463.314	1482.635
Target Compounds							
1) T	Dalapon	2.889	2.406	3477.7E6	1093.7E6	1351.601	1348.004
2) T	3,5-DICHL...	6.270	5.854	3021.4E6	1320.3E6	1349.492	1360.787
3) T	4-Nitroph...	6.856	6.273	1198.3E6	541.9E6	1340.578	1329.490
5) T	DICAMBA	7.212	6.790	8543.8E6	3651.8E6	1356.158	1346.931
6) T	MCPD	7.387	6.891	694.3E6	317.7E6	141.971	140.971
7) T	MCPA	7.535	7.102	939.7E6	440.2E6	138.841	138.505
8) T	DICHLORPROP	7.898	7.399	2157.5E6	970.7E6	1370.909	1383.695
9) T	2,4-D	8.126	7.687	2519.0E6	1161.5E6	1368.772	1378.145
10) T	Pentachlo...	8.421	8.099	26646.1E6	10499.9E6	1315.966	1292.747
11) T	2,4,5-TP ...	8.971	8.462	11423.2E6	4948.4E6	1356.307	1351.841
12) T	2,4,5-T	9.255	8.837	11935.7E6	4808.9E6	1363.882	1357.224
13) T	2,4-DB	9.800	9.339	2502.3E6	691.8E6	1395.845	1411.836
14) T	DINOSEB	10.943	9.660	8924.2E6	3476.8E6	1350.549	1363.140
15) T	Picloram	10.771	10.639	16284.6E6	6973.6E6	1385.887	1363.158
16) T	DCPA	11.213	10.585	14544.4E6	6007.0E6	1355.077	1351.136



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020822\
Data File : PS018261.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2022 15:02
Operator : AJ\MA
Sample : HSTDICC1500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 03:38:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
Quant Title : 8080.M
QLast Update : Wed Feb 09 03:30:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

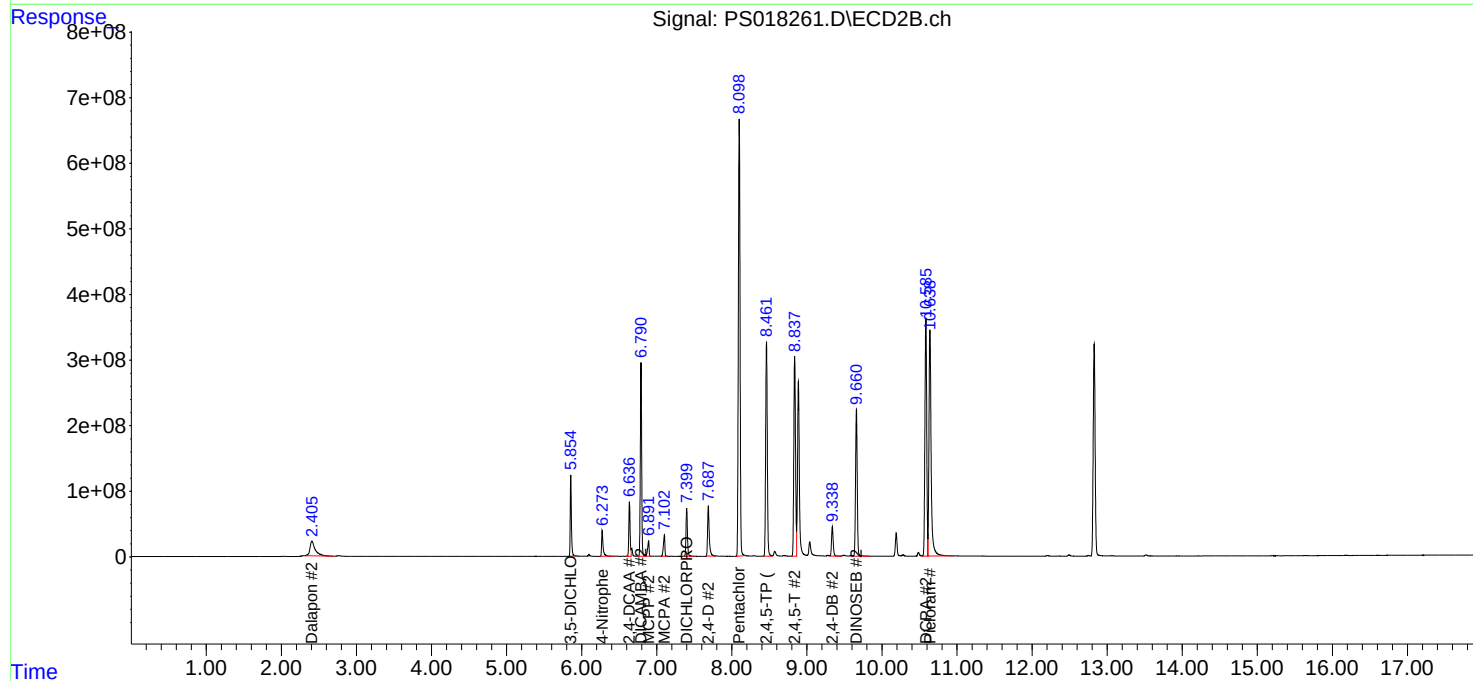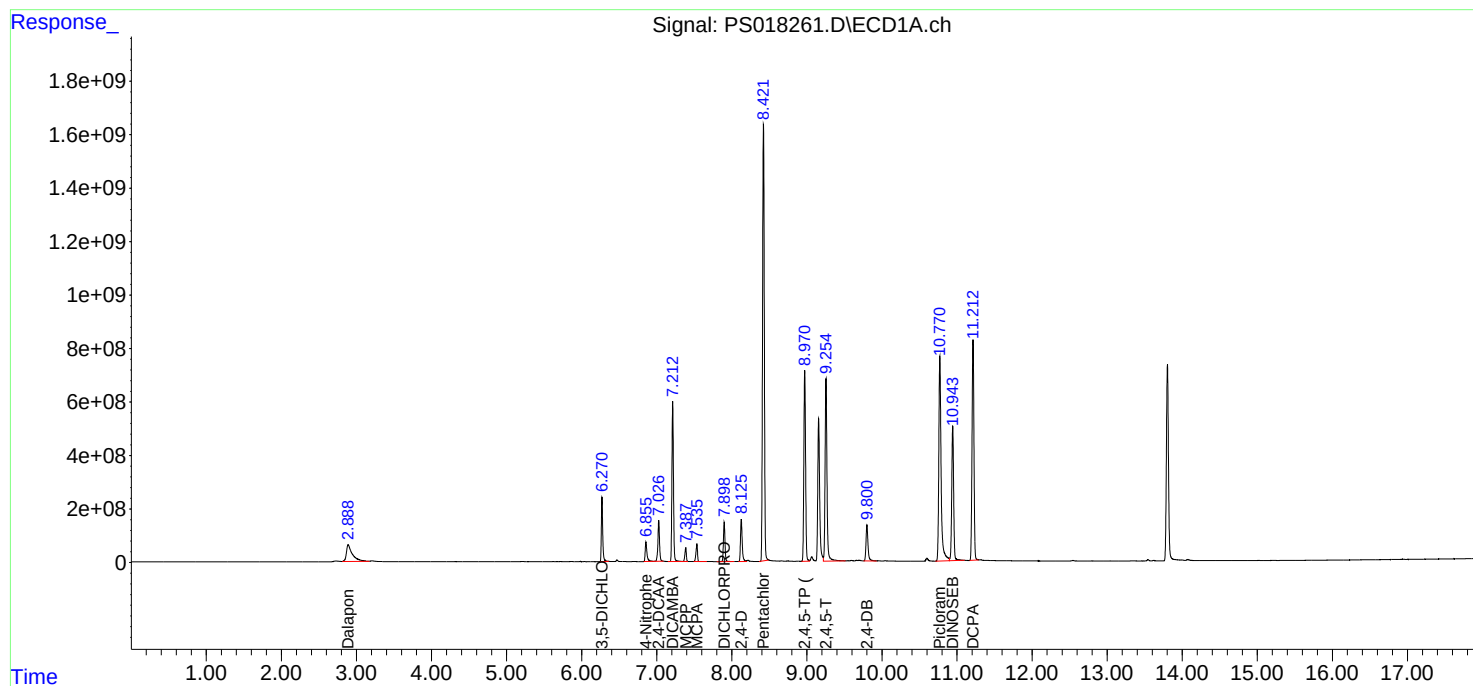


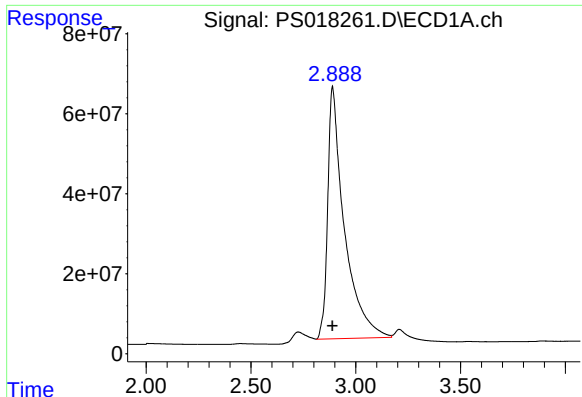

#1 Dalapon


R.T.: 2.889 min
Delta R.T.: 0.000 min
Response: 3477658874
Conc: 1351.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

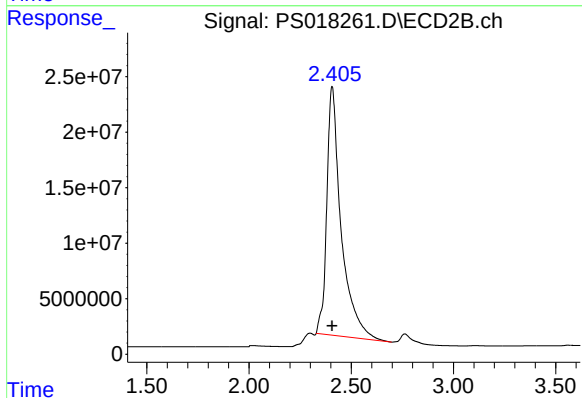


#1 Dalapon

R.T.: 2.406 min
Delta R.T.: 0.000 min
Response: 1093681772
Conc: 1348.00 ng/ml

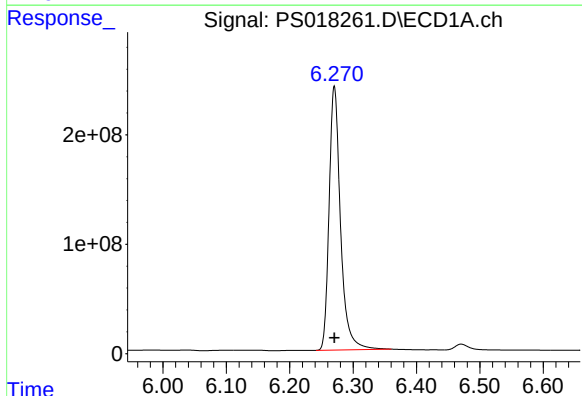


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.270 min
Delta R.T.: 0.000 min
Response: 3021412291
Conc: 1349.49 ng/ml

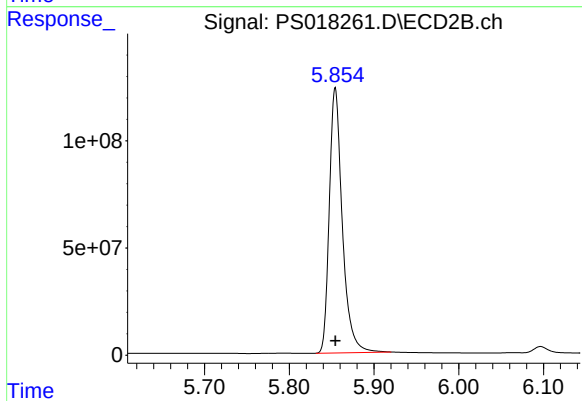

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.854 min
Delta R.T.: 0.000 min
Response: 1320298604
Conc: 1360.79 ng/ml

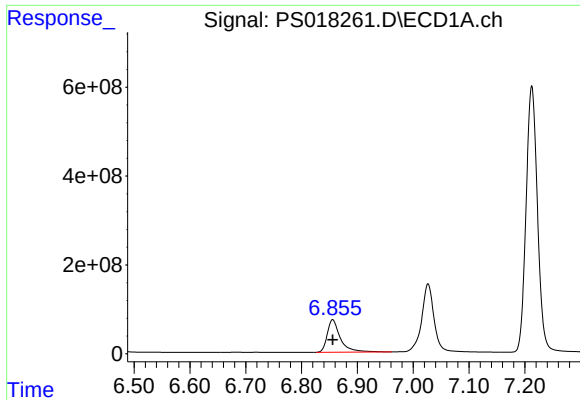

#3 4-Nitrophenol


R.T.: 6.856 min
Delta R.T.: 0.000 min
Response: 1198261080
Conc: 1340.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

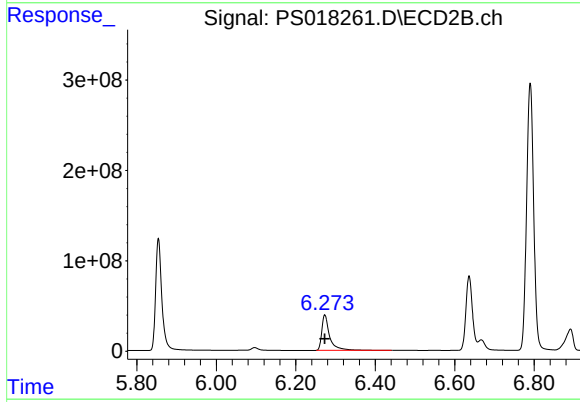


#3 4-Nitrophenol

R.T.: 6.273 min
Delta R.T.: 0.000 min
Response: 541852119
Conc: 1329.49 ng/ml

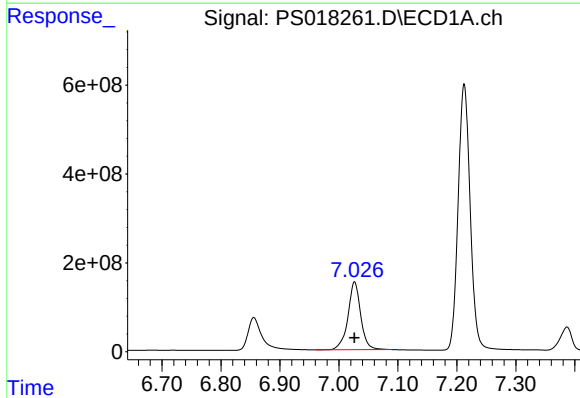


#4 2,4-DCAA

R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 2311819360
Conc: 1463.31 ng/ml

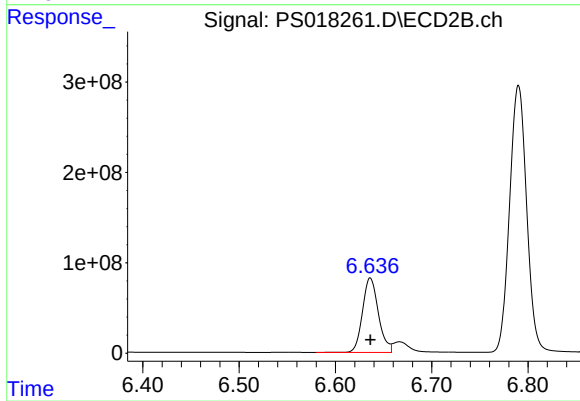

#4 2,4-DCAA


R.T.: 6.636 min
Delta R.T.: 0.000 min
Response: 945209496
Conc: 1482.63 ng/ml

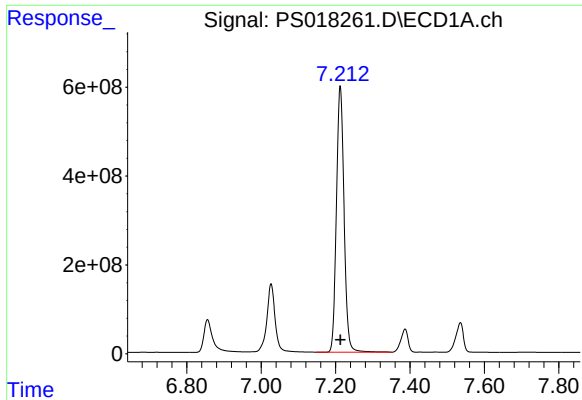

#5 DICAMBA


R.T.: 7.212 min
Delta R.T.: 0.000 min
Response: 8543837375
Conc: 1356.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

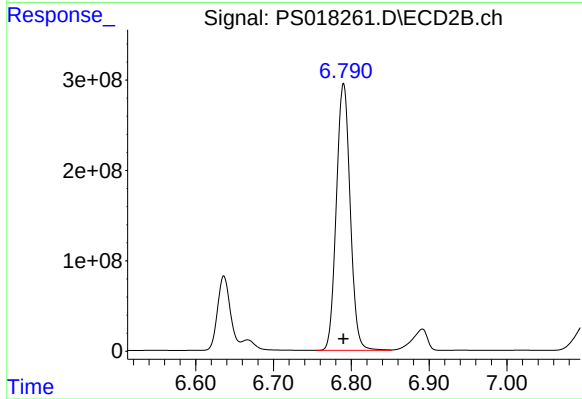


#5 DICAMBA

R.T.: 6.790 min
Delta R.T.: 0.000 min
Response: 3651788468
Conc: 1346.93 ng/ml

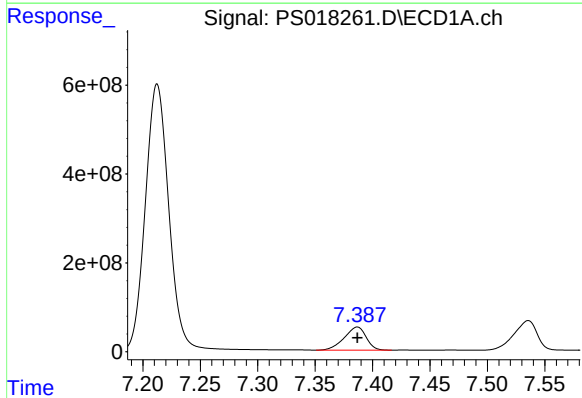


#6 MCP

R.T.: 7.387 min
Delta R.T.: 0.000 min
Response: 694346184
Conc: 141.97 ug/ml

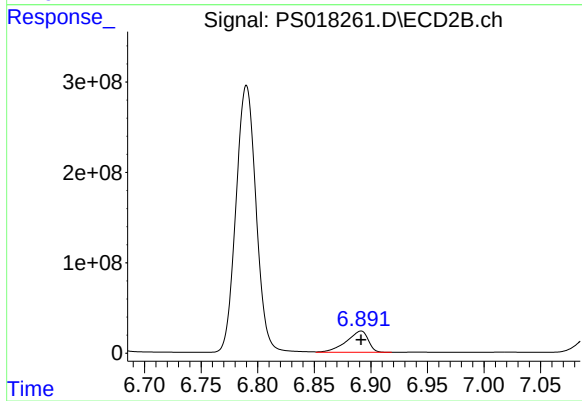

#6 MCP


R.T.: 6.891 min
Delta R.T.: 0.000 min
Response: 317716132
Conc: 140.97 ug/ml

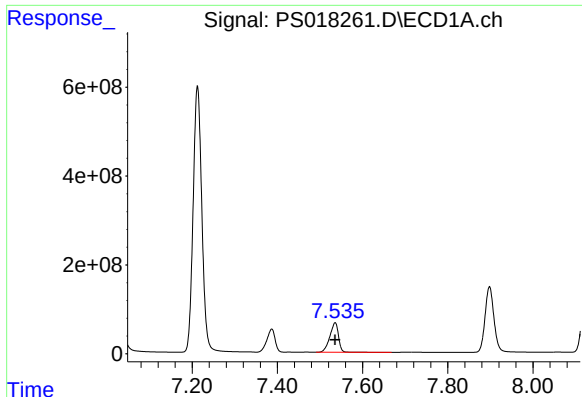

#7 MCPA


R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 939738440
Conc: 138.84 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

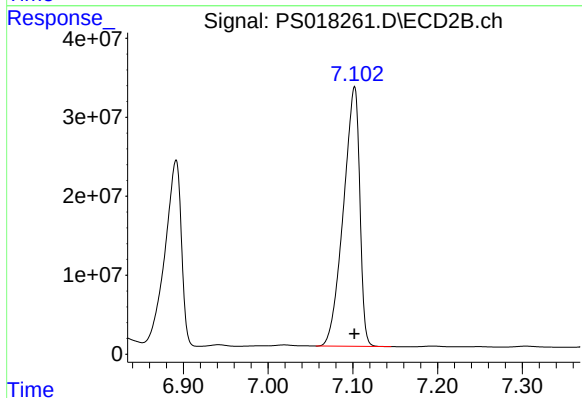


#7 MCPA

R.T.: 7.102 min
Delta R.T.: 0.000 min
Response: 440212420
Conc: 138.51 ug/ml

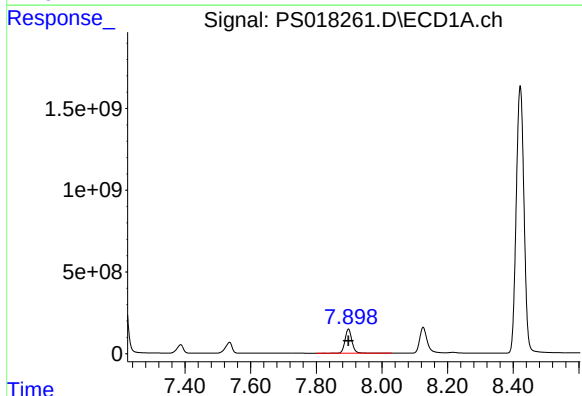


#8 DICHLORPROP

R.T.: 7.898 min
Delta R.T.: 0.000 min
Response: 2157454913
Conc: 1370.91 ng/ml

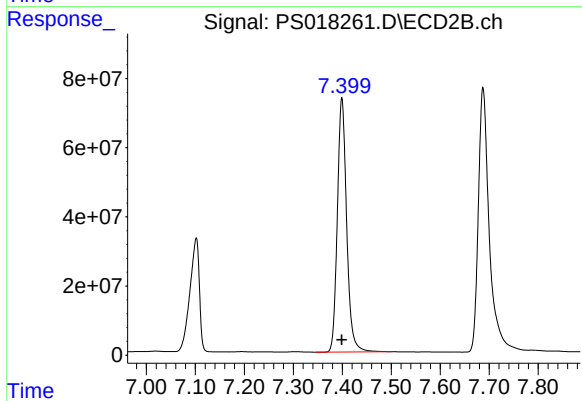

#8 DICHLORPROP


R.T.: 7.399 min
Delta R.T.: 0.000 min
Response: 970690037
Conc: 1383.69 ng/ml

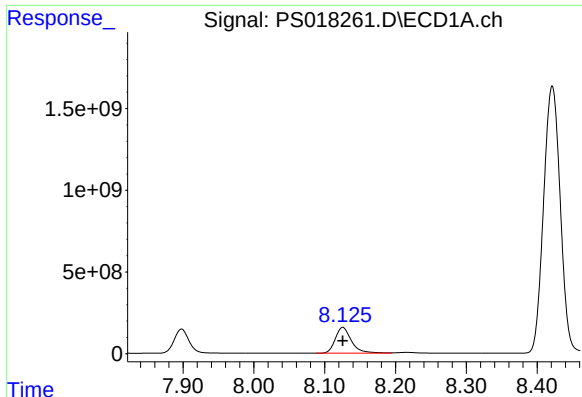

#9 2,4-D


R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 2519037614
Conc: 1368.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

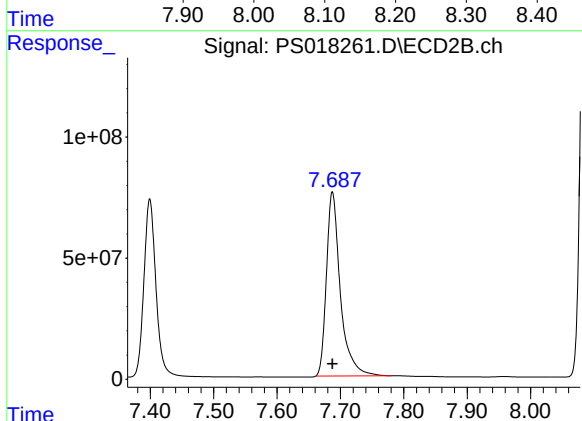


#9 2,4-D

R.T.: 7.687 min
Delta R.T.: 0.000 min
Response: 1161465327
Conc: 1378.14 ng/ml

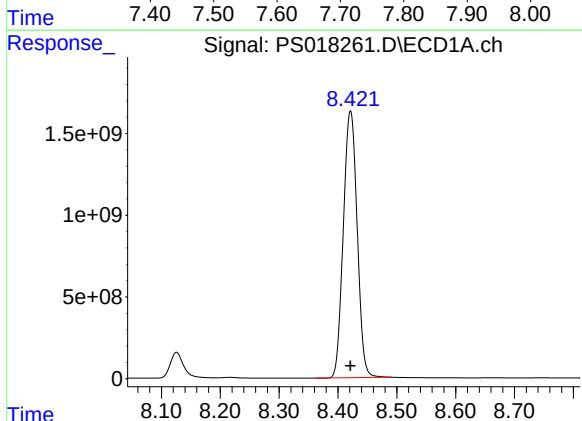


#10 Pentachlorophenol

R.T.: 8.421 min
Delta R.T.: 0.000 min
Response: 26646131868
Conc: 1315.97 ng/ml

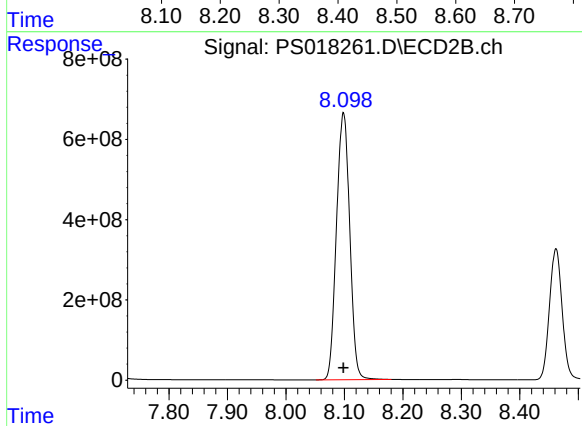

#10 Pentachlorophenol


R.T.: 8.099 min
Delta R.T.: 0.000 min
Response: 10499945923
Conc: 1292.75 ng/ml

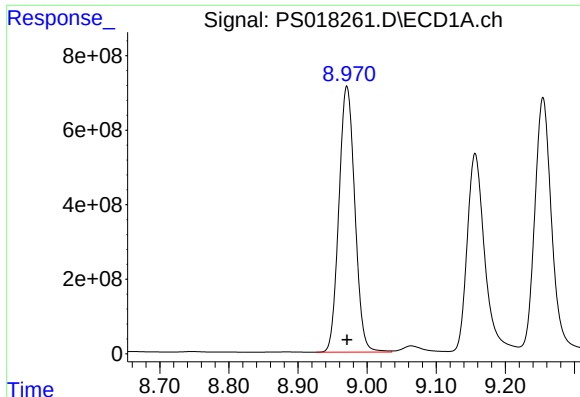

#11 2,4,5-TP (SILVEX)


R.T.: 8.971 min
Delta R.T.: 0.000 min
Response: 11423229389
Conc: 1356.31 ng/m

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

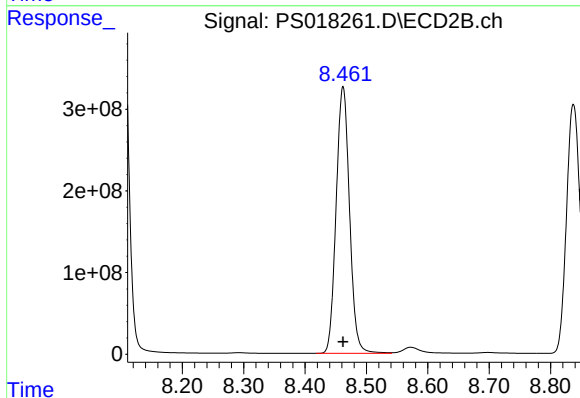


#11 2,4,5-TP (SILVEX)

R.T.: 8.462 min
Delta R.T.: 0.000 min
Response: 4948394848
Conc: 1351.84 ng/ml

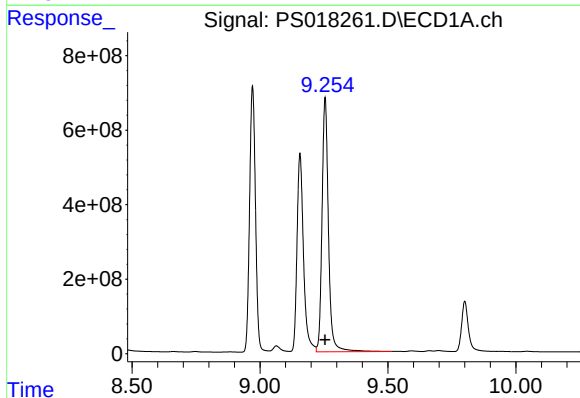


#12 2,4,5-T

R.T.: 9.255 min
Delta R.T.: 0.000 min
Response: 11935673142
Conc: 1363.88 ng/ml

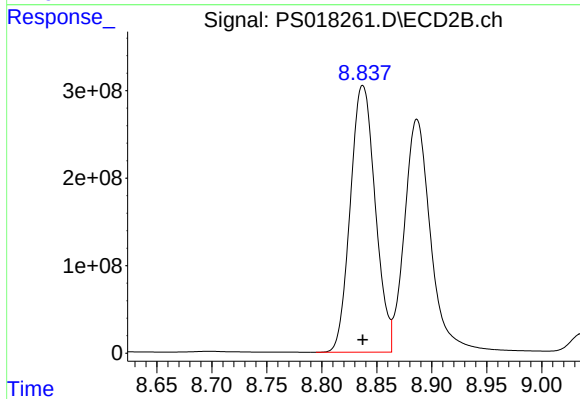

#12 2,4,5-T


R.T.: 8.837 min
Delta R.T.: 0.000 min
Response: 4808916910
Conc: 1357.22 ng/ml

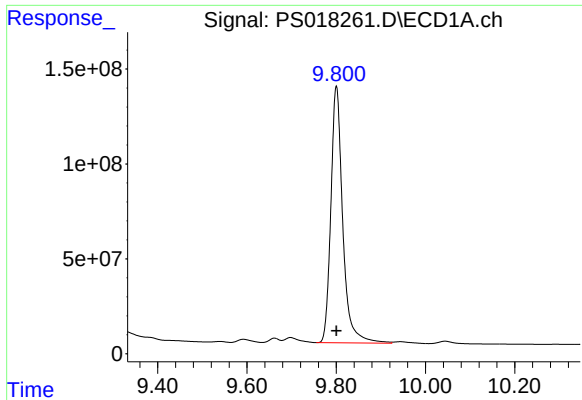

#13 2,4-DB


R.T.: 9.800 min
Delta R.T.: 0.000 min
Response: 2502310212
Conc: 1395.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

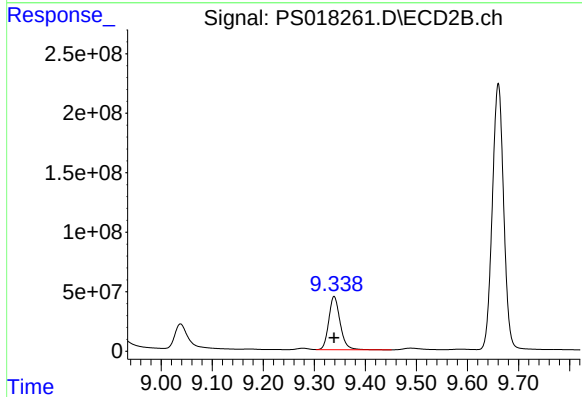


#13 2,4-DB

R.T.: 9.339 min
Delta R.T.: 0.000 min
Response: 691801929
Conc: 1411.84 ng/ml

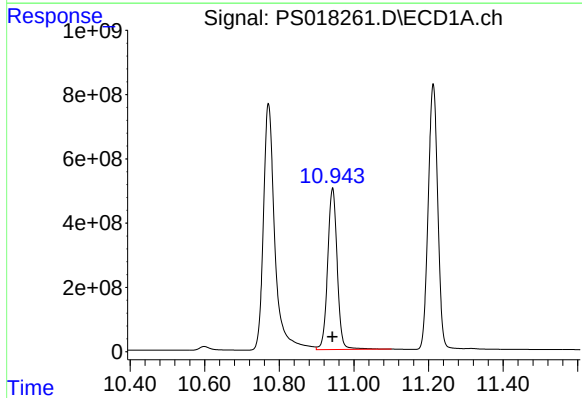


#14 DINOSEB

R.T.: 10.943 min
Delta R.T.: 0.000 min
Response: 8924247632
Conc: 1350.55 ng/ml

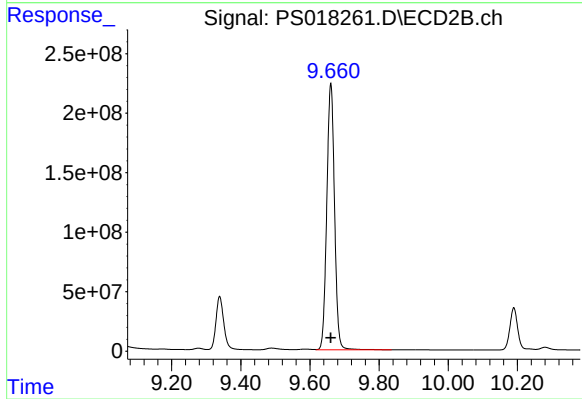

#14 DINOSEB


R.T.: 9.660 min
Delta R.T.: 0.000 min
Response: 3476786543
Conc: 1363.14 ng/ml

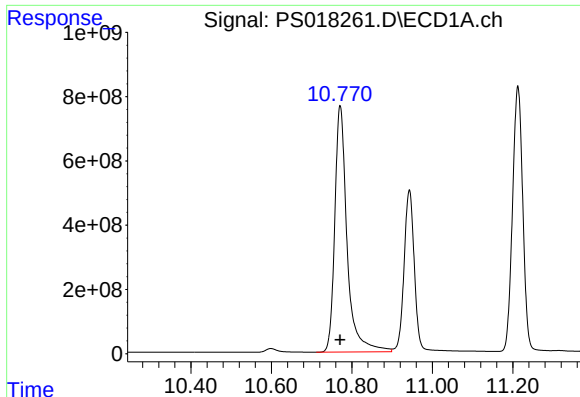

#15 Picloram


R.T.: 10.771 min
Delta R.T.: 0.000 min
Response: 16284565485
Conc: 1385.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

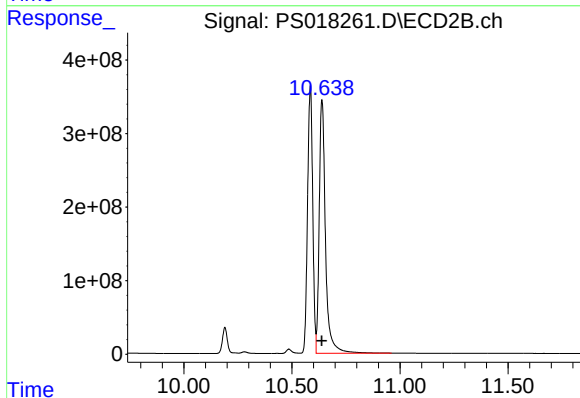


#15 Picloram

R.T.: 10.639 min
Delta R.T.: 0.000 min
Response: 6973625681
Conc: 1363.16 ng/ml

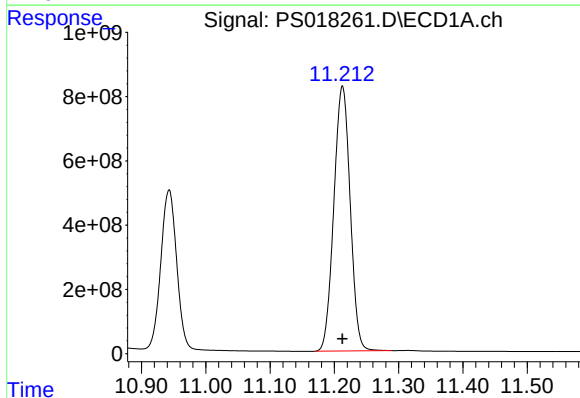

#16 DCPA

R.T.: 11.213 min
Delta R.T.: 0.000 min
Response: 14544411764
Conc: 1355.08 ng/ml

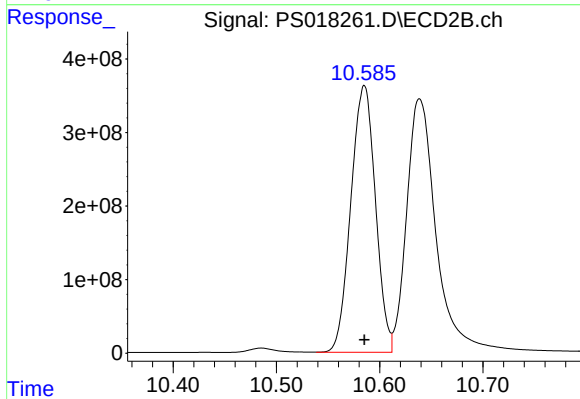

#16 DCPA

R.T.: 10.585 min
Delta R.T.: 0.000 min
Response: 6007043119
Conc: 1351.14 ng/ml