

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020824\
 Data File : PS025868.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2024 15:28
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 04:28:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.348	6.753	743.9E6	385.9E6	527.096	548.569
Target Compounds							
1) T	Dalapon	0.000	2.555	0	1646898	N.D.	1.485
2) T	3,5-DICHL...	5.691	0.000	9882234	0	4.585	N.D. #
3) T	4-Nitroph...	6.185	6.361	6929386	822059	7.465	1.799 #
5) T	DICAMBA	0.000	6.950	0	11034014	N.D.	3.636
6) T	MCP	6.706f	6.950f	54583413	11034014	15.004	5.393 #
7) T	MCPA	6.706f	0.000	54583413	0	10.139	N.D. #
8) T	DICHLORPROP	0.000	7.549	0	22870576	N.D.	28.640
9) T	2,4-D	7.244	7.761f	39552073	352969	22.255	<MDL #
10) T	Pentachlo...	0.000	8.227	0	847365	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020824\
Data File : PS025868.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2024 15:28
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 04:28:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

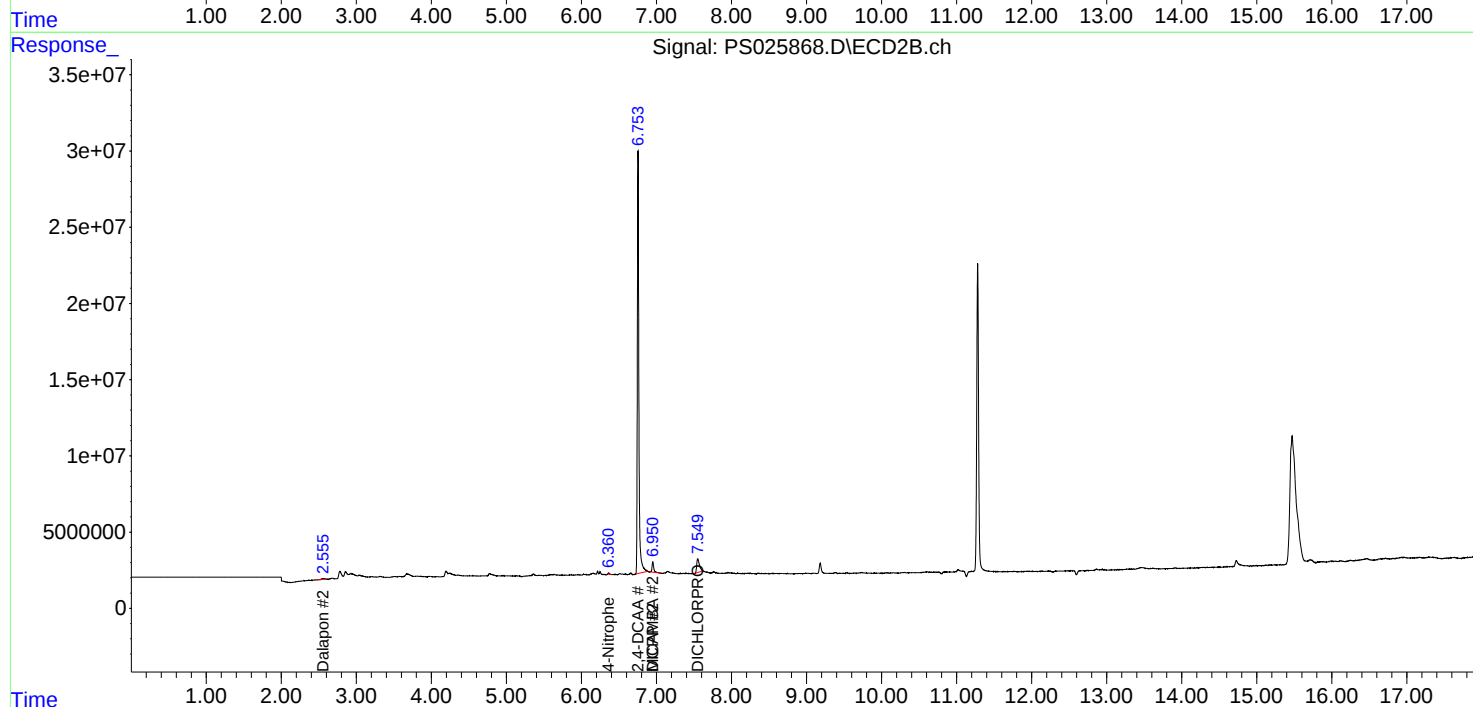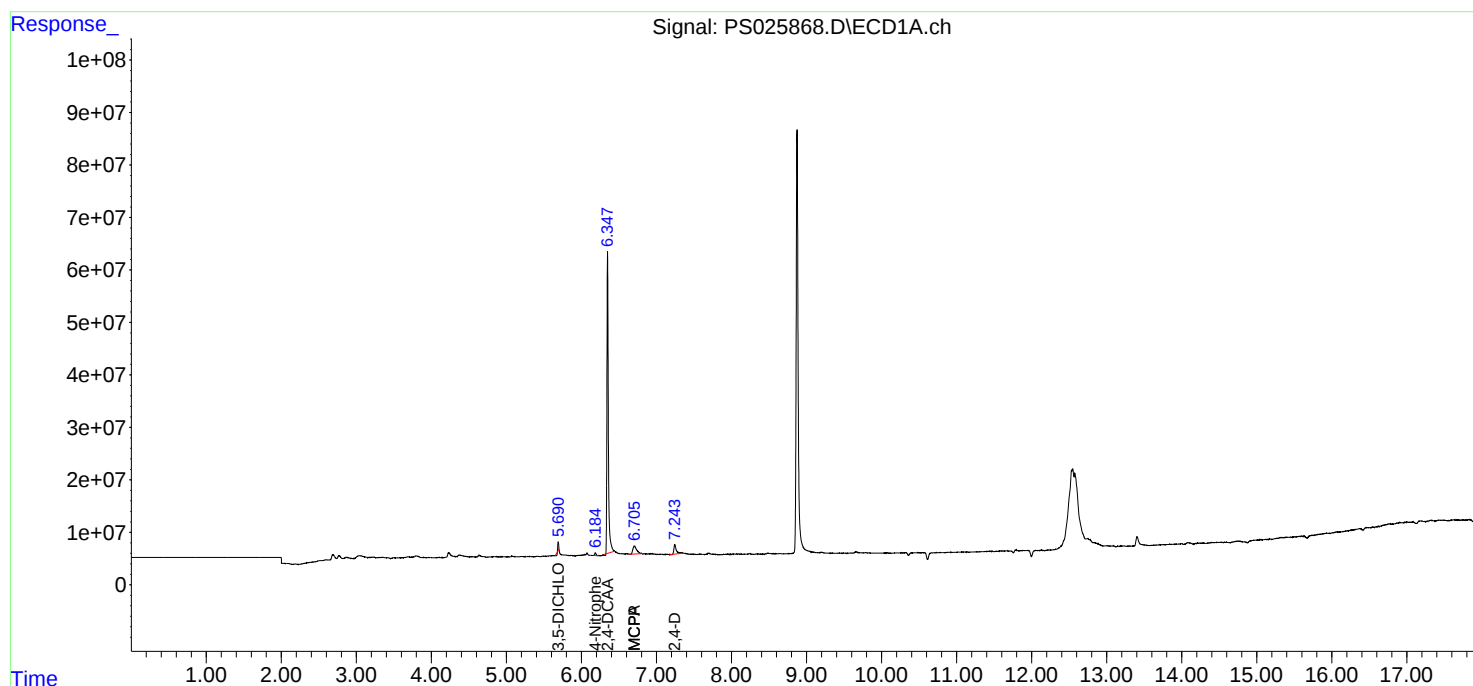


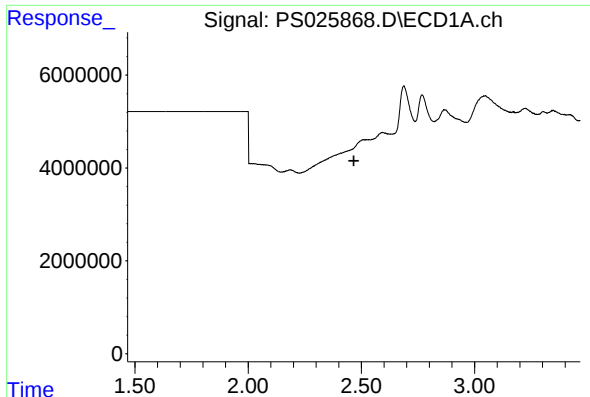

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

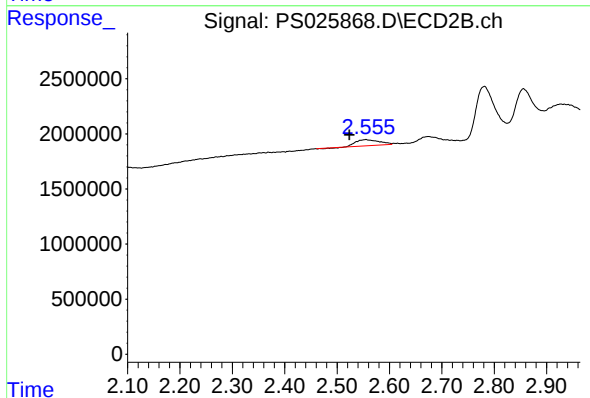


#1 Dalapon

R.T.: 2.555 min
Delta R.T.: 0.032 min
Response: 1646898
Conc: 1.48 ng/ml

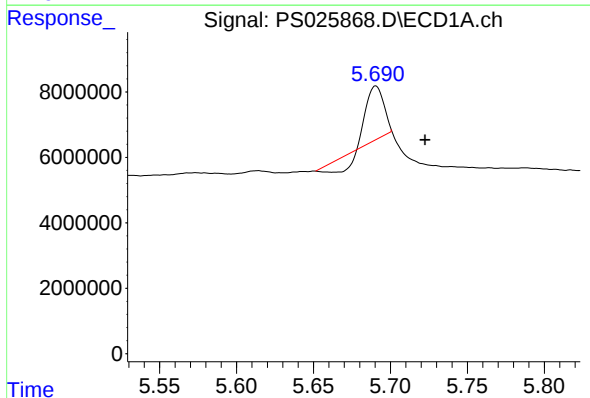


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.691 min
Delta R.T.: -0.032 min
Response: 9882234
Conc: 4.59 ng/ml

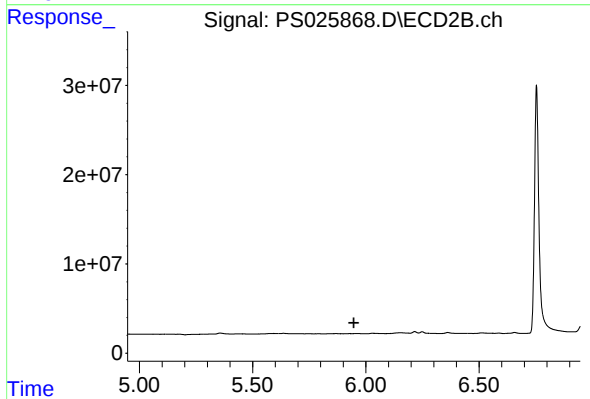

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.947 min
Response: 0
Conc: N.D.

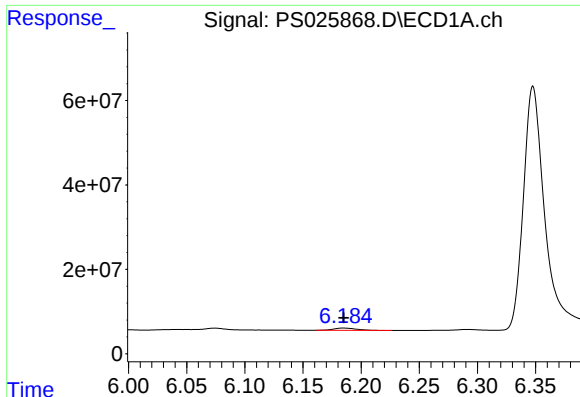

#3 4-Nitrophenol


R.T.: 6.185 min
Delta R.T.: 0.000 min
Response: 6929386
Conc: 7.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

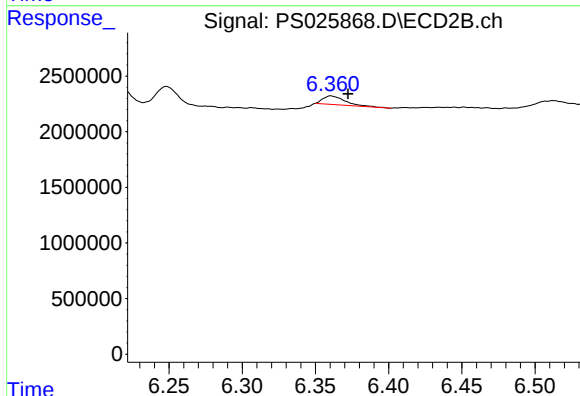


#3 4-Nitrophenol

R.T.: 6.361 min
Delta R.T.: -0.011 min
Response: 822059
Conc: 1.80 ng/ml

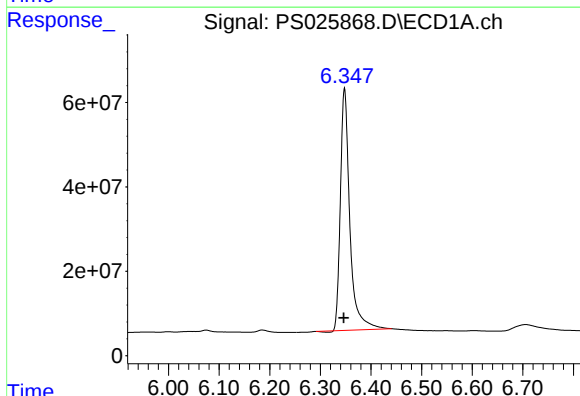


#4 2,4-DCAA

R.T.: 6.348 min
Delta R.T.: 0.002 min
Response: 743864808
Conc: 527.10 ng/ml

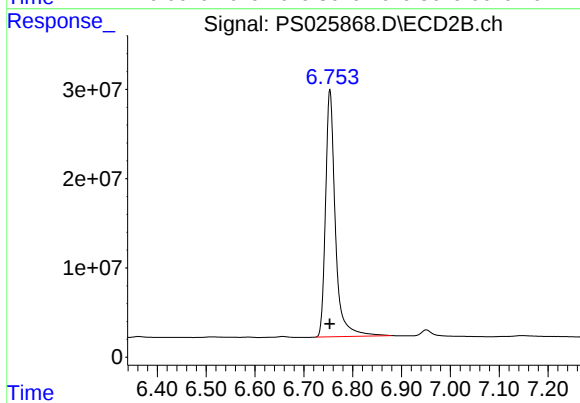

#4 2,4-DCAA


R.T.: 6.753 min
Delta R.T.: 0.000 min
Response: 385887461
Conc: 548.57 ng/ml

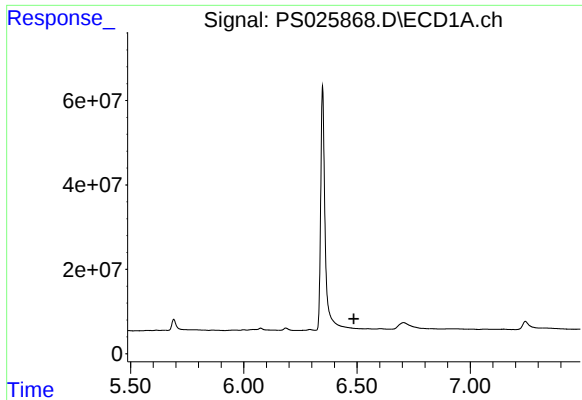

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

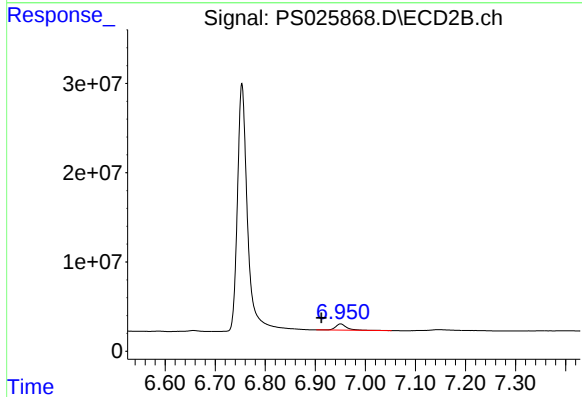


#5 DICAMBA

R.T.: 6.950 min
Delta R.T.: 0.038 min
Response: 11034014
Conc: 3.64 ng/ml

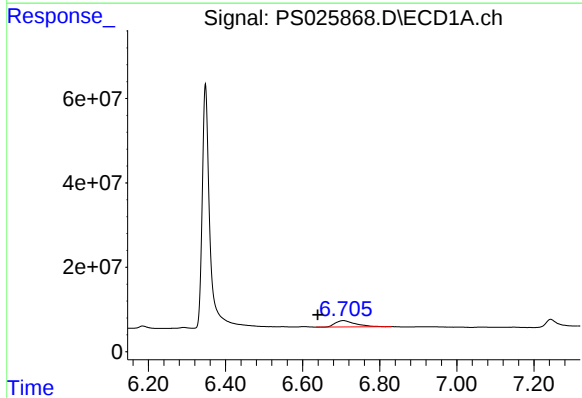


#6 MCP

R.T.: 6.706 min
Delta R.T.: 0.066 min
Response: 54583413
Conc: 15.00 ug/ml

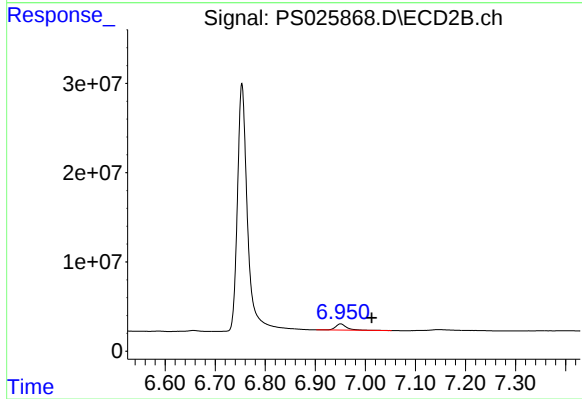

#6 MCP


R.T.: 6.950 min
Delta R.T.: -0.062 min
Response: 11034014
Conc: 5.39 ug/ml

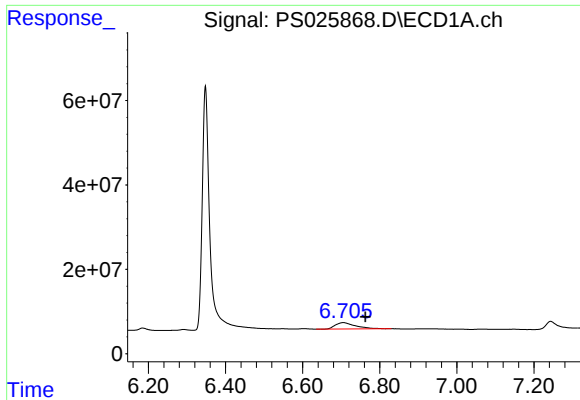

#7 MCPA


R.T.: 6.706 min
Delta R.T.: -0.057 min
Response: 54583413
Conc: 10.14 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

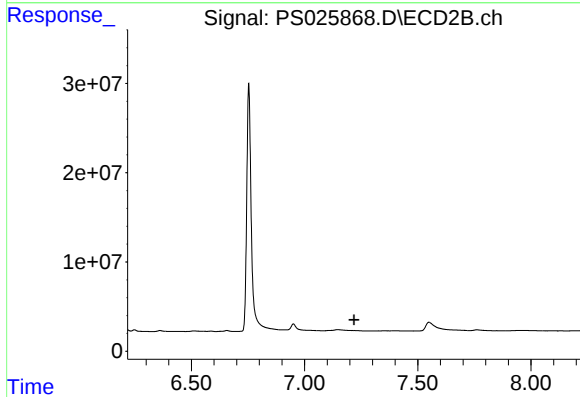


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.218 min
Response: 0
Conc: N.D.

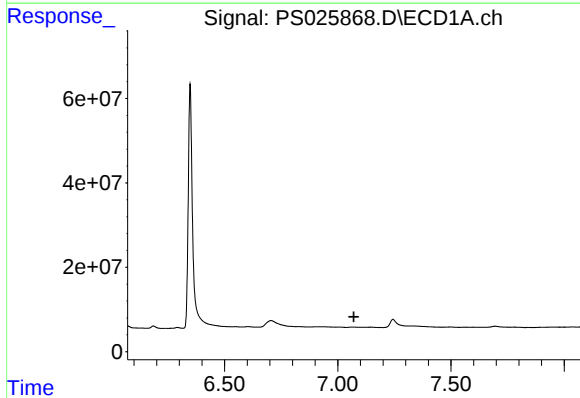


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.071 min
Response: 0
Conc: N.D.

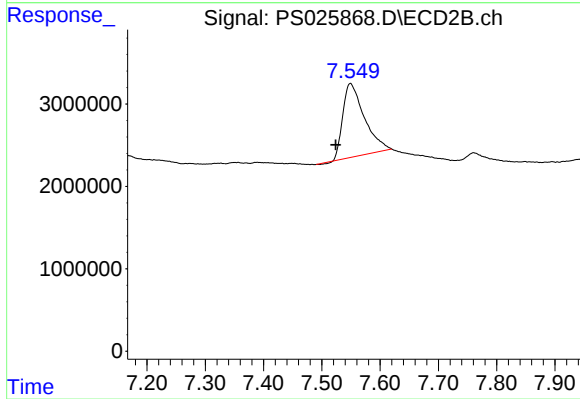

#8 DICHLORPROP


R.T.: 7.549 min
Delta R.T.: 0.025 min
Response: 22870576
Conc: 28.64 ng/ml

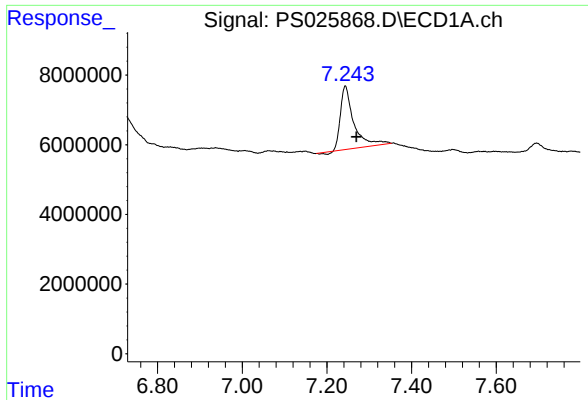

#9 2,4-D

R.T.: 7.244 min
Delta R.T.: -0.026 min
Response: 39552073
Conc: 22.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

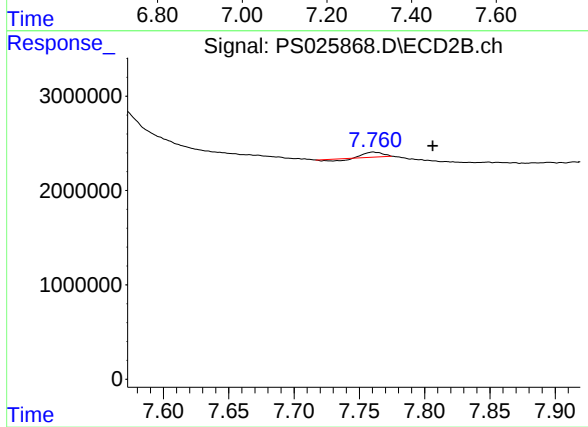

#9 2,4-D

R.T.: 7.761 min
Delta R.T.: -0.046 min
Response: 352969
Conc: N.D.