

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020824\
 Data File : PS025880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2024 20:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 04:32:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.347	6.754	777.3E6	396.6E6	550.779	563.754
Target Compounds							
1) T	Dalapon	0.000	2.554	0	2297482	N.D.	2.071
2) T	3,5-DICHL...	5.690	0.000	12137814	0	5.632	N.D. #
5) T	DICAMBA	0.000	6.951	0	16603449	N.D.	5.471
6) T	MCP	0.000	6.951f	0	16603449	N.D.	8.116
7) T	MCPA	6.710f	7.221	17337119	76355	3.220	<MDL #
8) T	DICHLORPROP	0.000	7.558	0	7197837	N.D.	9.014
9) T	2,4-D	7.242	7.763f	66182004	158934	37.239	<MDL #
16) T	DCPA	0.000	10.645f	0	44000	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020824\
Data File : PS025880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2024 20:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 04:32:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

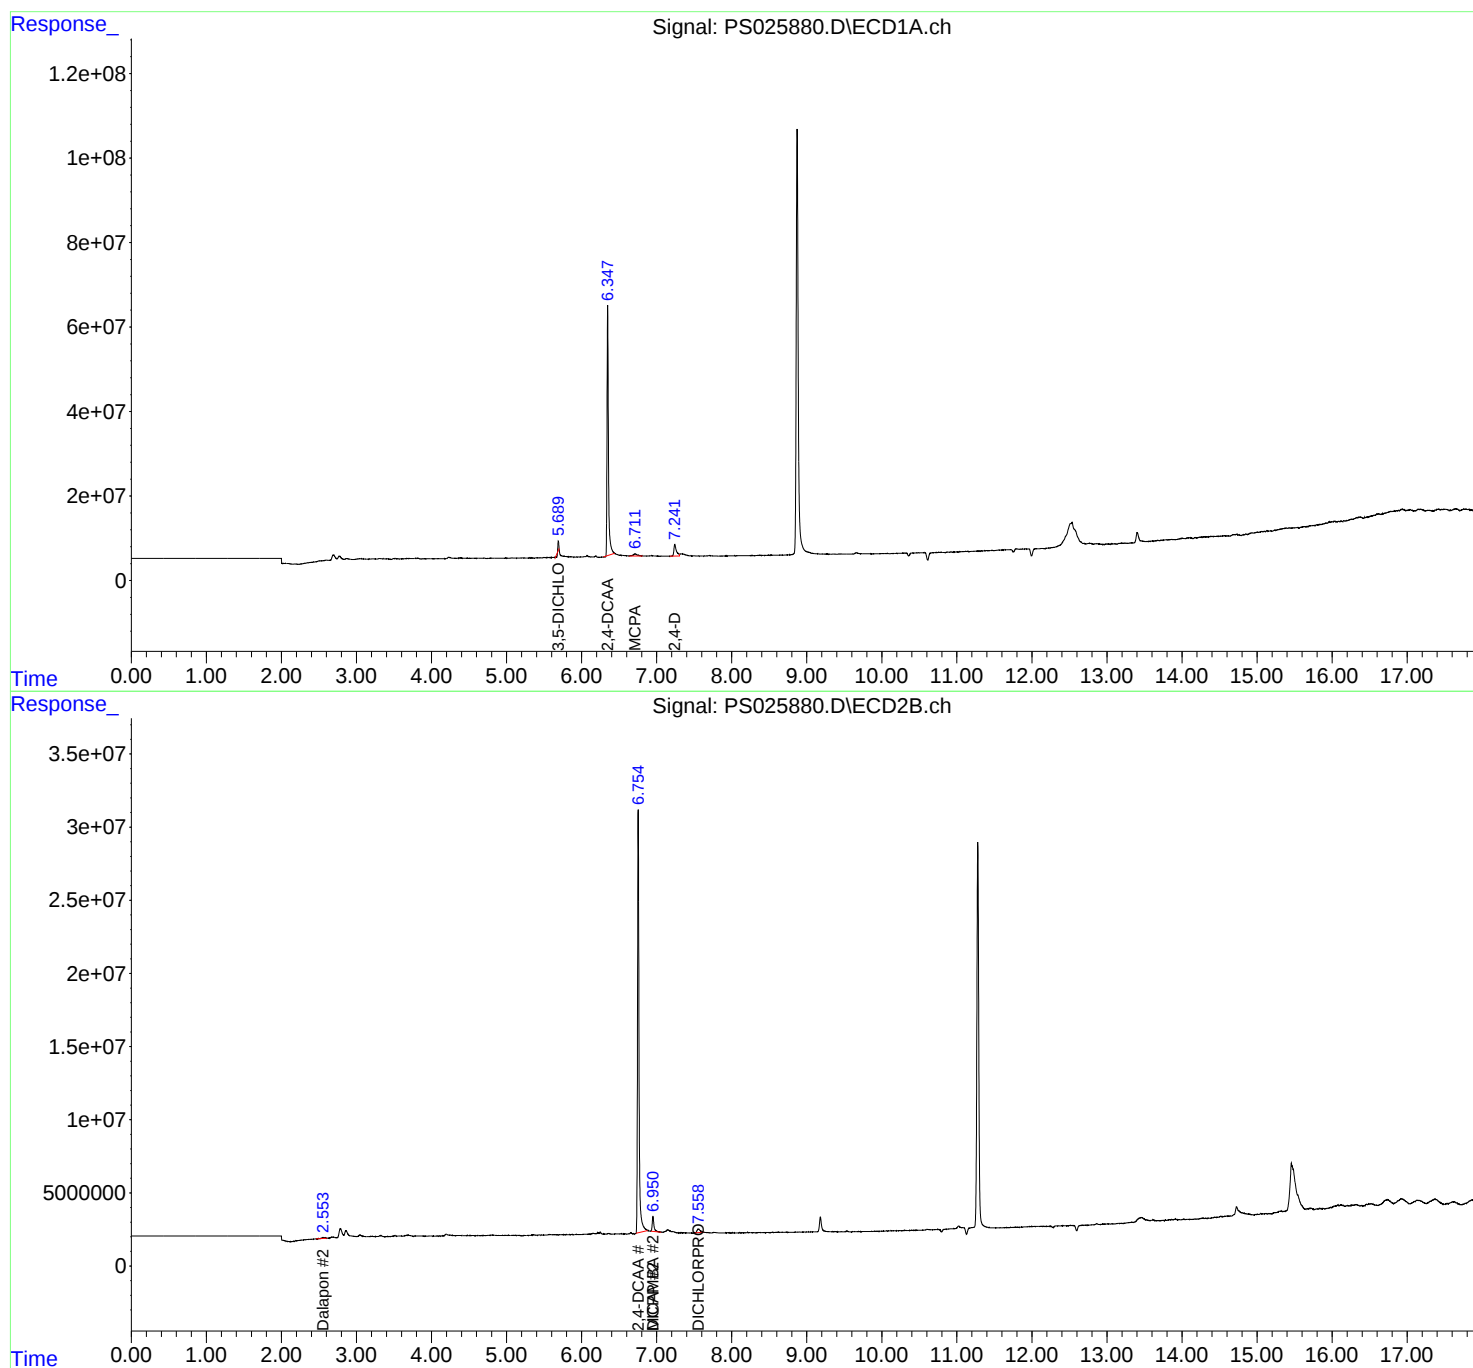


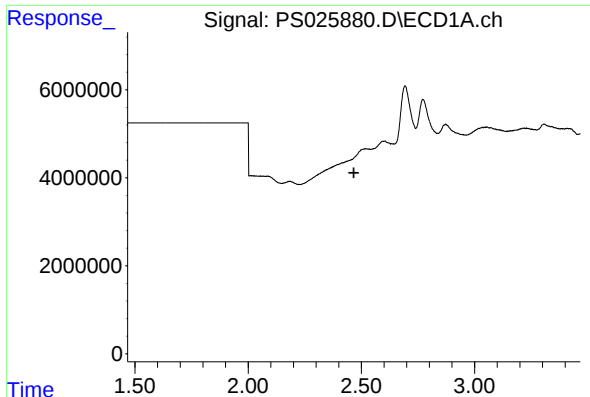

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

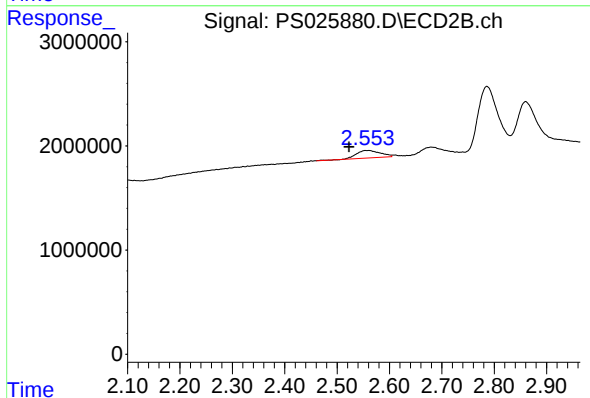


#1 Dalapon

R.T.: 2.554 min
Delta R.T.: 0.030 min
Response: 2297482
Conc: 2.07 ng/ml

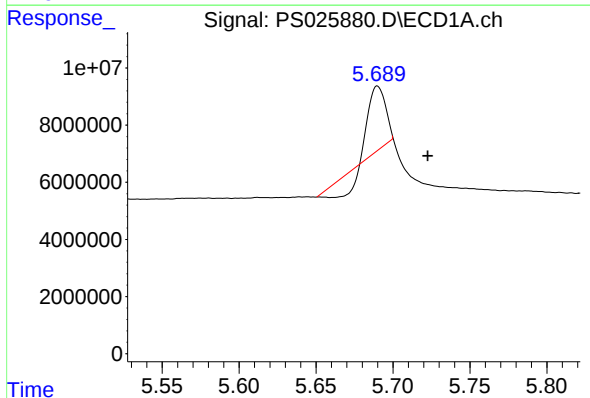


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.690 min
Delta R.T.: -0.032 min
Response: 12137814
Conc: 5.63 ng/ml

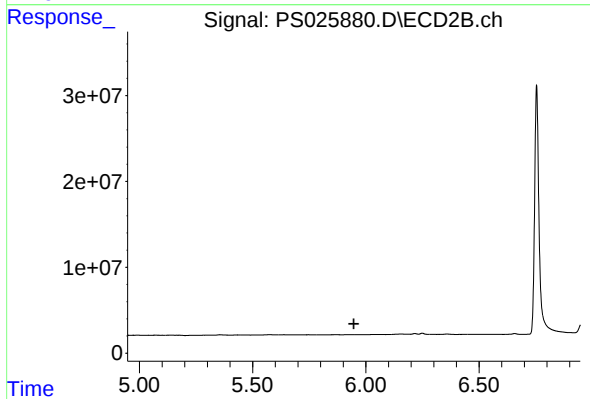

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.947 min
Response: 0
Conc: N.D.

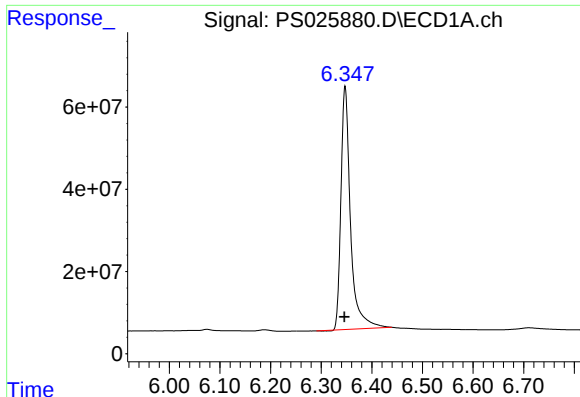

#4 2,4-DCAA


R.T.: 6.347 min
Delta R.T.: 0.001 min
Response: 777288082
Conc: 550.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

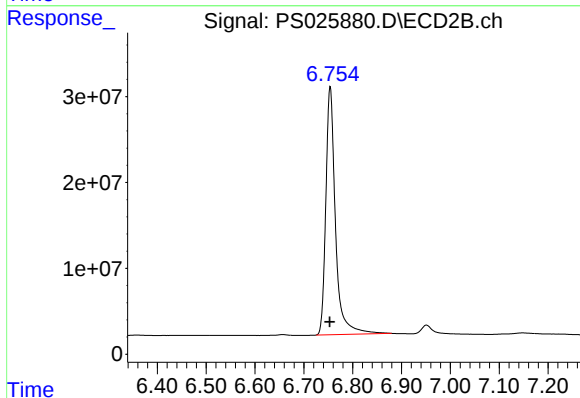


#4 2,4-DCAA

R.T.: 6.754 min
Delta R.T.: 0.000 min
Response: 396569164
Conc: 563.75 ng/ml

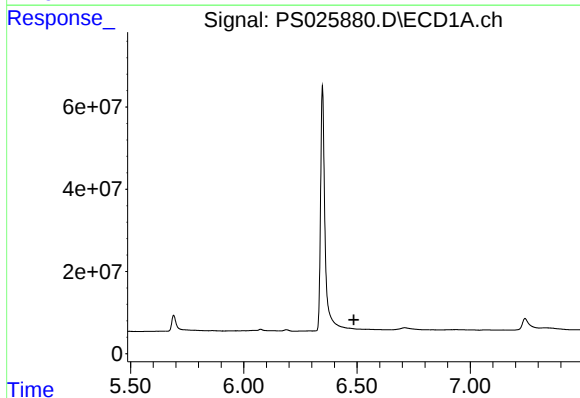


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.486 min
Response: 0
Conc: N.D.

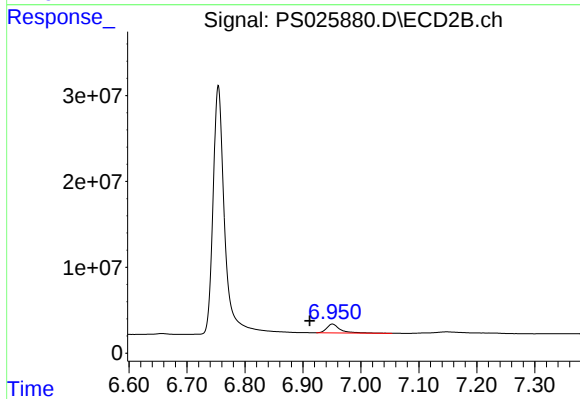

#5 DICAMBA


R.T.: 6.951 min
Delta R.T.: 0.039 min
Response: 16603449
Conc: 5.47 ng/ml

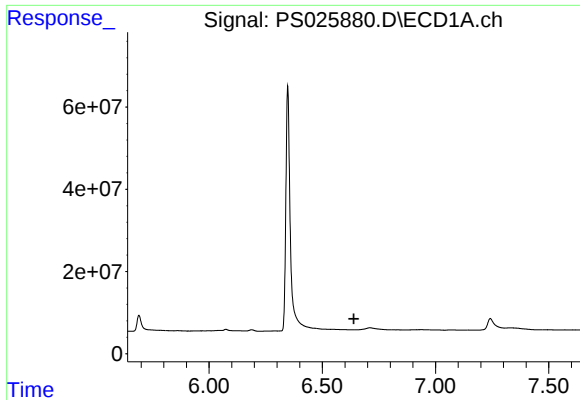

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

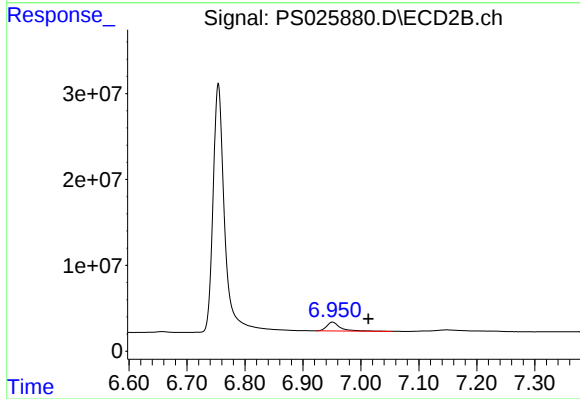


#6 MCP

R.T.: 6.951 min
Delta R.T.: -0.062 min
Response: 16603449
Conc: 8.12 ug/ml

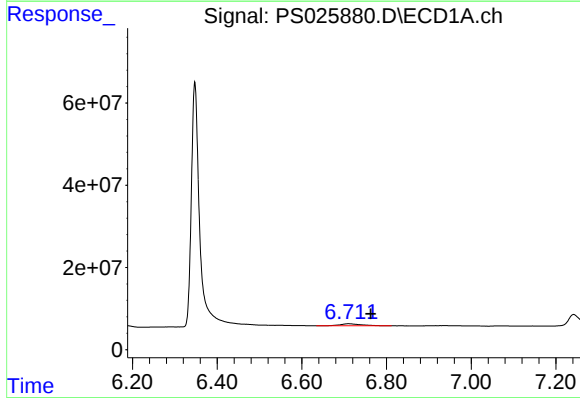


#7 MCP

R.T.: 6.710 min
Delta R.T.: -0.052 min
Response: 17337119
Conc: 3.22 ug/ml

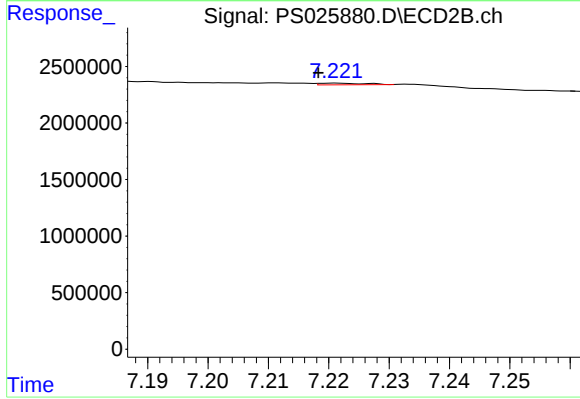

#7 MCP


R.T.: 7.221 min
Delta R.T.: 0.003 min
Response: 76355
Conc: N.D.

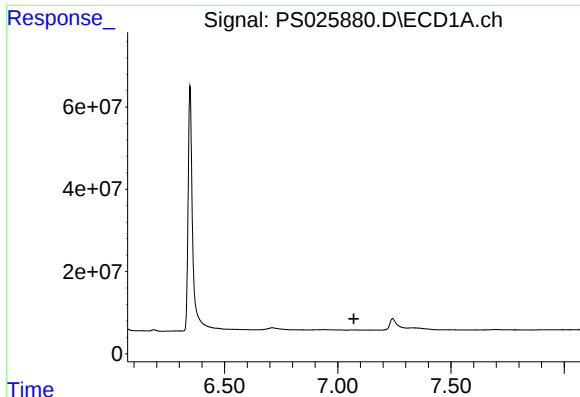

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

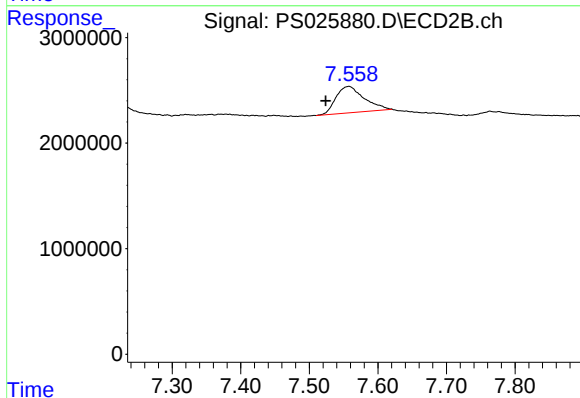


#8 DICHLORPROP

R.T.: 7.558 min
Delta R.T.: 0.034 min
Response: 7197837
Conc: 9.01 ng/ml

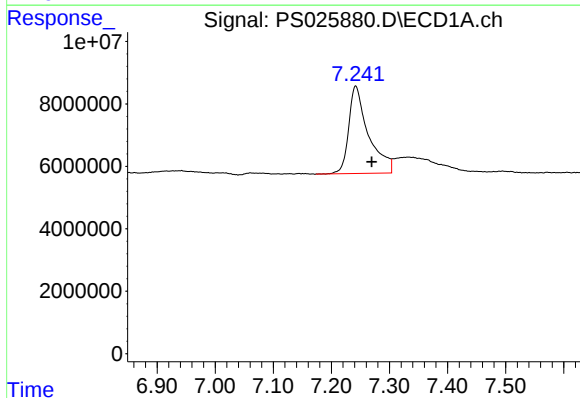

#9 2,4-D

R.T.: 7.242 min
Delta R.T.: -0.027 min
Response: 66182004
Conc: 37.24 ng/ml

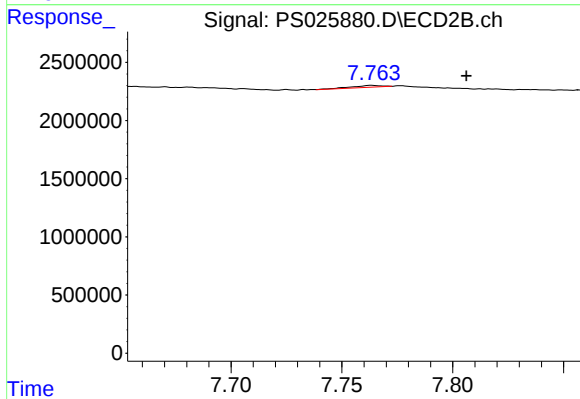

#9 2,4-D

R.T.: 7.763 min
Delta R.T.: -0.043 min
Response: 158934
Conc: N.D.