

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020922\
 Data File : PS018288.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2022 08:40
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 16:13:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 09 15:57:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.038	0.000	4916981	0	3.126	N.D. #
Target Compounds							
5) T	DICAMBA	7.217	6.791	14333637	5563150	2.269	2.051
8) T	DICHLORPROP	7.906	0.000	5196887	0	3.294	N.D. #
9) T	2,4-D	8.148	0.000	16377897	0	8.895	N.D. #
10) T	Pentachlo...	8.425	8.099	26833416	11004745	1.270	1.275
11) T	2,4,5-TP ...	8.978	8.463	20930157	8837983	2.450	2.386
12) T	2,4,5-T	9.269	8.849	46929413	14819842	5.303	4.186
13) T	2,4-DB	9.825	0.000	25113506	0	14.269	N.D. #
14) T	DINOSEB	10.947	9.661	26363960	7390235	3.948	2.928 #
15) T	Picloram	10.798	10.655	290.7E6	130.3E6	25.445	25.990
16) T	DCPA	11.216	10.584	25500204	12085118	2.313	2.655



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020922\
Data File : PS018288.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2022 08:40
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 16:13:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
Quant Title : 8080.M
QLast Update : Wed Feb 09 15:57:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

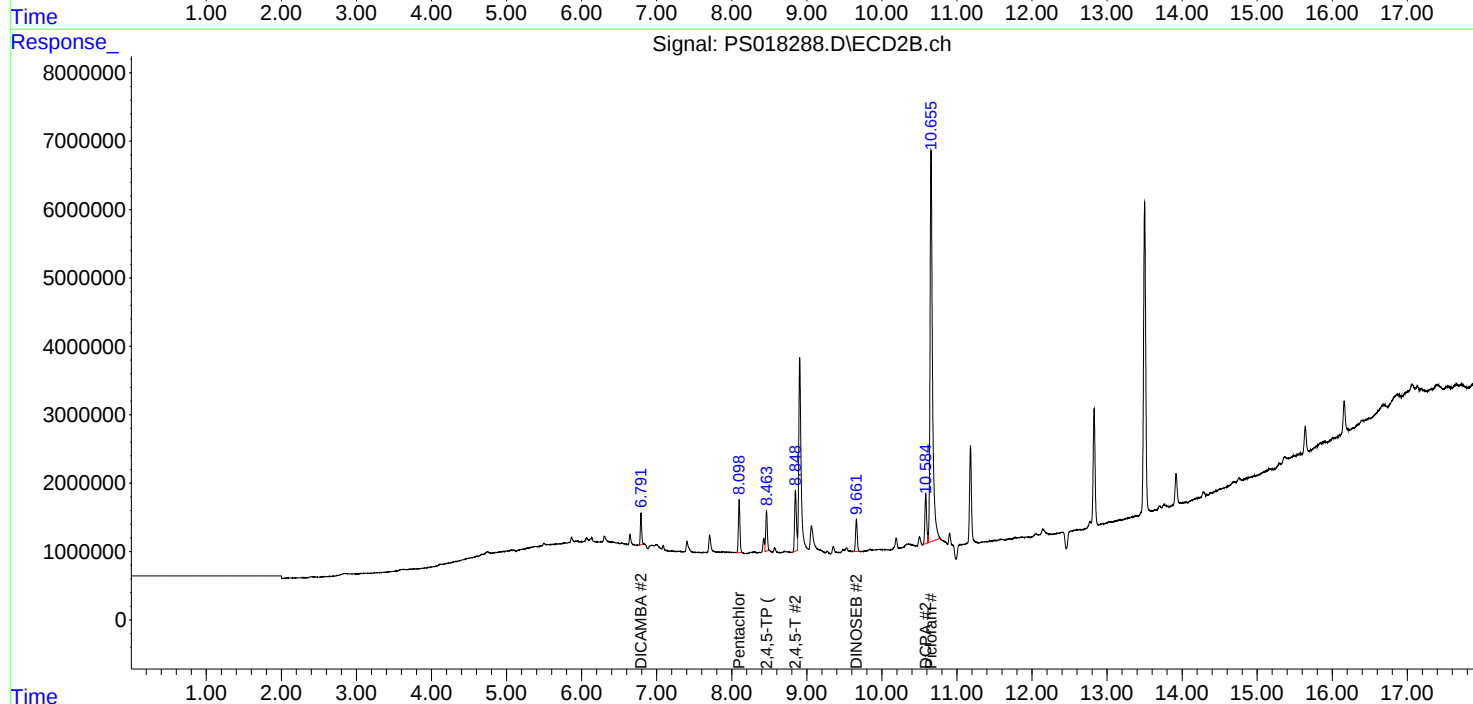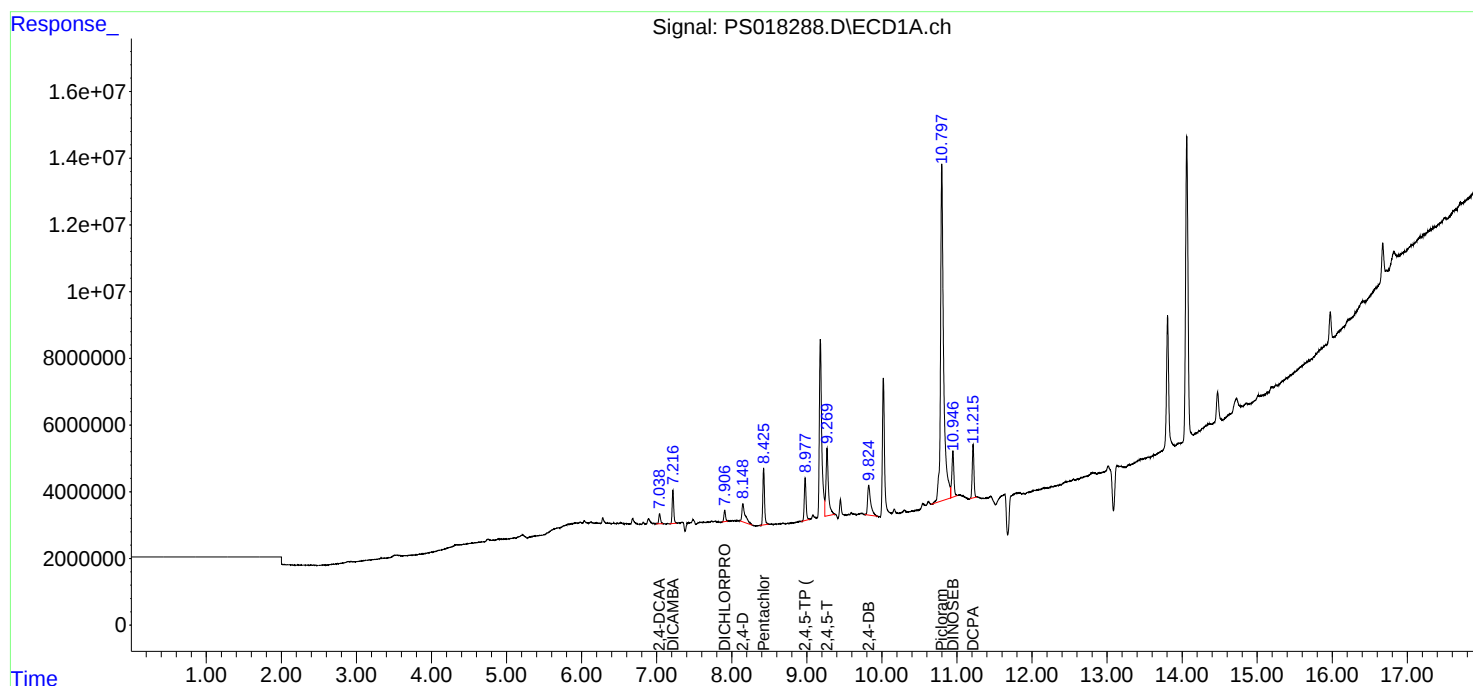


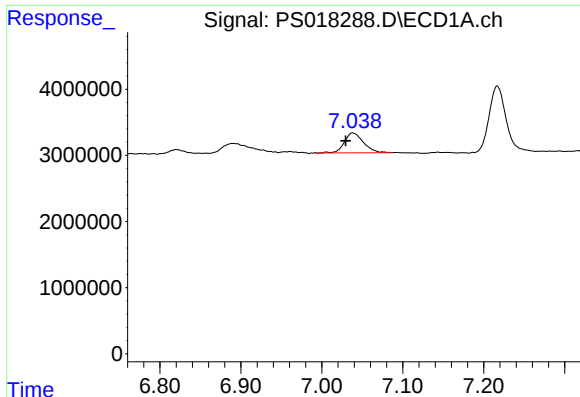

#4 2,4-DCAA


R.T.: 7.038 min
Delta R.T.: 0.009 min
Response: 4916981
Conc: 3.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

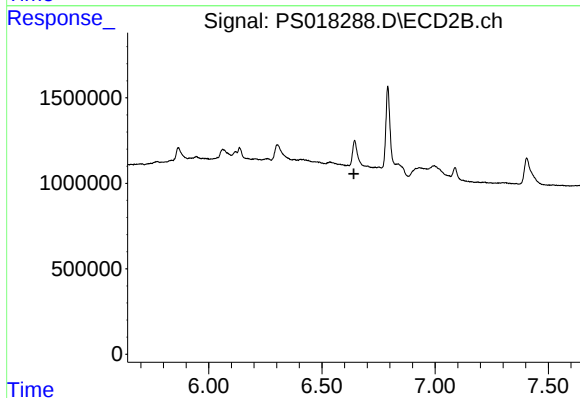


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.641 min
Response: 0
Conc: N.D.

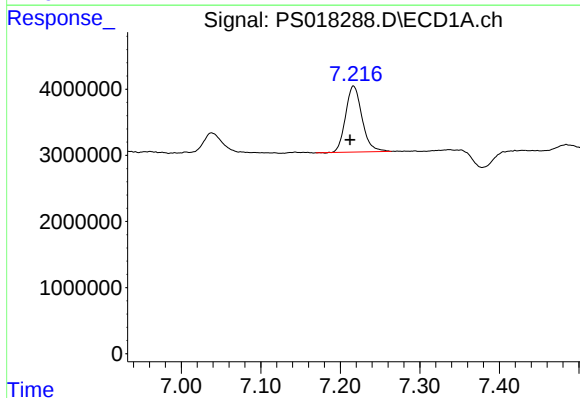


#5 DICAMBA

R.T.: 7.217 min
Delta R.T.: 0.004 min
Response: 14333637
Conc: 2.27 ng/ml

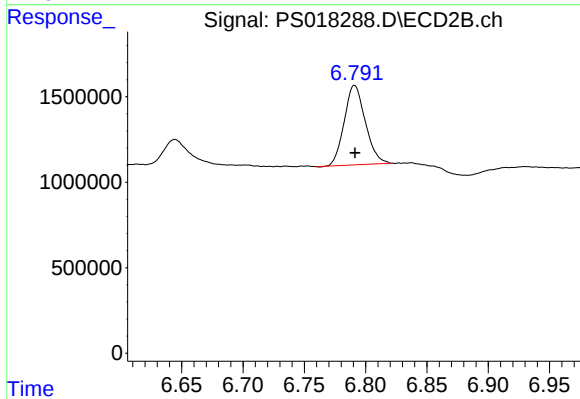

#5 DICAMBA


R.T.: 6.791 min
Delta R.T.: 0.000 min
Response: 5563150
Conc: 2.05 ng/ml

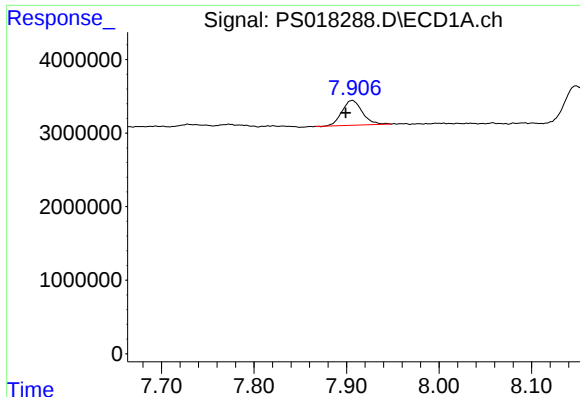

#8 DICHLORPROP


R.T.: 7.906 min
Delta R.T.: 0.007 min
Response: 5196887
Conc: 3.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

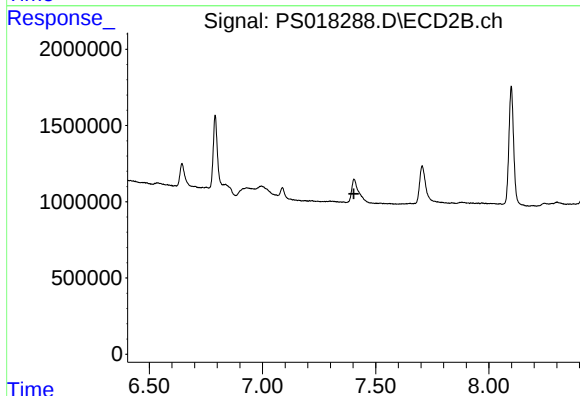


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.404 min
Response: 0
Conc: N.D.

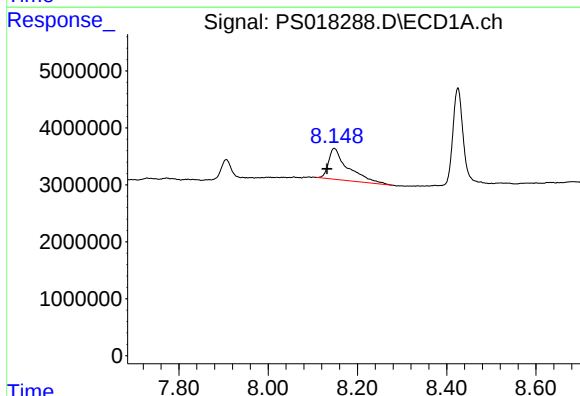


#9 2,4-D

R.T.: 8.148 min
Delta R.T.: 0.016 min
Response: 16377897
Conc: 8.89 ng/ml

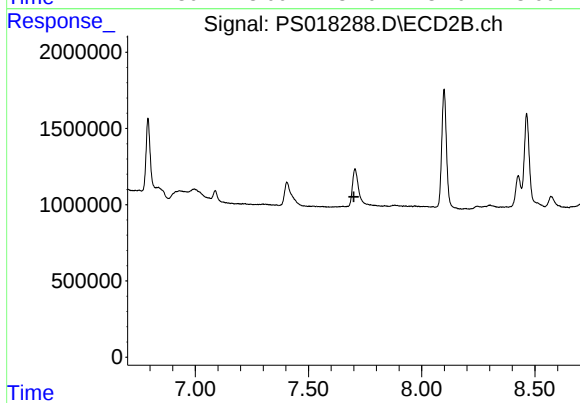

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.

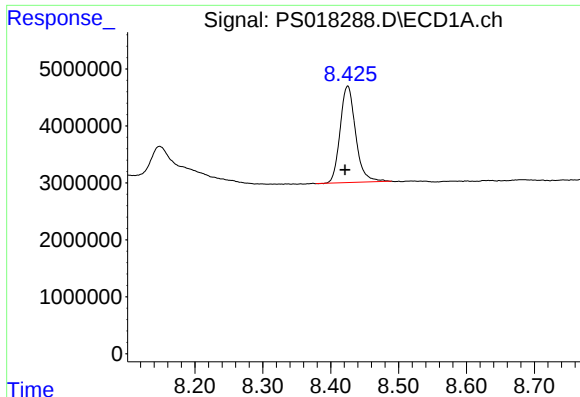

#10 Pentachlorophenol


R.T.: 8.425 min
Delta R.T.: 0.004 min
Response: 26833416
Conc: 1.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

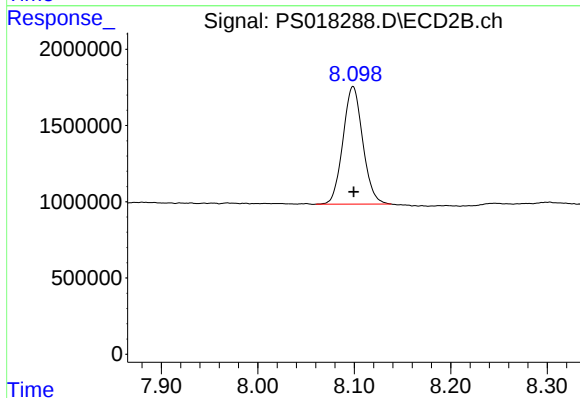


#10 Pentachlorophenol

R.T.: 8.099 min
Delta R.T.: 0.000 min
Response: 11004745
Conc: 1.27 ng/ml

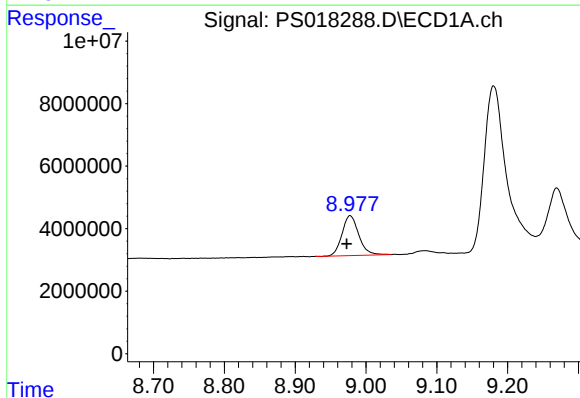


#11 2,4,5-TP (SILVEX)

R.T.: 8.978 min
Delta R.T.: 0.005 min
Response: 20930157
Conc: 2.45 ng/ml

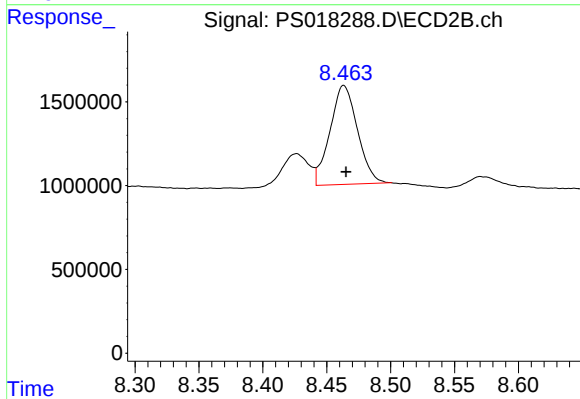

#11 2,4,5-TP (SILVEX)


R.T.: 8.463 min
Delta R.T.: -0.002 min
Response: 8837983
Conc: 2.39 ng/ml

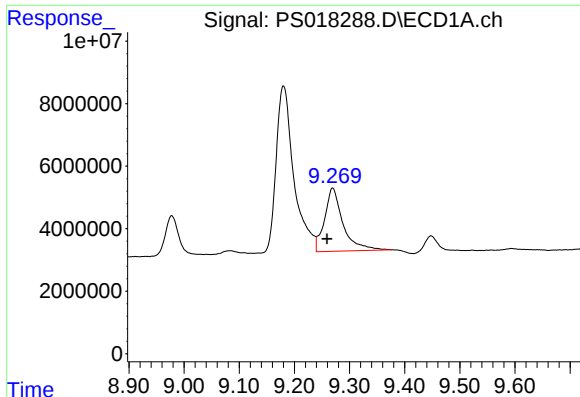

#12 2,4,5-T


R.T.: 9.269 min
Delta R.T.: 0.010 min
Response: 46929413
Conc: 5.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

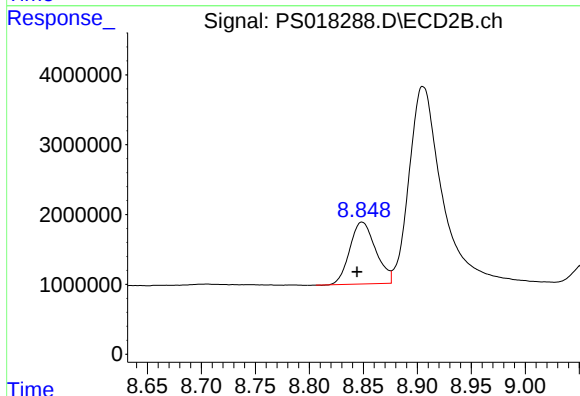


#12 2,4,5-T

R.T.: 8.849 min
Delta R.T.: 0.005 min
Response: 14819842
Conc: 4.19 ng/ml

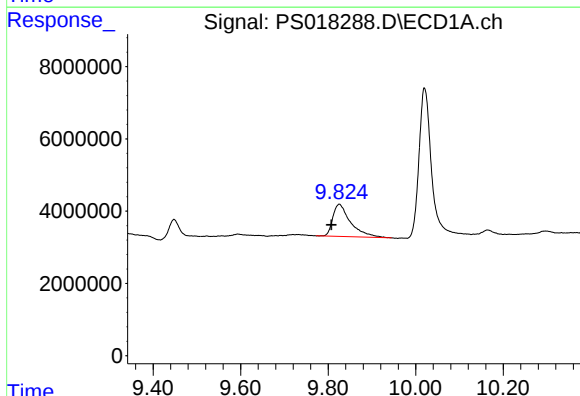


#13 2,4-DB

R.T.: 9.825 min
Delta R.T.: 0.018 min
Response: 25113506
Conc: 14.27 ng/ml

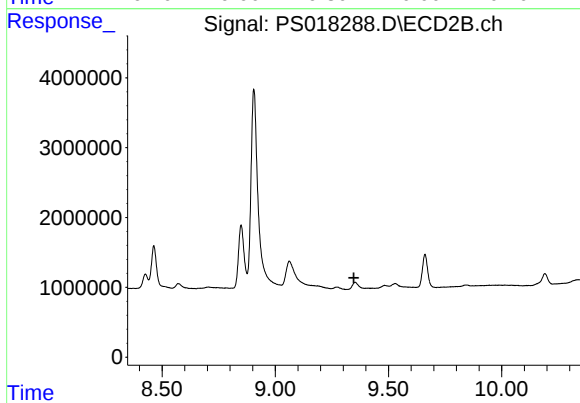

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.347 min
Response: 0
Conc: N.D.

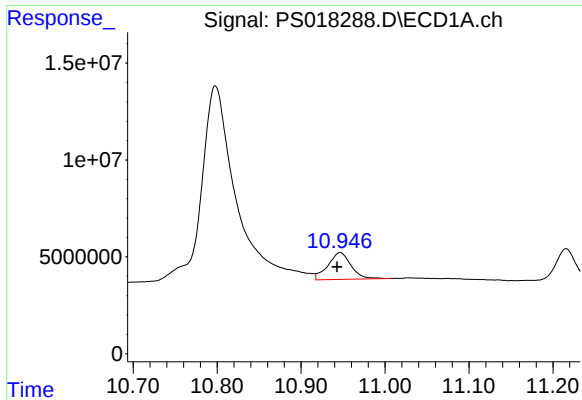

#14 DINOSEB


R.T.: 10.947 min
Delta R.T.: 0.004 min
Response: 26363960
Conc: 3.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

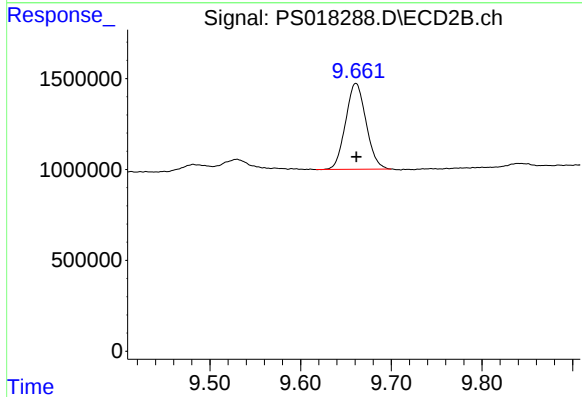


#14 DINOSEB

R.T.: 9.661 min
Delta R.T.: 0.000 min
Response: 7390235
Conc: 2.93 ng/ml

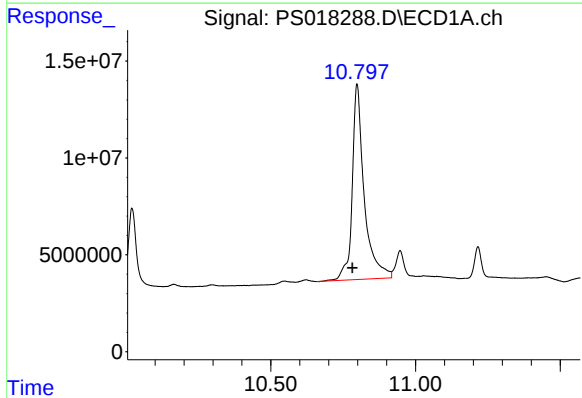


#15 Picloram

R.T.: 10.798 min
Delta R.T.: 0.016 min
Response: 290700840
Conc: 25.44 ng/ml

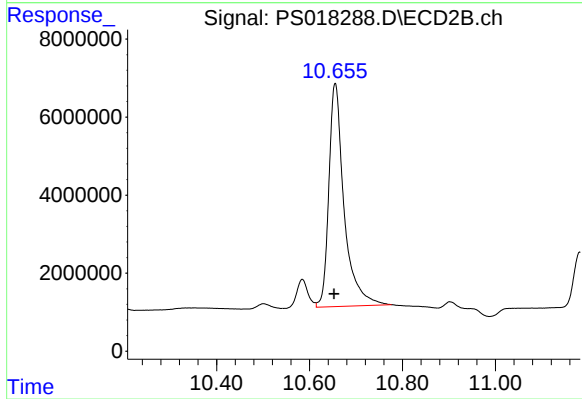

#15 Picloram


R.T.: 10.655 min
Delta R.T.: 0.003 min
Response: 130258418
Conc: 25.99 ng/ml

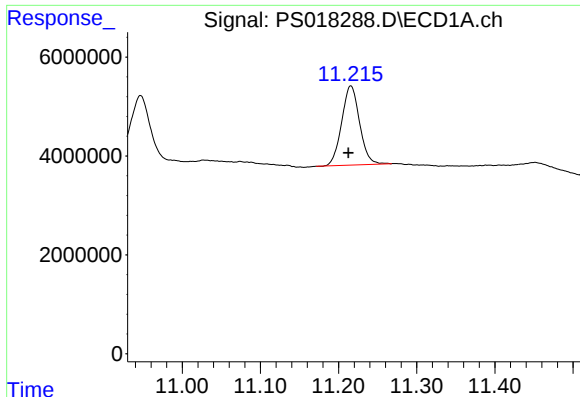

#16 DCPA

R.T.: 11.216 min
Delta R.T.: 0.003 min
Response: 25500204
Conc: 2.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

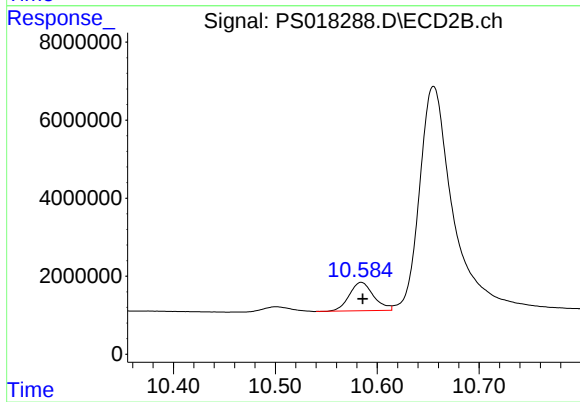

#16 DCPA

R.T.: 10.584 min
Delta R.T.: -0.002 min
Response: 12085118
Conc: 2.66 ng/ml