

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020922\
 Data File : PS018289.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2022 09:05
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 16:13:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 09 15:57:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.030	6.639	620.3E6	309.4E6	394.333	493.287 #
Target Compounds							
9) T	2,4-D	8.192f	0.000	11099723	0	6.028	N.D. #
11) T	2,4,5-TP ...	8.983	0.000	4382047	0	<MDL	N.D. #
12) T	2,4,5-T	9.285	0.000	33720787	0	3.810	N.D. #
13) T	2,4-DB	9.867f	0.000	7994445	0	4.542	N.D. #
14) T	DINOSEB	10.941	0.000	20473013	0	3.066	N.D. #
15) T	Picloram	10.765	10.679	3570563	78534109	<MDL	15.669 #
16) T	DCPA	11.212	0.000	7602481	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020922\
Data File : PS018289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2022 09:05
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 16:13:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
Quant Title : 8080.M
QLast Update : Wed Feb 09 15:57:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

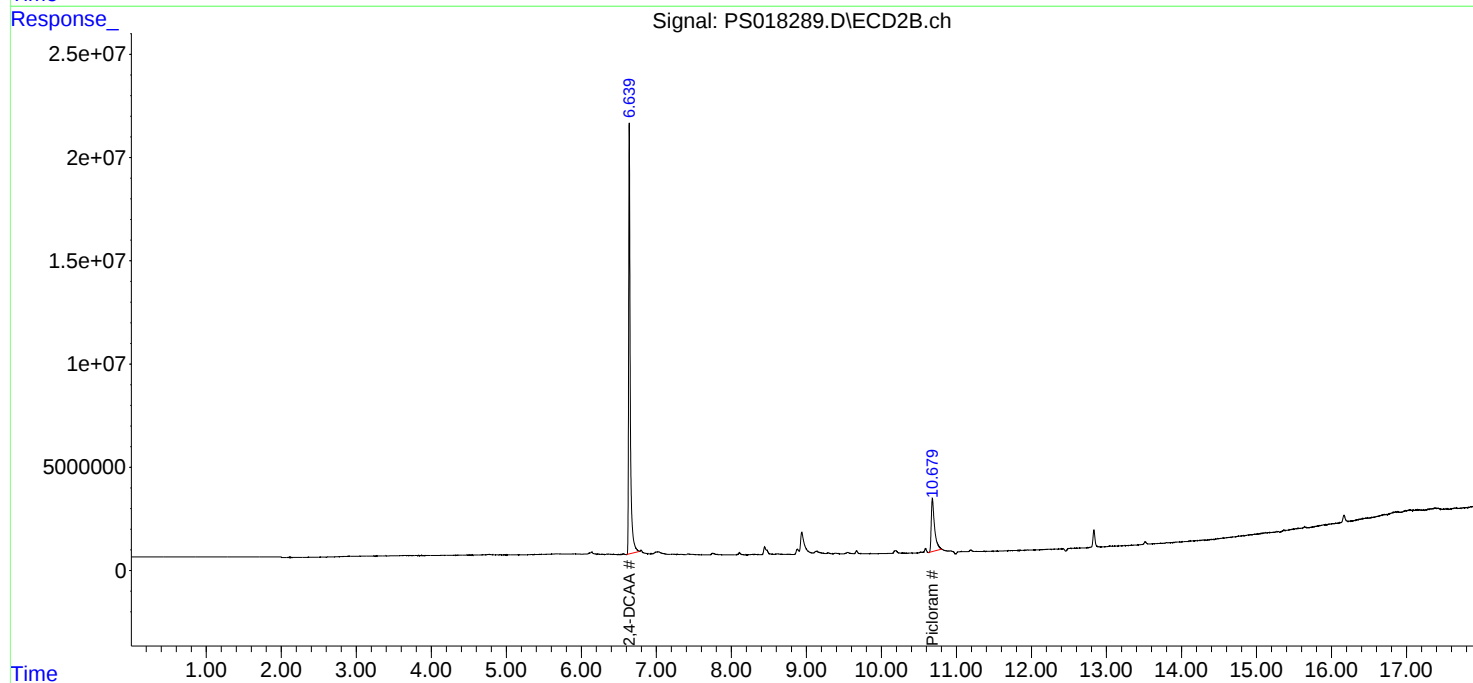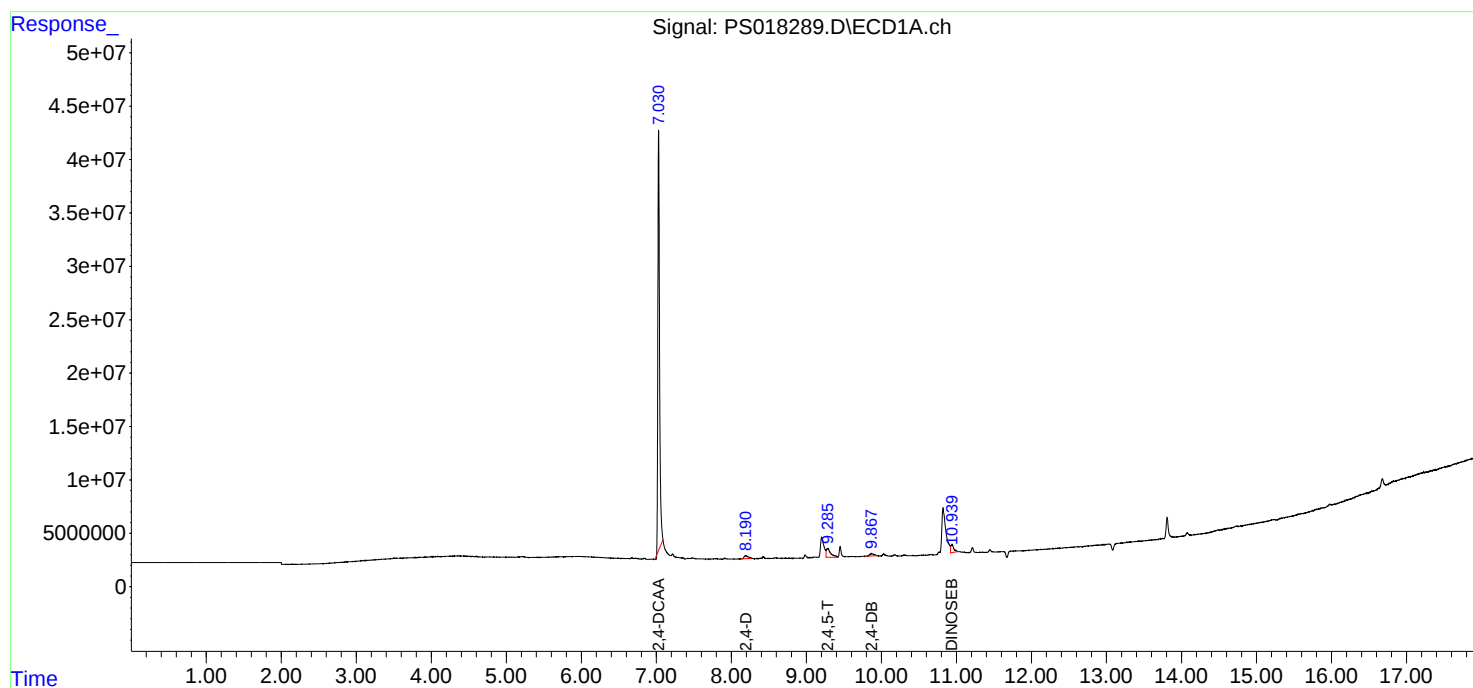


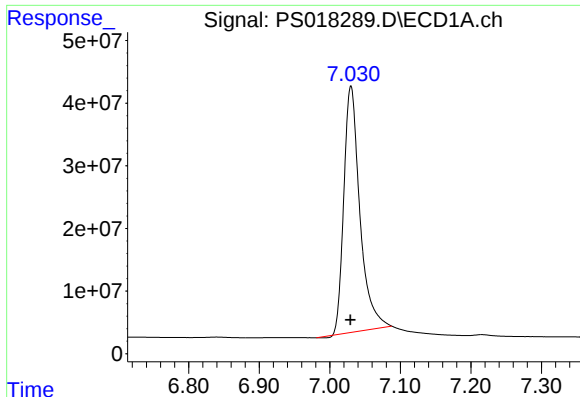

#4 2,4-DCAA


R.T.: 7.030 min
Delta R.T.: 0.000 min
Response: 620315324
Conc: 394.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

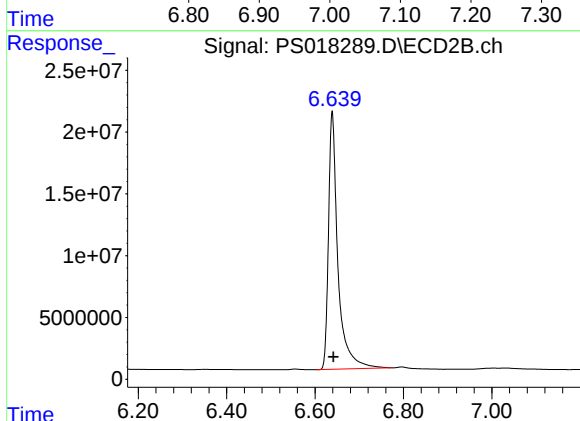


#4 2,4-DCAA

R.T.: 6.639 min
Delta R.T.: -0.002 min
Response: 309404848
Conc: 493.29 ng/ml

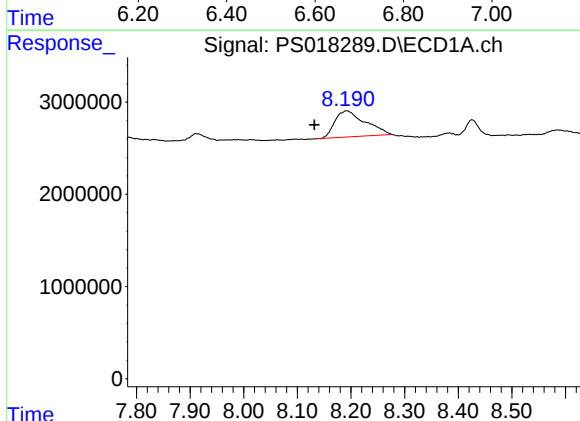


#9 2,4-D

R.T.: 8.192 min
Delta R.T.: 0.060 min
Response: 11099723
Conc: 6.03 ng/ml

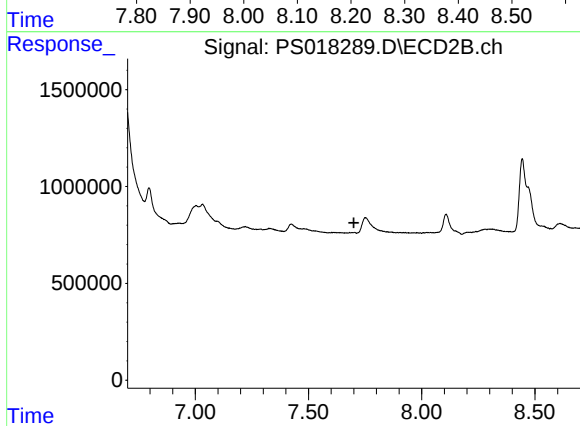

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.

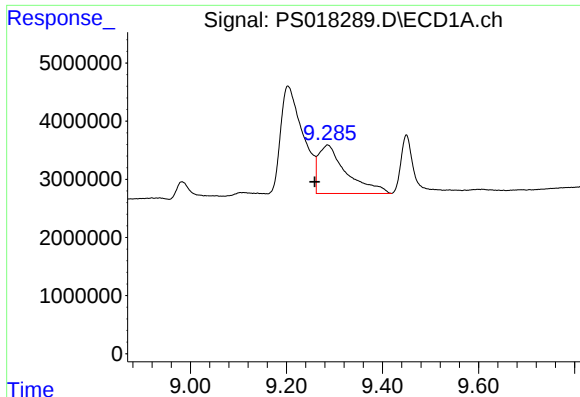

#12 2,4,5-T


R.T.: 9.285 min
Delta R.T.: 0.026 min
Response: 33720787
Conc: 3.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

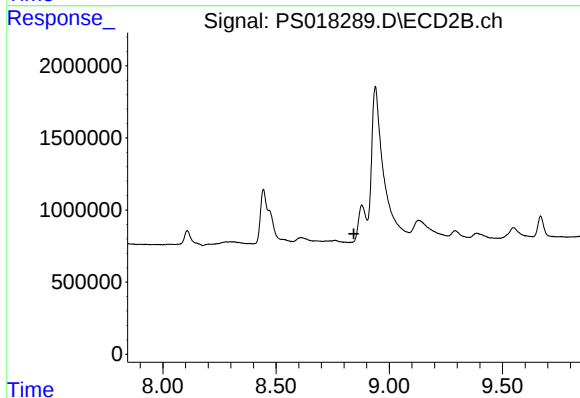


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.844 min
Response: 0
Conc: N.D.

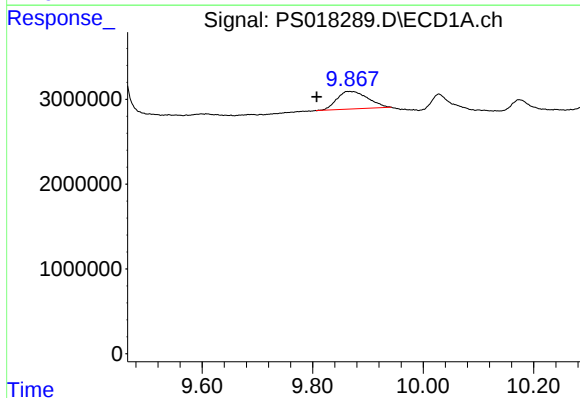


#13 2,4-DB

R.T.: 9.867 min
Delta R.T.: 0.060 min
Response: 7994445
Conc: 4.54 ng/ml

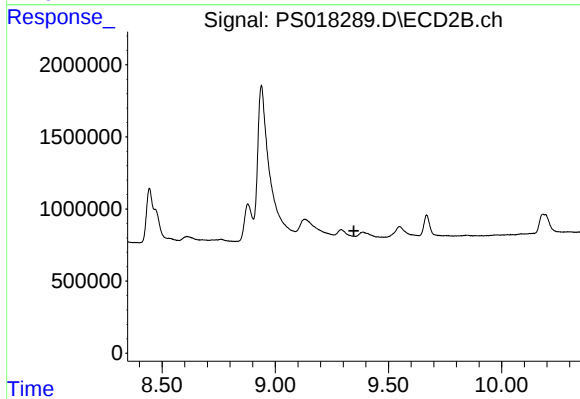

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.347 min
Response: 0
Conc: N.D.

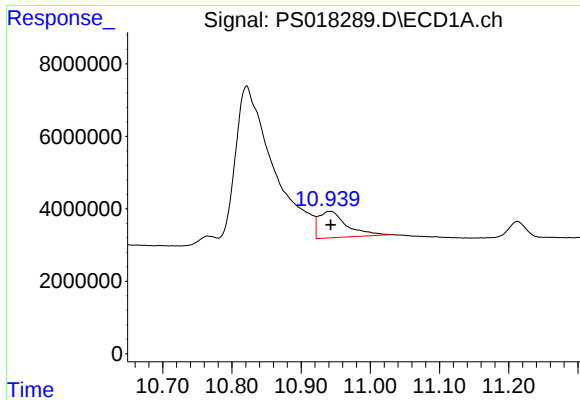

#14 DINOSEB


R.T.: 10.941 min
Delta R.T.: -0.002 min
Response: 20473013
Conc: 3.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

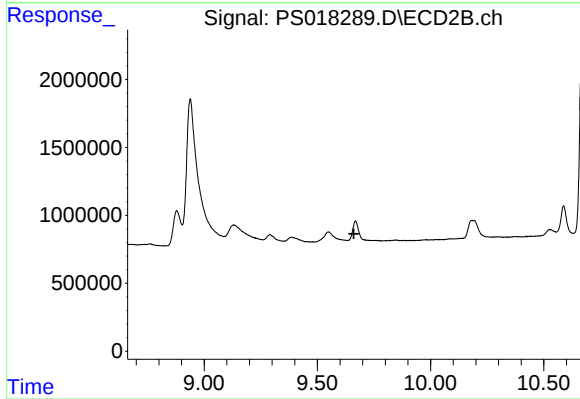


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.661 min
Response: 0
Conc: N.D.

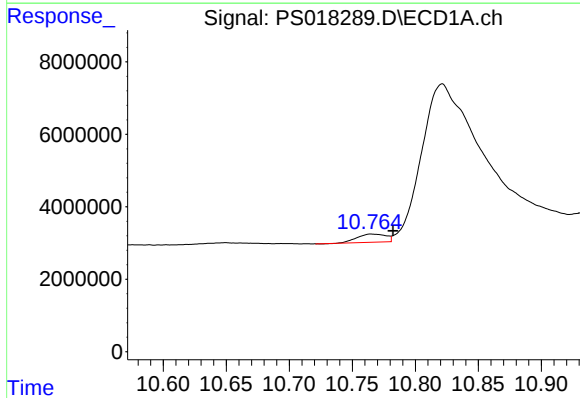

#15 Picloram

R.T.: 10.765 min
Delta R.T.: -0.017 min
Response: 3570563
Conc: N.D.

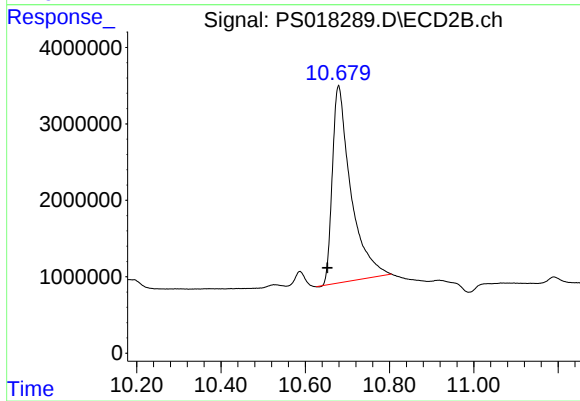

#15 Picloram

R.T.: 10.679 min
Delta R.T.: 0.026 min
Response: 78534109
Conc: 15.67 ng/ml