

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020823\
 Data File : PS022082.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2023 08:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 15:04:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020223.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 03 10:03:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.303	6.727	1189.6E6	1112.1E6	521.879	549.394
Target Compounds							
1) T	Dalapon	2.443	0.000	1021658	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.670	0.000	2068834	0	<MDL	N.D. #
3) T	4-Nitroph...	6.163	0.000	4374050	0	3.250	N.D. #
5) T	DICAMBA	0.000	6.888	0	14346062	N.D.	1.518
6) T	MCP	0.000	6.940f	0	10789596	N.D.	1.446
7) T	MCPA	0.000	7.131f	0	27722894	N.D.	2.760
8) T	DICHLORPROP	7.050	7.569f	1762164	7340270	<MDL	3.068 #
9) T	2,4-D	7.216	0.000	10474483	0	3.484	N.D. #
10) T	Pentachlo...	7.455	8.221	8421187	8008625	<MDL	<MDL #
11) T	2,4,5-TP ...	7.999	8.595	4909328	4934175	<MDL	<MDL #
12) T	2,4,5-T	8.198	9.005f	41661	5340127	<MDL	<MDL #
14) T	DINOSEB	9.787	9.789	7786422	3736543	<MDL	<MDL #
15) T	Picloram	9.650	10.709f	3258383	19826254	<MDL	1.092 #
16) T	DCPA	10.052	10.709	7203240	19826254	<MDL	1.288 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020823\
Data File : PS022082.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2023 08:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 15:04:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020223.M
Quant Title : 8080.M
QLast Update : Fri Feb 03 10:03:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

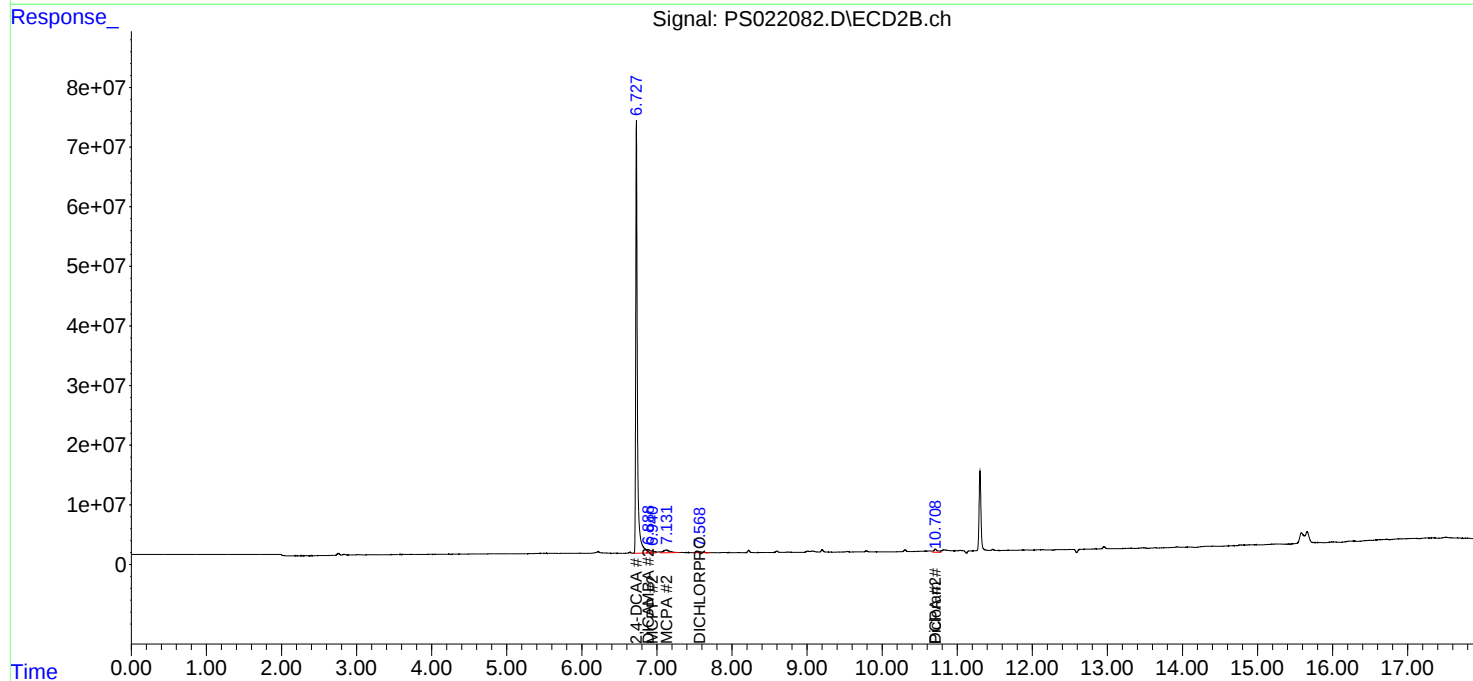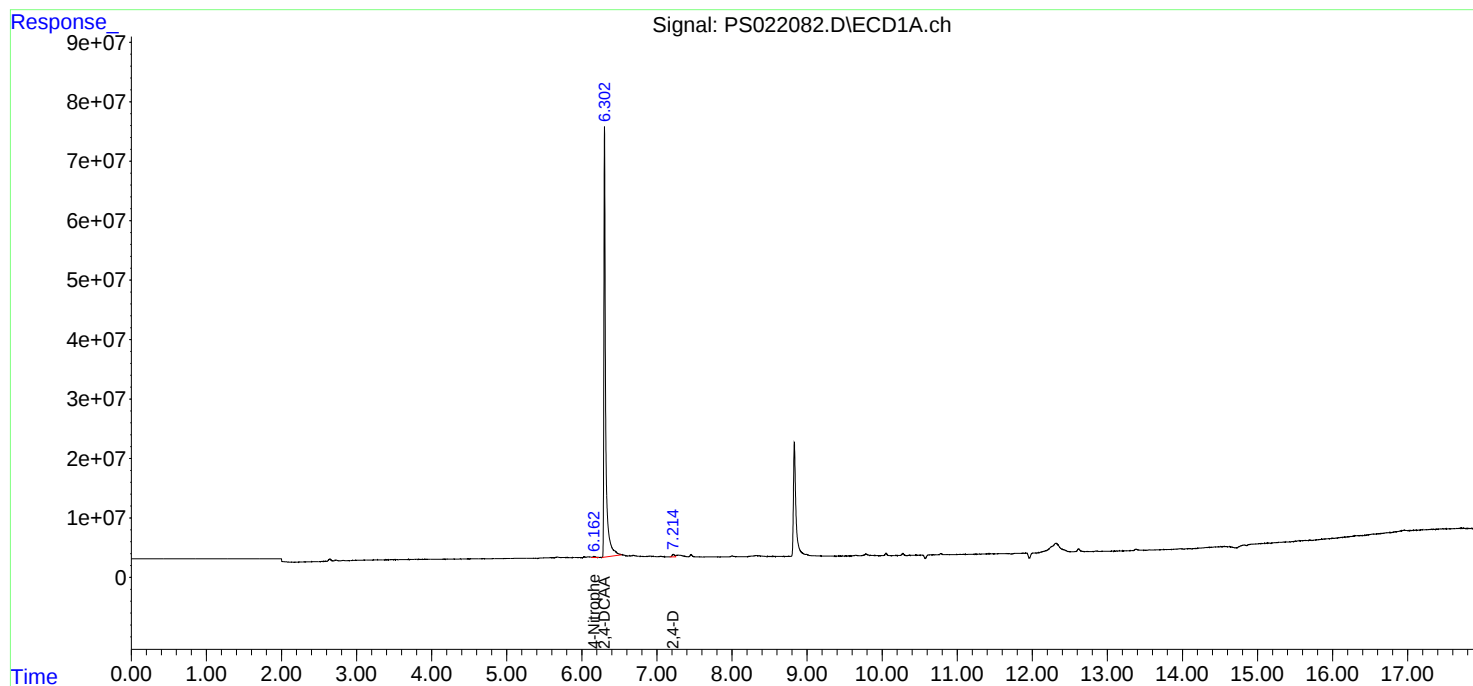


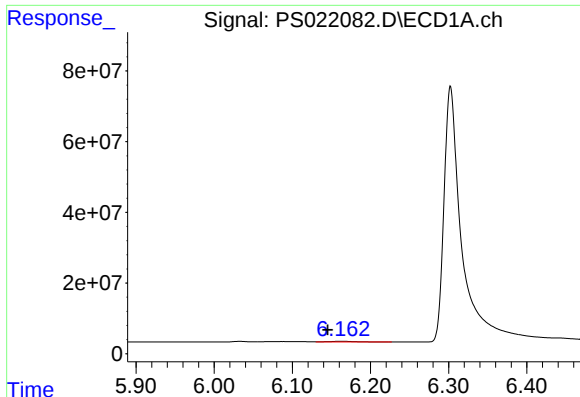

#3 4-Nitrophenol


R.T.: 6.163 min
Delta R.T.: 0.018 min
Response: 4374050
Conc: 3.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

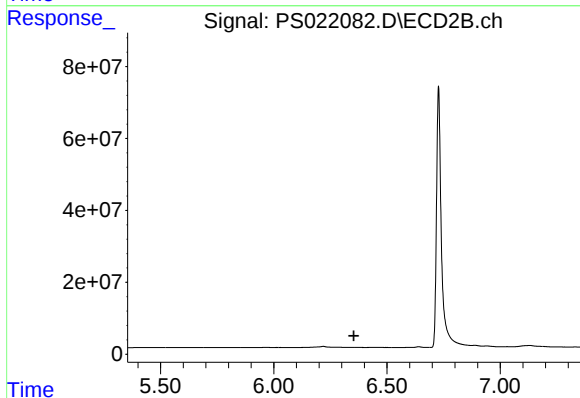


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.354 min
Response: 0
Conc: N.D.

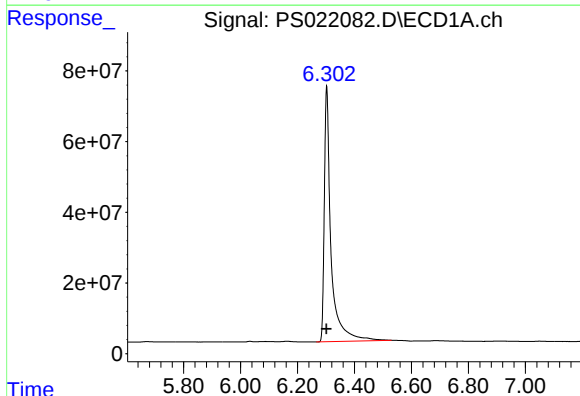


#4 2,4-DCAA

R.T.: 6.303 min
Delta R.T.: 0.000 min
Response: 1189552651
Conc: 521.88 ng/ml

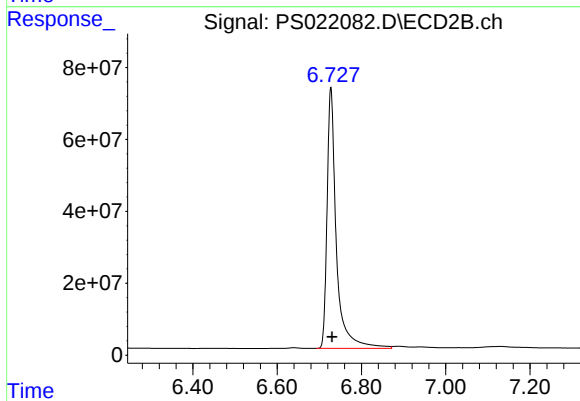

#4 2,4-DCAA


R.T.: 6.727 min
Delta R.T.: -0.003 min
Response: 1112104220
Conc: 549.39 ng/ml

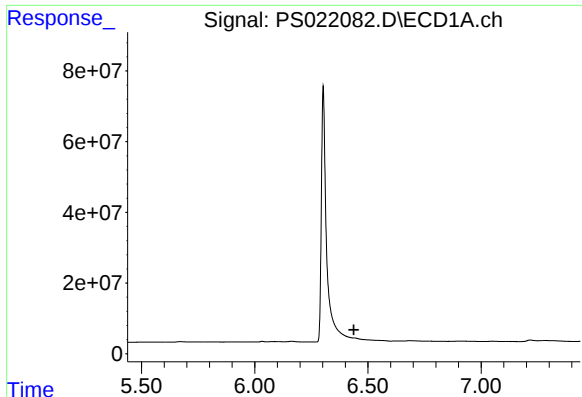

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

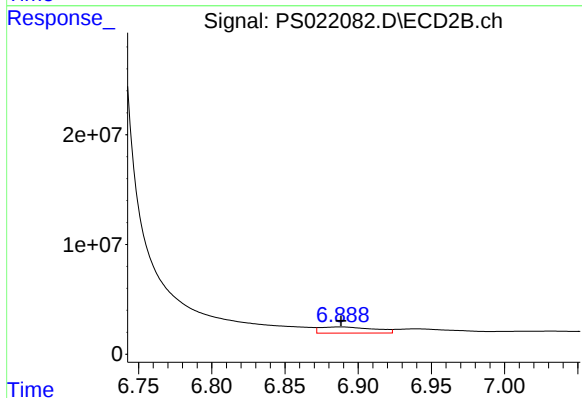


#5 DICAMBA

R.T.: 6.888 min
Delta R.T.: 0.000 min
Response: 14346062
Conc: 1.52 ng/ml

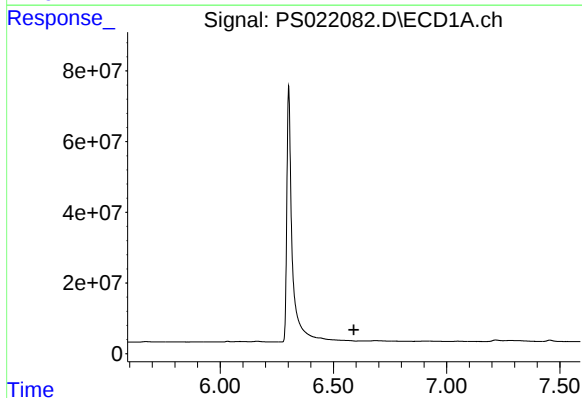


#6 MCP

R.T.: 0.000 min
Exp R.T.: 6.590 min
Response: 0
Conc: N.D.

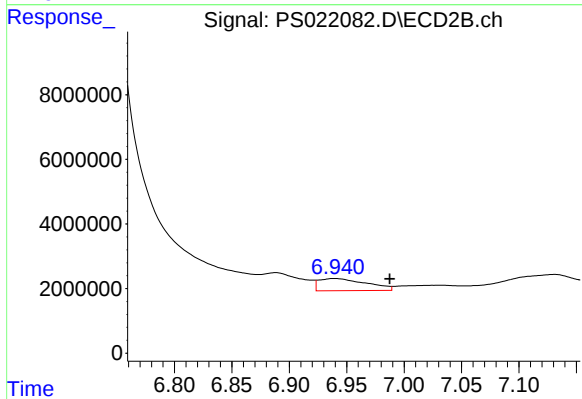

#6 MCP


R.T.: 6.940 min
Delta R.T.: -0.048 min
Response: 10789596
Conc: 1.45 ug/ml

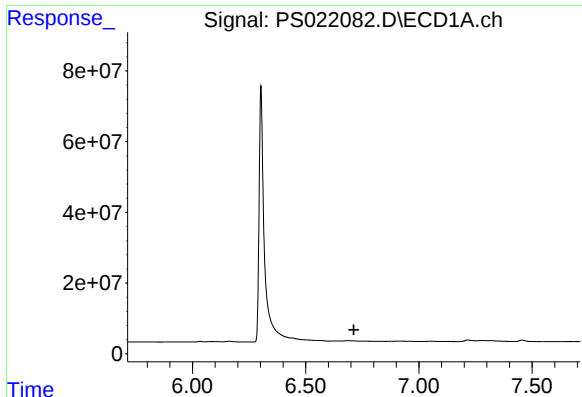

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.713 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

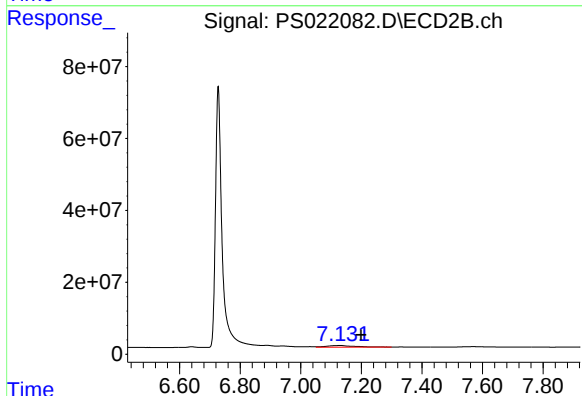


#7 MCPA

R.T.: 7.131 min
Delta R.T.: -0.067 min
Response: 27722894
Conc: 2.76 ug/ml

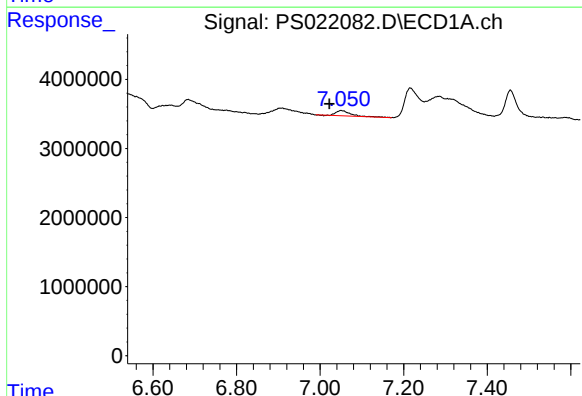


#8 DICHLORPROP

R.T.: 7.050 min
Delta R.T.: 0.028 min
Response: 1762164
Conc: N.D.

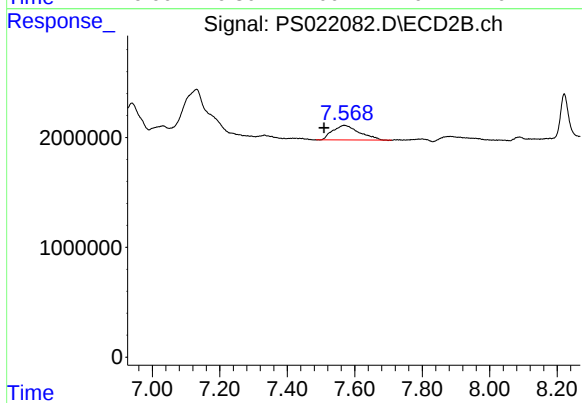

#8 DICHLORPROP


R.T.: 7.569 min
Delta R.T.: 0.060 min
Response: 7340270
Conc: 3.07 ng/ml

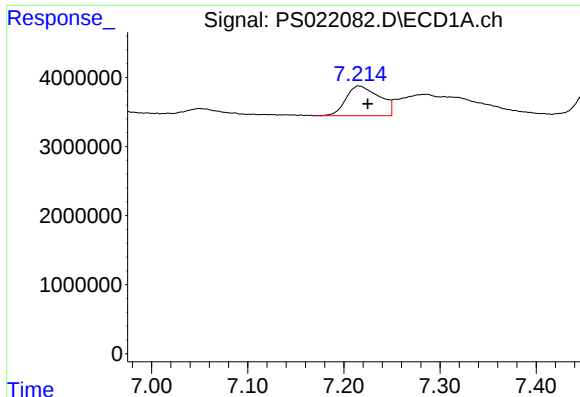

#9 2,4-D


R.T.: 7.216 min
Delta R.T.: -0.009 min
Response: 10474483
Conc: 3.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

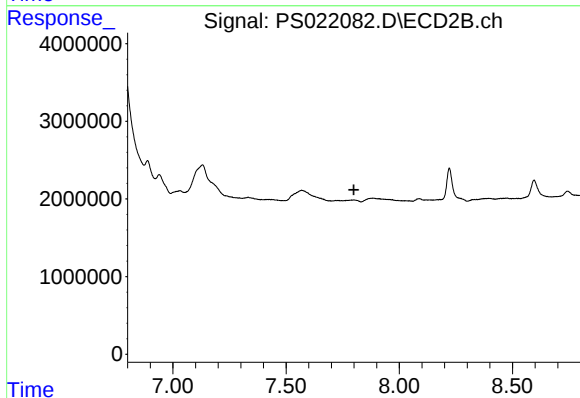


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.799 min
Response: 0
Conc: N.D.

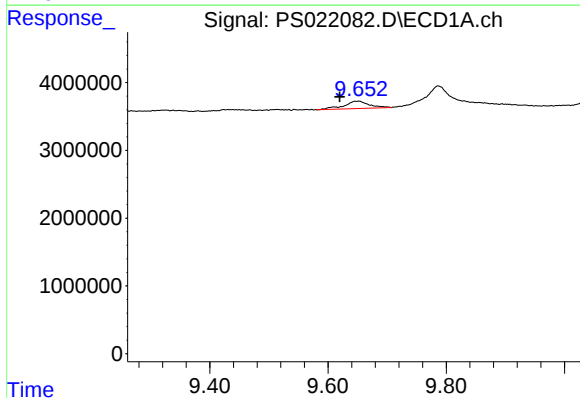


#15 Picloram

R.T.: 9.650 min
Delta R.T.: 0.031 min
Response: 3258383
Conc: N.D.

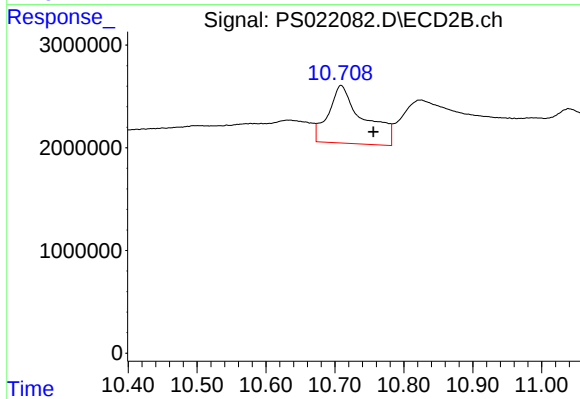

#15 Picloram


R.T.: 10.709 min
Delta R.T.: -0.047 min
Response: 19826254
Conc: 1.09 ng/ml

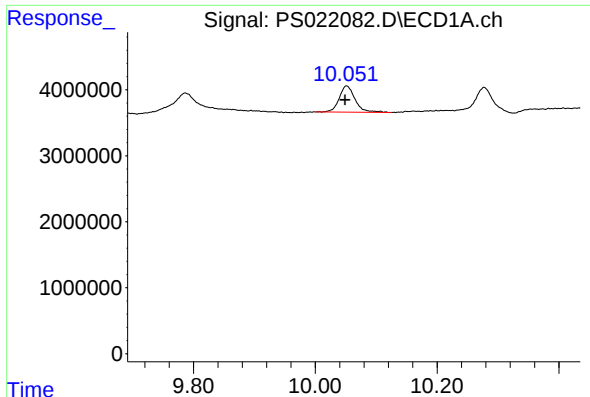

#16 DCPA

R.T.: 10.052 min
Delta R.T.: 0.003 min
Response: 7203240
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

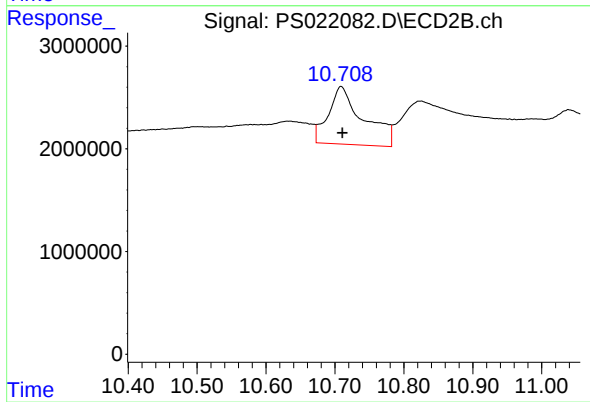

#16 DCPA

R.T.: 10.709 min
Delta R.T.: -0.002 min
Response: 19826254
Conc: 1.29 ng/ml