

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020923\
 Data File : PS022096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2023 14:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 14:48:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020223.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 03 10:03:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.302	6.728	1218.4E6	1143.6E6	534.531	564.967
Target Compounds							
1) T	Dalapon	2.432	0.000	1059329	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.670	0.000	2619817	0	<MDL	N.D. #
3) T	4-Nitroph...	6.159	6.355	6422524	2225572	4.772	1.667 #
5) T	DICAMBA	0.000	6.940f	0	13154737	N.D.	1.392
6) T	MCP	0.000	7.029f	0	4929107	N.D.	<MDL
7) T	MCPA	6.710	7.131f	9154751	34016574	<MDL	3.387 #
8) T	DICHLORPROP	7.048	7.566f	690113	22451232	<MDL	9.384 #
9) T	2,4-D	7.216	0.000	16594855	0	5.520	N.D. #
10) T	Pentachlo...	7.456	8.221	7109844	7200592	<MDL	<MDL #
11) T	2,4,5-TP ...	7.997	8.593	4348780	3888782	<MDL	<MDL #
12) T	2,4,5-T	8.256	9.001f	2819517	3426792	<MDL	<MDL #
13) T	2,4-DB	8.731	0.000	469292	0	<MDL	N.D. #
14) T	DINOSEB	9.785	9.788	6520517	4314970	<MDL	<MDL #
15) T	Picloram	9.648	10.709f	5176722	21445722	<MDL	1.182 #
16) T	DCPA	10.052	10.709	4991150	21445722	<MDL	1.393 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020923\
Data File : PS022096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2023 14:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 14:48:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020223.M
Quant Title : 8080.M
QLast Update : Fri Feb 03 10:03:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

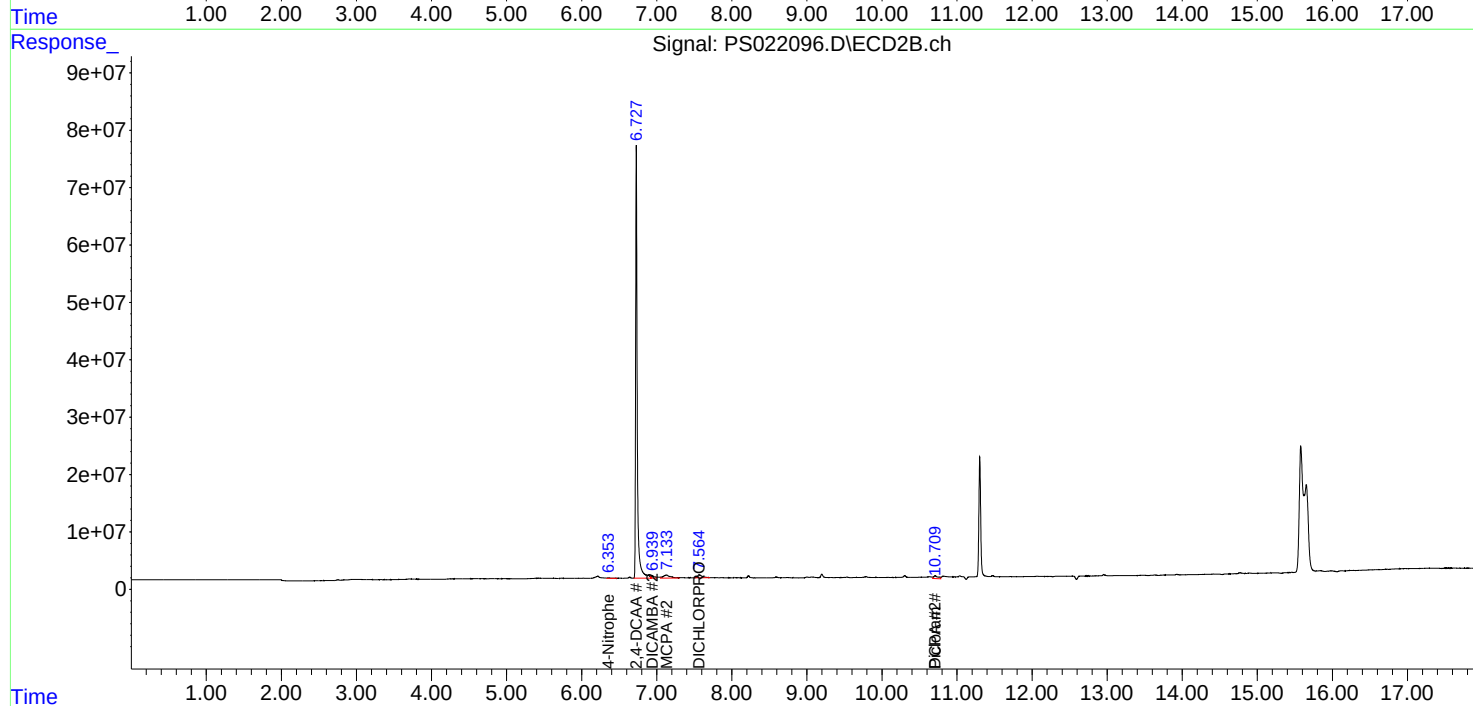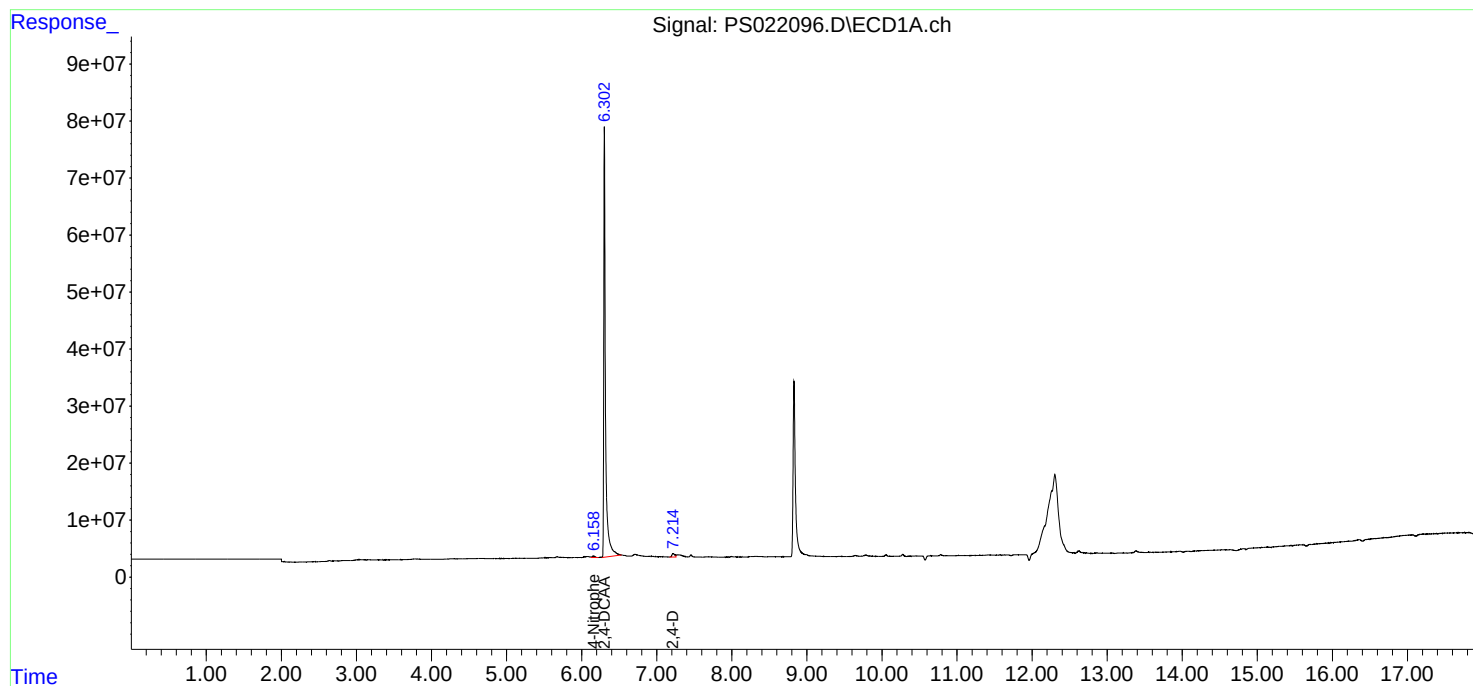


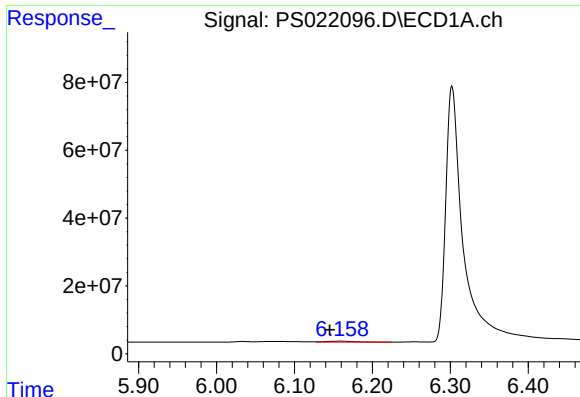

#3 4-Nitrophenol


R.T.: 6.159 min
Delta R.T.: 0.013 min
Response: 6422524
Conc: 4.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

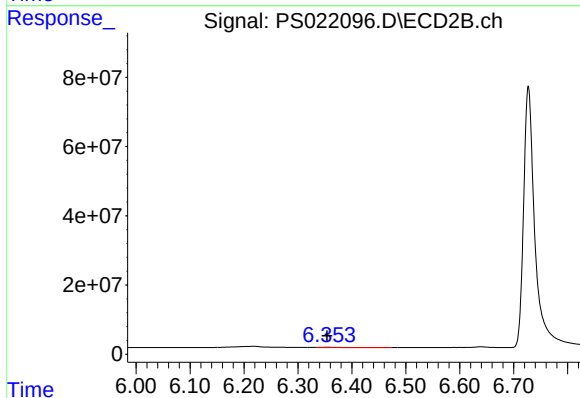


#3 4-Nitrophenol

R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 2225572
Conc: 1.67 ng/ml

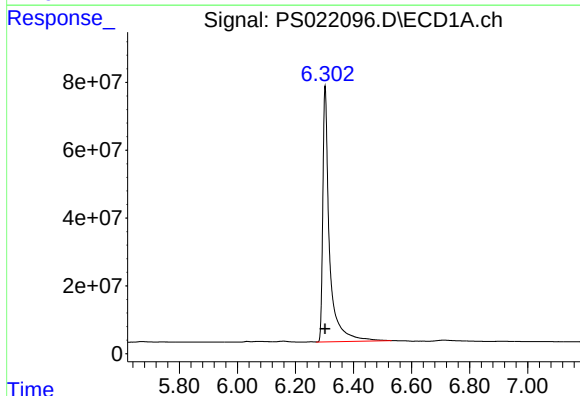


#4 2,4-DCAA

R.T.: 6.302 min
Delta R.T.: 0.000 min
Response: 1218391599
Conc: 534.53 ng/ml

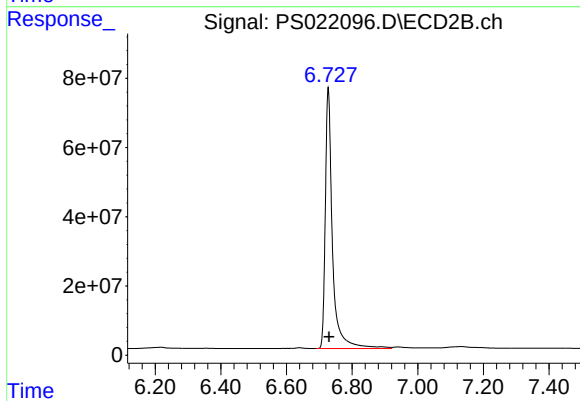

#4 2,4-DCAA


R.T.: 6.728 min
Delta R.T.: -0.003 min
Response: 1143628842
Conc: 564.97 ng/ml

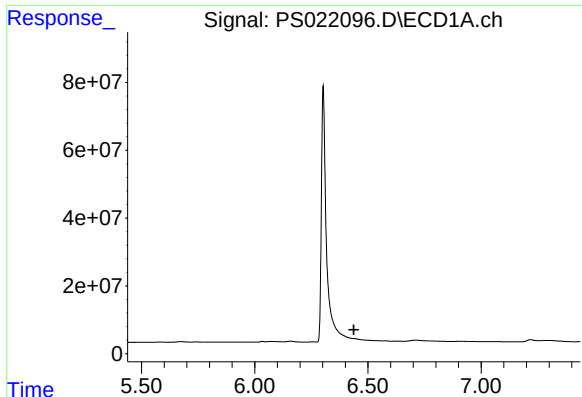

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

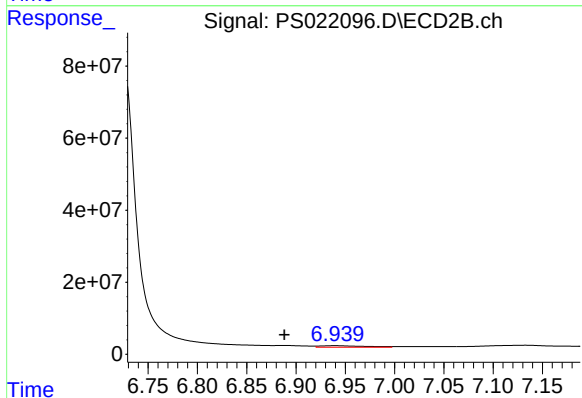


#5 DICAMBA

R.T.: 6.940 min
Delta R.T.: 0.051 min
Response: 13154737
Conc: 1.39 ng/ml

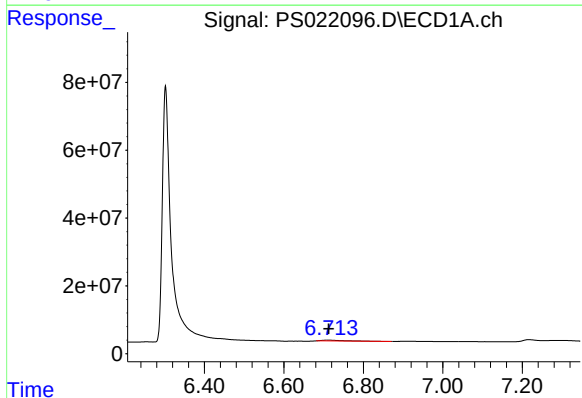


#7 MCPA

R.T.: 6.710 min
Delta R.T.: -0.003 min
Response: 9154751
Conc: N.D.

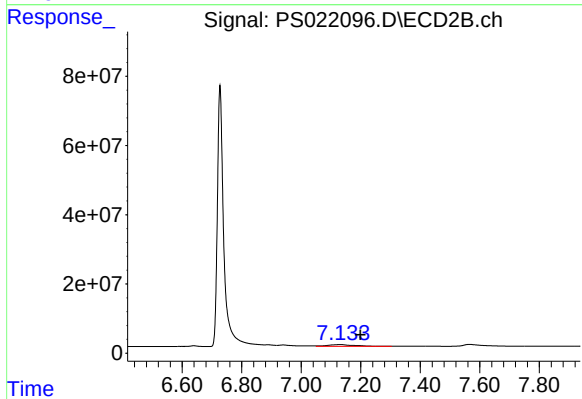

#7 MCPA


R.T.: 7.131 min
Delta R.T.: -0.067 min
Response: 34016574
Conc: 3.39 ug/ml

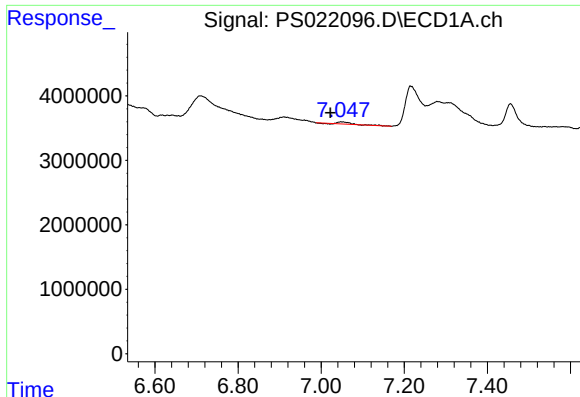

#8 DICHLORPROP


R.T.: 7.048 min
Delta R.T.: 0.026 min
Response: 690113
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

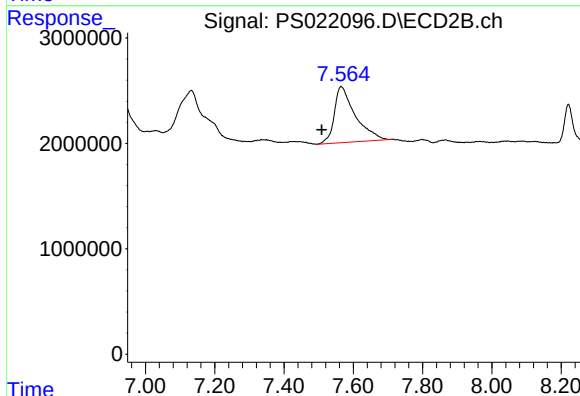


#8 DICHLORPROP

R.T.: 7.566 min
Delta R.T.: 0.057 min
Response: 22451232
Conc: 9.38 ng/ml

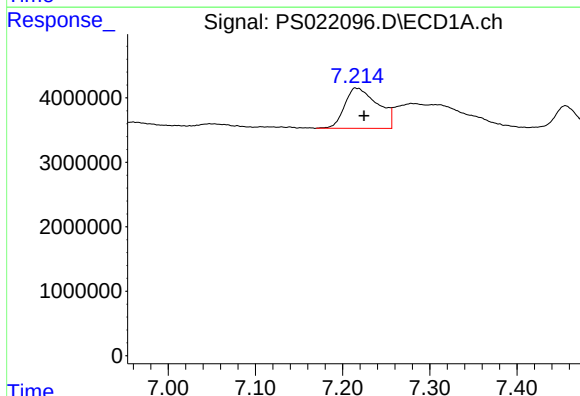


#9 2,4-D

R.T.: 7.216 min
Delta R.T.: -0.008 min
Response: 16594855
Conc: 5.52 ng/ml

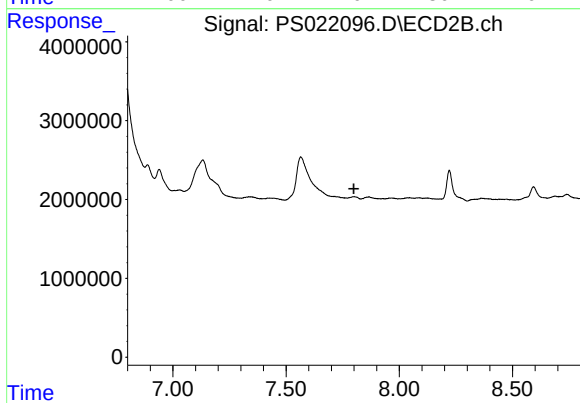

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.799 min
Response: 0
Conc: N.D.

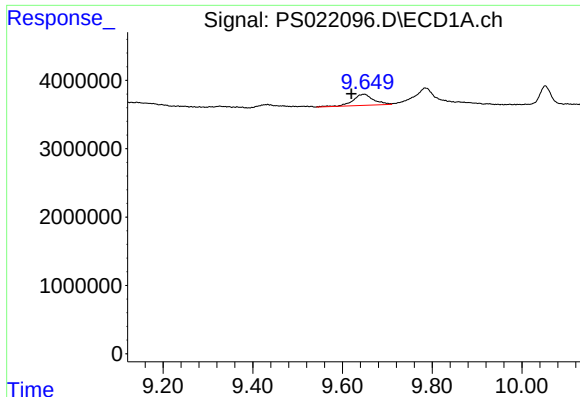

#15 Picloram


R.T.: 9.648 min
Delta R.T.: 0.029 min
Response: 5176722
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

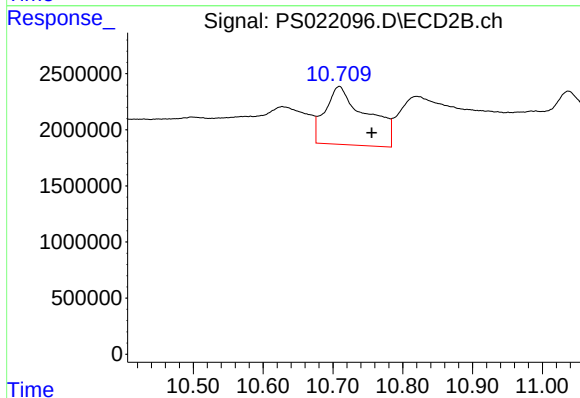


#15 Picloram

R.T.: 10.709 min
Delta R.T.: -0.047 min
Response: 21445722
Conc: 1.18 ng/ml

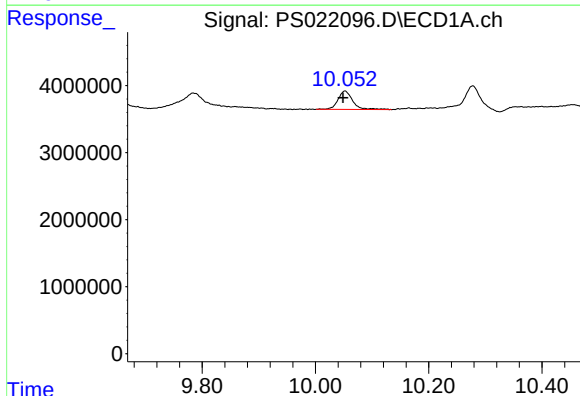

#16 DCPA

R.T.: 10.052 min
Delta R.T.: 0.003 min
Response: 4991150
Conc: N.D.

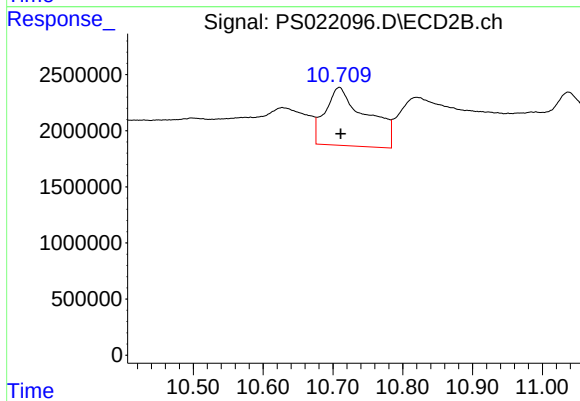

#16 DCPA

R.T.: 10.709 min
Delta R.T.: -0.002 min
Response: 21445722
Conc: 1.39 ng/ml