

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020924\
 Data File : PS025896.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2024 09:02
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 02:02:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.348	6.753	770.9E6	400.1E6	546.218	568.764
Target Compounds							
1) T	Dalapon	0.000	2.557	0	2366011	N.D.	2.133
2) T	3,5-DICHL...	5.691	0.000	6351843	0	2.947	N.D. #
3) T	4-Nitroph...	6.185	6.361	6884382	686838	7.417	1.503 #
5) T	DICAMBA	0.000	6.951	0	15118521	N.D.	4.982
6) T	MCP	0.000	6.951f	0	15118521	N.D.	7.390
8) T	DICHLORPROP	0.000	7.559	0	5432488	N.D.	6.803
9) T	2,4-D	7.244	0.000	82098391	0	46.195	N.D. #
15) T	Picloram	0.000	10.771	0	1494723	N.D.	<MDL
16) T	DCPA	0.000	10.771f	0	1494723	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020924\
Data File : PS025896.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2024 09:02
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 02:02:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

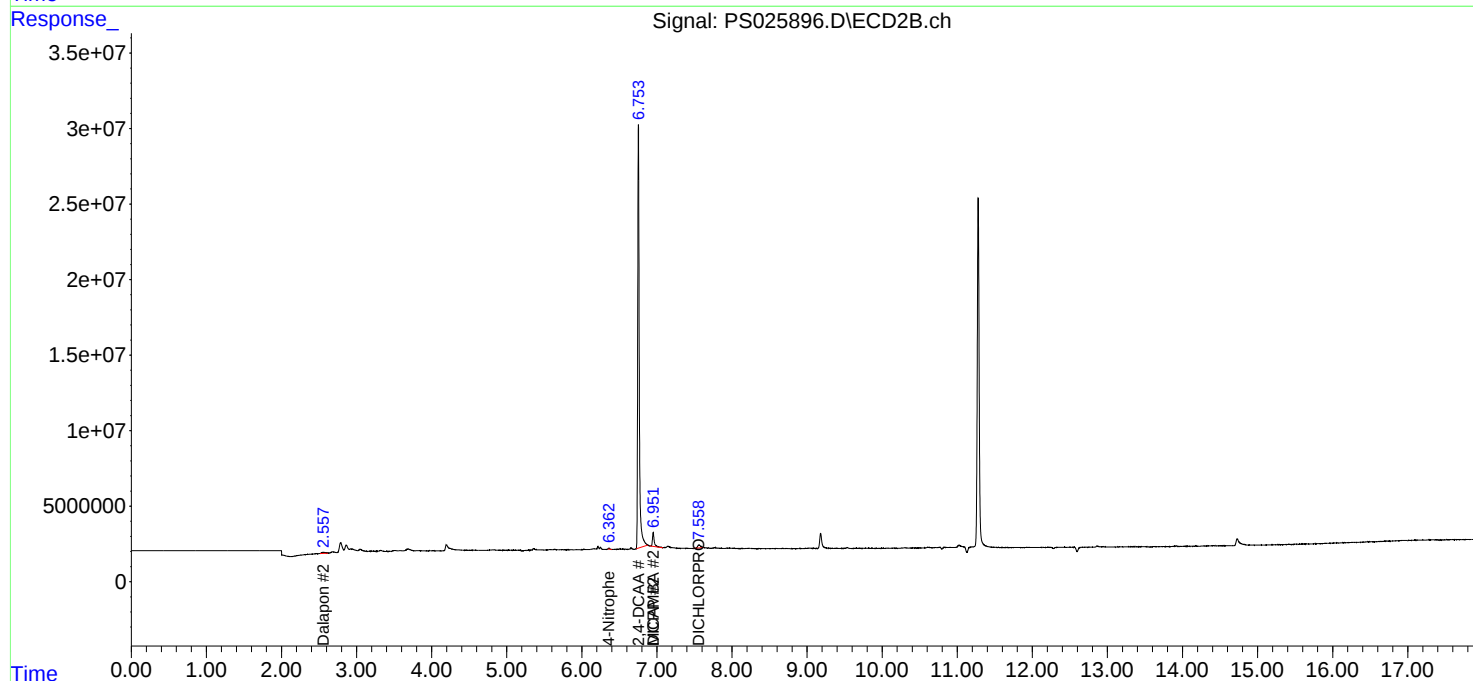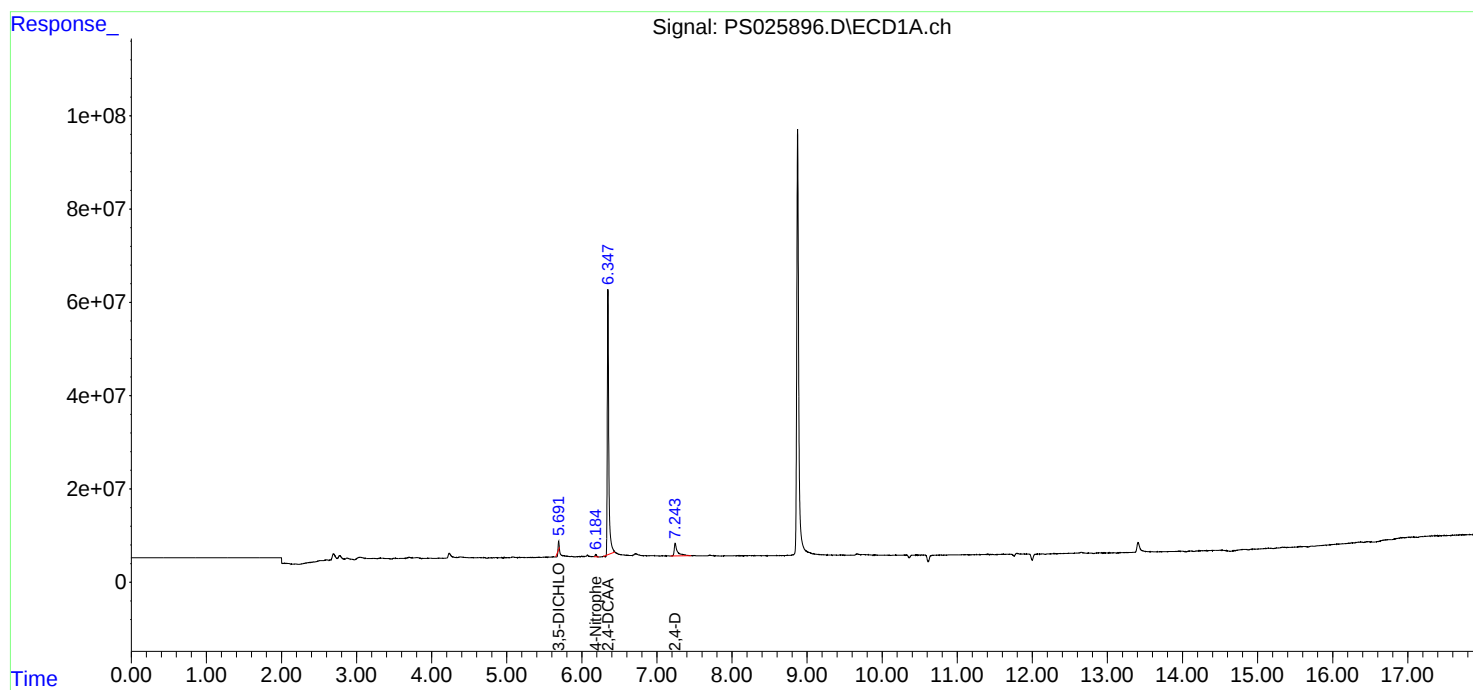

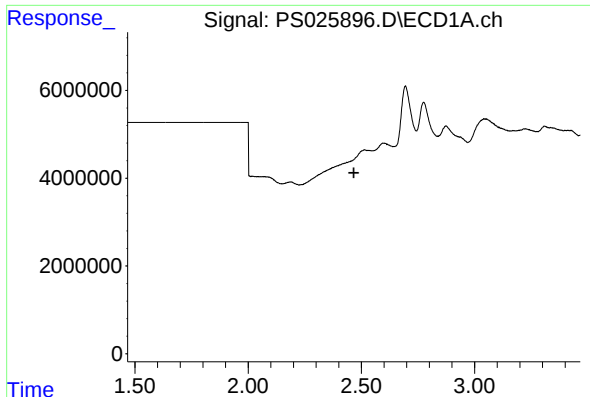

#1 Dalapon

R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

#1 Dalapon


R.T.: 2.557 min
Delta R.T.: 0.034 min
Response: 2366011
Conc: 2.13 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.691 min
Delta R.T.: -0.031 min
Response: 6351843
Conc: 2.95 ng/ml

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.947 min
Response: 0
Conc: N.D.

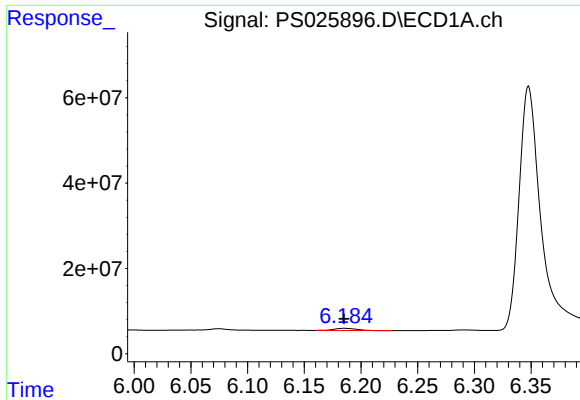

#3 4-Nitrophenol


R.T.: 6.185 min
Delta R.T.: 0.000 min
Response: 6884382
Conc: 7.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

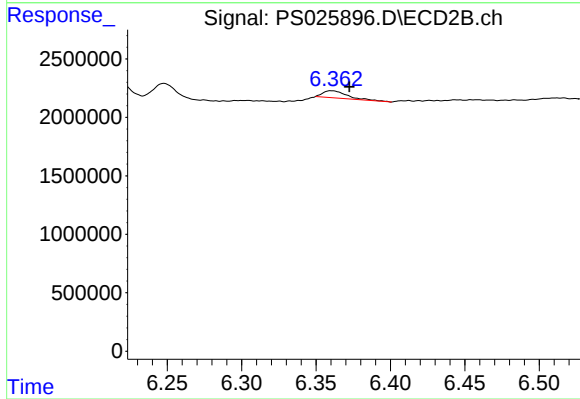


#3 4-Nitrophenol

R.T.: 6.361 min
Delta R.T.: -0.012 min
Response: 686838
Conc: 1.50 ng/ml

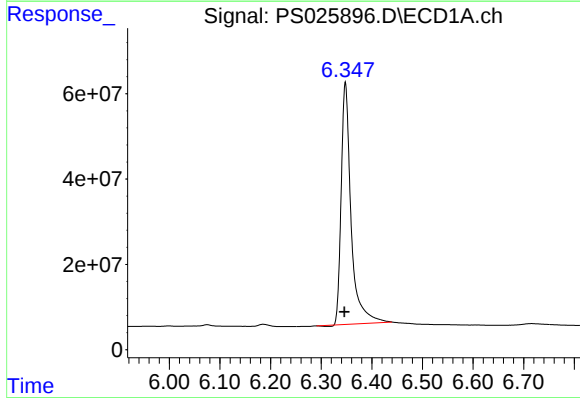


#4 2,4-DCAA

R.T.: 6.348 min
Delta R.T.: 0.002 min
Response: 770851655
Conc: 546.22 ng/ml

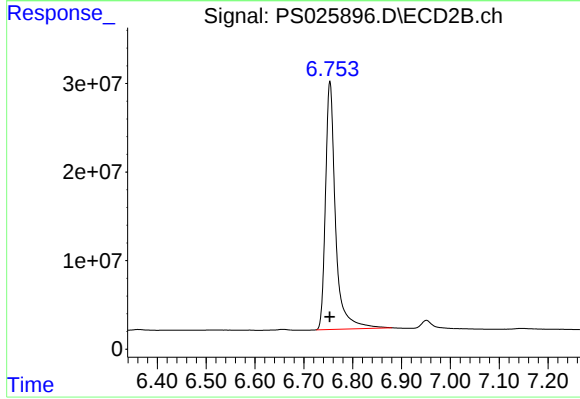

#4 2,4-DCAA


R.T.: 6.753 min
Delta R.T.: 0.000 min
Response: 400093017
Conc: 568.76 ng/ml

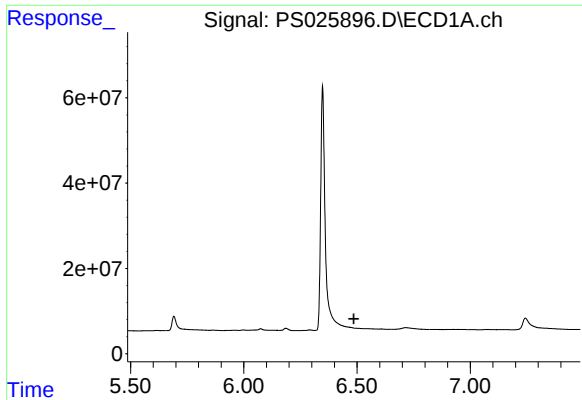

#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 6.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

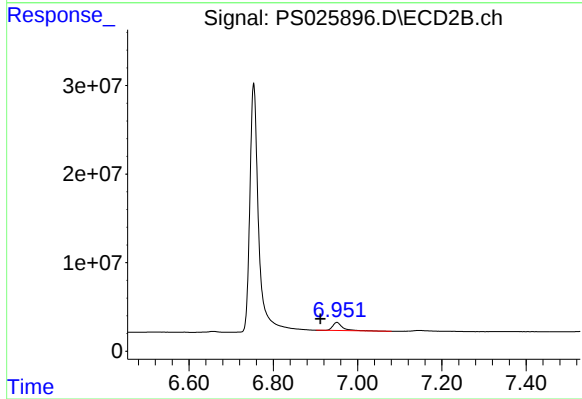


#5 DICAMBA

R.T.: 6.951 min
Delta R.T.: 0.039 min
Response: 15118521
Conc: 4.98 ng/ml


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

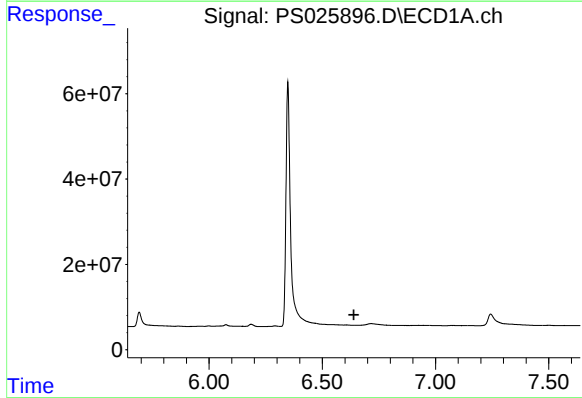

#6 MCPP


R.T.: 6.951 min
Delta R.T.: -0.062 min
Response: 15118521
Conc: 7.39 ug/ml

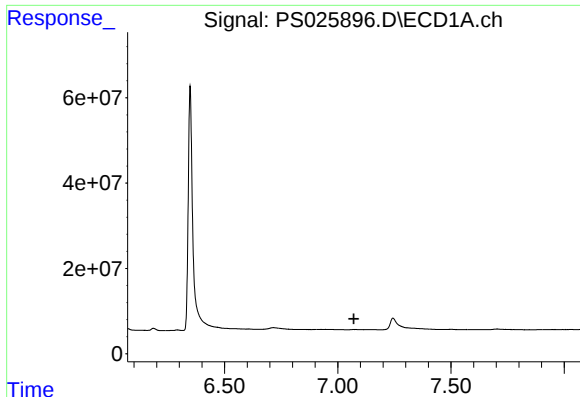

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

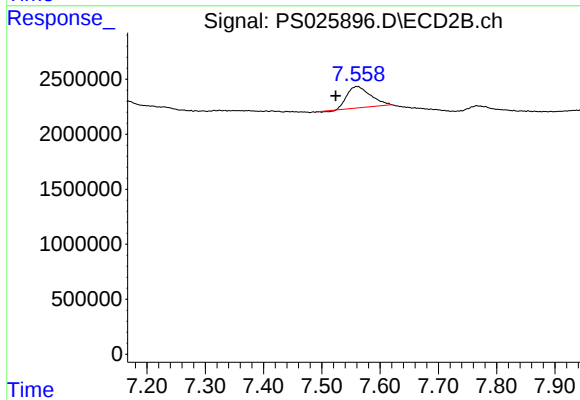


#8 DICHLORPROP

R.T.: 7.559 min
Delta R.T.: 0.036 min
Response: 5432488
Conc: 6.80 ng/ml

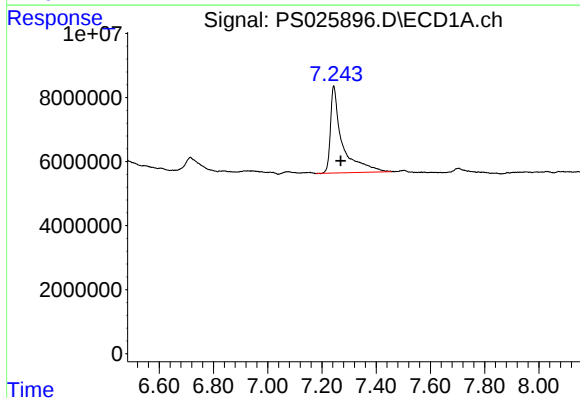

#9 2,4-D

R.T.: 7.244 min
Delta R.T.: -0.025 min
Response: 82098391
Conc: 46.20 ng/ml

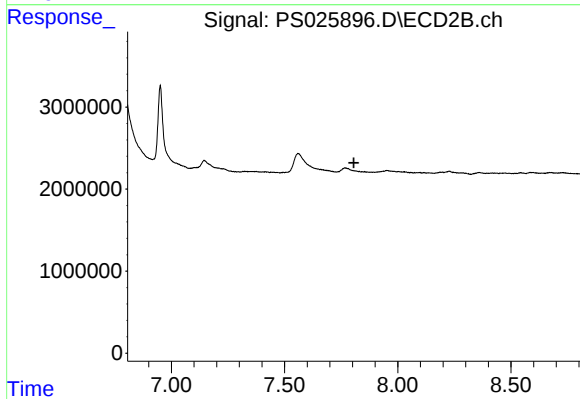

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.806 min
Response: 0
Conc: N.D.