

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020924\
 Data File : PS025908.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2024 17:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 02:08:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.348	6.754	809.3E6	417.4E6	573.445	593.406
Target Compounds							
1) T	Dalapon	0.000	2.558	0	1896855	N.D.	1.710
2) T	3,5-DICHL...	5.691	0.000	7031221	0	3.263	N.D. #
5) T	DICAMBA	0.000	6.951	0	17092396	N.D.	5.632
6) T	MCP	0.000	6.951f	0	17092396	N.D.	8.355
8) T	DICHLORPROP	0.000	7.563	0	4391975	N.D.	5.500
9) T	2,4-D	7.246	0.000	97290412	0	54.744	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020924\
Data File : PS025908.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2024 17:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 02:08:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

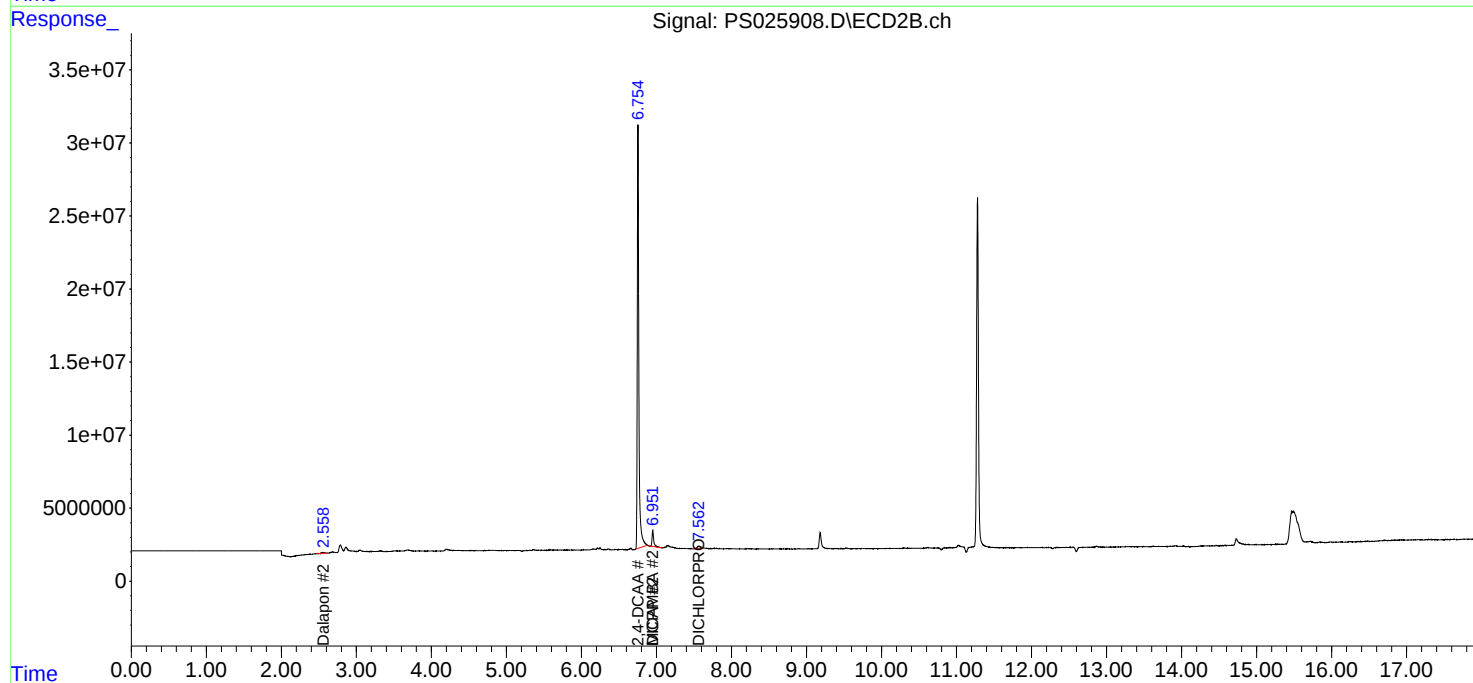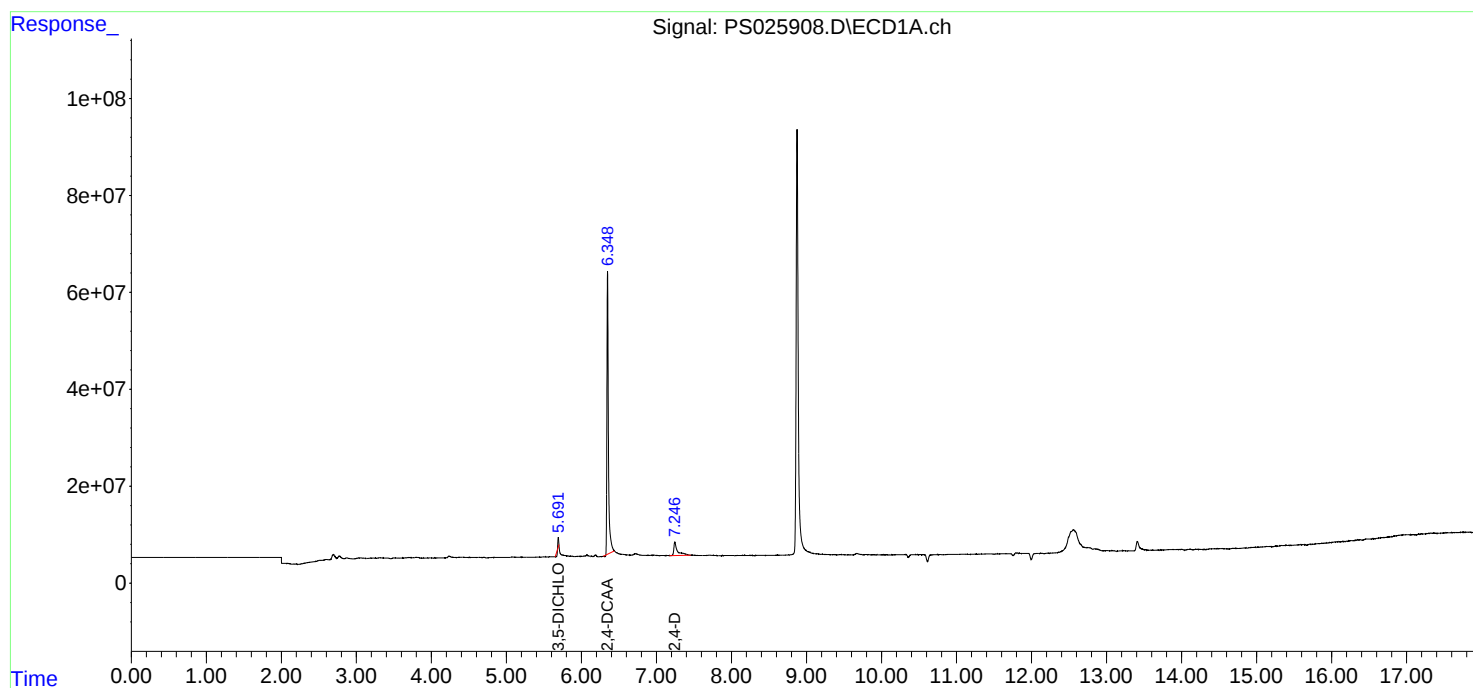


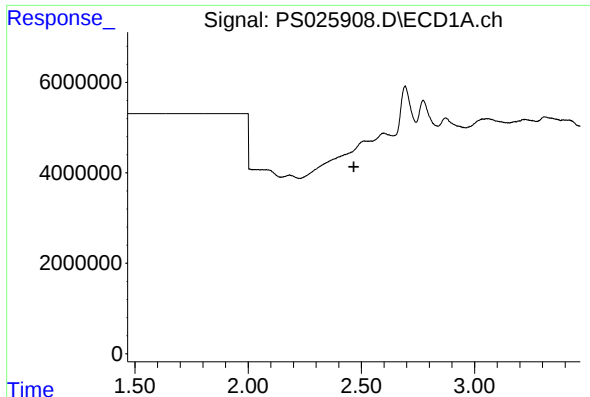

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

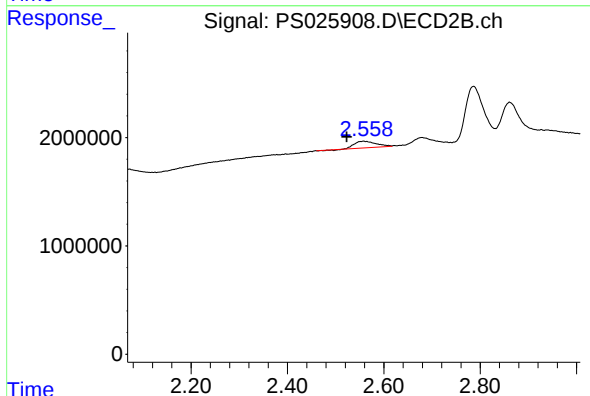


#1 Dalapon

R.T.: 2.558 min
Delta R.T.: 0.035 min
Response: 1896855
Conc: 1.71 ng/ml

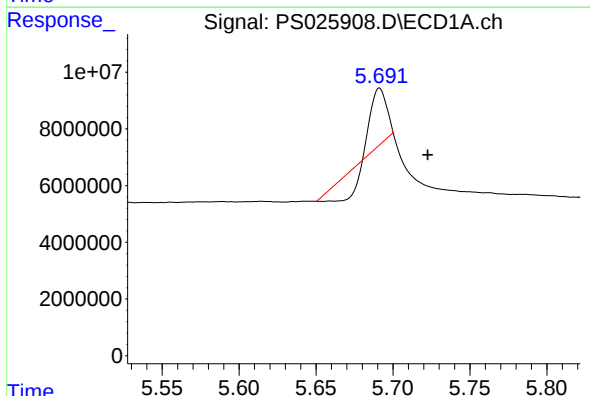


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.691 min
Delta R.T.: -0.031 min
Response: 7031221
Conc: 3.26 ng/ml

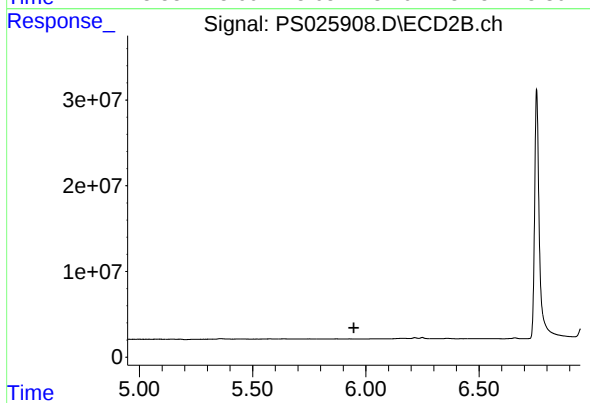

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.947 min
Response: 0
Conc: N.D.

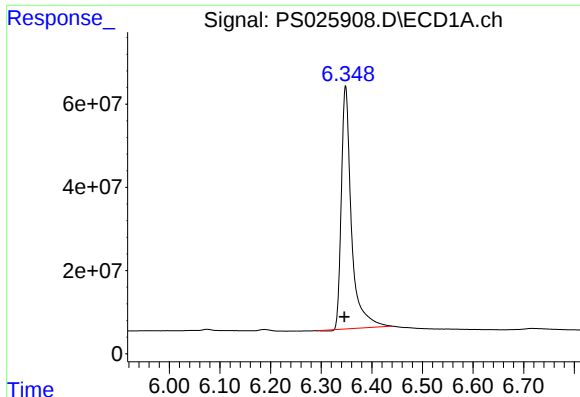

#4 2,4-DCAA


R.T.: 6.348 min
Delta R.T.: 0.002 min
Response: 809275894
Conc: 573.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

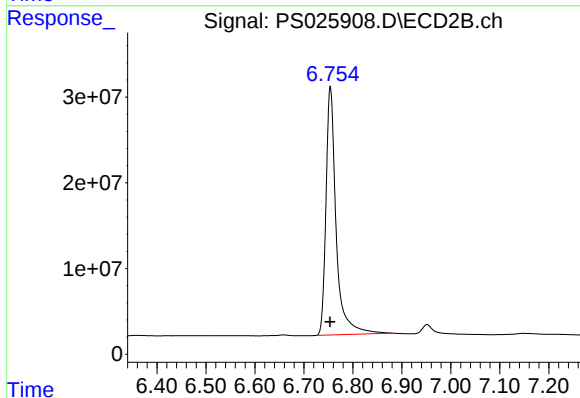


#4 2,4-DCAA

R.T.: 6.754 min
Delta R.T.: 0.000 min
Response: 417427580
Conc: 593.41 ng/ml

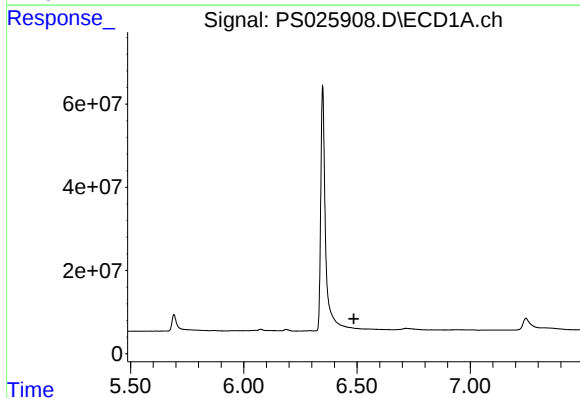


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.486 min
Response: 0
Conc: N.D.

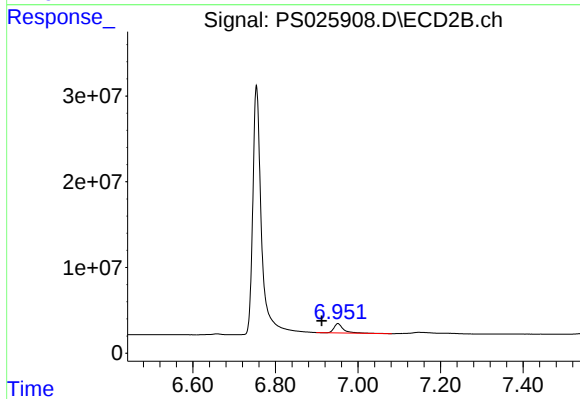

#5 DICAMBA


R.T.: 6.951 min
Delta R.T.: 0.039 min
Response: 17092396
Conc: 5.63 ng/ml

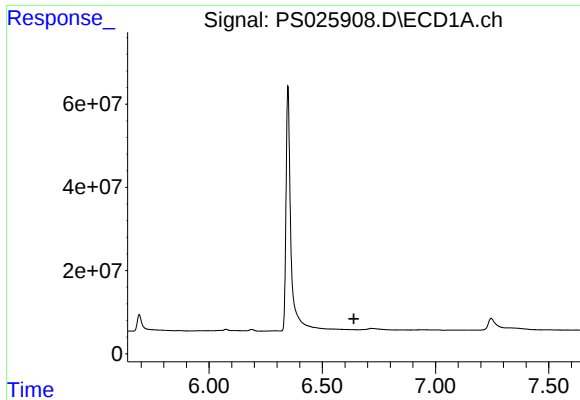

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

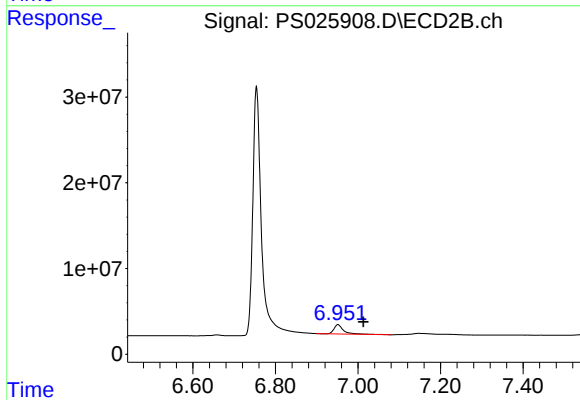


#6 MCP

R.T.: 6.951 min
Delta R.T.: -0.062 min
Response: 17092396
Conc: 8.35 ug/ml

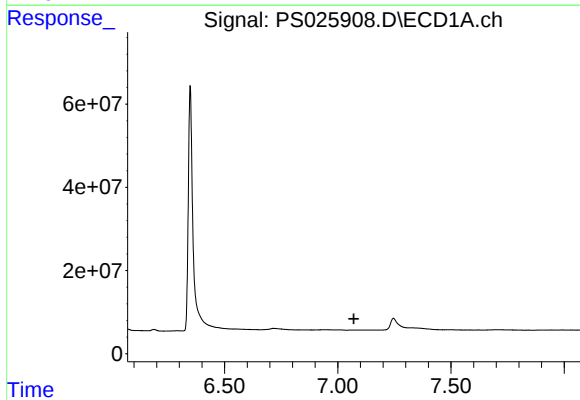


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

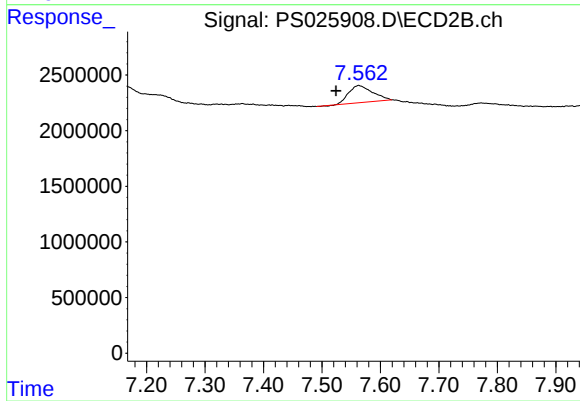

#8 DICHLORPROP


R.T.: 7.563 min
Delta R.T.: 0.039 min
Response: 4391975
Conc: 5.50 ng/ml

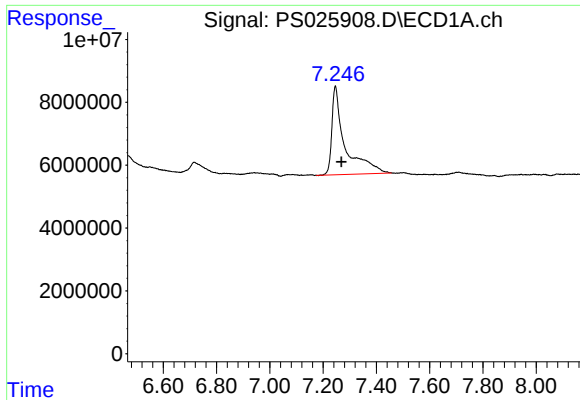

#9 2,4-D

R.T.: 7.246 min
Delta R.T.: -0.023 min
Response: 97290412
Conc: 54.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

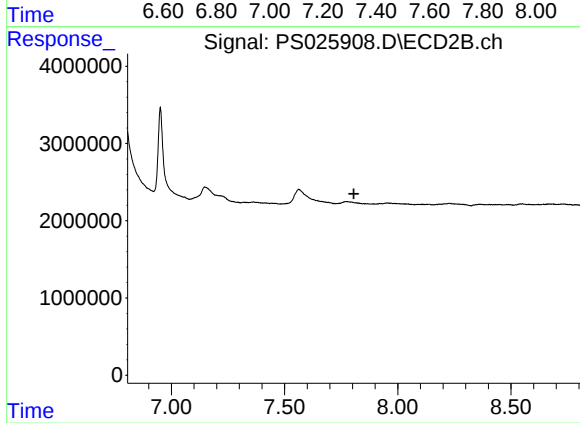

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.806 min
Response: 0
Conc: N.D.