

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020924\
 Data File : PS025917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2024 21:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 02:12:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.349	6.754	809.0E6	416.5E6	573.235	592.135
Target Compounds							
1) T	Dalapon	0.000	2.556	0	968360	N.D.	<MDL
2) T	3,5-DICHL...	5.691	0.000	11889709	0	5.517	N.D. #
5) T	DICAMBA	0.000	6.951	0	16797106	N.D.	5.535
6) T	MCP	0.000	6.951f	0	16797106	N.D.	8.210
7) T	MCPA	0.000	7.218	0	342755	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.562	0	5489202	N.D.	6.874
9) T	2,4-D	7.246	7.772	70527579	392712	39.685	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020924\
Data File : PS025917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2024 21:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 02:12:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

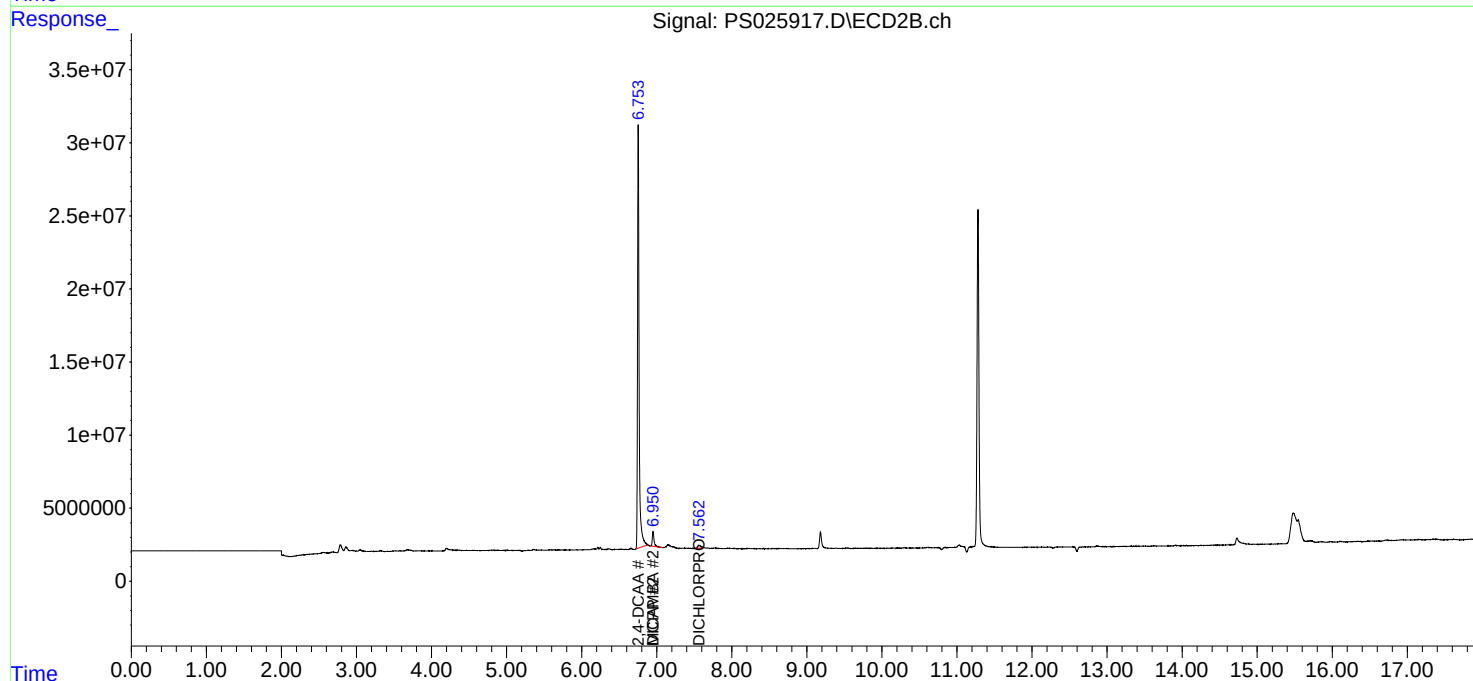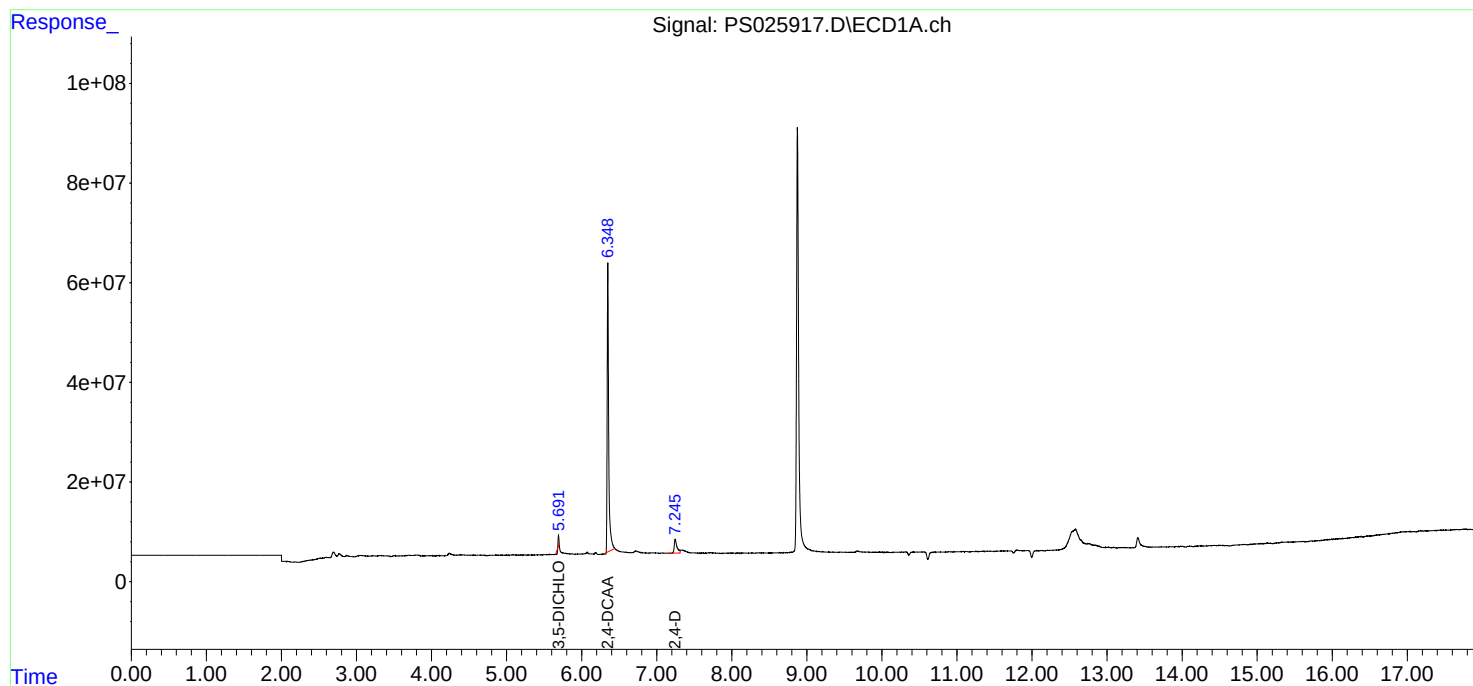


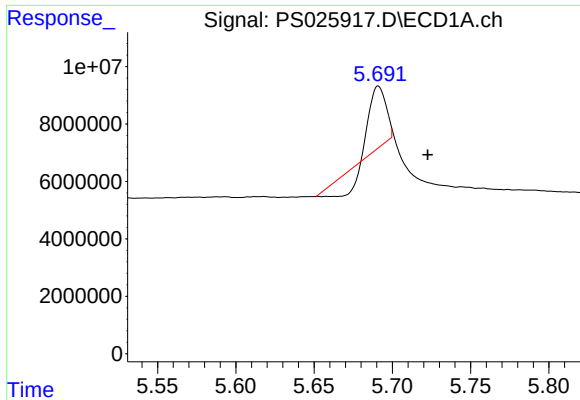

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.691 min
Delta R.T.: -0.031 min
Response: 11889709
Conc: 5.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

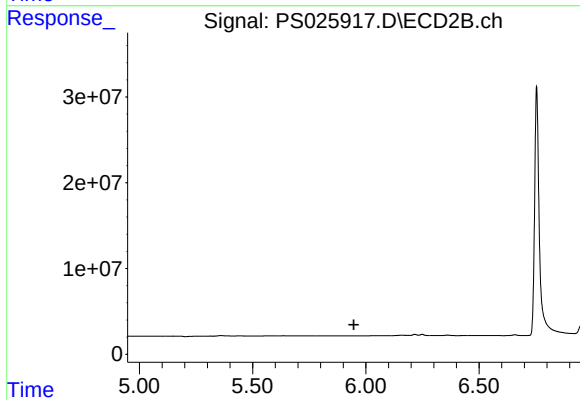


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.947 min
Response: 0
Conc: N.D.

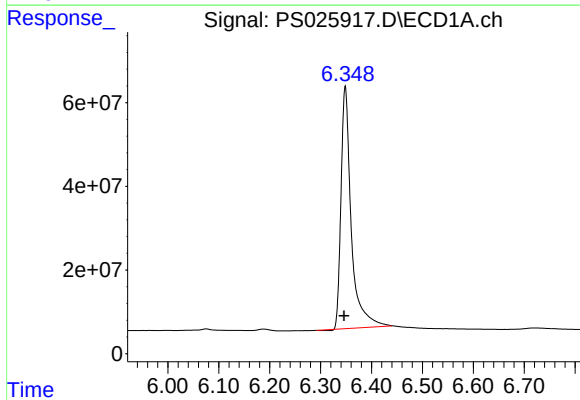


#4 2,4-DCAA

R.T.: 6.349 min
Delta R.T.: 0.003 min
Response: 808978637
Conc: 573.23 ng/ml

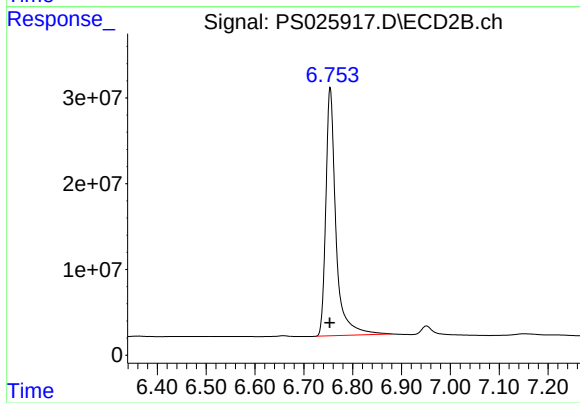

#4 2,4-DCAA


R.T.: 6.754 min
Delta R.T.: 0.000 min
Response: 416533234
Conc: 592.13 ng/ml

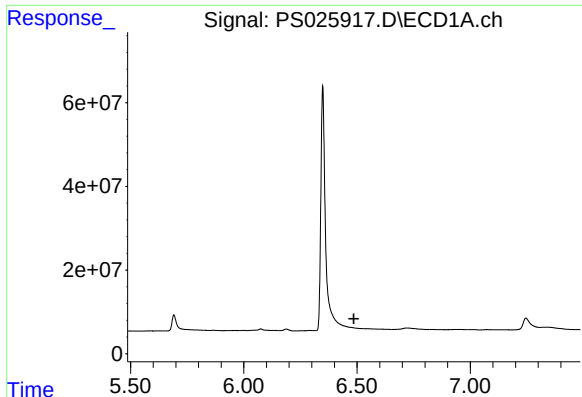

#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 6.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

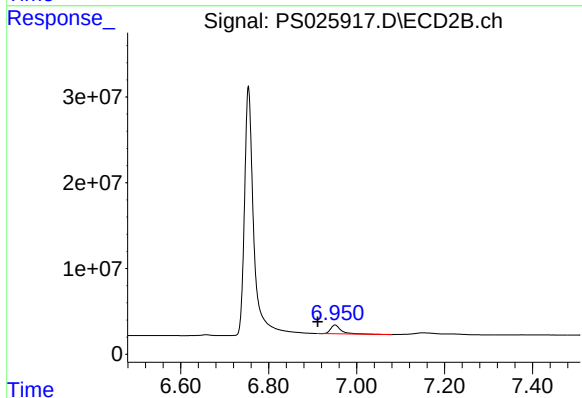

#5 DICAMBA


R.T.: 6.951 min
Delta R.T.: 0.039 min
Response: 16797106
Conc: 5.53 ng/ml

#6 MCPP

R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

#6 MCPP


R.T.: 6.951 min
Delta R.T.: -0.062 min
Response: 16797106
Conc: 8.21 ug/ml

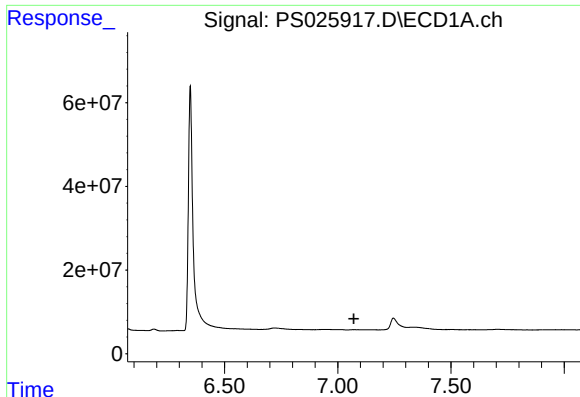

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

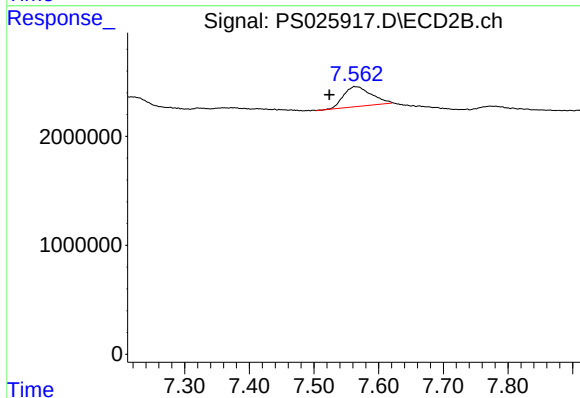


#8 DICHLORPROP

R.T.: 7.562 min
Delta R.T.: 0.039 min
Response: 5489202
Conc: 6.87 ng/ml

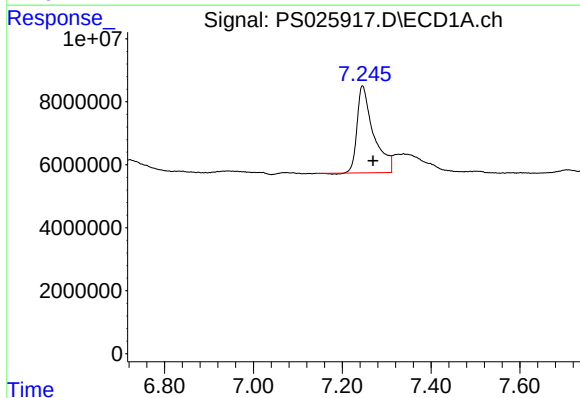

#9 2,4-D

R.T.: 7.246 min
Delta R.T.: -0.023 min
Response: 70527579
Conc: 39.68 ng/ml

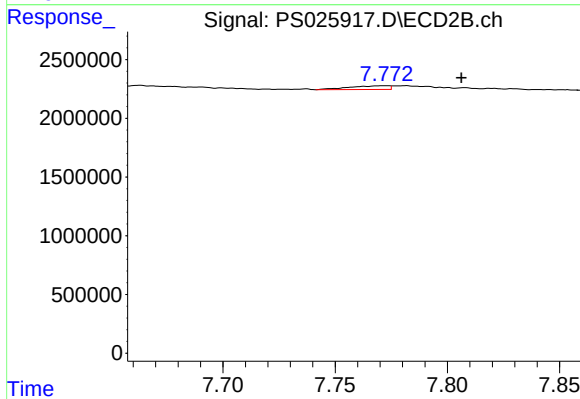

#9 2,4-D

R.T.: 7.772 min
Delta R.T.: -0.034 min
Response: 392712
Conc: N.D.