

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021022\
 Data File : PS018315.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2022 09:17
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 13:45:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 09 15:57:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) T	DICAMBA	7.218	0.000	3898262	0	<MDL	N.D.	#
7) T	MCPA	7.513	0.000	20592282	0	3.161	N.D.	#
9) T	2,4-D	8.181f	0.000	13103578	0	7.116	N.D.	#
11) T	2,4,5-TP ...	8.980	8.435	5440667	6290852	<MDL	1.698	#
12) T	2,4,5-T	9.279	8.864	36981153	8179615	4.179	2.310	#
13) T	2,4-DB	9.852f	0.000	43678573	0	24.818	N.D.	#
14) T	DINOSEB	10.939	0.000	36977890	0	5.538	N.D.	#
15) T	Picloram	10.761	10.665	8256588	179.0E6	<MDL	35.720	#
16) T	DCPA	11.212	0.000	7813527	0	<MDL	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021022\
Data File : PS018315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2022 09:17
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 13:45:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
Quant Title : 8080.M
QLast Update : Wed Feb 09 15:57:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

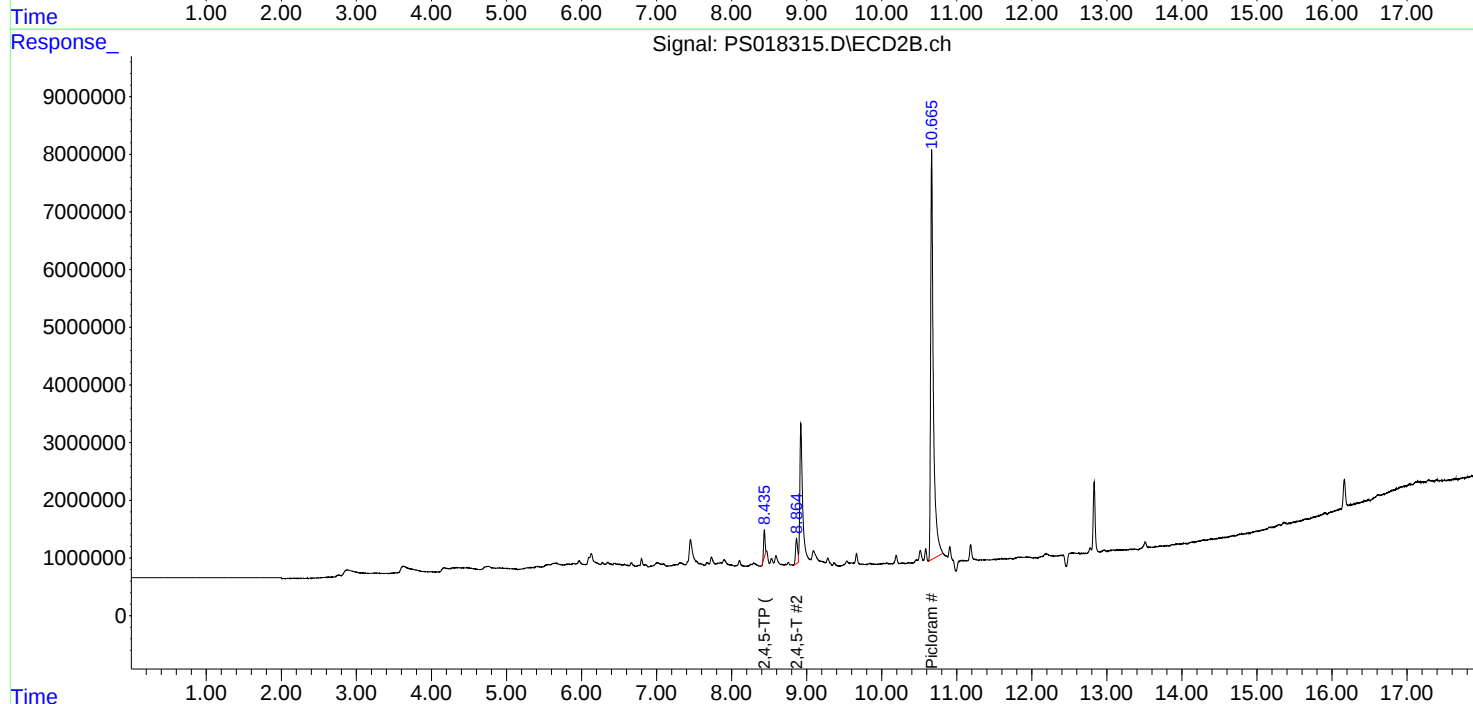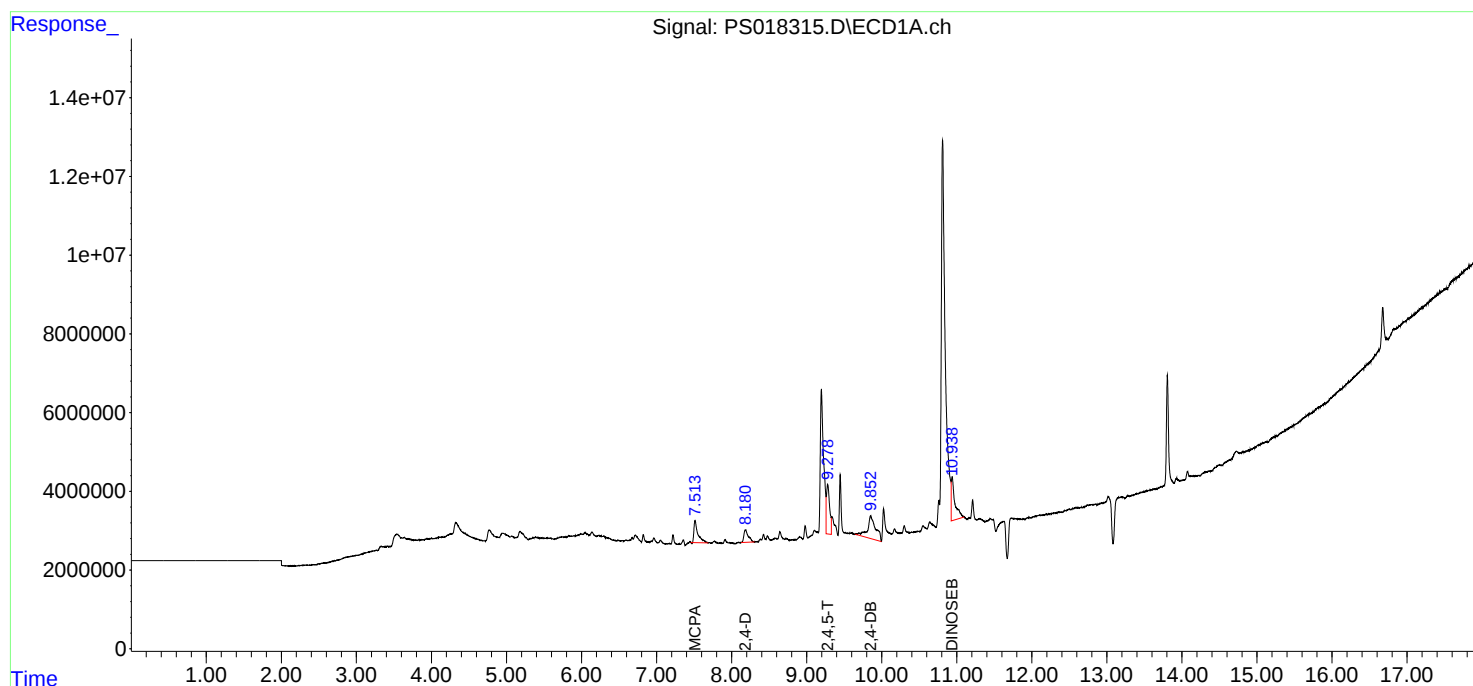


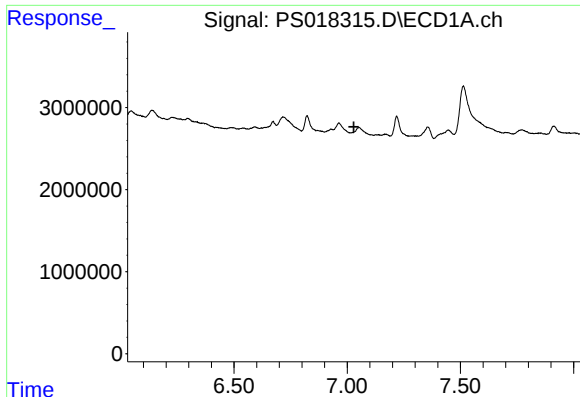

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

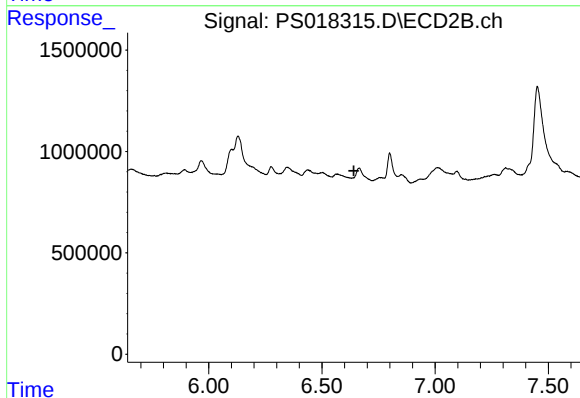


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.641 min
Response: 0
Conc: N.D.

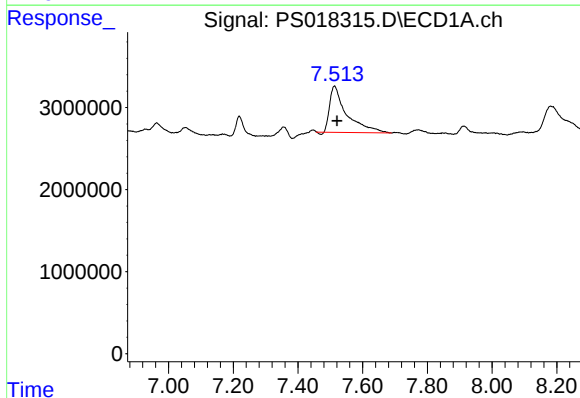


#7 MCPA

R.T.: 7.513 min
Delta R.T.: -0.009 min
Response: 20592282
Conc: 3.16 ug/ml

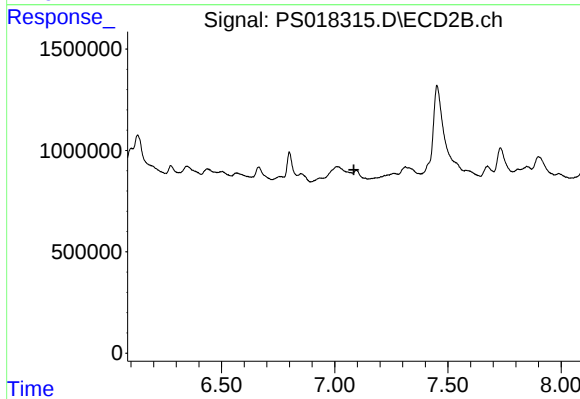

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

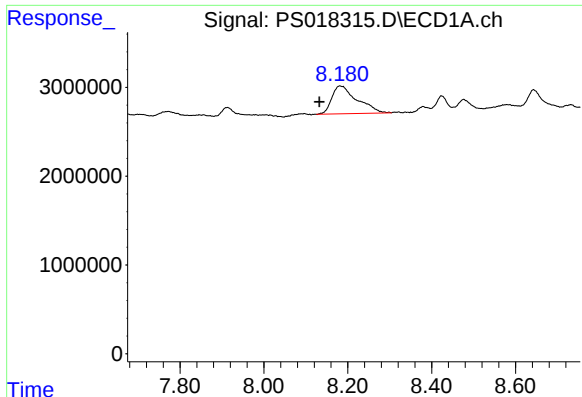

#9 2,4-D


R.T.: 8.181 min
Delta R.T.: 0.049 min
Response: 13103578
Conc: 7.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

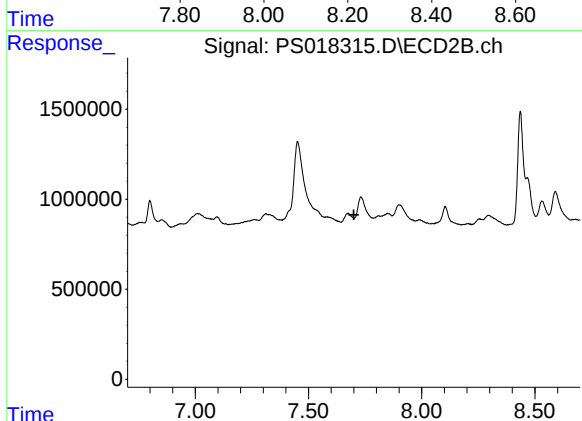


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.

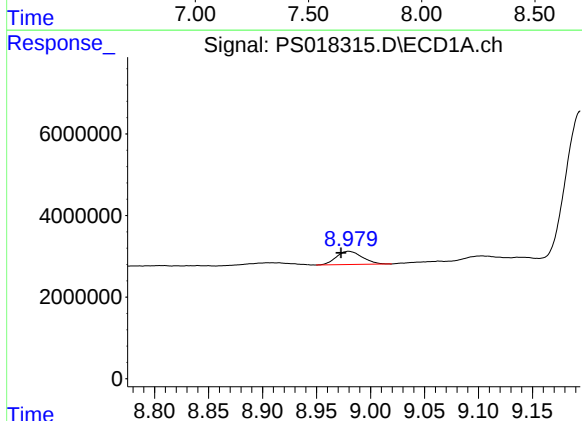


#11 2,4,5-TP (SILVEX)

R.T.: 8.980 min
Delta R.T.: 0.007 min
Response: 5440667
Conc: N.D.

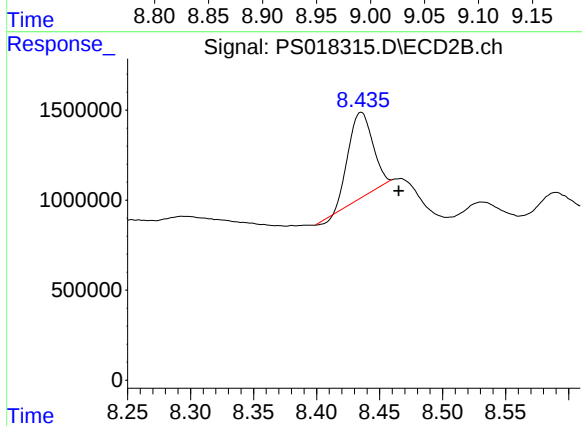

#11 2,4,5-TP (SILVEX)


R.T.: 8.435 min
Delta R.T.: -0.030 min
Response: 6290852
Conc: 1.70 ng/ml

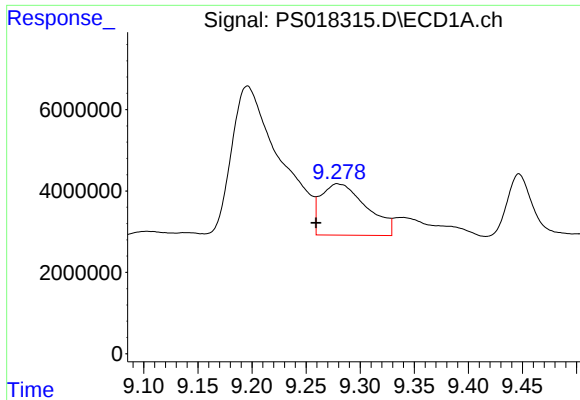

#12 2,4,5-T


R.T.: 9.279 min
Delta R.T.: 0.019 min
Response: 36981153
Conc: 4.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

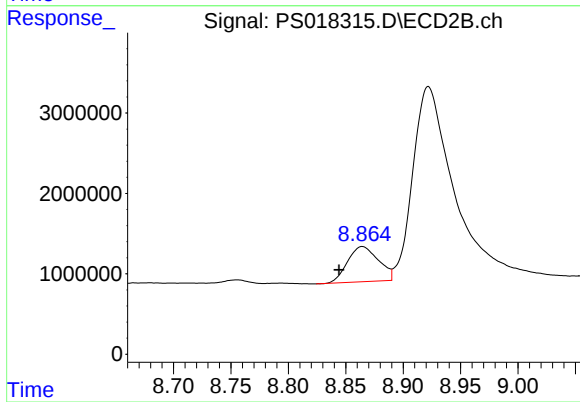


#12 2,4,5-T

R.T.: 8.864 min
Delta R.T.: 0.020 min
Response: 8179615
Conc: 2.31 ng/ml

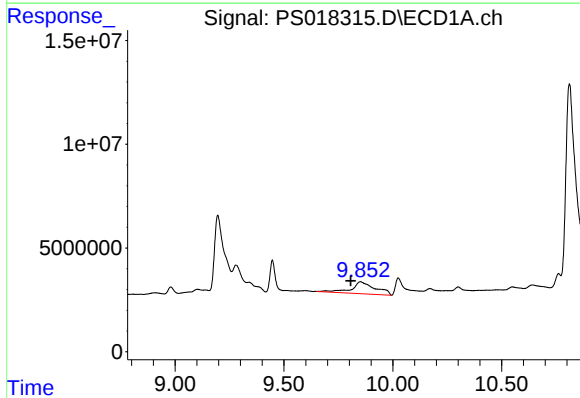


#13 2,4-DB

R.T.: 9.852 min
Delta R.T.: 0.045 min
Response: 43678573
Conc: 24.82 ng/ml

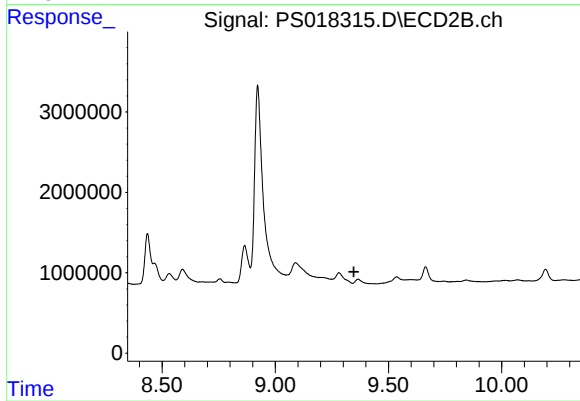

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.347 min
Response: 0
Conc: N.D.

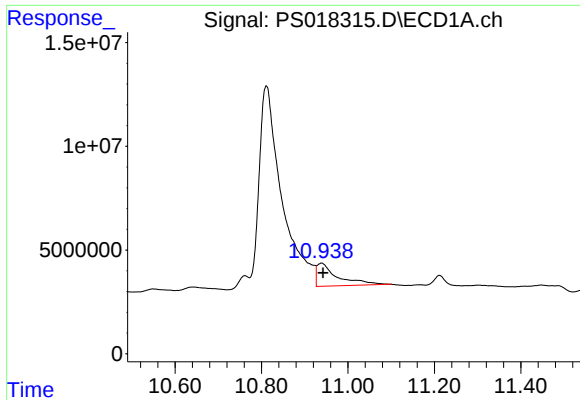

#14 DINoseb


R.T.: 10.939 min
Delta R.T.: -0.004 min
Response: 36977890
Conc: 5.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

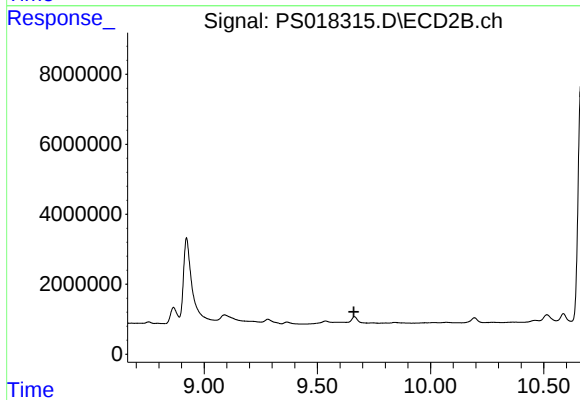


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 9.661 min
Response: 0
Conc: N.D.

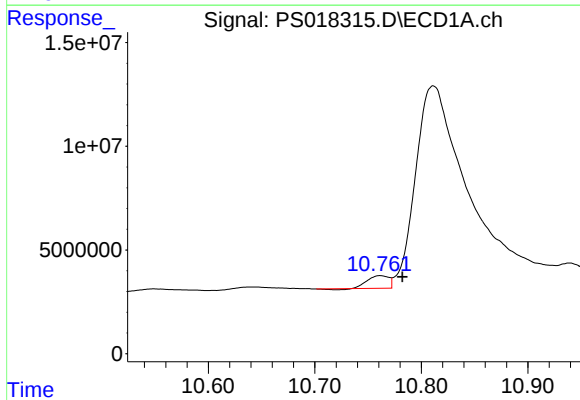

#15 Picloram

R.T.: 10.761 min
Delta R.T.: -0.021 min
Response: 8256588
Conc: N.D.

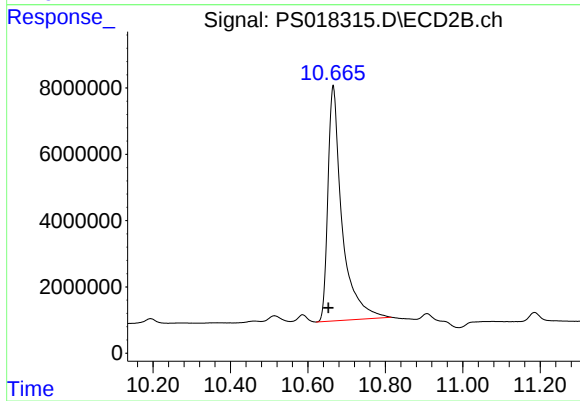

#15 Picloram

R.T.: 10.665 min
Delta R.T.: 0.013 min
Response: 179025179
Conc: 35.72 ng/ml