

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021023\
 Data File : PS022112.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2023 19:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 04:03:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020223.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 03 10:03:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.303	6.727	1235.2E6	1158.5E6	541.902	572.293
Target Compounds							
1) T	Dalapon	2.448	0.000	1437742	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.670	0.000	4329042	0	1.257	N.D. #
3) T	4-Nitroph...	6.161	6.359	5712867	1376580	4.245	1.031 #
5) T	DICAMBA	0.000	6.888	0	9686919	N.D.	1.025
6) T	MCPD	0.000	6.940f	0	8993005	N.D.	1.205
7) T	MCPA	6.707	7.131f	764283	21359408	<MDL	2.126 #
8) T	DICHLORPROP	7.050	7.574f	993759	11528385	<MDL	4.819 #
9) T	2,4-D	7.215	0.000	25342529	0	8.429	N.D. #
10) T	Pentachlo...	7.455	8.221	10901965	7558105	<MDL	<MDL #
11) T	2,4,5-TP ...	7.945	8.595	283652	4020182	<MDL	<MDL #
12) T	2,4,5-T	0.000	9.004f	0	3950733	N.D.	<MDL
13) T	2,4-DB	8.735	0.000	194018	0	<MDL	N.D. #
14) T	DINOSEB	9.787	9.789	8003651	3176791	<MDL	<MDL #
15) T	Picloram	9.648	10.710f	4754403	18033370	<MDL	<MDL #
16) T	DCPA	10.052	10.710	5503680	18033370	<MDL	1.172 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021023\
Data File : PS022112.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2023 19:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 04:03:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020223.M
Quant Title : 8080.M
QLast Update : Fri Feb 03 10:03:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

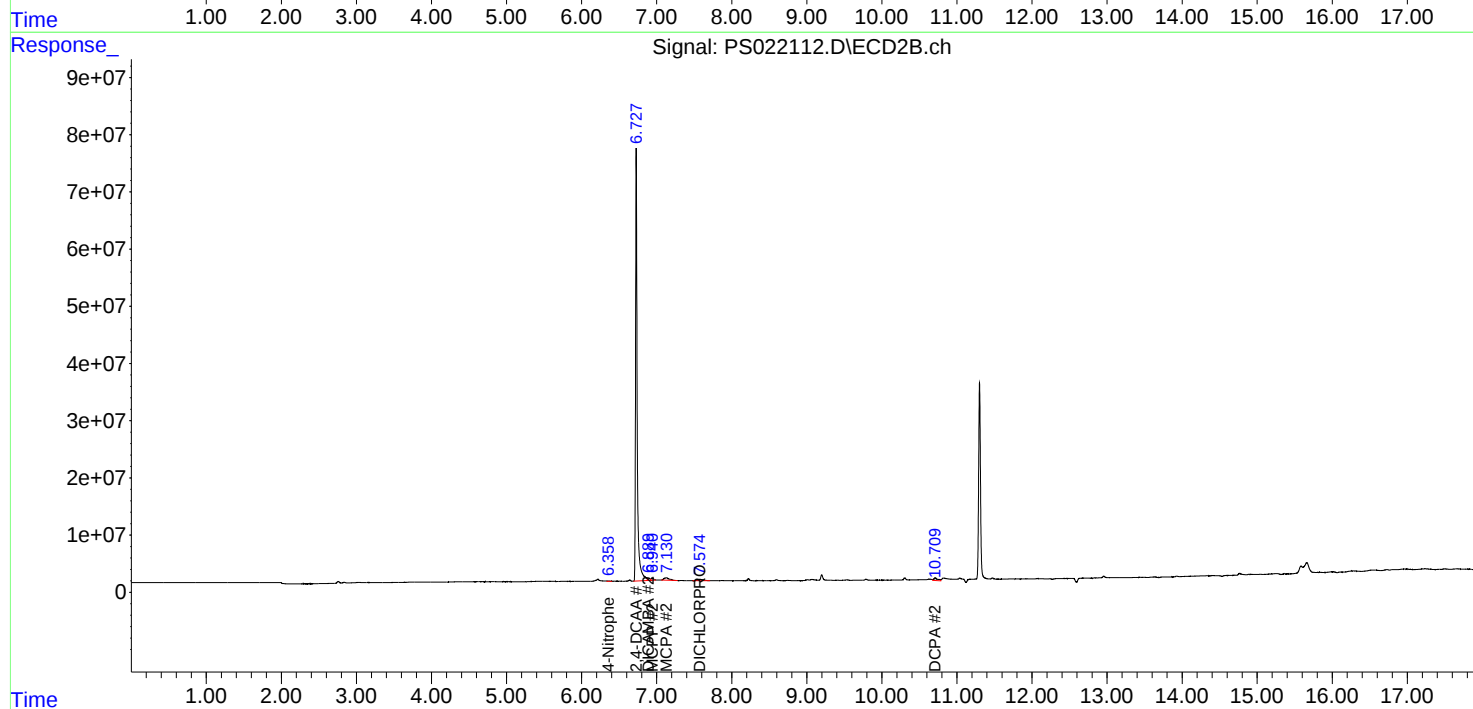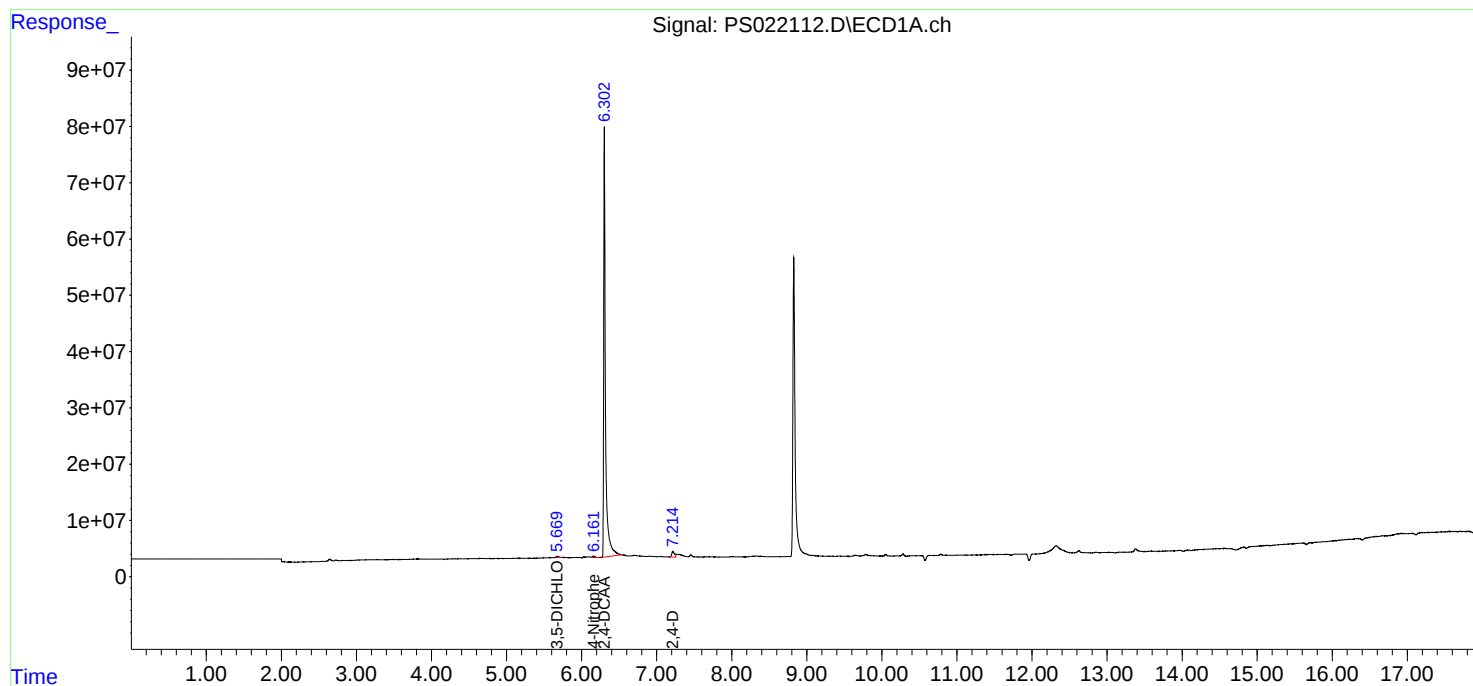


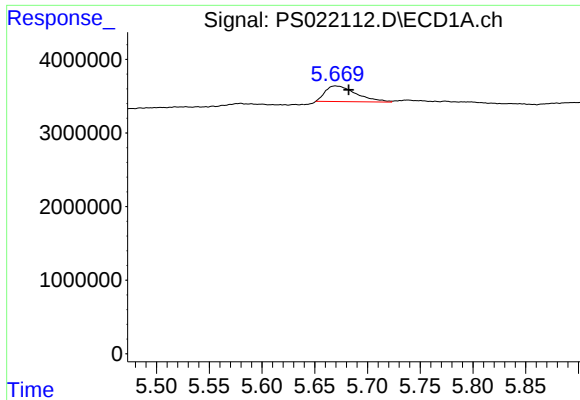

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.670 min
Delta R.T.: -0.013 min
Response: 4329042
Conc: 1.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

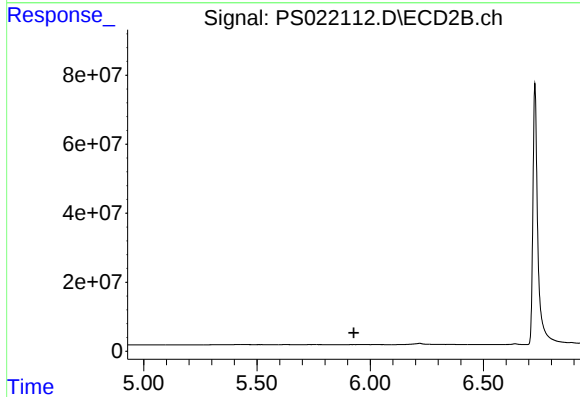


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

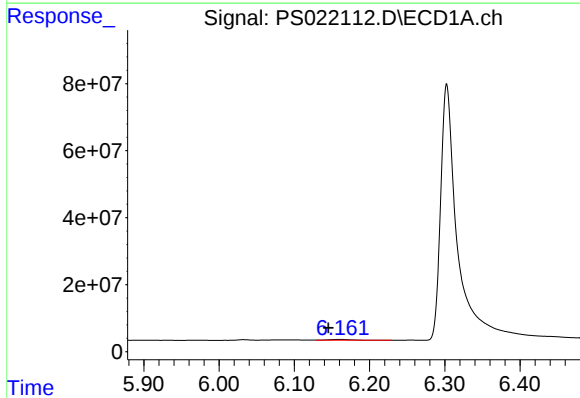


#3 4-Nitrophenol

R.T.: 6.161 min
Delta R.T.: 0.015 min
Response: 5712867
Conc: 4.24 ng/ml

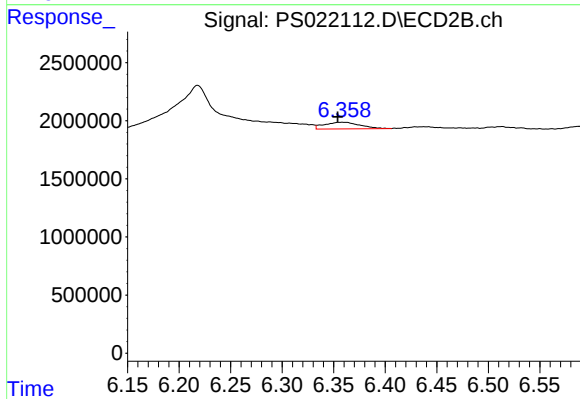

#3 4-Nitrophenol


R.T.: 6.359 min
Delta R.T.: 0.005 min
Response: 1376580
Conc: 1.03 ng/ml

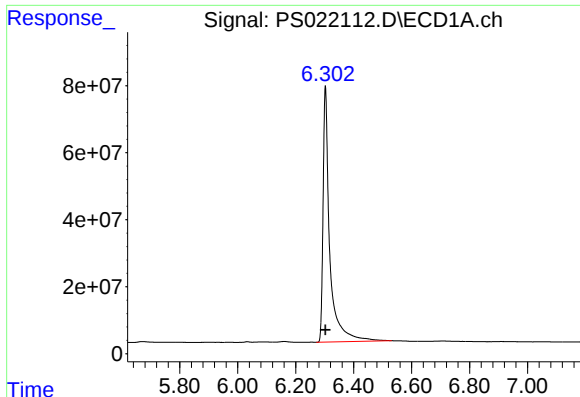

#4 2,4-DCAA


R.T.: 6.303 min
Delta R.T.: 0.000 min
Response: 1235192576
Conc: 541.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

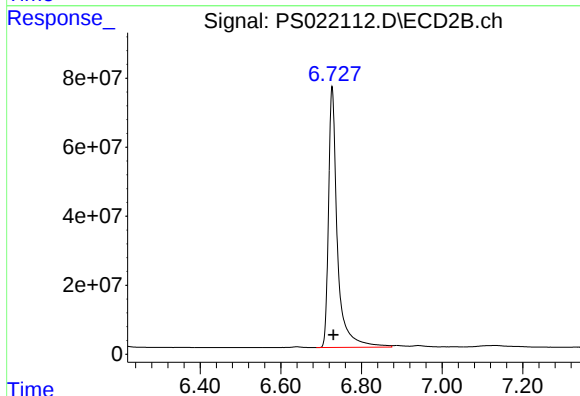


#4 2,4-DCAA

R.T.: 6.727 min
Delta R.T.: -0.003 min
Response: 1158457189
Conc: 572.29 ng/ml

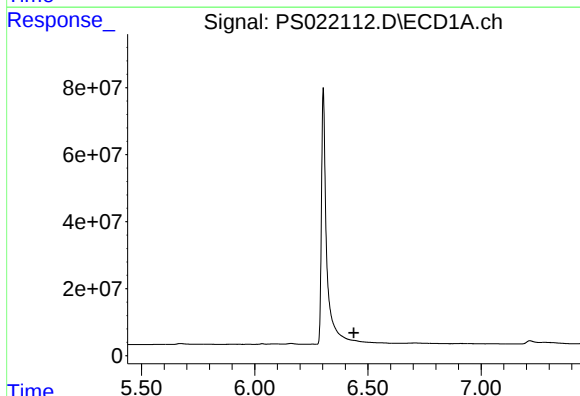


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.438 min
Response: 0
Conc: N.D.

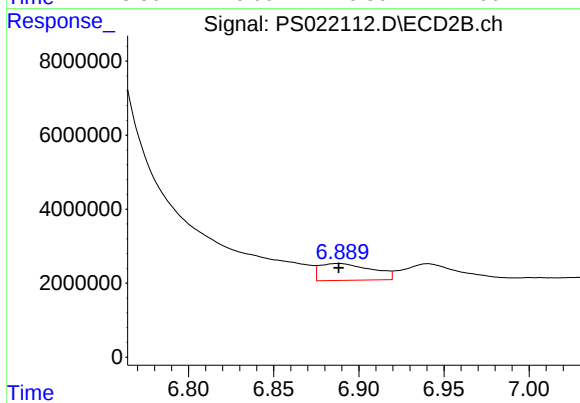

#5 DICAMBA


R.T.: 6.888 min
Delta R.T.: 0.000 min
Response: 9686919
Conc: 1.03 ng/ml

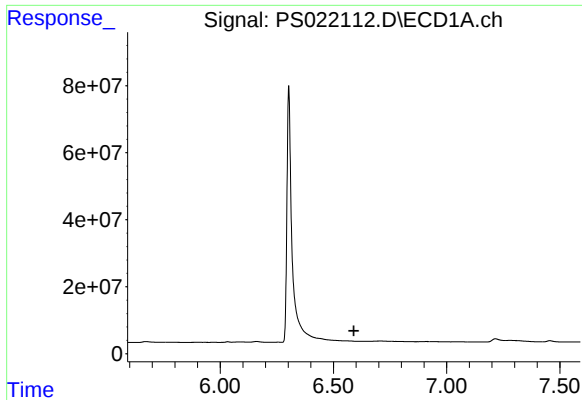

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.590 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

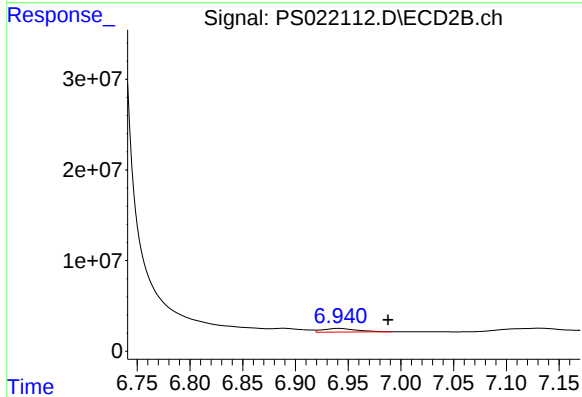


#6 MCPP

R.T.: 6.940 min
Delta R.T.: -0.047 min
Response: 8993005
Conc: 1.21 ug/ml

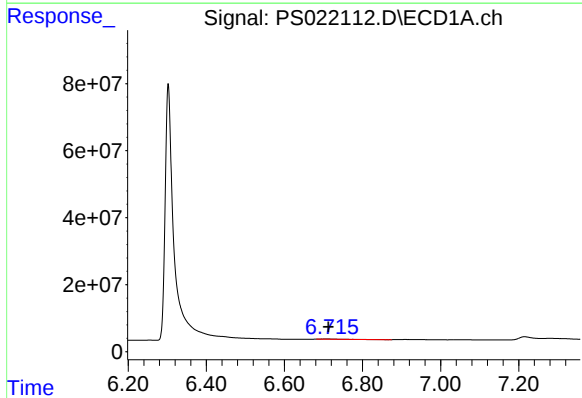


#7 MCPA

R.T.: 6.707 min
Delta R.T.: -0.005 min
Response: 764283
Conc: N.D.

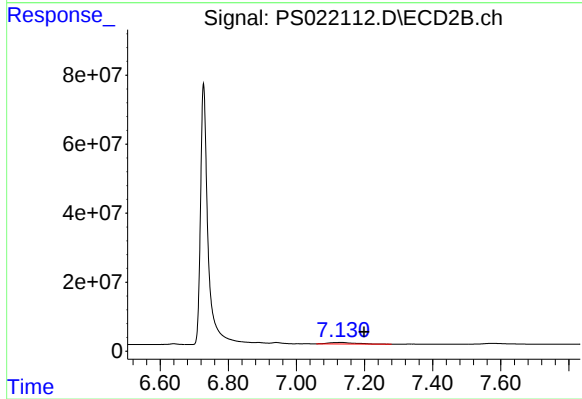

#7 MCPA


R.T.: 7.131 min
Delta R.T.: -0.067 min
Response: 21359408
Conc: 2.13 ug/ml

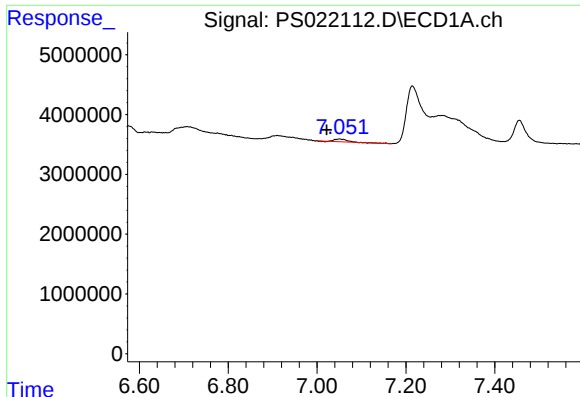

#8 DICHLORPROP


R.T.: 7.050 min
Delta R.T.: 0.028 min
Response: 993759
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

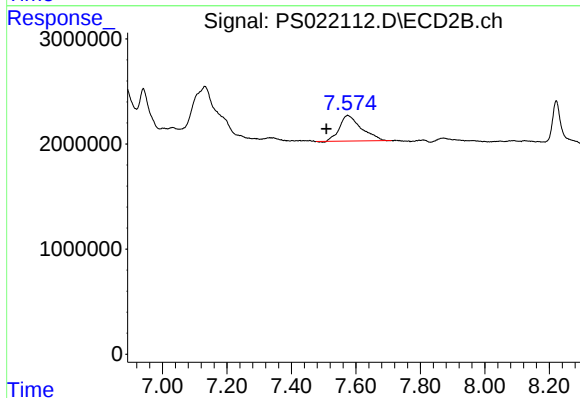


#8 DICHLORPROP

R.T.: 7.574 min
Delta R.T.: 0.065 min
Response: 11528385
Conc: 4.82 ng/ml

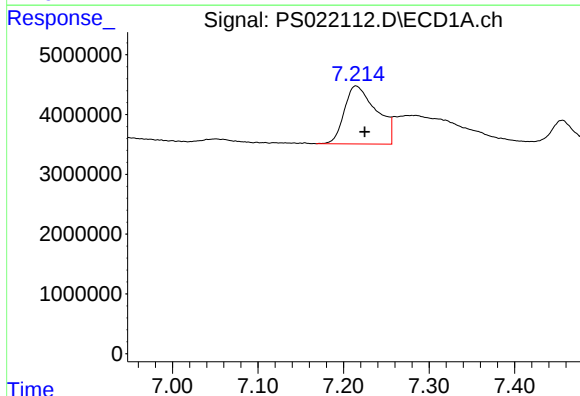


#9 2,4-D

R.T.: 7.215 min
Delta R.T.: -0.010 min
Response: 25342529
Conc: 8.43 ng/ml

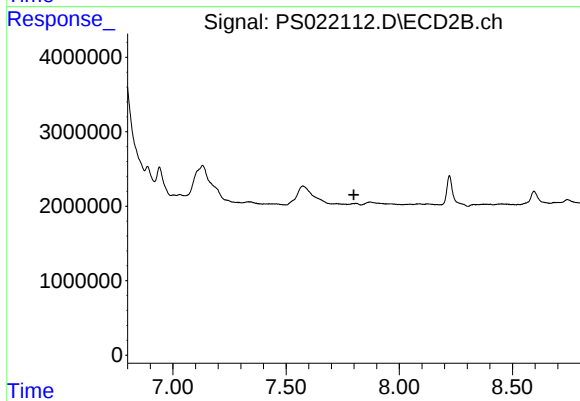

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.799 min
Response: 0
Conc: N.D.

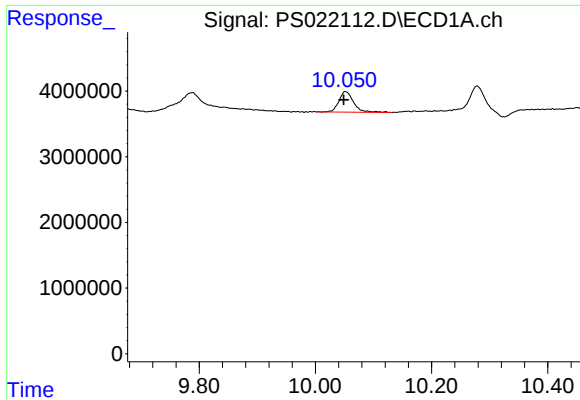

#16 DCPA

R.T.: 10.052 min
Delta R.T.: 0.004 min
Response: 5503680
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

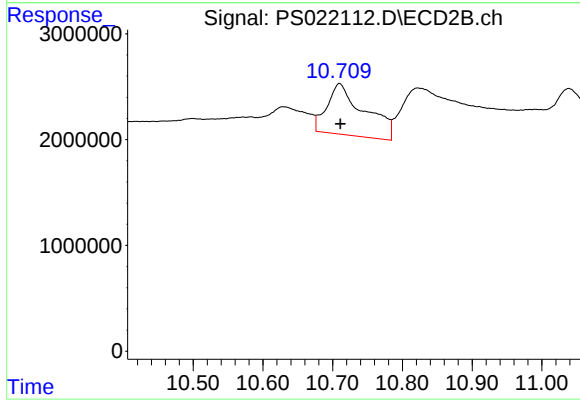

#16 DCPA

R.T.: 10.710 min
Delta R.T.: -0.001 min
Response: 18033370
Conc: 1.17 ng/ml