

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021023\
 Data File : PS022120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2023 22:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 04:06:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020223.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 03 10:03:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.303	6.728	1245.8E6	1157.3E6	546.572	571.739
Target Compounds							
1) T	Dalapon	2.414	0.000	401388	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.669	0.000	3946902	0	1.146	N.D. #
3) T	4-Nitroph...	6.158	6.355	6461739	1400210	4.801	1.049 #
5) T	DICAMBA	0.000	6.888	0	7786897	N.D.	<MDL
6) T	MCP	0.000	6.940f	0	8721469	N.D.	1.169
7) T	MCPA	6.708	7.132f	4958647	19357385	<MDL	1.927 #
8) T	DICHLORPROP	7.054	7.567f	777676	19088194	<MDL	7.978 #
9) T	2,4-D	7.214	0.000	26077459	0	8.674	N.D. #
10) T	Pentachlo...	7.456	8.222	10289631	7076031	<MDL	<MDL #
11) T	2,4,5-TP ...	7.949	8.594	404249	3910045	<MDL	<MDL #
12) T	2,4,5-T	8.251	9.000f	3560906	3449639	<MDL	<MDL #
14) T	DINOSEB	9.785	9.789	8475079	3192782	<MDL	<MDL #
15) T	Picloram	9.645	10.710f	5778041	20109415	<MDL	1.108 #
16) T	DCPA	10.052	10.710	4864117	20109415	<MDL	1.307 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021023\
Data File : PS022120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2023 22:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 04:06:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020223.M
Quant Title : 8080.M
QLast Update : Fri Feb 03 10:03:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

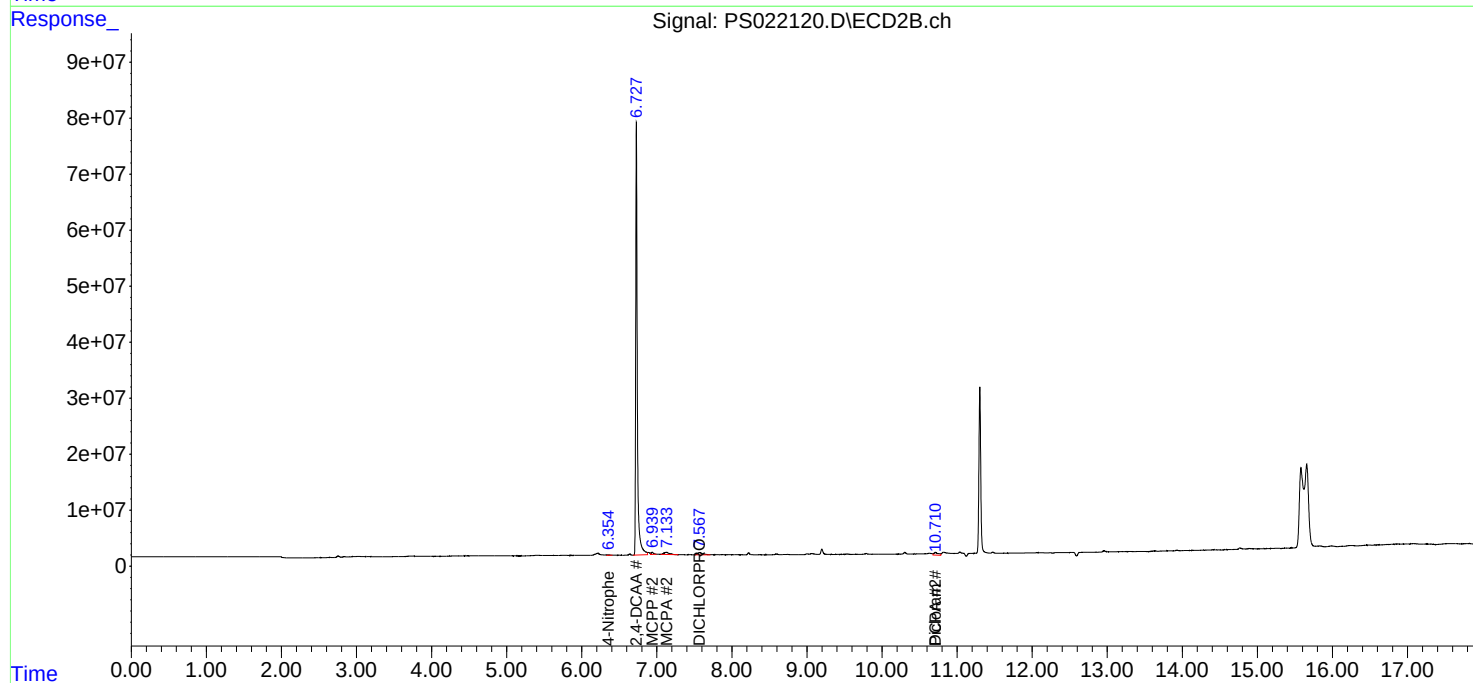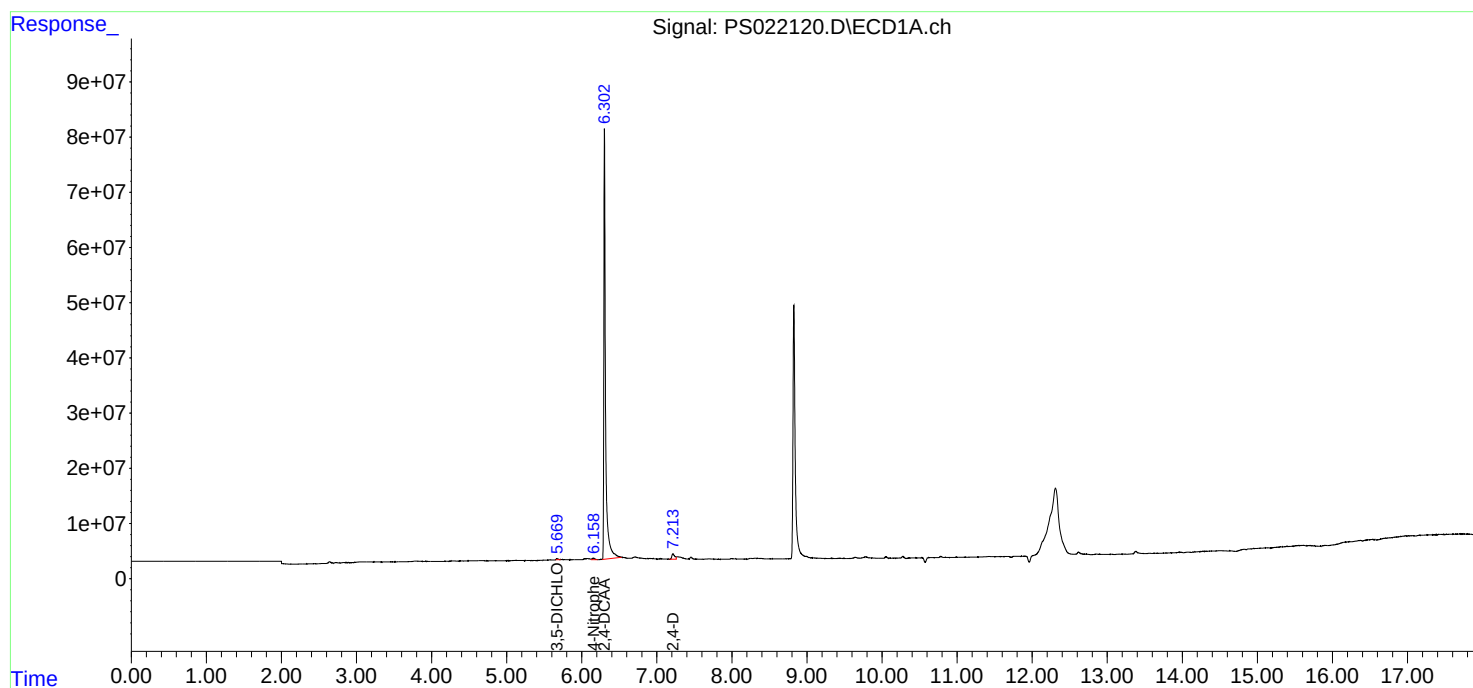


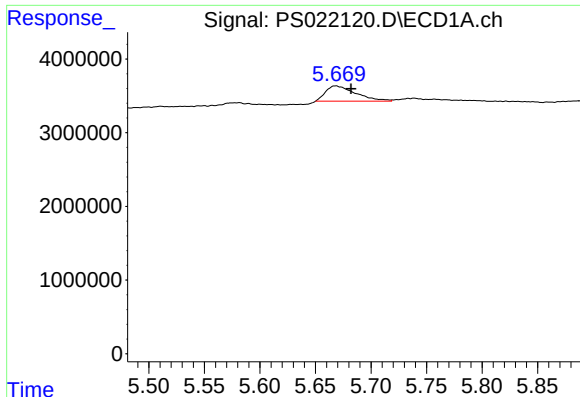

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.669 min
Delta R.T.: -0.013 min
Response: 3946902
Conc: 1.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

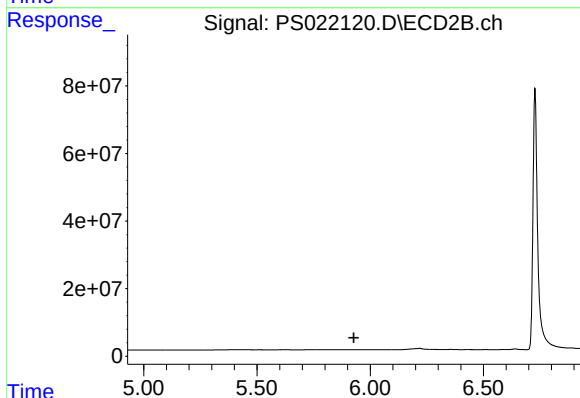


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

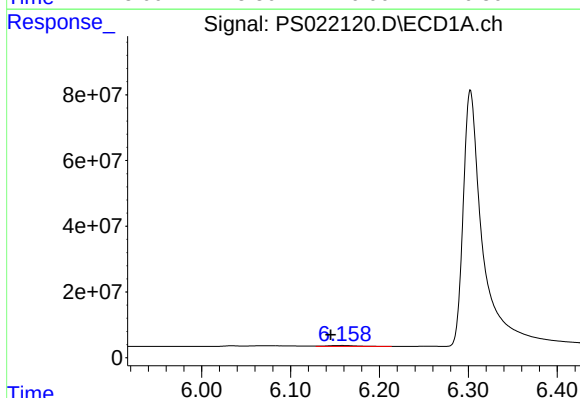


#3 4-Nitrophenol

R.T.: 6.158 min
Delta R.T.: 0.013 min
Response: 6461739
Conc: 4.80 ng/ml

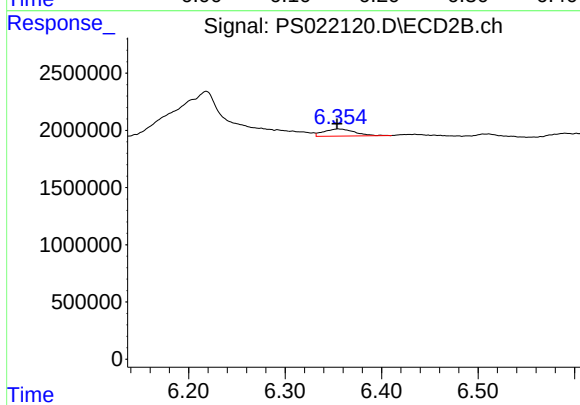

#3 4-Nitrophenol


R.T.: 6.355 min
Delta R.T.: 0.002 min
Response: 1400210
Conc: 1.05 ng/ml

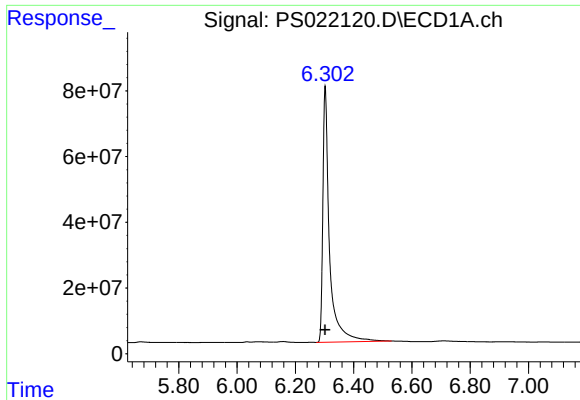

#4 2,4-DCAA


R.T.: 6.303 min
Delta R.T.: 0.000 min
Response: 1245836846
Conc: 546.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

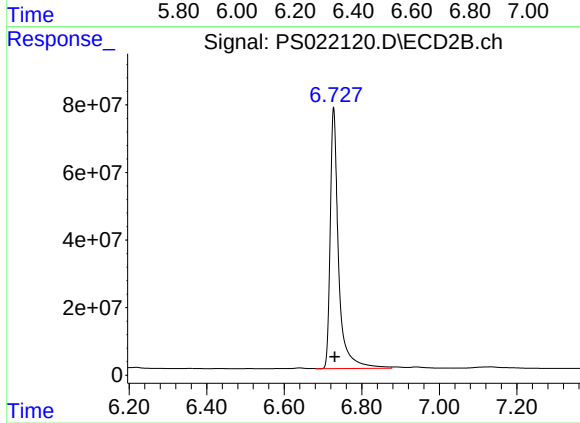


#4 2,4-DCAA

R.T.: 6.728 min
Delta R.T.: -0.003 min
Response: 1157337045
Conc: 571.74 ng/ml

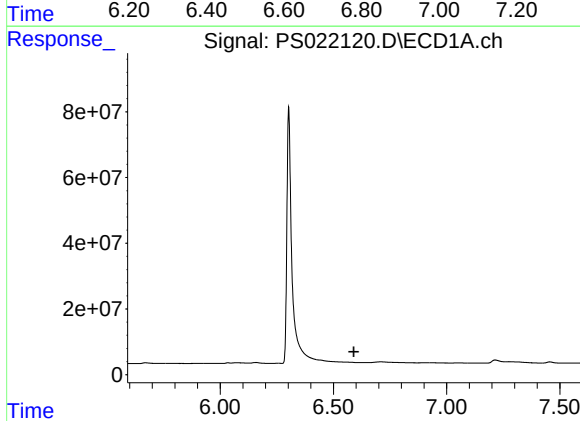


#6 MCP

R.T.: 0.000 min
Exp R.T. : 6.590 min
Response: 0
Conc: N.D.

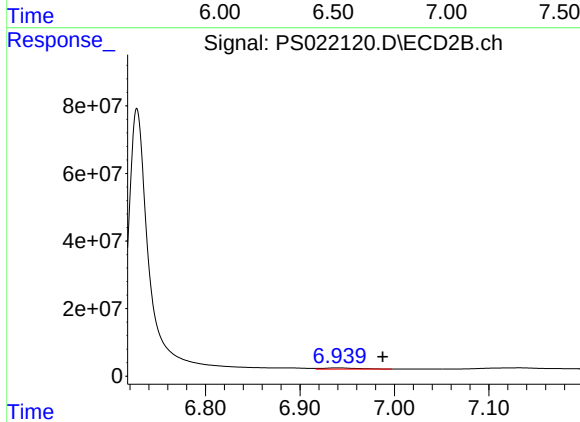

#6 MCP


R.T.: 6.940 min
Delta R.T.: -0.048 min
Response: 8721469
Conc: 1.17 ug/ml

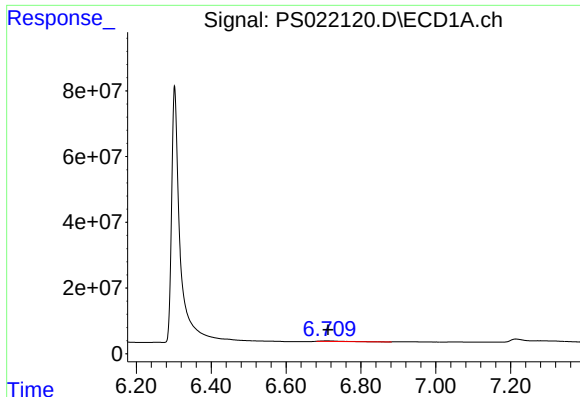

#7 MCPA


R.T.: 6.708 min
Delta R.T.: -0.005 min
Response: 4958647
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

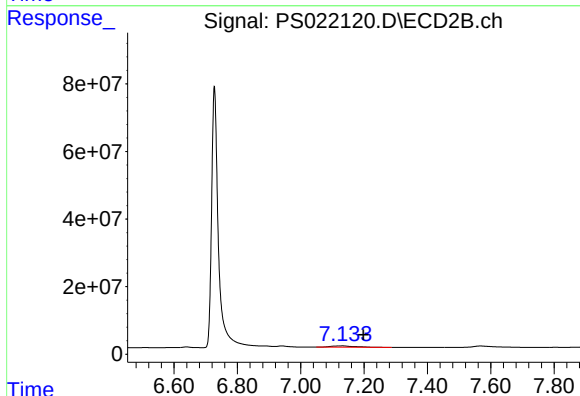


#7 MCPA

R.T.: 7.132 min
Delta R.T.: -0.066 min
Response: 19357385
Conc: 1.93 ug/ml

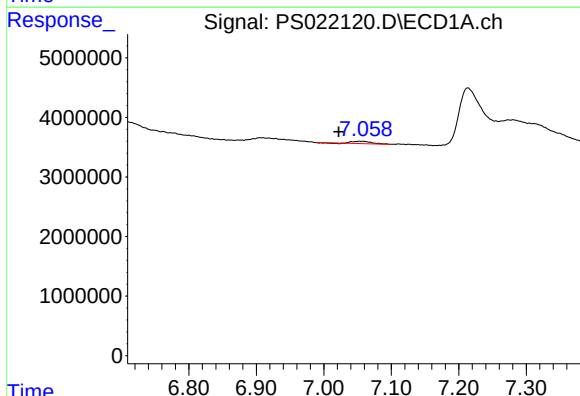


#8 DICHLORPROP

R.T.: 7.054 min
Delta R.T.: 0.032 min
Response: 777676
Conc: N.D.

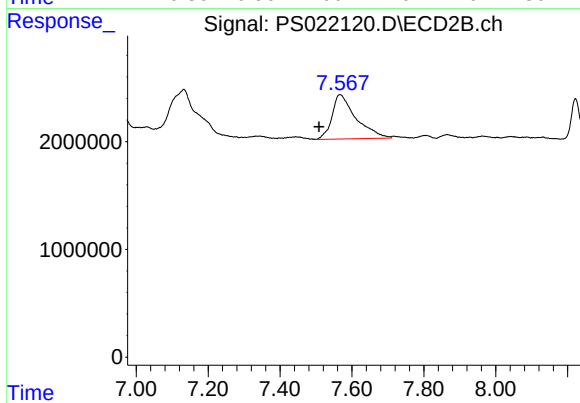

#8 DICHLORPROP


R.T.: 7.567 min
Delta R.T.: 0.058 min
Response: 19088194
Conc: 7.98 ng/ml

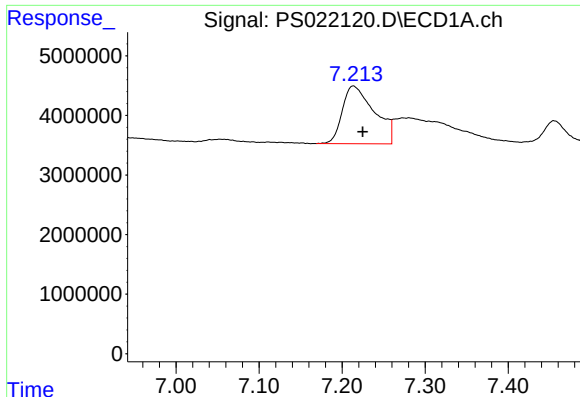

#9 2,4-D


R.T.: 7.214 min
Delta R.T.: -0.011 min
Response: 26077459
Conc: 8.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

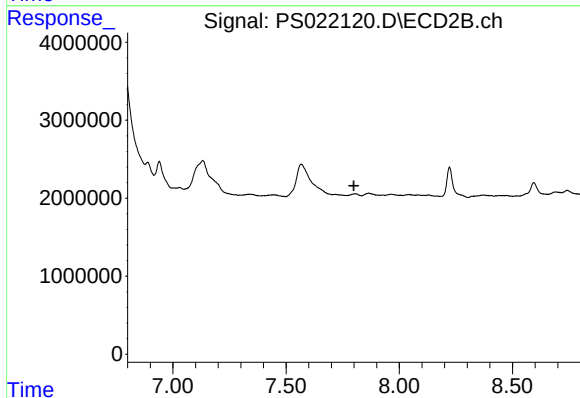


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.799 min
Response: 0
Conc: N.D.

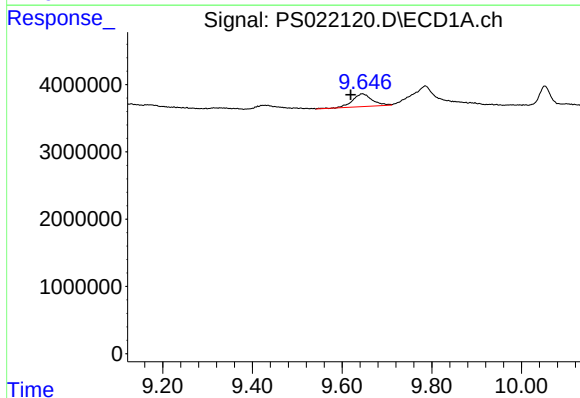


#15 Picloram

R.T.: 9.645 min
Delta R.T.: 0.026 min
Response: 5778041
Conc: N.D.

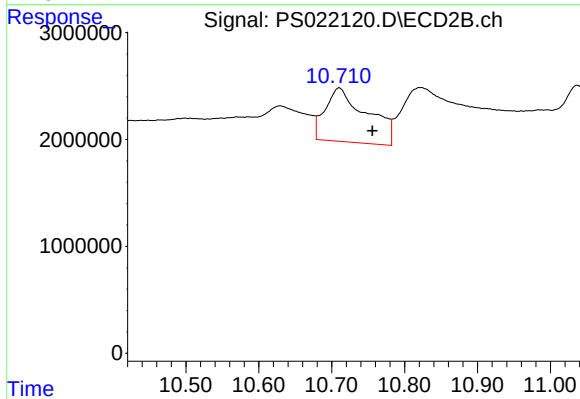

#15 Picloram


R.T.: 10.710 min
Delta R.T.: -0.046 min
Response: 20109415
Conc: 1.11 ng/ml

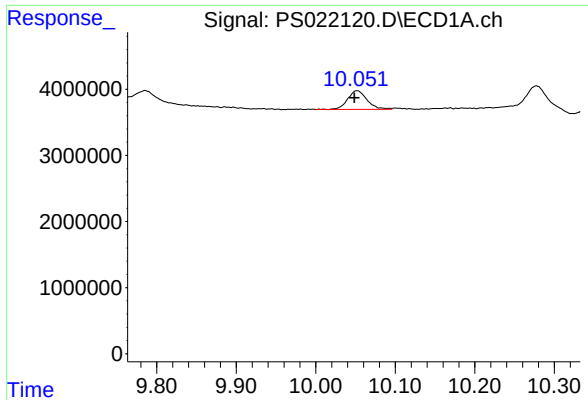

#16 DCPA

R.T.: 10.052 min
Delta R.T.: 0.003 min
Response: 4864117
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

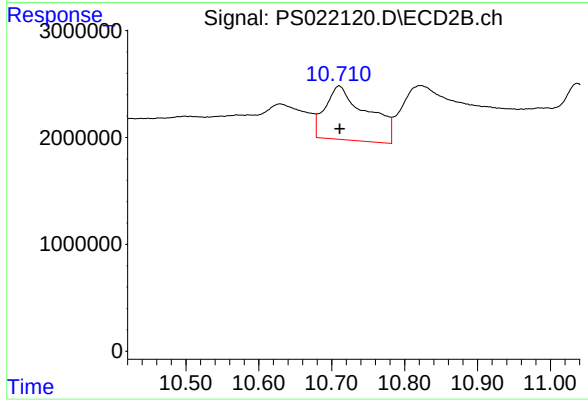

#16 DCPA

R.T.: 10.710 min
Delta R.T.: 0.000 min
Response: 20109415
Conc: 1.31 ng/ml