

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
 Data File : PS003101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2019 12:18
 Operator : EI\SJ
 Sample : PB116923TB
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB116923TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 22:07:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.276	10.769	101.8E6	234.5E6	268.230	548.455 #
Target Compounds							
3) T	4-Nitroph...	0.000	9.988	0	36881853	N.D.	176.449 #
6) T	MCP	11.951	0.000	7988525	0	6.668	N.D. #
10) T	Pentachlo...	0.000	13.268	0	2233173	N.D.	0.361 #
11) T	2,4,5-TP ...	14.464	0.000	11352027	0	4.508	N.D. #
12) T	2,4,5-T	0.000	14.375	0	8028465	N.D.	4.196 #
14) T	DINOSEB	0.000	15.479	0	5011977	N.D.	2.859 #
15) T	Picloram	16.789	16.694	10331887	47251006	3.266	15.717 #
16) T	DCPA	0.000	16.694	0	47251006	N.D.	15.254 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
Data File : PS003101.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2019 12:18
Operator : EI\SJ
Sample : PB116923TB
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB116923TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 22:07:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

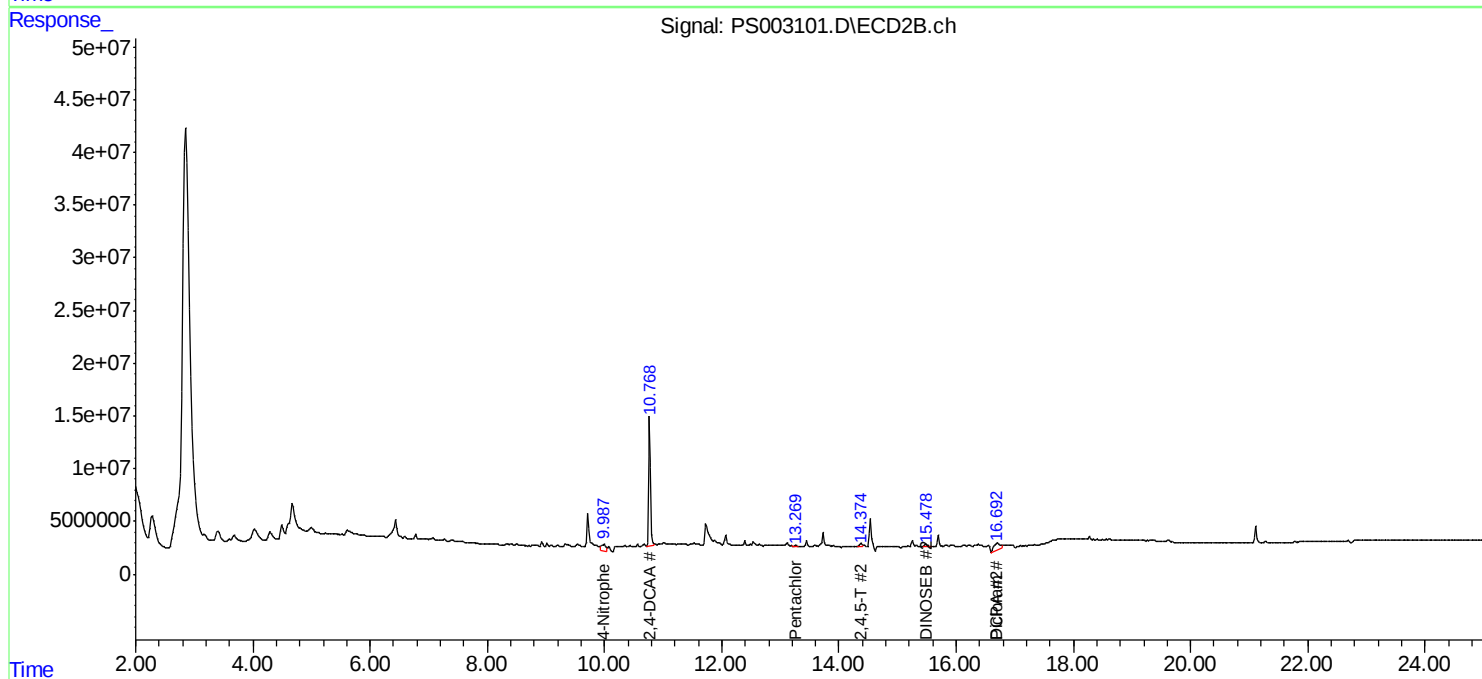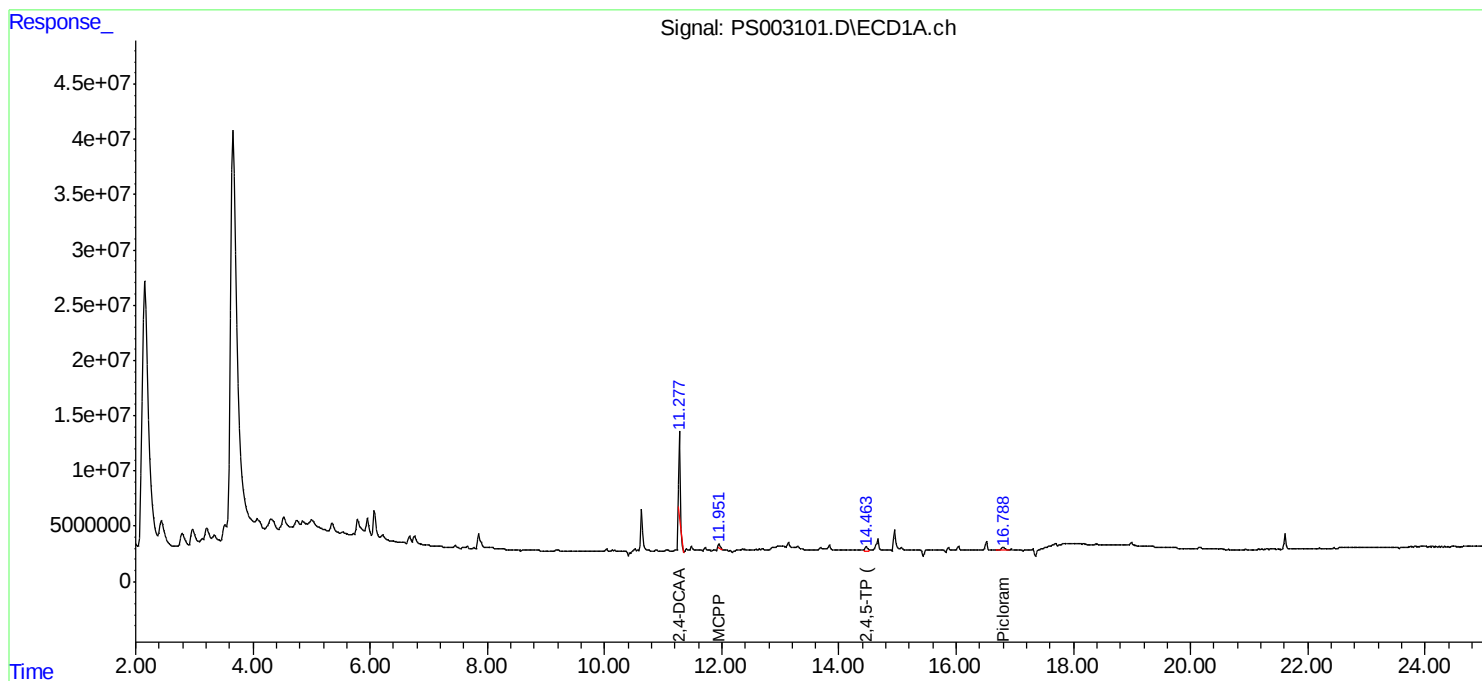


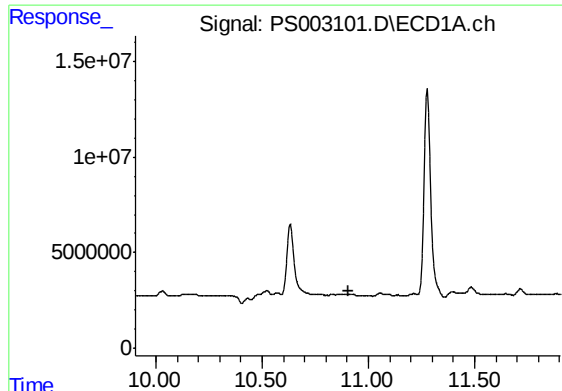

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116923TB

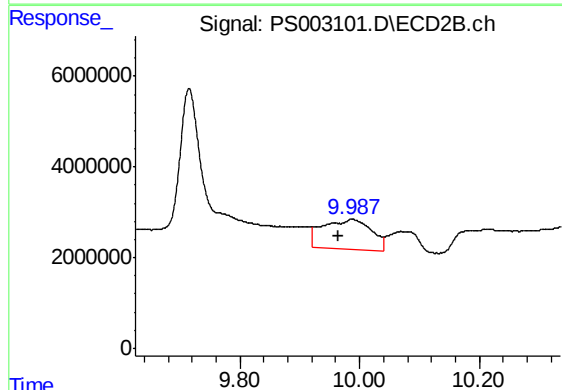


#3 4-Nitrophenol

R.T.: 9.988 min
Delta R.T.: 0.022 min
Response: 36881853
Conc: 176.45 ng/ml

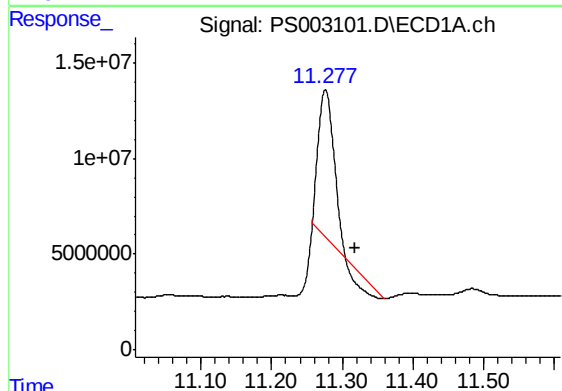


#4 2,4-DCAA

R.T.: 11.276 min
Delta R.T.: -0.042 min
Response: 101830926
Conc: 268.23 ng/ml

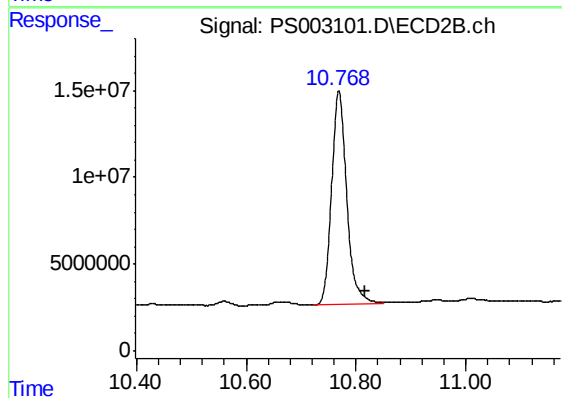

#4 2,4-DCAA


R.T.: 10.769 min
Delta R.T.: -0.048 min
Response: 234489643
Conc: 548.46 ng/ml

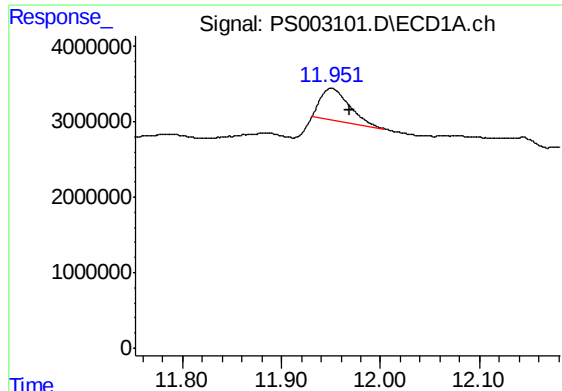

#6 MCP


R.T.: 11.951 min
Delta R.T.: -0.019 min
Response: 7988525
Conc: 6.67 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB116923TB

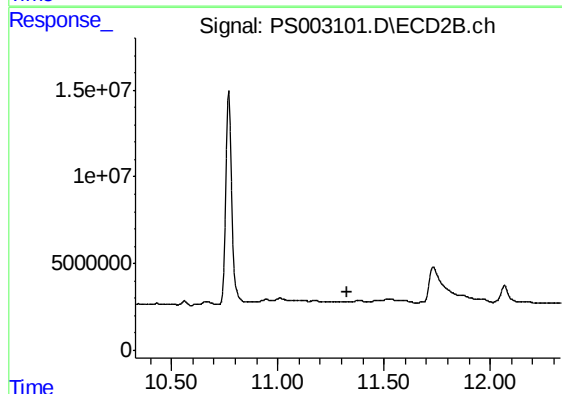


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

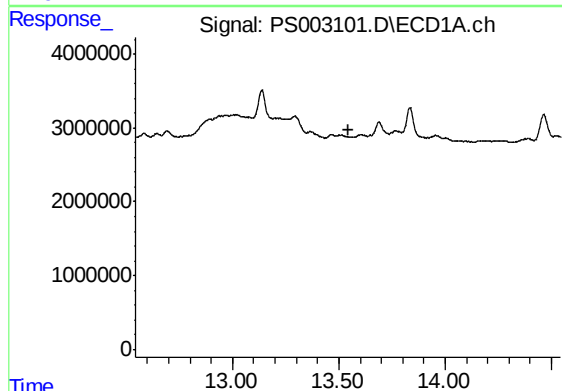


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.543 min
Response: 0
Conc: N.D.

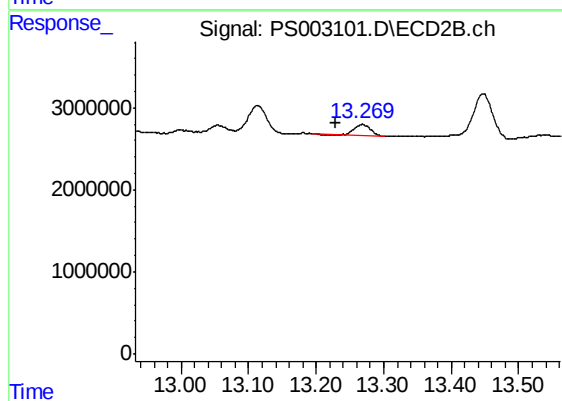

#10 Pentachlorophenol


R.T.: 13.268 min
Delta R.T.: 0.039 min
Response: 2233173
Conc: 0.36 ng/ml

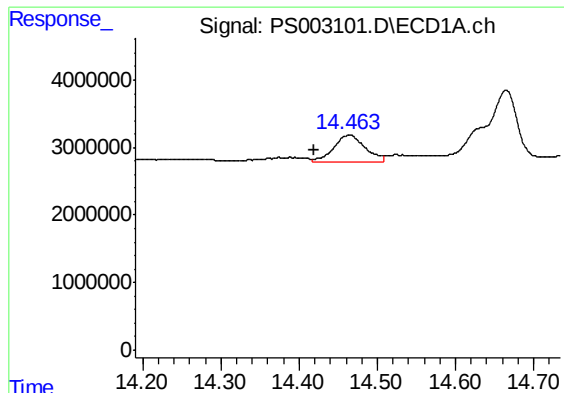

#11 2,4,5-TP (SILVEX)


R.T.: 14.464 min
Delta R.T.: 0.045 min
Response: 11352027
Conc: 4.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116923TB

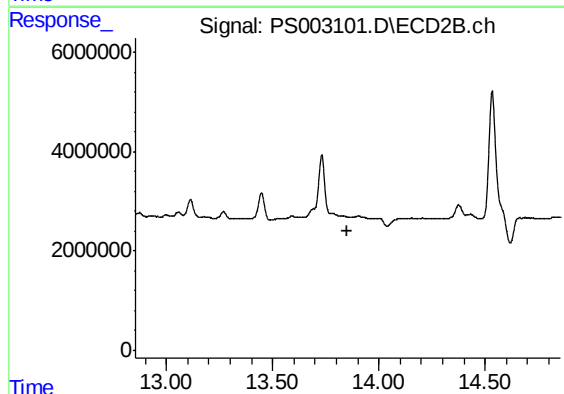


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

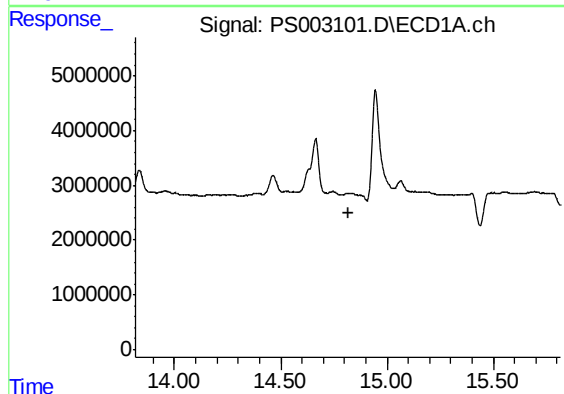


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

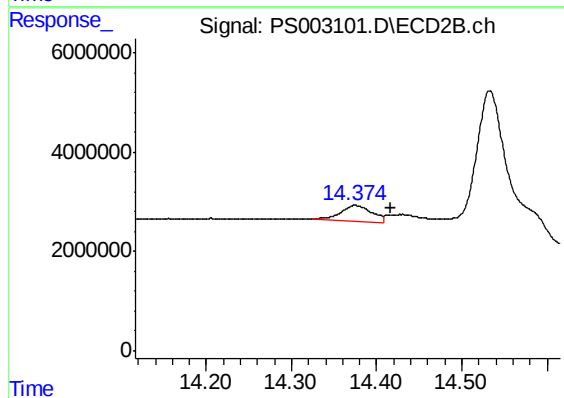

#12 2,4,5-T


R.T.: 14.375 min
Delta R.T.: -0.042 min
Response: 8028465
Conc: 4.20 ng/ml

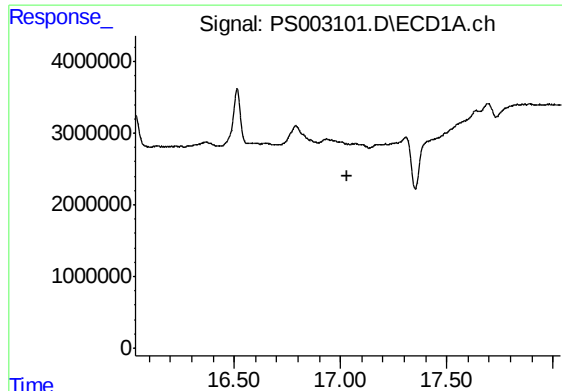

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116923TB

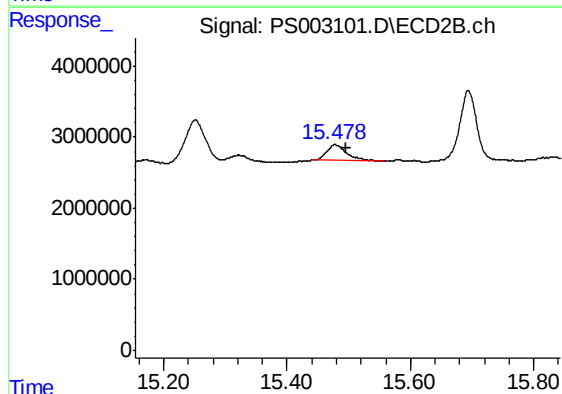


#14 DINOSEB

R.T.: 15.479 min
Delta R.T.: -0.016 min
Response: 5011977
Conc: 2.86 ng/ml

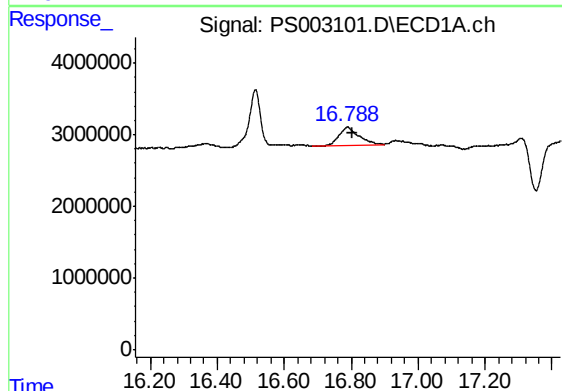


#15 Picloram

R.T.: 16.789 min
Delta R.T.: -0.017 min
Response: 10331887
Conc: 3.27 ng/ml

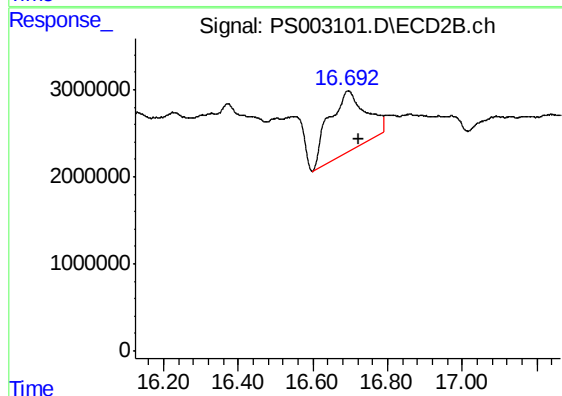

#15 Picloram


R.T.: 16.694 min
Delta R.T.: -0.030 min
Response: 47251006
Conc: 15.72 ng/ml

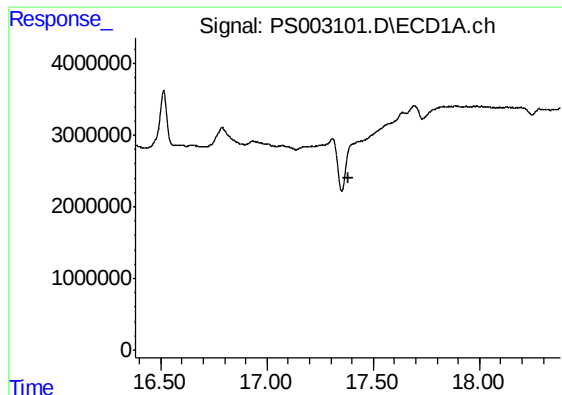

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116923TB

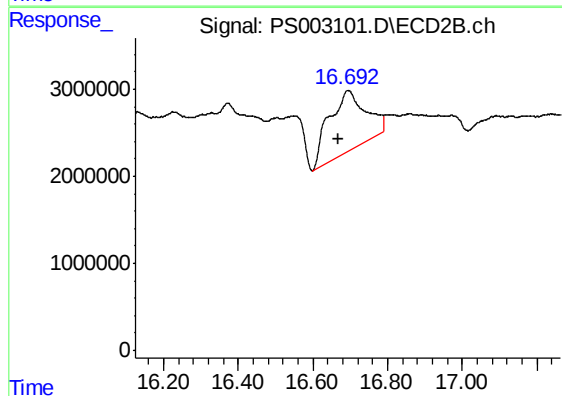

#16 DCPA

R.T.: 16.694 min
Delta R.T.: 0.024 min
Response: 47251006
Conc: 15.25 ng/ml