

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
 Data File : PS003110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2019 21:27
 Operator : EI\SJ
 Sample : K1442-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 22:09:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.284	10.784	15048795	23832641	39.640	55.743 #
Target Compounds							
1) T	Dalapon	0.000	2.287	0	49713504	N.D.	92.763 #
2) T	3,5-DICHL...	0.000	8.949	0	3210799	N.D.	5.697 #
5) T	DICAMBA	11.645	11.138	2359235	2901973	1.472	1.829
7) T	MCPA	0.000	11.721	0	74896654	N.D.	47.612 #
8) T	DICHLORPROP	12.823	12.217	4113090	9276363	10.724	24.262 #
13) T	2,4-DB	15.610	15.010	1745122	1523751	6.675	5.999
14) T	DINOSEB	0.000	15.487	0	2656727	N.D.	1.516 #
15) T	Picloram	0.000	16.740	0	10903184	N.D.	3.627 #
16) T	DCPA	17.432	16.696	-3023659	21007815	N.D.	6.782



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
Data File : PS003110.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2019 21:27
Operator : EI\SJ
Sample : K1442-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 22:09:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

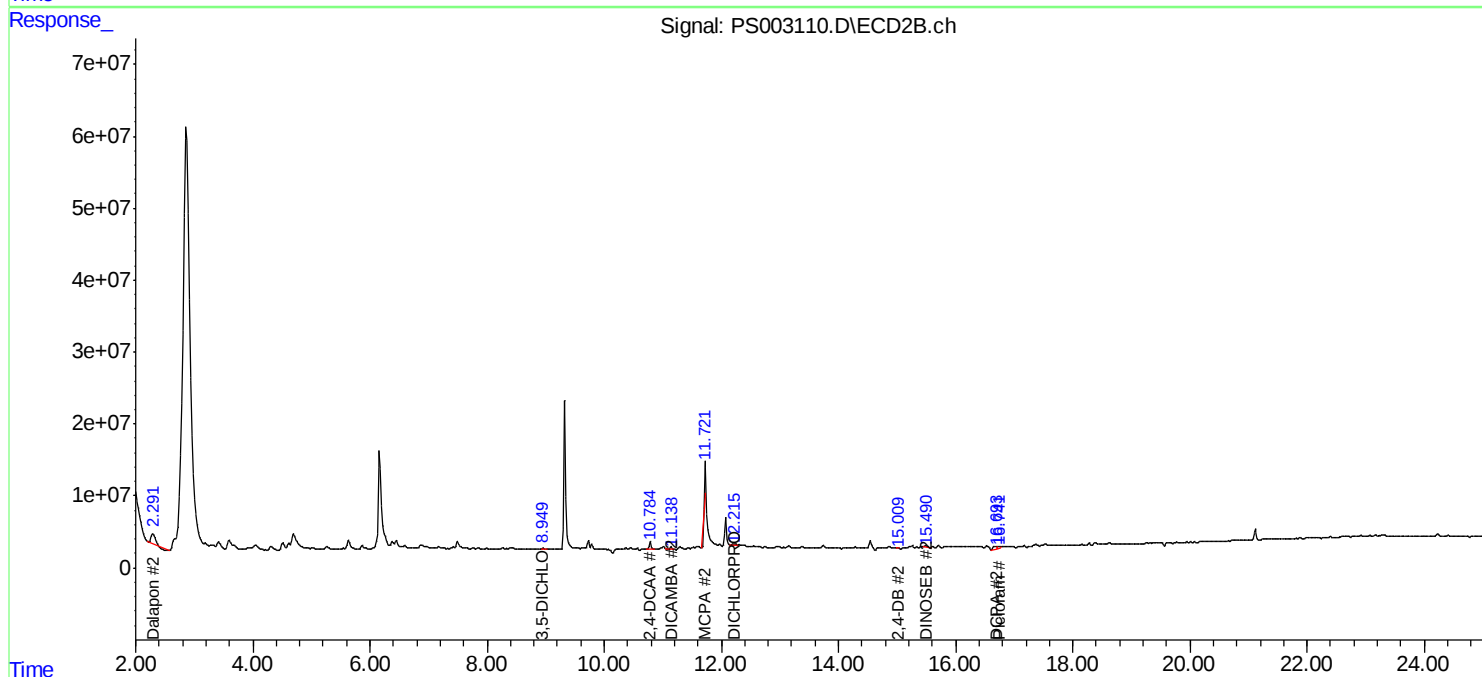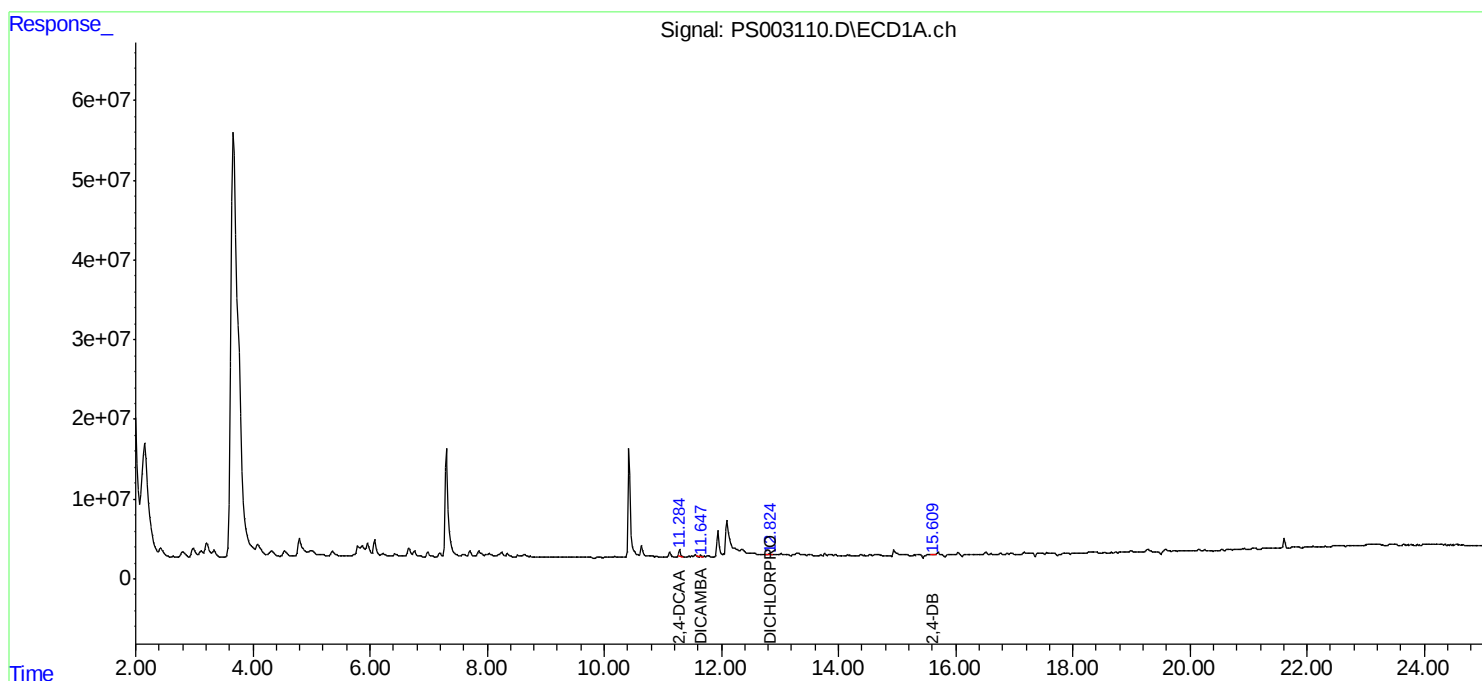


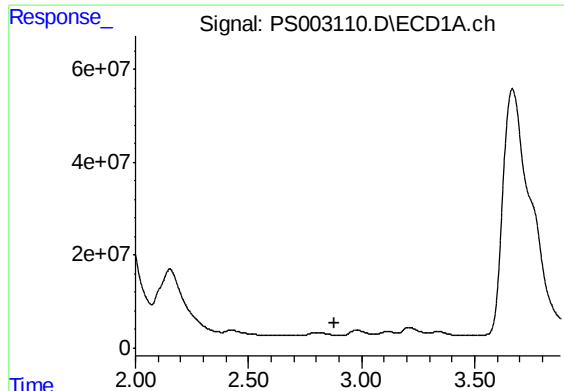

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-10

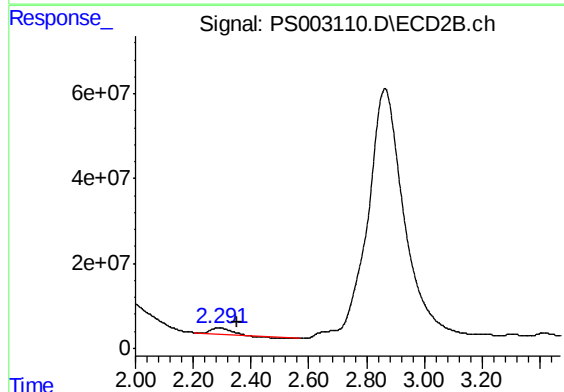


#1 Dalapon

R.T.: 2.287 min
Delta R.T.: -0.063 min
Response: 49713504
Conc: 92.76 ng/ml

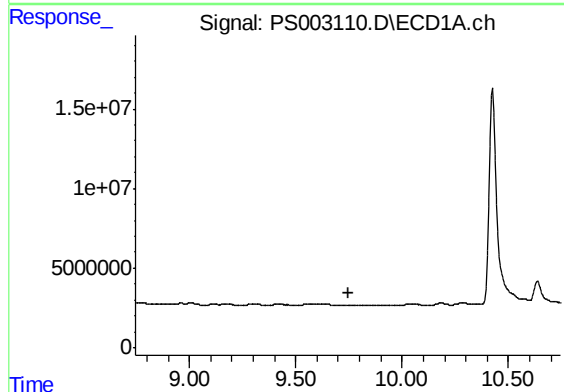


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

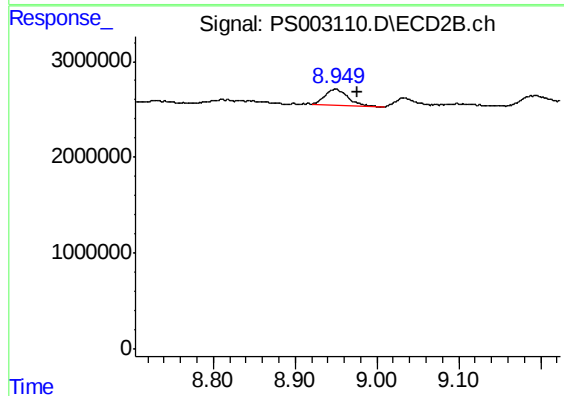

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.949 min
Delta R.T.: -0.027 min
Response: 3210799
Conc: 5.70 ng/ml

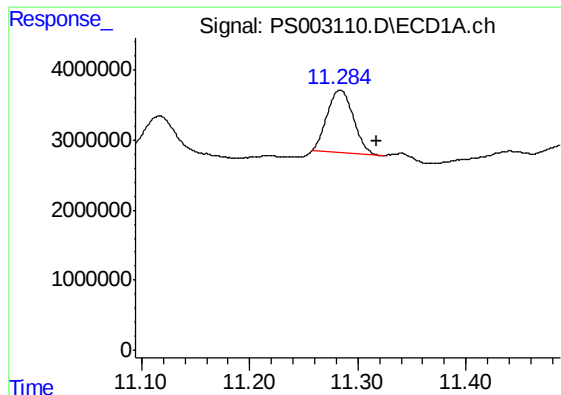

#4 2,4-DCAA


R.T.: 11.284 min
Delta R.T.: -0.034 min
Response: 15048795
Conc: 39.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-10

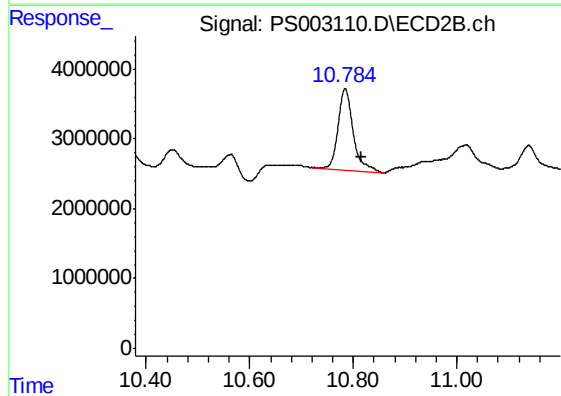


#4 2,4-DCAA

R.T.: 10.784 min
Delta R.T.: -0.032 min
Response: 23832641
Conc: 55.74 ng/ml

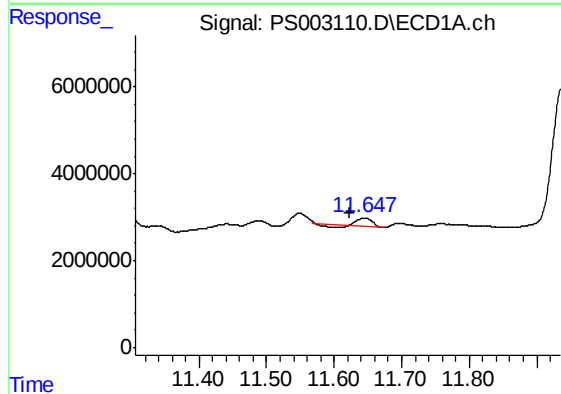


#5 DICAMBA

R.T.: 11.645 min
Delta R.T.: 0.021 min
Response: 2359235
Conc: 1.47 ng/ml

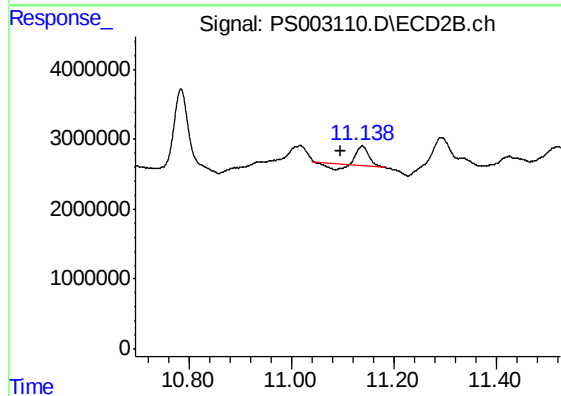

#5 DICAMBA


R.T.: 11.138 min
Delta R.T.: 0.041 min
Response: 2901973
Conc: 1.83 ng/ml

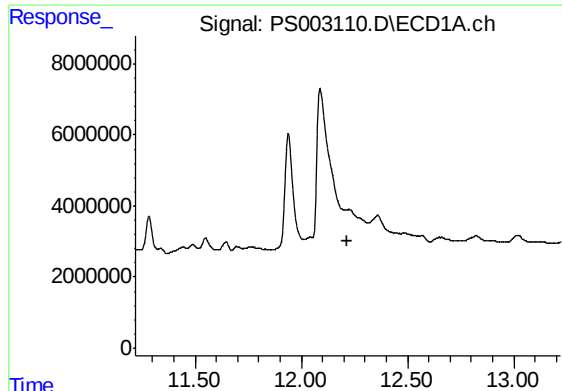

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-10

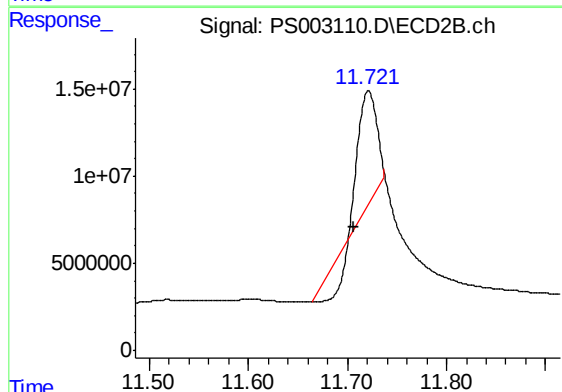


#7 MCPA

R.T.: 11.721 min
Delta R.T.: 0.015 min
Response: 74896654
Conc: 47.61 ug/ml

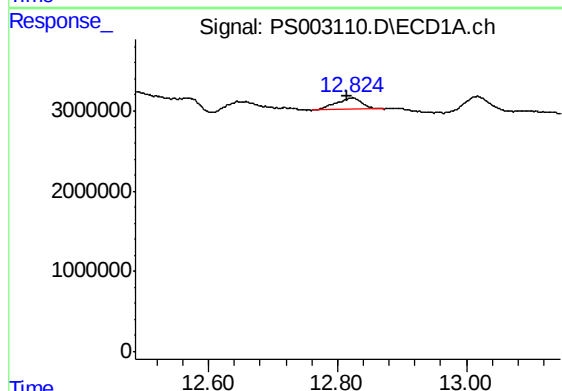


#8 DICHLORPROP

R.T.: 12.823 min
Delta R.T.: 0.009 min
Response: 4113090
Conc: 10.72 ng/ml

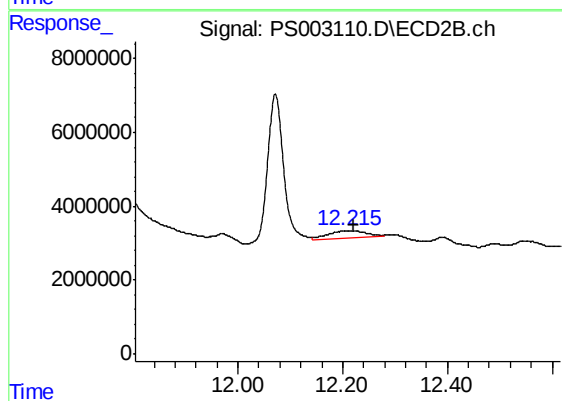

#8 DICHLORPROP


R.T.: 12.217 min
Delta R.T.: -0.005 min
Response: 9276363
Conc: 24.26 ng/ml

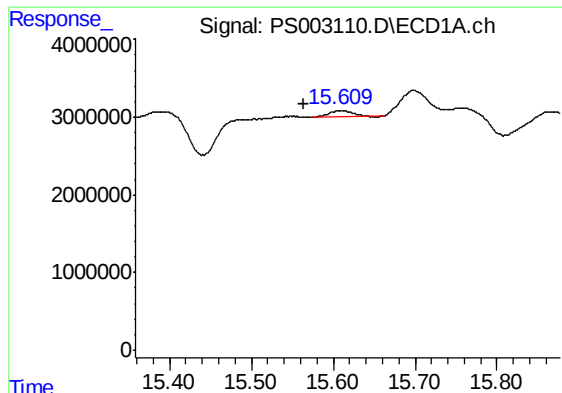

#13 2,4-DB


R.T.: 15.610 min
Delta R.T.: 0.045 min
Response: 1745122
Conc: 6.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-10

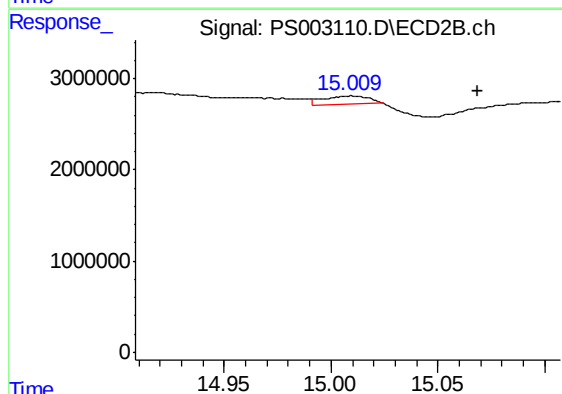


#13 2,4-DB

R.T.: 15.010 min
Delta R.T.: -0.059 min
Response: 1523751
Conc: 6.00 ng/ml

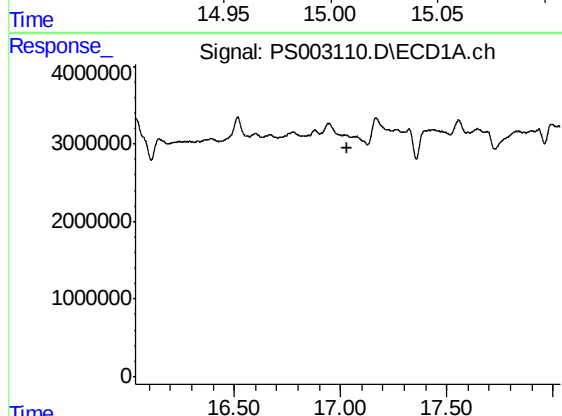


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

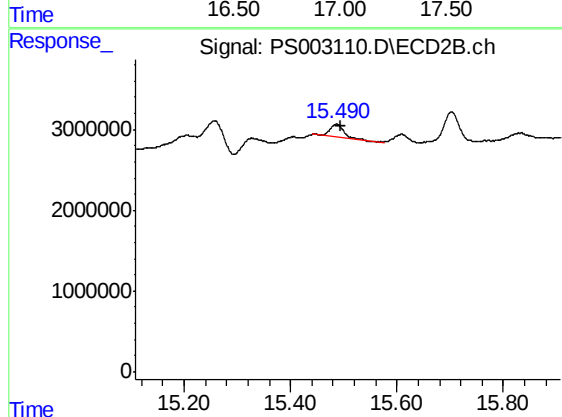

#14 DINOSEB


R.T.: 15.487 min
Delta R.T.: -0.008 min
Response: 2656727
Conc: 1.52 ng/ml

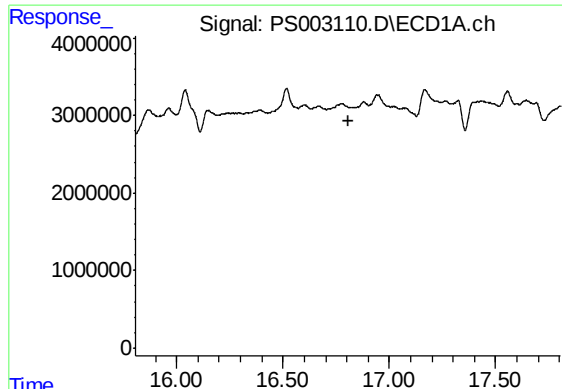

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-10

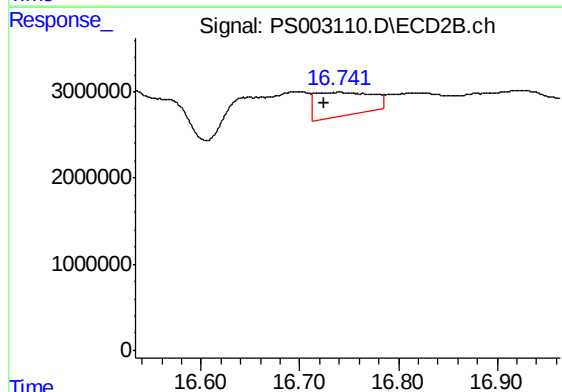


#15 Picloram

R.T.: 16.740 min
Delta R.T.: 0.016 min
Response: 10903184
Conc: 3.63 ng/ml

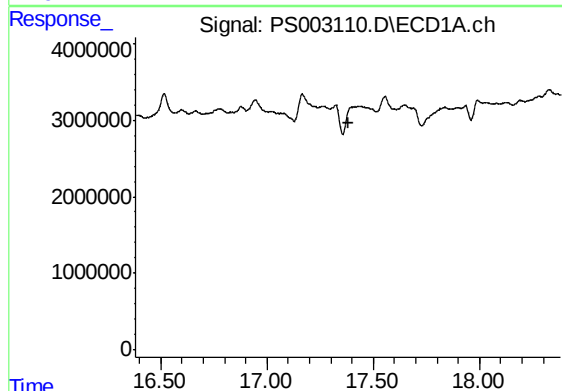

#16 DCPA

R.T.: 17.432 min
Delta R.T.: 0.050 min
Response: -3023659
Conc: N.D.

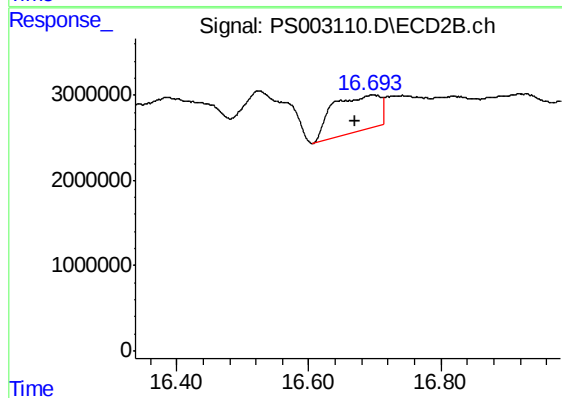

#16 DCPA

R.T.: 16.696 min
Delta R.T.: 0.026 min
Response: 21007815
Conc: 6.78 ng/ml