

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
 Data File : PS003115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 00:02
 Operator : EI\SJ
 Sample : PB116998TB
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB116998TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 00:33:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.297	10.799	103.2E6	102.6E6	271.926	239.957
Target Compounds							
1) T	Dalapon	0.000	2.308	0	55219229	N.D.	103.036 #
2) T	3,5-DICHL...	0.000	8.965	0	5834105	N.D.	10.352 #
6) T	MCP	11.959	0.000	45524571	0	37.997	N.D. #
8) T	DICHLORPROP	0.000	12.266	0	8457441	N.D.	22.120 #
12) T	2,4,5-T	0.000	14.405	0	2974215	N.D.	1.554 #
14) T	DINOSEB	0.000	15.501	0	2790618	N.D.	1.592 #
15) T	Picloram	16.791	16.714	5918070	22206755	1.871	7.386 #
16) T	DCPA	17.420	16.714	-2462628	22206755	N.D.	7.169



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
Data File : PS003115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 00:02
Operator : EI\SJ
Sample : PB116998TB
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB116998TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 00:33:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

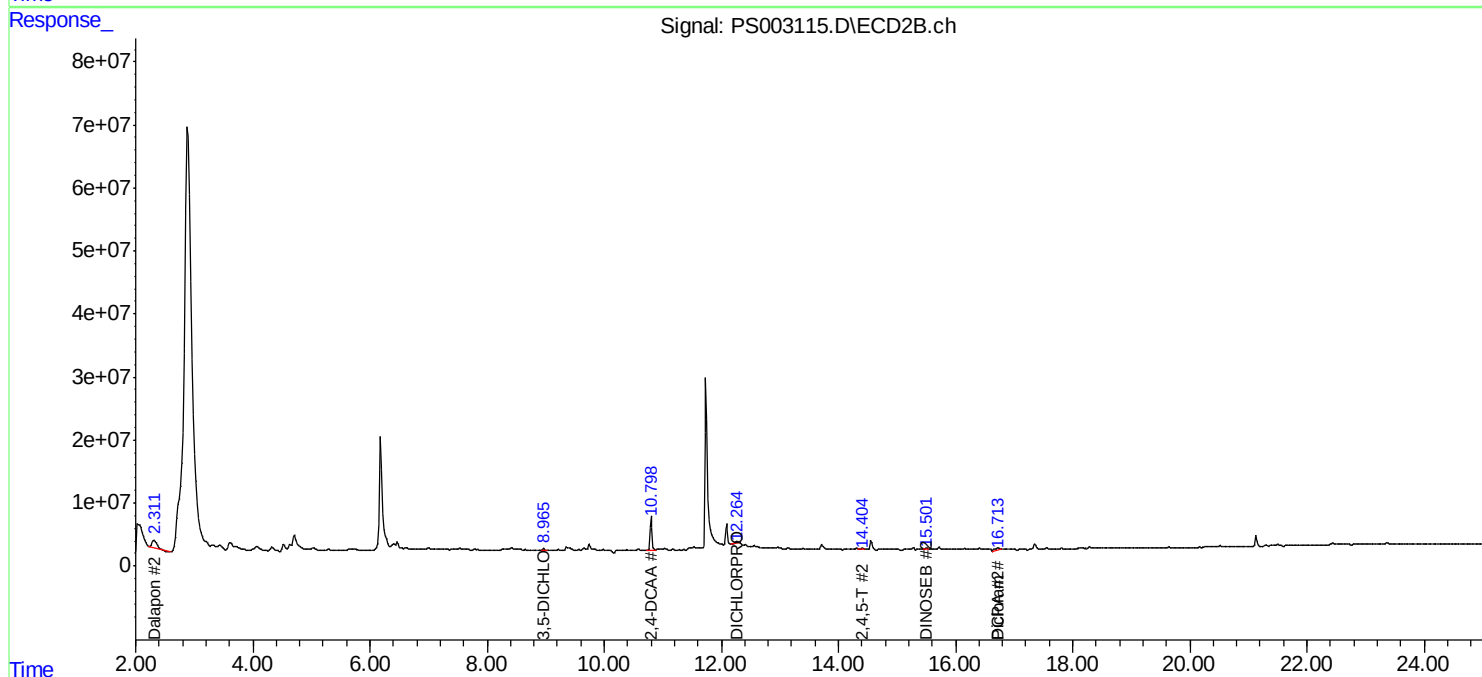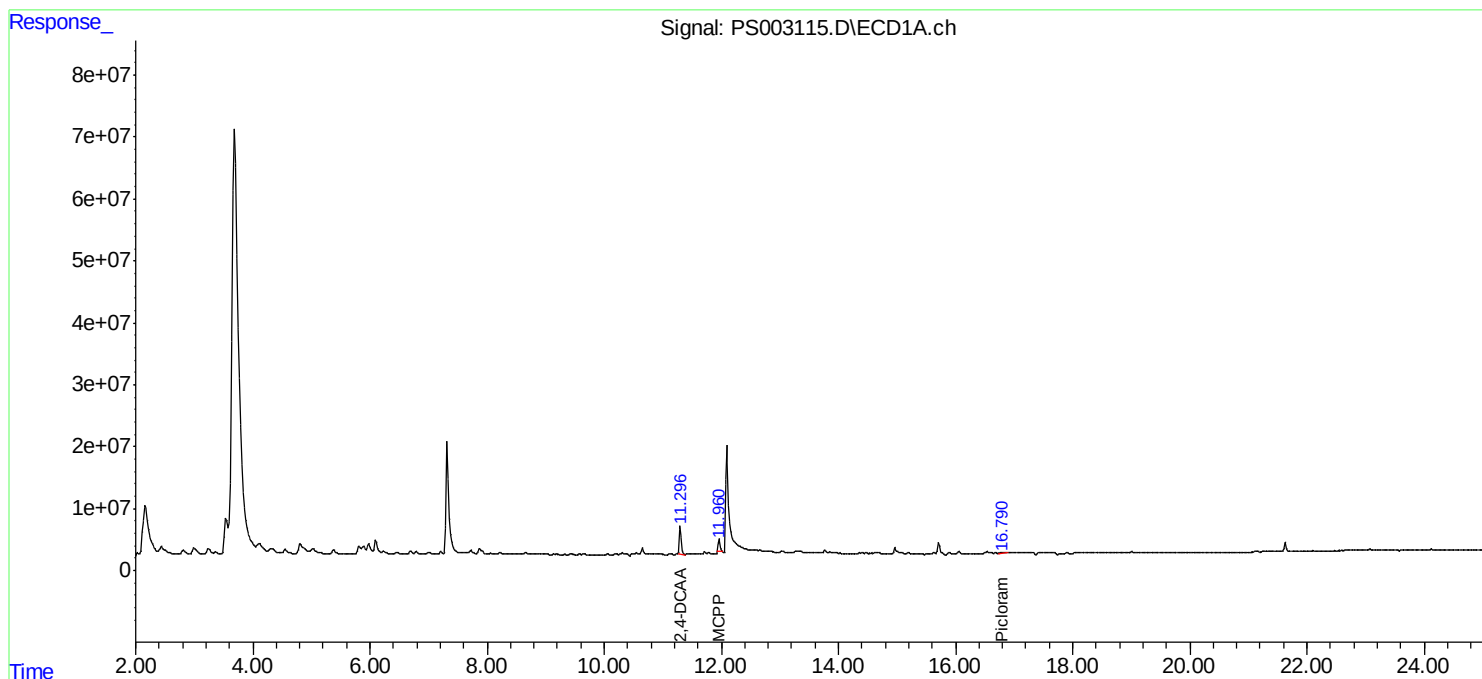


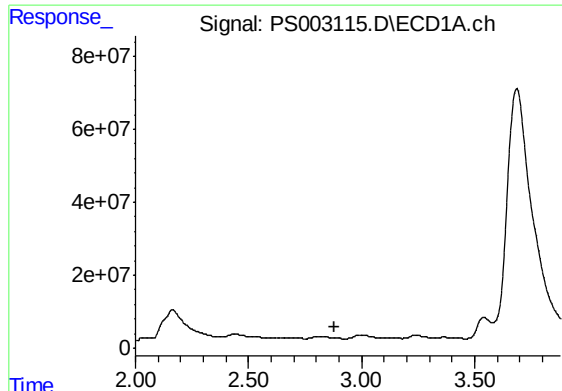

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116998TB

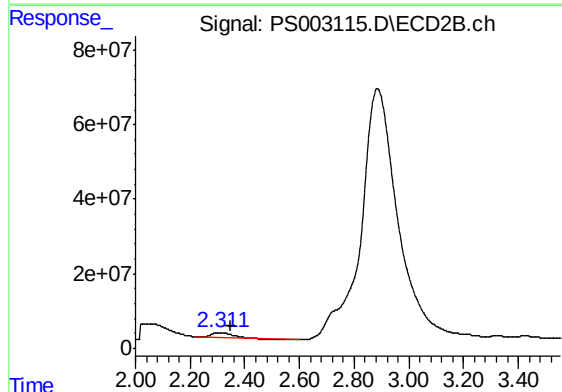


#1 Dalapon

R.T.: 2.308 min
Delta R.T.: -0.043 min
Response: 55219229
Conc: 103.04 ng/ml

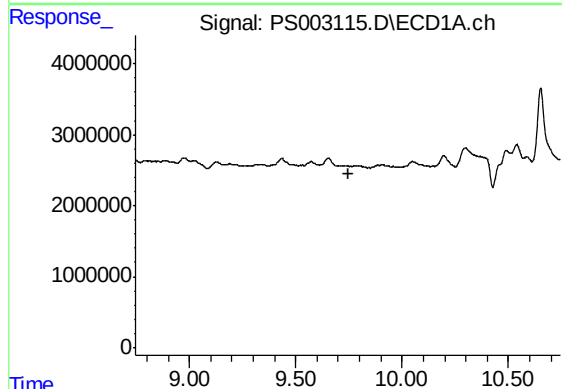


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

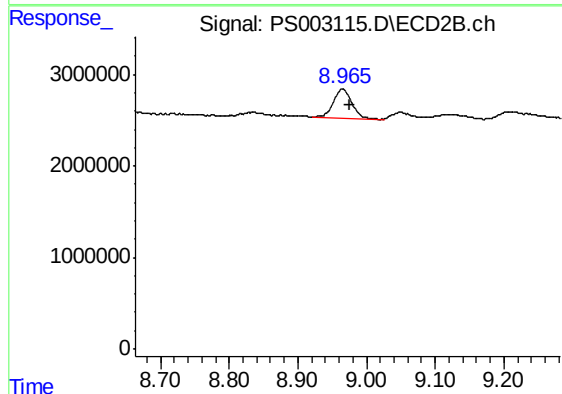

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.965 min
Delta R.T.: -0.011 min
Response: 5834105
Conc: 10.35 ng/ml

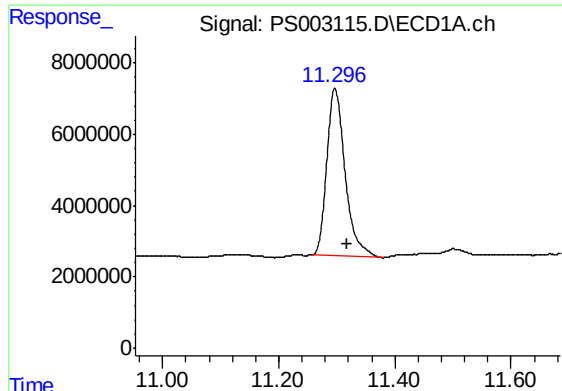

#4 2,4-DCAA


R.T.: 11.297 min
Delta R.T.: -0.021 min
Response: 103234349
Conc: 271.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116998TB

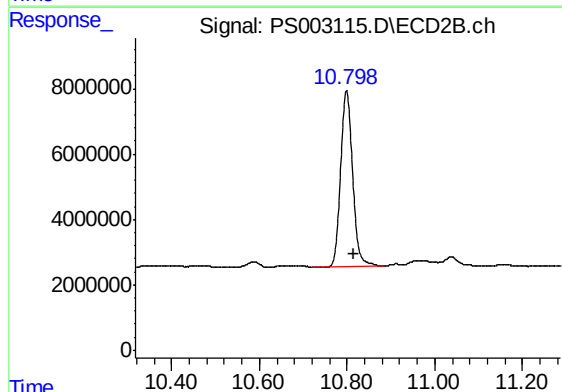


#4 2,4-DCAA

R.T.: 10.799 min
Delta R.T.: -0.018 min
Response: 102592532
Conc: 239.96 ng/ml

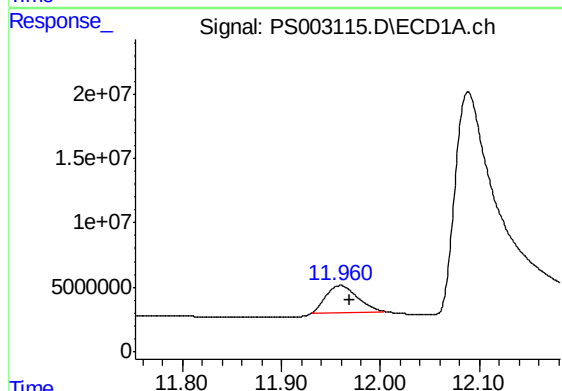


#6 MCP

R.T.: 11.959 min
Delta R.T.: -0.010 min
Response: 45524571
Conc: 38.00 ug/ml

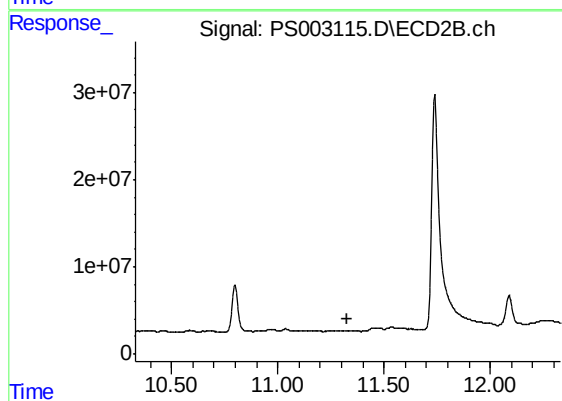

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

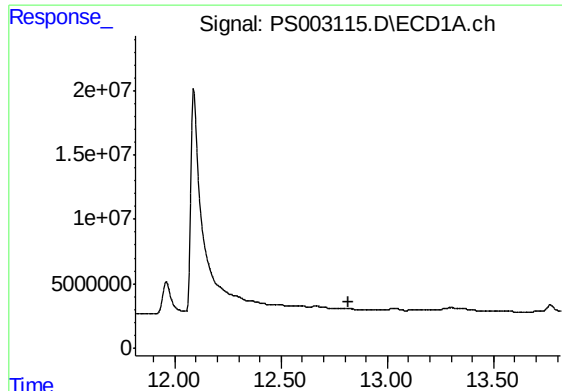

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.815 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116998TB

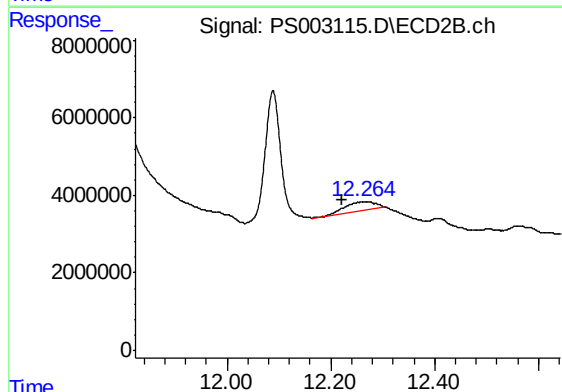


#8 DICHLORPROP

R.T.: 12.266 min
Delta R.T.: 0.044 min
Response: 8457441
Conc: 22.12 ng/ml

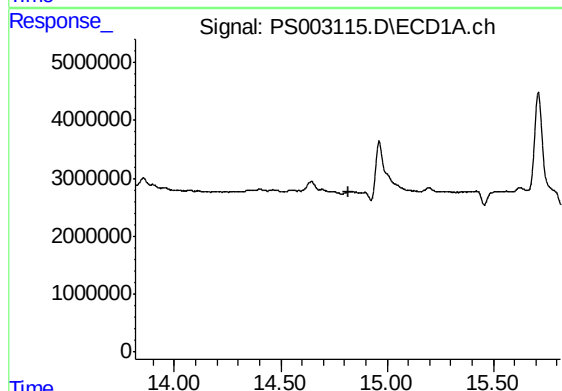


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

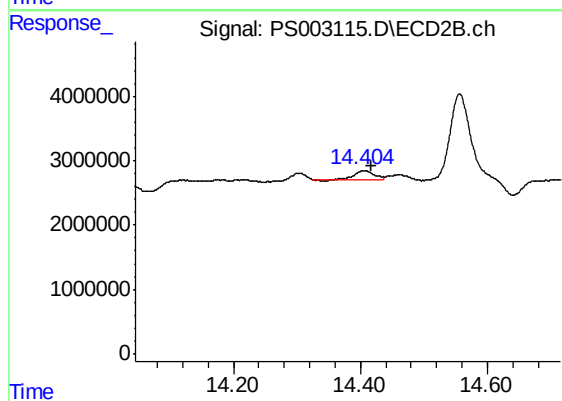

#12 2,4,5-T


R.T.: 14.405 min
Delta R.T.: -0.012 min
Response: 2974215
Conc: 1.55 ng/ml

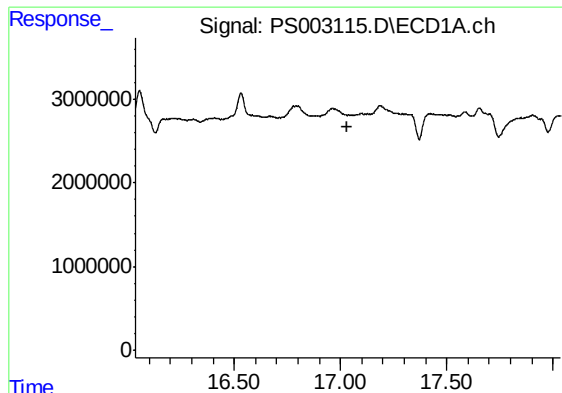

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116998TB

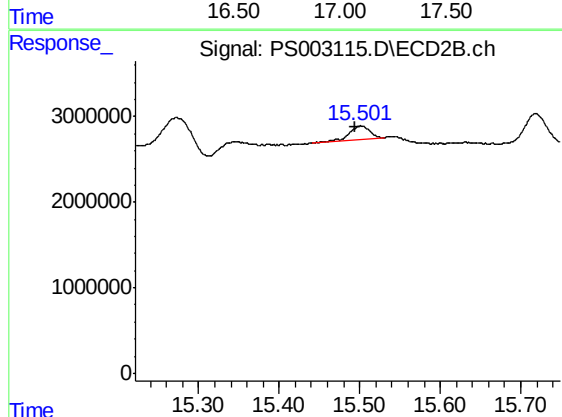


#14 DINOSEB

R.T.: 15.501 min
Delta R.T.: 0.007 min
Response: 2790618
Conc: 1.59 ng/ml

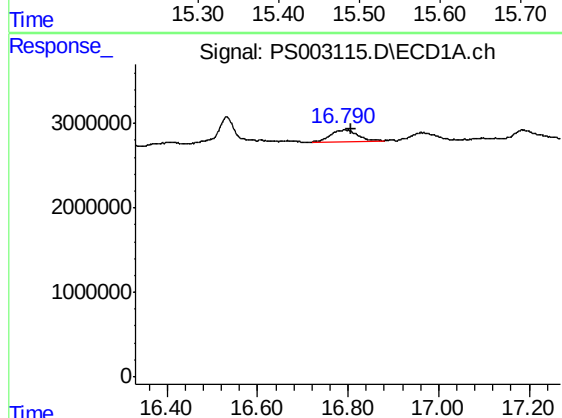


#15 Picloram

R.T.: 16.791 min
Delta R.T.: -0.014 min
Response: 5918070
Conc: 1.87 ng/ml

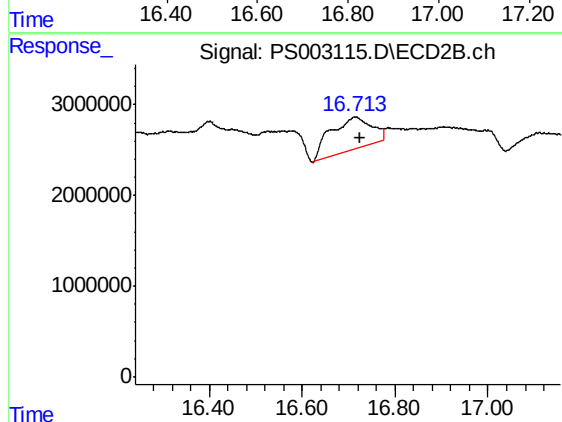

#15 Picloram


R.T.: 16.714 min
Delta R.T.: -0.010 min
Response: 22206755
Conc: 7.39 ng/ml

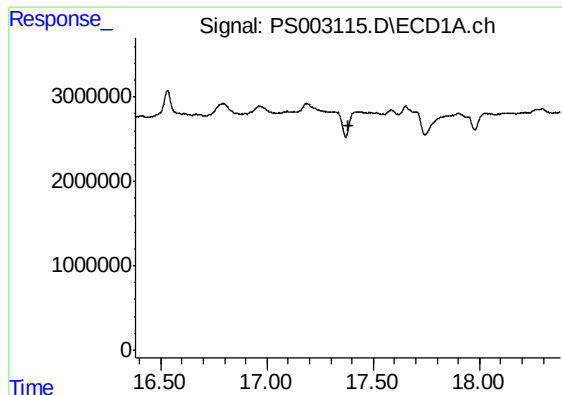

#16 DCPA

R.T.: 17.420 min
Delta R.T.: 0.038 min
Response: -2462628
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116998TB

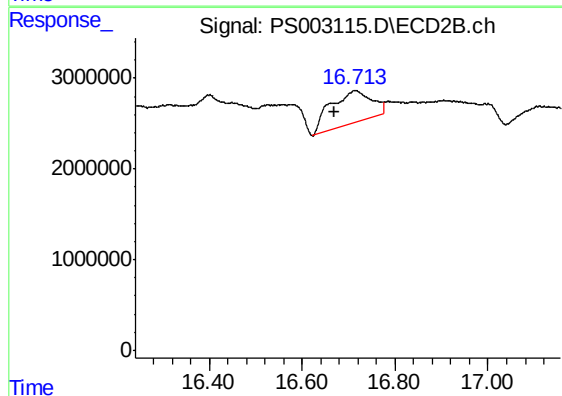

#16 DCPA

R.T.: 16.714 min
Delta R.T.: 0.044 min
Response: 22206755
Conc: 7.17 ng/ml