

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
 Data File : PS003120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 02:38
 Operator : EI\SJ
 Sample : K1423-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HB-VJ210

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 03:06:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.296	10.797	187.6E6	216.2E6	494.020	505.605
Target Compounds							
1) T	Dalapon	2.818	2.307	3919909	81491565	7.106	152.059 #
2) T	3,5-DICHL...	0.000	8.966	0	6478768	N.D.	11.496 #
3) T	4-Nitroph...	10.903	10.013	11458263	18901496	59.204	90.428 #
6) T	MCP	11.966	0.000	29010274	0	24.213	N.D. #
10) T	Pentachlo...	13.520	13.210	1252.5E6	1152.8E6	195.300	186.519
11) T	2,4,5-TP ...	0.000	13.839	0	9059499	N.D.	3.653 #
14) T	DINOSEB	0.000	15.503	0	7007050	N.D.	3.997 #
15) T	Picloram	0.000	16.713	0	21172265	N.D.	7.042 #
16) T	DCPA	17.422	16.713	-4839377	21172265	N.D.	6.835



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
Data File : PS003120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 02:38
Operator : EI\SJ
Sample : K1423-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HB-VJ210

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 03:06:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

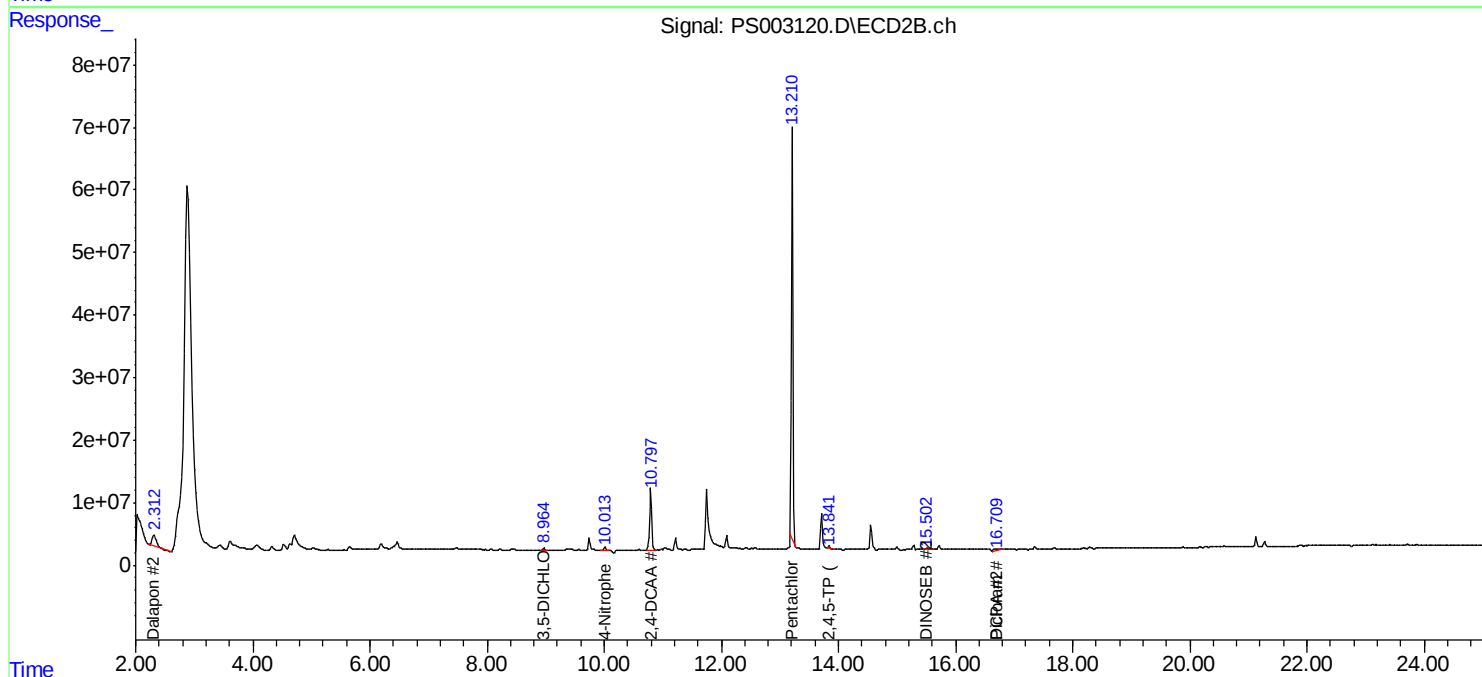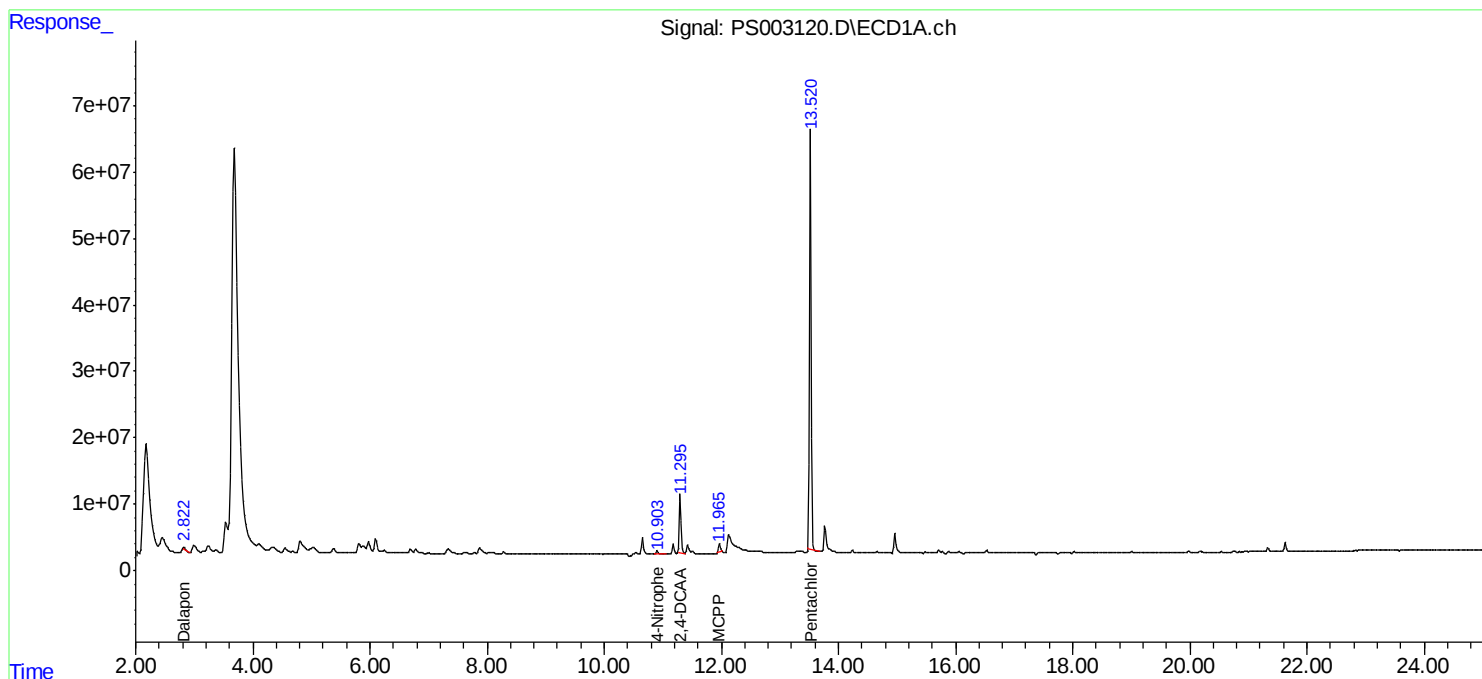


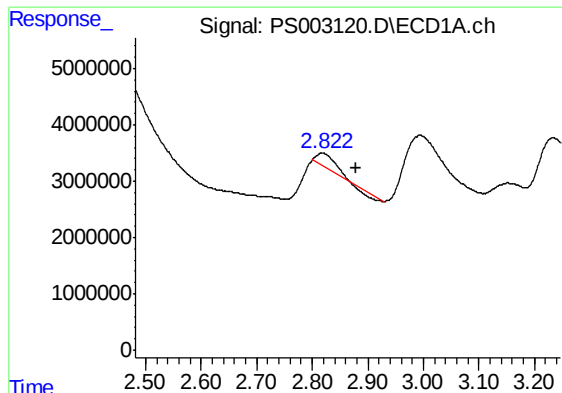

#1 Dalapon


R.T.: 2.818 min
Delta R.T.: -0.062 min
Response: 3919909
Conc: 7.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
HB-VJ210

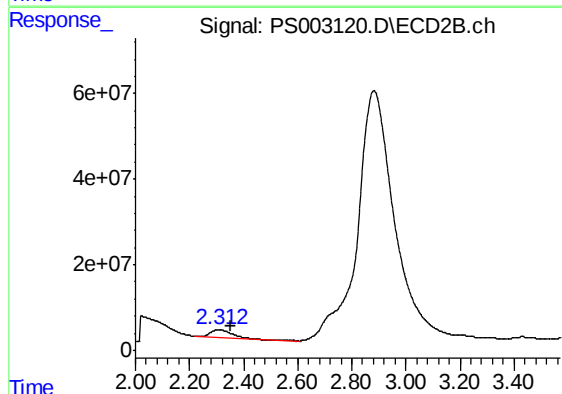


#1 Dalapon

R.T.: 2.307 min
Delta R.T.: -0.043 min
Response: 81491565
Conc: 152.06 ng/ml

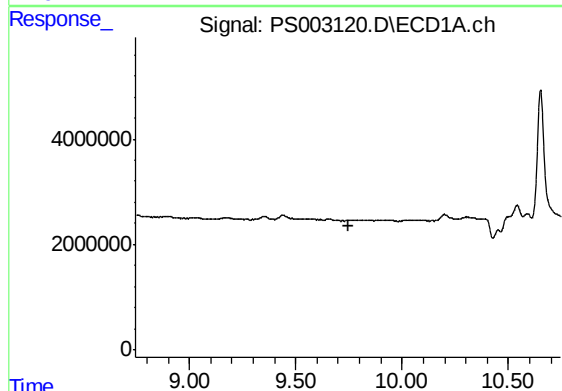


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

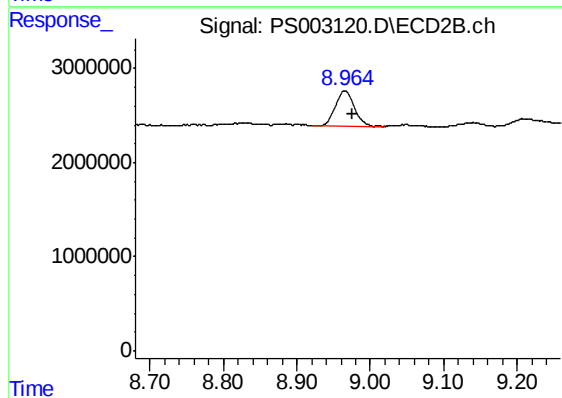

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.966 min
Delta R.T.: -0.011 min
Response: 6478768
Conc: 11.50 ng/ml

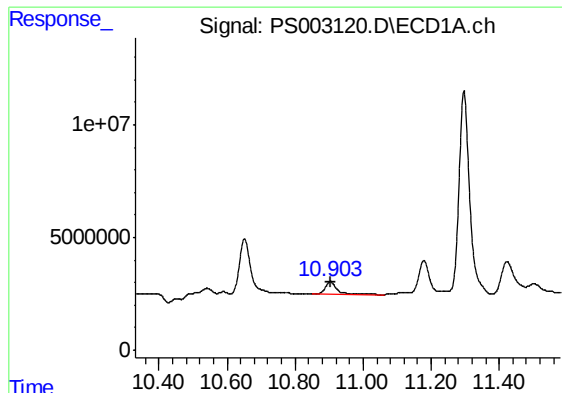

#3 4-Nitrophenol


R.T.: 10.903 min
Delta R.T.: 0.000 min
Response: 11458263
Conc: 59.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
HB-VJ210

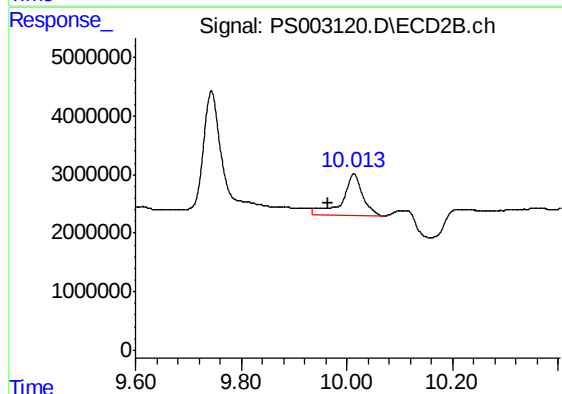


#3 4-Nitrophenol

R.T.: 10.013 min
Delta R.T.: 0.048 min
Response: 18901496
Conc: 90.43 ng/ml

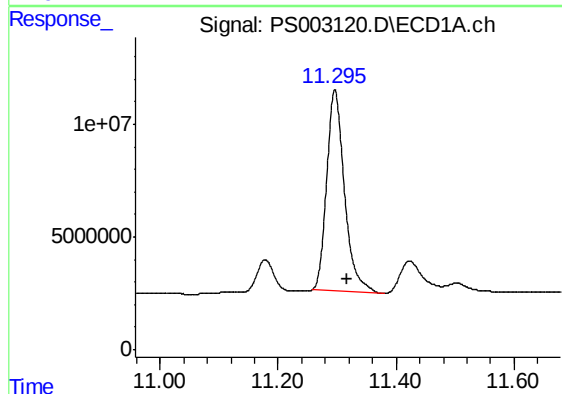


#4 2,4-DCAA

R.T.: 11.296 min
Delta R.T.: -0.022 min
Response: 187550060
Conc: 494.02 ng/ml

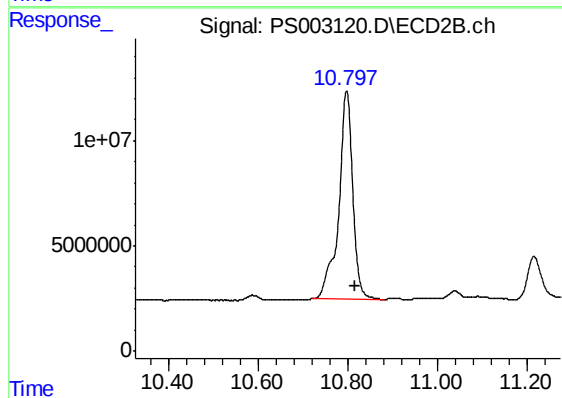

#4 2,4-DCAA


R.T.: 10.797 min
Delta R.T.: -0.019 min
Response: 216169401
Conc: 505.61 ng/ml

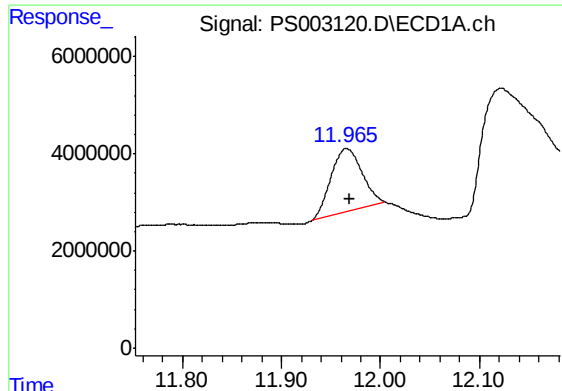

#6 MCP


R.T.: 11.966 min
Delta R.T.: -0.004 min
Response: 29010274
Conc: 24.21 ug/ml

Instrument :
ECD_S
ClientSampleId :
HB-VJ210

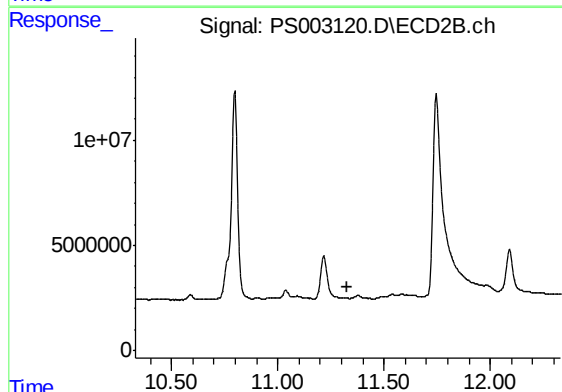


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

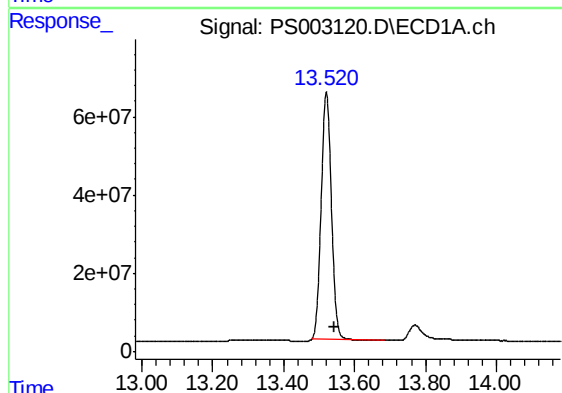


#10 Pentachlorophenol

R.T.: 13.520 min
Delta R.T.: -0.023 min
Response: 1252457681
Conc: 195.30 ng/ml

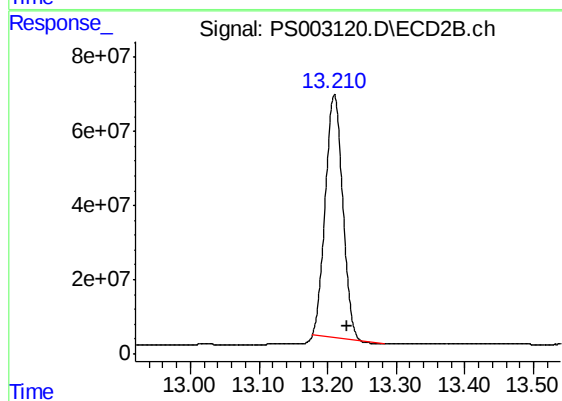

#10 Pentachlorophenol


R.T.: 13.210 min
Delta R.T.: -0.020 min
Response: 1152798592
Conc: 186.52 ng/ml

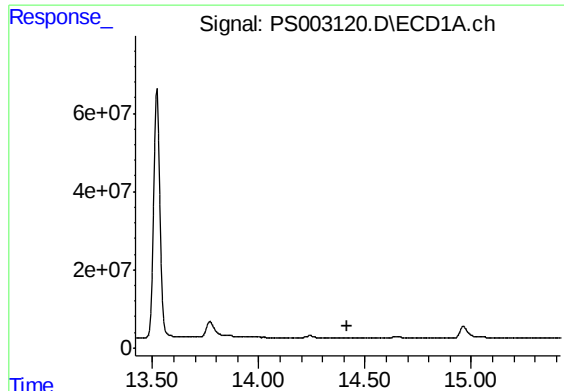

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HB-VJ210

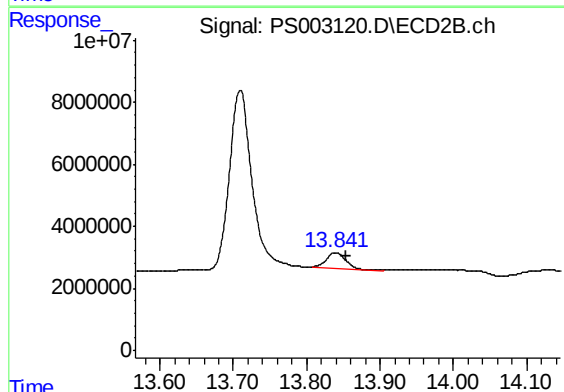


#11 2,4,5-TP (SILVEX)

R.T.: 13.839 min
Delta R.T.: -0.015 min
Response: 9059499
Conc: 3.65 ng/ml

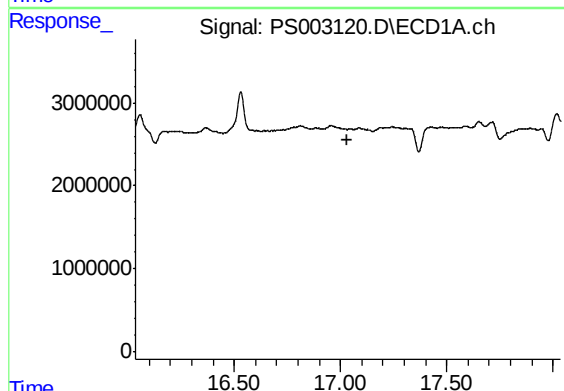


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

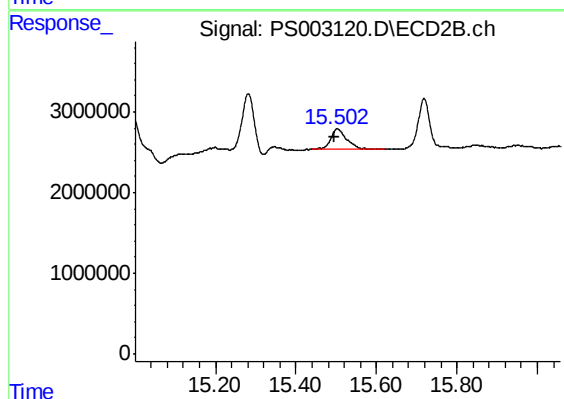

#14 DINOSEB


R.T.: 15.503 min
Delta R.T.: 0.008 min
Response: 7007050
Conc: 4.00 ng/ml

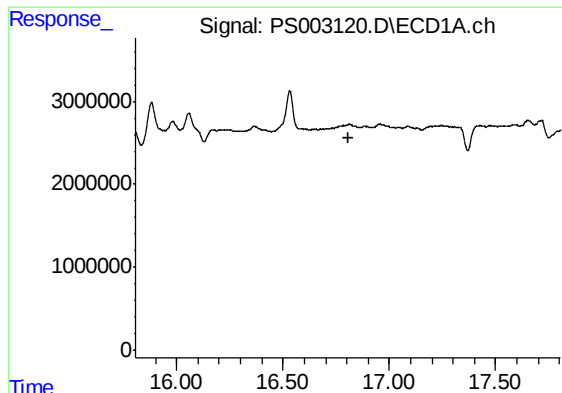

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HB-VJ210

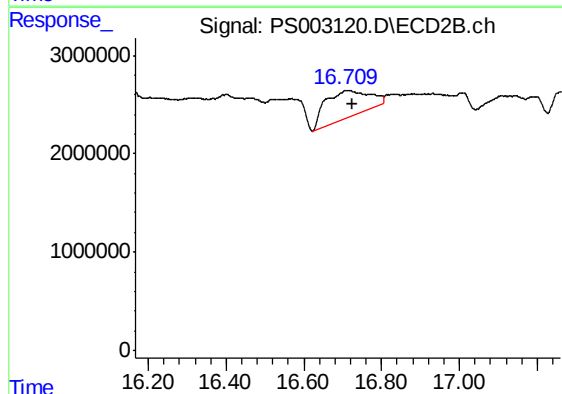


#15 Picloram

R.T.: 16.713 min
Delta R.T.: -0.011 min
Response: 21172265
Conc: 7.04 ng/ml

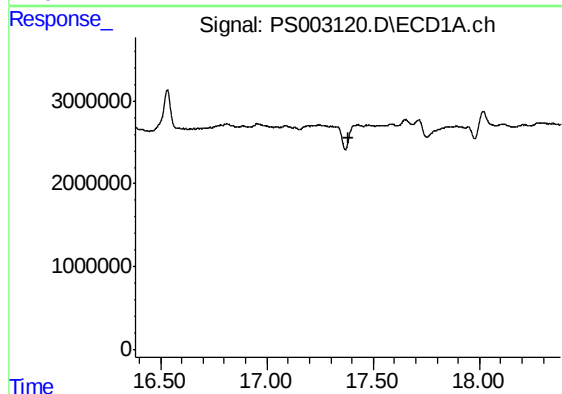

#16 DCPA

R.T.: 17.422 min
Delta R.T.: 0.041 min
Response: -4839377
Conc: N.D.

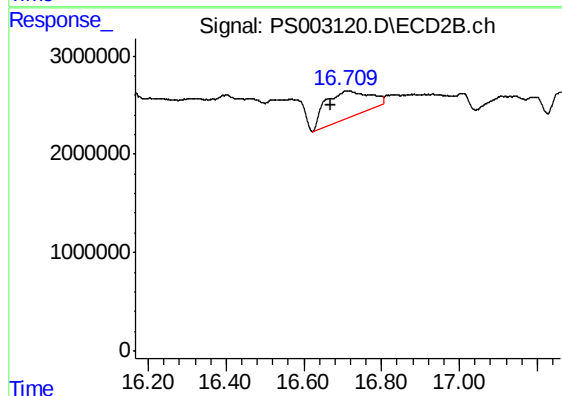

#16 DCPA

R.T.: 16.713 min
Delta R.T.: 0.043 min
Response: 21172265
Conc: 6.84 ng/ml