

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
 Data File : PS003122.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 03:40
 Operator : EI\SJ
 Sample : K1442-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 04:15:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.297	10.798	176.4E6	173.4E6	464.716	405.511
Target Compounds							
1) T	Dalapon	0.000	2.308	0	103.6E6	N.D.	193.323 #
2) T	3,5-DICHL...	0.000	8.965	0	5958056	N.D.	10.572 #
6) T	MCP	11.967	0.000	27914211	0	23.298	N.D. #
14) T	DINOSEB	0.000	15.505	0	7754608	N.D.	4.424 #
15) T	Picloram	16.777	16.719	5544081	12918629	1.752	4.297 #
16) T	DCPA	17.442	16.719	-2346001	12918629	N.D.	4.171



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
Data File : PS003122.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 03:40
Operator : EI\SJ
Sample : K1442-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 04:15:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

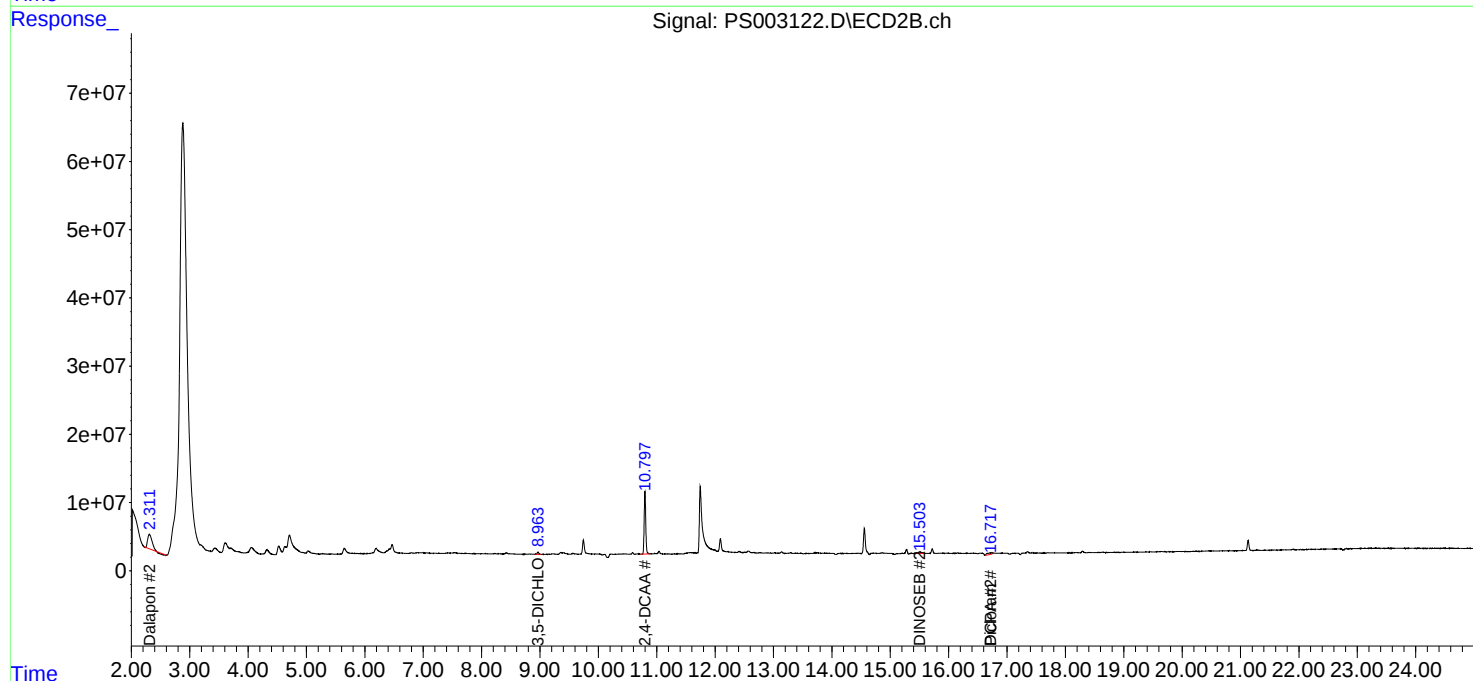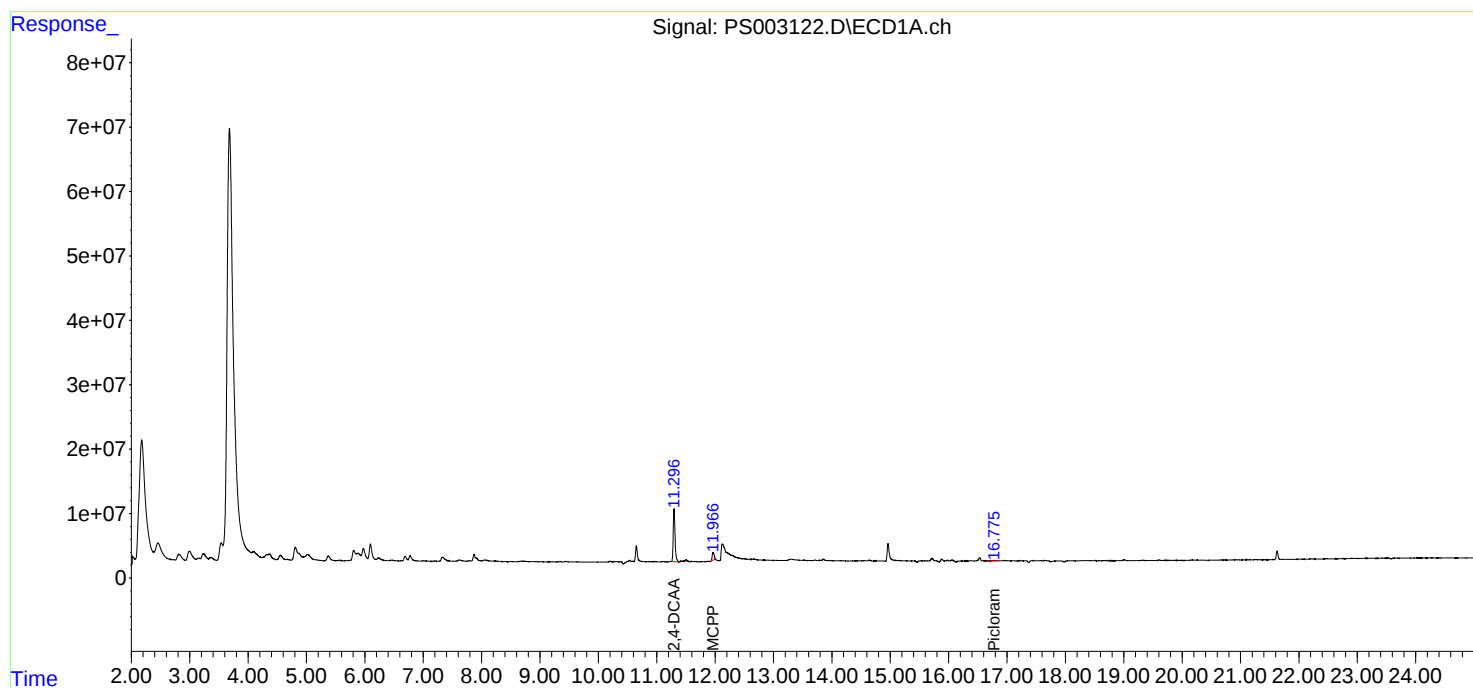


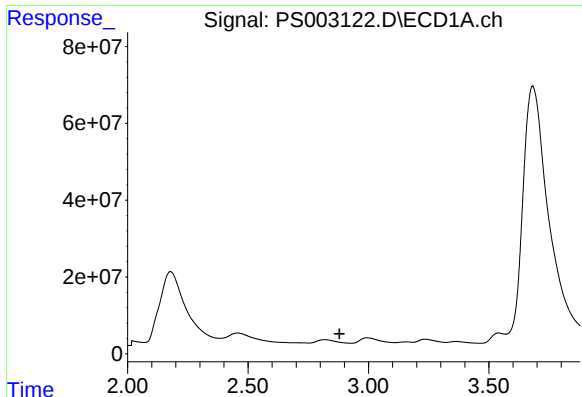

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

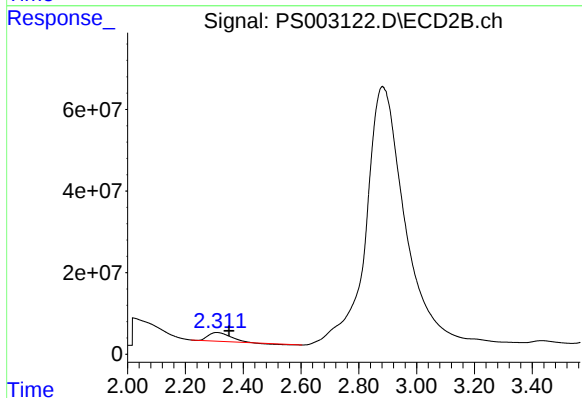


#1 Dalapon

R.T.: 2.308 min
Delta R.T.: -0.043 min
Response: 103605889
Conc: 193.32 ng/ml

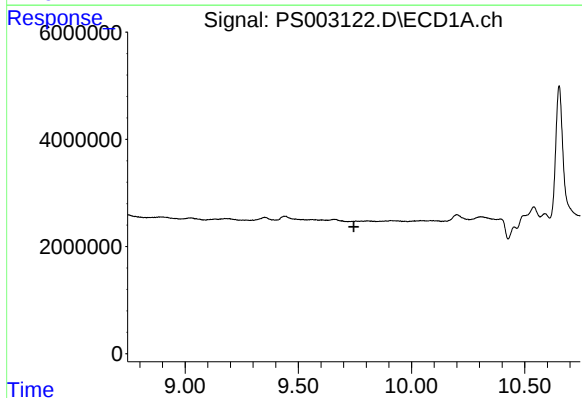


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

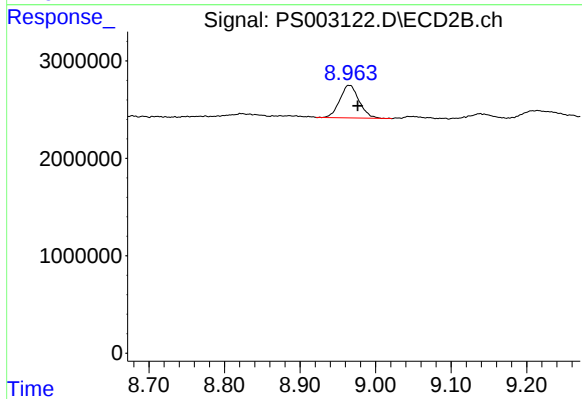

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.965 min
Delta R.T.: -0.011 min
Response: 5958056
Conc: 10.57 ng/ml

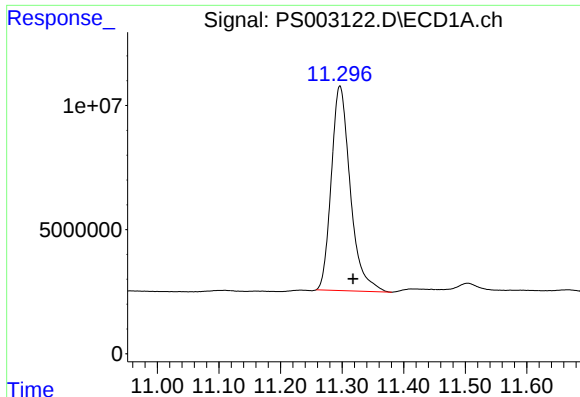

#4 2,4-DCAA


R.T.: 11.297 min
Delta R.T.: -0.021 min
Response: 176425276
Conc: 464.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

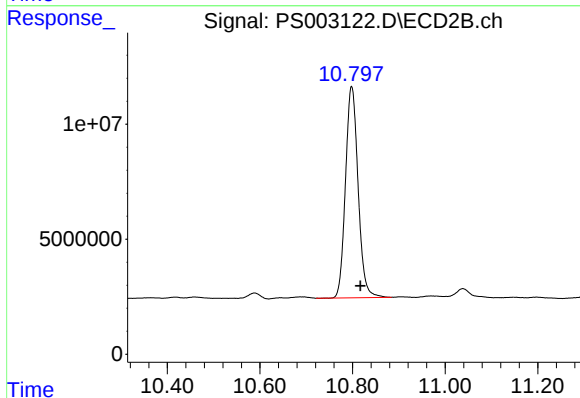


#4 2,4-DCAA

R.T.: 10.798 min
Delta R.T.: -0.019 min
Response: 173374284
Conc: 405.51 ng/ml

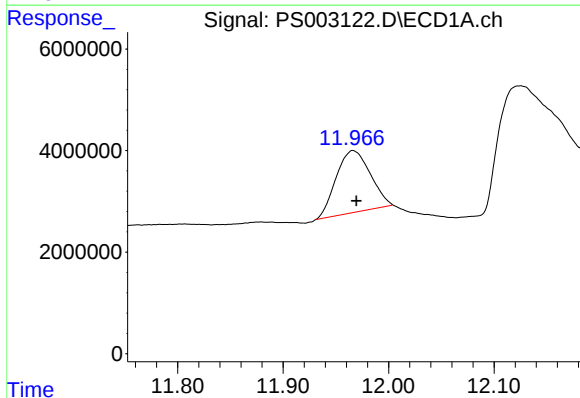


#6 MCP

R.T.: 11.967 min
Delta R.T.: -0.003 min
Response: 27914211
Conc: 23.30 ug/ml

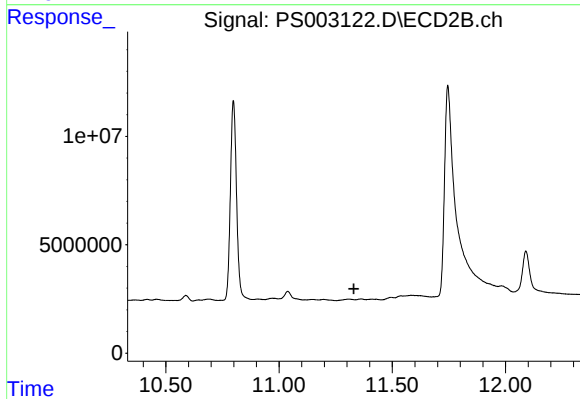

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

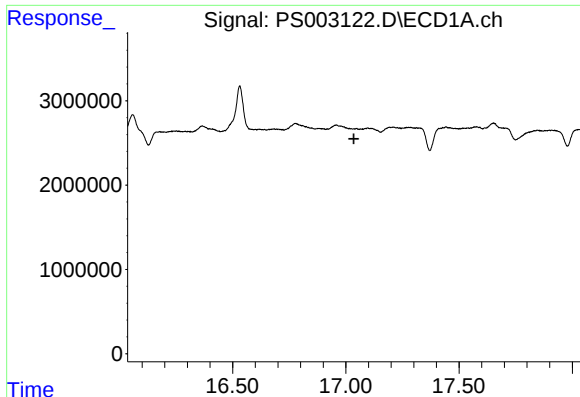

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

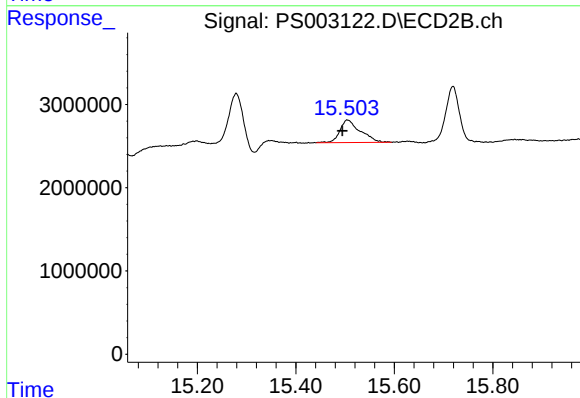


#14 DINOSEB

R.T.: 15.505 min
Delta R.T.: 0.010 min
Response: 7754608
Conc: 4.42 ng/ml

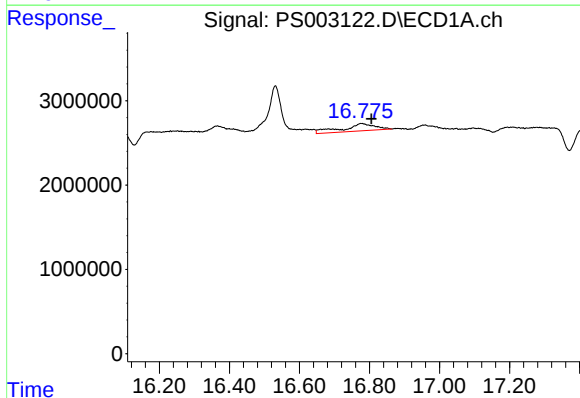


#15 Picloram

R.T.: 16.777 min
Delta R.T.: -0.029 min
Response: 5544081
Conc: 1.75 ng/ml

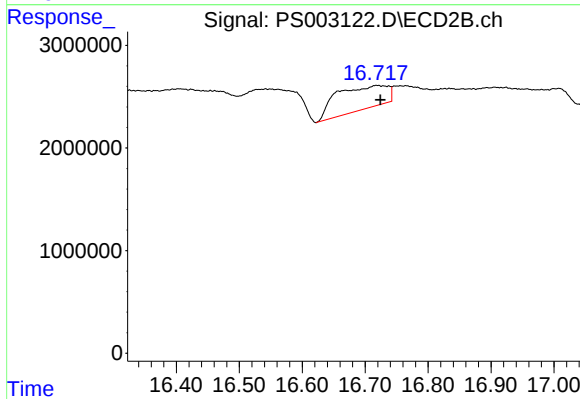

#15 Picloram


R.T.: 16.719 min
Delta R.T.: -0.006 min
Response: 12918629
Conc: 4.30 ng/ml

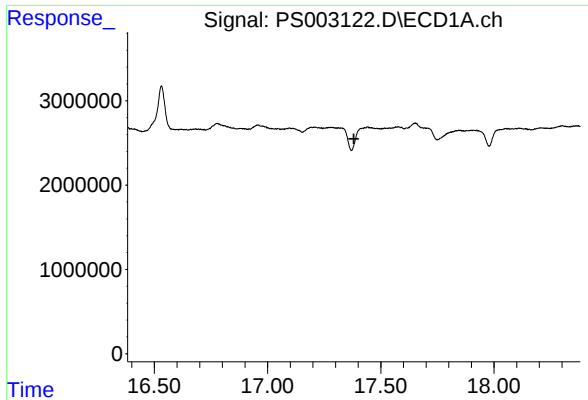

#16 DCPA

R.T.: 17.442 min
Delta R.T.: 0.061 min
Response: -2346001
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

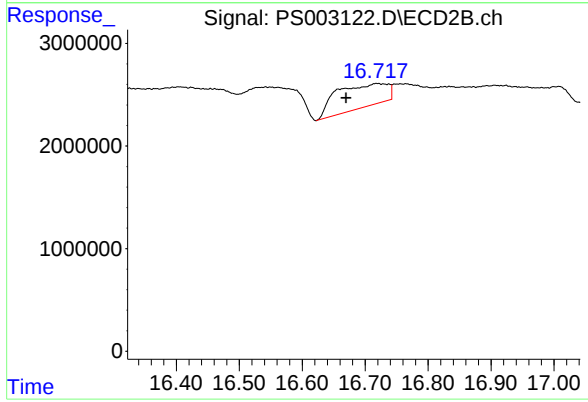

#16 DCPA

R.T.: 16.719 min
Delta R.T.: 0.049 min
Response: 12918629
Conc: 4.17 ng/ml