

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
 Data File : PS003125.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 05:13
 Operator : EI\SJ
 Sample : K1442-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 05:41:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.282	10.783	51688156	69297916	136.150	162.083
Target Compounds							
1) T	Dalapon	0.000	2.284	0	17172224	N.D.	32.042 #
2) T	3,5-DICHL...	0.000	8.945	0	2802823	N.D.	4.973 #
3) T	4-Nitroph...	0.000	10.019	0	3445028	N.D.	16.482 #
7) T	MCPA	12.234	11.686	7950414	2929245	4.492	1.862 #
8) T	DICHLORPROP	12.827	0.000	9405695	0	24.524	N.D. #
10) T	Pentachlo...	13.505	0.000	3447717	0	0.538	N.D. #
14) T	DINOSEB	0.000	15.496	0	16136054	N.D.	9.205 #
15) T	Picloram	0.000	16.741	0	24341827	N.D.	8.097 #
16) T	DCPA	17.440	16.648	-8246540	18682780	N.D.	6.031



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
Data File : PS003125.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 05:13
Operator : EI\SJ
Sample : K1442-05
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 05:41:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

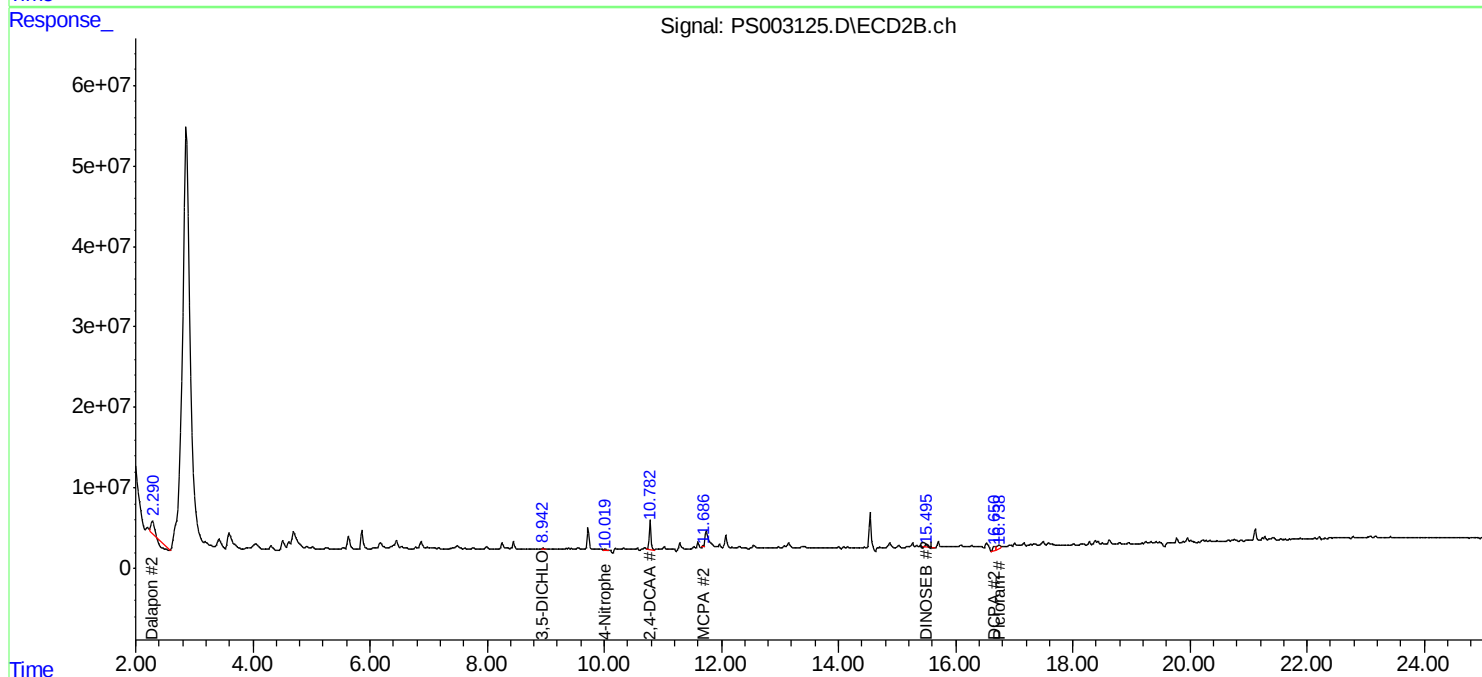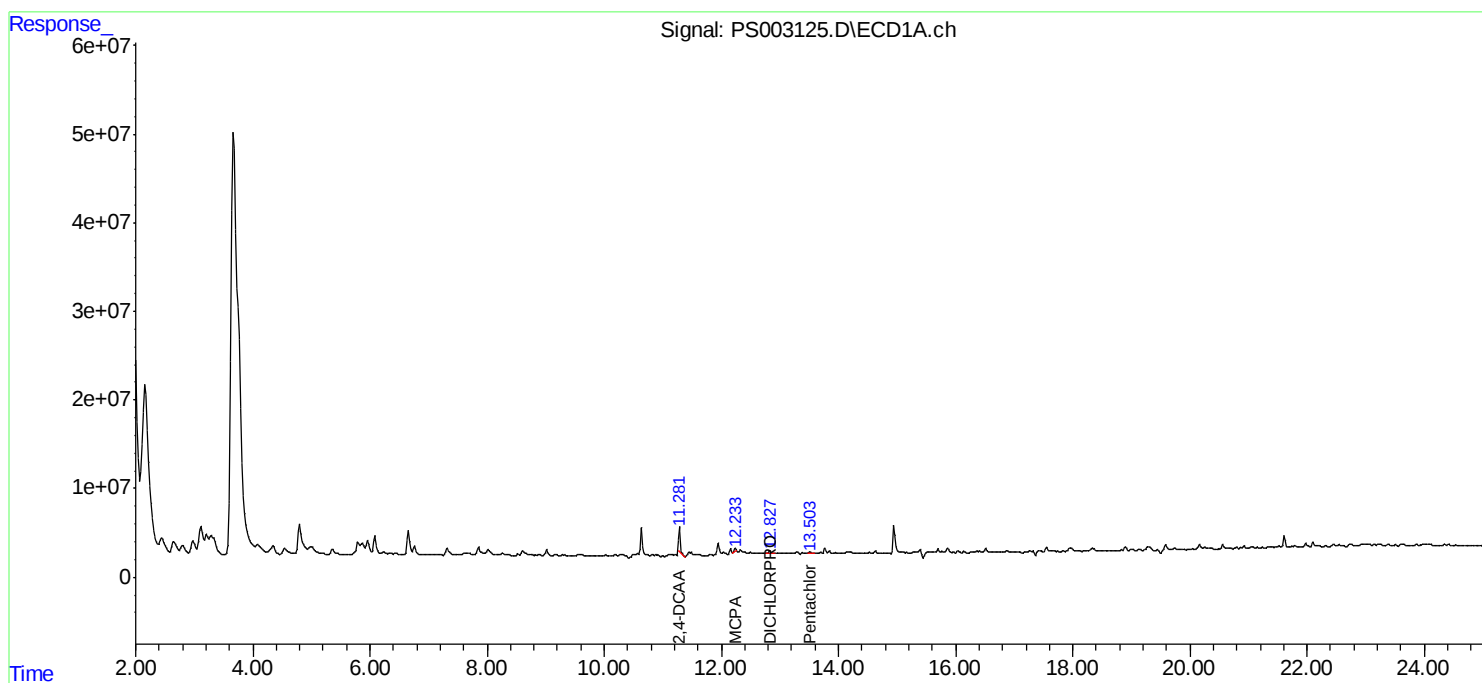


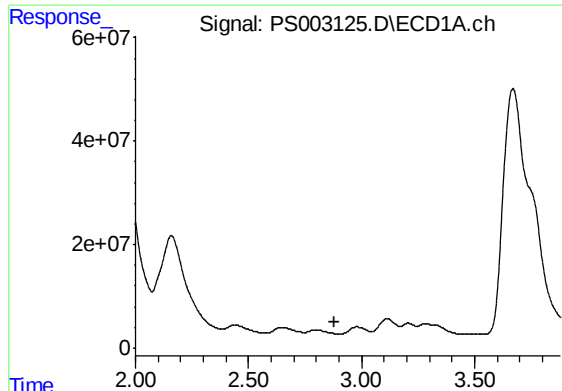

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-11

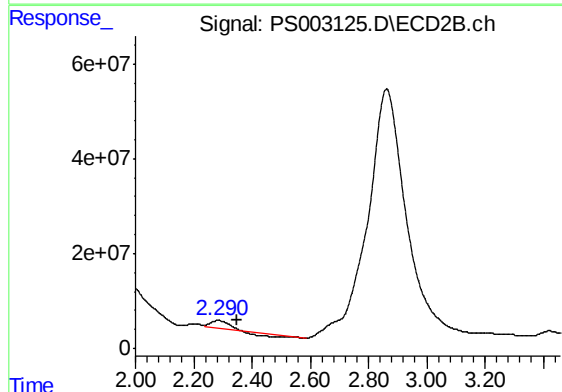


#1 Dalapon

R.T.: 2.284 min
Delta R.T.: -0.066 min
Response: 17172224
Conc: 32.04 ng/ml

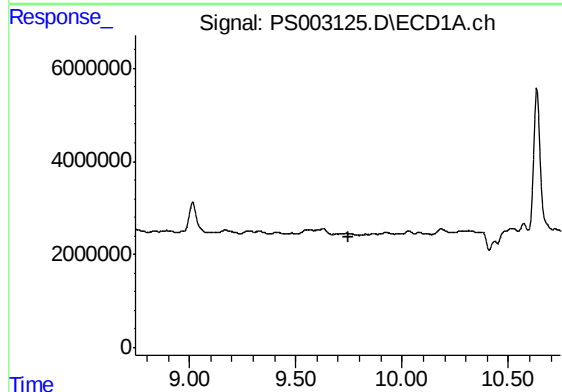


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

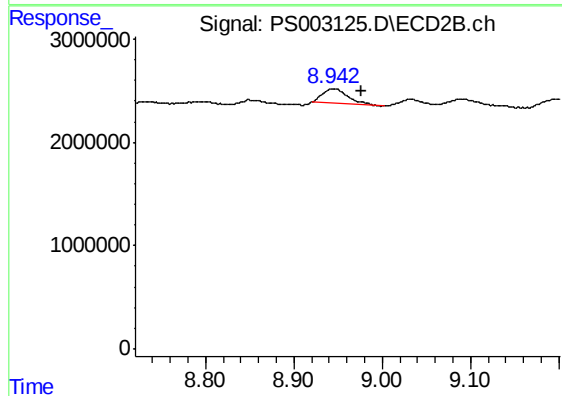

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.945 min
Delta R.T.: -0.032 min
Response: 2802823
Conc: 4.97 ng/ml

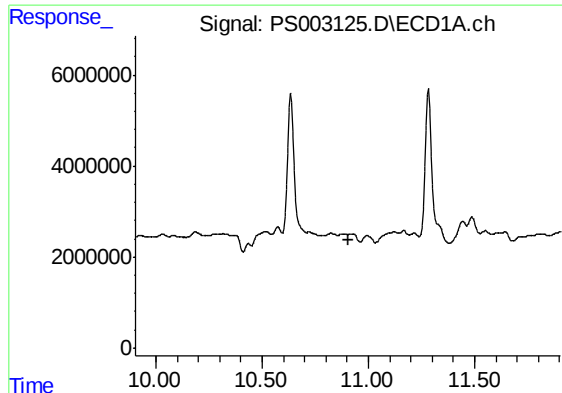

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-11

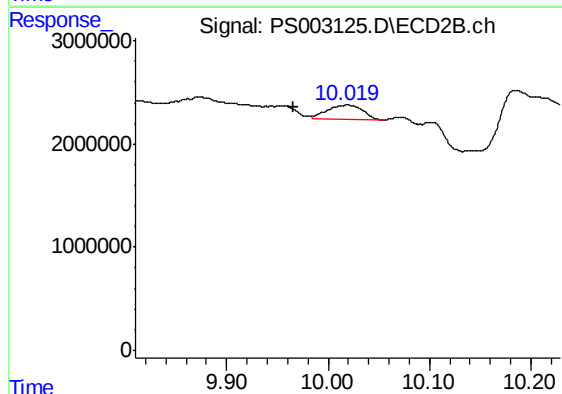


#3 4-Nitrophenol

R.T.: 10.019 min
Delta R.T.: 0.054 min
Response: 3445028
Conc: 16.48 ng/ml

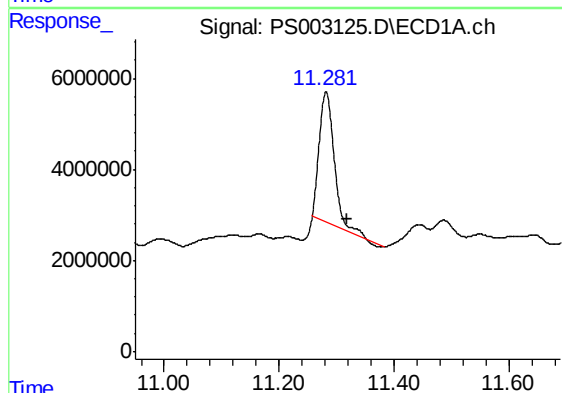


#4 2,4-DCAA

R.T.: 11.282 min
Delta R.T.: -0.036 min
Response: 51688156
Conc: 136.15 ng/ml

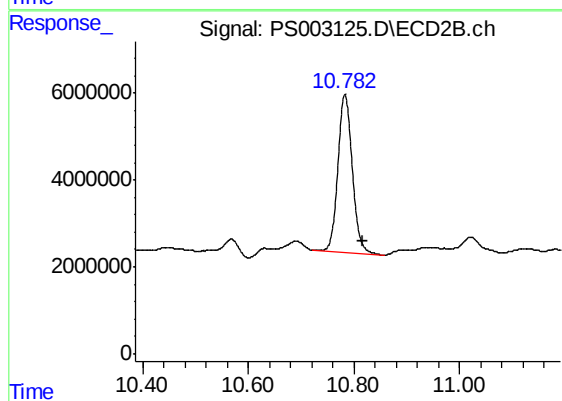

#4 2,4-DCAA


R.T.: 10.783 min
Delta R.T.: -0.034 min
Response: 69297916
Conc: 162.08 ng/ml

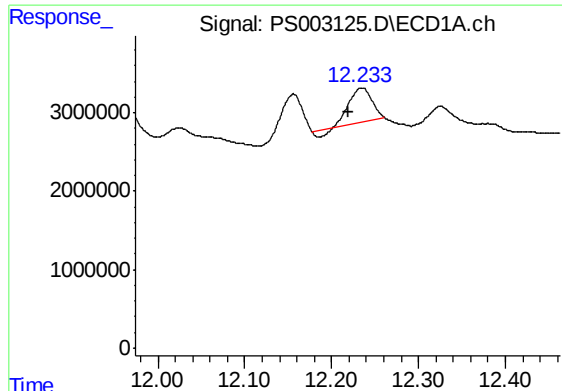

#7 MCPA


R.T.: 12.234 min
Delta R.T.: 0.015 min
Response: 7950414
Conc: 4.49 ug/ml

Instrument :
ECD_S
ClientSampleId :
COMP-11

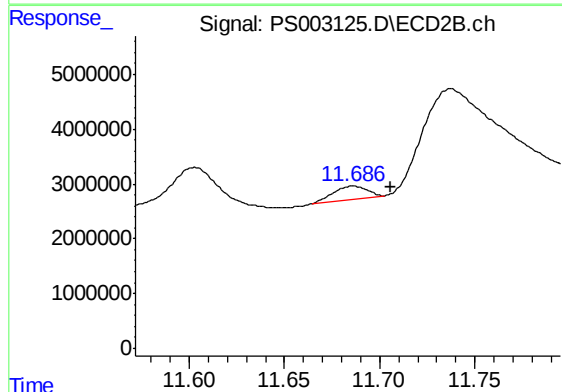


#7 MCPA

R.T.: 11.686 min
Delta R.T.: -0.020 min
Response: 2929245
Conc: 1.86 ug/ml

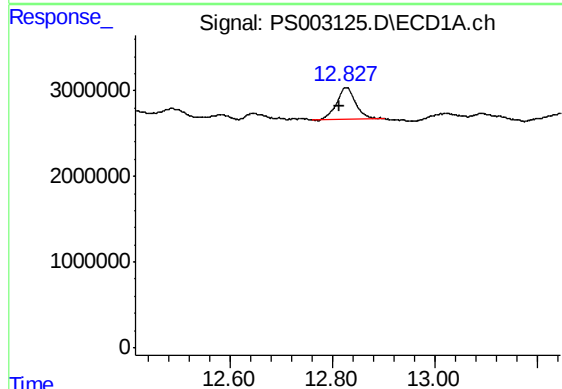


#8 DICHLORPROP

R.T.: 12.827 min
Delta R.T.: 0.013 min
Response: 9405695
Conc: 24.52 ng/ml

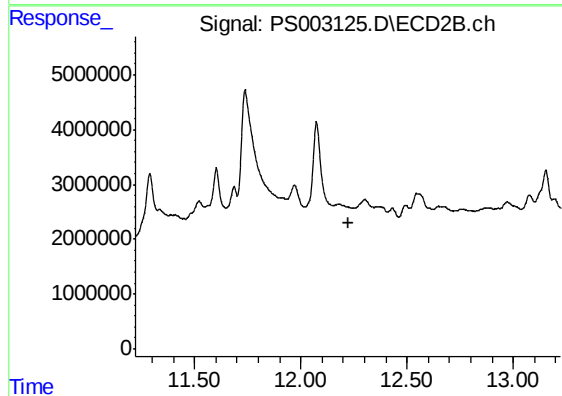

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.222 min
Response: 0
Conc: N.D.

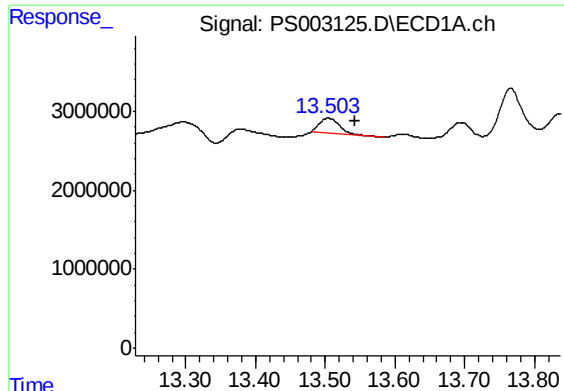

#10 Pentachlorophenol


R.T.: 13.505 min
Delta R.T.: -0.039 min
Response: 3447717
Conc: 0.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-11

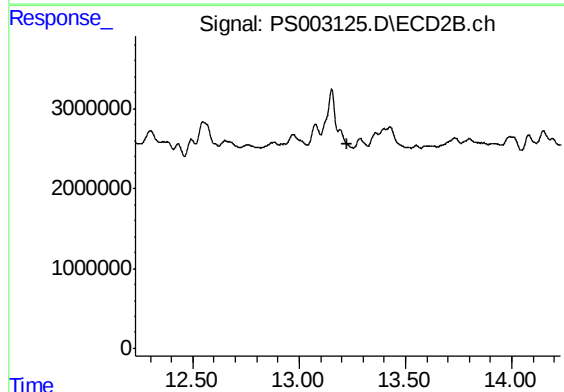


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.229 min
Response: 0
Conc: N.D.

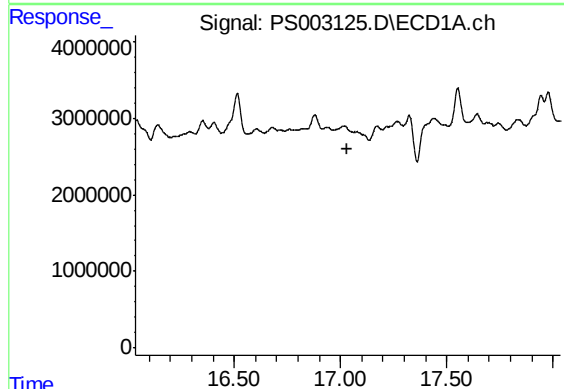


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

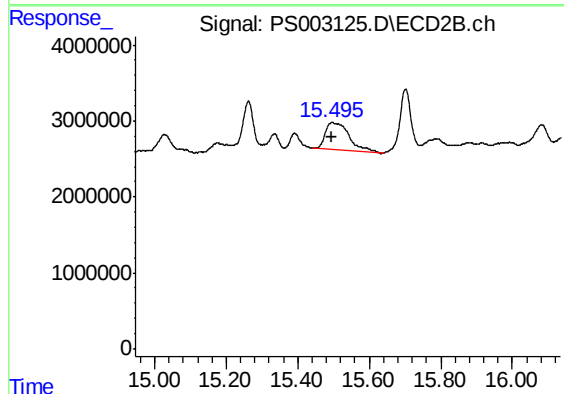

#14 DINOSEB


R.T.: 15.496 min
Delta R.T.: 0.000 min
Response: 16136054
Conc: 9.20 ng/ml

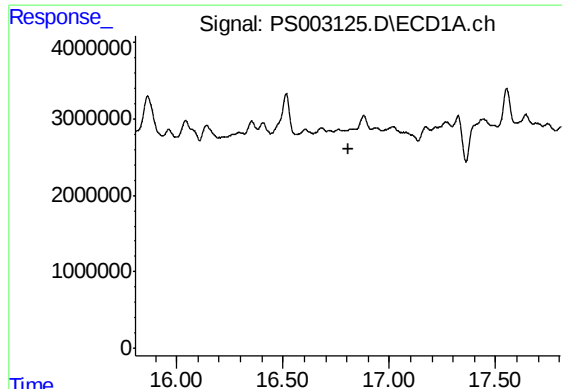

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-11

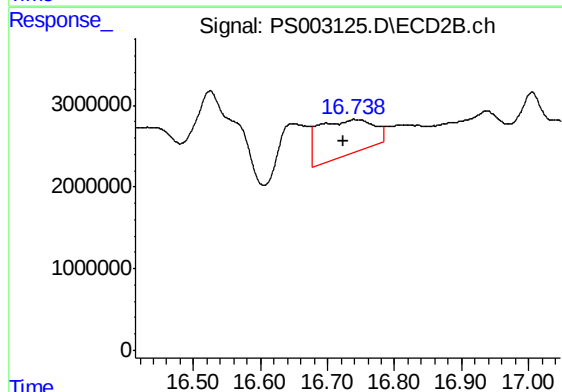


#15 Picloram

R.T.: 16.741 min
Delta R.T.: 0.017 min
Response: 24341827
Conc: 8.10 ng/ml

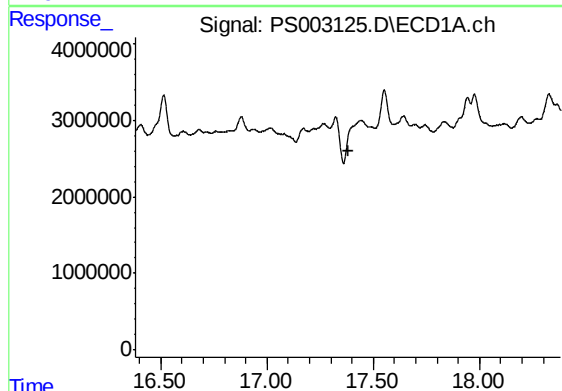

#16 DCPA

R.T.: 17.440 min
Delta R.T.: 0.059 min
Response: -8246540
Conc: N.D.

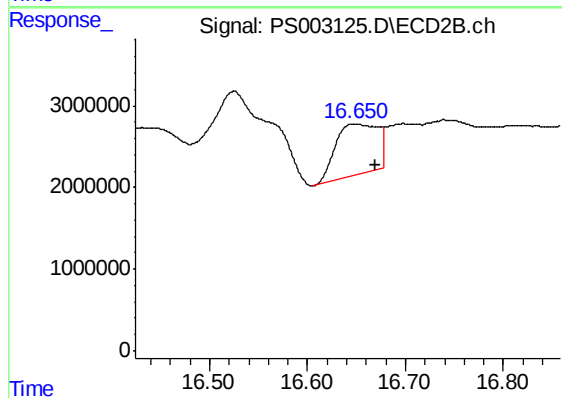

#16 DCPA

R.T.: 16.648 min
Delta R.T.: -0.021 min
Response: 18682780
Conc: 6.03 ng/ml