

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
 Data File : PS003126.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 05:44
 Operator : EI\SJ
 Sample : K1442-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 07:43:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.279	10.780	124.5E6	229.1E6	327.966	535.739 #
Target Compounds							
1) T	Dalapon	0.000	2.285	0	30311807	N.D.	56.560 #
2) T	3,5-DICHL...	0.000	8.944	0	2624142	N.D.	4.656 #
3) T	4-Nitroph...	0.000	10.017	0	3393082	N.D.	16.233 #
7) T	MCPA	12.245	11.720	3038963	1576819	1.717	1.002 #
8) T	DICHLORPROP	12.830	0.000	5638989	0	14.703	N.D. #
10) T	Pentachlo...	13.505	13.292	4568105	-2485355	0.712	N.D. #
13) T	2,4-DB	15.563	0.000	13477531	0	51.553	N.D. #
14) T	DINOSEB	0.000	15.510	0	16550569	N.D.	9.441 #
15) T	Picloram	0.000	16.740	0	10441605	N.D.	3.473 #
16) T	DCPA	17.420	16.648	-14746924	17622122	N.D.	5.689



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
Data File : PS003126.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 05:44
Operator : EI\SJ
Sample : K1442-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 07:43:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

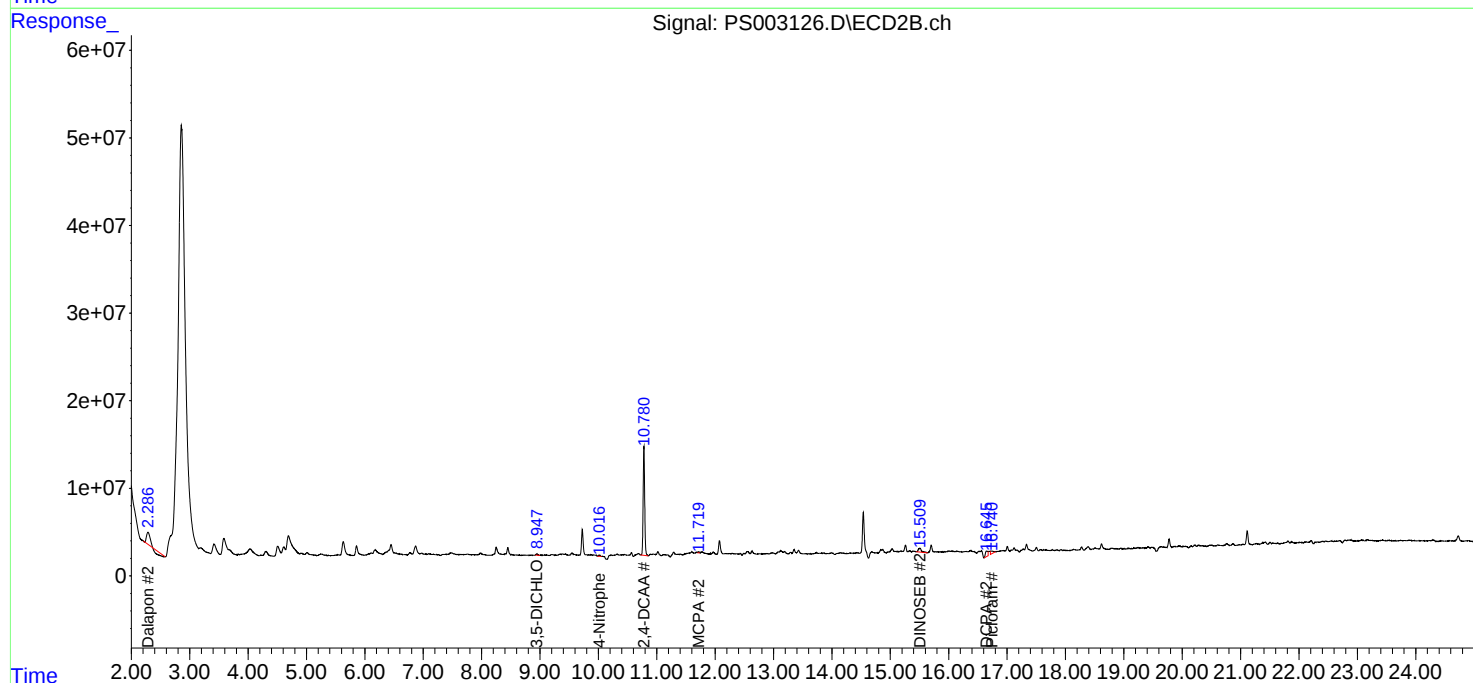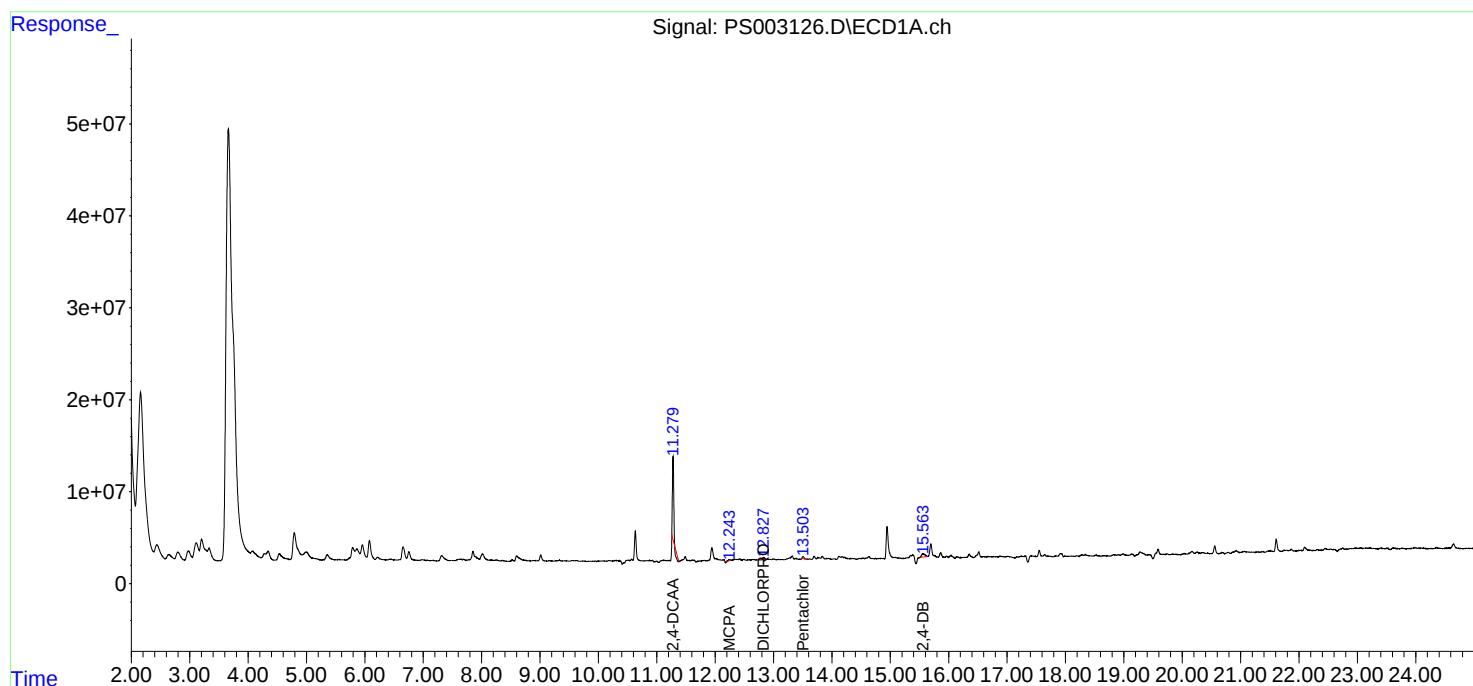


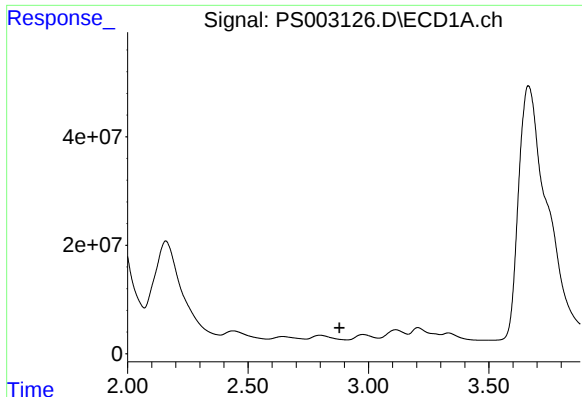

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

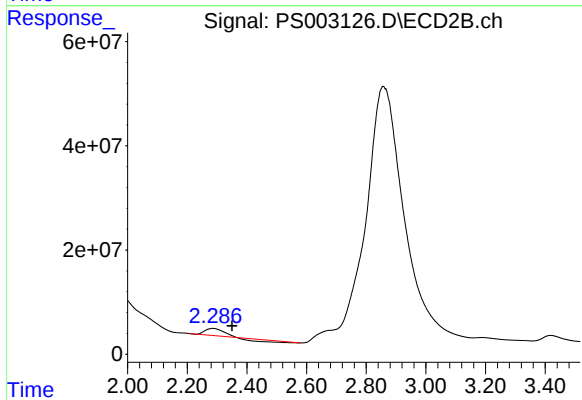


#1 Dalapon

R.T.: 2.285 min
Delta R.T.: -0.065 min
Response: 30311807
Conc: 56.56 ng/ml

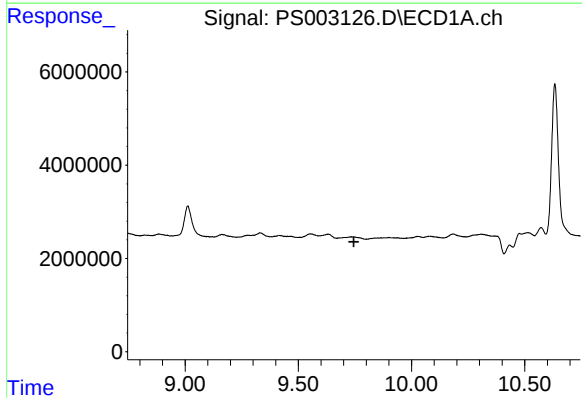


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

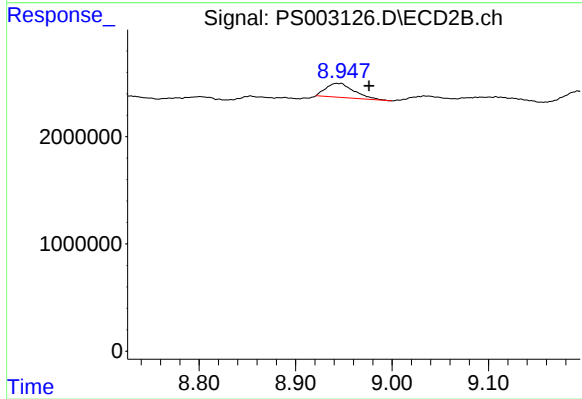

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.944 min
Delta R.T.: -0.032 min
Response: 2624142
Conc: 4.66 ng/ml

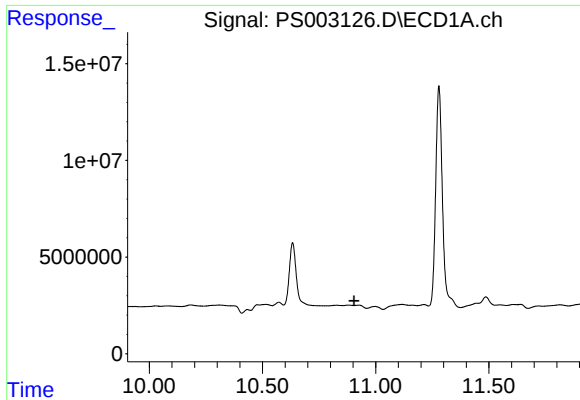

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

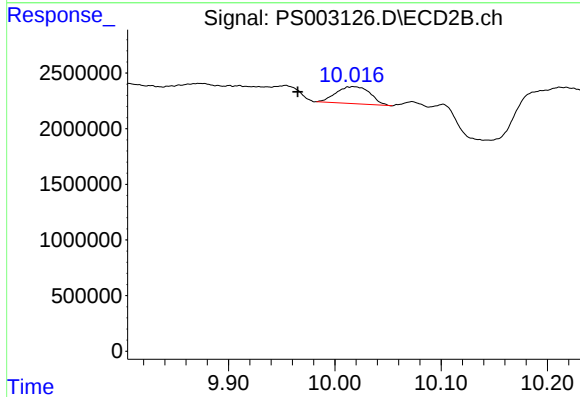


#3 4-Nitrophenol

R.T.: 10.017 min
Delta R.T.: 0.052 min
Response: 3393082
Conc: 16.23 ng/ml

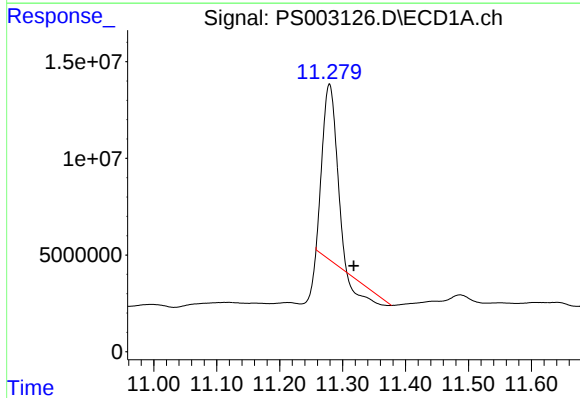


#4 2,4-DCAA

R.T.: 11.279 min
Delta R.T.: -0.039 min
Response: 124509288
Conc: 327.97 ng/ml

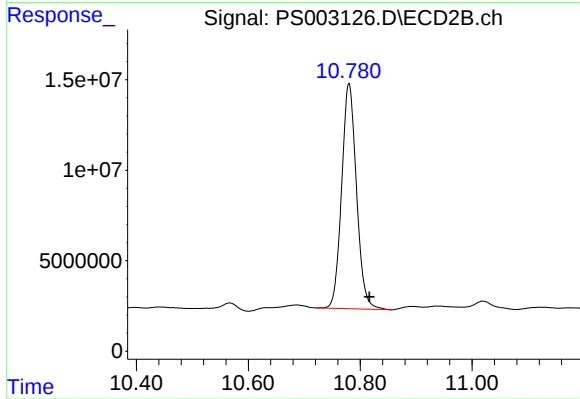

#4 2,4-DCAA


R.T.: 10.780 min
Delta R.T.: -0.037 min
Response: 229052720
Conc: 535.74 ng/ml

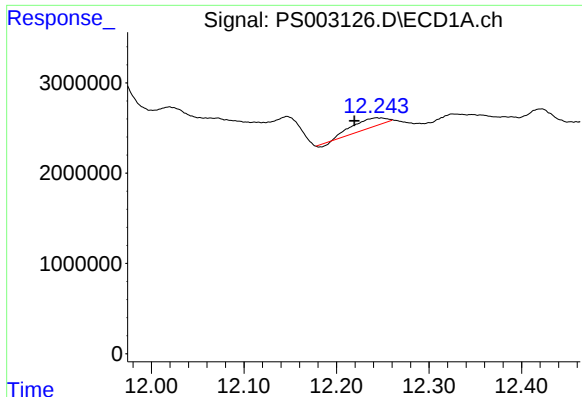

#7 MCPA


R.T.: 12.245 min
Delta R.T.: 0.026 min
Response: 3038963
Conc: 1.72 ug/ml

Instrument :
ECD_S
ClientSampleId :

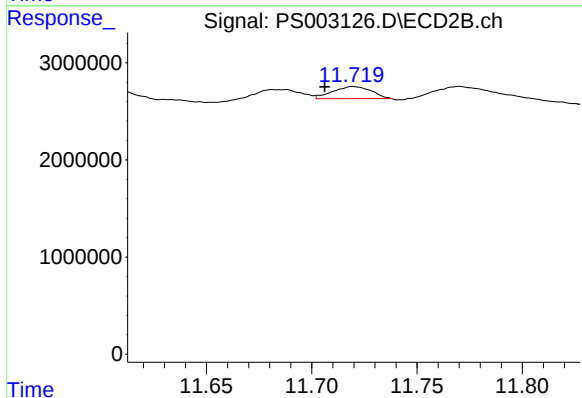


#7 MCPA

R.T.: 11.720 min
Delta R.T.: 0.014 min
Response: 1576819
Conc: 1.00 ug/ml

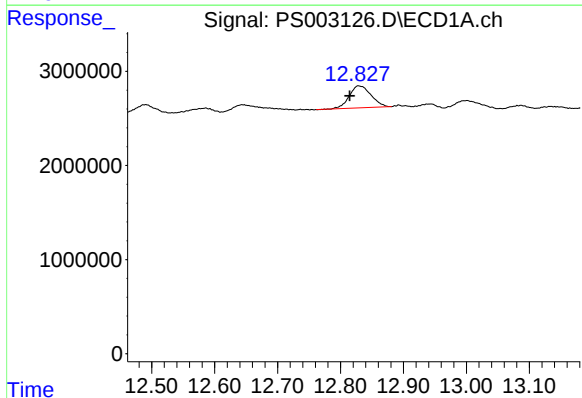


#8 DICHLORPROP

R.T.: 12.830 min
Delta R.T.: 0.015 min
Response: 5638989
Conc: 14.70 ng/ml

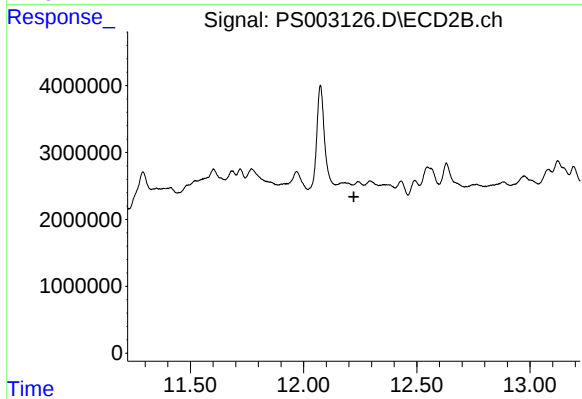

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.222 min
Response: 0
Conc: N.D.

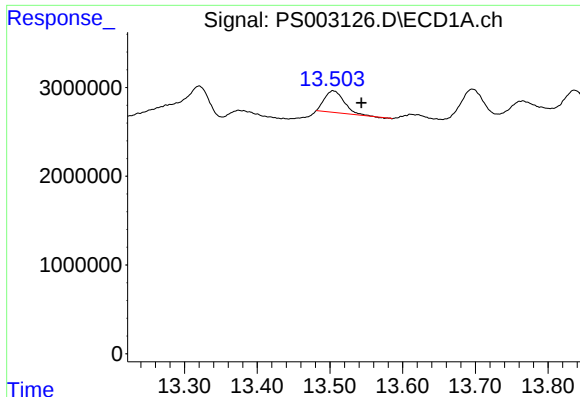

#10 Pentachlorophenol


R.T.: 13.505 min
Delta R.T.: -0.039 min
Response: 4568105
Conc: 0.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

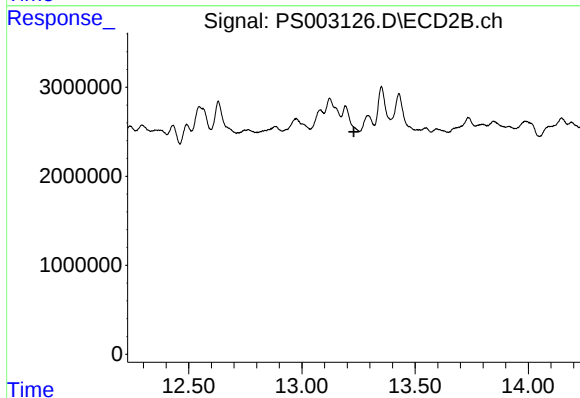


#10 Pentachlorophenol

R.T.: 13.292 min
Delta R.T.: 0.063 min
Response: -2485355
Conc: N.D.

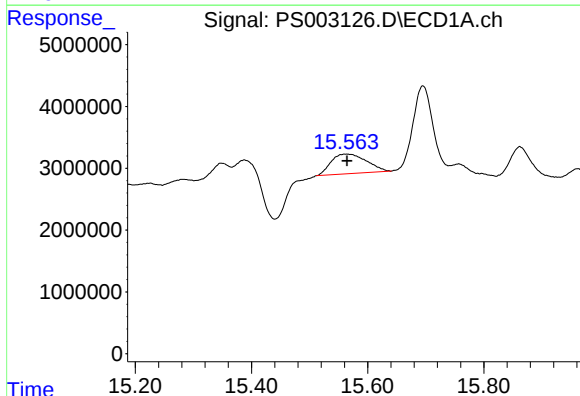


#13 2,4-DB

R.T.: 15.563 min
Delta R.T.: -0.001 min
Response: 13477531
Conc: 51.55 ng/ml

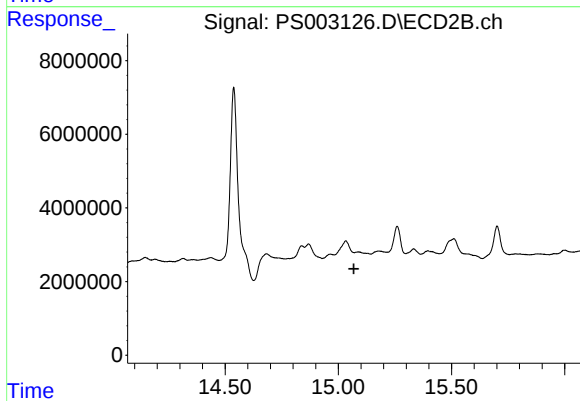

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.069 min
Response: 0
Conc: N.D.

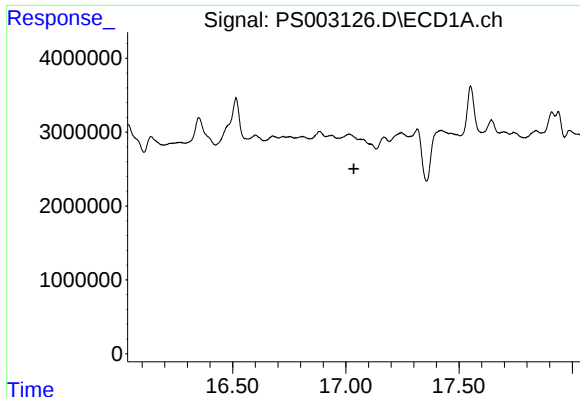

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

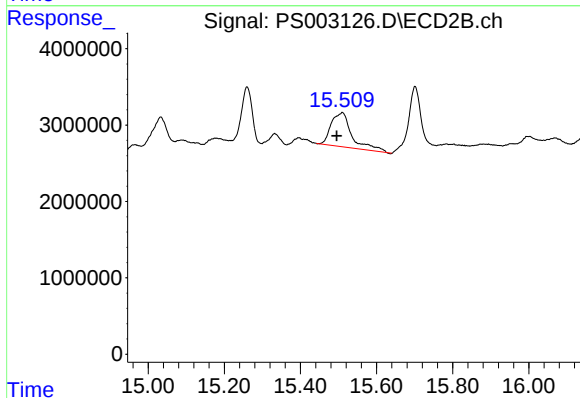


#14 DINOSEB

R.T.: 15.510 min
Delta R.T.: 0.015 min
Response: 16550569
Conc: 9.44 ng/ml

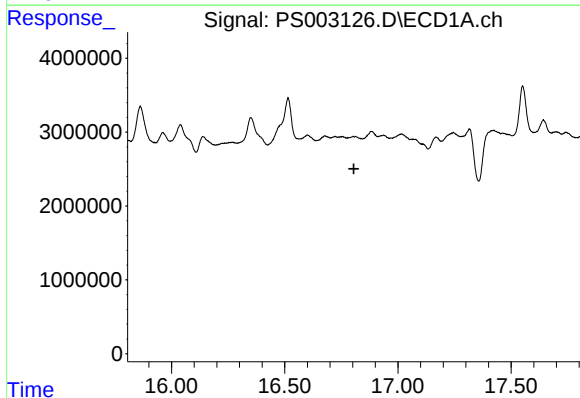


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

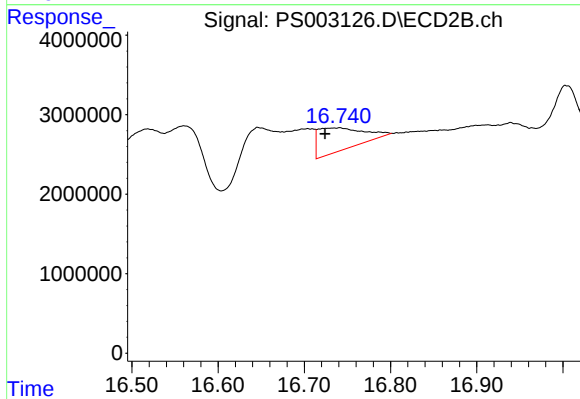

#15 Picloram


R.T.: 16.740 min
Delta R.T.: 0.016 min
Response: 10441605
Conc: 3.47 ng/ml

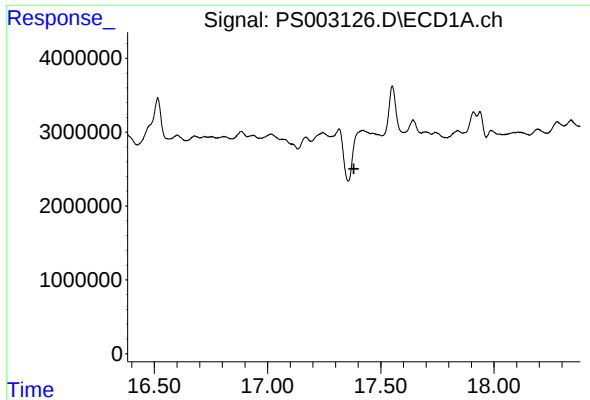

#16 DCPA

R.T.: 17.420 min
Delta R.T.: 0.039 min
Response: -14746924
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

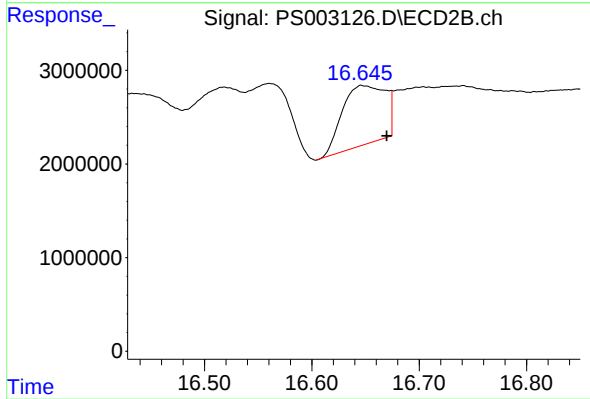

#16 DCPA

R.T.: 16.648 min
Delta R.T.: -0.022 min
Response: 17622122
Conc: 5.69 ng/ml