

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
 Data File : PS003117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 01:04
 Operator : EI\SJ
 Sample : K1356-06MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SU-03-020819-AMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 03:06:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.275	10.777	158.9E6	156.8E6	418.564m	366.829
Target Compounds							
1) T	Dalapon	2.844	2.314	253.5E6	302.2E6	459.538m	563.821
2) T	3,5-DICHL...	9.703	8.937	289.8E6	289.4E6	503.307m	513.447m
5) T	DICAMBA	11.581	11.057	877.4E6	854.1E6	547.367m	538.270m
6) T	MCP	11.927	11.288	90835475	56627435	75.815m	51.342m#
7) T	MCPA	12.173	11.663	114.7E6	78514392	64.794m	49.912m
8) T	DICHLORPROP	12.770	12.182	226.0E6	223.4E6	589.350m	584.387
9) T	2,4-D	13.129	12.652	278.3E6	303.4E6	603.538m	605.181m
10) T	Pentachlo...	13.499	13.188	2899.7E6	2800.2E6	452.155m	453.055m
11) T	2,4,5-TP ...	14.375	13.814	1410.6E6	1367.5E6	560.119	551.325m
12) T	2,4,5-T	14.773	14.376	1350.6E6	700.9E6	553.656	366.270m#
13) T	2,4-DB	15.521	15.028	151.7E6	149.1E6	580.263m	587.040m
14) T	DINOSEB	16.990	15.453	691.8E6	629.2E6	367.720	358.925m
15) T	Picloram	16.761	16.683	1578.1E6	1484.7E6	498.830	493.853
16) T	DCPA	17.335	16.628	1123.3E6	1186.8E6	373.522m	383.140m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021119\
Data File : PS003117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 01:04
Operator : EI\SJ
Sample : K1356-06MS
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SU-03-020819-AMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 03:06:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

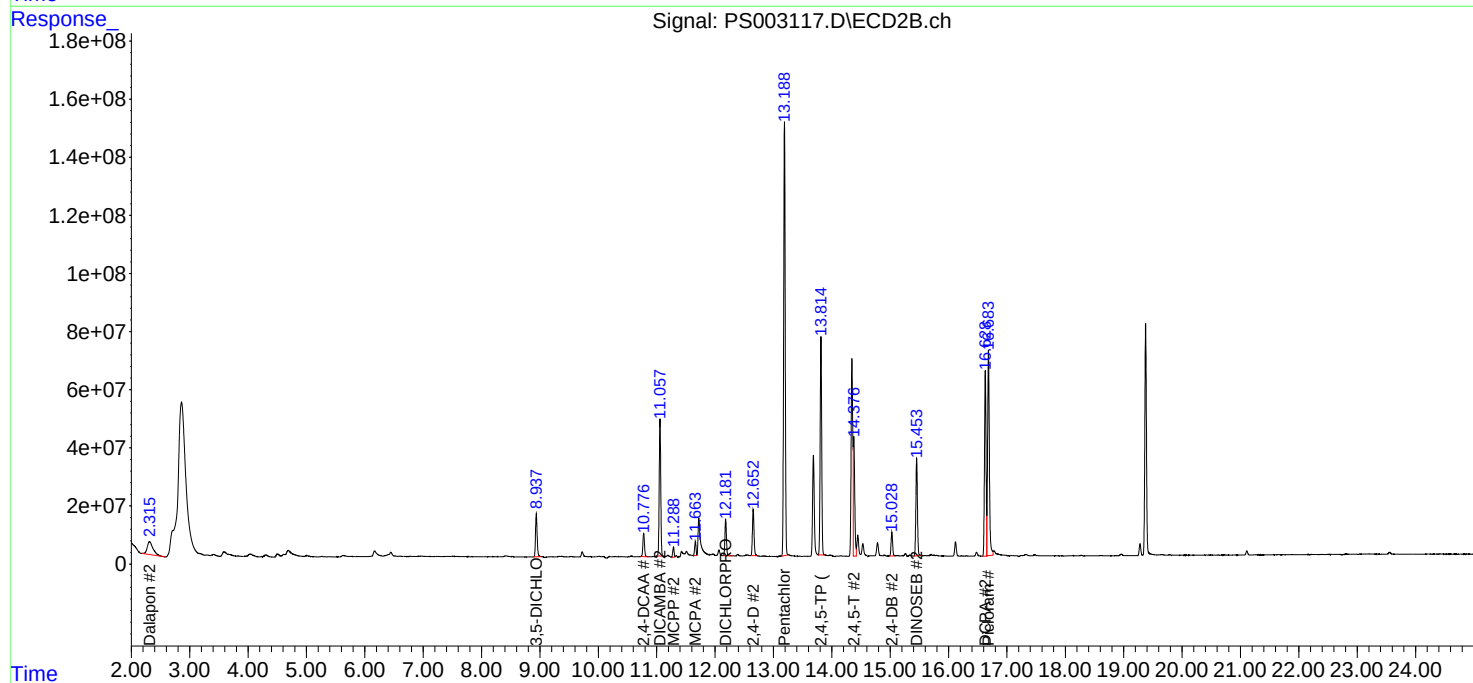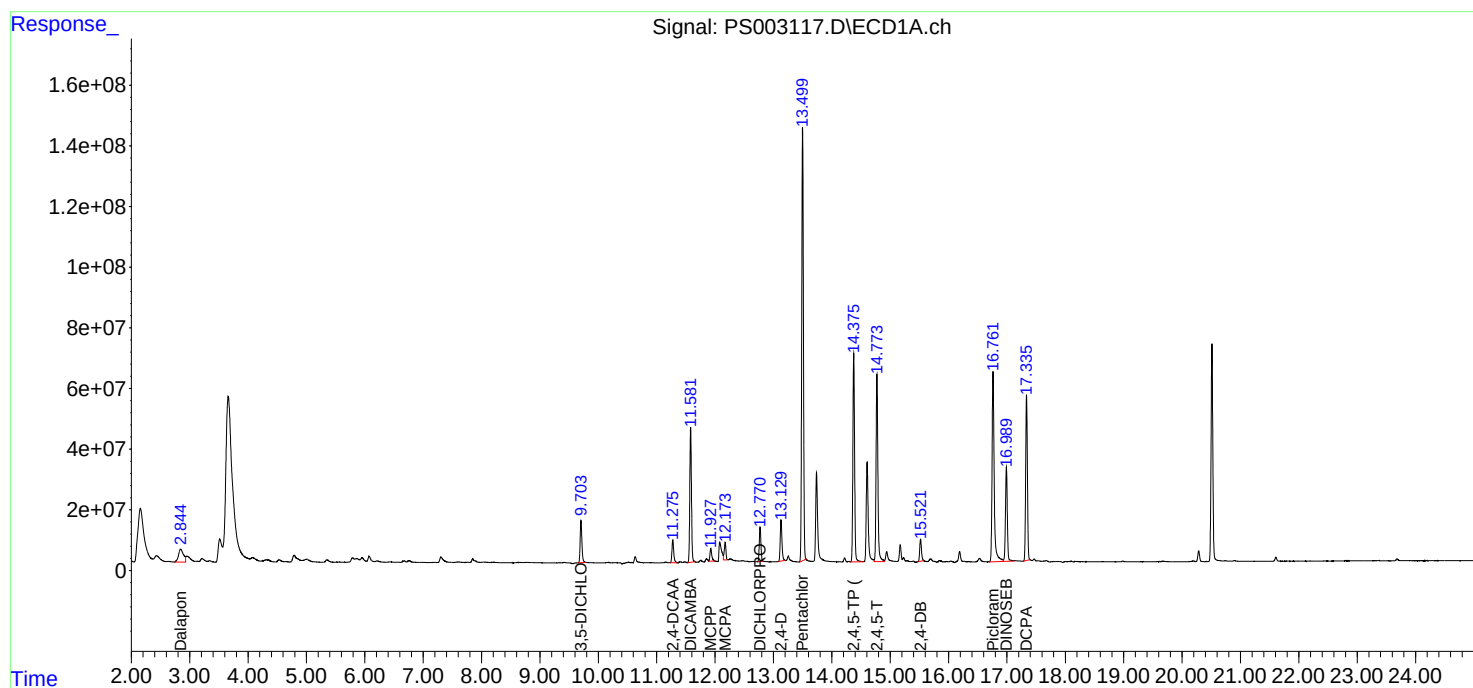


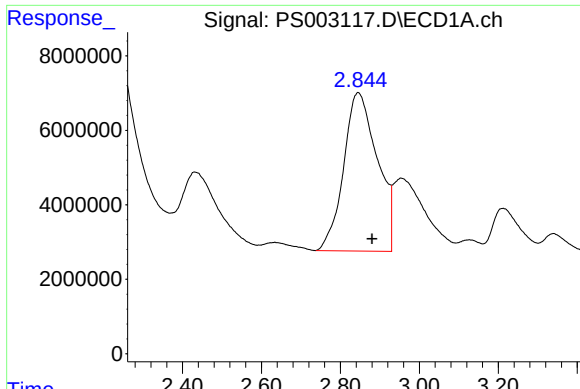

#1 Dalapon


R.T.: 2.844 min
Delta R.T.: -0.036 min
Response: 253502744
Conc: 459.54 ng/ml m

Instrument :
ECD_S
ClientSampleId :
SU-03-020819-AMS

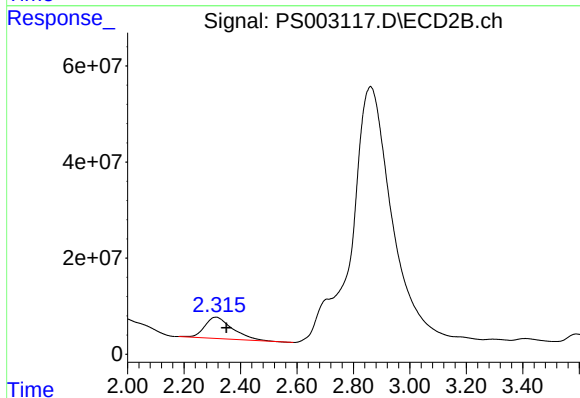


#1 Dalapon

R.T.: 2.314 min
Delta R.T.: -0.037 min
Response: 302163662
Conc: 563.82 ng/ml

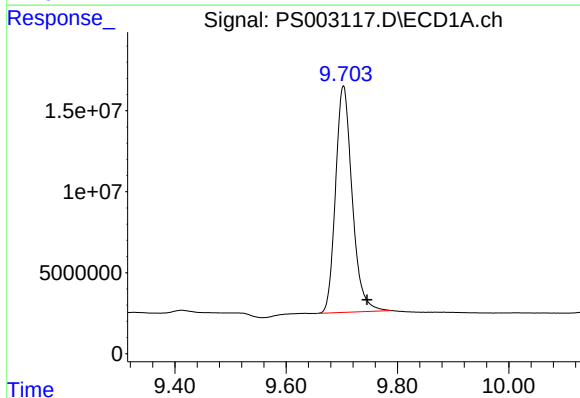


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.703 min
Delta R.T.: -0.043 min
Response: 289825811
Conc: 503.31 ng/ml m

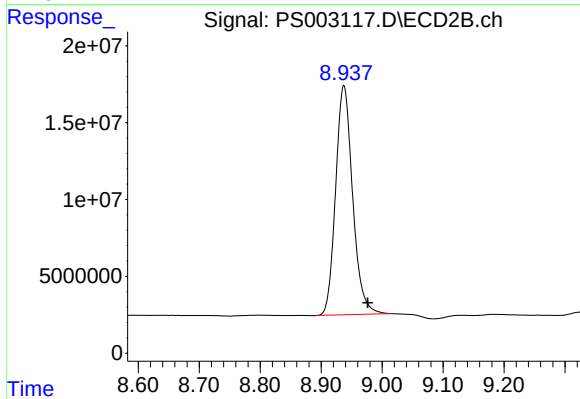

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.937 min
Delta R.T.: -0.039 min
Response: 289362383
Conc: 513.45 ng/ml m

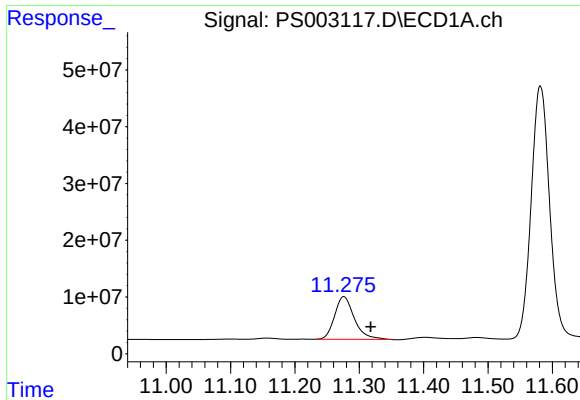

#4 2,4-DCAA


R.T.: 11.275 min
Delta R.T.: -0.042 min
Response: 158904051
Conc: 418.56 ng/ml m

Instrument :
ECD_S
ClientSampleId :
SU-03-020819-AMS

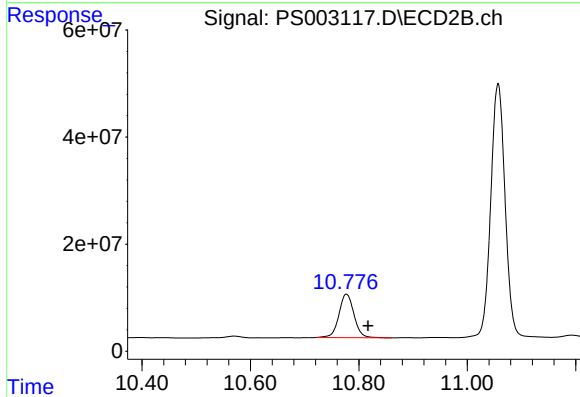


#4 2,4-DCAA

R.T.: 10.777 min
Delta R.T.: -0.040 min
Response: 156836212
Conc: 366.83 ng/ml

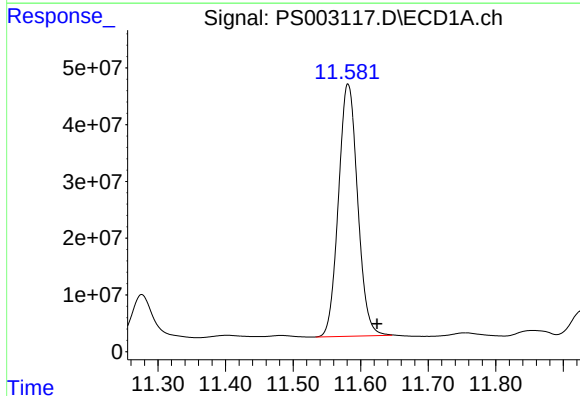


#5 DICAMBA

R.T.: 11.581 min
Delta R.T.: -0.044 min
Response: 877367870
Conc: 547.37 ng/ml m

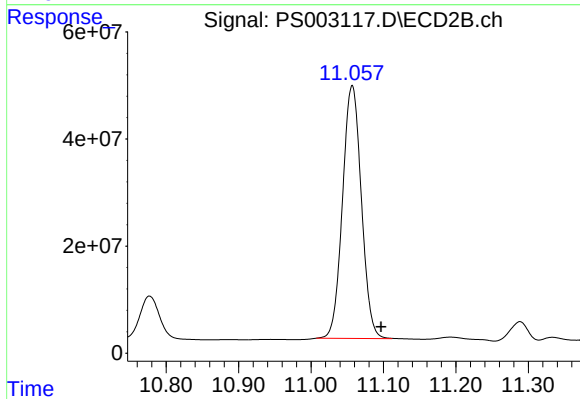

#5 DICAMBA


R.T.: 11.057 min
Delta R.T.: -0.040 min
Response: 854054440
Conc: 538.27 ng/ml m

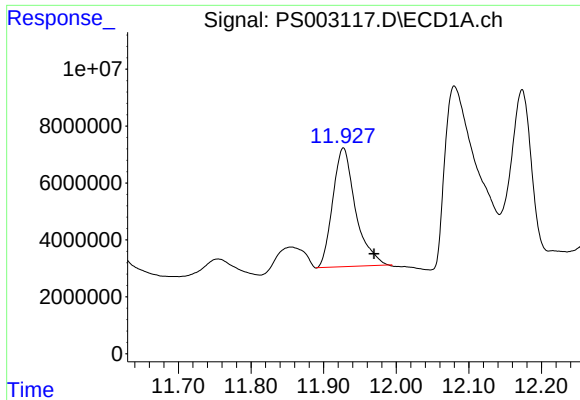

#6 MCPP


R.T.: 11.927 min
Delta R.T.: -0.043 min
Response: 90835475
Conc: 75.81 ug/ml m

Instrument :
ECD_S
ClientSampleId :
SU-03-020819-AMS

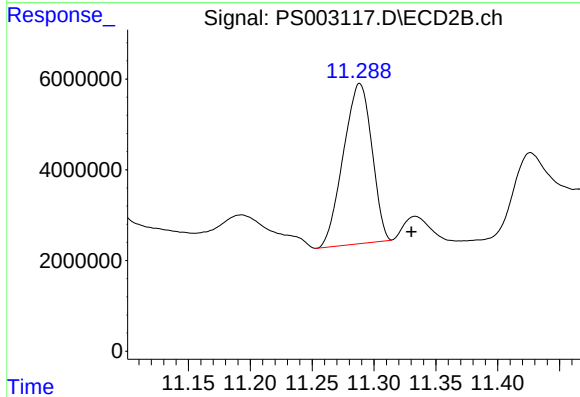


#6 MCPP

R.T.: 11.288 min
Delta R.T.: -0.042 min
Response: 56627435
Conc: 51.34 ug/ml m

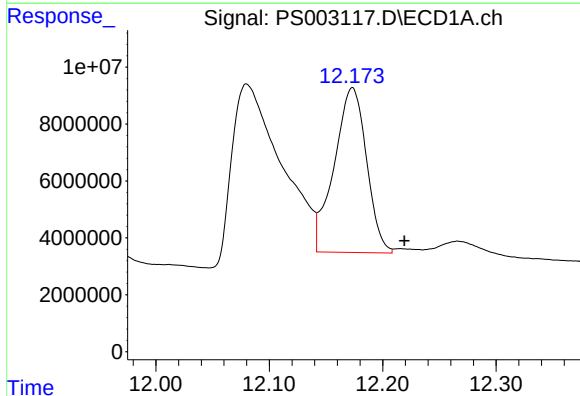


#7 MCPA

R.T.: 12.173 min
Delta R.T.: -0.046 min
Response: 114682306
Conc: 64.79 ug/ml m

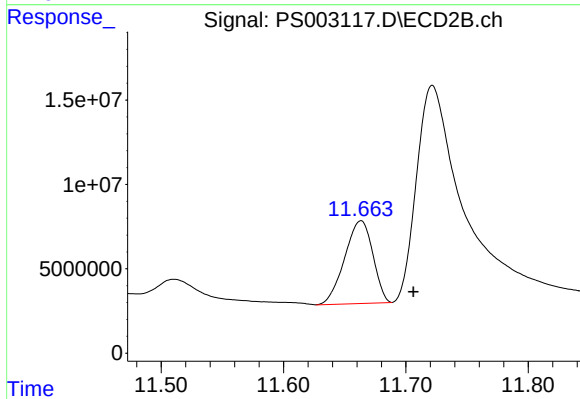

#7 MCPA


R.T.: 11.663 min
Delta R.T.: -0.043 min
Response: 78514392
Conc: 49.91 ug/ml m

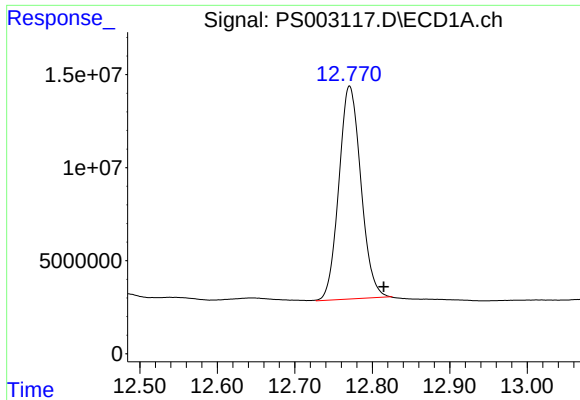

#8 DICHLORPROP


R.T.: 12.770 min
Delta R.T.: -0.044 min
Response: 226033685
Conc: 589.35 ng/ml m

Instrument :
ECD_S
ClientSampleId :
SU-03-020819-AMS

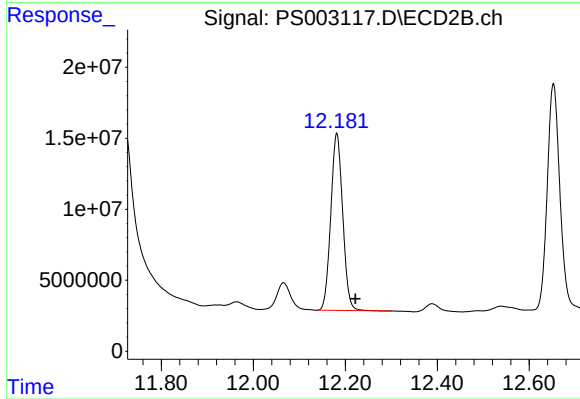


#8 DICHLORPROP

R.T.: 12.182 min
Delta R.T.: -0.041 min
Response: 223435131
Conc: 584.39 ng/ml

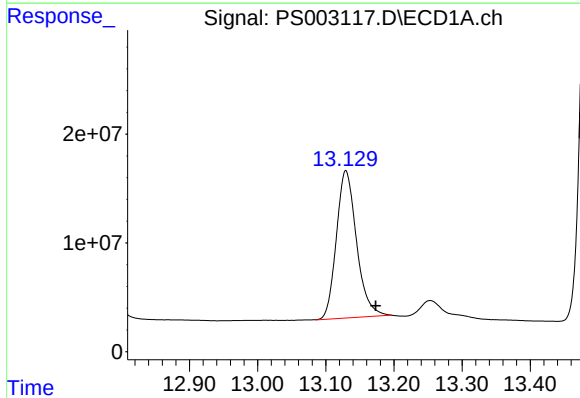


#9 2,4-D

R.T.: 13.129 min
Delta R.T.: -0.044 min
Response: 278266282
Conc: 603.54 ng/ml m

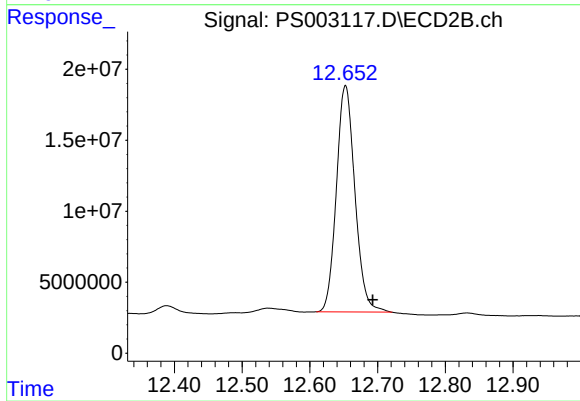

#9 2,4-D


R.T.: 12.652 min
Delta R.T.: -0.041 min
Response: 303429140
Conc: 605.18 ng/ml m

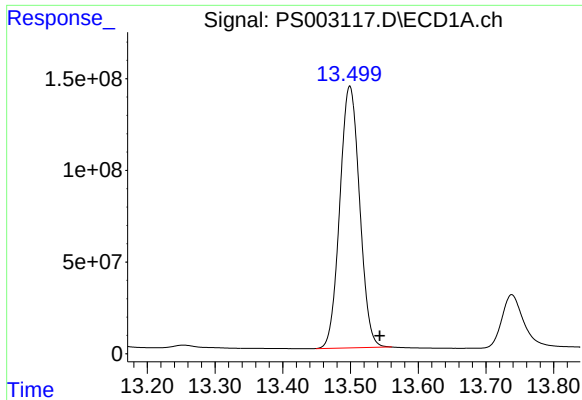

#10 Pentachlorophenol


R.T.: 13.499 min
Delta R.T.: -0.045 min
Response: 2899665890
Conc: 452.15 ng/ml m

Instrument :
ECD_S
ClientSampleId :
SU-03-020819-AMS

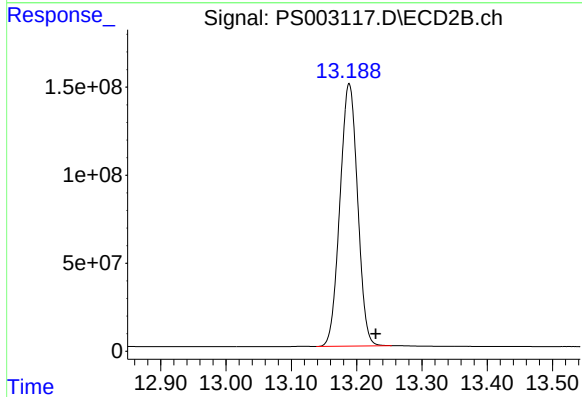


#10 Pentachlorophenol

R.T.: 13.188 min
Delta R.T.: -0.041 min
Response: 2800157071
Conc: 453.06 ng/ml m

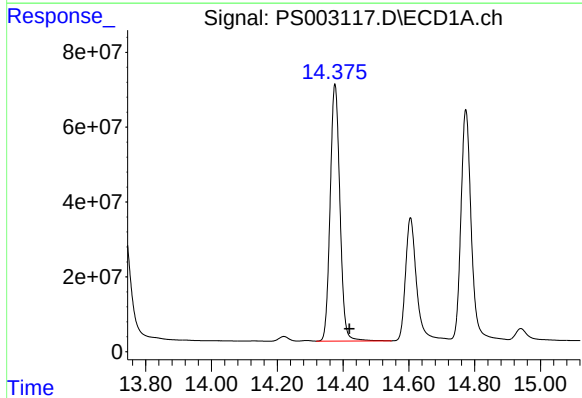


#11 2,4,5-TP (SILVEX)

R.T.: 14.375 min
Delta R.T.: -0.044 min
Response: 1410587612
Conc: 560.12 ng/ml

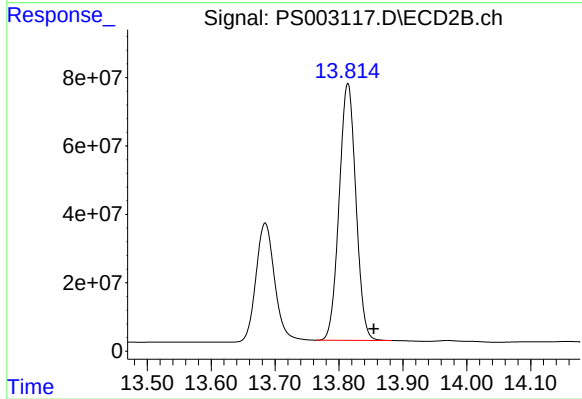

#11 2,4,5-TP (SILVEX)


R.T.: 13.814 min
Delta R.T.: -0.041 min
Response: 1367482019
Conc: 551.32 ng/ml m

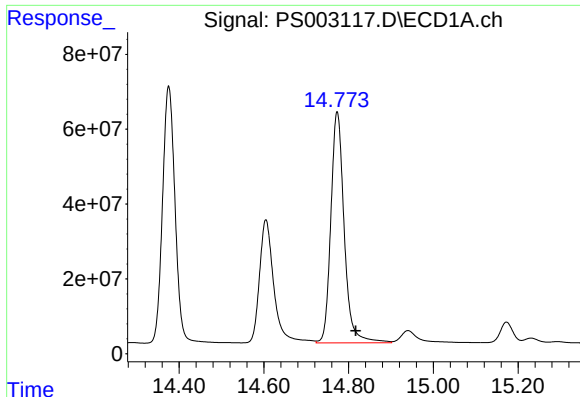

#12 2,4,5-T


R.T.: 14.773 min
Delta R.T.: -0.043 min
Response: 1350592246
Conc: 553.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-03-020819-AMS

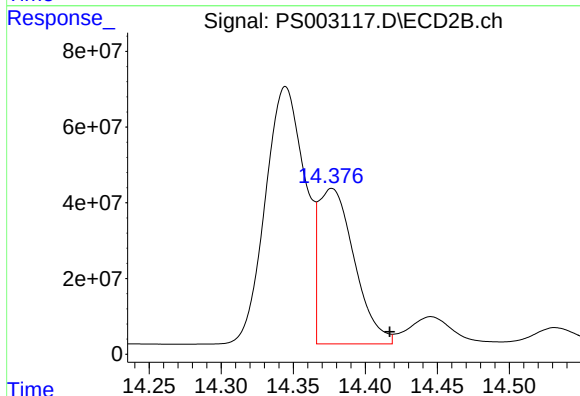


#12 2,4,5-T

R.T.: 14.376 min
Delta R.T.: -0.041 min
Response: 700853840
Conc: 366.27 ng/ml m

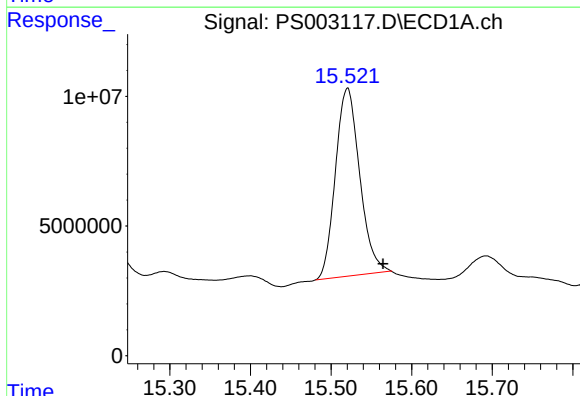


#13 2,4-DB

R.T.: 15.521 min
Delta R.T.: -0.044 min
Response: 151697260
Conc: 580.26 ng/ml m

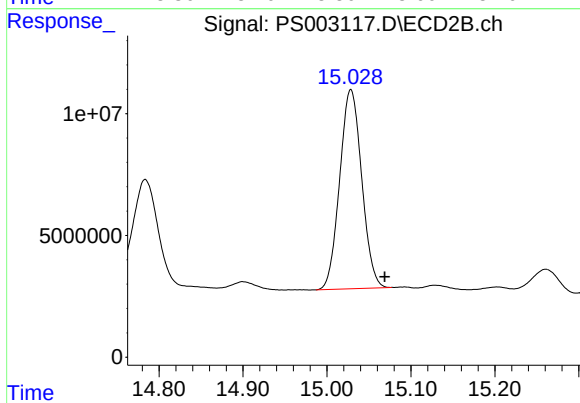

#13 2,4-DB


R.T.: 15.028 min
Delta R.T.: -0.041 min
Response: 149107857
Conc: 587.04 ng/ml m

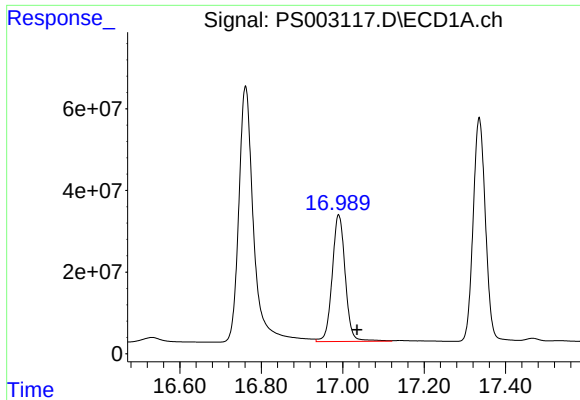

#14 DINOSEB


R.T.: 16.990 min
Delta R.T.: -0.045 min
Response: 691801225
Conc: 367.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-03-020819-AMS

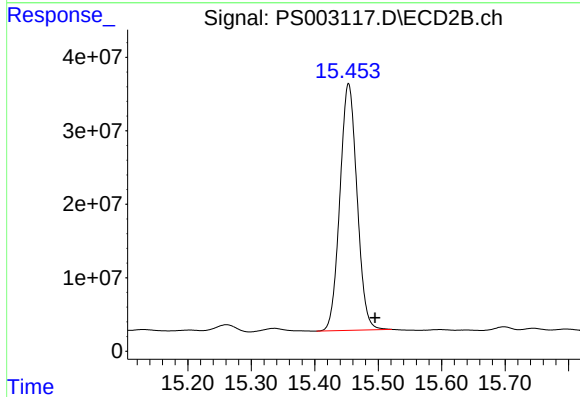


#14 DINOSEB

R.T.: 15.453 min
Delta R.T.: -0.042 min
Response: 629193994
Conc: 358.92 ng/ml m

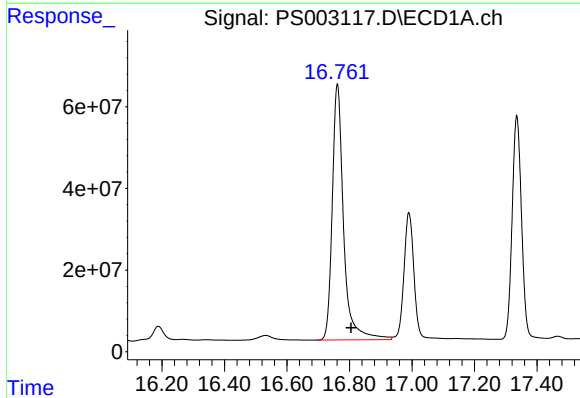


#15 Picloram

R.T.: 16.761 min
Delta R.T.: -0.044 min
Response: 1578115576
Conc: 498.83 ng/ml

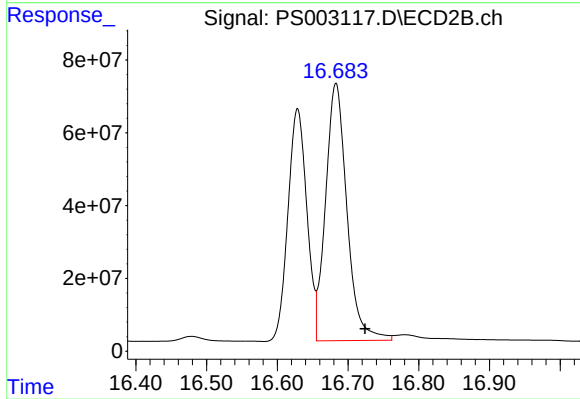

#15 Picloram


R.T.: 16.683 min
Delta R.T.: -0.041 min
Response: 1484719955
Conc: 493.85 ng/ml

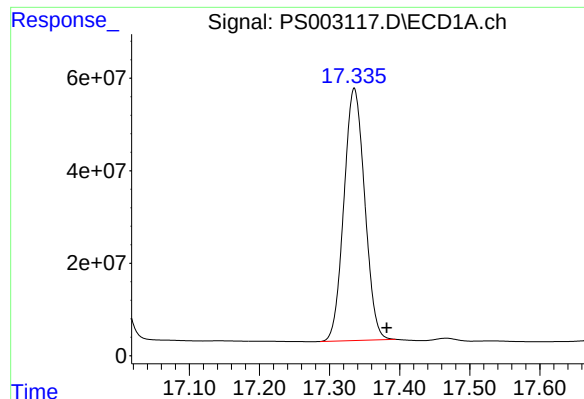

#16 DCPA

R.T.: 17.335 min
Delta R.T.: -0.047 min
Response: 1123291251
Conc: 373.52 ng/ml m

Instrument :
ECD_S
ClientSampleId :
SU-03-020819-AMS

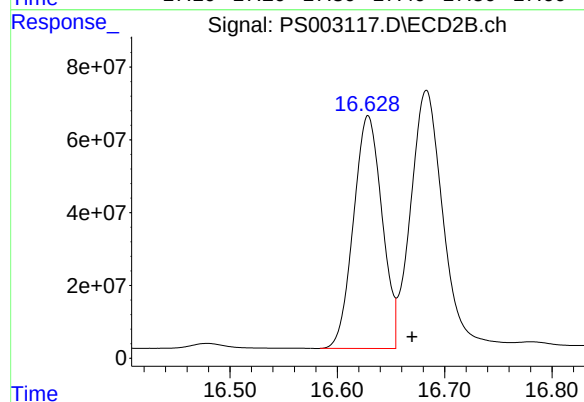

#16 DCPA

R.T.: 16.628 min
Delta R.T.: -0.042 min
Response: 1186810290
Conc: 383.14 ng/ml m