

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021120\
 Data File : PS008784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2020 15:47
 Operator : DD\AJ
 Sample : L1437-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 03:30:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.249	6.943	1061.8E6	514.0E6	494.692	554.567
Target Compounds							
1) T	Dalapon	0.000	2.597	0	299.7E6	N.D.	249.887
2) T	3,5-DICHL...	0.000	6.117	0	155.7E6	N.D.	113.199
6) T	MCP	7.689	0.000	114.2E6	0	18.586	N.D. #
7) T	MCPA	7.802	7.412	65266423	49537920	7.598	11.869 #
8) T	DICHLORPROP	0.000	7.765	0	79498885	N.D.	83.446
11) T	2,4,5-TP ...	0.000	8.800	0	156.5E6	N.D.	30.538
14) T	DINOSEB	11.199	0.000	81077592	0	9.608	N.D. #
15) T	Picloram	11.080	0.000	391.7E6	0	25.866	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021120\
Data File : PS008784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2020 15:47
Operator : DD\AJ
Sample : L1437-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 03:30:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

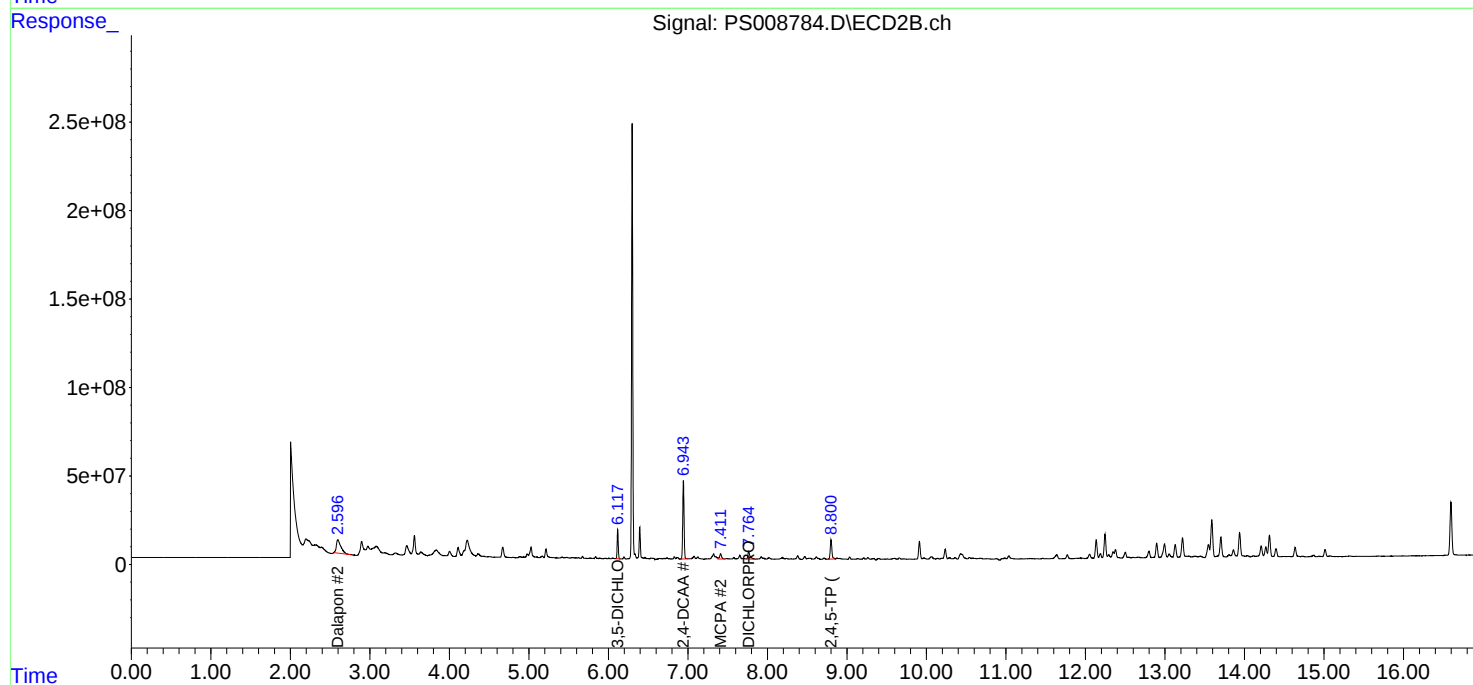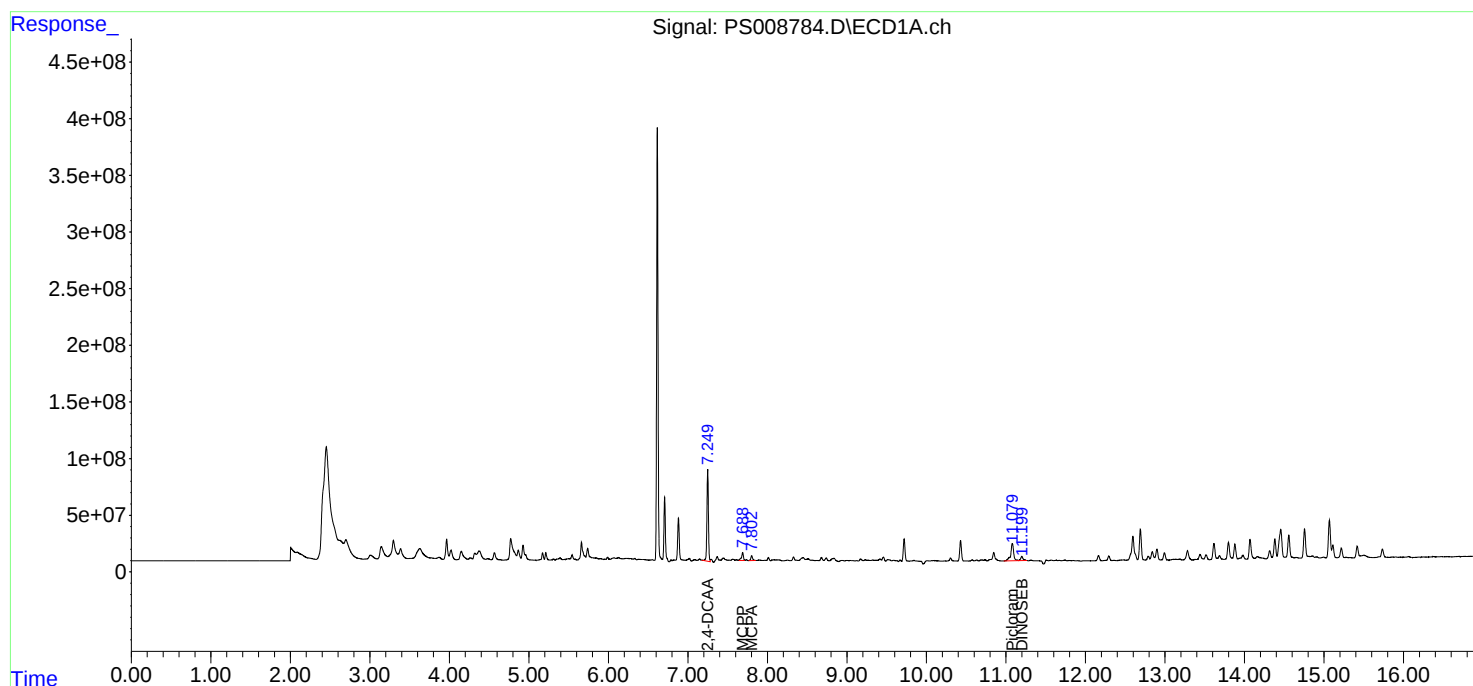


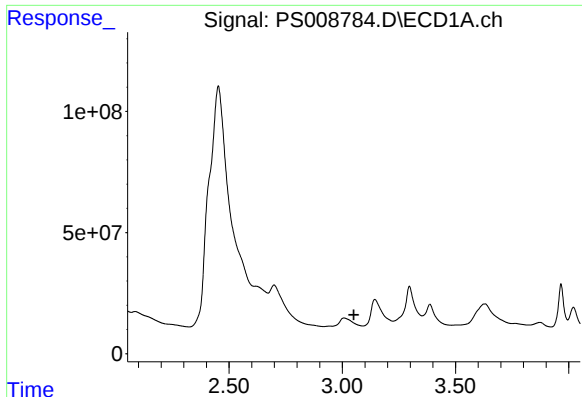

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

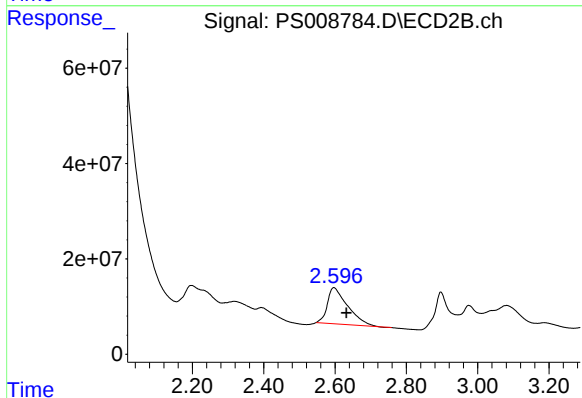


#1 Dalapon

R.T.: 2.597 min
Delta R.T.: -0.035 min
Response: 299693385
Conc: 249.89 ng/ml

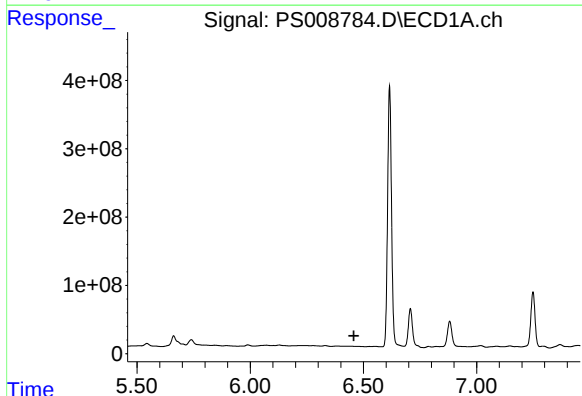


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.458 min
Response: 0
Conc: N.D.

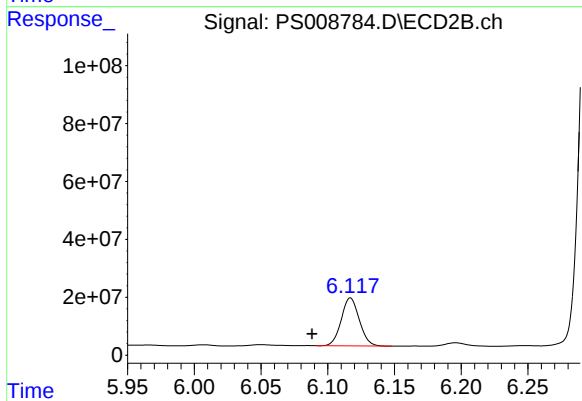

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.117 min
Delta R.T.: 0.029 min
Response: 155748935
Conc: 113.20 ng/ml

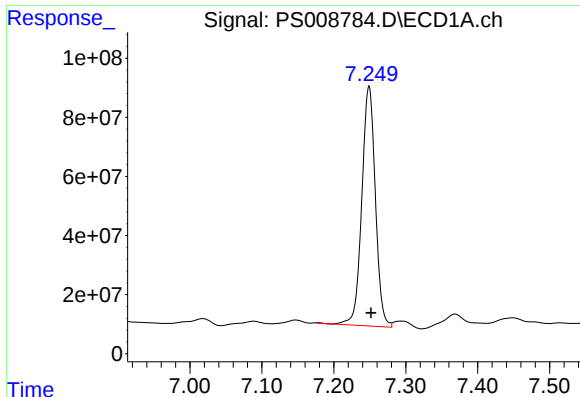

#4 2,4-DCAA


R.T.: 7.249 min
Delta R.T.: -0.003 min
Response: 1061761808
Conc: 494.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

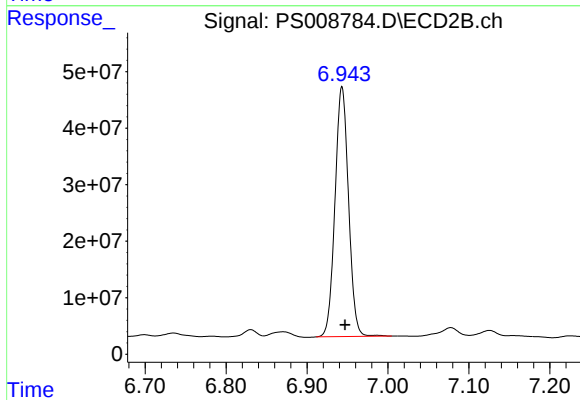


#4 2,4-DCAA

R.T.: 6.943 min
Delta R.T.: -0.004 min
Response: 513985815
Conc: 554.57 ng/ml

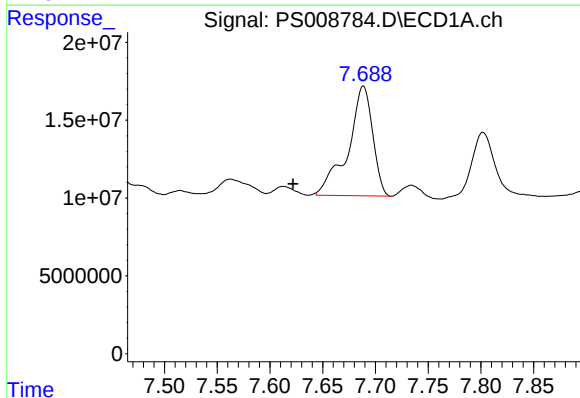


#6 MCP

R.T.: 7.689 min
Delta R.T.: 0.067 min
Response: 114242213
Conc: 18.59 ug/ml

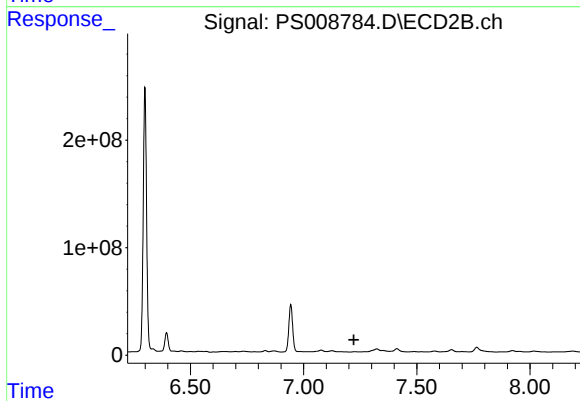

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.222 min
Response: 0
Conc: N.D.

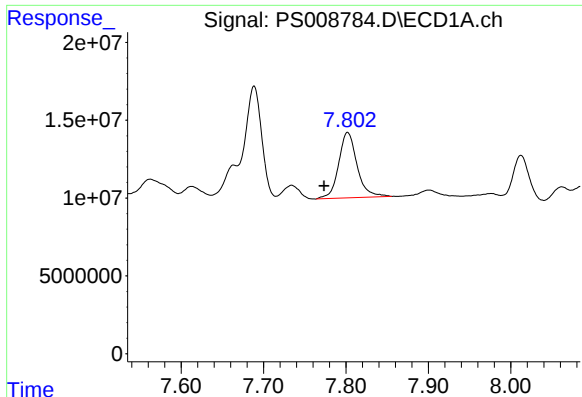

#7 MCPA


R.T.: 7.802 min
Delta R.T.: 0.029 min
Response: 65266423
Conc: 7.60 ug/ml

Instrument :
ECD_S
ClientSampleId :

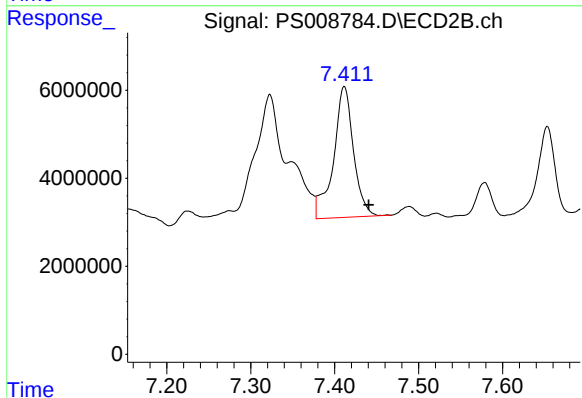


#7 MCPA

R.T.: 7.412 min
Delta R.T.: -0.029 min
Response: 49537920
Conc: 11.87 ug/ml

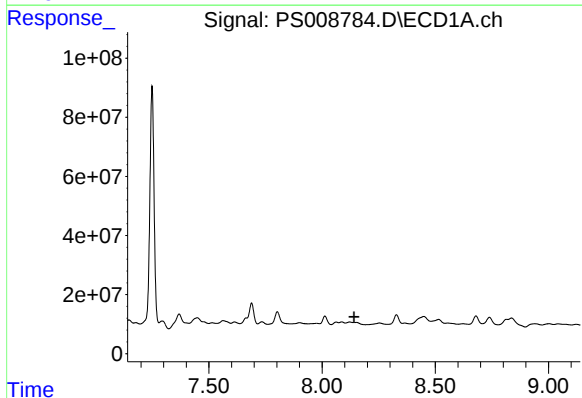


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.141 min
Response: 0
Conc: N.D.

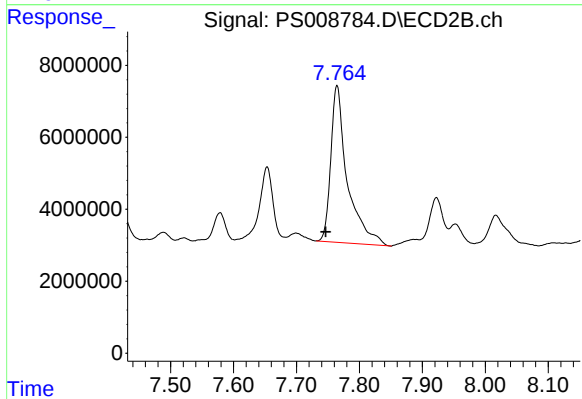

#8 DICHLORPROP


R.T.: 7.765 min
Delta R.T.: 0.018 min
Response: 79498885
Conc: 83.45 ng/ml

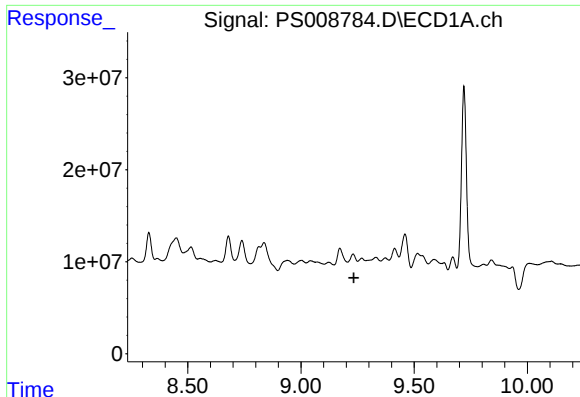

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.234 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

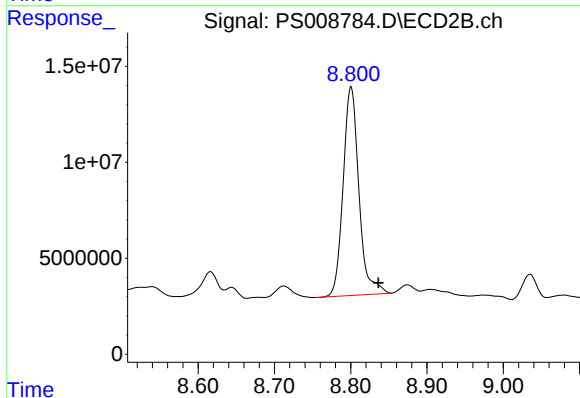


#11 2,4,5-TP (SILVEX)

R.T.: 8.800 min
Delta R.T.: -0.036 min
Response: 156511610
Conc: 30.54 ng/ml

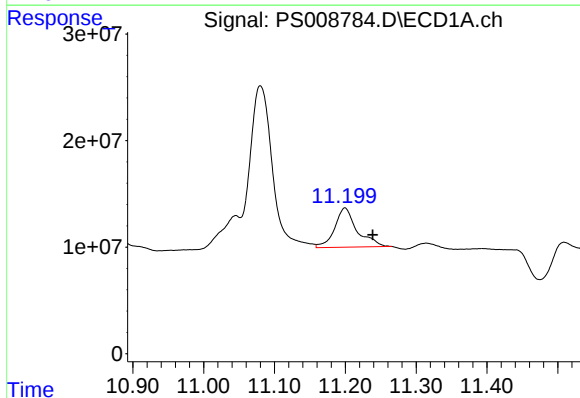


#14 DINOSEB

R.T.: 11.199 min
Delta R.T.: -0.039 min
Response: 81077592
Conc: 9.61 ng/ml

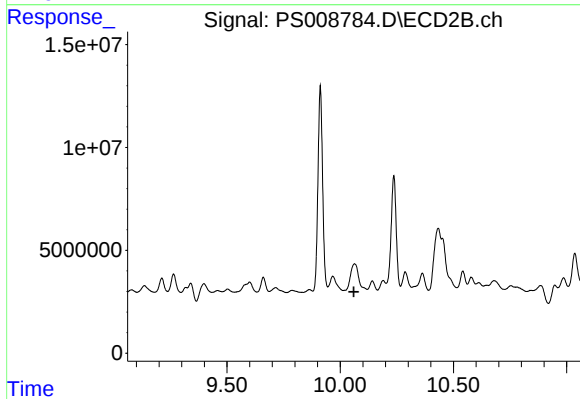

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 10.061 min
Response: 0
Conc: N.D.

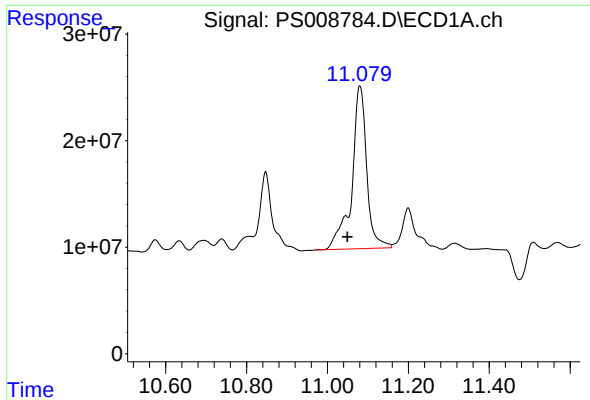

#15 Picloram

R.T.: 11.080 min
Delta R.T.: 0.030 min
Response: 391703083
Conc: 25.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

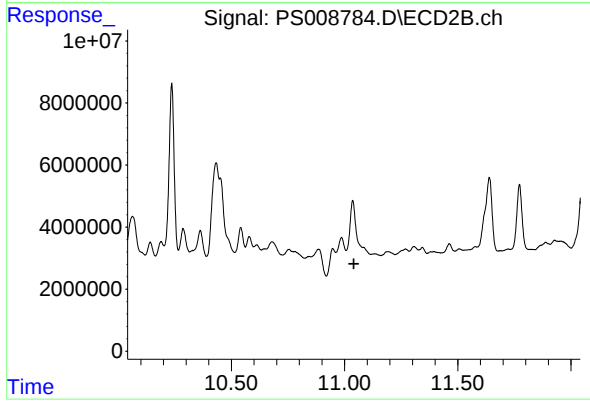

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.041 min
Response: 0
Conc: N.D.