

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021120\
 Data File : PS008789.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2020 17:41
 Operator : DD\AJ
 Sample : PB126747TB
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 03:32:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.249	6.944	1036.1E6	468.3E6	482.740	505.225
Target Compounds							
1) T	Dalapon	0.000	2.596	0	268.6E6	N.D.	223.949
2) T	3,5-DICHL...	0.000	6.117	0	167.2E6	N.D.	121.503



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021120\
Data File : PS008789.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2020 17:41
Operator : DD\AJ
Sample : PB126747TB
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 03:32:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

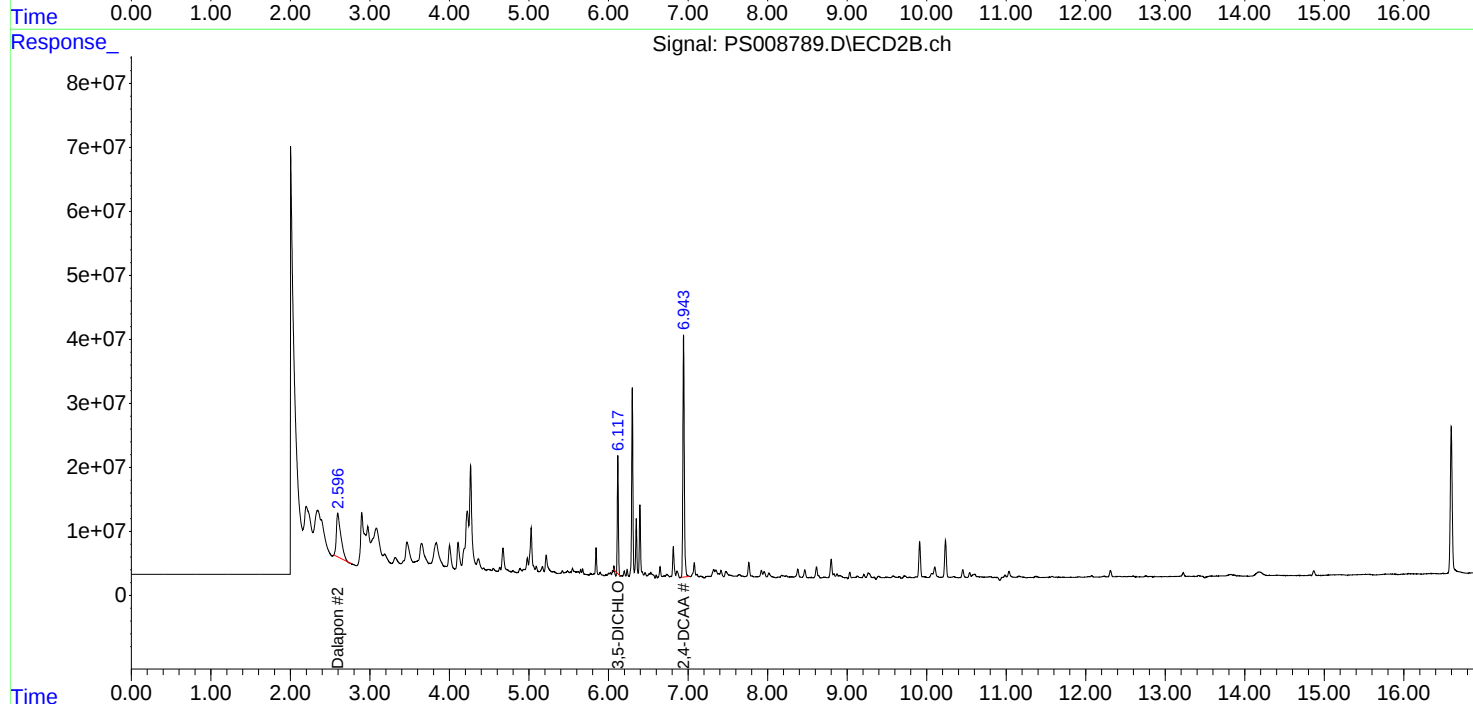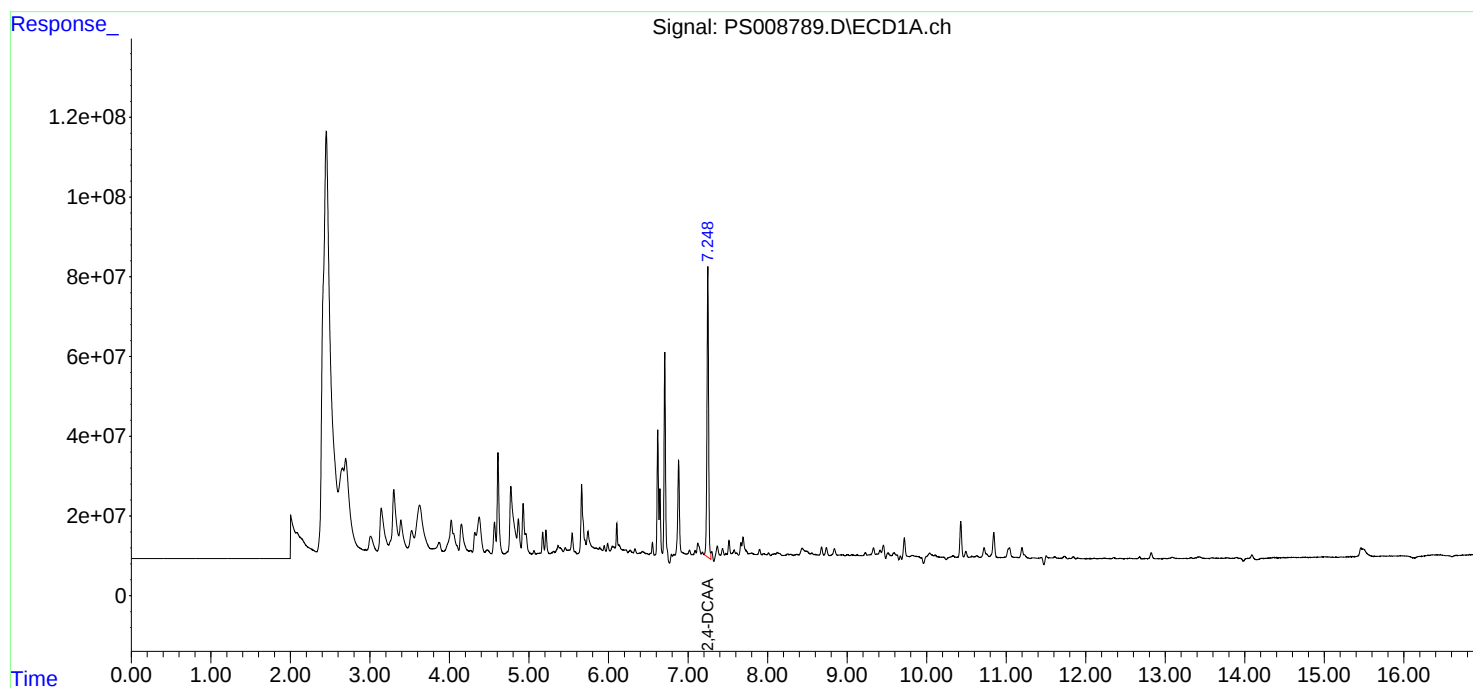


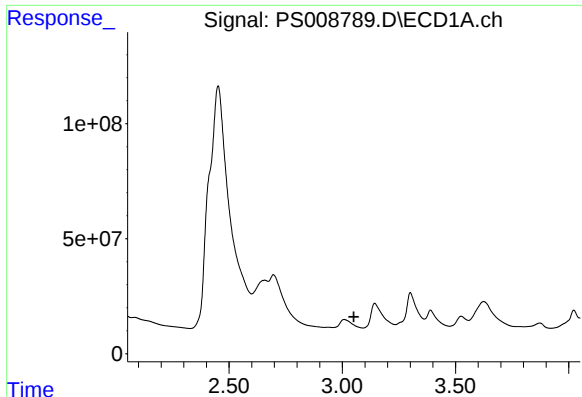

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

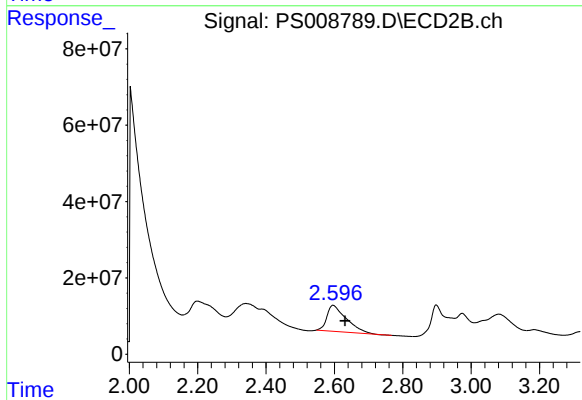


#1 Dalapon

R.T.: 2.596 min
Delta R.T.: -0.036 min
Response: 268586008
Conc: 223.95 ng/ml

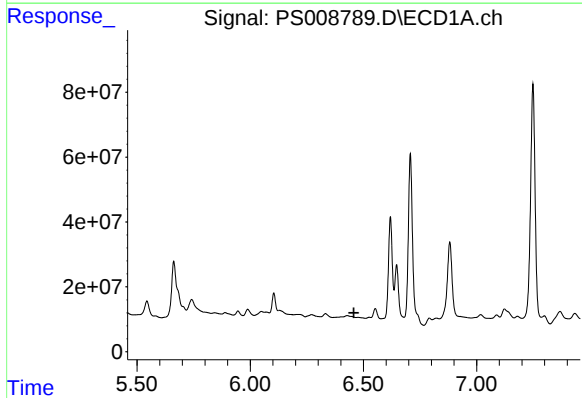


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.458 min
Response: 0
Conc: N.D.

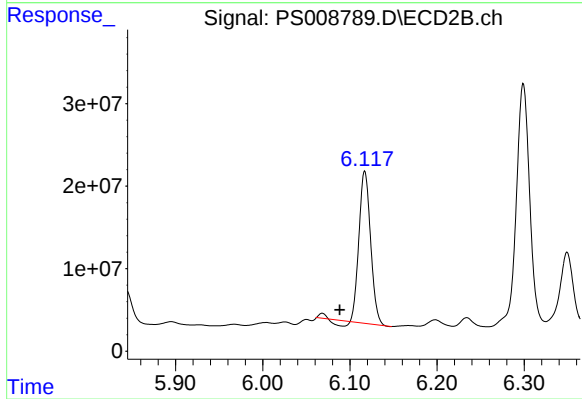

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.117 min
Delta R.T.: 0.029 min
Response: 167174413
Conc: 121.50 ng/ml

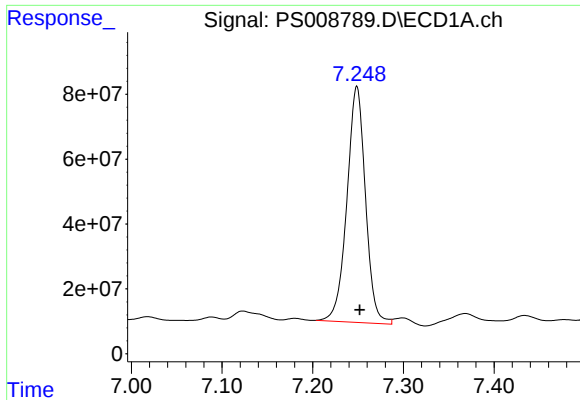

#4 2,4-DCAA

R.T.: 7.249 min
Delta R.T.: -0.003 min
Response: 1036109887
Conc: 482.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

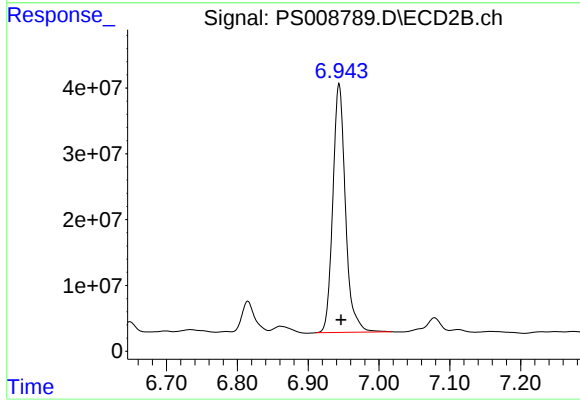

#4 2,4-DCAA

R.T.: 6.944 min
Delta R.T.: -0.003 min
Response: 468254532
Conc: 505.22 ng/ml