

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021120\
 Data File : PS008799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2020 21:30
 Operator : DD\AJ
 Sample : L1367-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 03:35:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.942	753.5E6	350.4E6	351.083	378.110
Target Compounds							
1) T	Dalapon	0.000	2.596	0	244.8E6	N.D.	204.151
2) T	3,5-DICHL...	0.000	6.117	0	139.0E6	N.D.	101.020
15) T	Picloram	11.045	11.034	296.8E6	153.2E6	19.596	20.294
16) T	DCPA	0.000	11.034	0	153.2E6	N.D.	23.552



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021120\
Data File : PS008799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2020 21:30
Operator : DD\AJ
Sample : L1367-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 03:35:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

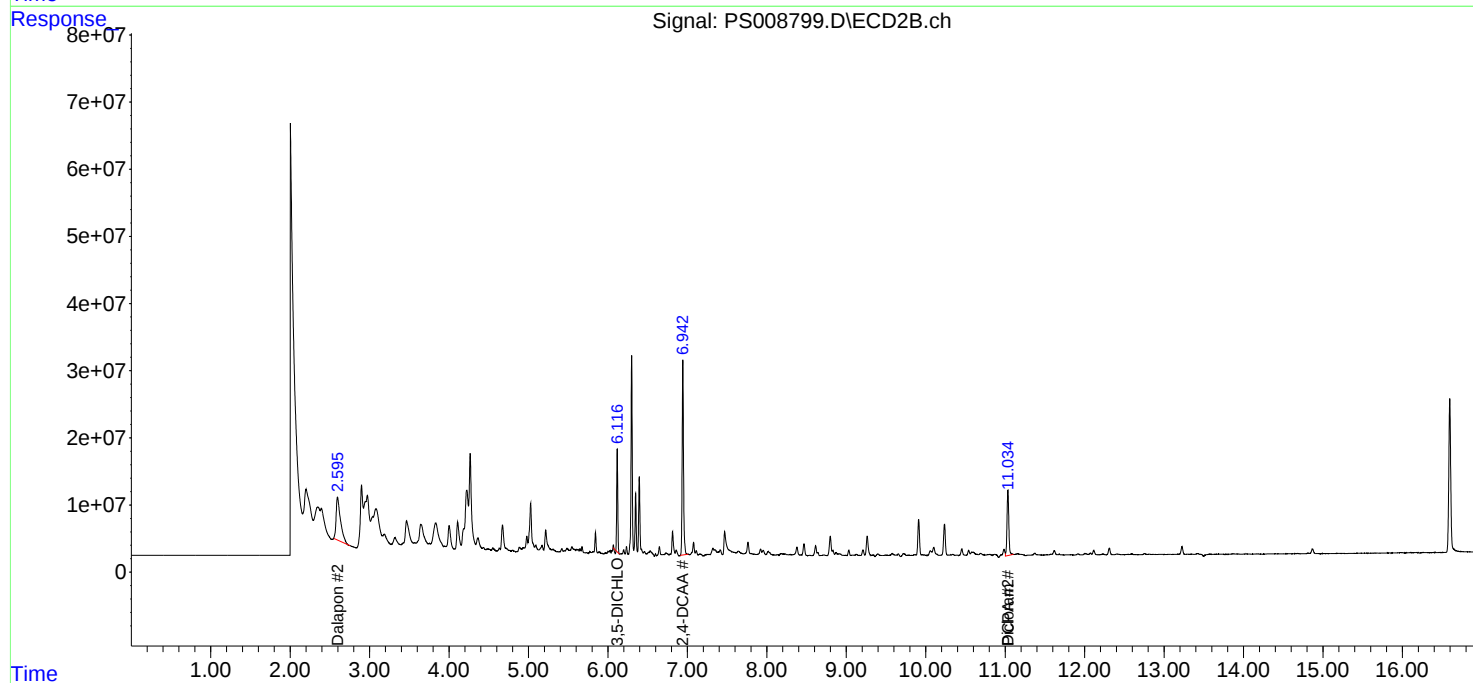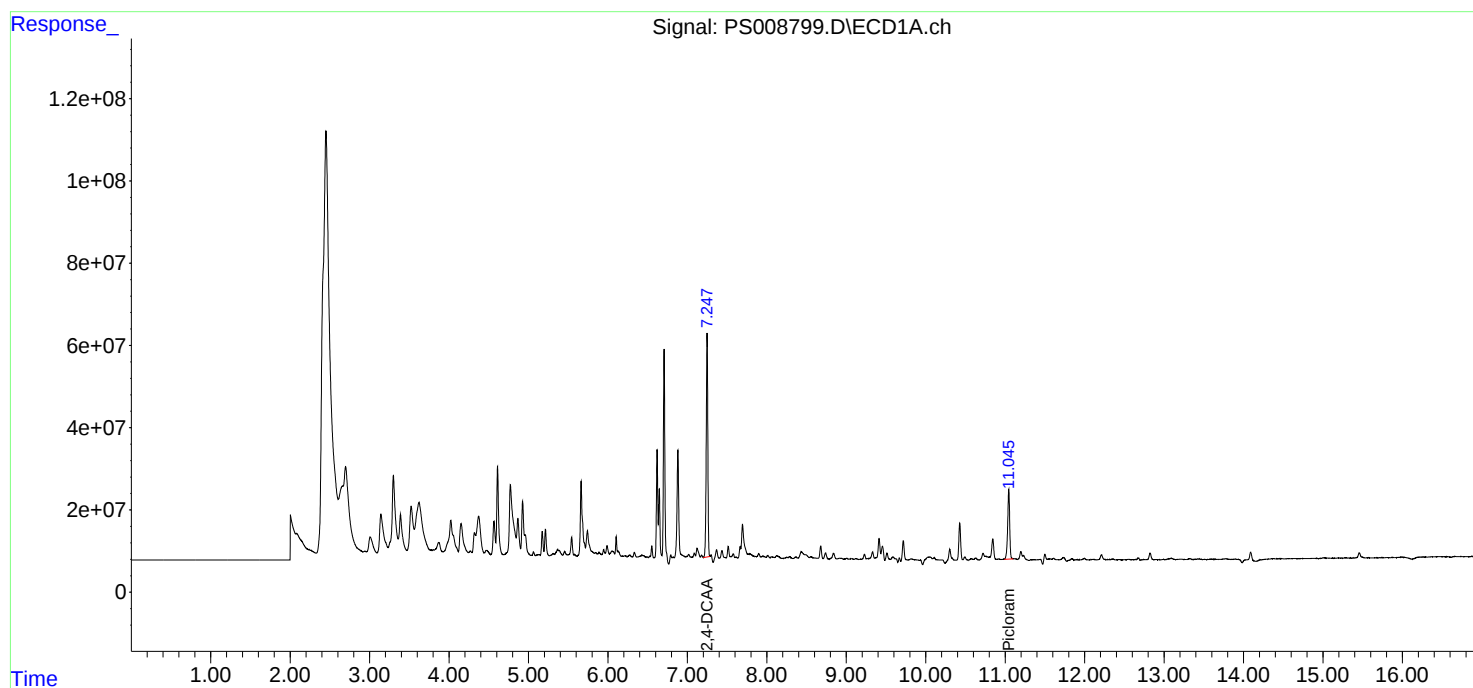


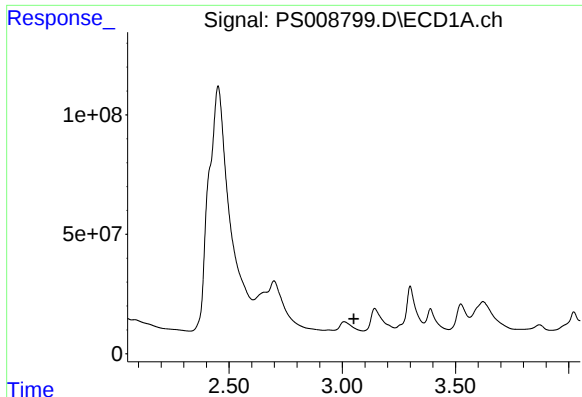

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

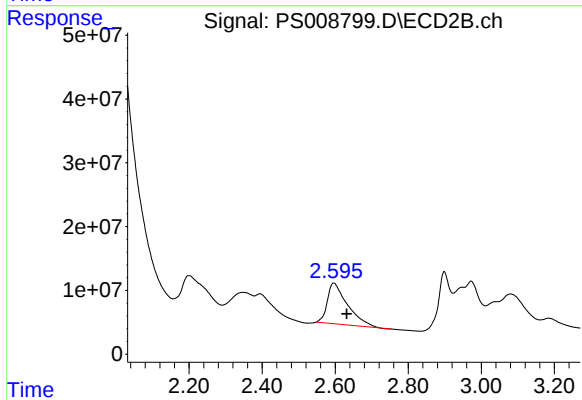


#1 Dalapon

R.T.: 2.596 min
Delta R.T.: -0.036 min
Response: 244842296
Conc: 204.15 ng/ml

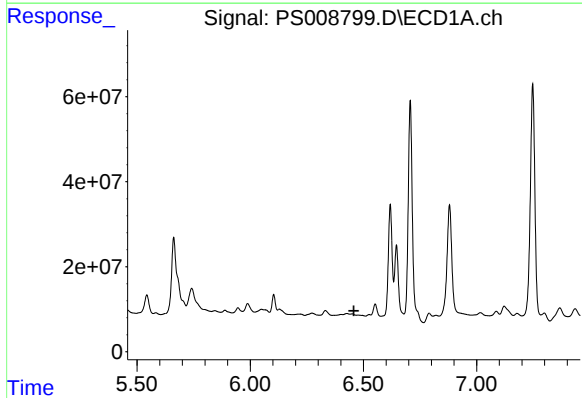


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

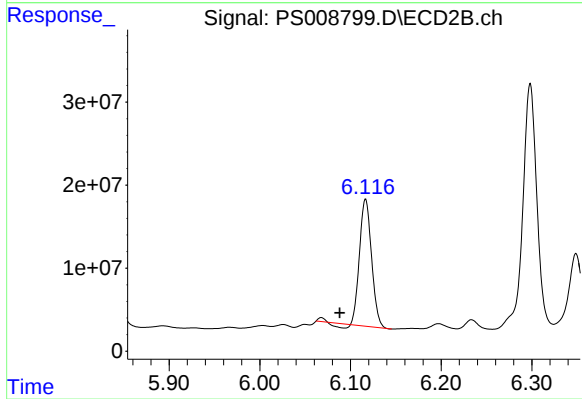

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.117 min
Delta R.T.: 0.028 min
Response: 138991316
Conc: 101.02 ng/ml

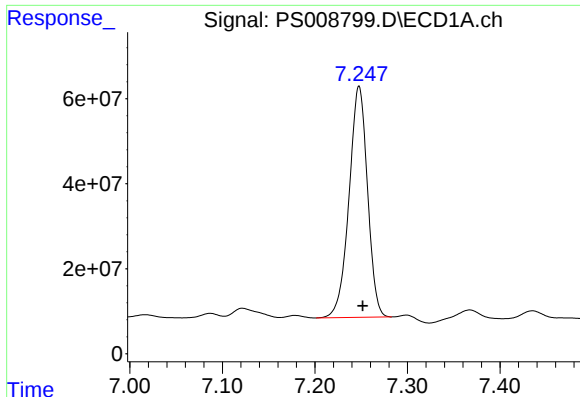

#4 2,4-DCAA


R.T.: 7.248 min
Delta R.T.: -0.004 min
Response: 753533018
Conc: 351.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

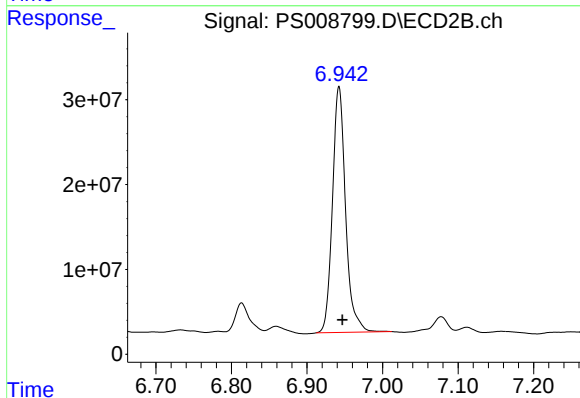


#4 2,4-DCAA

R.T.: 6.942 min
Delta R.T.: -0.004 min
Response: 350441552
Conc: 378.11 ng/ml

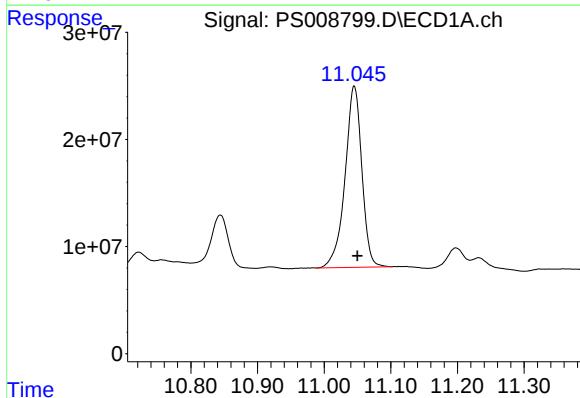


#15 Picloram

R.T.: 11.045 min
Delta R.T.: -0.005 min
Response: 296758604
Conc: 19.60 ng/ml

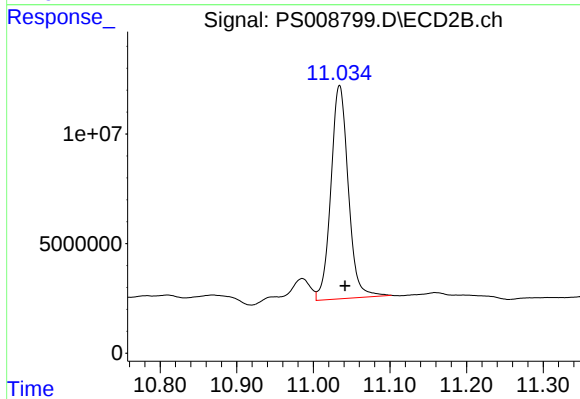

#15 Picloram


R.T.: 11.034 min
Delta R.T.: -0.007 min
Response: 153184045
Conc: 20.29 ng/ml

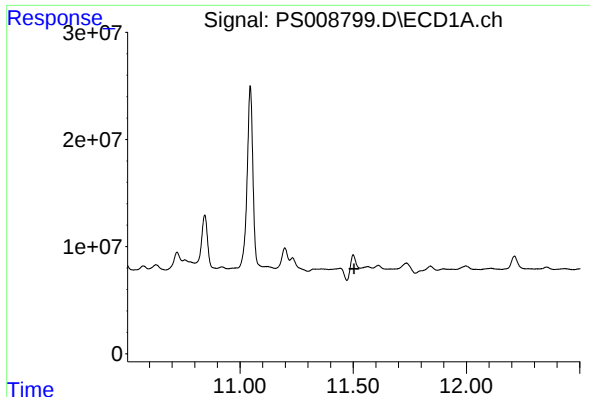

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.503 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

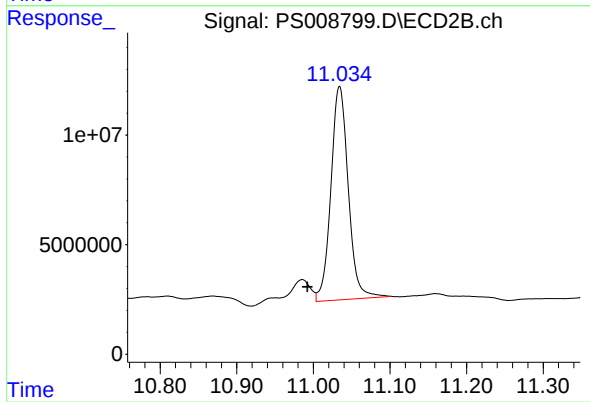

#16 DCPA

R.T.: 11.034 min
Delta R.T.: 0.042 min
Response: 153184045
Conc: 23.55 ng/ml