

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021120\
 Data File : PS008803.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2020 23:01
 Operator : DD\AJ
 Sample : L1421-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 03:36:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.943	869.8E6	245.3E6	405.265	264.645 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.117	0	118.0E6	N.D.	85.743
5) T	DICAMBA	7.376	0.000	326.5E6	0	40.477	N.D. #
7) T	MCPA	7.800	7.435	142.2E6	54027958	16.551	12.945
8) T	DICHLORPROP	0.000	7.815	0	64164472	N.D.	67.350
10) T	Pentachlo...	8.678	8.469	936.0E6	417.6E6	32.924	31.663
11) T	2,4,5-TP ...	0.000	8.800	0	132.5E6	N.D.	25.856
12) T	2,4,5-T	9.459	0.000	120.5E6	0	10.951	N.D. #
13) T	2,4-DB	10.078	0.000	29305784	0	18.017	N.D. #
14) T	DINOSEB	11.199	10.009	138.6E6	120.5E6	16.420	32.810 #
16) T	DCPA	11.513	0.000	153.4E6	0	10.942	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021120\
Data File : PS008803.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2020 23:01
Operator : DD\AJ
Sample : L1421-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 03:36:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

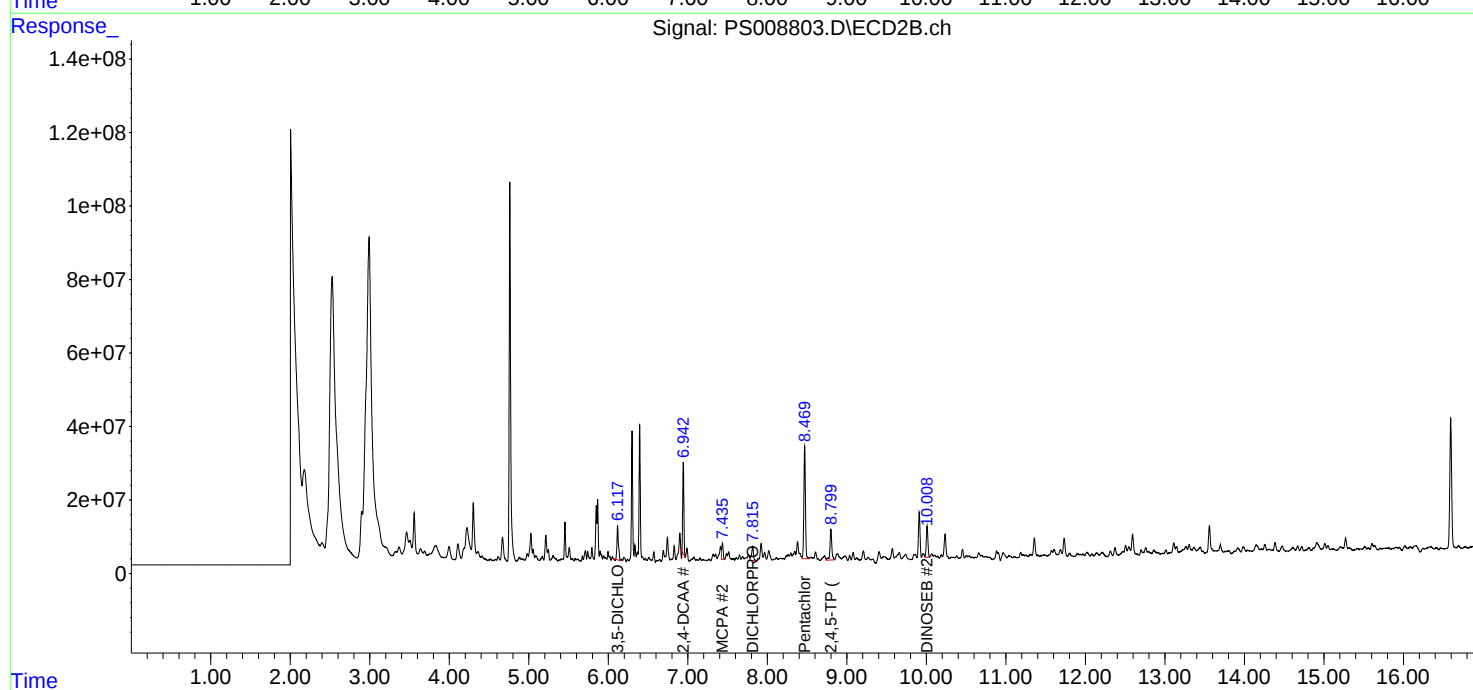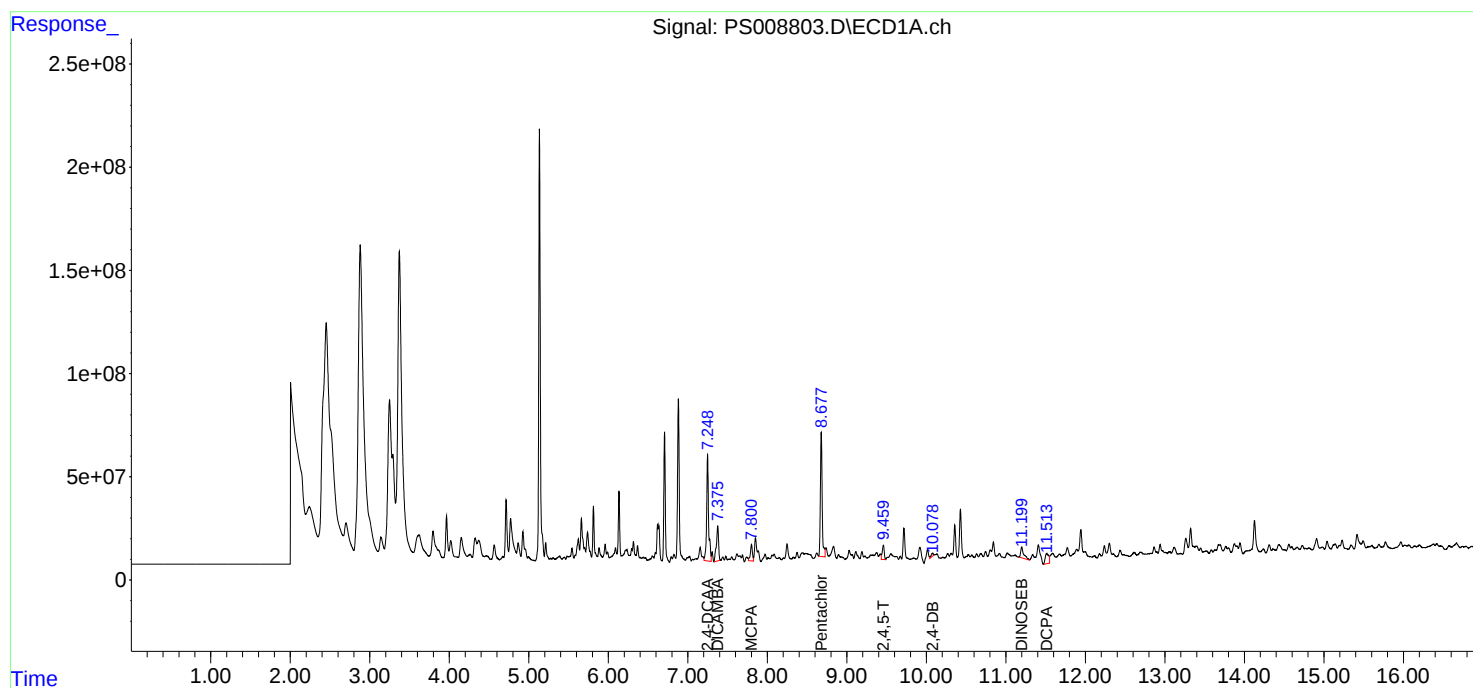


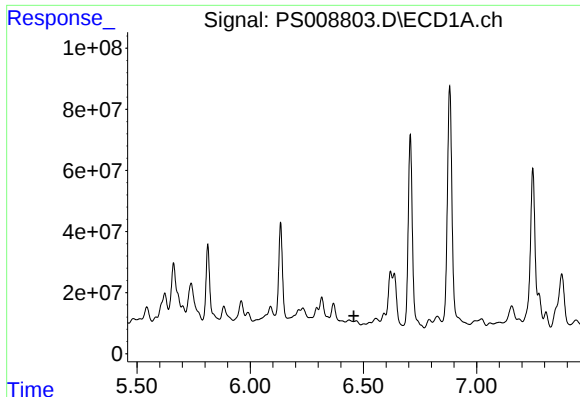

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

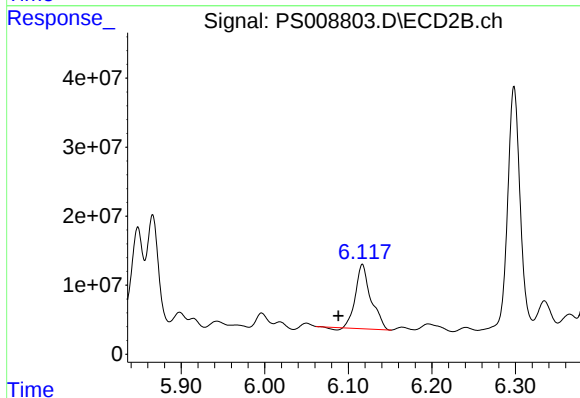


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.117 min
Delta R.T.: 0.029 min
Response: 117972872
Conc: 85.74 ng/ml

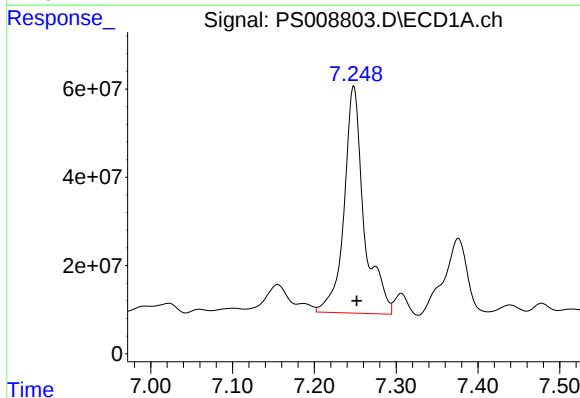


#4 2,4-DCAA

R.T.: 7.248 min
Delta R.T.: -0.004 min
Response: 869824297
Conc: 405.27 ng/ml

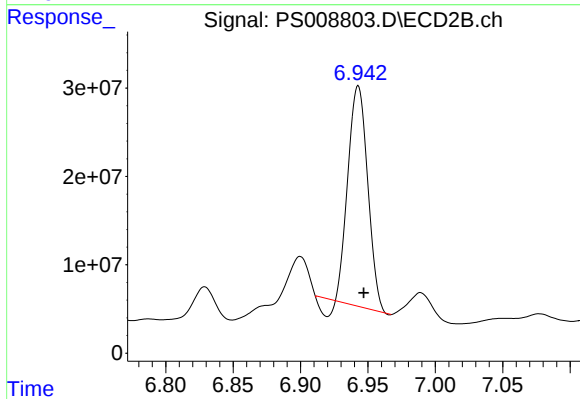

#4 2,4-DCAA


R.T.: 6.943 min
Delta R.T.: -0.004 min
Response: 245279451
Conc: 264.65 ng/ml

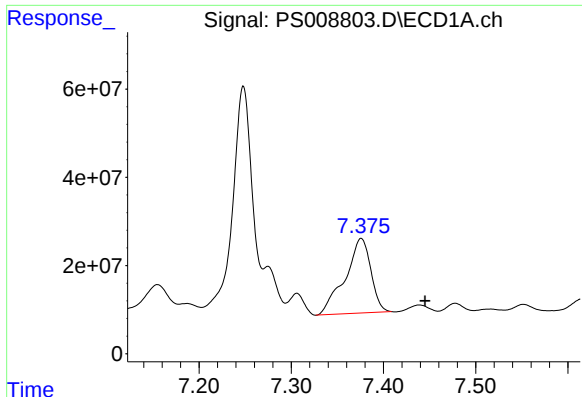

#5 DICAMBA


R.T.: 7.376 min
Delta R.T.: -0.070 min
Response: 326479176
Conc: 40.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

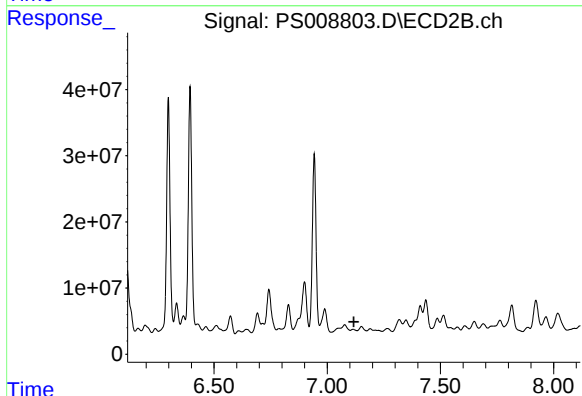


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.118 min
Response: 0
Conc: N.D.

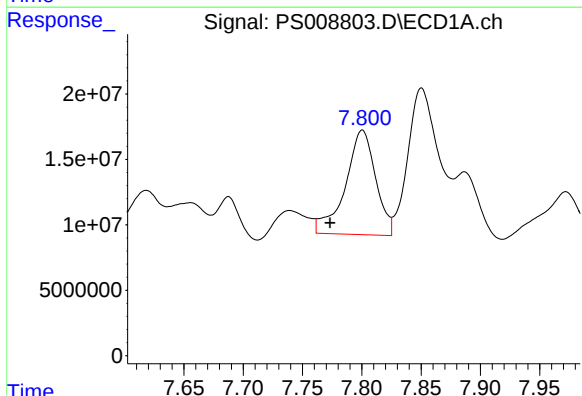


#7 MCPA

R.T.: 7.800 min
Delta R.T.: 0.027 min
Response: 142182076
Conc: 16.55 ug/ml

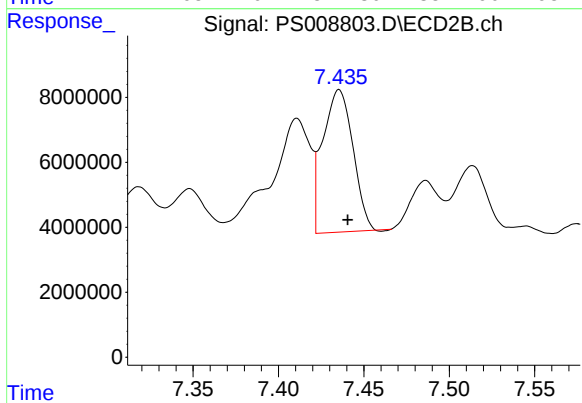

#7 MCPA


R.T.: 7.435 min
Delta R.T.: -0.005 min
Response: 54027958
Conc: 12.95 ug/ml

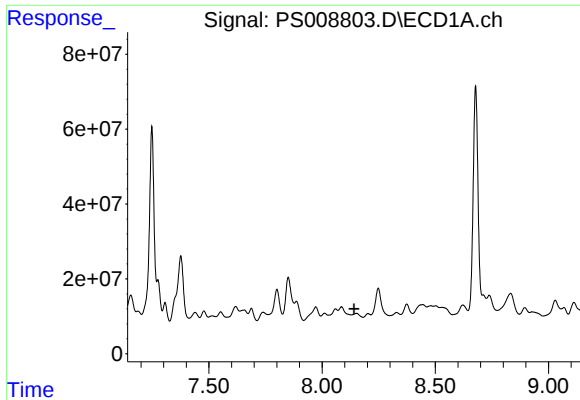

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

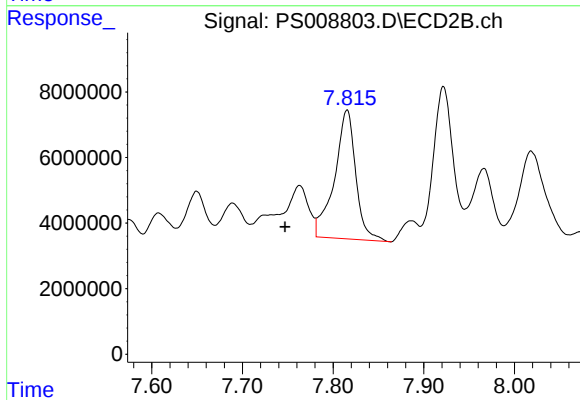


#8 DICHLORPROP

R.T.: 7.815 min
Delta R.T.: 0.068 min
Response: 64164472
Conc: 67.35 ng/ml

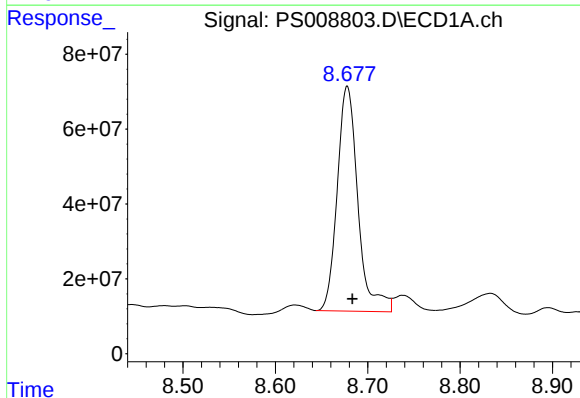


#10 Pentachlorophenol

R.T.: 8.678 min
Delta R.T.: -0.005 min
Response: 935990514
Conc: 32.92 ng/ml

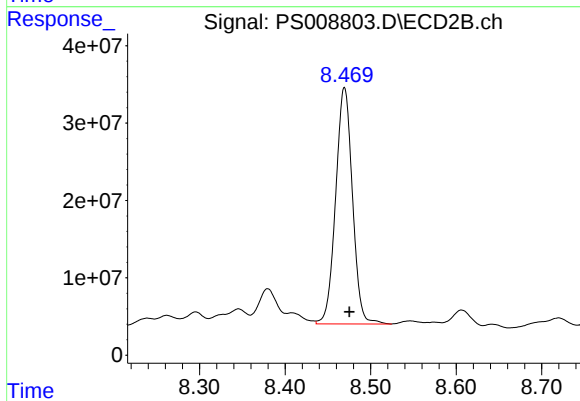

#10 Pentachlorophenol


R.T.: 8.469 min
Delta R.T.: -0.006 min
Response: 417603865
Conc: 31.66 ng/ml

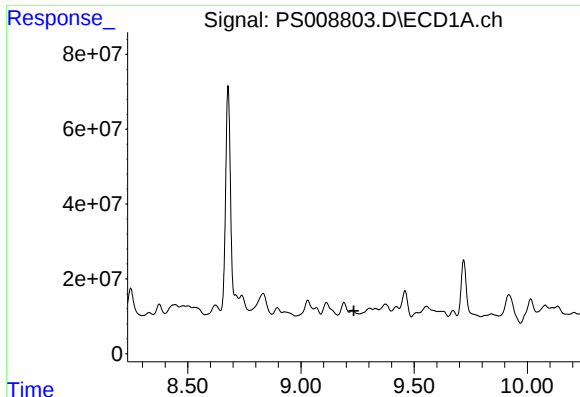

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.234 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

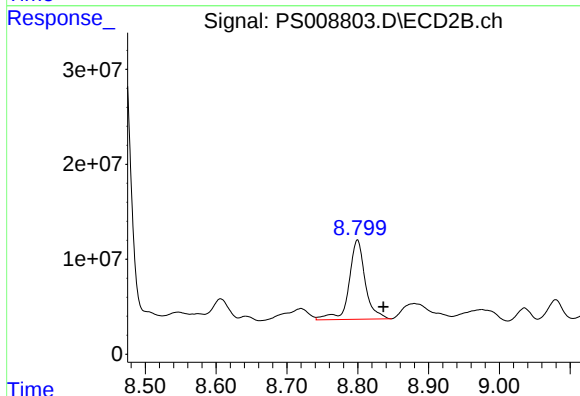


#11 2,4,5-TP (SILVEX)

R.T.: 8.800 min
Delta R.T.: -0.037 min
Response: 132514415
Conc: 25.86 ng/ml

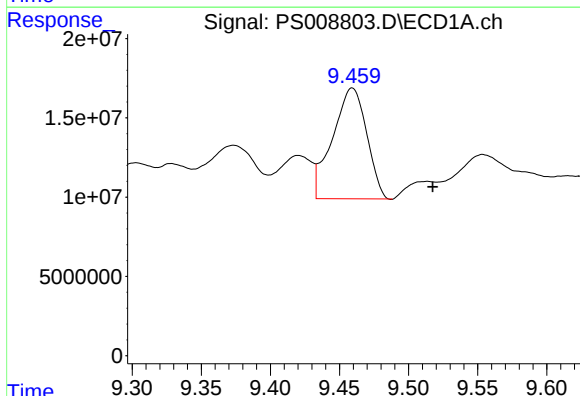


#12 2,4,5-T

R.T.: 9.459 min
Delta R.T.: -0.058 min
Response: 120523854
Conc: 10.95 ng/ml

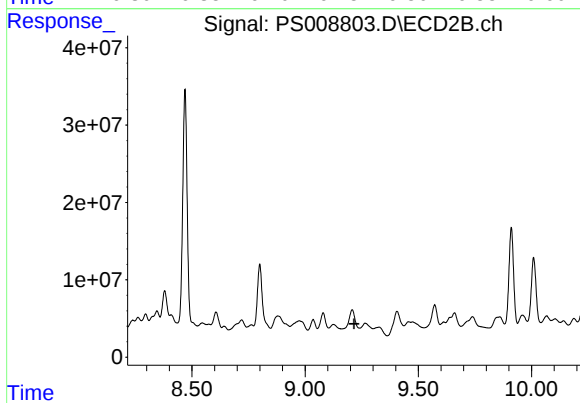

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.216 min
Response: 0
Conc: N.D.

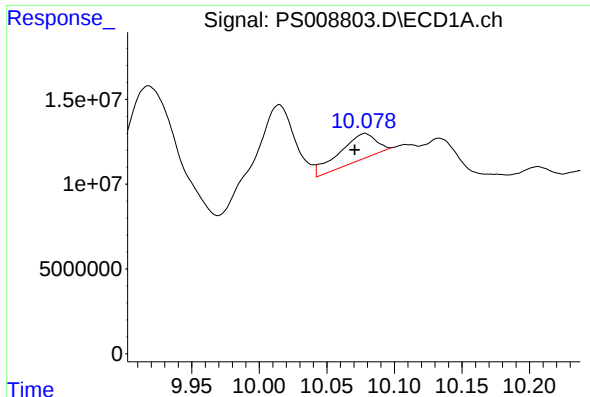

#13 2,4-DB


R.T.: 10.078 min
Delta R.T.: 0.008 min
Response: 29305784
Conc: 18.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

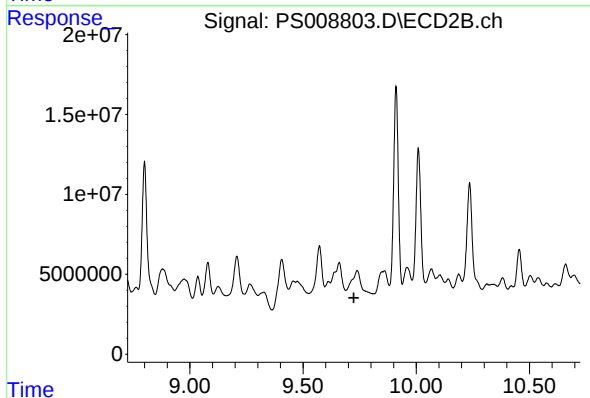


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.724 min
Response: 0
Conc: N.D.

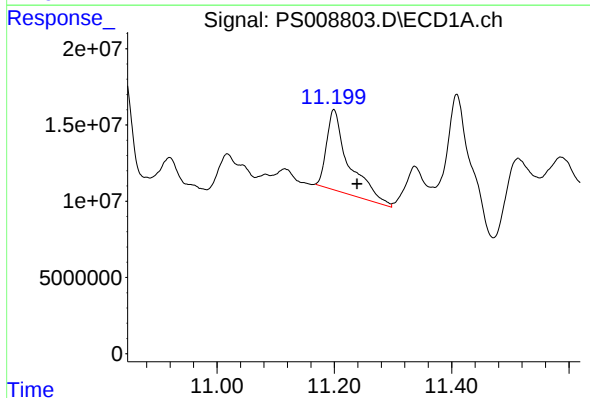


#14 DINOSEB

R.T.: 11.199 min
Delta R.T.: -0.039 min
Response: 138562628
Conc: 16.42 ng/ml

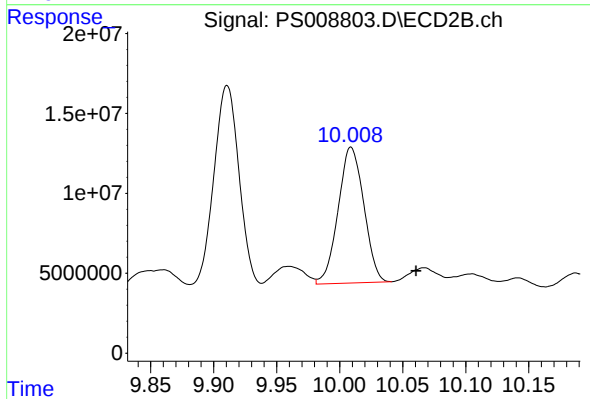

#14 DINOSEB


R.T.: 10.009 min
Delta R.T.: -0.051 min
Response: 120513362
Conc: 32.81 ng/ml

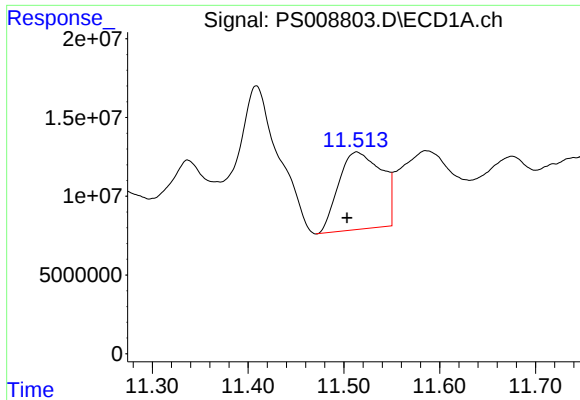

#16 DCPA

R.T.: 11.513 min
Delta R.T.: 0.010 min
Response: 153397724
Conc: 10.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

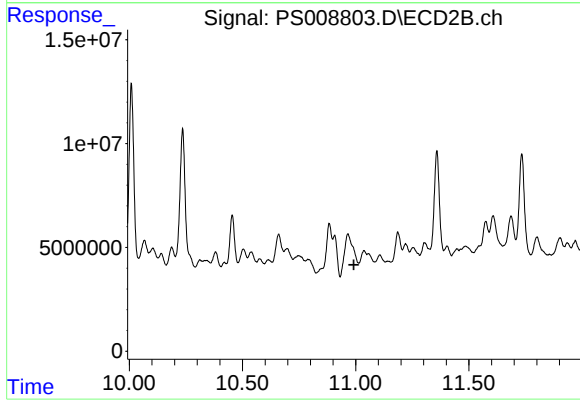

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.992 min
Response: 0
Conc: N.D.