

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021120\
 Data File : PS008806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2020 00:10
 Operator : DD\AJ
 Sample : L1439-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 03:39:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.942	688.6E6	283.4E6	320.822	305.777
Target Compounds							
1) T	Dalapon	0.000	2.592	0	114.6E6	N.D.	95.572
2) T	3,5-DICHL...	0.000	6.117	0	75348145	N.D.	54.763
7) T	MCPA	7.800	7.412	63224494	58687878	7.360	14.062 #
10) T	Pentachlo...	8.742	0.000	100.7E6	0	3.542	N.D. #
11) T	2,4,5-TP ...	0.000	8.799	0	100.3E6	N.D.	19.568
12) T	2,4,5-T	9.458	0.000	146.4E6	0	13.304	N.D. #
13) T	2,4-DB	10.113	0.000	379.7E6	0	233.443	N.D. #
14) T	DINOSEB	11.200	0.000	139.2E6	0	16.495	N.D. #
16) T	DCPA	11.505	0.000	77907998	0	5.557	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021120\
Data File : PS008806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2020 00:10
Operator : DD\AJ
Sample : L1439-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 03:39:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

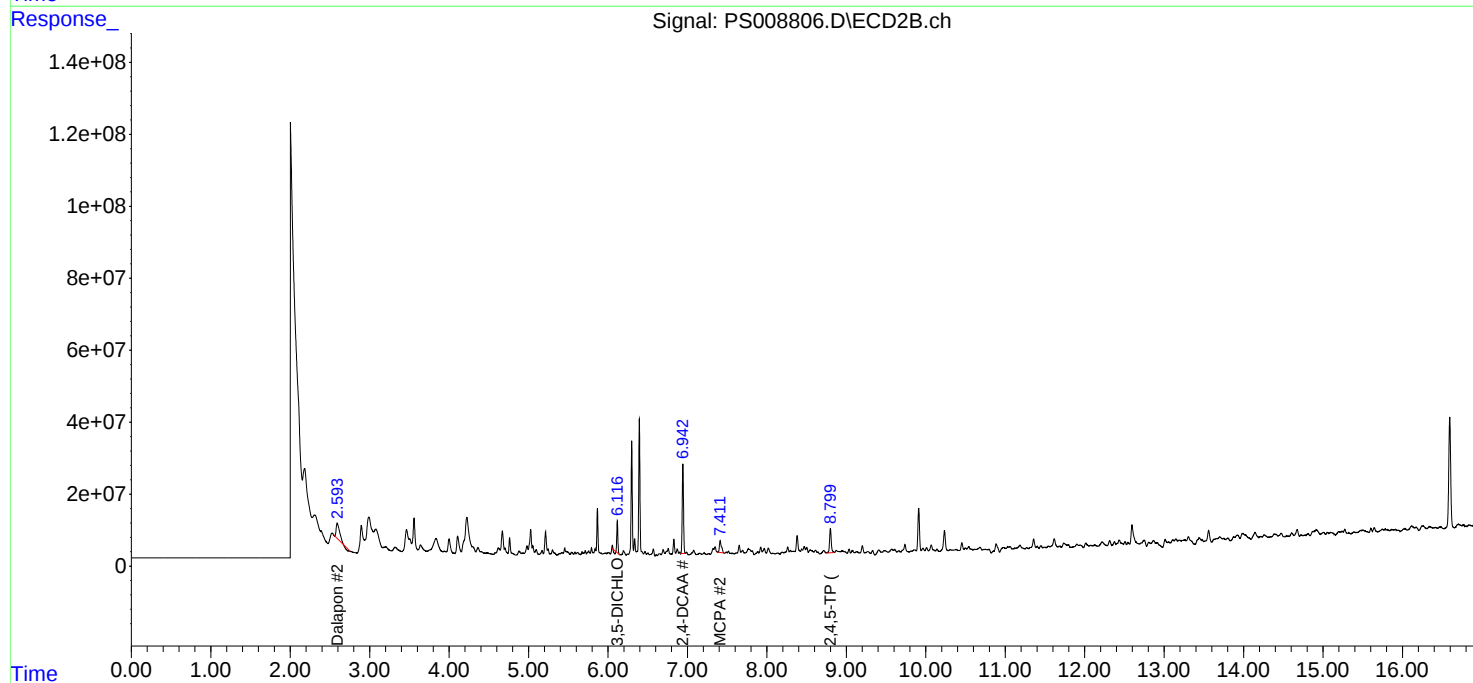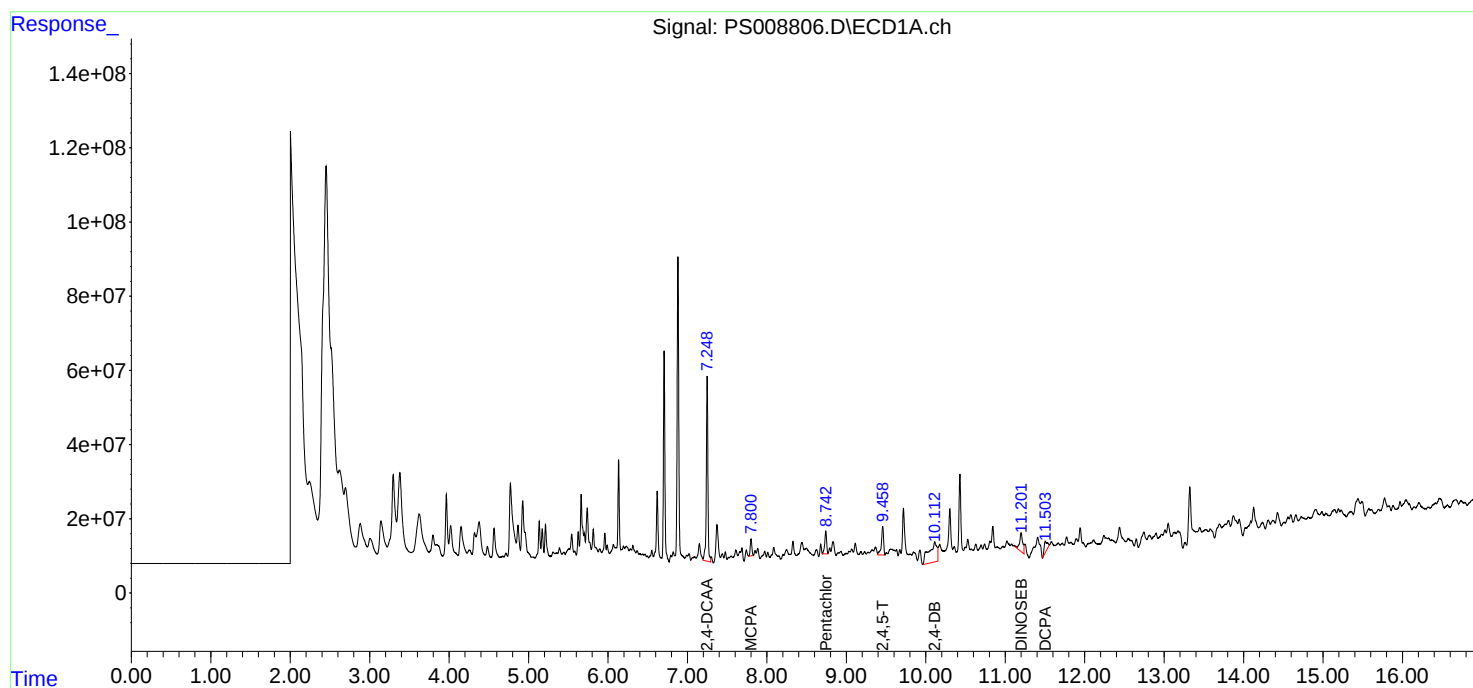


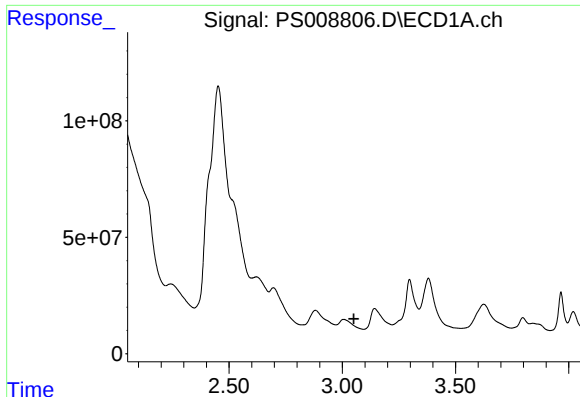

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

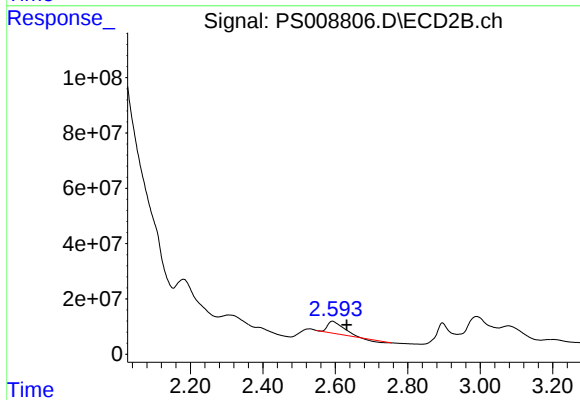


#1 Dalapon

R.T.: 2.592 min
Delta R.T.: -0.040 min
Response: 114621044
Conc: 95.57 ng/ml

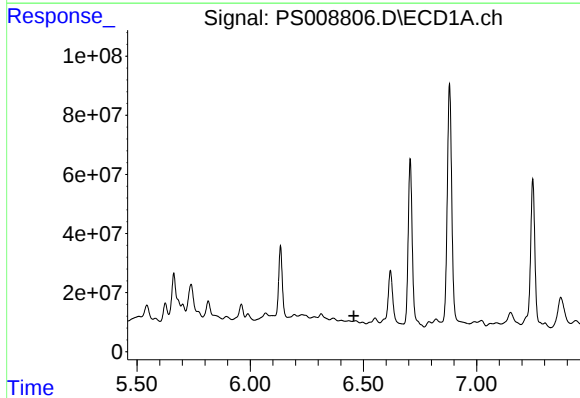


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

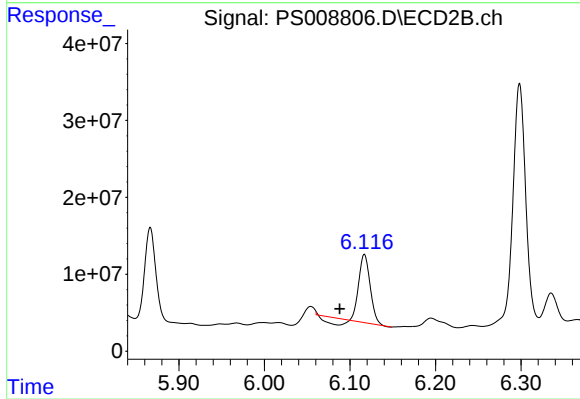

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.117 min
Delta R.T.: 0.029 min
Response: 75348145
Conc: 54.76 ng/ml

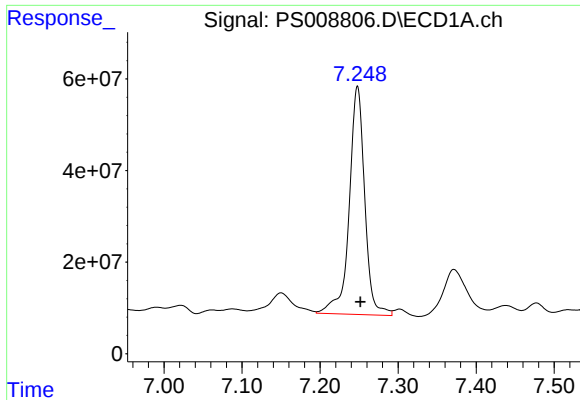

#4 2,4-DCAA


R.T.: 7.248 min
Delta R.T.: -0.004 min
Response: 688582742
Conc: 320.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

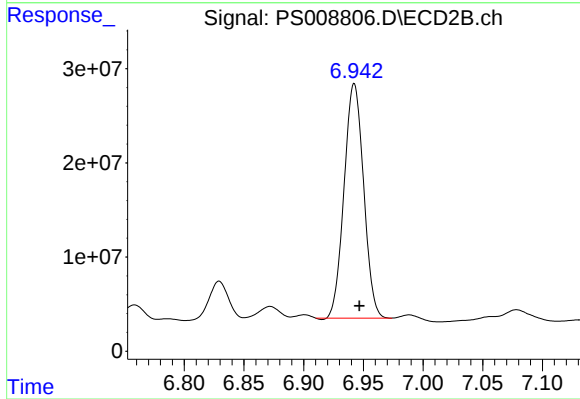


#4 2,4-DCAA

R.T.: 6.942 min
Delta R.T.: -0.004 min
Response: 283401437
Conc: 305.78 ng/ml

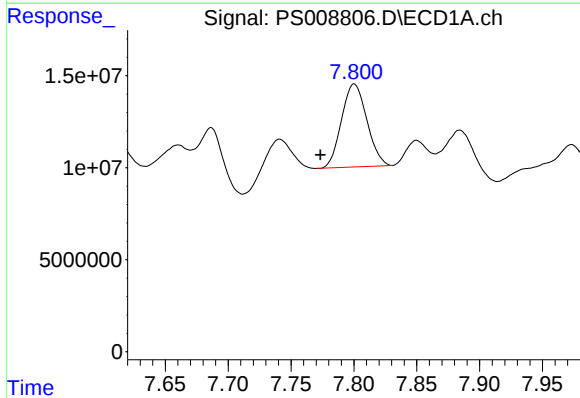


#7 MCPA

R.T.: 7.800 min
Delta R.T.: 0.027 min
Response: 63224494
Conc: 7.36 ug/ml

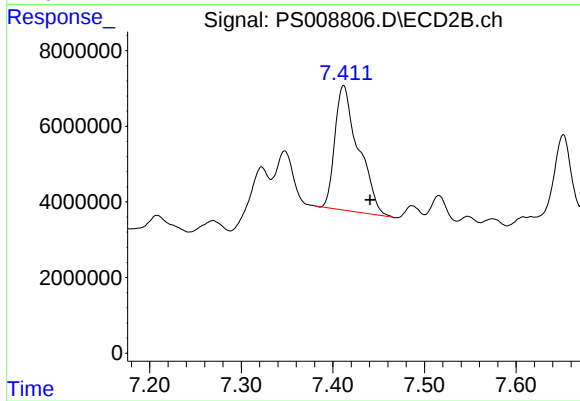

#7 MCPA


R.T.: 7.412 min
Delta R.T.: -0.029 min
Response: 58687878
Conc: 14.06 ug/ml

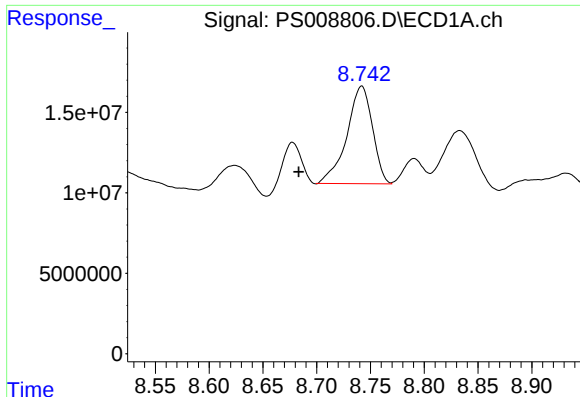

#10 Pentachlorophenol


R.T.: 8.742 min
Delta R.T.: 0.058 min
Response: 100690753
Conc: 3.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

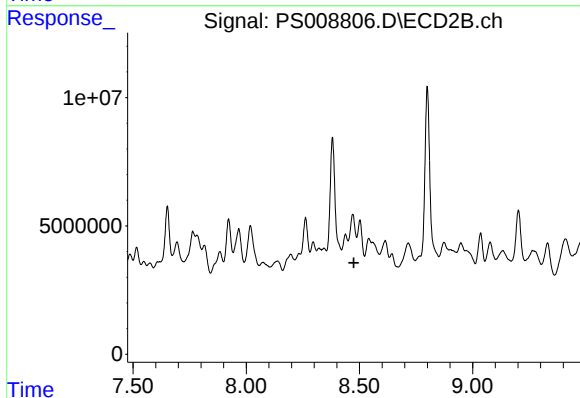


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.475 min
Response: 0
Conc: N.D.

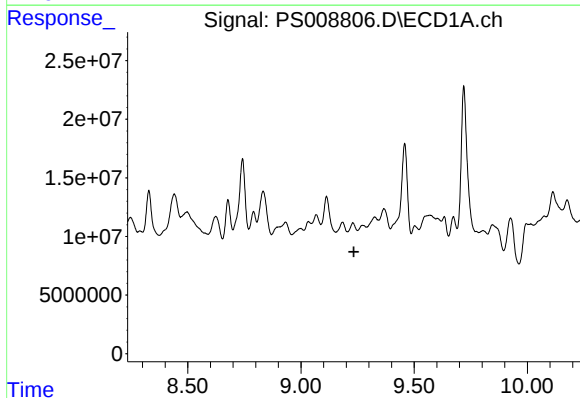


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.234 min
Response: 0
Conc: N.D.

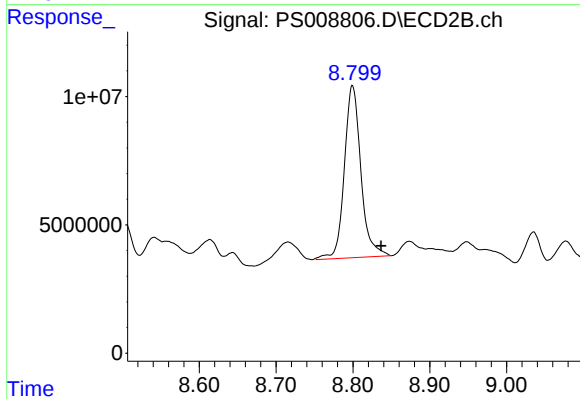

#11 2,4,5-TP (SILVEX)


R.T.: 8.799 min
Delta R.T.: -0.037 min
Response: 100290683
Conc: 19.57 ng/ml

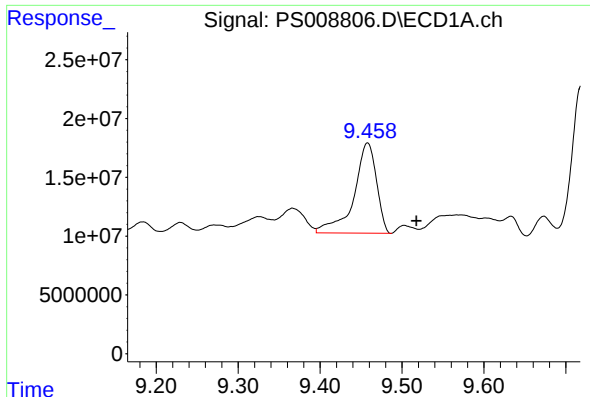

#12 2,4,5-T


R.T.: 9.458 min
Delta R.T.: -0.060 min
Response: 146425743
Conc: 13.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

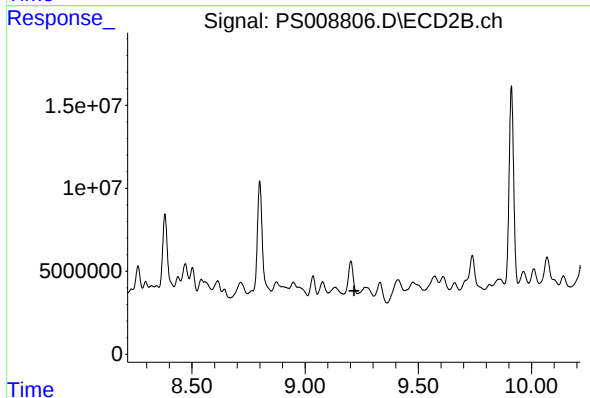


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.216 min
Response: 0
Conc: N.D.

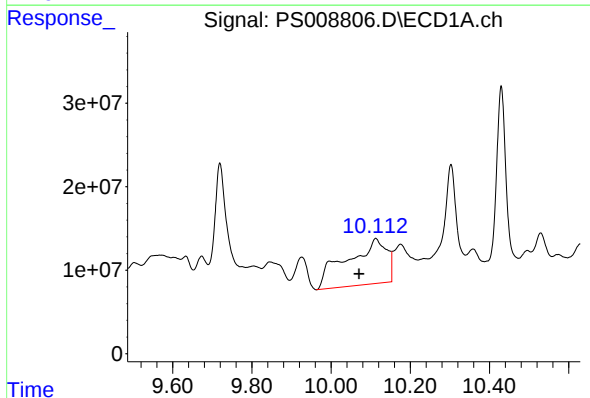


#13 2,4-DB

R.T.: 10.113 min
Delta R.T.: 0.042 min
Response: 379716684
Conc: 233.44 ng/ml

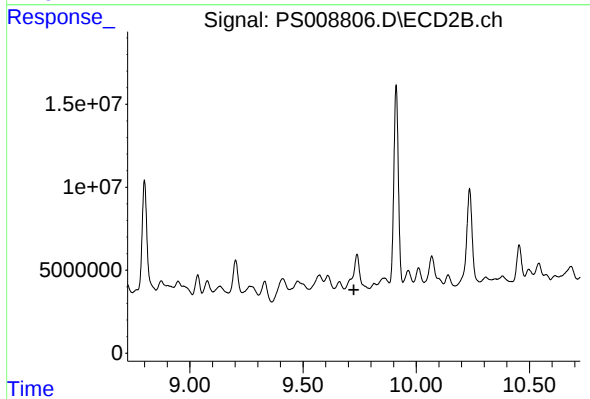

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.724 min
Response: 0
Conc: N.D.

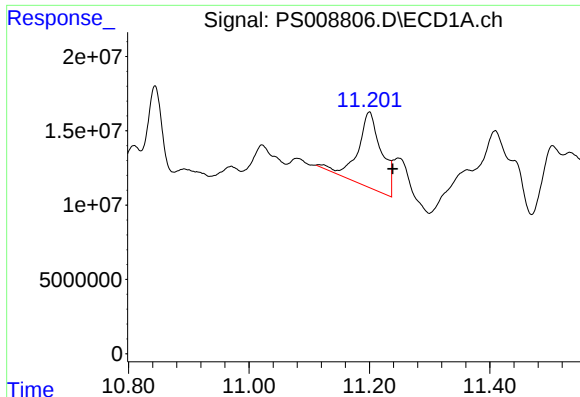

#14 DINOSEB


R.T.: 11.200 min
Delta R.T.: -0.039 min
Response: 139197324
Conc: 16.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

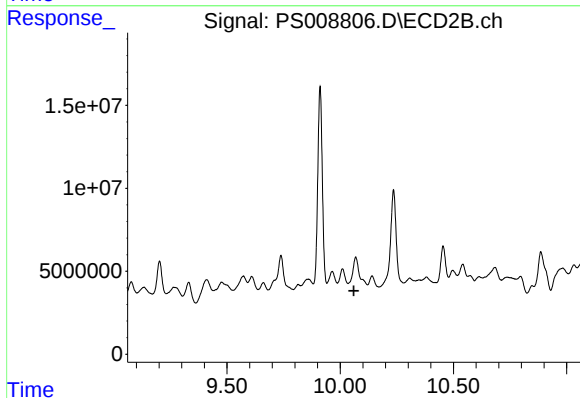


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.061 min
Response: 0
Conc: N.D.

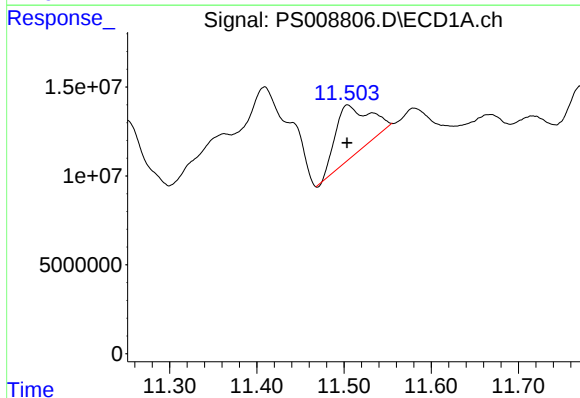

#16 DCPA

R.T.: 11.505 min
Delta R.T.: 0.001 min
Response: 77907998
Conc: 5.56 ng/ml

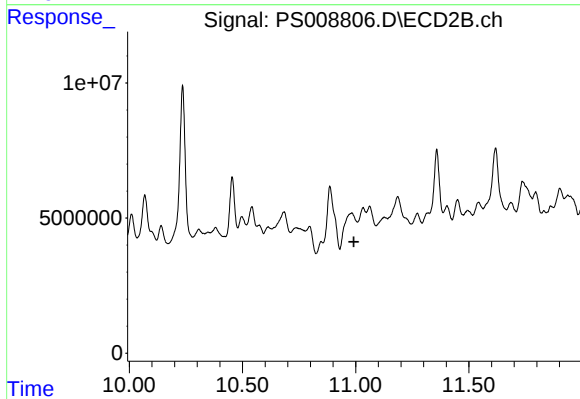

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.992 min
Response: 0
Conc: N.D.