

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021219\
 Data File : PS003132.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 10:42
 Operator : EI\SJ
 Sample : K1450-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SHORE-RD-BOX-CULVERT-TP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 01:16:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.296	10.791	165.8E6	163.8E6	436.608	383.171
Target Compounds							
1) T	Dalapon	2.815	2.299	5436184	90360306	9.854	168.607 #
2) T	3,5-DICHL...	0.000	8.956	0	5134096	N.D.	9.110 #
5) T	DICAMBA	0.000	11.031	0	3805040	N.D.	2.398 #
6) T	MCP	11.965	0.000	36910660	0	30.807	N.D. #
7) T	MCPA	12.150	0.000	32498388	0	18.361	N.D. #
9) T	2,4-D	0.000	12.756	0	3986768	N.D.	7.951 #
11) T	2,4,5-TP ...	14.378	0.000	3116189	0	1.237	N.D. #
14) T	DINOSEB	0.000	15.498	0	5446438	N.D.	3.107 #
15) T	Picloram	16.810	16.713	6011691	22308341	1.900	7.420 #
16) T	DCPA	0.000	16.713	0	22308341	N.D.	7.202 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021219\
Data File : PS003132.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 10:42
Operator : EI\SJ
Sample : K1450-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SHORE-RD-BOX-CULVERT-TP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 01:16:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

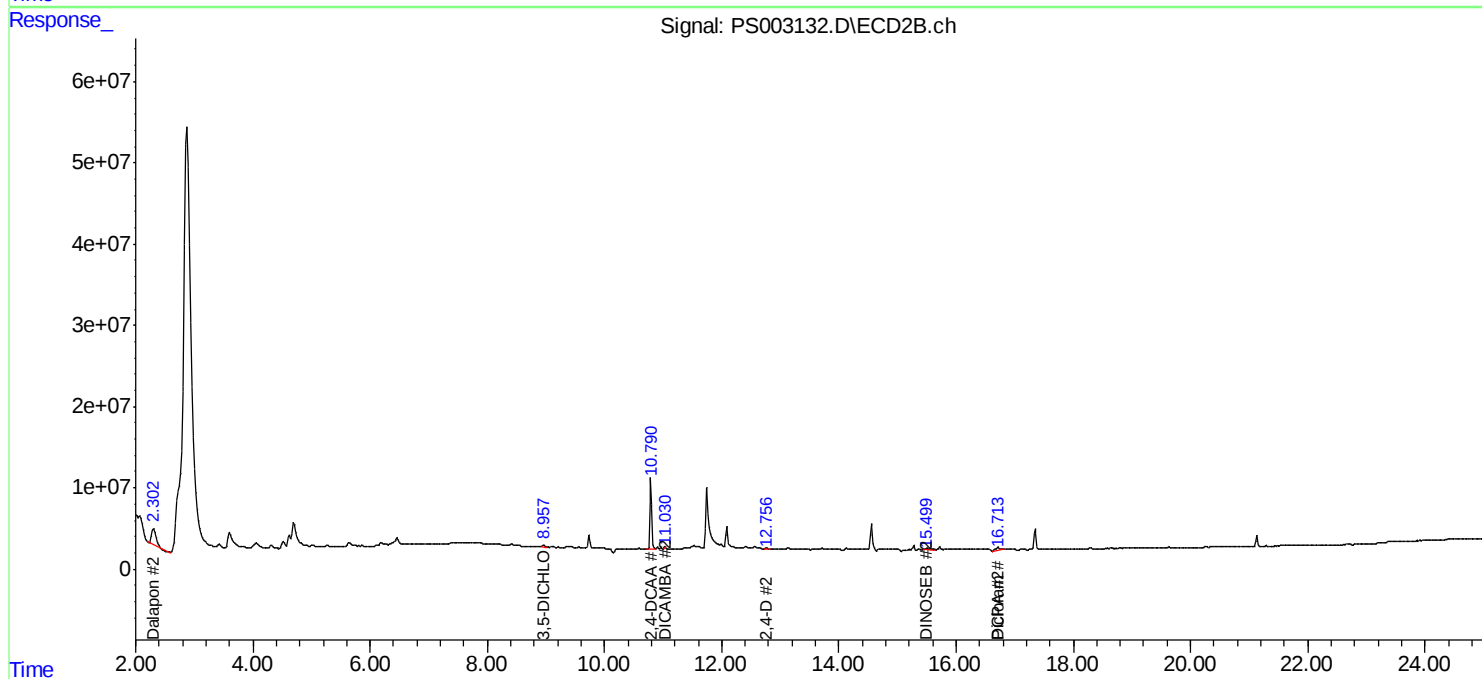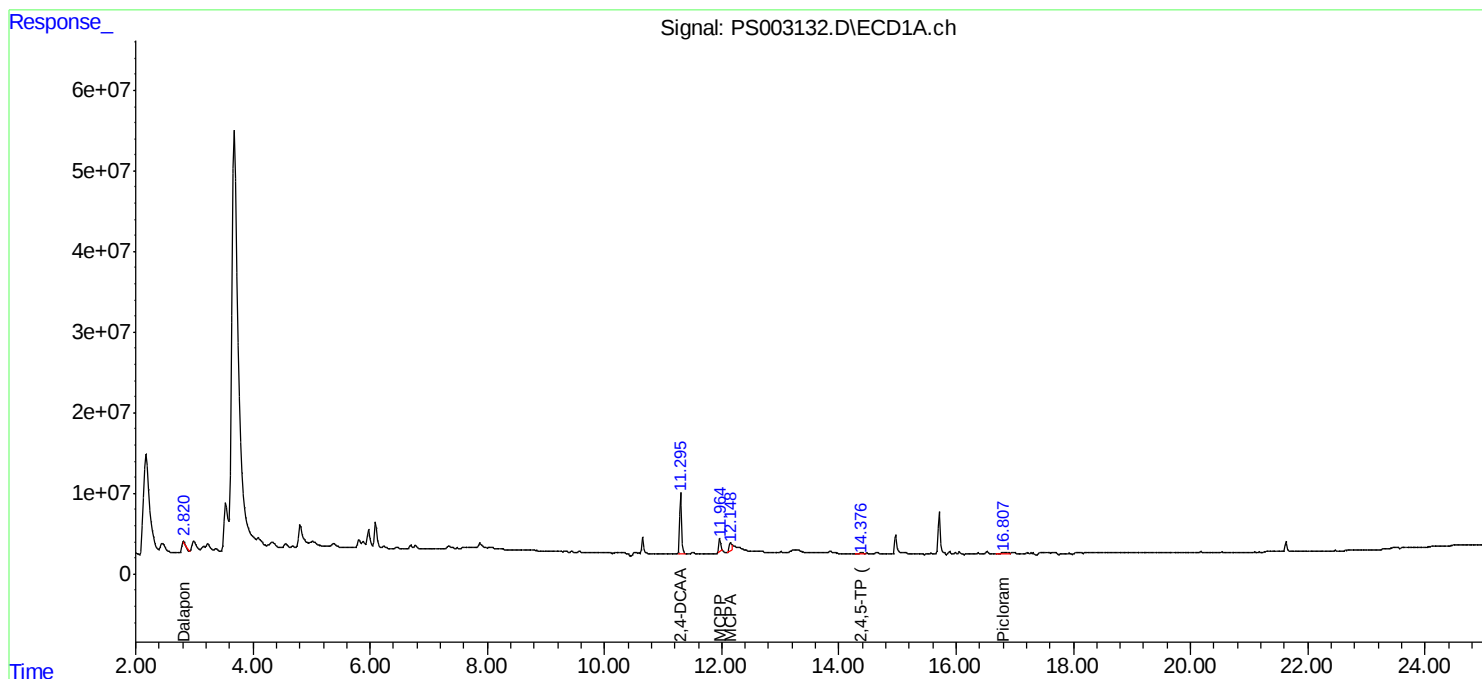


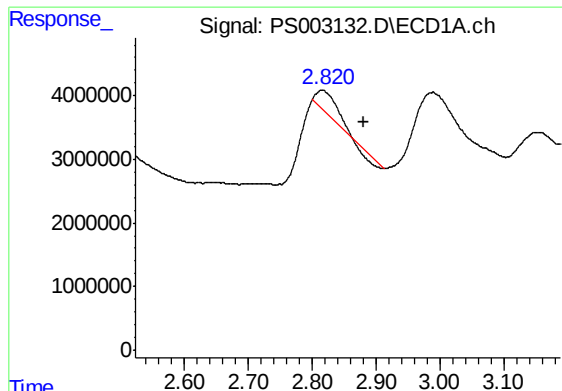

#1 Dalapon


R.T.: 2.815 min
Delta R.T.: -0.065 min
Response: 5436184
Conc: 9.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
SHORE-RD-BOX-CULVERT-TP

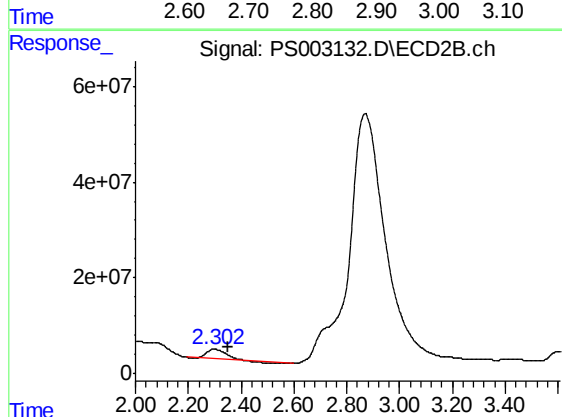


#1 Dalapon

R.T.: 2.299 min
Delta R.T.: -0.052 min
Response: 90360306
Conc: 168.61 ng/ml

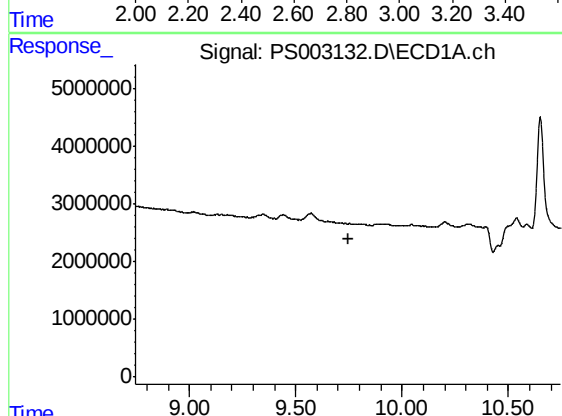


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

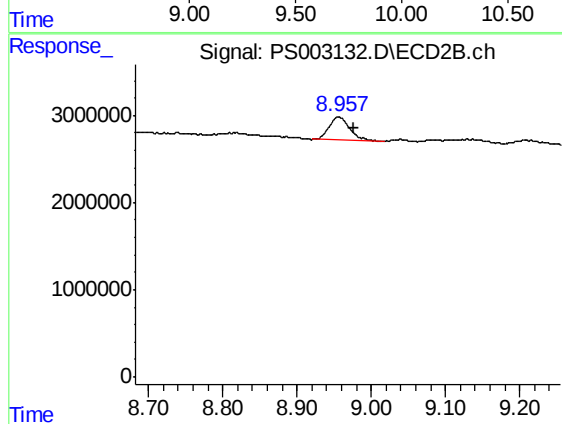

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.956 min
Delta R.T.: -0.020 min
Response: 5134096
Conc: 9.11 ng/ml

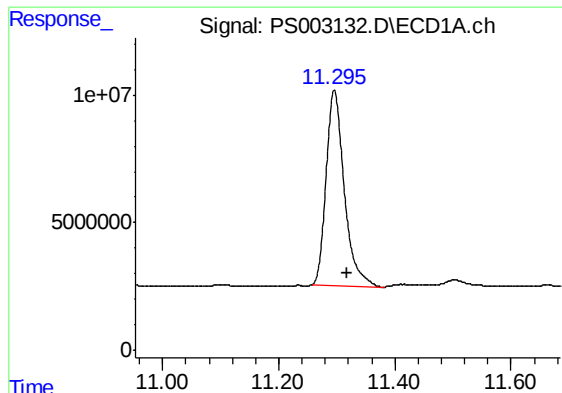

#4 2,4-DCAA


R.T.: 11.296 min
Delta R.T.: -0.022 min
Response: 165754383
Conc: 436.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
SHORE-RD-BOX-CULVERT-TP

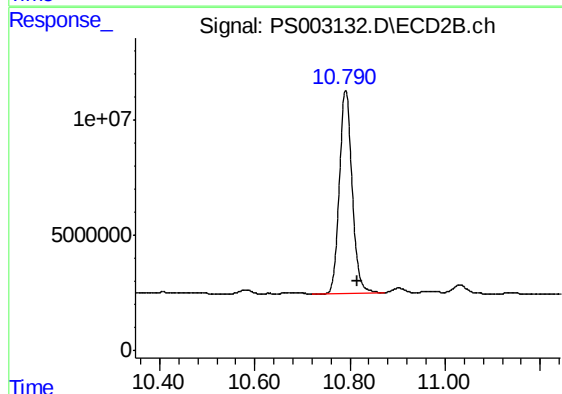


#4 2,4-DCAA

R.T.: 10.791 min
Delta R.T.: -0.026 min
Response: 163822981
Conc: 383.17 ng/ml

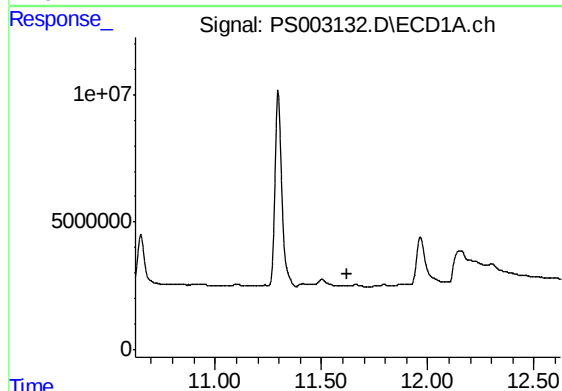


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.624 min
Response: 0
Conc: N.D.

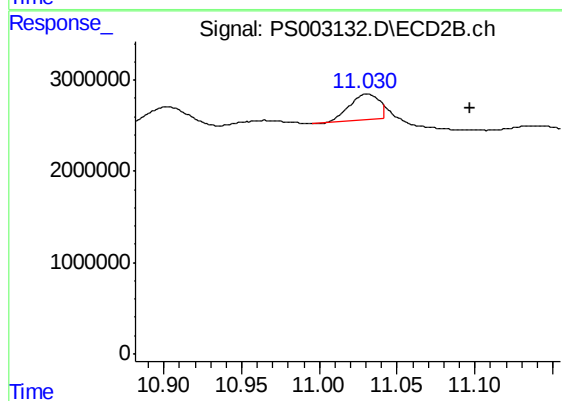

#5 DICAMBA


R.T.: 11.031 min
Delta R.T.: -0.066 min
Response: 3805040
Conc: 2.40 ng/ml

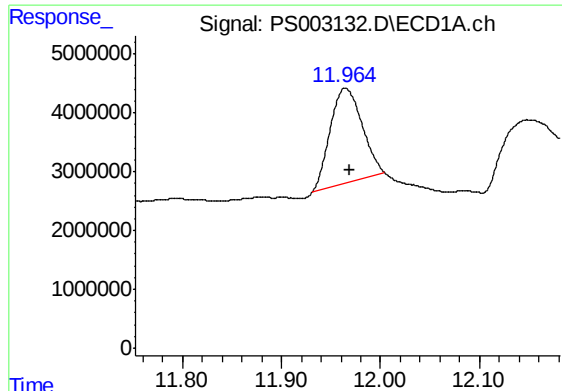

#6 MCPP


R.T.: 11.965 min
Delta R.T.: -0.005 min
Response: 36910660
Conc: 30.81 ug/ml

Instrument :
ECD_S
ClientSampleId :
SHORE-RD-BOX-CULVERT-TP

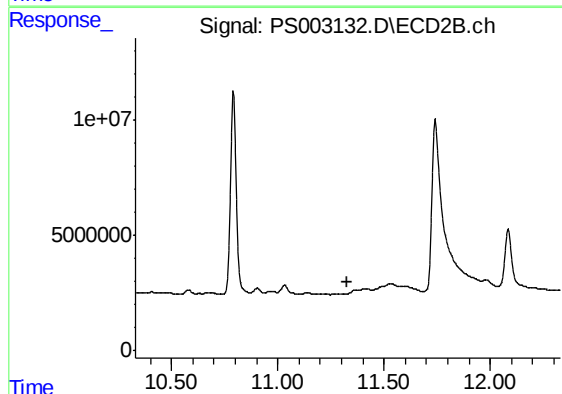


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

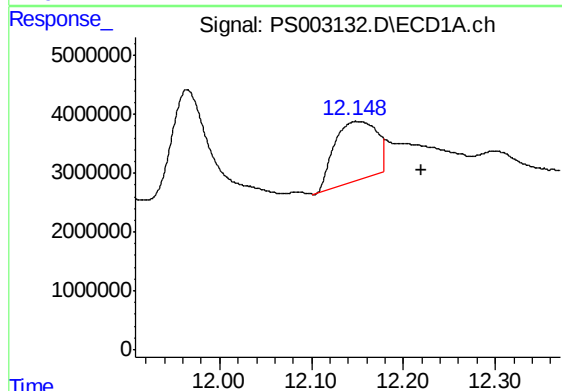


#7 MCPA

R.T.: 12.150 min
Delta R.T.: -0.069 min
Response: 32498388
Conc: 18.36 ug/ml

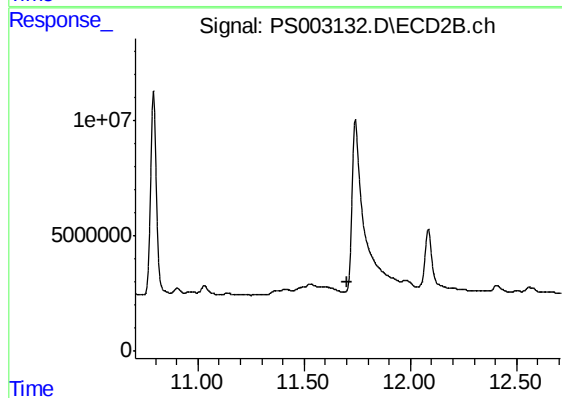

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 11.706 min
Response: 0
Conc: N.D.

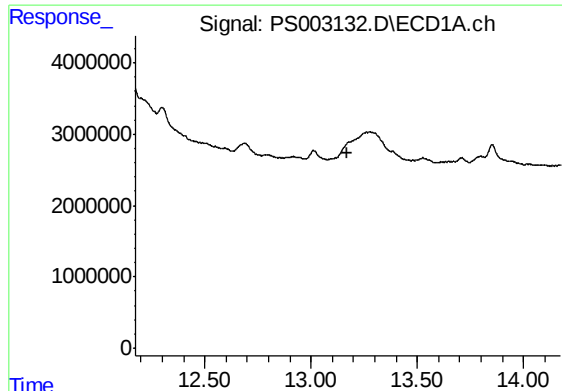

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 13.173 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SHORE-RD-BOX-CULVERT-TP

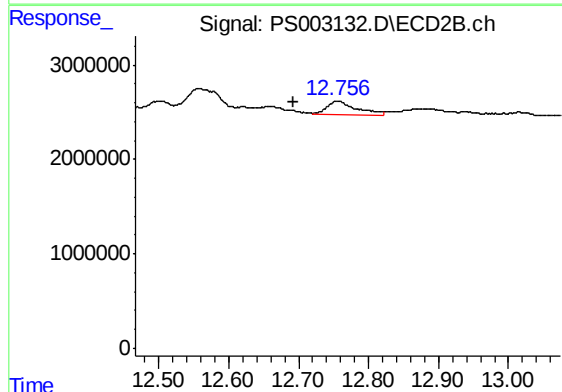


#9 2,4-D

R.T.: 12.756 min
Delta R.T.: 0.063 min
Response: 3986768
Conc: 7.95 ng/ml

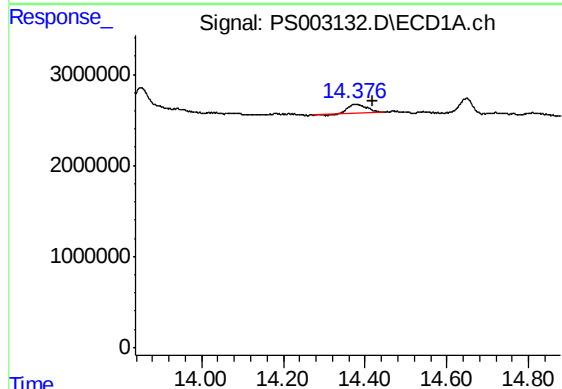


#11 2,4,5-TP (SILVEX)

R.T.: 14.378 min
Delta R.T.: -0.042 min
Response: 3116189
Conc: 1.24 ng/ml

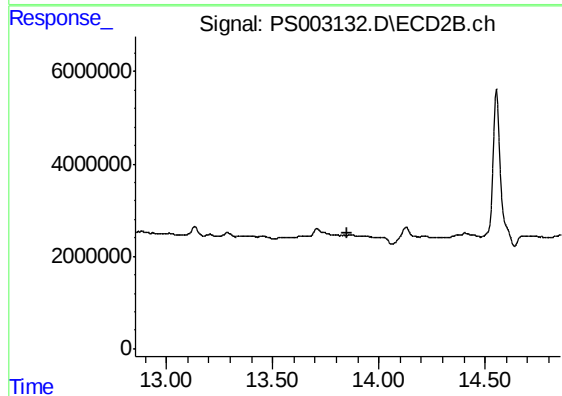

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

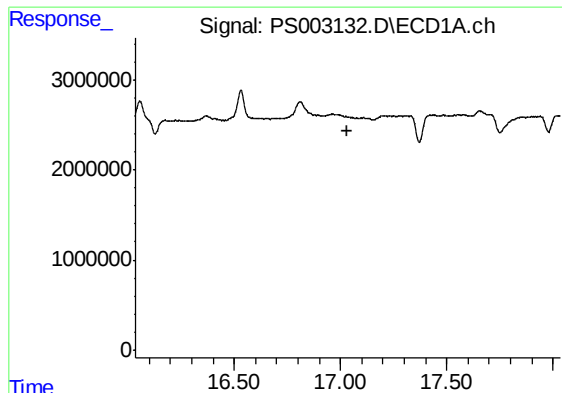

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SHORE-RD-BOX-CULVERT-TP

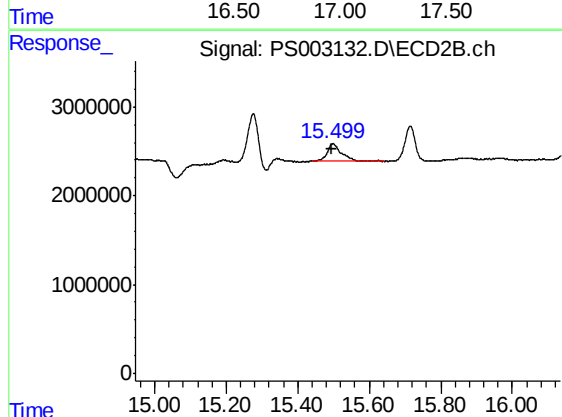


#14 DINOSEB

R.T.: 15.498 min
Delta R.T.: 0.004 min
Response: 5446438
Conc: 3.11 ng/ml

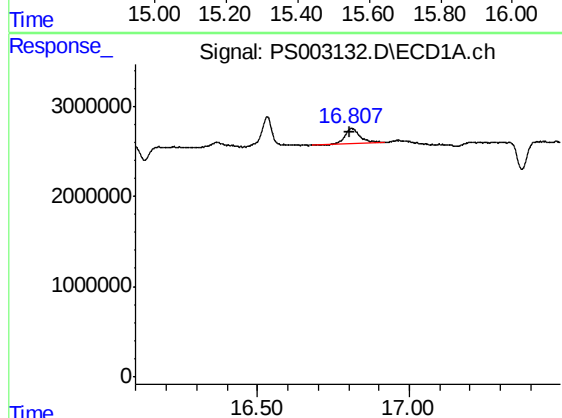


#15 Picloram

R.T.: 16.810 min
Delta R.T.: 0.004 min
Response: 6011691
Conc: 1.90 ng/ml

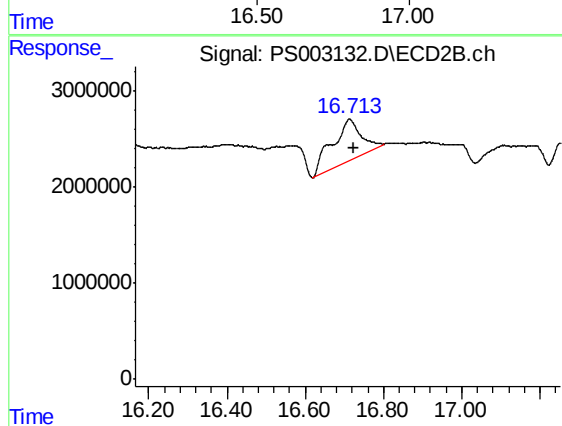

#15 Picloram


R.T.: 16.713 min
Delta R.T.: -0.011 min
Response: 22308341
Conc: 7.42 ng/ml

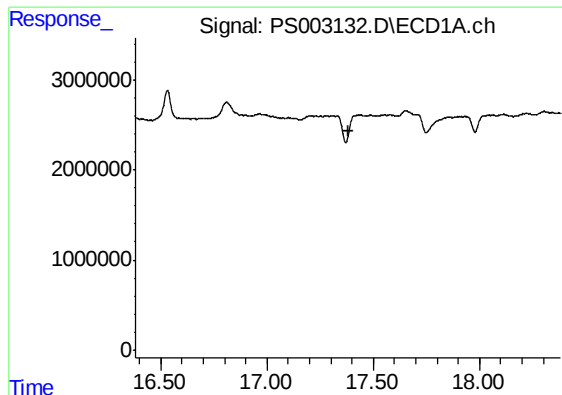

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SHORE-RD-BOX-CULVERT-TP

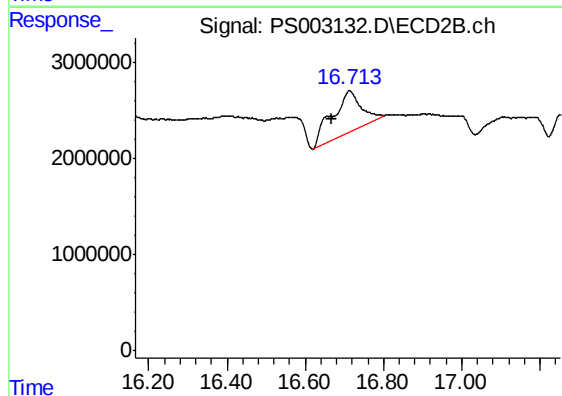

#16 DCPA

R.T.: 16.713 min
Delta R.T.: 0.043 min
Response: 22308341
Conc: 7.20 ng/ml