

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021219\
 Data File : PS003135.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 12:15
 Operator : EI\SJ
 Sample : K1454-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 01:16:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.314	10.815	118.1E6	115.4E6	311.072	269.845
Target Compounds							
1) T	Dalapon	2.833	2.326	14377616	91106844	26.063	170.000 #
2) T	3,5-DICHL...	0.000	8.982	0	3900032	N.D.	6.920 #
6) T	MCP	11.976	0.000	52025703	0	43.423	N.D. #
7) T	MCPA	0.000	11.759	0	137.0E6	N.D.	87.119 #
11) T	2,4,5-TP ...	0.000	13.846	0	3652341	N.D.	1.473 #
12) T	2,4,5-T	14.856	14.473	11482355	386919	4.707	0.202 #
13) T	2,4-DB	0.000	15.005	0	1116628	N.D.	4.396 #
14) T	DINOSEB	0.000	15.518	0	2269671	N.D.	1.295 #
15) T	Picloram	0.000	16.737	0	22282039	N.D.	7.412 #
16) T	DCPA	17.437	16.737	-5773586	22282039	N.D.	7.193



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021219\
Data File : PS003135.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 12:15
Operator : EI\SJ
Sample : K1454-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 01:16:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

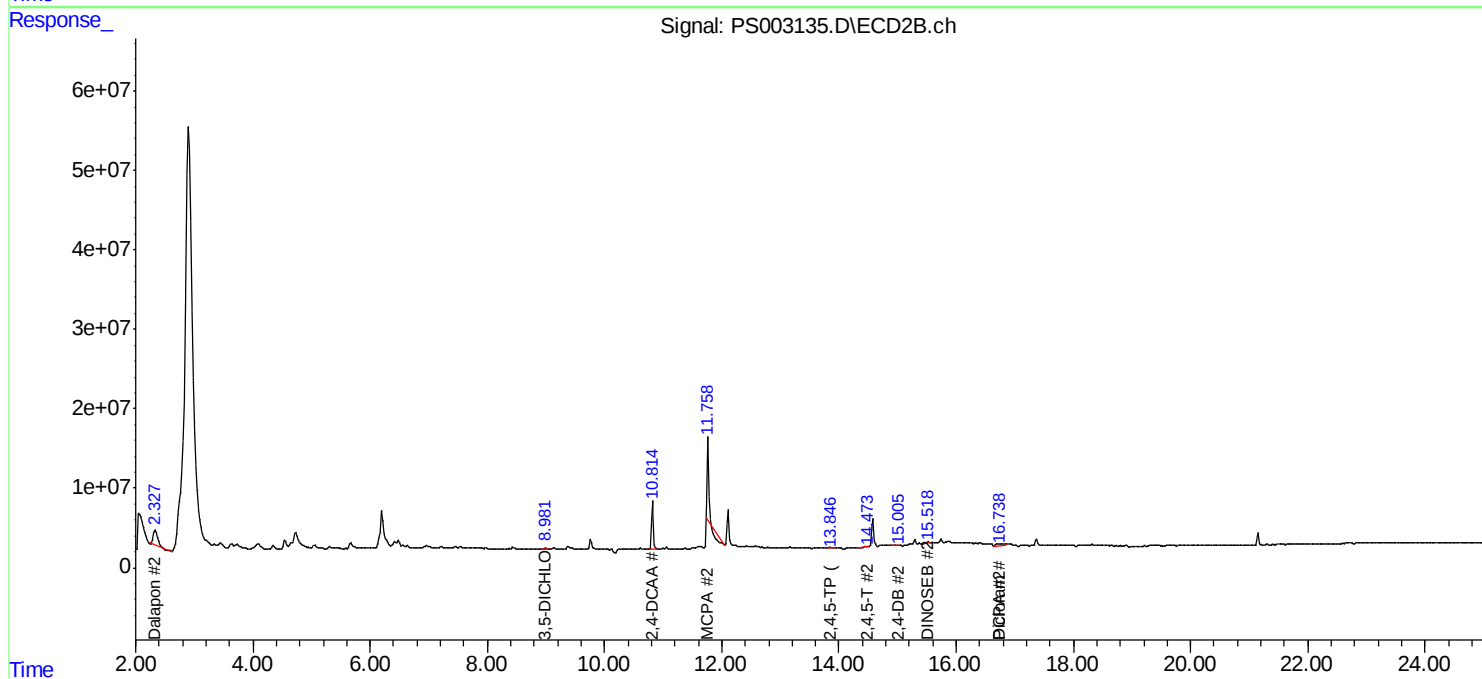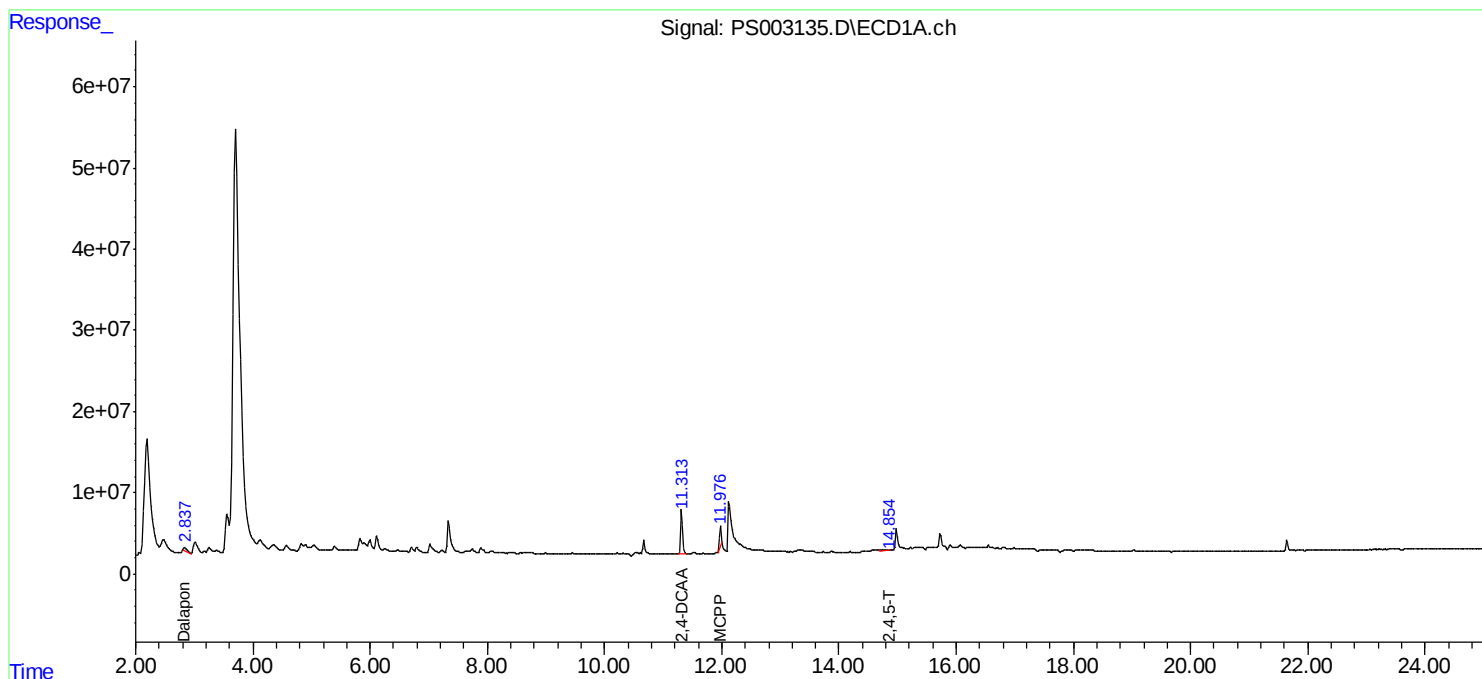


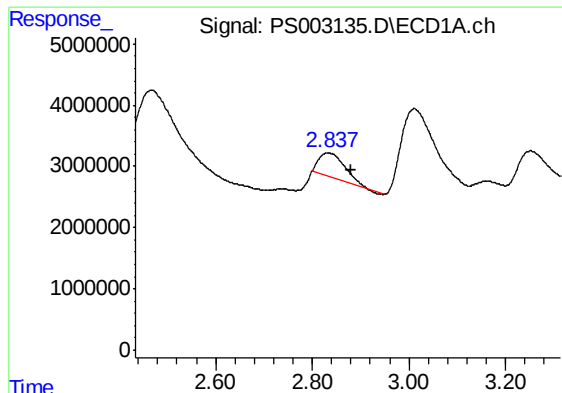

#1 Dalapon


R.T.: 2.833 min
Delta R.T.: -0.047 min
Response: 14377616
Conc: 26.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

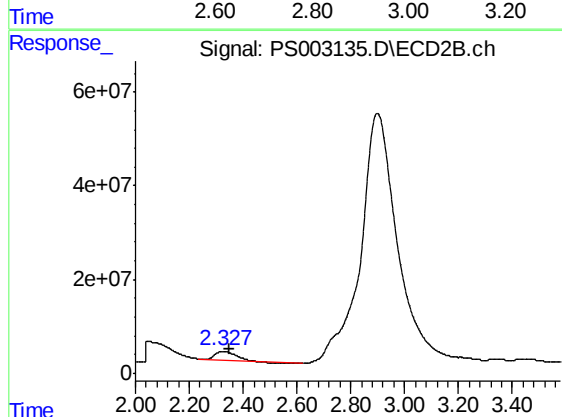


#1 Dalapon

R.T.: 2.326 min
Delta R.T.: -0.025 min
Response: 91106844
Conc: 170.00 ng/ml

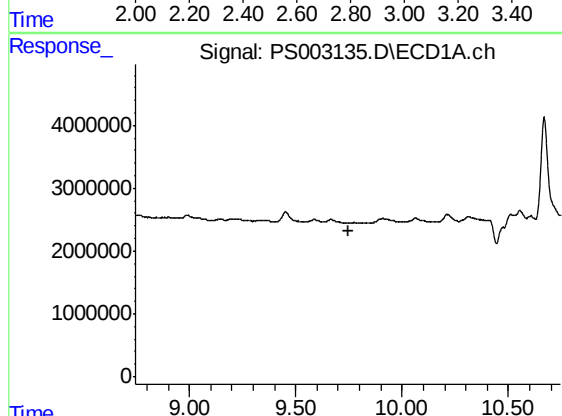


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

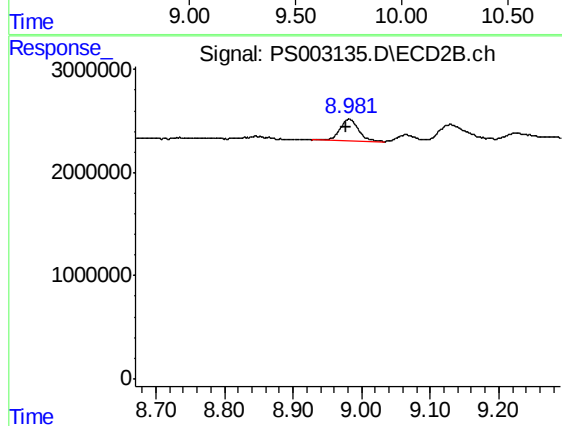

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.982 min
Delta R.T.: 0.005 min
Response: 3900032
Conc: 6.92 ng/ml

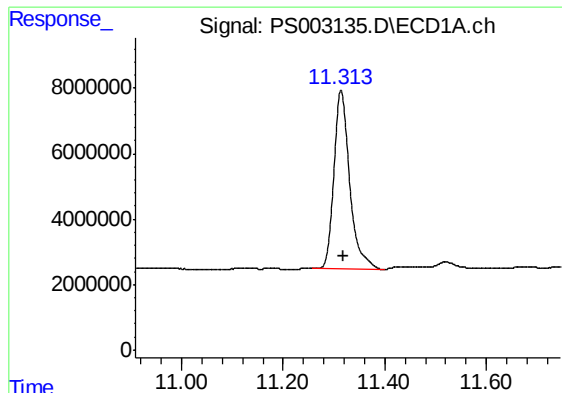

#4 2,4-DCAA


R.T.: 11.314 min
Delta R.T.: -0.004 min
Response: 118095485
Conc: 311.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

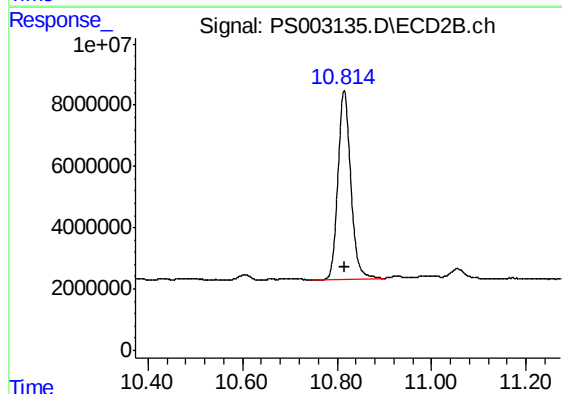


#4 2,4-DCAA

R.T.: 10.815 min
Delta R.T.: -0.002 min
Response: 115371120
Conc: 269.85 ng/ml

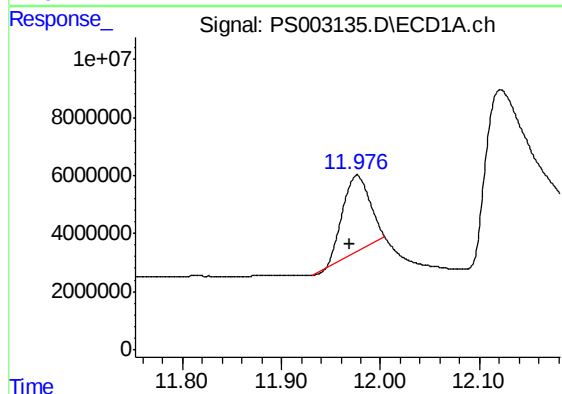


#6 MCPP

R.T.: 11.976 min
Delta R.T.: 0.007 min
Response: 52025703
Conc: 43.42 ug/ml

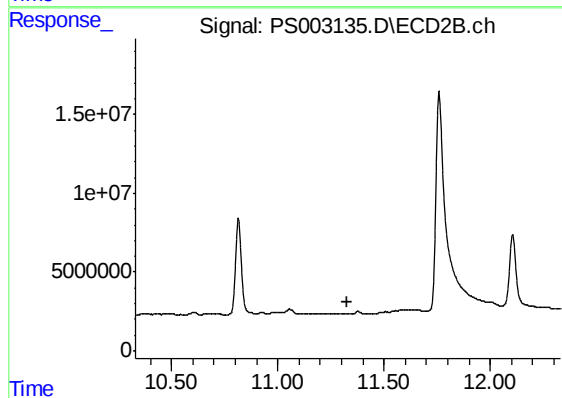

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

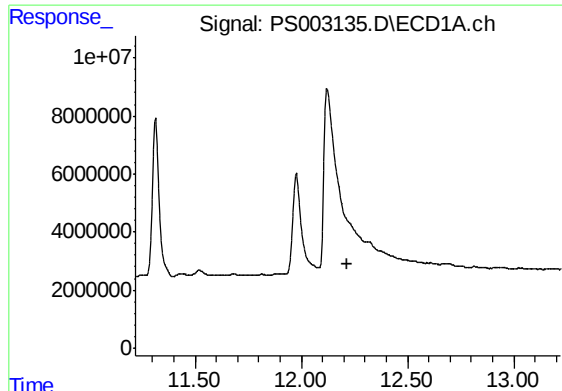

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1

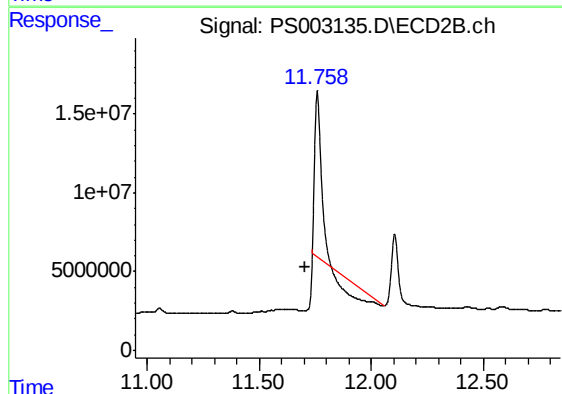


#7 MCPA

R.T.: 11.759 min
Delta R.T.: 0.053 min
Response: 137044181
Conc: 87.12 ug/ml

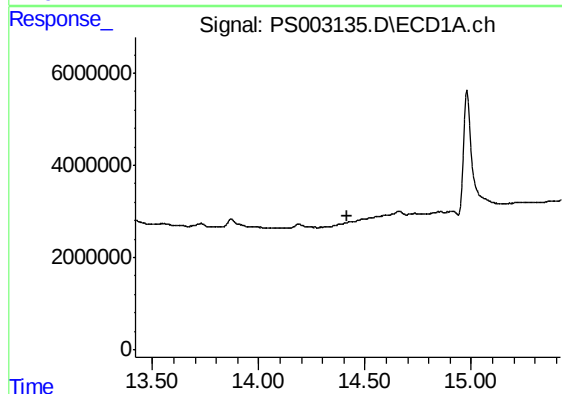


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.419 min
Response: 0
Conc: N.D.

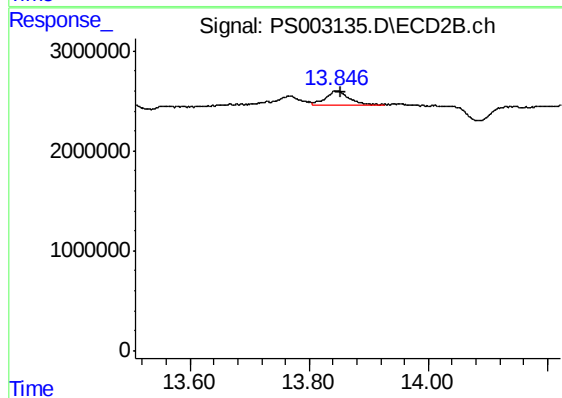

#11 2,4,5-TP (SILVEX)


R.T.: 13.846 min
Delta R.T.: -0.008 min
Response: 3652341
Conc: 1.47 ng/ml

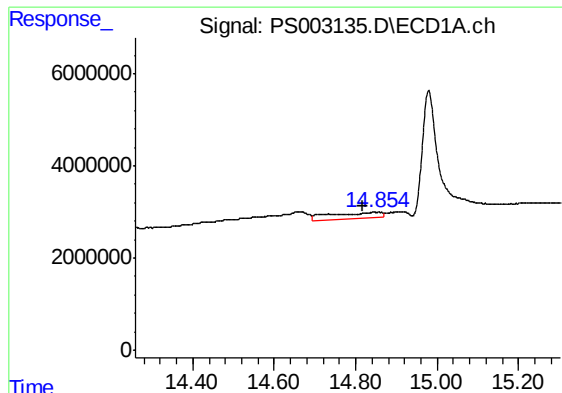

#12 2,4,5-T


R.T.: 14.856 min
Delta R.T.: 0.040 min
Response: 11482355
Conc: 4.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

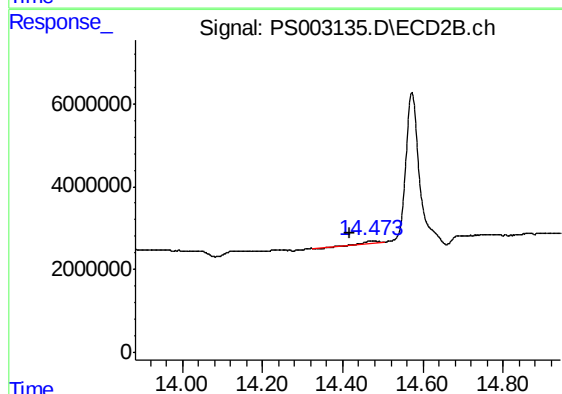


#12 2,4,5-T

R.T.: 14.473 min
Delta R.T.: 0.056 min
Response: 386919
Conc: 0.20 ng/ml

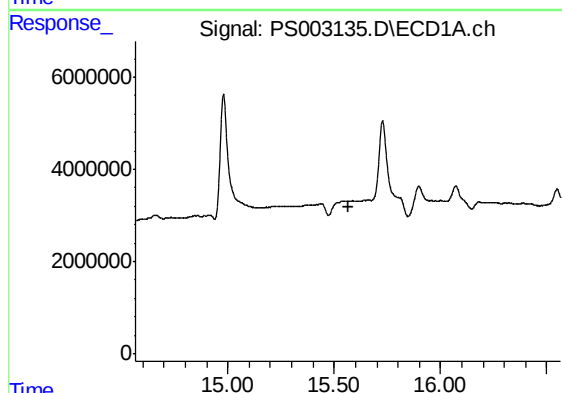


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.565 min
Response: 0
Conc: N.D.

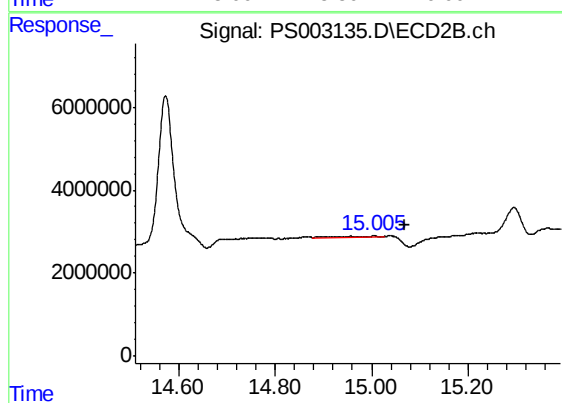

#13 2,4-DB


R.T.: 15.005 min
Delta R.T.: -0.064 min
Response: 1116628
Conc: 4.40 ng/ml

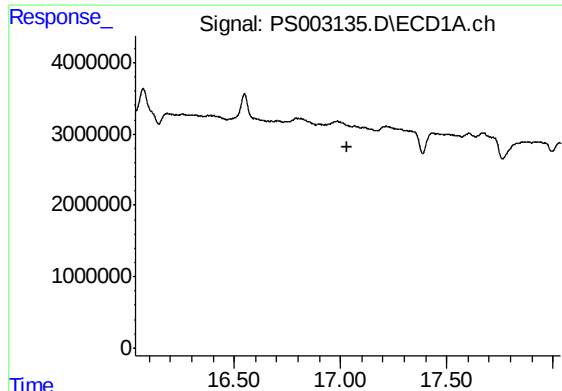

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1

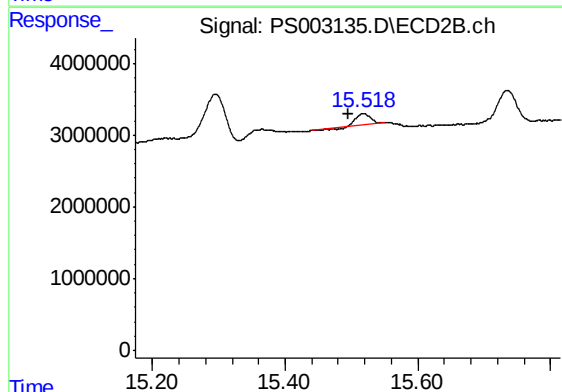


#14 DINOSEB

R.T.: 15.518 min
Delta R.T.: 0.023 min
Response: 2269671
Conc: 1.29 ng/ml

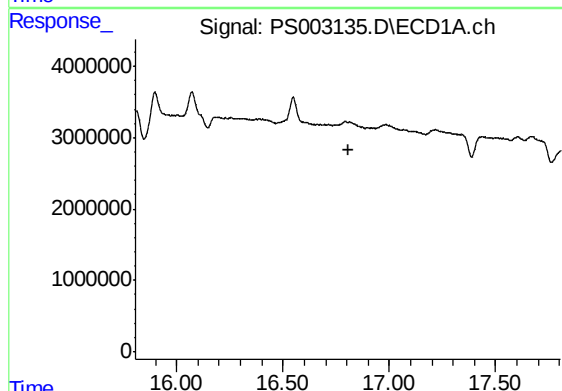


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

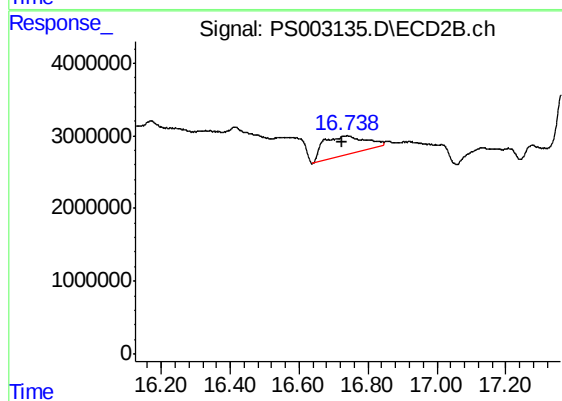

#15 Picloram


R.T.: 16.737 min
Delta R.T.: 0.013 min
Response: 22282039
Conc: 7.41 ng/ml

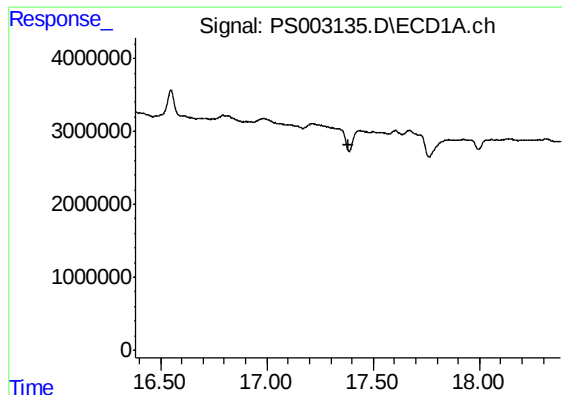

#16 DCPA

R.T.: 17.437 min
Delta R.T.: 0.056 min
Response: -5773586
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1

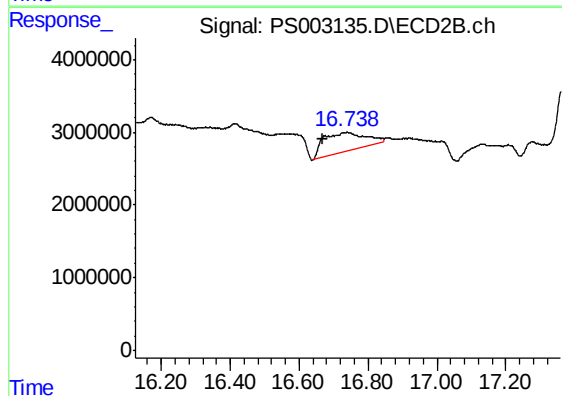

#16 DCPA

R.T.: 16.737 min
Delta R.T.: 0.068 min
Response: 22282039
Conc: 7.19 ng/ml