

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021219\
 Data File : PS003136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 12:46
 Operator : EI\SJ
 Sample : K1453-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 M-8-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 01:17:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.279	10.780	83459941	111.9E6	219.839	261.697
Target Compounds							
1) T	Dalapon	0.000	2.287	0 46694899	N.D.	87.130	#
2) T	3,5-DICHL...	0.000	8.947	0 4135876	N.D.	7.339	#
5) T	DICAMBA	11.692	0.000	4408724	0	2.750	N.D. #
7) T	MCPA	0.000	11.722	0 78196784	N.D.	49.710	#
14) T	DINOSEB	0.000	15.482	0 4912375	N.D.	2.802	#
15) T	Picloram	0.000	16.707	0 15452147	N.D.	5.140	#
16) T	DCPA	0.000	16.707	0 15452147	N.D.	4.988	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021219\
Data File : PS003136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 12:46
Operator : EI\SJ
Sample : K1453-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
M-8-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 01:17:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

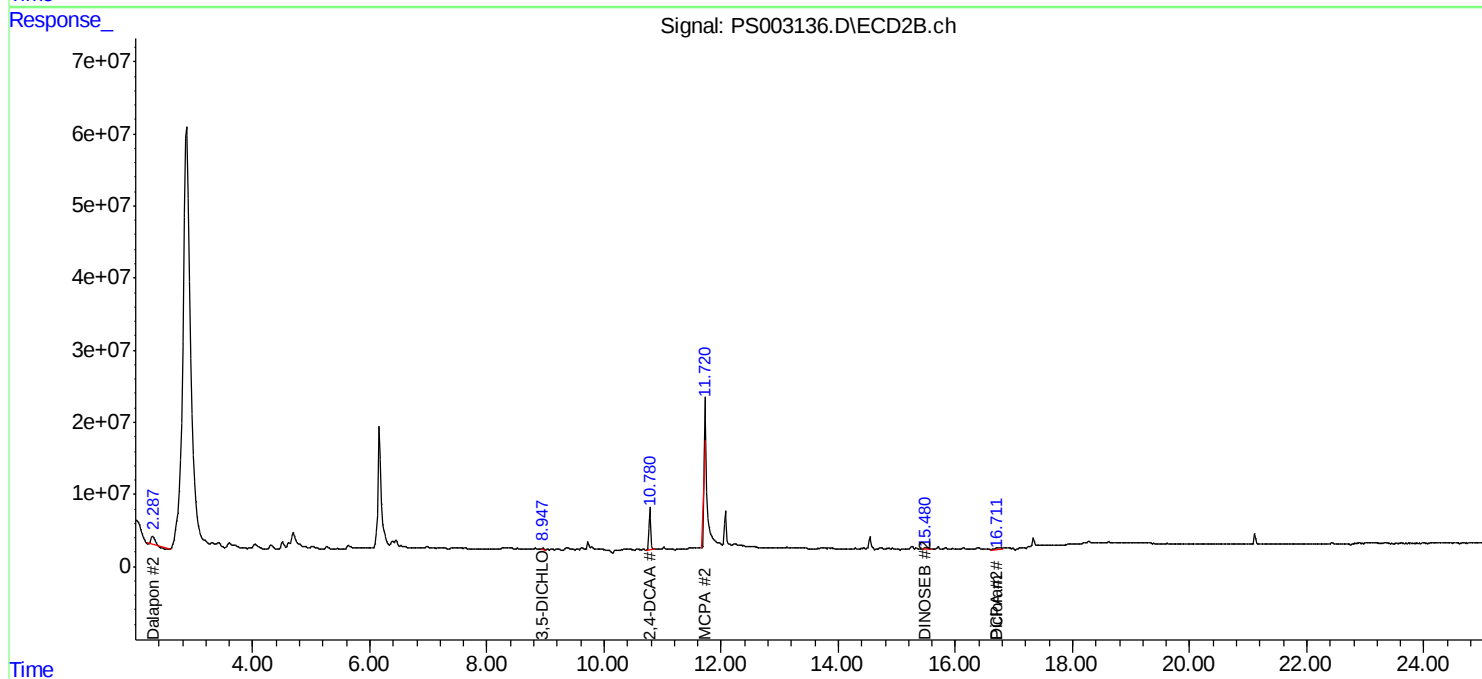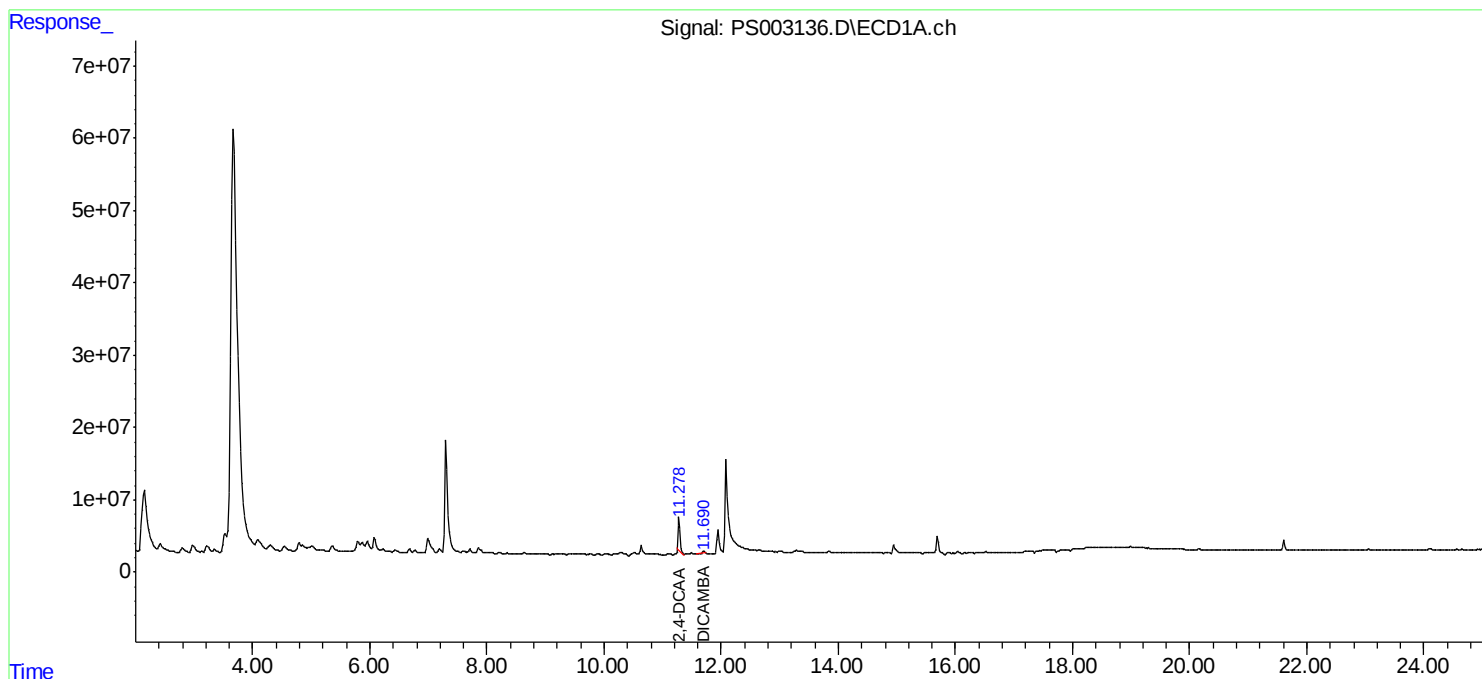


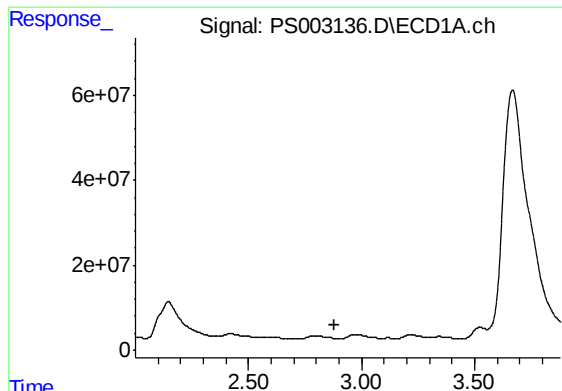

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-8-S

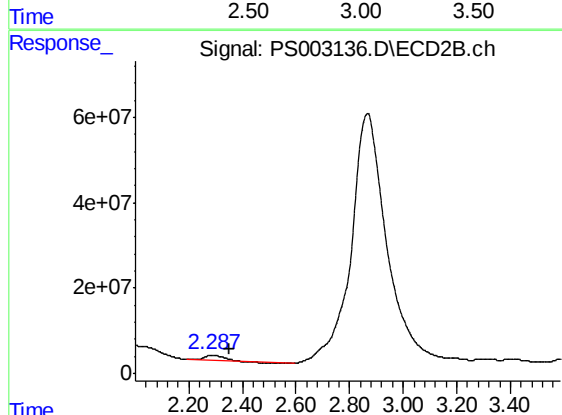


#1 Dalapon

R.T.: 2.287 min
Delta R.T.: -0.064 min
Response: 46694899
Conc: 87.13 ng/ml

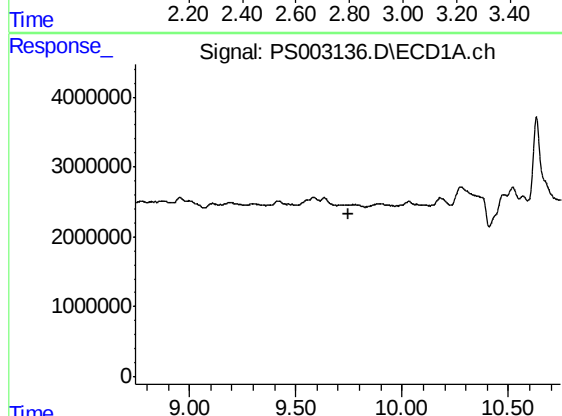


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

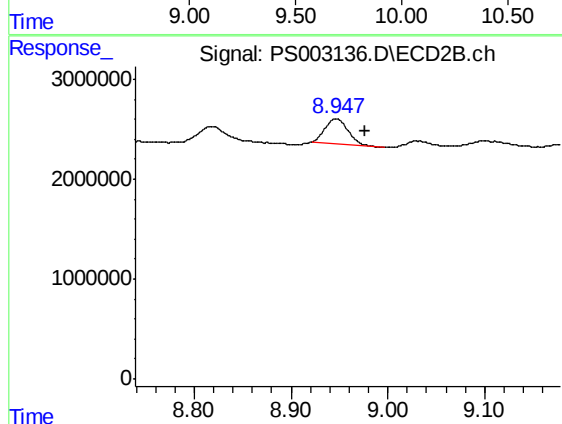

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.947 min
Delta R.T.: -0.030 min
Response: 4135876
Conc: 7.34 ng/ml

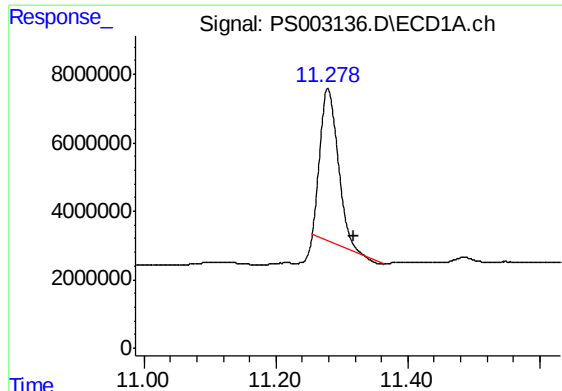

#4 2,4-DCAA


R.T.: 11.279 min
Delta R.T.: -0.039 min
Response: 83459941
Conc: 219.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
M-8-S

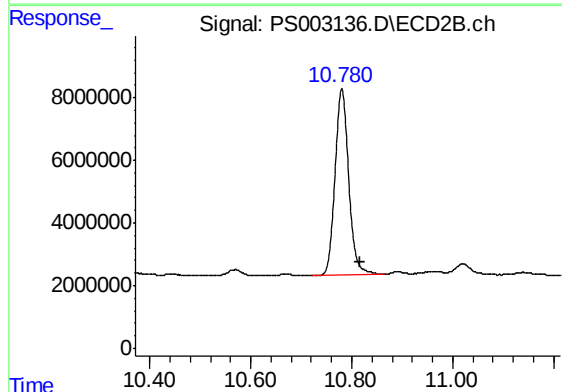


#4 2,4-DCAA

R.T.: 10.780 min
Delta R.T.: -0.036 min
Response: 111887518
Conc: 261.70 ng/ml

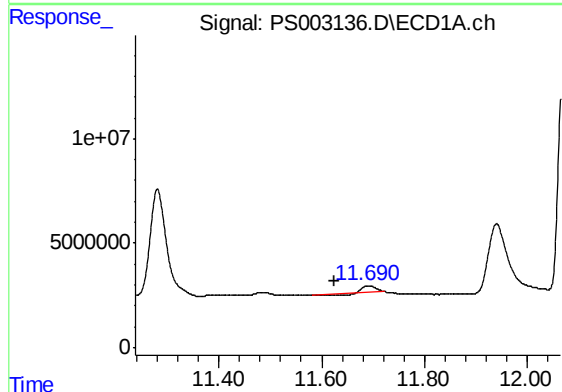


#5 DICAMBA

R.T.: 11.692 min
Delta R.T.: 0.068 min
Response: 4408724
Conc: 2.75 ng/ml

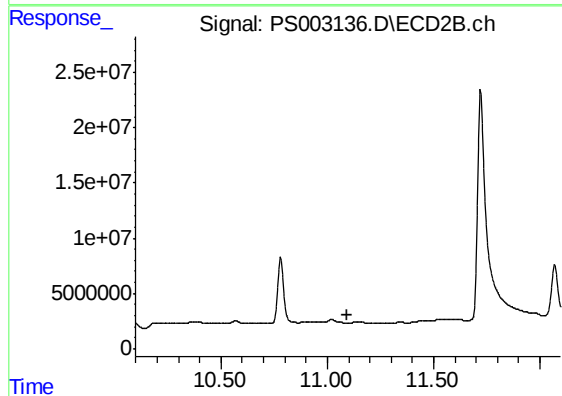

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.097 min
Response: 0
Conc: N.D.

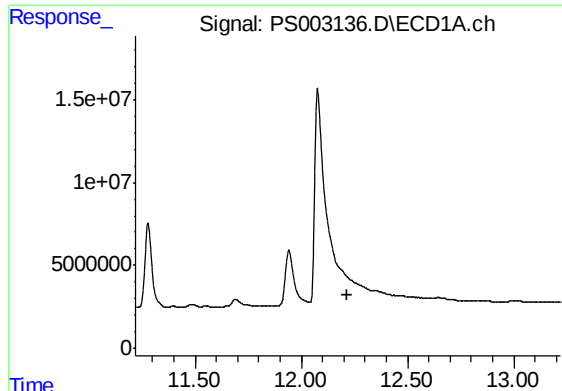

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-8-S

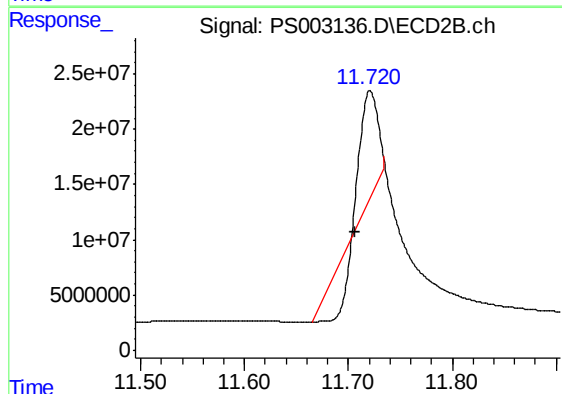


#7 MCPA

R.T.: 11.722 min
Delta R.T.: 0.016 min
Response: 78196784
Conc: 49.71 ug/ml

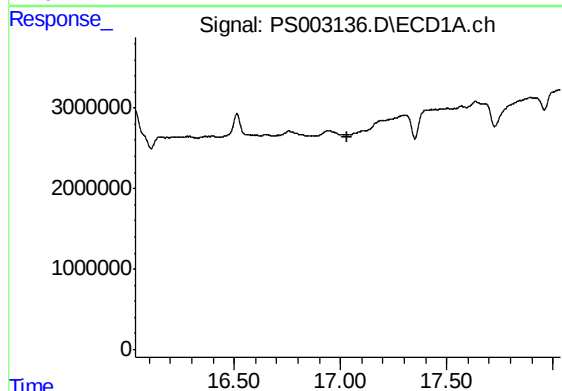


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

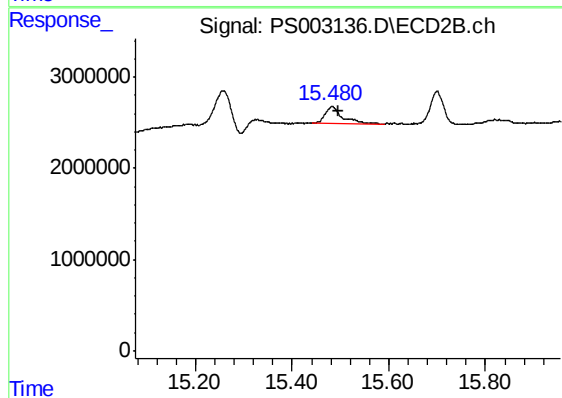

#14 DINOSEB


R.T.: 15.482 min
Delta R.T.: -0.012 min
Response: 4912375
Conc: 2.80 ng/ml

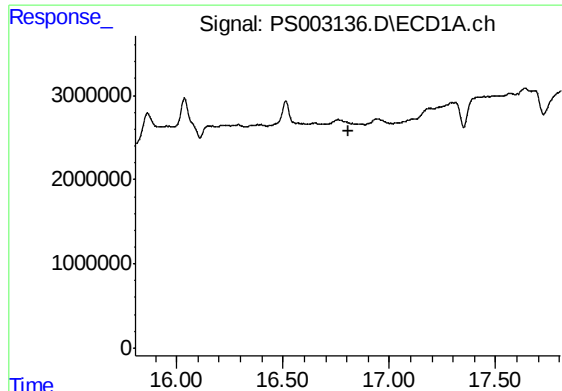

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-8-S

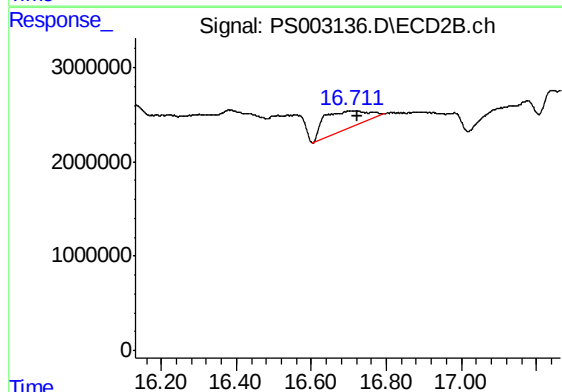


#15 Picloram

R.T.: 16.707 min
Delta R.T.: -0.017 min
Response: 15452147
Conc: 5.14 ng/ml

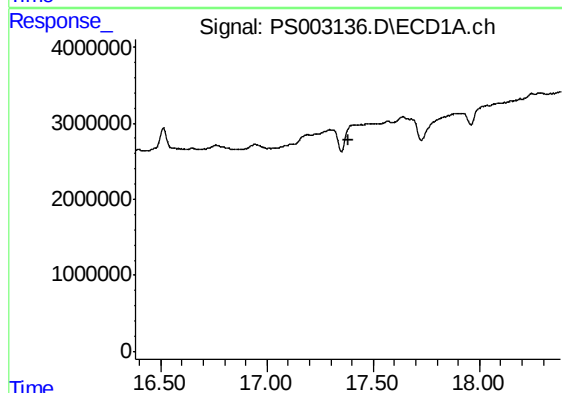

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

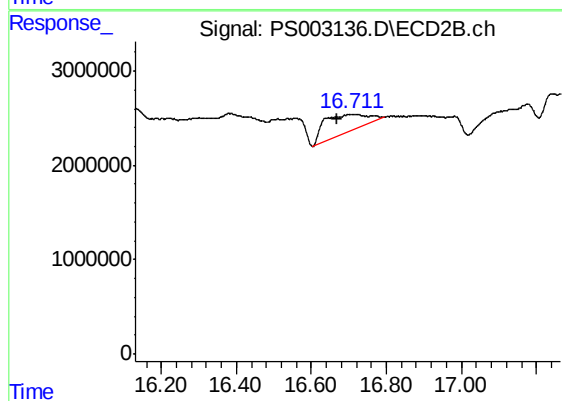

#16 DCPA

R.T.: 16.707 min
Delta R.T.: 0.037 min
Response: 15452147
Conc: 4.99 ng/ml