

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021219\
 Data File : PS003139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 14:20
 Operator : EI\SJ
 Sample : K1453-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 M-9-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 01:17:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.294	10.795	150.8E6	148.0E6	397.182	346.049
Target Compounds							
1) T	Dalapon	0.000	2.303	0 78789752		N.D.	147.017 #
2) T	3,5-DICHL...	0.000	8.961	0 4815673		N.D.	8.545 #
3) T	4-Nitroph...	0.000	9.977	0 52854201		N.D.	252.864 #
6) T	MCP	11.961	0.000	29387038	0	24.528	N.D. #
14) T	DINOSEB	0.000	15.499	0 5940290		N.D.	3.389 #
15) T	Picloram	0.000	16.719	0 15227796		N.D.	5.065 #
16) T	DCPA	17.424	16.719	-4327177	15227796	N.D.	4.916



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021219\
Data File : PS003139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 14:20
Operator : EI\SJ
Sample : K1453-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
M-9-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 01:17:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

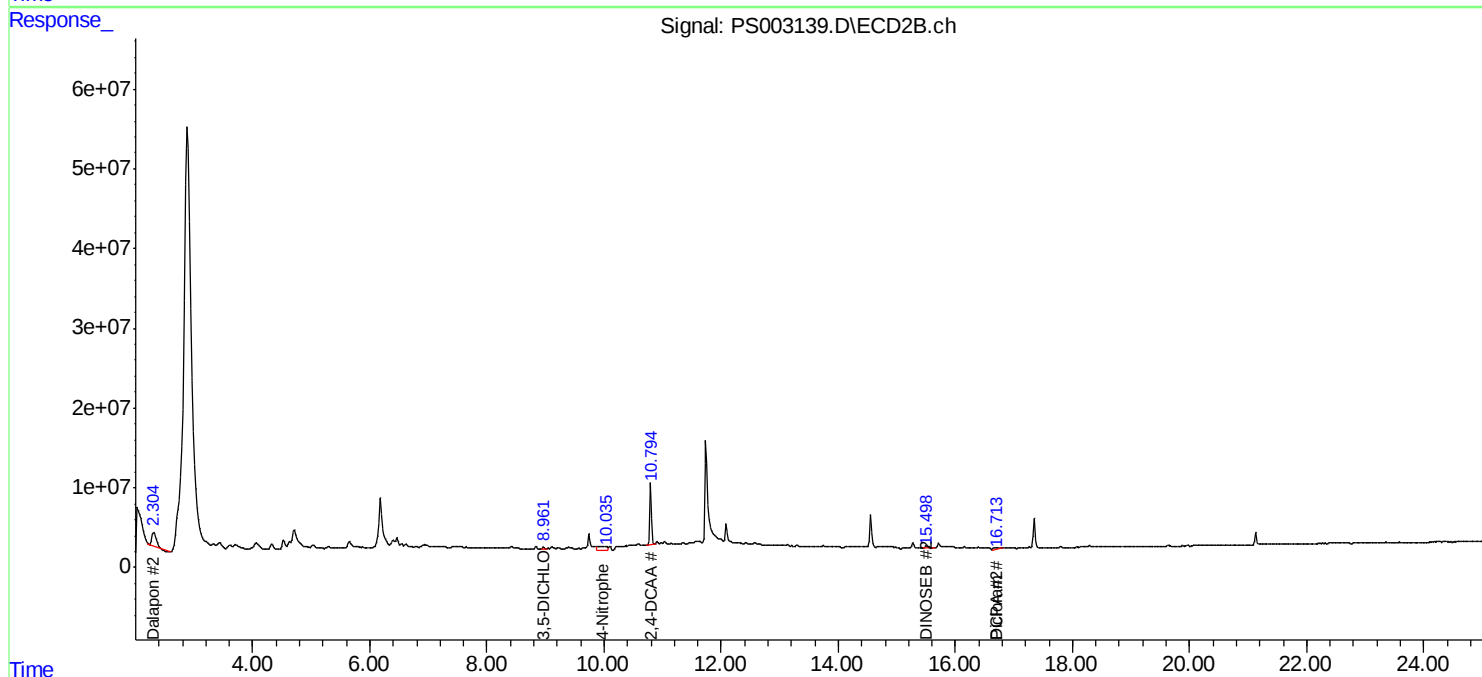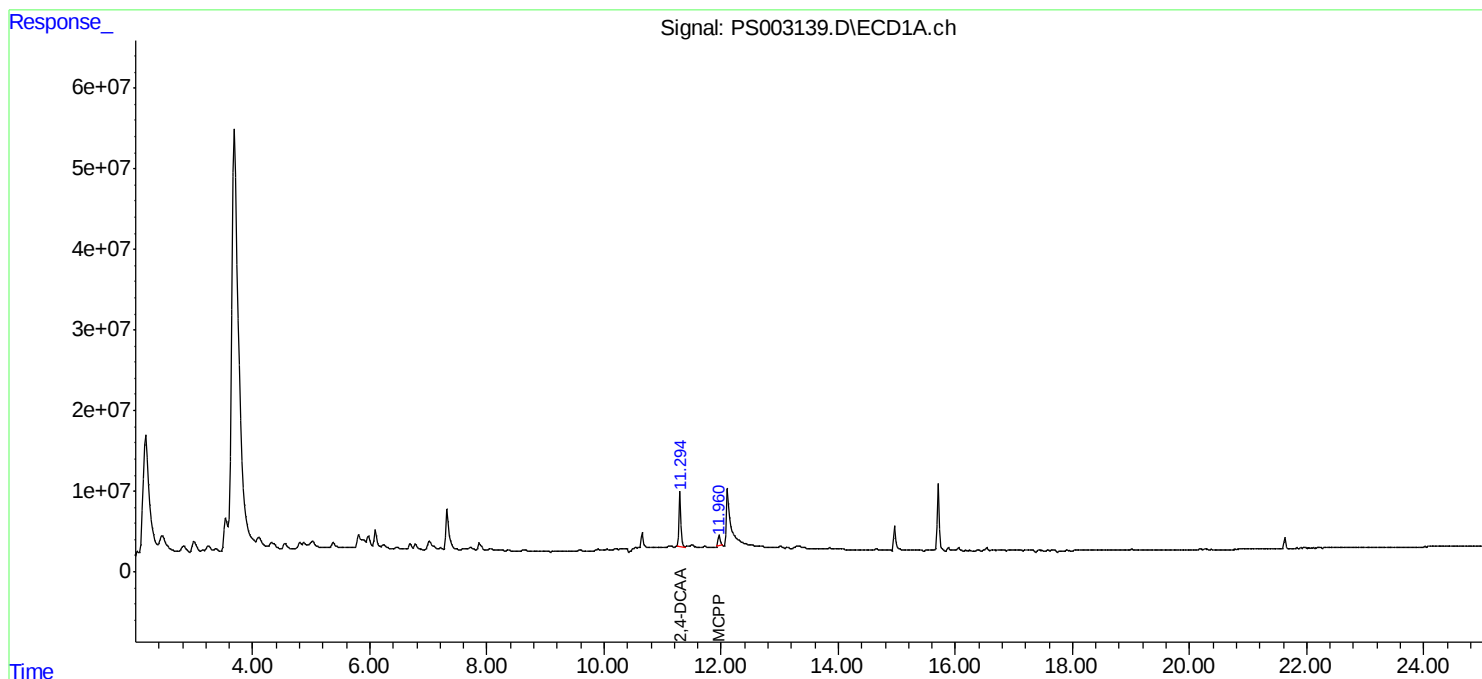


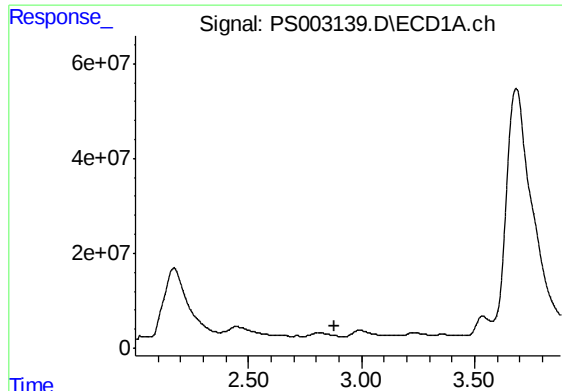

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-9-D

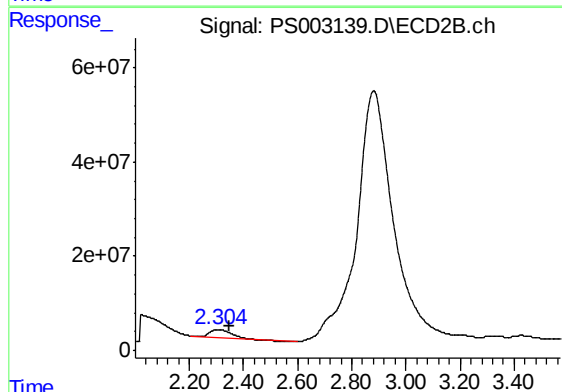


#1 Dalapon

R.T.: 2.303 min
Delta R.T.: -0.048 min
Response: 78789752
Conc: 147.02 ng/ml

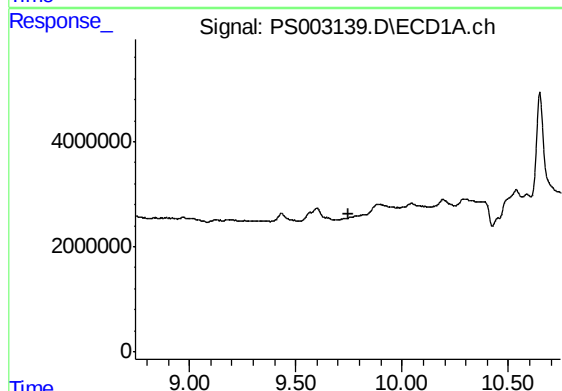


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

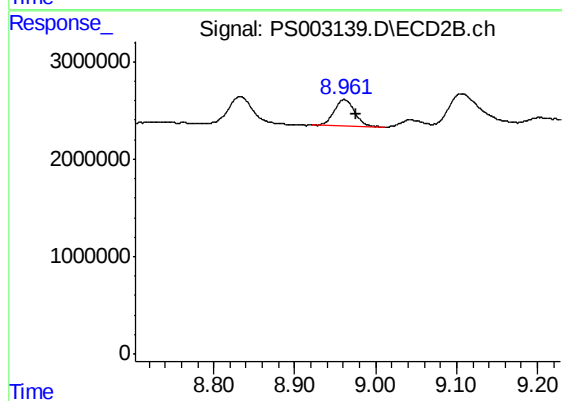

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.961 min
Delta R.T.: -0.015 min
Response: 4815673
Conc: 8.54 ng/ml

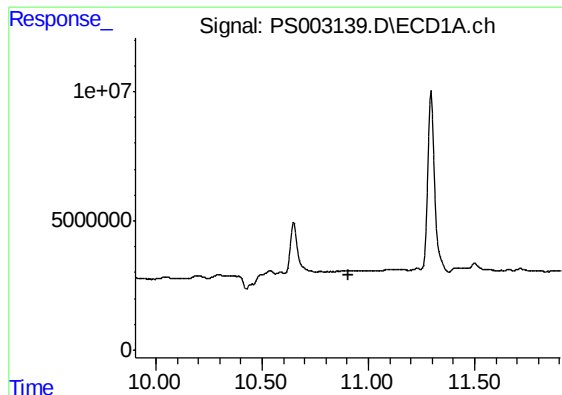

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-9-D

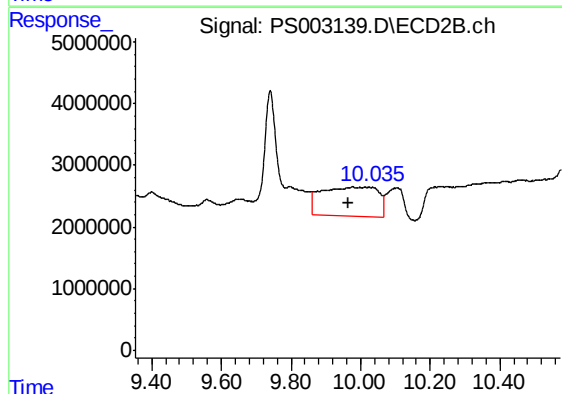


#3 4-Nitrophenol

R.T.: 9.977 min
Delta R.T.: 0.012 min
Response: 52854201
Conc: 252.86 ng/ml

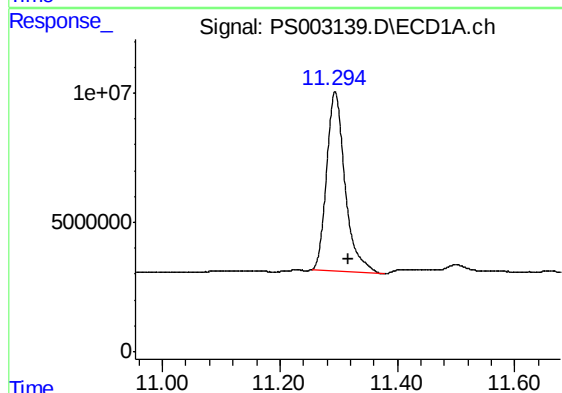


#4 2,4-DCAA

R.T.: 11.294 min
Delta R.T.: -0.024 min
Response: 150786570
Conc: 397.18 ng/ml

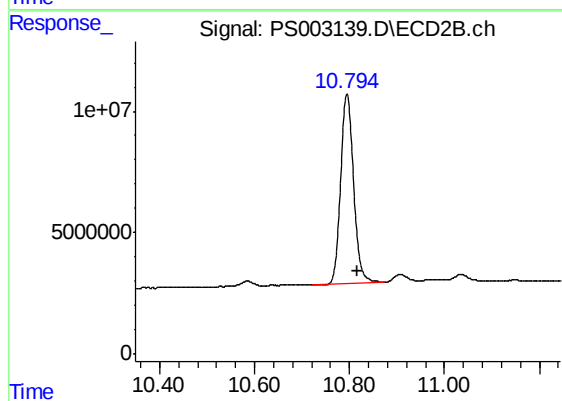

#4 2,4-DCAA


R.T.: 10.795 min
Delta R.T.: -0.022 min
Response: 147951932
Conc: 346.05 ng/ml

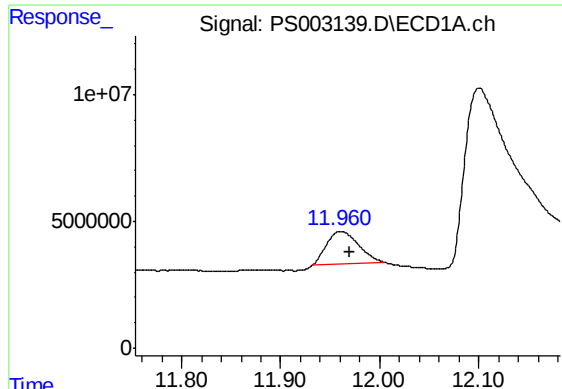

#6 MCP


R.T.: 11.961 min
Delta R.T.: -0.009 min
Response: 29387038
Conc: 24.53 ug/ml

Instrument :
ECD_S
ClientSampleId :
M-9-D

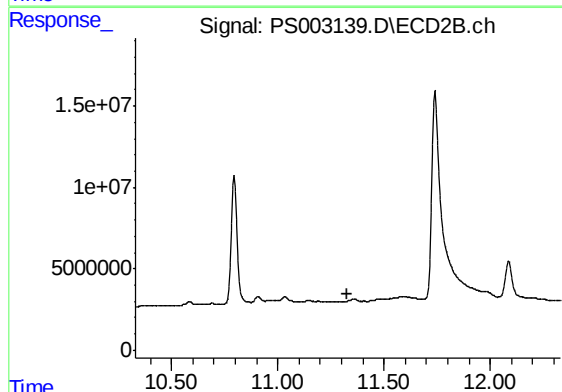


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

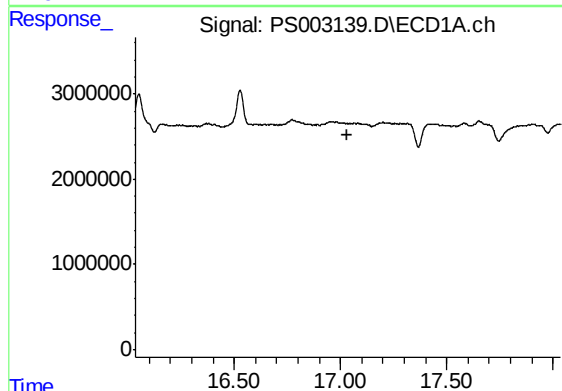


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

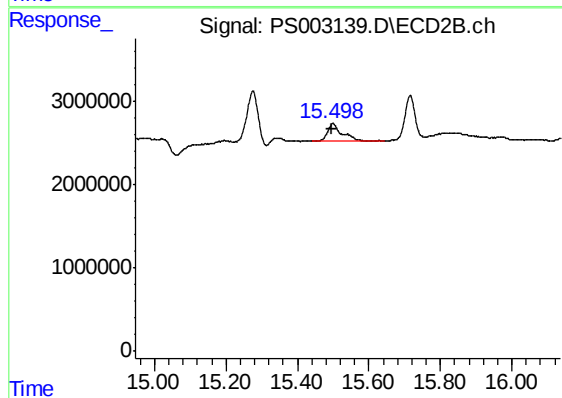

#14 DINOSEB


R.T.: 15.499 min
Delta R.T.: 0.004 min
Response: 5940290
Conc: 3.39 ng/ml

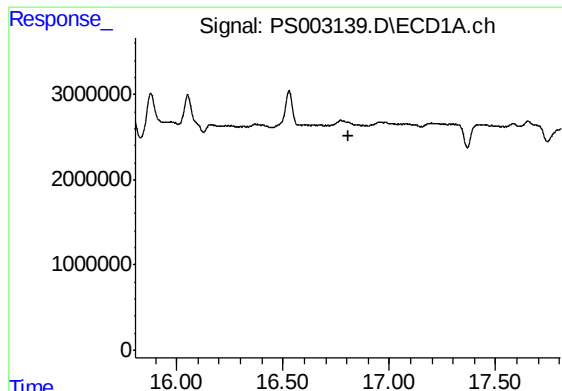

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-9-D

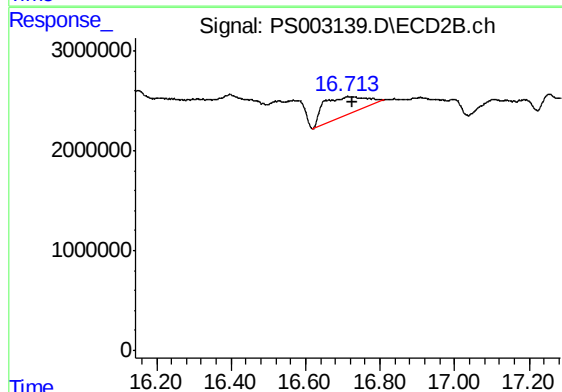


#15 Picloram

R.T.: 16.719 min
Delta R.T.: -0.005 min
Response: 15227796
Conc: 5.07 ng/ml

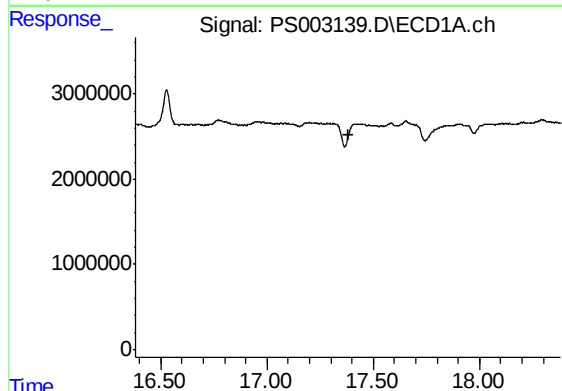

#16 DCPA

R.T.: 17.424 min
Delta R.T.: 0.042 min
Response: -4327177
Conc: N.D.

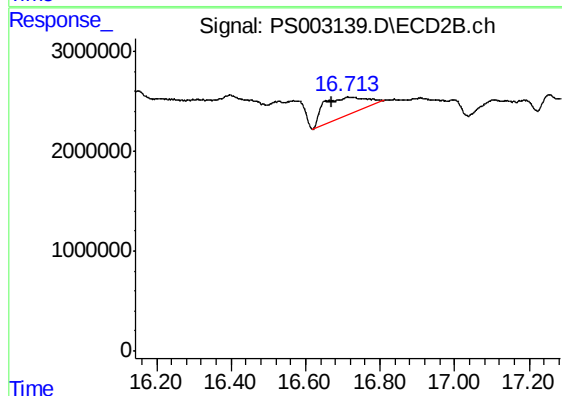

#16 DCPA

R.T.: 16.719 min
Delta R.T.: 0.049 min
Response: 15227796
Conc: 4.92 ng/ml