

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021220\
 Data File : PS008823.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2020 12:21
 Operator : DD\AJ
 Sample : L1481-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 72-11989

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 15:55:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.943	1154.4E6	504.3E6	537.871	544.163
Target Compounds							
2) T	3,5-DICHL...	0.000	6.117	0	135.5E6	N.D.	98.457
7) T	MCPA	7.801	0.000	78603653	0	9.150	N.D. #
10) T	Pentachlo...	8.678	8.470	305.2E6	153.6E6	10.735	11.643
11) T	2,4,5-TP ...	0.000	8.801	0	61826677	N.D.	12.063
16) T	DCPA	11.515	0.000	48042829	0	3.427	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021220\
Data File : PS008823.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2020 12:21
Operator : DD\AJ
Sample : L1481-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
72-11989

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 15:55:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

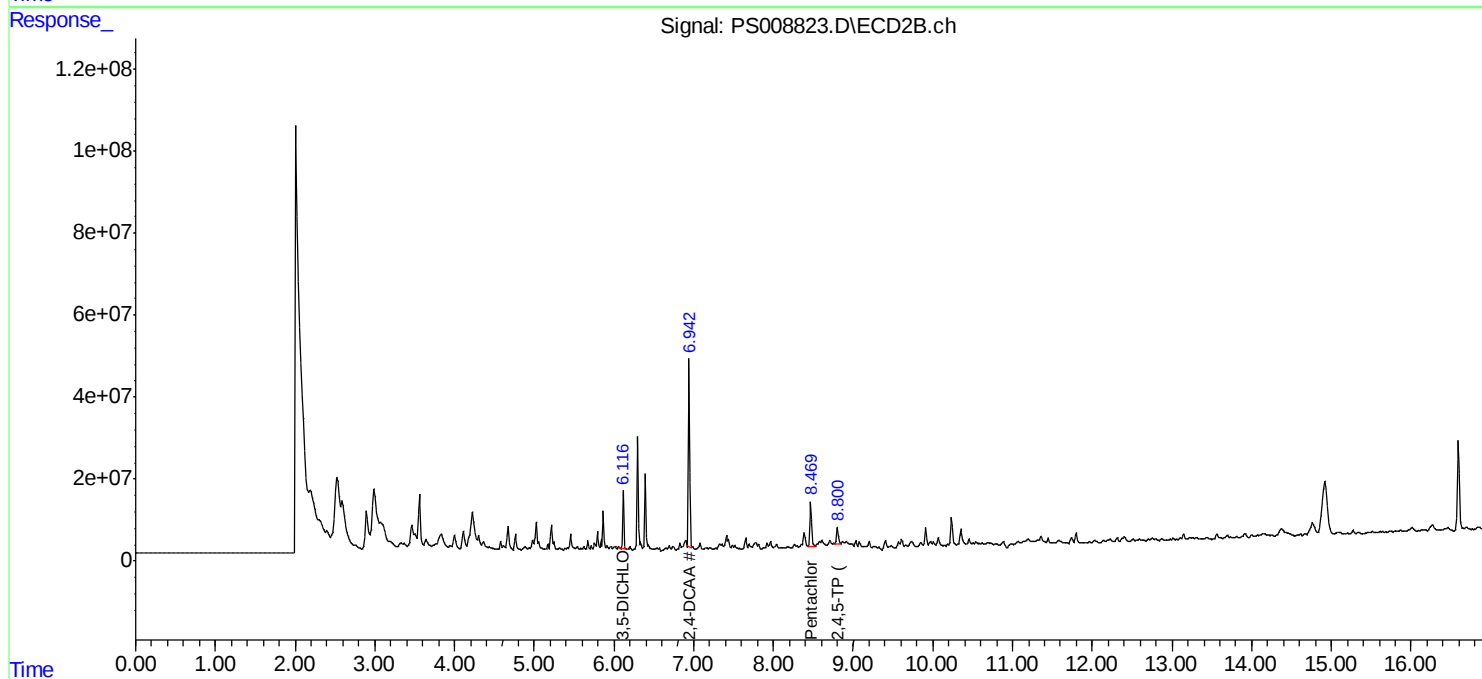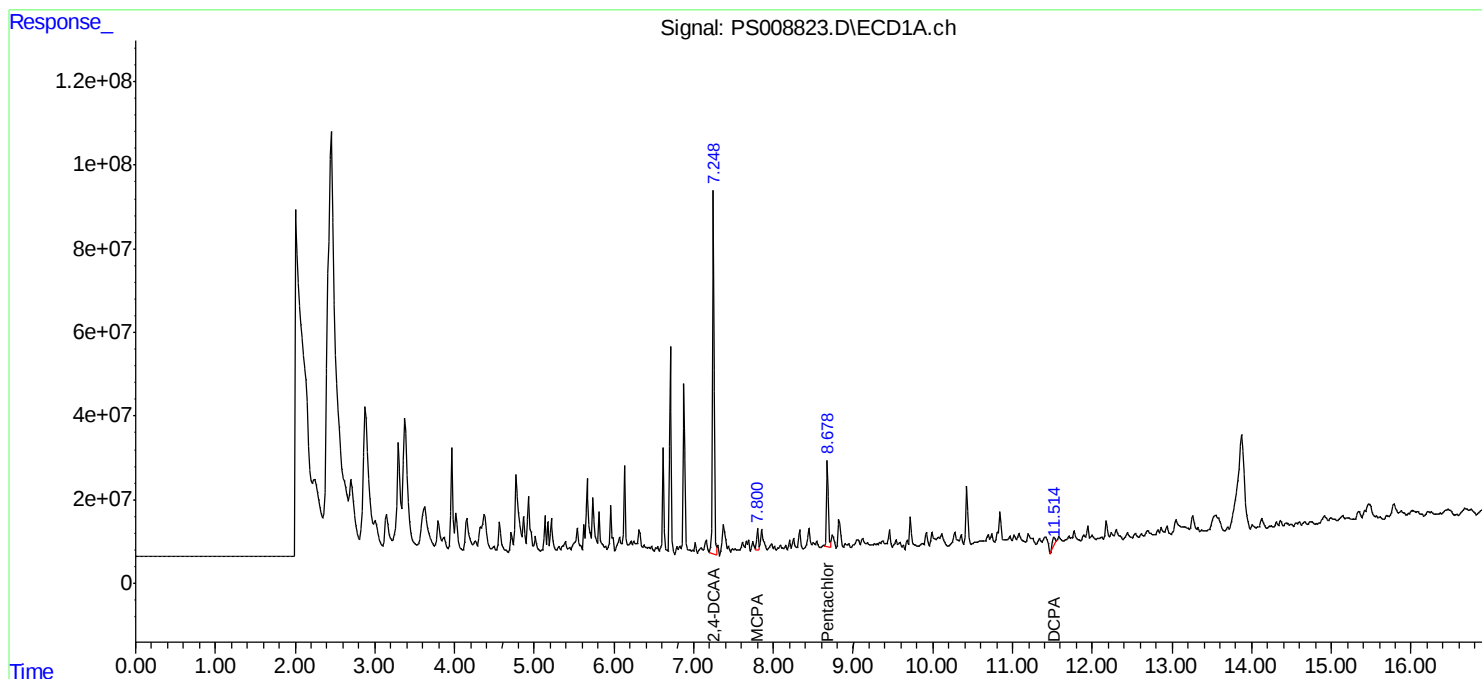


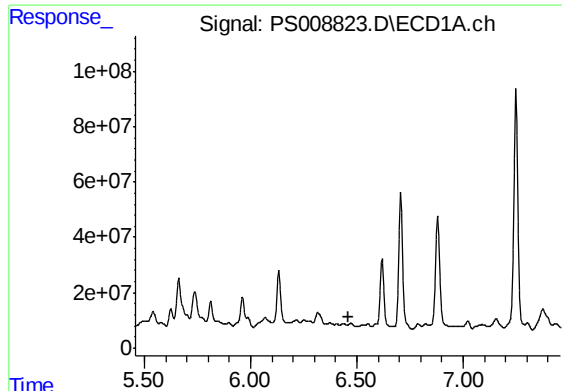

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
72-11989

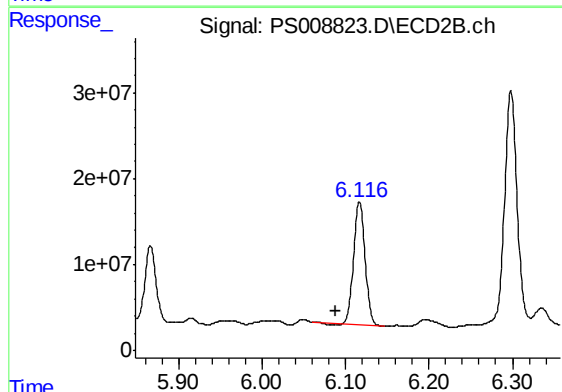


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.117 min
Delta R.T.: 0.029 min
Response: 135465054
Conc: 98.46 ng/ml

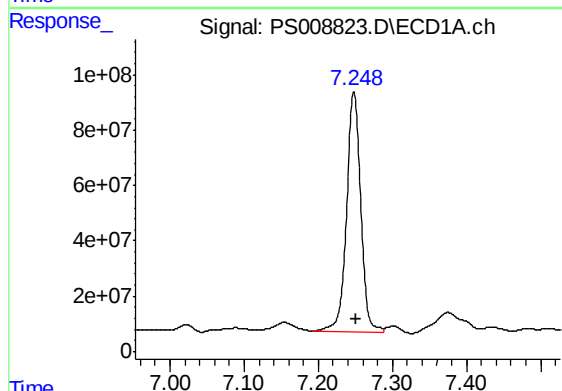


#4 2,4-DCAA

R.T.: 7.248 min
Delta R.T.: -0.004 min
Response: 1154436568
Conc: 537.87 ng/ml

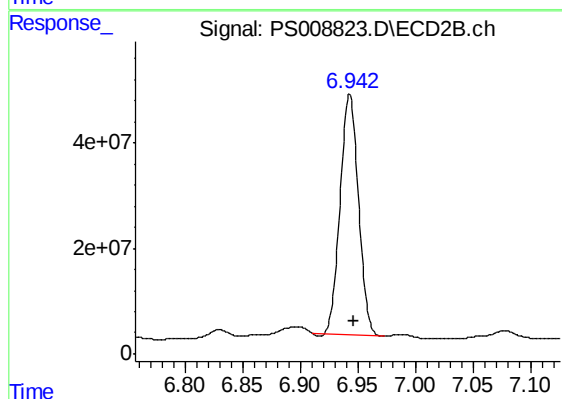

#4 2,4-DCAA


R.T.: 6.943 min
Delta R.T.: -0.004 min
Response: 504343369
Conc: 544.16 ng/ml

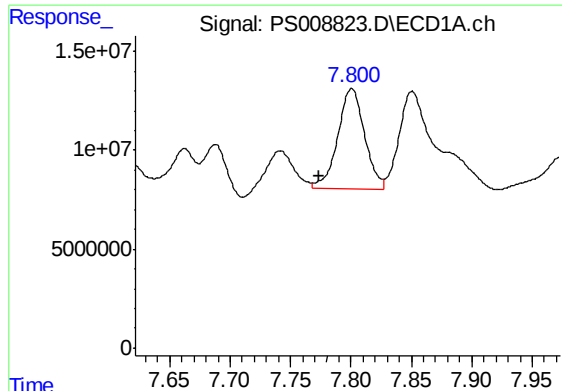

#7 MCPA


R.T.: 7.801 min
Delta R.T.: 0.027 min
Response: 78603653
Conc: 9.15 ug/ml

Instrument :
ECD_S
ClientSampleId :
72-11989

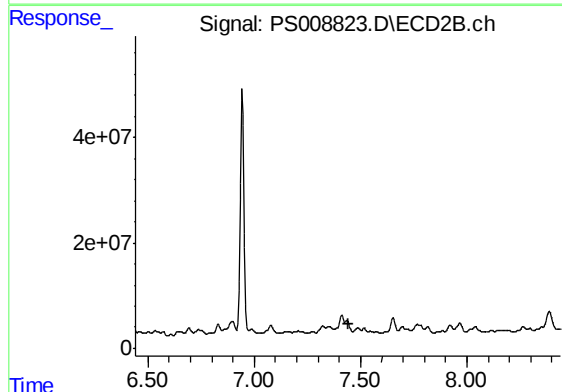


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.441 min
Response: 0
Conc: N.D.

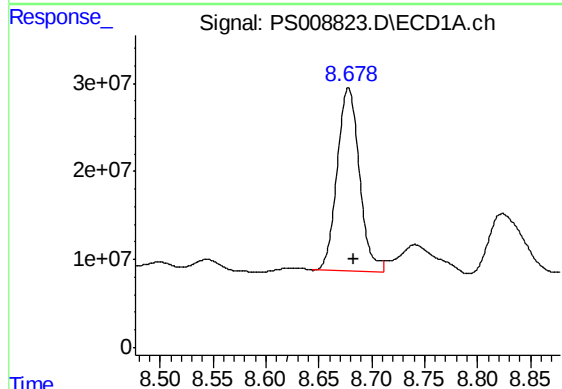


#10 Pentachlorophenol

R.T.: 8.678 min
Delta R.T.: -0.005 min
Response: 305183409
Conc: 10.74 ng/ml

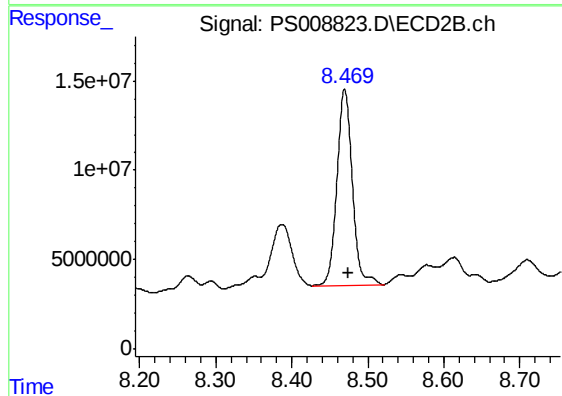

#10 Pentachlorophenol


R.T.: 8.470 min
Delta R.T.: -0.006 min
Response: 153558089
Conc: 11.64 ng/ml

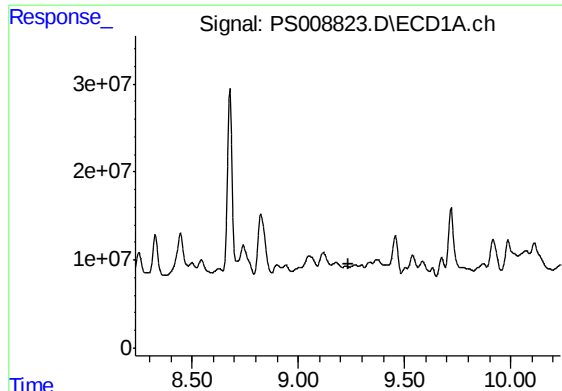

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.234 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
72-11989

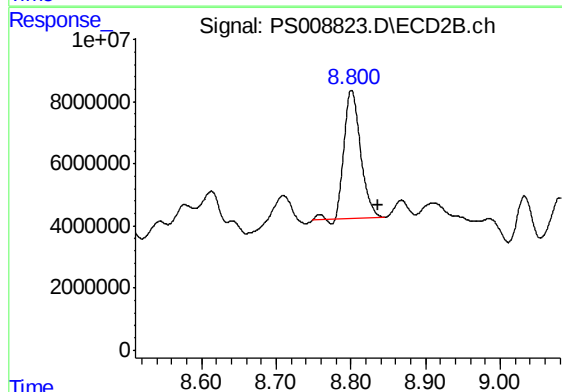


#11 2,4,5-TP (SILVEX)

R.T.: 8.801 min
Delta R.T.: -0.035 min
Response: 61826677
Conc: 12.06 ng/ml

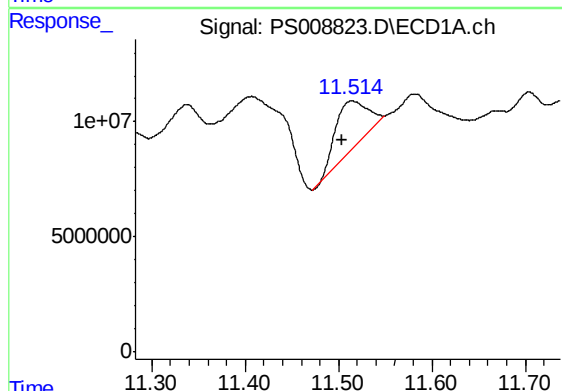

#16 DCPA

R.T.: 11.515 min
Delta R.T.: 0.011 min
Response: 48042829
Conc: 3.43 ng/ml

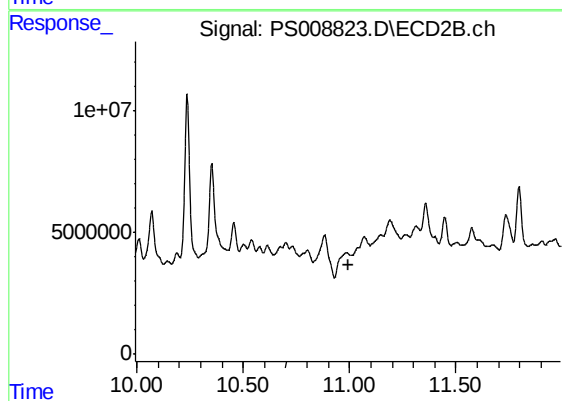

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.992 min
Response: 0
Conc: N.D.