

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021220\
 Data File : PS008826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2020 14:44
 Operator : DD\AJ
 Sample : L1481-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 72-11931RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 16:07:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.244	6.941	2380.7E6	557.2E6	1109.214	601.152 #
Target Compounds							
1) T	Dalapon	0.000	2.586	0	129.8E6	N.D.	108.229
2) T	3,5-DICHL...	0.000	6.114	0	165.9E6	N.D.	120.608
7) T	MCPA	7.804	7.409	66918974	62677952	7.790	15.018 #
8) T	DICHLORPROP	8.205	0.000	30882044	0	15.609	N.D. #
9) T	2,4-D	8.303	8.093	53685752	43841397	25.086	38.408 #
10) T	Pentachlo...	8.683	8.469	34820.6E6	16192.6E6	1224.834	1227.728
11) T	2,4,5-TP ...	9.255	8.808	120.5E6	272.9E6	10.777	53.250 #
12) T	2,4,5-T	9.465	0.000	154.6E6	0	14.046	N.D. #
13) T	2,4-DB	10.048	9.714	469.4E6	233.2E6	288.555	333.518



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021220\
Data File : PS008826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2020 14:44
Operator : DD\AJ
Sample : L1481-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
72-11931RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 16:07:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

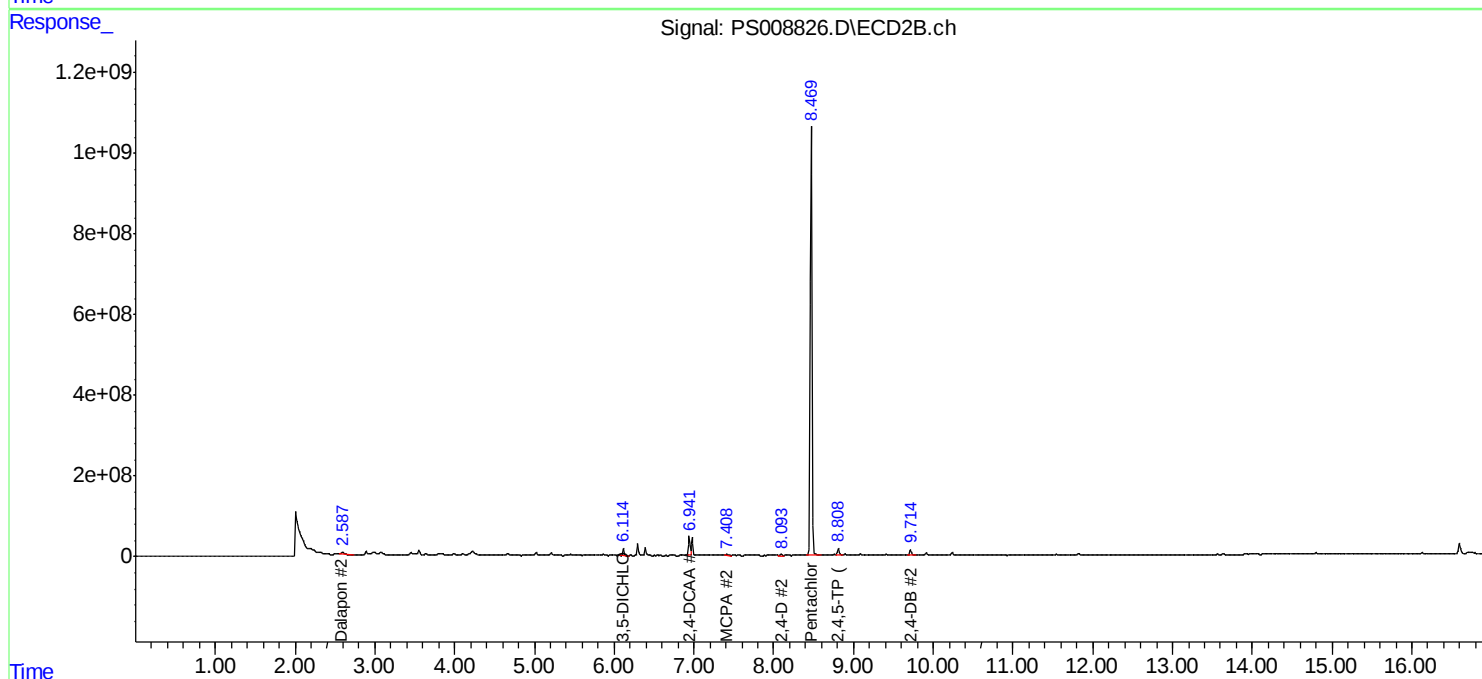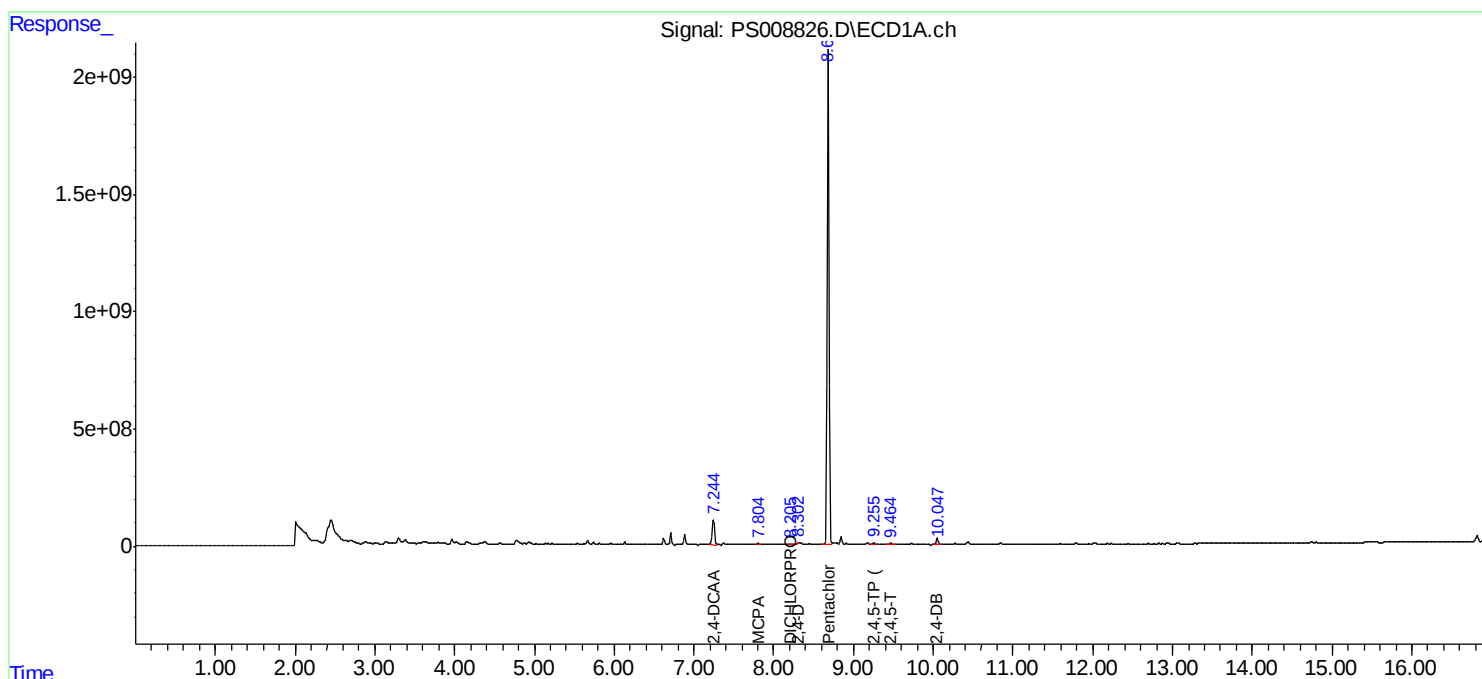


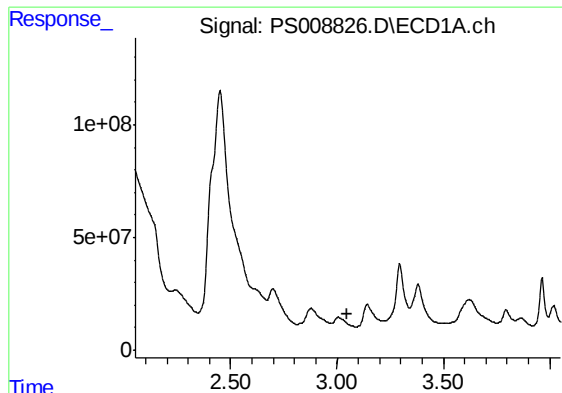

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
72-11931RE

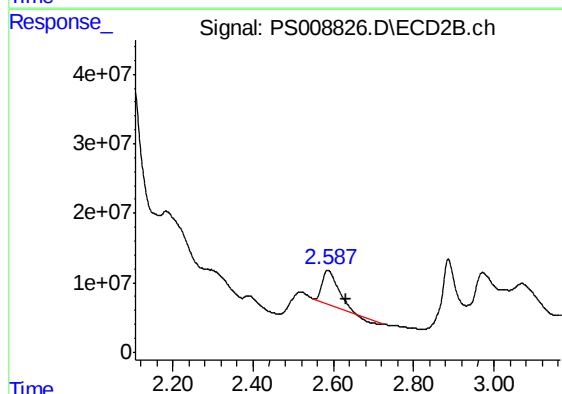


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.046 min
Response: 129801260
Conc: 108.23 ng/ml

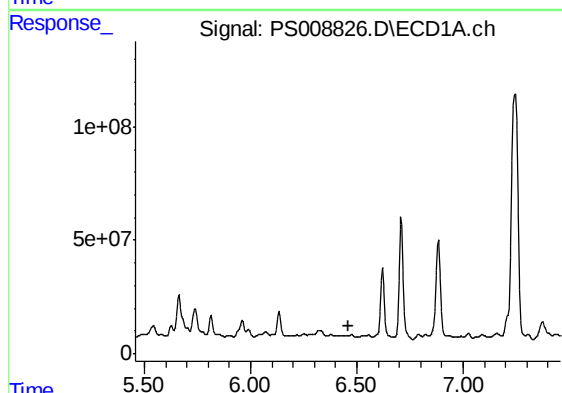


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.458 min
Response: 0
Conc: N.D.

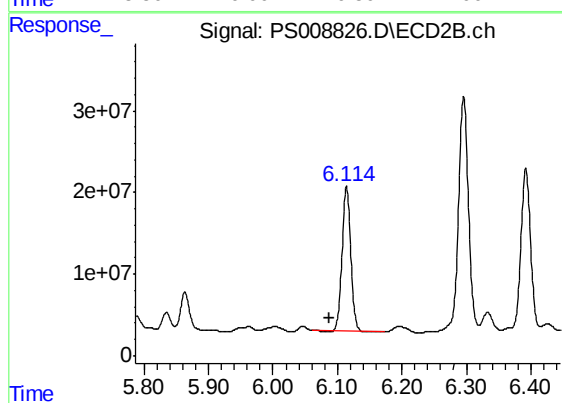

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.026 min
Response: 165943321
Conc: 120.61 ng/ml

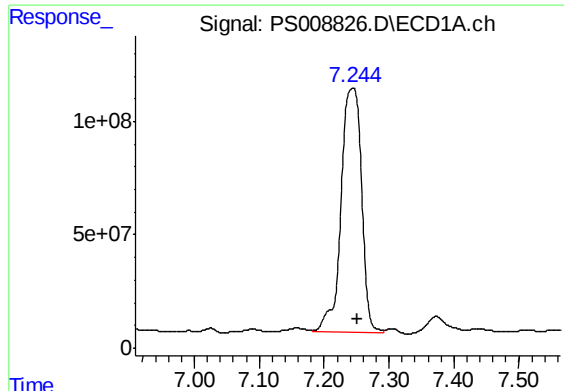

#4 2,4-DCAA


R.T.: 7.244 min
Delta R.T.: -0.008 min
Response: 2380714999
Conc: 1109.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
72-11931RE

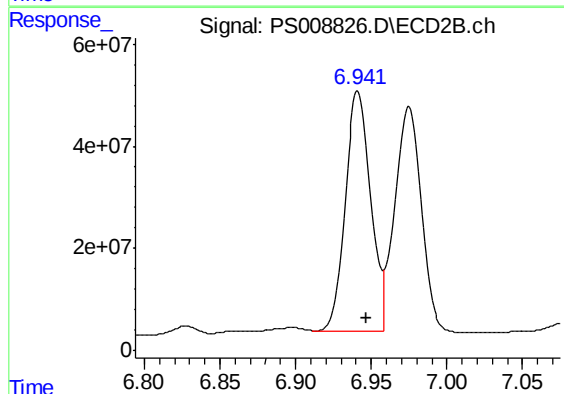


#4 2,4-DCAA

R.T.: 6.941 min
Delta R.T.: -0.005 min
Response: 557162007
Conc: 601.15 ng/ml

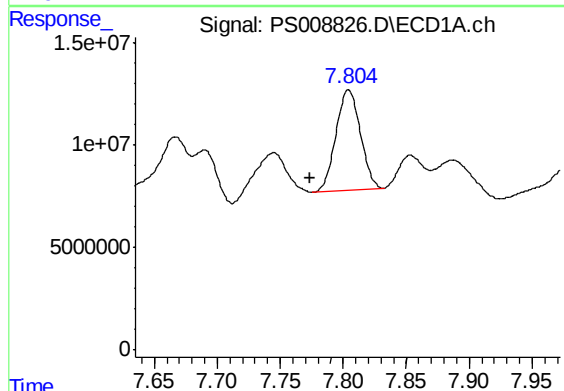


#7 MCPA

R.T.: 7.804 min
Delta R.T.: 0.031 min
Response: 66918974
Conc: 7.79 ug/ml

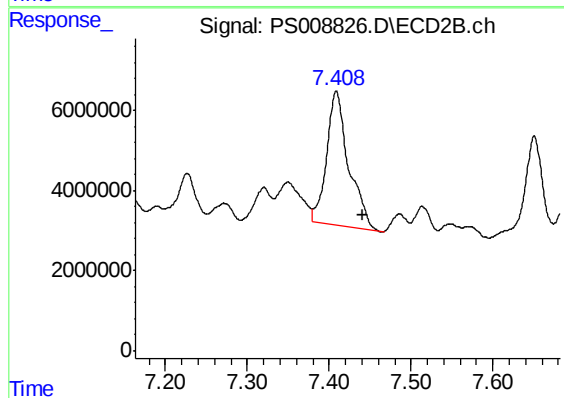

#7 MCPA


R.T.: 7.409 min
Delta R.T.: -0.032 min
Response: 62677952
Conc: 15.02 ug/ml

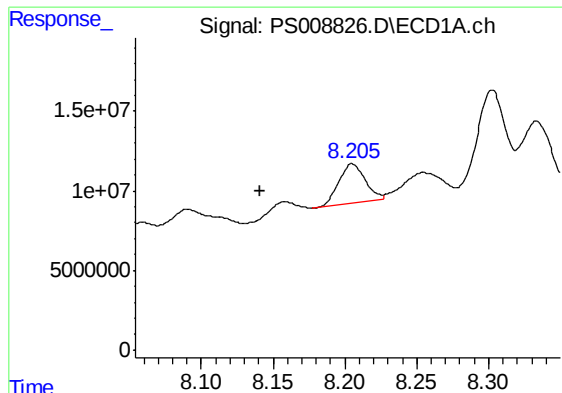

#8 DICHLORPROP


R.T.: 8.205 min
Delta R.T.: 0.064 min
Response: 30882044
Conc: 15.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
72-11931RE

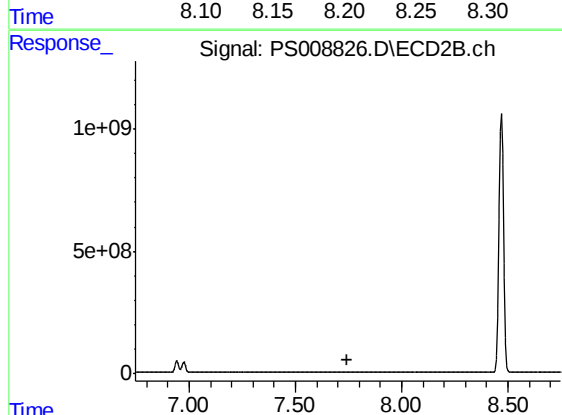


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.747 min
Response: 0
Conc: N.D.

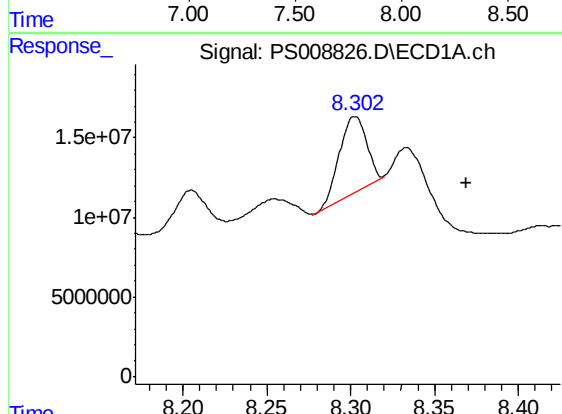


#9 2,4-D

R.T.: 8.303 min
Delta R.T.: -0.066 min
Response: 53685752
Conc: 25.09 ng/ml

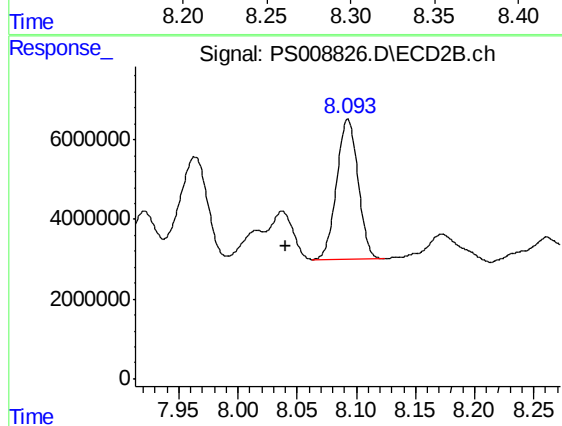

#9 2,4-D


R.T.: 8.093 min
Delta R.T.: 0.052 min
Response: 43841397
Conc: 38.41 ng/ml

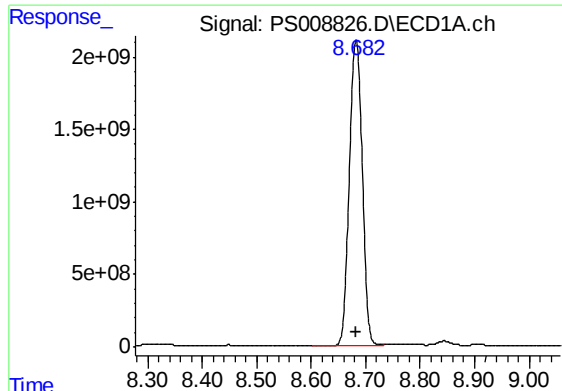

#10 Pentachlorophenol


R.T.: 8.683 min
Delta R.T.: 0.000 min
Response: 34820588391
Conc: 1224.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
72-11931RE

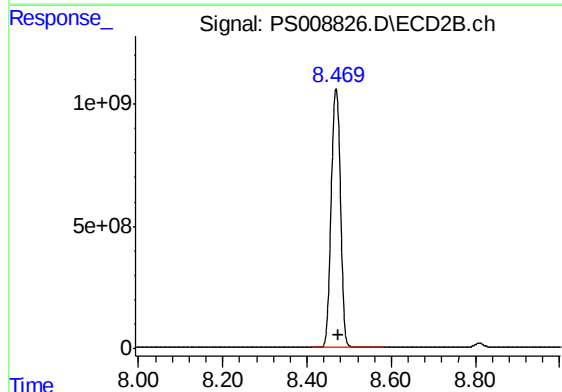


#10 Pentachlorophenol

R.T.: 8.469 min
Delta R.T.: -0.006 min
Response: 16192612051
Conc: 1227.73 ng/ml

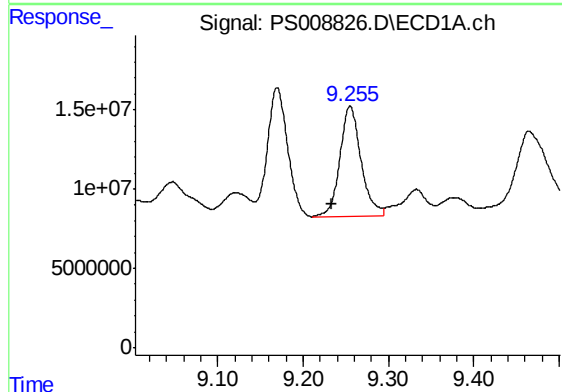


#11 2,4,5-TP (SILVEX)

R.T.: 9.255 min
Delta R.T.: 0.021 min
Response: 120464446
Conc: 10.78 ng/ml

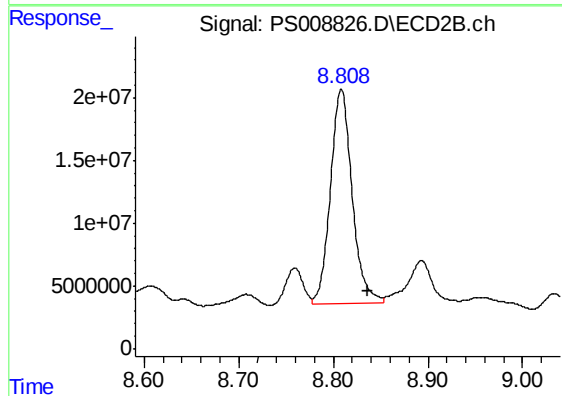

#11 2,4,5-TP (SILVEX)


R.T.: 8.808 min
Delta R.T.: -0.028 min
Response: 272915731
Conc: 53.25 ng/ml

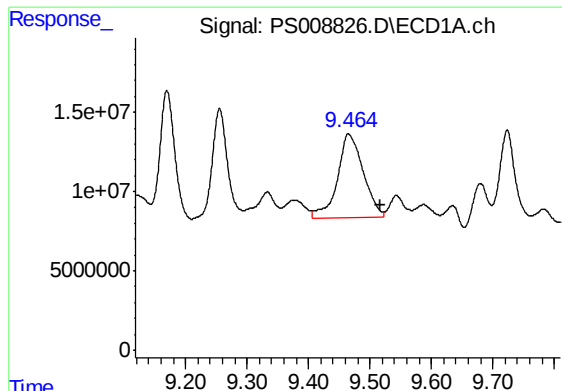

#12 2,4,5-T


R.T.: 9.465 min
Delta R.T.: -0.052 min
Response: 154593031
Conc: 14.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
72-11931RE

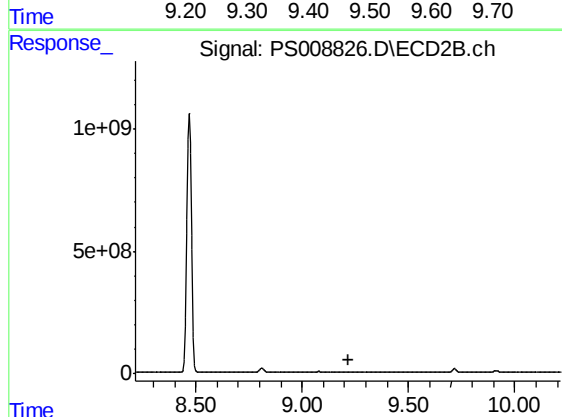


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.216 min
Response: 0
Conc: N.D.

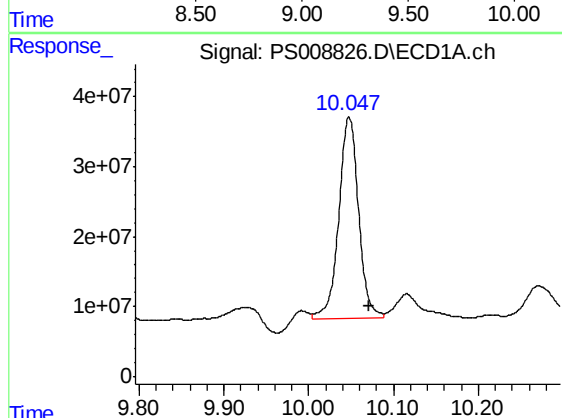

#13 2,4-DB

R.T.: 10.048 min
Delta R.T.: -0.023 min
Response: 469360393
Conc: 288.55 ng/ml

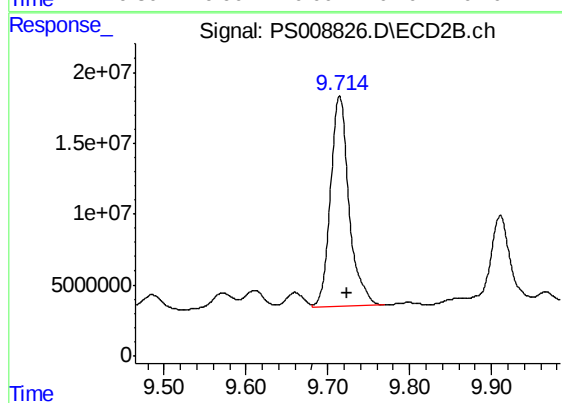

#13 2,4-DB

R.T.: 9.714 min
Delta R.T.: -0.010 min
Response: 233218693
Conc: 333.52 ng/ml