

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021221\
 Data File : PS014004.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2021 08:03
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 17:36:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 28 01:00:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) T	DICAMBA	7.397	7.067	6387290	2863263	1.485 1.737
7) T	MCPA	7.671	0.000	7291307	0	1.611 N.D. #
10) T	Pentachlo...	8.626	8.413	13023108	5921351	<MDL 1.063 #
11) T	2,4,5-TP ...	9.177	8.777	11880207	5778148	1.892 2.517 #
12) T	2,4,5-T	9.472	9.168	18395961	6404630	2.856 2.876
14) T	DINOSEB	11.168	9.990	12047524	4337196	2.377 2.655
15) T	Picloram	11.014	10.998	136.9E6	67638751	16.123 19.820
16) T	DCPA	11.433	10.915	15538860	10422566	1.922 3.479 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS0121221\
Data File : PS014004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2021 08:03
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 17:36:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
Quant Title : 8080.M
QLast Update : Thu Jan 28 01:00:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

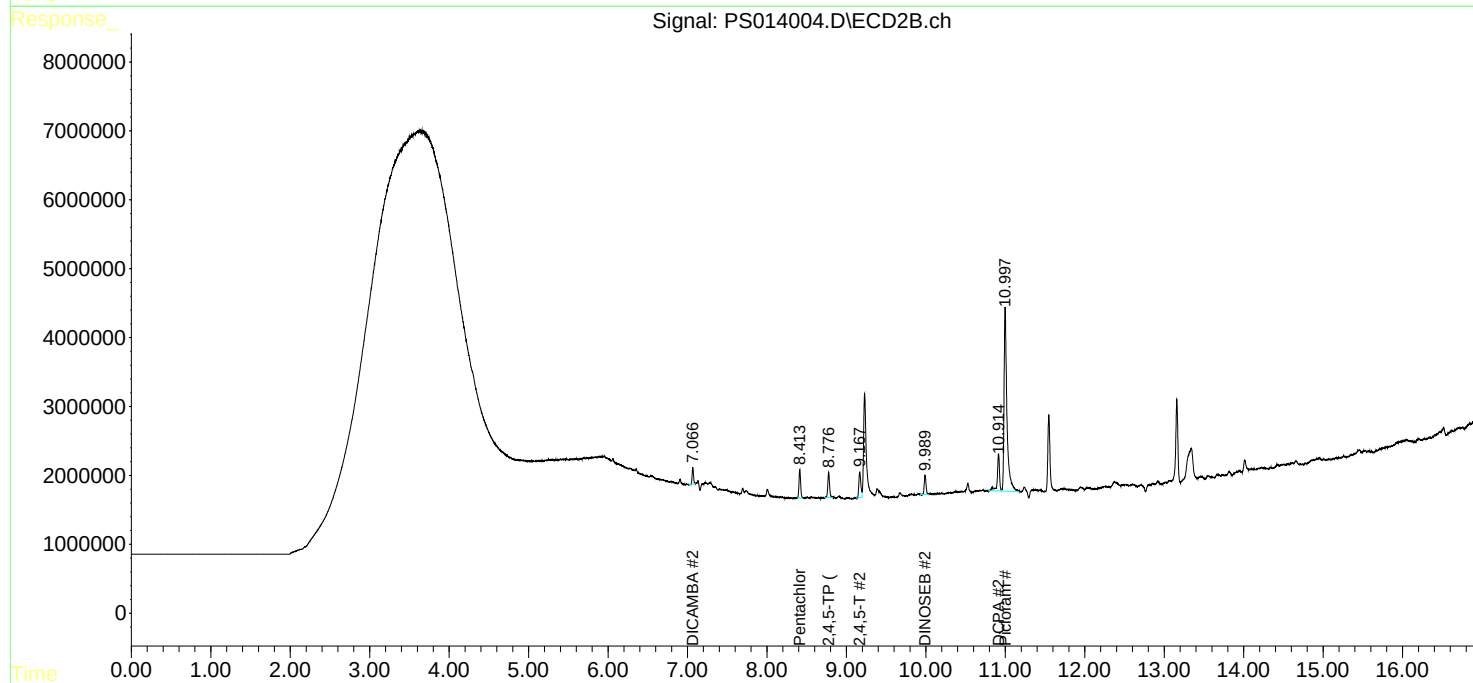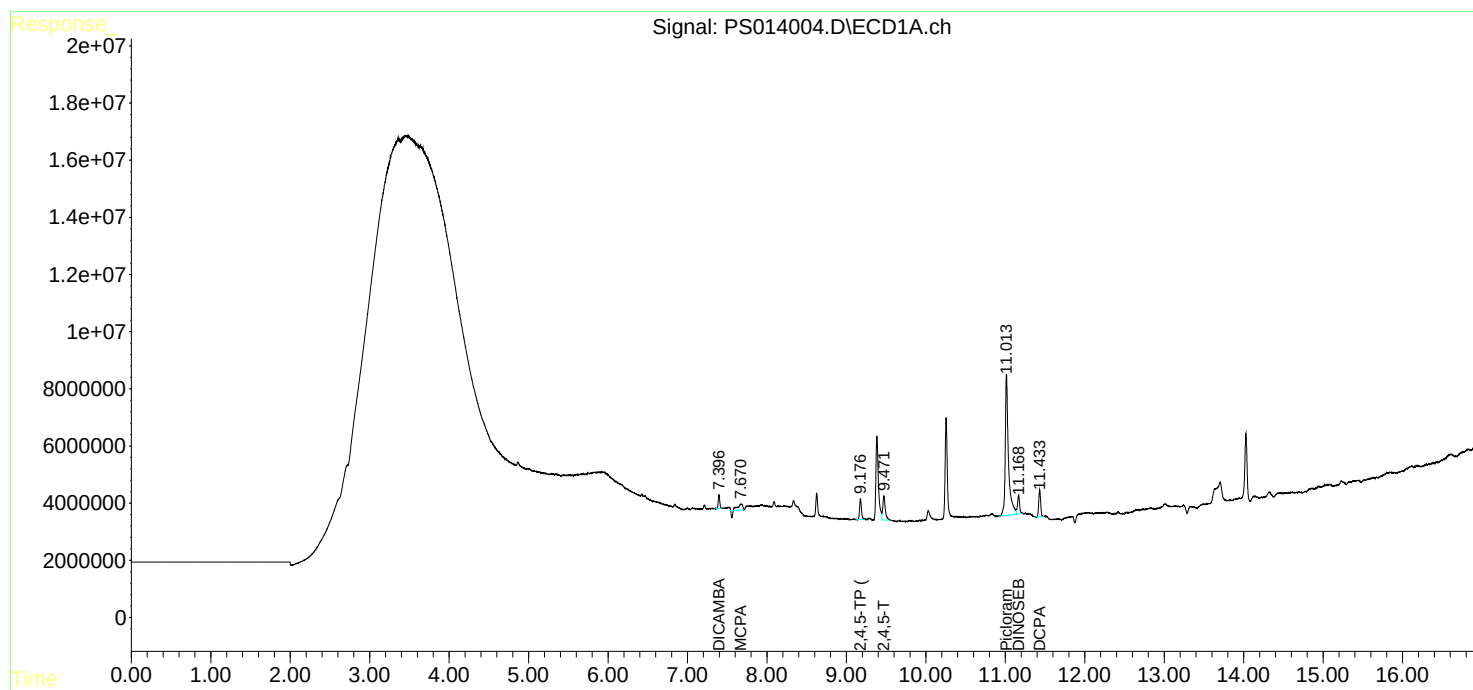


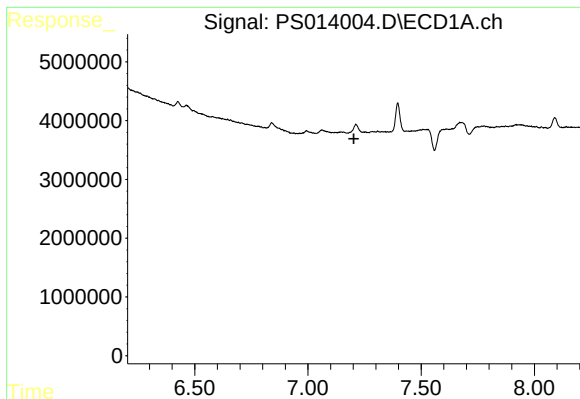

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

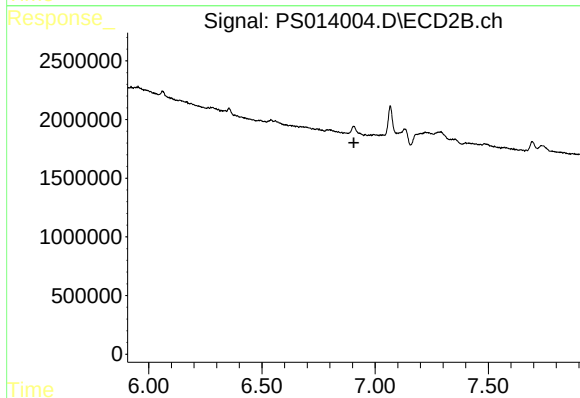


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.906 min
Response: 0
Conc: N.D.

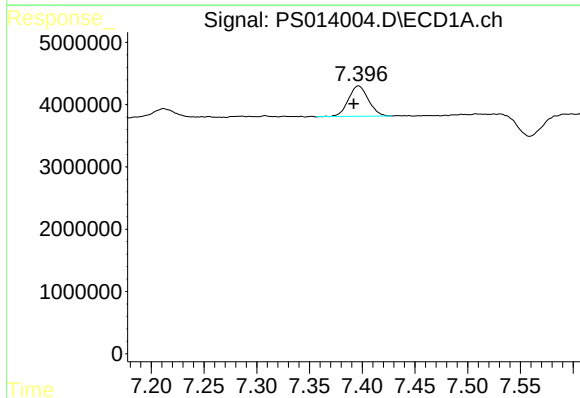


#5 DICAMBA

R.T.: 7.397 min
Delta R.T.: 0.005 min
Response: 6387290
Conc: 1.49 ng/ml

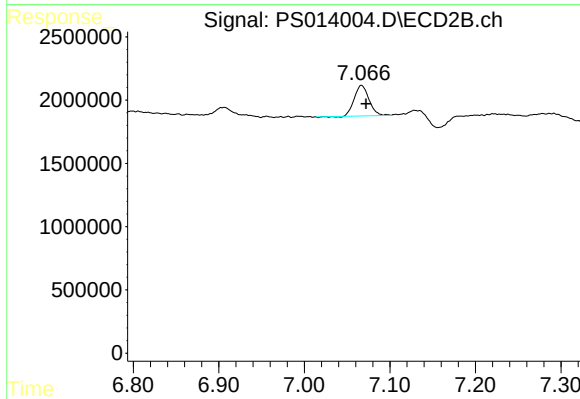

#5 DICAMBA


R.T.: 7.067 min
Delta R.T.: -0.005 min
Response: 2863263
Conc: 1.74 ng/ml

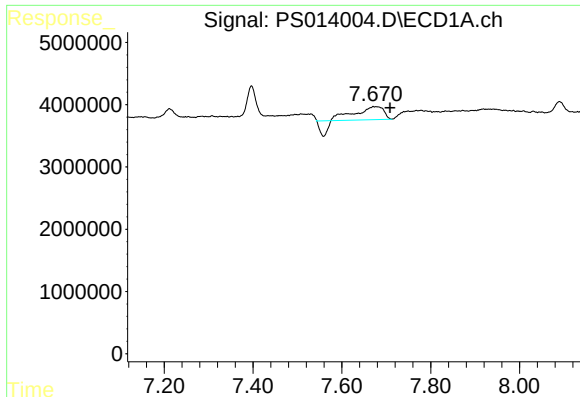

#7 MCPA


R.T.: 7.671 min
Delta R.T.: -0.038 min
Response: 7291307
Conc: 1.61 ug/ml

Instrument :
ECD_S
ClientSampleId :

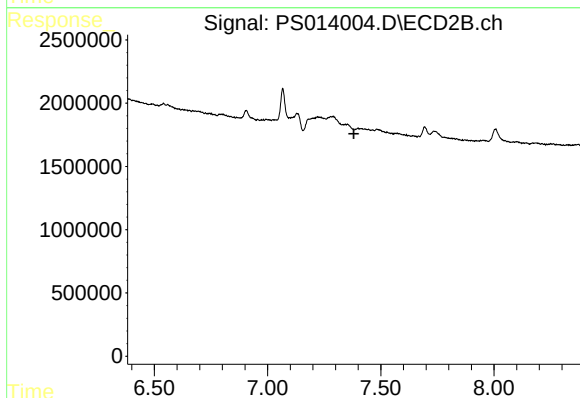


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.381 min
Response: 0
Conc: N.D.

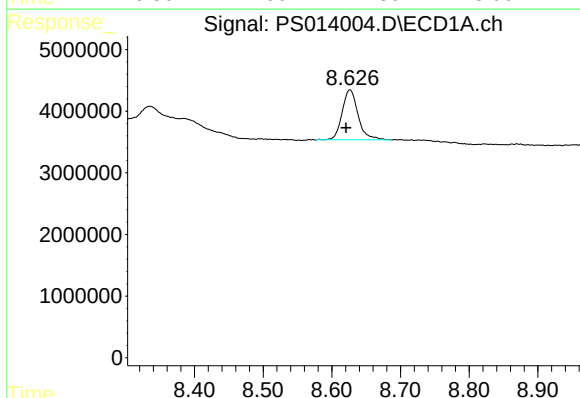


#10 Pentachlorophenol

R.T.: 8.626 min
Delta R.T.: 0.006 min
Response: 13023108
Conc: N.D.

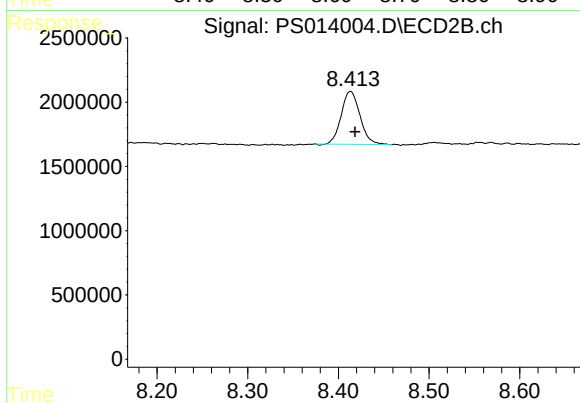

#10 Pentachlorophenol


R.T.: 8.413 min
Delta R.T.: -0.005 min
Response: 5921351
Conc: 1.06 ng/ml

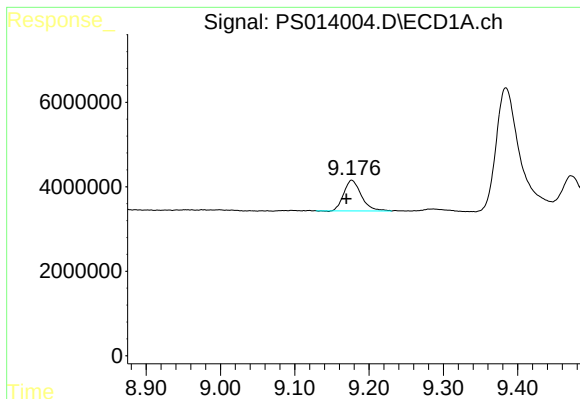

#11 2,4,5-TP (SILVEX)


R.T.: 9.177 min
Delta R.T.: 0.007 min
Response: 11880207
Conc: 1.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

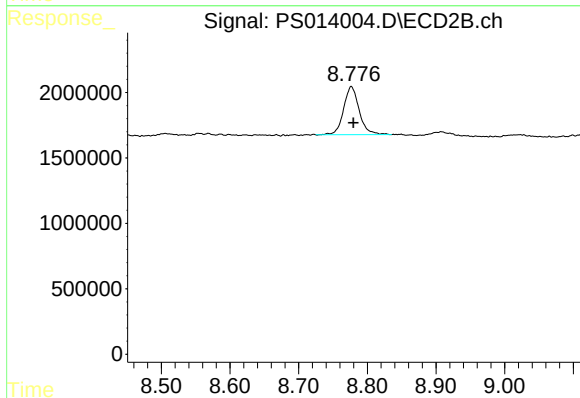


#11 2,4,5-TP (SILVEX)

R.T.: 8.777 min
Delta R.T.: -0.003 min
Response: 5778148
Conc: 2.52 ng/ml

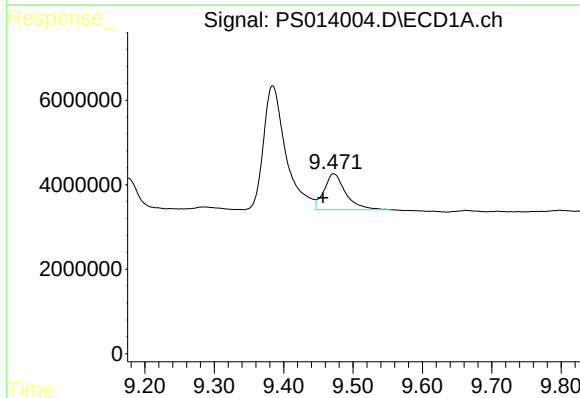


#12 2,4,5-T

R.T.: 9.472 min
Delta R.T.: 0.015 min
Response: 18395961
Conc: 2.86 ng/ml

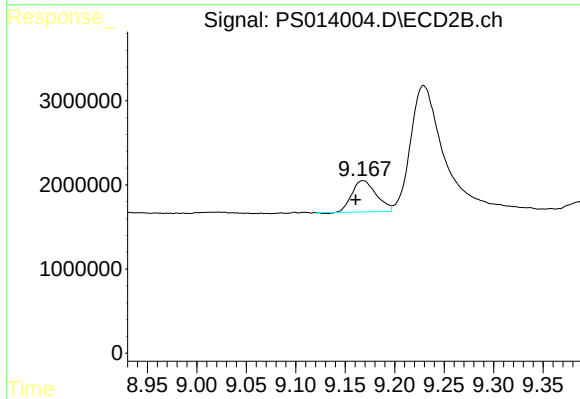

#12 2,4,5-T


R.T.: 9.168 min
Delta R.T.: 0.007 min
Response: 6404630
Conc: 2.88 ng/ml

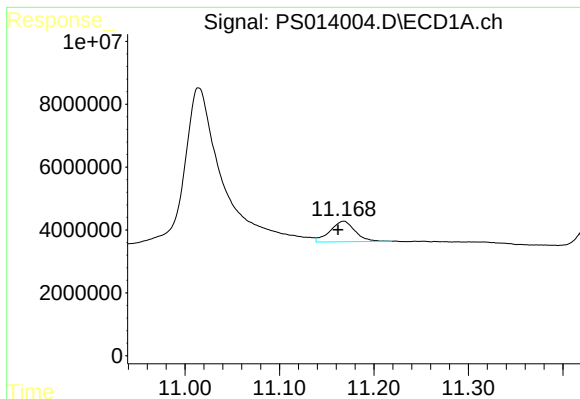

#14 DINOSEB


R.T.: 11.168 min
Delta R.T.: 0.006 min
Response: 12047524
Conc: 2.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

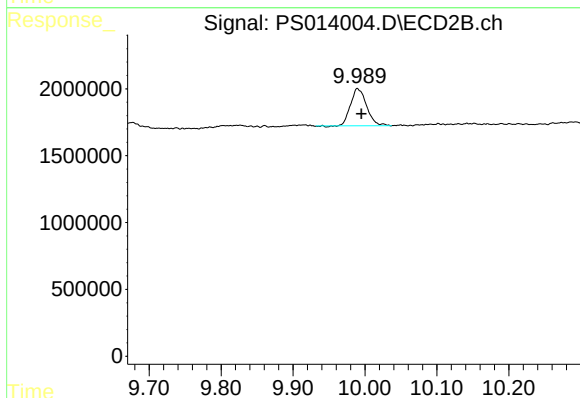


#14 DINOSEB

R.T.: 9.990 min
Delta R.T.: -0.004 min
Response: 4337196
Conc: 2.65 ng/ml

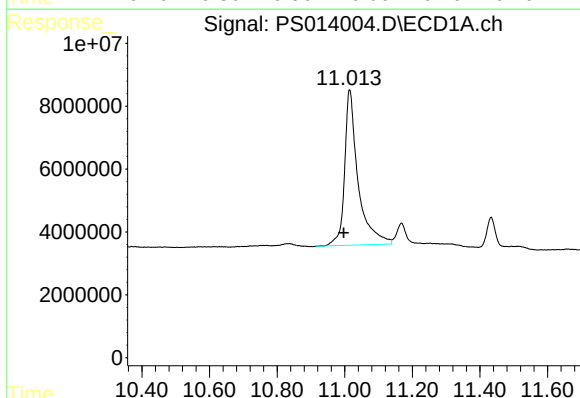


#15 Picloram

R.T.: 11.014 min
Delta R.T.: 0.018 min
Response: 136899146
Conc: 16.12 ng/ml

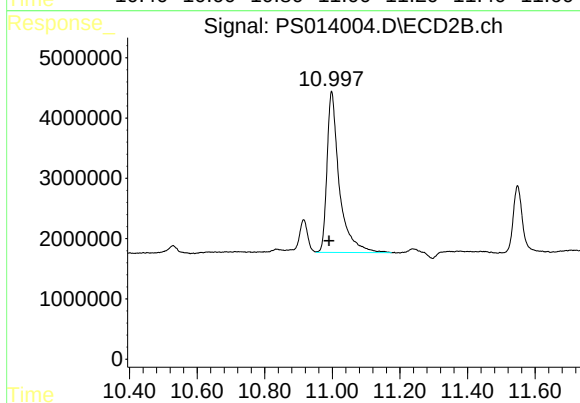

#15 Picloram


R.T.: 10.998 min
Delta R.T.: 0.008 min
Response: 67638751
Conc: 19.82 ng/ml

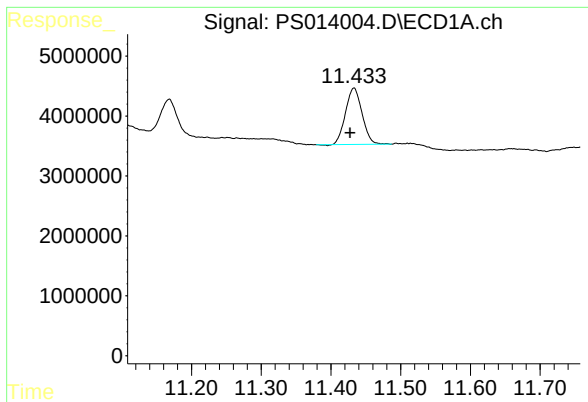

#16 DCPA

R.T.: 11.433 min
Delta R.T.: 0.006 min
Response: 15538860
Conc: 1.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

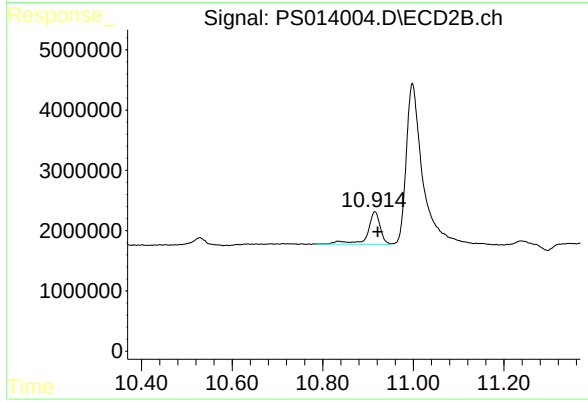

#16 DCPA

R.T.: 10.915 min
Delta R.T.: -0.006 min
Response: 10422566
Conc: 3.48 ng/ml