

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
 Data File : PS003149.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2019 13:09
 Operator : EI\SJ
 Sample : PB117060TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 00:45:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.295	10.795	206.1E6	202.9E6	542.898	474.529
Target Compounds							
1) T	Dalapon	0.000	2.297	0	56570504	N.D.	105.557 #
6) T	MCPD	11.972	0.000	19026080	0	15.880	N.D. #
7) T	MCPA	12.163	0.000	24382020	0	13.775	N.D. #
12) T	2,4,5-T	0.000	14.414	0	5189124	N.D.	2.712 #
15) T	Picloram	0.000	16.720	0	25992728	N.D.	8.646 #
16) T	DCPA	17.448	16.720	-6169526	25992728	N.D.	8.391



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
Data File : PS003149.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2019 13:09
Operator : EI\SJ
Sample : PB117060TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 00:45:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

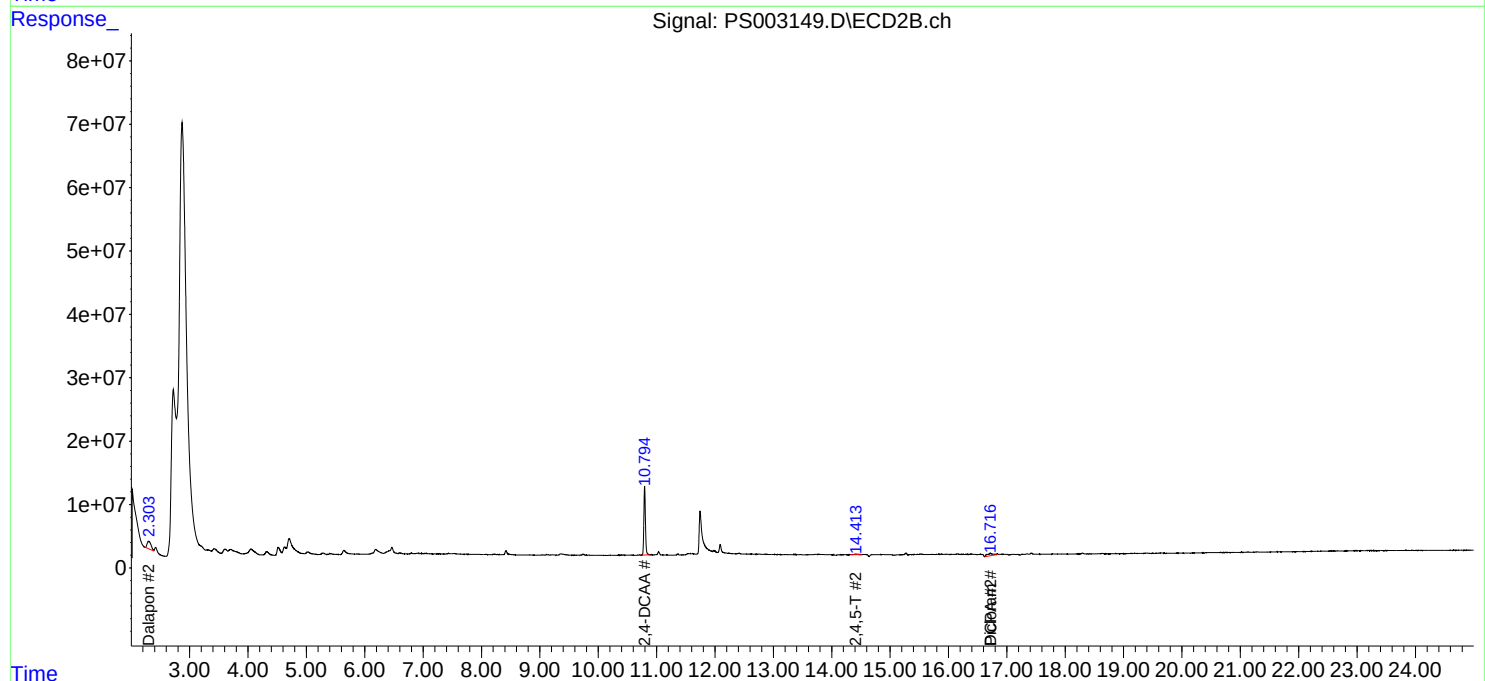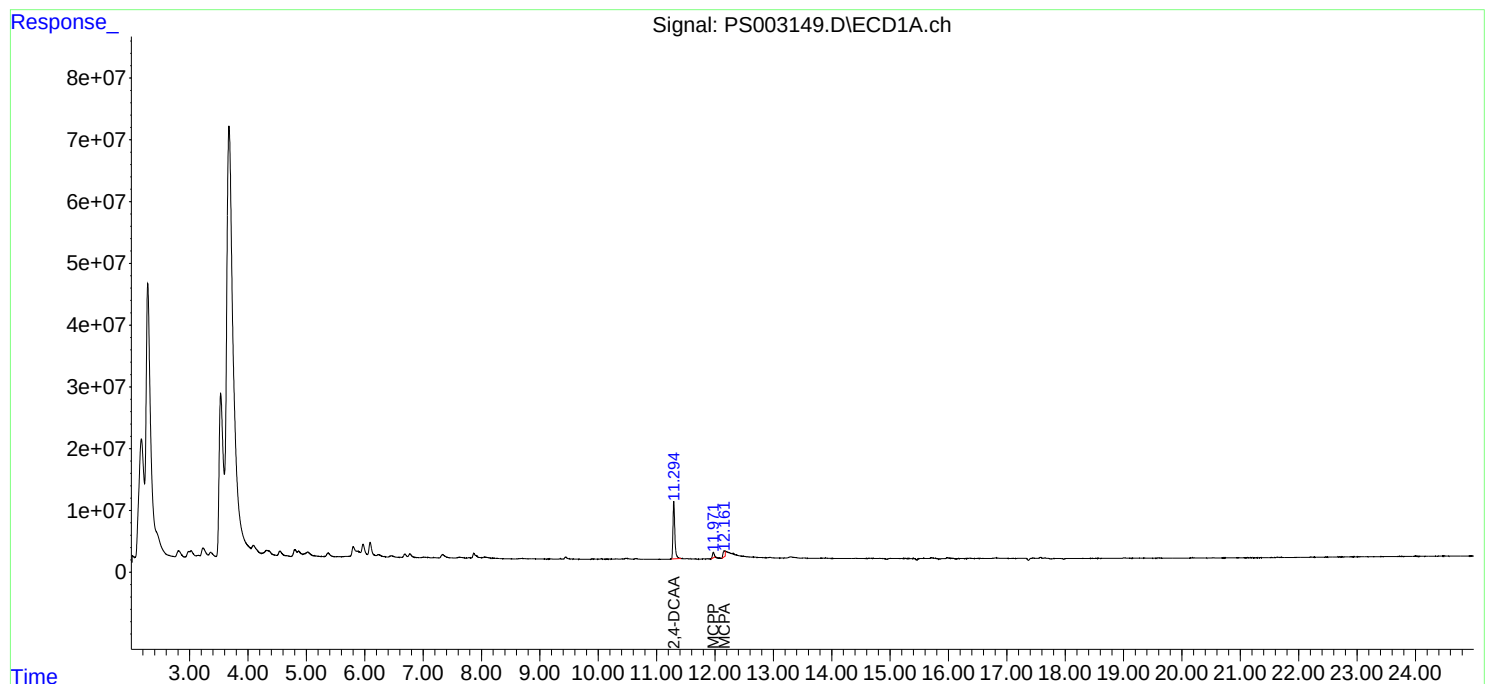


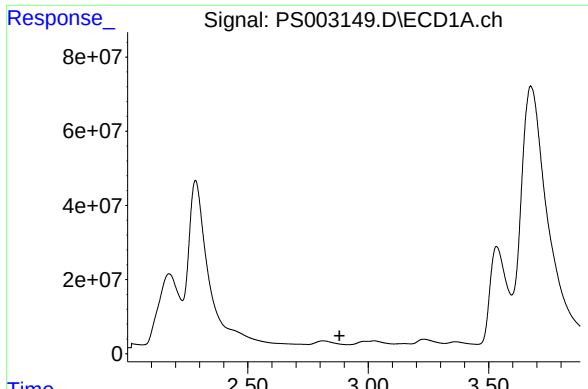

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

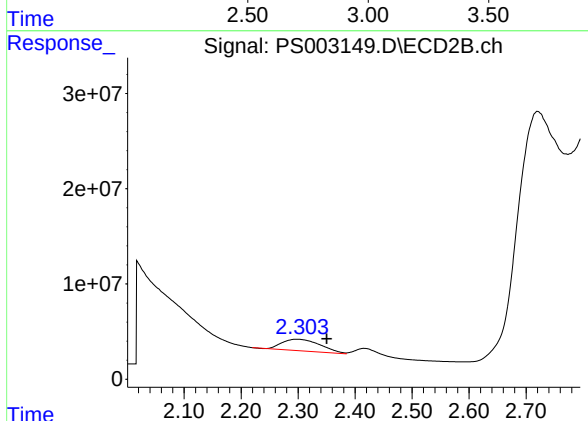


#1 Dalapon

R.T.: 2.297 min
Delta R.T.: -0.053 min
Response: 56570504
Conc: 105.56 ng/ml

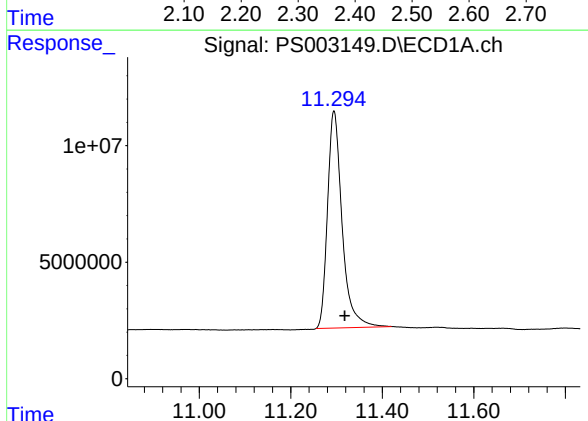


#4 2,4-DCAA

R.T.: 11.295 min
Delta R.T.: -0.023 min
Response: 206106220
Conc: 542.90 ng/ml

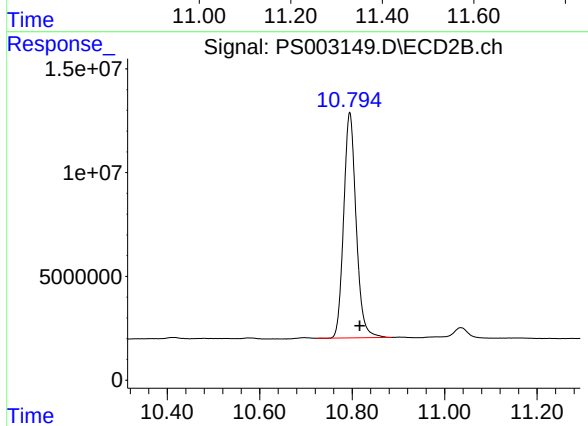

#4 2,4-DCAA


R.T.: 10.795 min
Delta R.T.: -0.022 min
Response: 202882857
Conc: 474.53 ng/ml

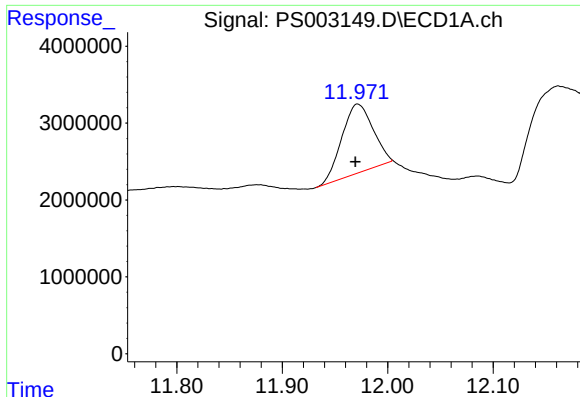

#6 MCPP


R.T.: 11.972 min
Delta R.T.: 0.002 min
Response: 19026080
Conc: 15.88 ug/ml

Instrument :
ECD_S
ClientSampleId :

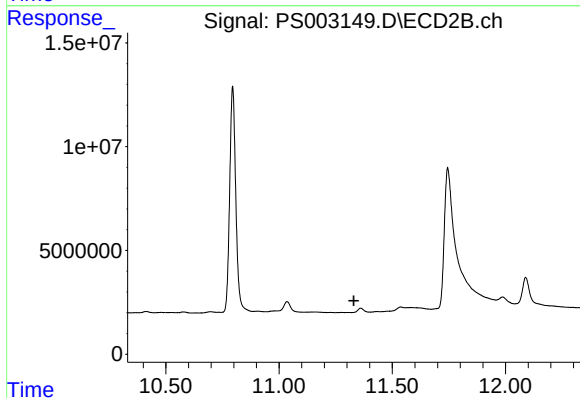


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

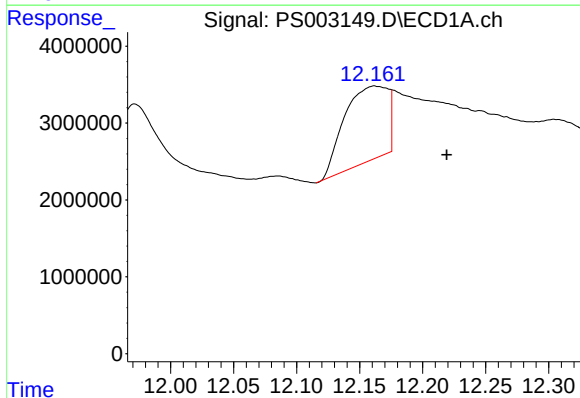


#7 MCPA

R.T.: 12.163 min
Delta R.T.: -0.057 min
Response: 24382020
Conc: 13.78 ug/ml

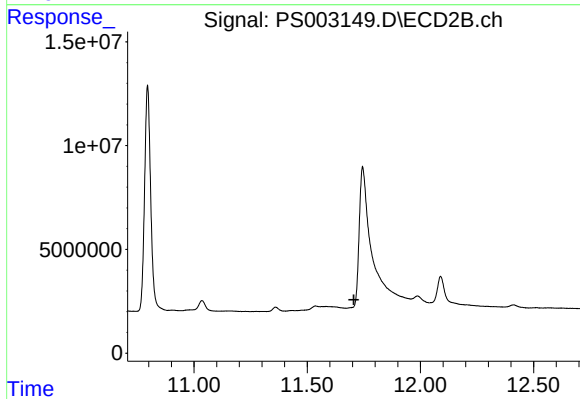

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 11.706 min
Response: 0
Conc: N.D.

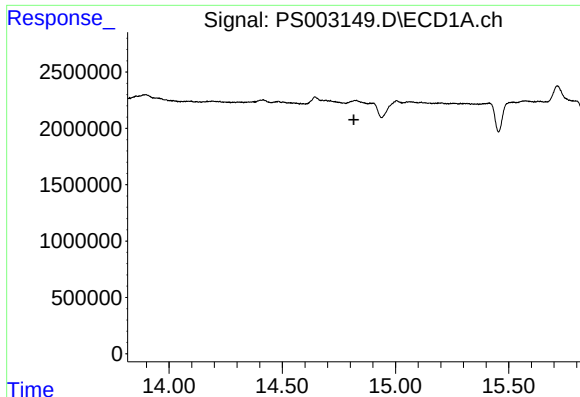

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

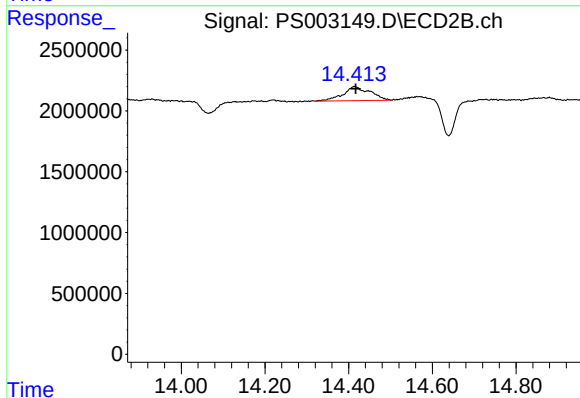


#12 2,4,5-T

R.T.: 14.414 min
Delta R.T.: -0.003 min
Response: 5189124
Conc: 2.71 ng/ml

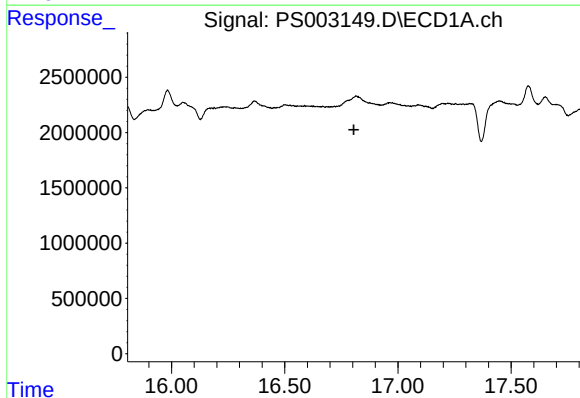


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

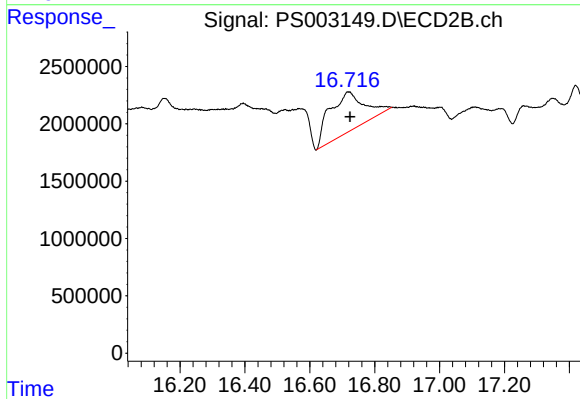

#15 Picloram


R.T.: 16.720 min
Delta R.T.: -0.005 min
Response: 25992728
Conc: 8.65 ng/ml

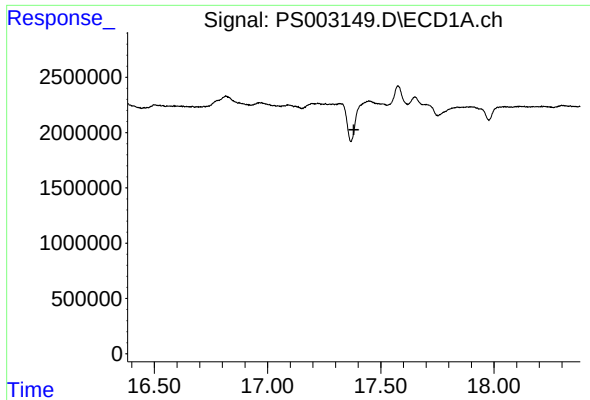

#16 DCPA

R.T.: 17.448 min
Delta R.T.: 0.067 min
Response: -6169526
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

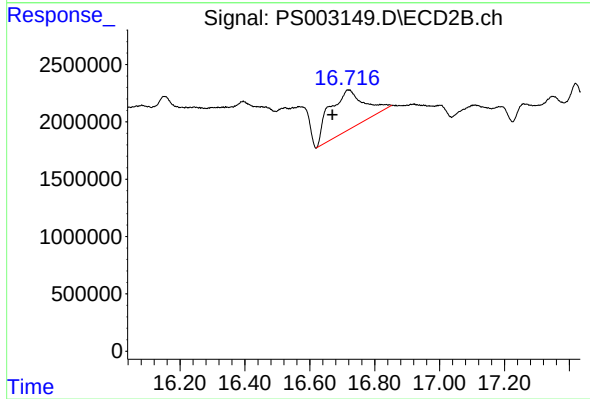

#16 DCPA

R.T.: 16.720 min
Delta R.T.: 0.050 min
Response: 25992728
Conc: 8.39 ng/ml