

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
 Data File : PS003151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2019 14:11
 Operator : EI\SJ
 Sample : K1442-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 00:46:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.281	10.782	213.9E6	269.0E6	563.421	629.101
Target Compounds							
1) T	Dalapon	0.000	2.283	0	28749682	N.D.	53.645 #
2) T	3,5-DICHL...	0.000	8.947	0	2440431	N.D.	4.330 #
3) T	4-Nitroph...	10.836	0.000	956373	0	4.941	N.D. #
7) T	MCPA	0.000	11.757	0	6413954	N.D.	4.077 #
10) T	Pentachlo...	13.510	13.282	3016179	2386016	0.470	0.386
14) T	DINOSEB	0.000	15.492	0	8711620	N.D.	4.970 #
15) T	Picloram	16.799	16.703	9775390	36040913	3.090	11.988 #
16) T	DCPA	17.421	16.703	-10368184	36040913	N.D.	11.635



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
Data File : PS003151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2019 14:11
Operator : EI\SJ
Sample : K1442-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 00:46:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

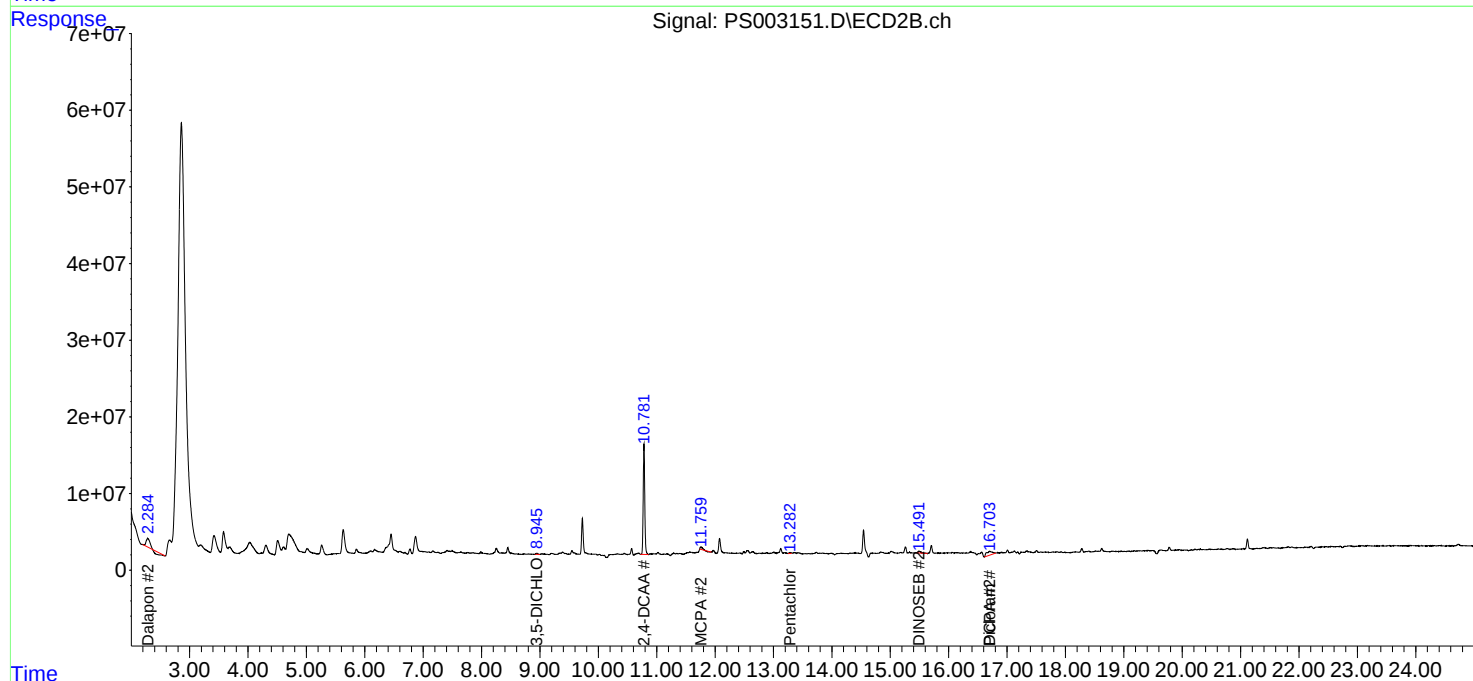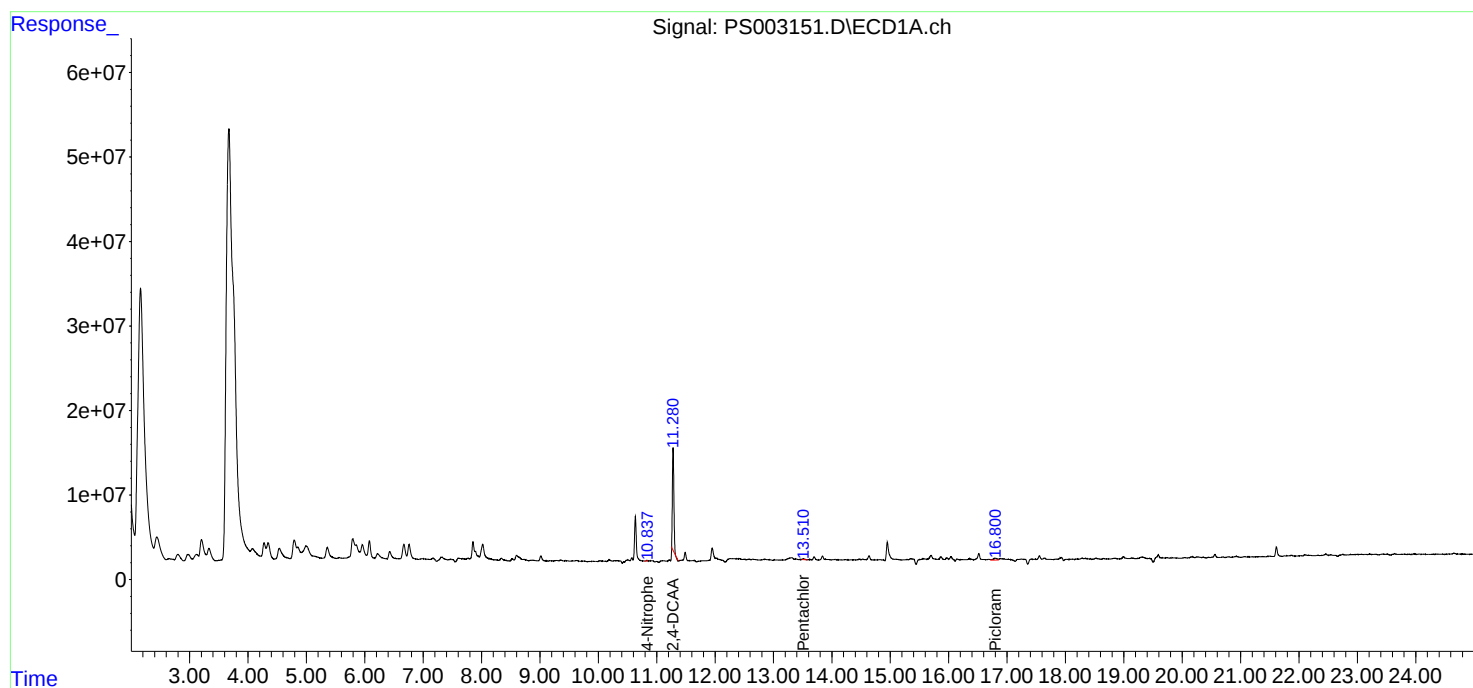


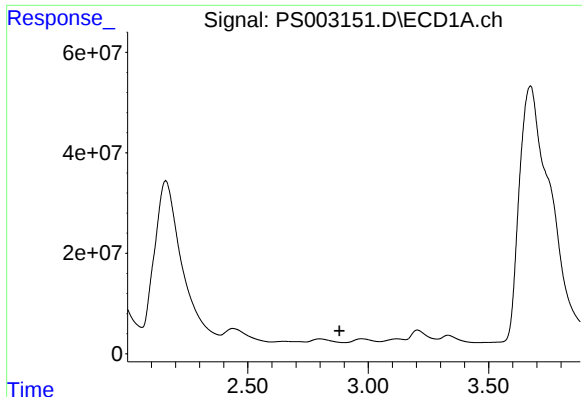

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

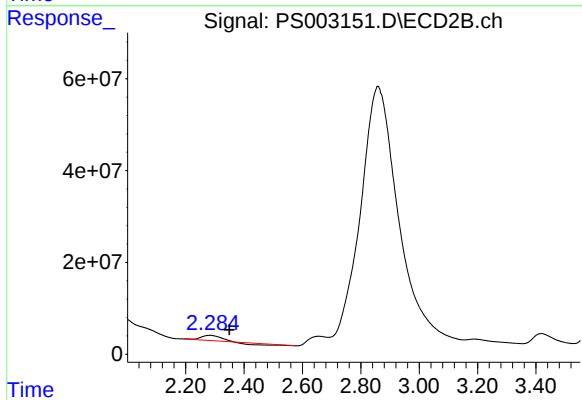


#1 Dalapon

R.T.: 2.283 min
Delta R.T.: -0.068 min
Response: 28749682
Conc: 53.65 ng/ml

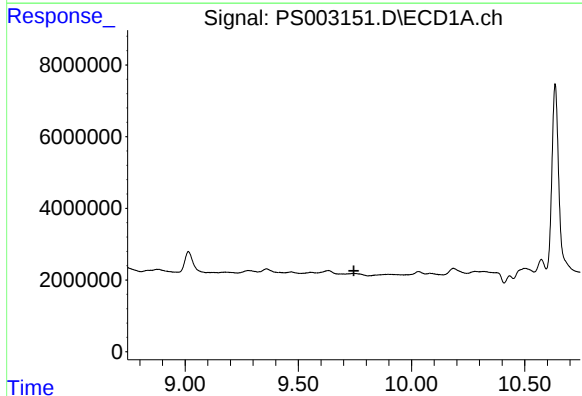


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

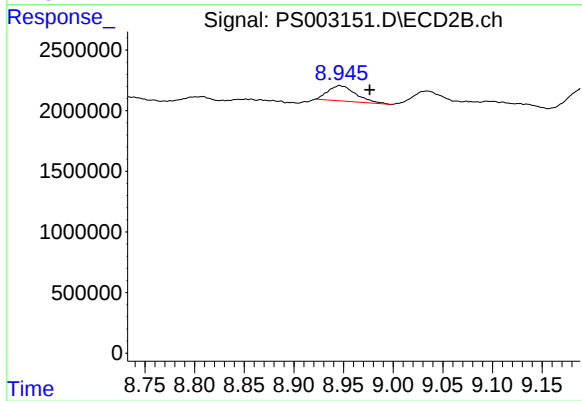

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.947 min
Delta R.T.: -0.030 min
Response: 2440431
Conc: 4.33 ng/ml

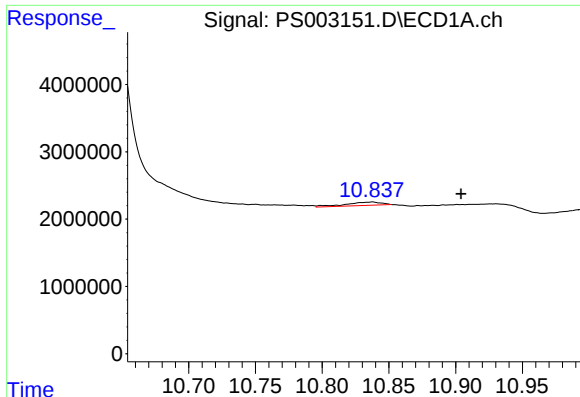

#3 4-Nitrophenol


R.T.: 10.836 min
Delta R.T.: -0.068 min
Response: 956373
Conc: 4.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

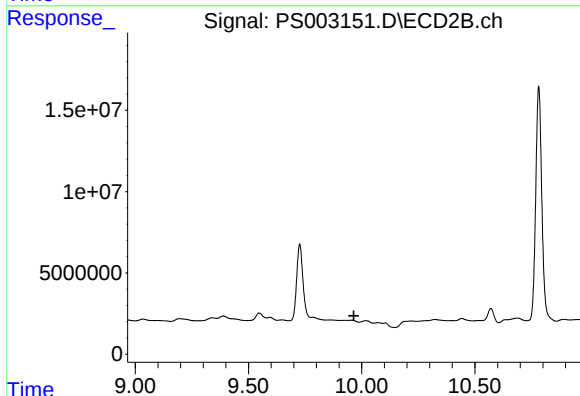


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 9.965 min
Response: 0
Conc: N.D.

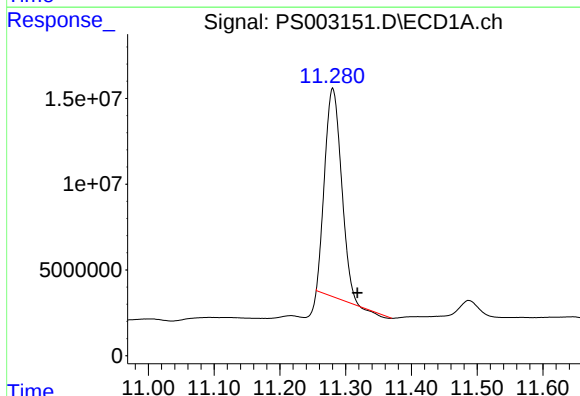


#4 2,4-DCAA

R.T.: 11.281 min
Delta R.T.: -0.037 min
Response: 213897614
Conc: 563.42 ng/ml

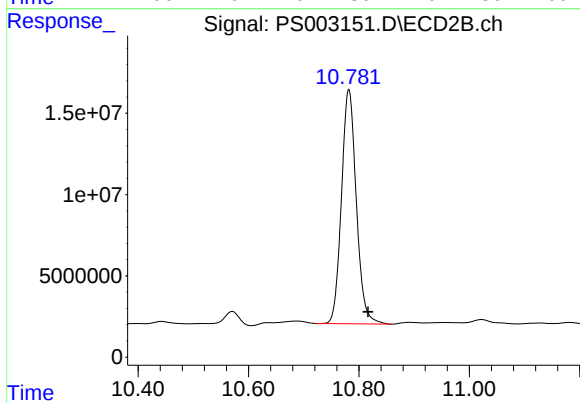

#4 2,4-DCAA


R.T.: 10.782 min
Delta R.T.: -0.035 min
Response: 268969378
Conc: 629.10 ng/ml

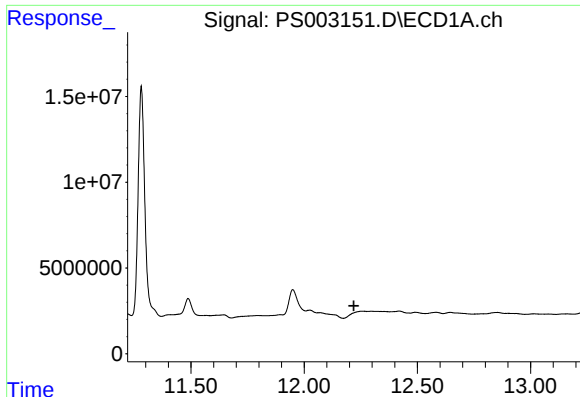

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

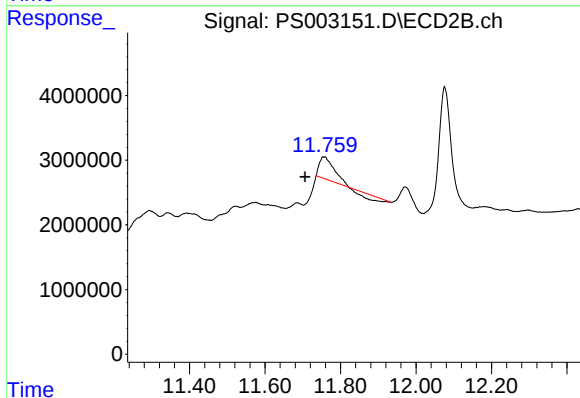


#7 MCPA

R.T.: 11.757 min
Delta R.T.: 0.051 min
Response: 6413954
Conc: 4.08 ug/ml

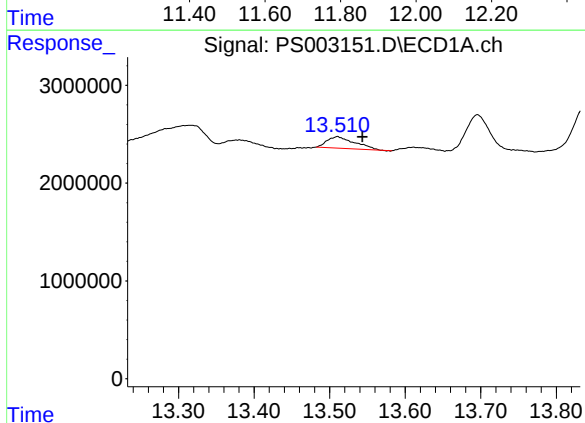


#10 Pentachlorophenol

R.T.: 13.510 min
Delta R.T.: -0.033 min
Response: 3016179
Conc: 0.47 ng/ml

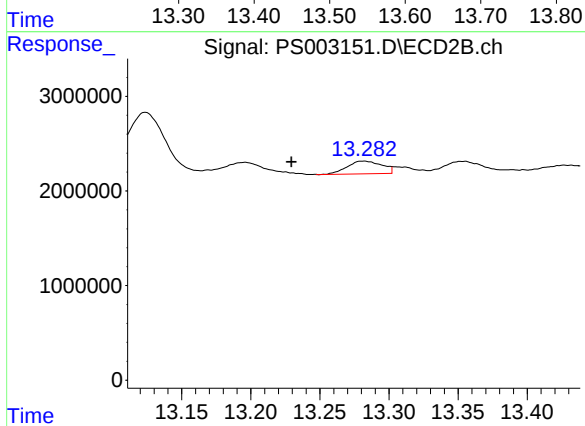

#10 Pentachlorophenol


R.T.: 13.282 min
Delta R.T.: 0.052 min
Response: 2386016
Conc: 0.39 ng/ml

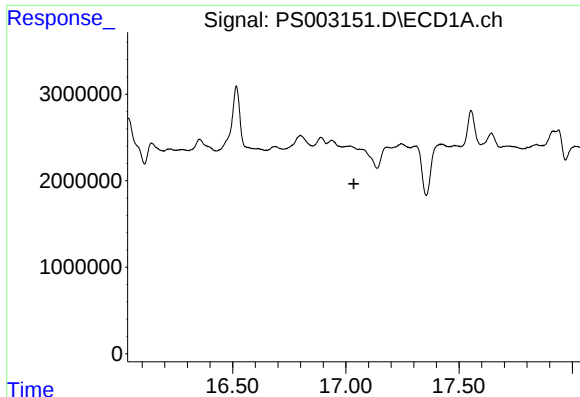

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

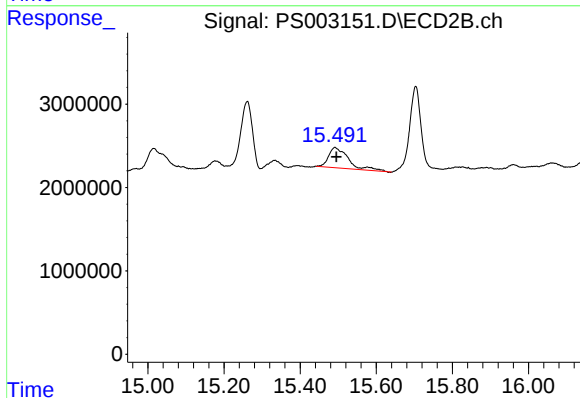


#14 DINOSEB

R.T.: 15.492 min
Delta R.T.: -0.003 min
Response: 8711620
Conc: 4.97 ng/ml

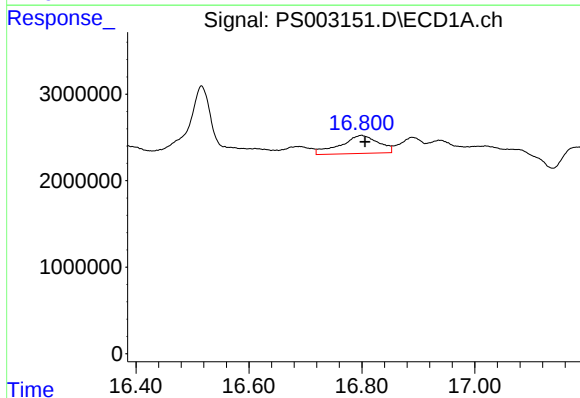


#15 Picloram

R.T.: 16.799 min
Delta R.T.: -0.006 min
Response: 9775390
Conc: 3.09 ng/ml

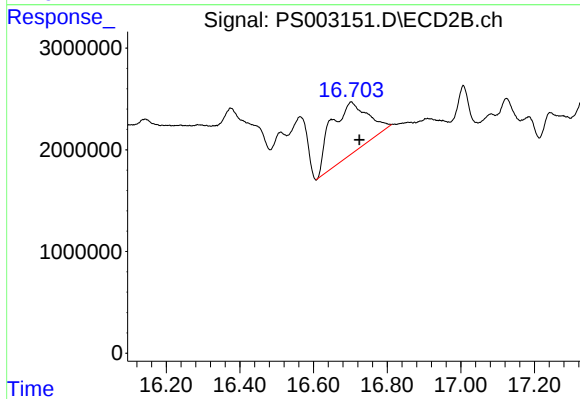

#15 Picloram


R.T.: 16.703 min
Delta R.T.: -0.022 min
Response: 36040913
Conc: 11.99 ng/ml

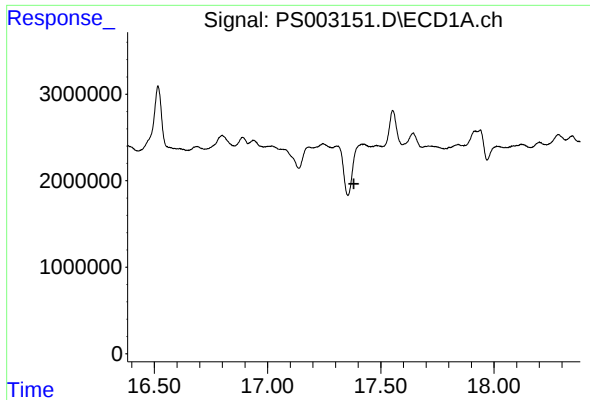

#16 DCPA

R.T.: 17.421 min
Delta R.T.: 0.040 min
Response: -10368184
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

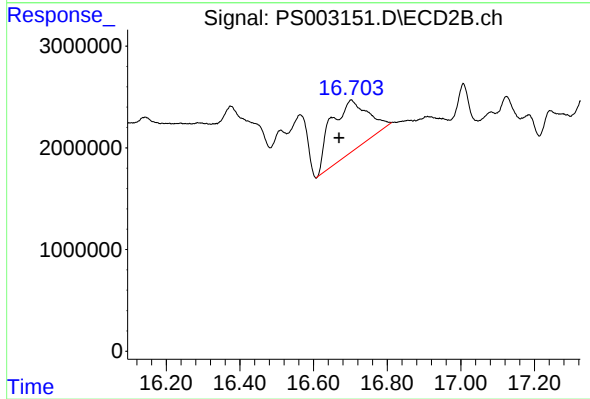

#16 DCPA

R.T.: 16.703 min
Delta R.T.: 0.033 min
Response: 36040913
Conc: 11.64 ng/ml