

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
 Data File : PS003152.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2019 14:42
 Operator : EI\SJ
 Sample : K1345-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 00:46:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.297	10.798	175.4E6	172.6E6	461.898	403.771
Target Compounds							
1) T	Dalapon	2.817	2.302	4397183	38429933	7.971	71.708 #
6) T	MCP	11.970	0.000	23715020	0	19.793	N.D. #
15) T	Picloram	0.000	16.723	0	13851476	N.D.	4.607 #
16) T	DCPA	0.000	16.723	0	13851476	N.D.	4.472 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
Data File : PS003152.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2019 14:42
Operator : EI\SJ
Sample : K1345-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 00:46:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

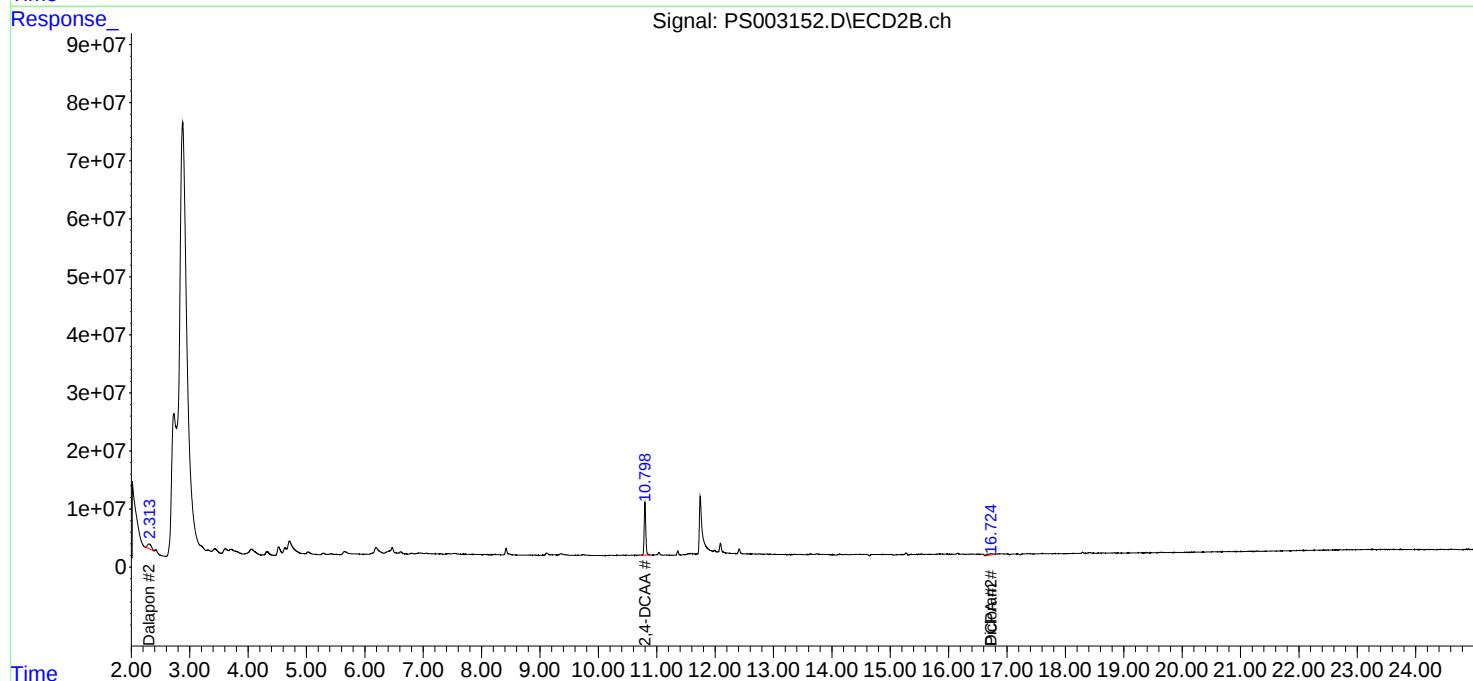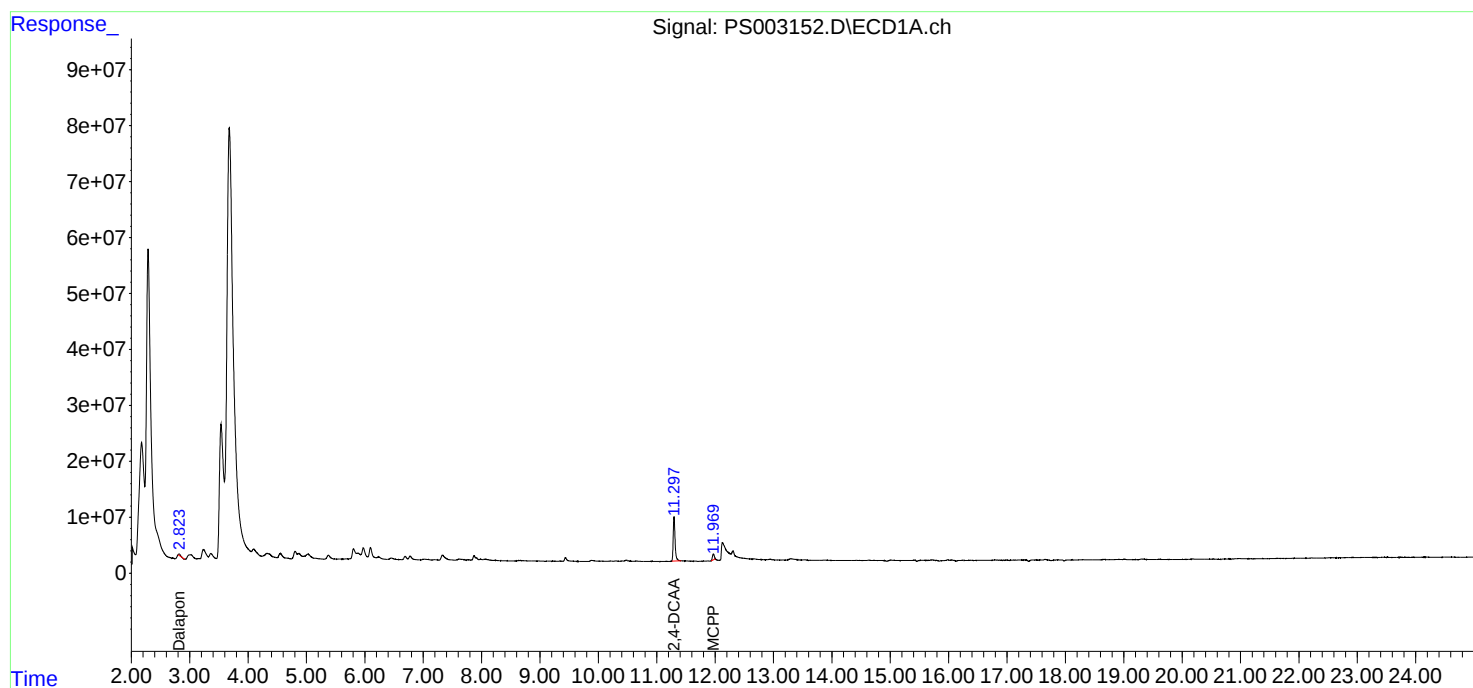


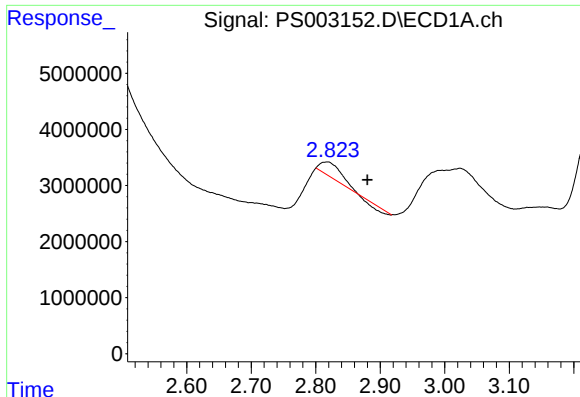

#1 Dalapon


R.T.: 2.817 min
Delta R.T.: -0.063 min
Response: 4397183
Conc: 7.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

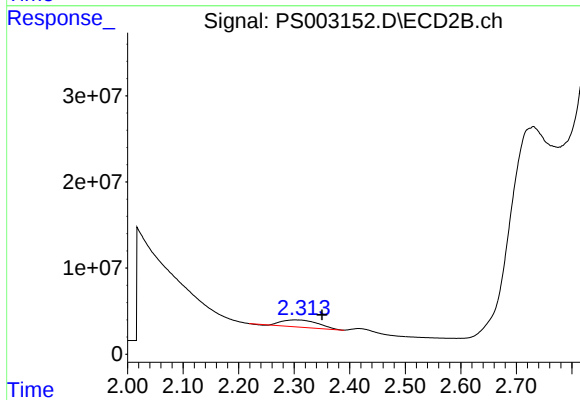


#1 Dalapon

R.T.: 2.302 min
Delta R.T.: -0.048 min
Response: 38429933
Conc: 71.71 ng/ml

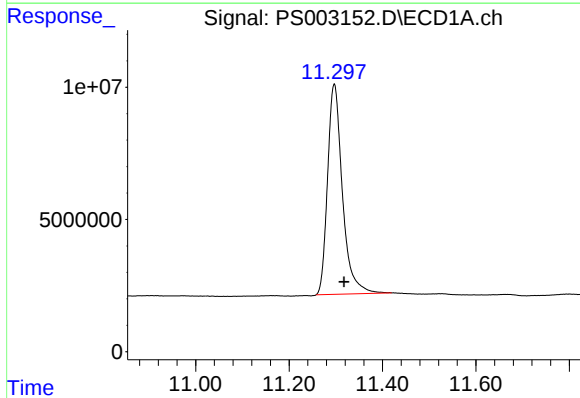


#4 2,4-DCAA

R.T.: 11.297 min
Delta R.T.: -0.021 min
Response: 175355376
Conc: 461.90 ng/ml

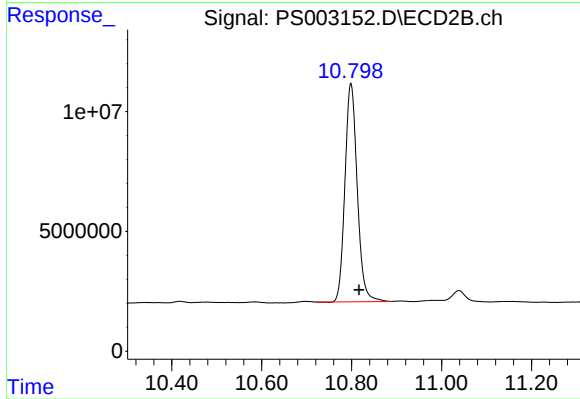

#4 2,4-DCAA


R.T.: 10.798 min
Delta R.T.: -0.018 min
Response: 172630442
Conc: 403.77 ng/ml

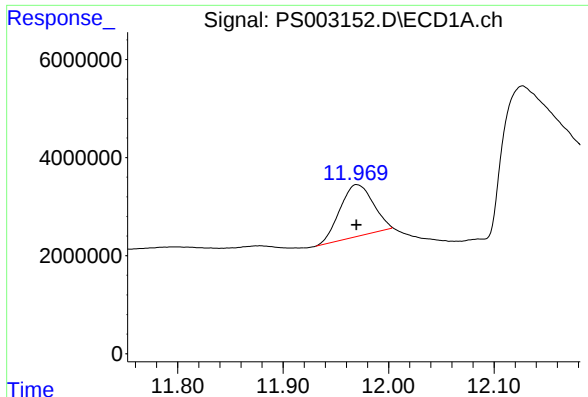

#6 MCP


R.T.: 11.970 min
Delta R.T.: 0.000 min
Response: 23715020
Conc: 19.79 ug/ml

Instrument :
ECD_S
ClientSampleId :

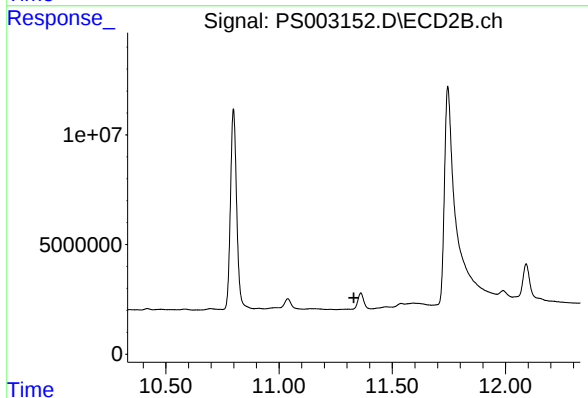


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

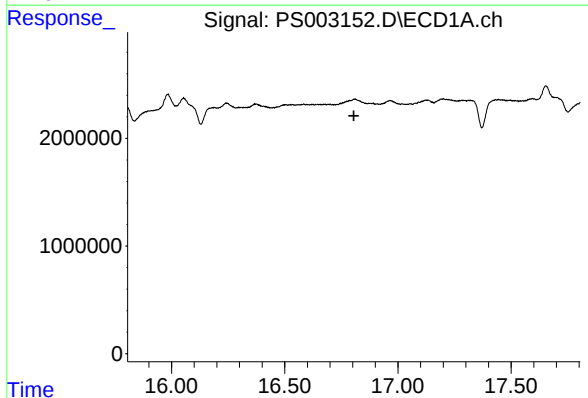


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

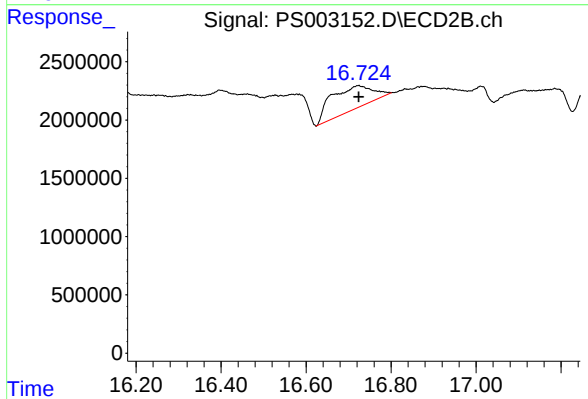

#15 Picloram


R.T.: 16.723 min
Delta R.T.: -0.002 min
Response: 13851476
Conc: 4.61 ng/ml

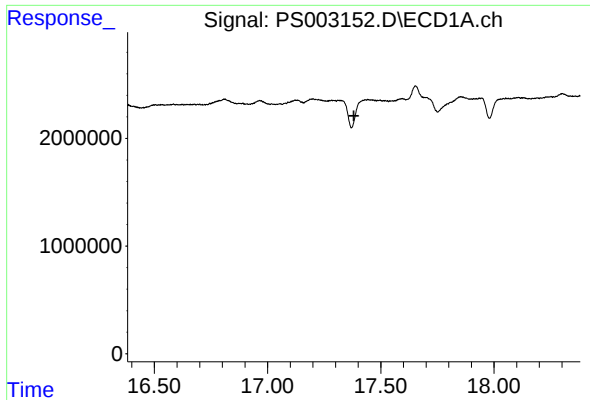

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

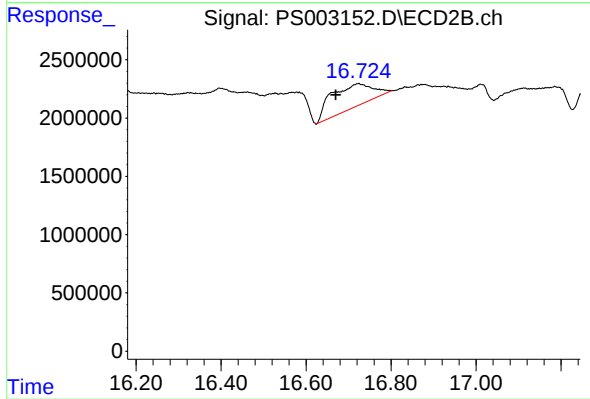

#16 DCPA

R.T.: 16.723 min
Delta R.T.: 0.053 min
Response: 13851476
Conc: 4.47 ng/ml