

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
 Data File : PS003154.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2019 15:44
 Operator : EI\SJ
 Sample : K1458-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 00:47:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.282	10.783	137.8E6	180.1E6	362.895	421.294
Target Compounds							
1) T	Dalapon	0.000	2.299	0	36946544	N.D.	68.940 #
2) T	3,5-DICHL...	0.000	9.032	0	610858	N.D.	1.084 #
6) T	MCP	11.952	11.345	18892834	5603094	15.769	5.080 #
14) T	DINOSEB	17.089	0.000	2413509	0	1.283	N.D. #
15) T	Picloram	16.791	0.000	3831500	0	1.211	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
Data File : PS003154.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2019 15:44
Operator : EI\SJ
Sample : K1458-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 00:47:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

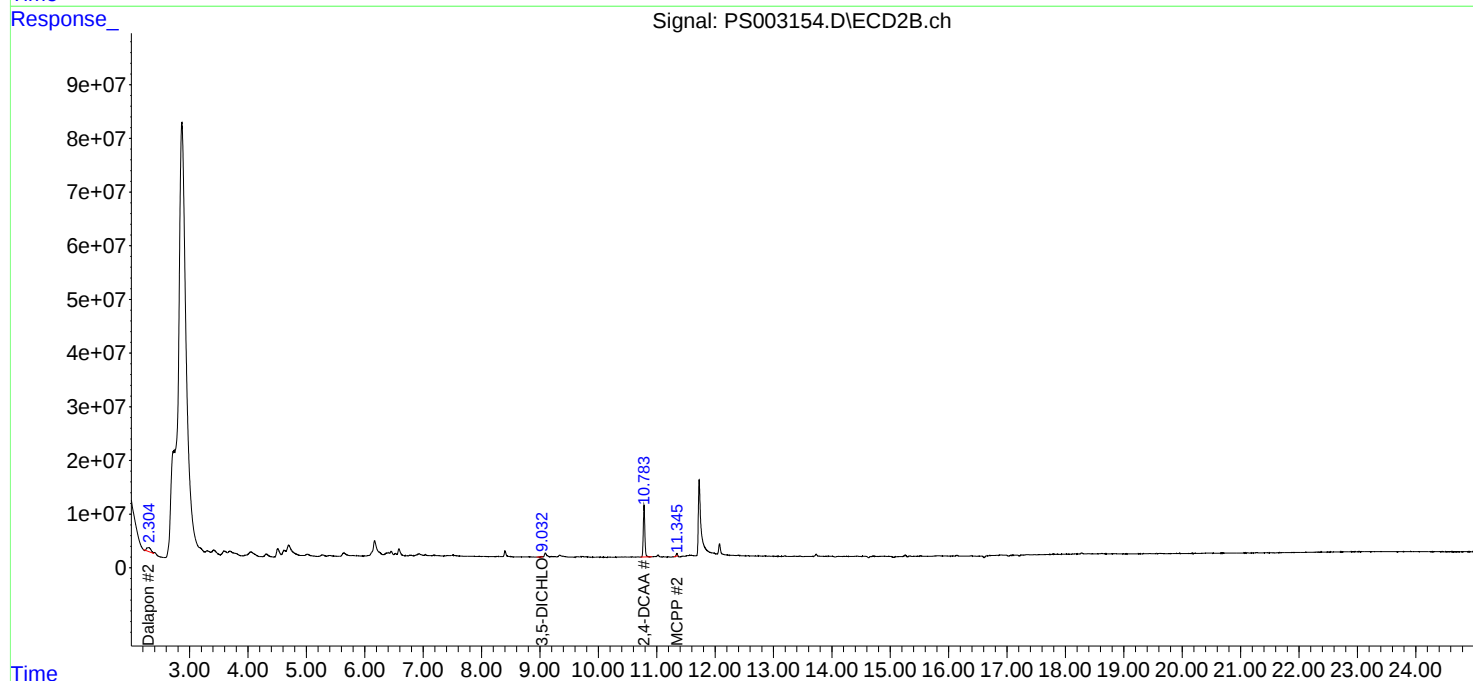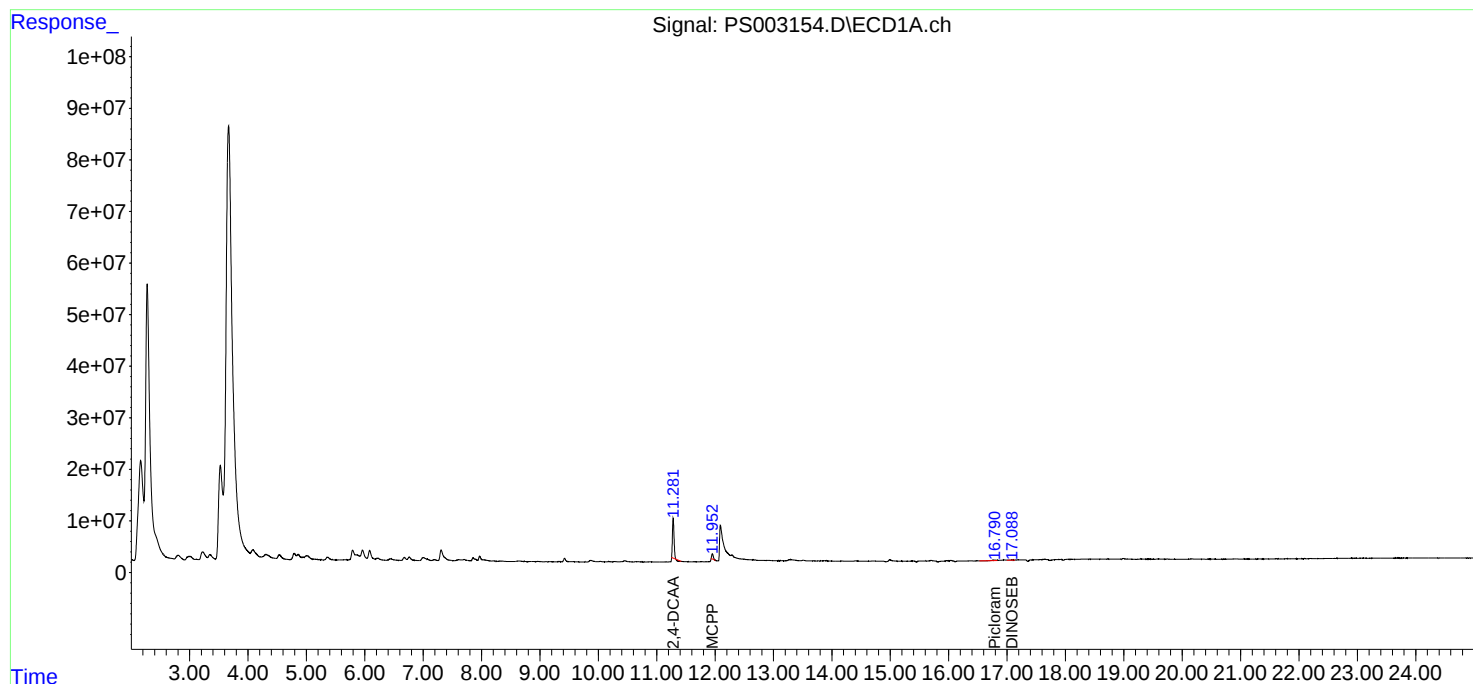


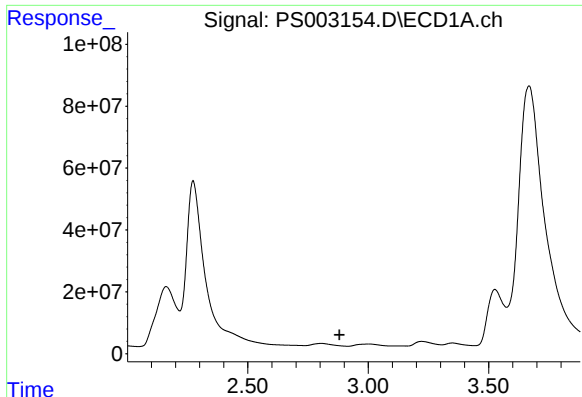

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

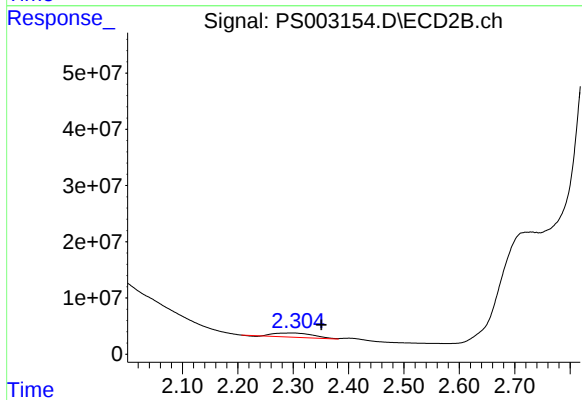


#1 Dalapon

R.T.: 2.299 min
Delta R.T.: -0.052 min
Response: 36946544
Conc: 68.94 ng/ml

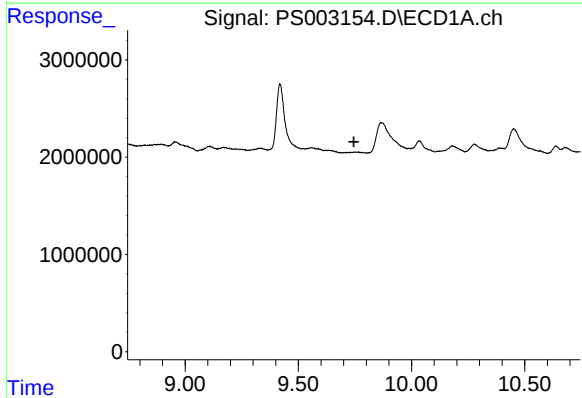


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

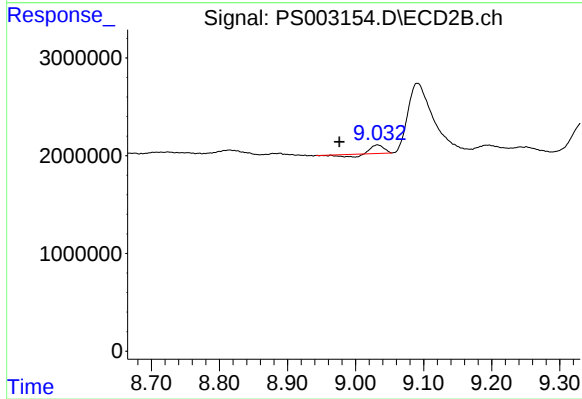

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.032 min
Delta R.T.: 0.056 min
Response: 610858
Conc: 1.08 ng/ml

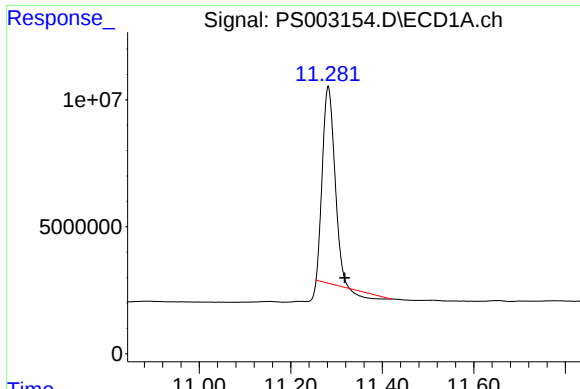

#4 2,4-DCAA


R.T.: 11.282 min
Delta R.T.: -0.036 min
Response: 137769697
Conc: 362.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

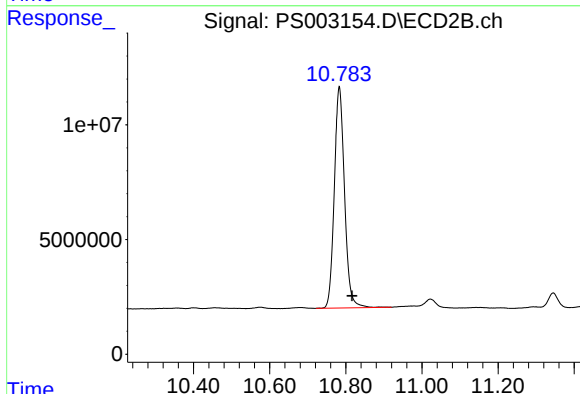


#4 2,4-DCAA

R.T.: 10.783 min
Delta R.T.: -0.034 min
Response: 180122641
Conc: 421.29 ng/ml

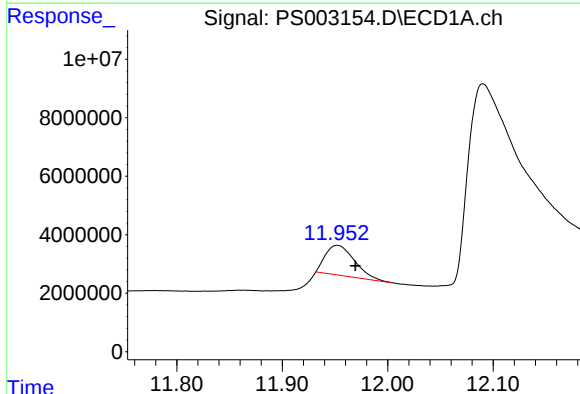


#6 MCP

R.T.: 11.952 min
Delta R.T.: -0.017 min
Response: 18892834
Conc: 15.77 ug/ml

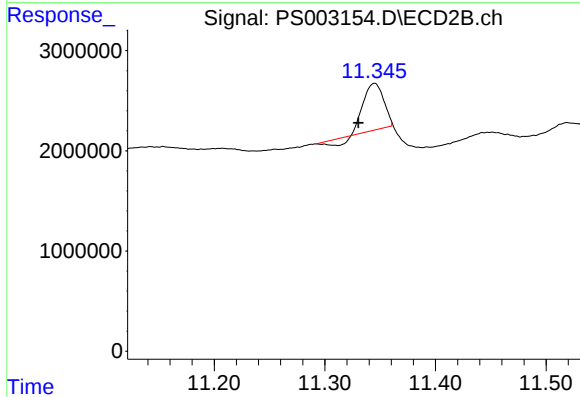

#6 MCP


R.T.: 11.345 min
Delta R.T.: 0.014 min
Response: 5603094
Conc: 5.08 ug/ml

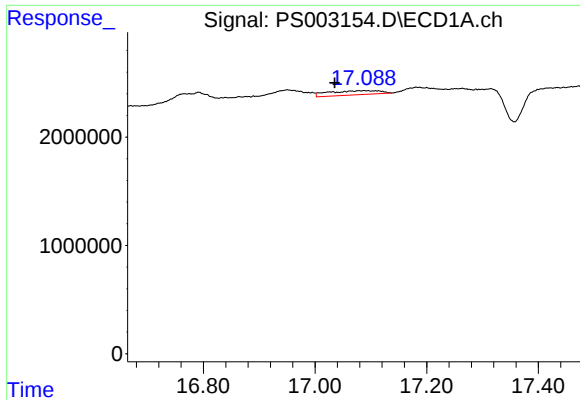

#14 DINOSEB


R.T.: 17.089 min
Delta R.T.: 0.053 min
Response: 2413509
Conc: 1.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

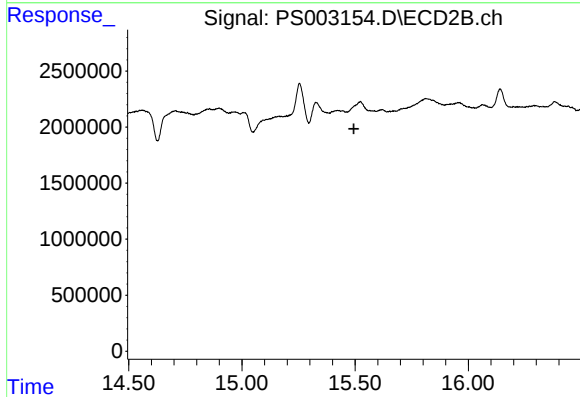


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 15.495 min
Response: 0
Conc: N.D.

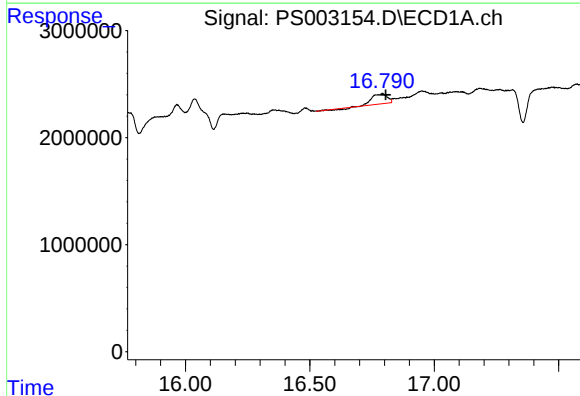

#15 Picloram

R.T.: 16.791 min
Delta R.T.: -0.014 min
Response: 3831500
Conc: 1.21 ng/ml

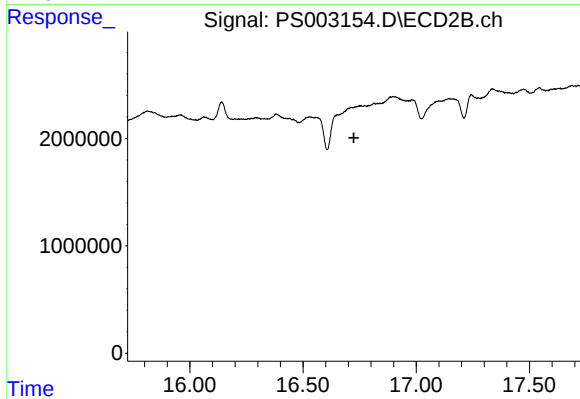

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.724 min
Response: 0
Conc: N.D.