

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
 Data File : PS003157.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2019 17:18
 Operator : EI\SJ
 Sample : K1459-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 00:47:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.280	10.782	160.7E6	240.1E6	423.276	561.560 #
Target Compounds							
6) T	MCP	11.956	11.344	16265737	8137018	13.576	7.378 #
15) T	Picloram	0.000	16.718	0	14567641	N.D.	4.846 #
16) T	DCPA	17.420	16.718	-3361797	14567641	N.D.	4.703



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
Data File : PS003157.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2019 17:18
Operator : EI\SJ
Sample : K1459-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 00:47:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

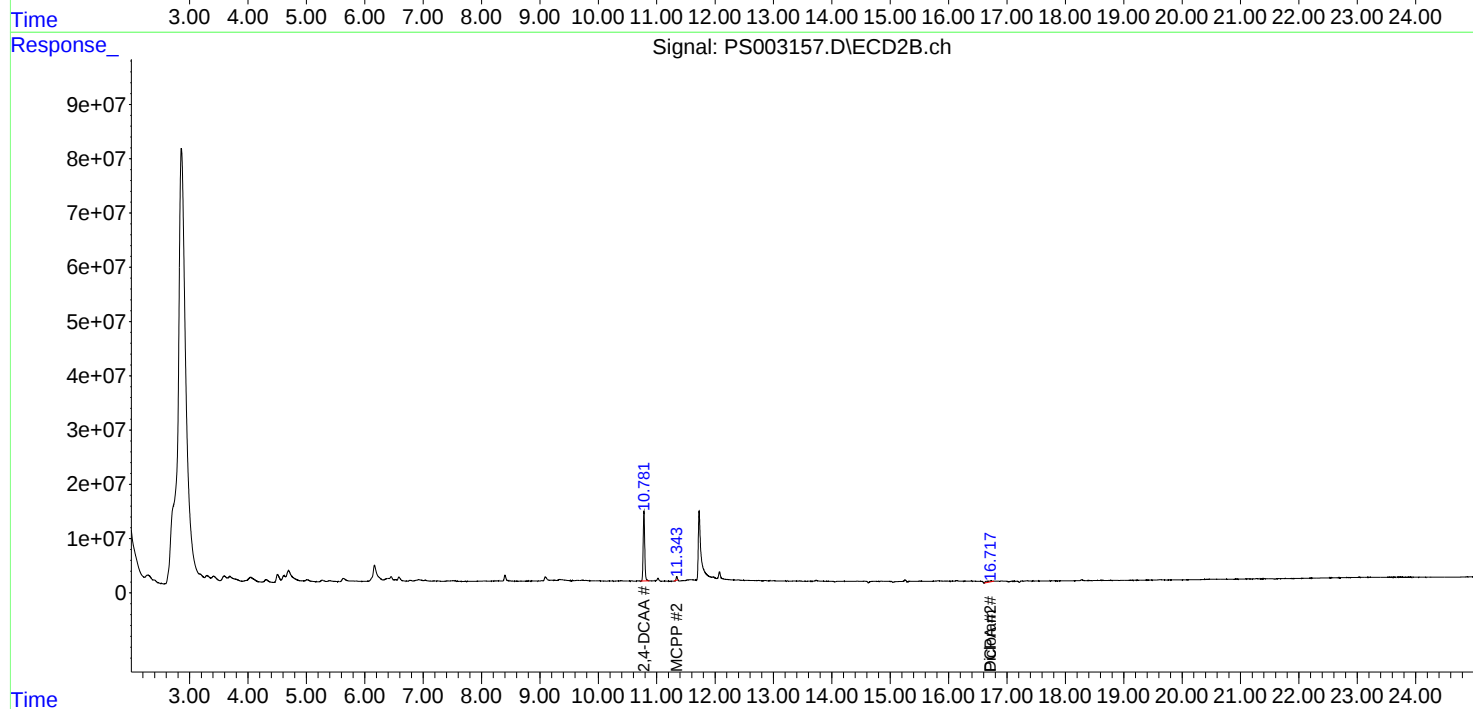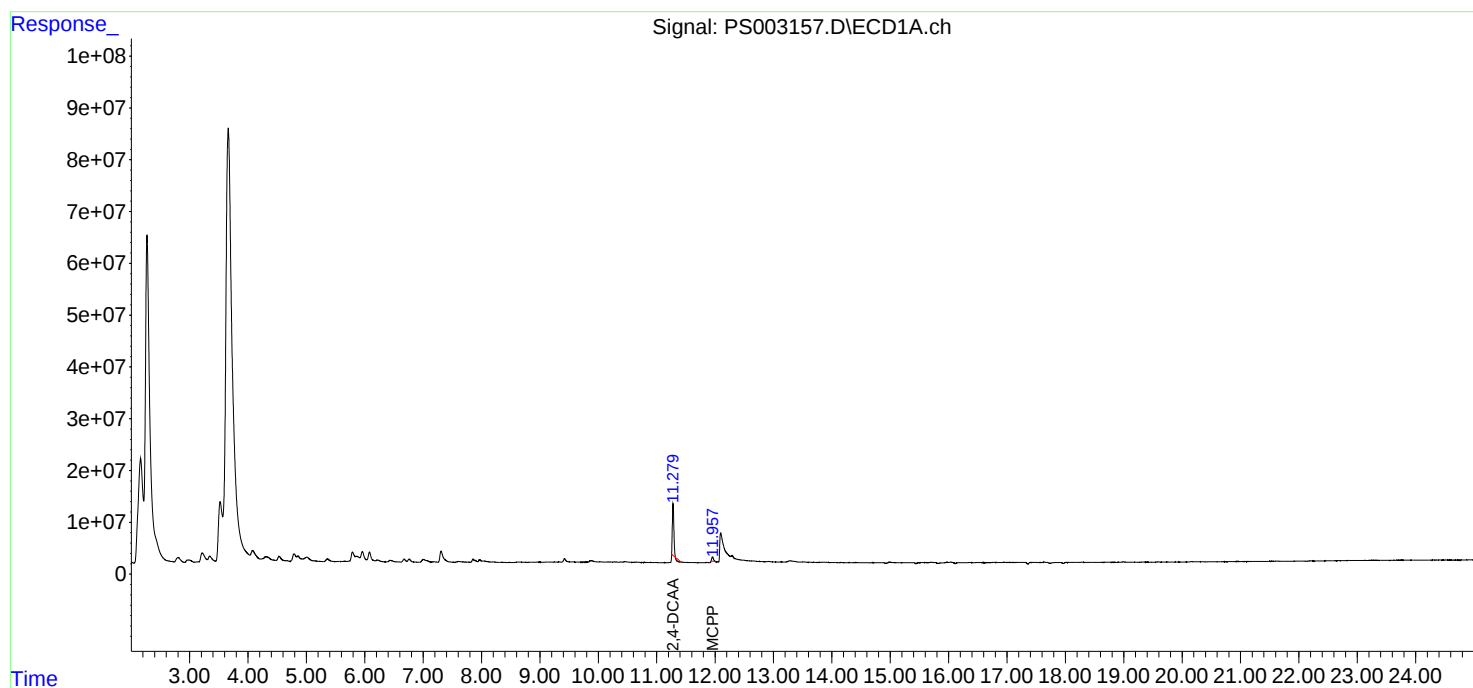


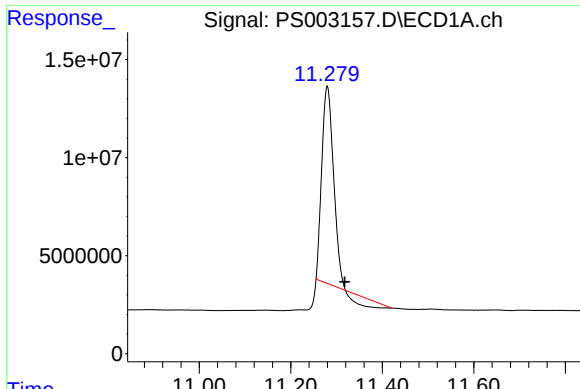

#4 2,4-DCAA


R.T.: 11.280 min
Delta R.T.: -0.038 min
Response: 160692695
Conc: 423.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

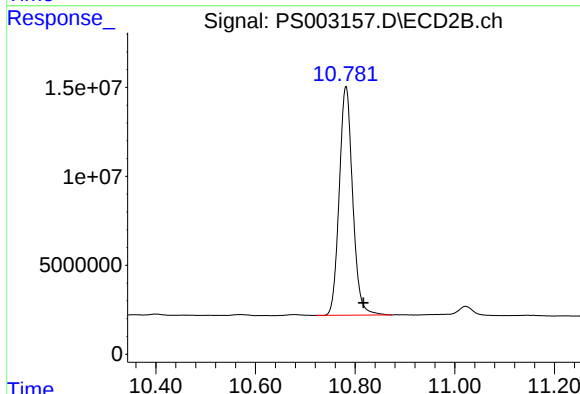


#4 2,4-DCAA

R.T.: 10.782 min
Delta R.T.: -0.035 min
Response: 240092380
Conc: 561.56 ng/ml

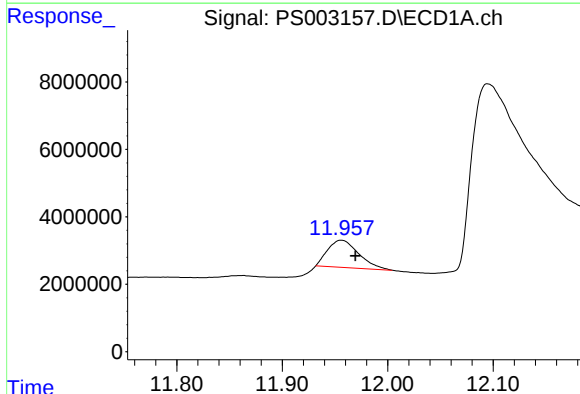


#6 MCP

R.T.: 11.956 min
Delta R.T.: -0.013 min
Response: 16265737
Conc: 13.58 ug/ml

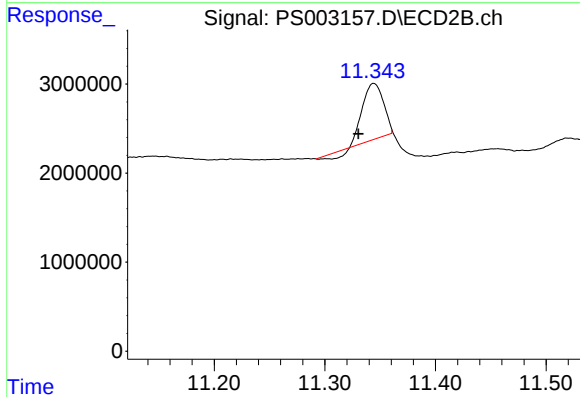

#6 MCP


R.T.: 11.344 min
Delta R.T.: 0.014 min
Response: 8137018
Conc: 7.38 ug/ml

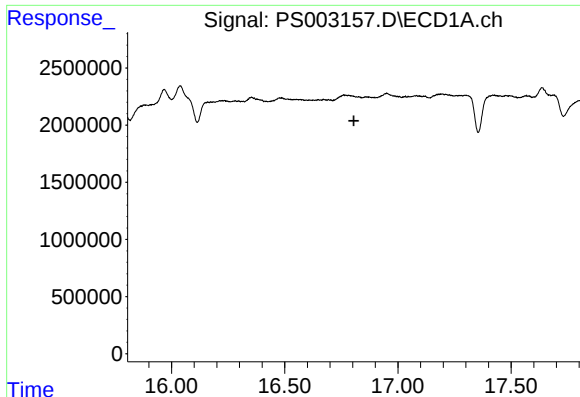

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

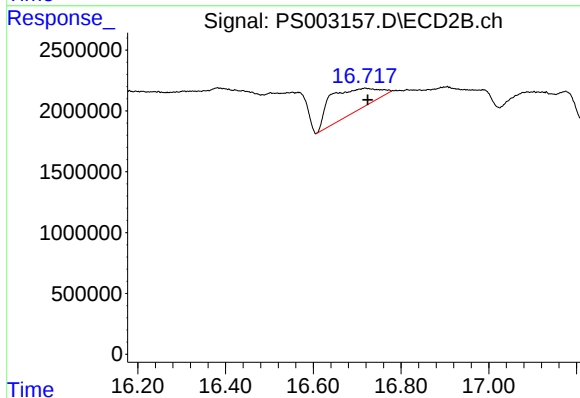


#15 Picloram

R.T.: 16.718 min
Delta R.T.: -0.006 min
Response: 14567641
Conc: 4.85 ng/ml

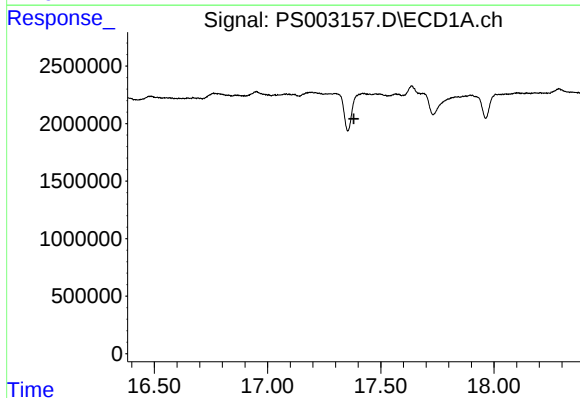

#16 DCPA

R.T.: 17.420 min
Delta R.T.: 0.038 min
Response: -3361797
Conc: N.D.

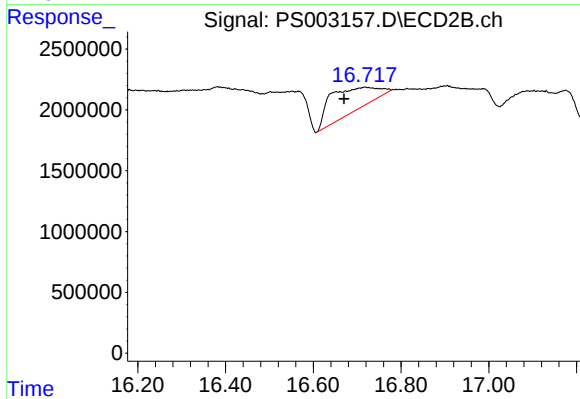

#16 DCPA

R.T.: 16.718 min
Delta R.T.: 0.048 min
Response: 14567641
Conc: 4.70 ng/ml